


Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN121121\
 Data File : BN017893.D
 Acq On : 11 Dec 2021 06:18
 Operator : CG/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\8270-SIM-BN121121.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Sat Dec 11 00:01:30 2021

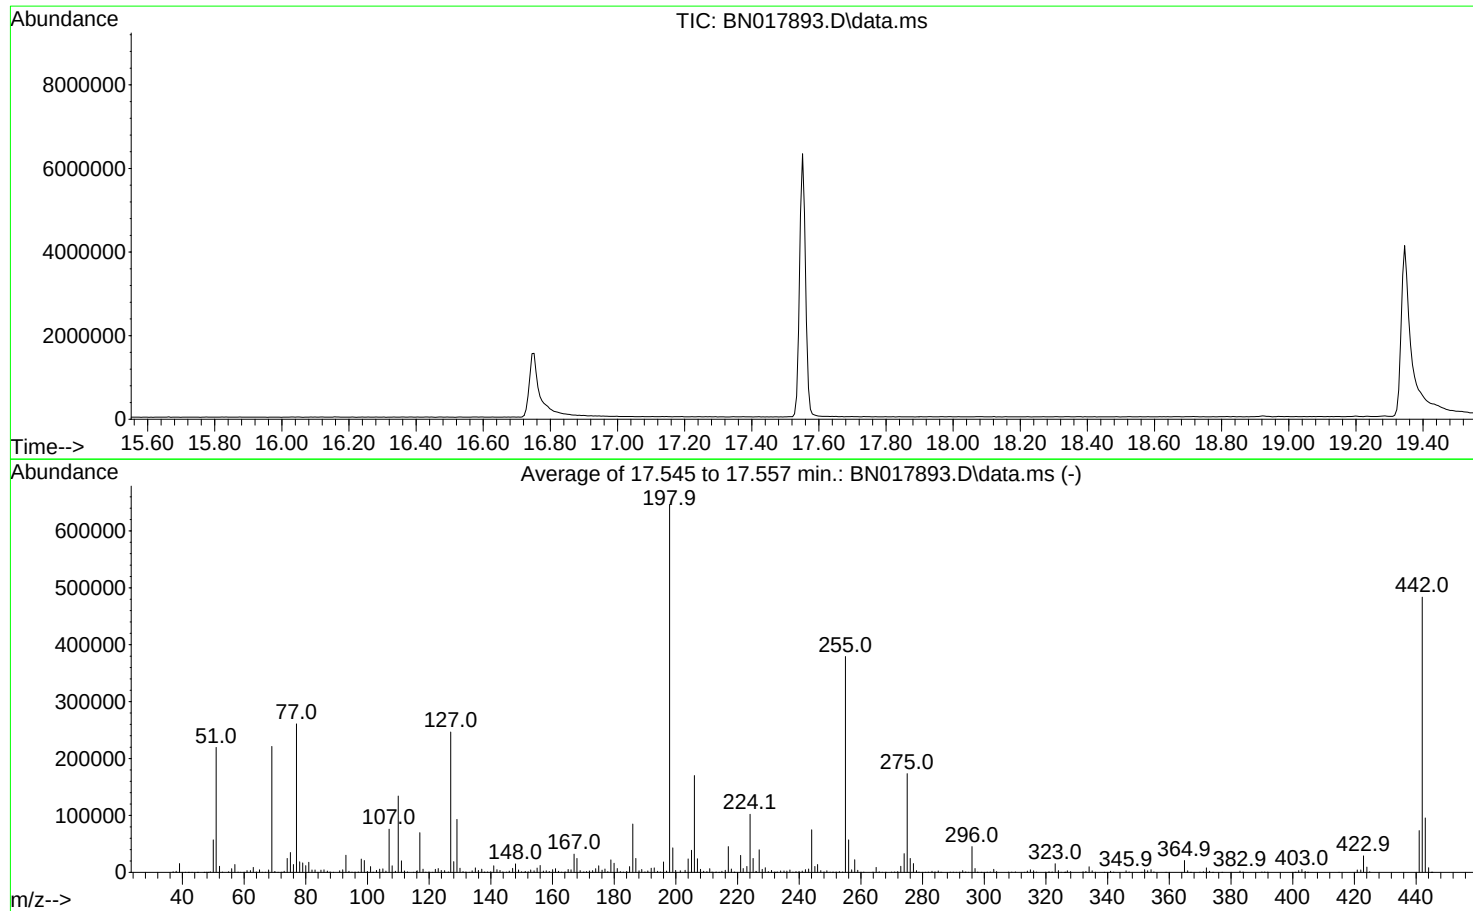




AutoFind: Scans 2475, 2476, 2477; Background Corrected with Scan 2468

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	34.0	219551	PASS
68	69	0.00	2	1.9	4105	PASS
69	198	0.00	100	34.2	221312	PASS
70	69	0.00	2	0.7	1596	PASS
127	198	10	80	38.1	246613	PASS
197	198	0.00	2	0.4	2371	PASS
198	198	100	100	100.0	646443	PASS
199	198	5	9	6.6	42949	PASS
275	198	10	60	26.9	173589	PASS
365	198	1	100	3.2	20924	PASS
441	198	0.01	100	11.4	73424	PASS
442	442	50	100	100.0	483584	PASS
443	442	15	24	19.8	95595	PASS

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN121121\
Data File : BN017893.D
Acq On : 11 Dec 2021 06:18
Operator : CG/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
DFTPP

Quant Time: Dec 11 07:33:16 2021
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\8270E-Tune.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Sat Dec 11 07:33:12 2021
Response via : Initial Calibration

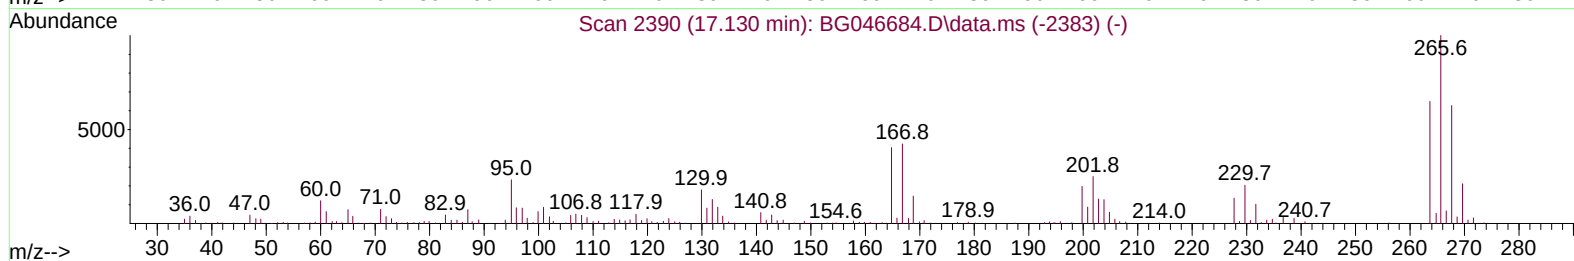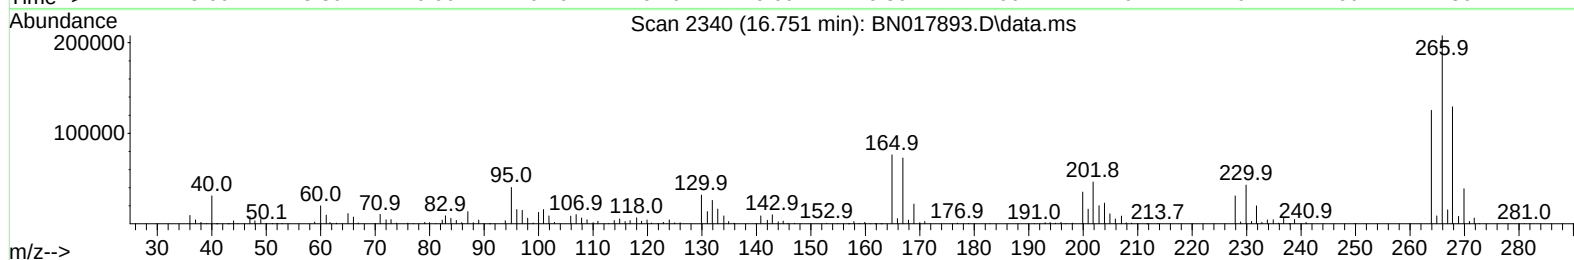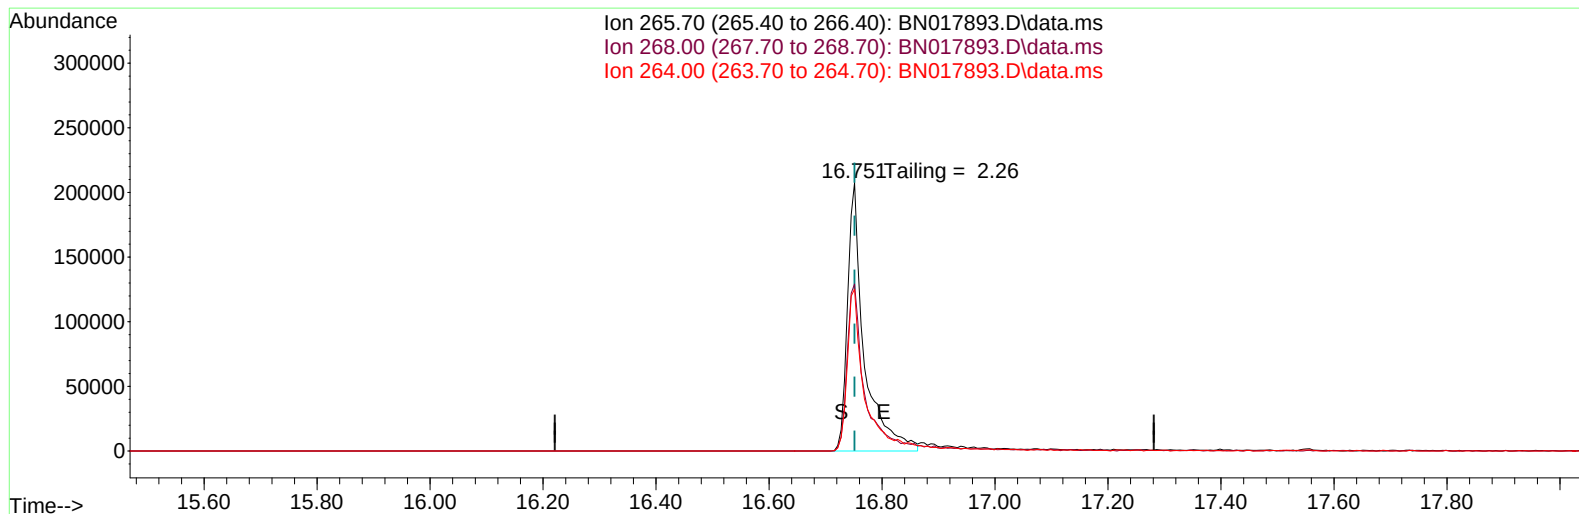

TIC: BN017893.D\data.ms

(70) Pentachlorophenol (C)

16.751min (0.000) 14086.35 ng




response 441079

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	62.20	62.24
264.00	61.60	60.37
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN121121\
 Data File : BN017893.D
 Acq On : 11 Dec 2021 06:18
 Operator : CG/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 DFTPP

Quant Time: Dec 11 07:33:16 2021
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\8270E-Tune.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Sat Dec 11 07:33:12 2021
 Response via : Initial Calibration

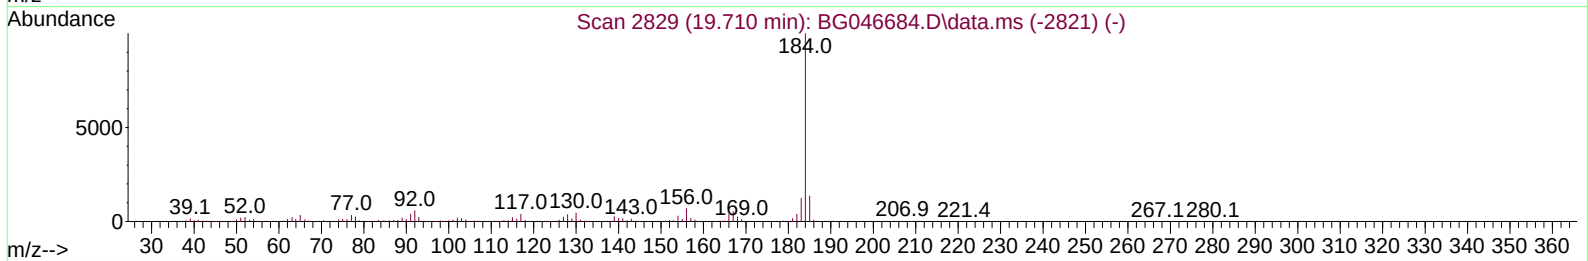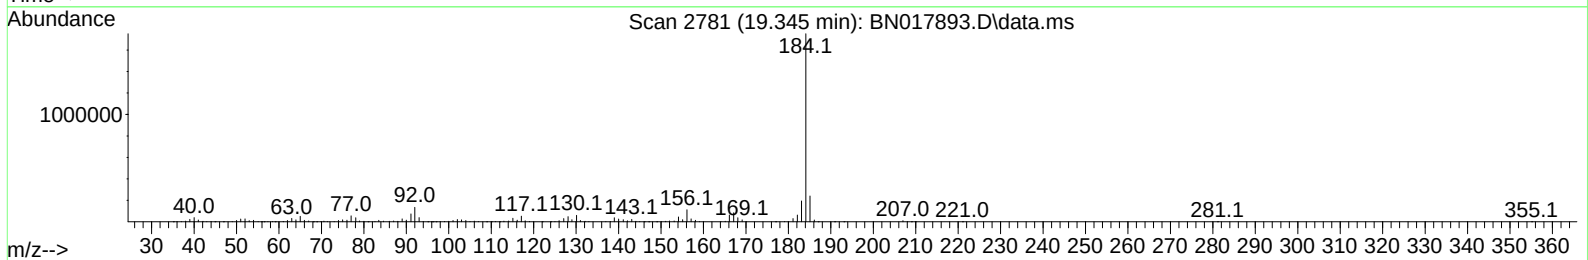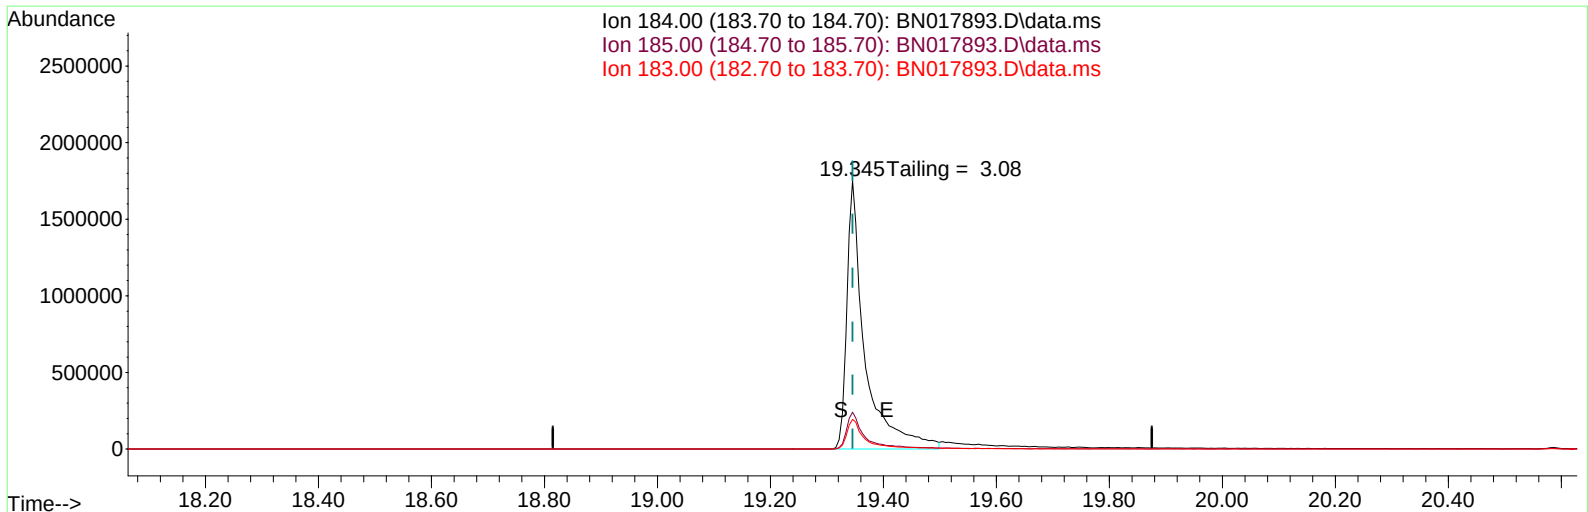

TIC: BN017893.D\data.ms

(77) Benzidine

19.345min (0.000) 0.00 ng m

response 3895064

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	15.50	13.74
183.00	13.20	11.06
0.00	0.00	0.00

Instrument :
BNA_N
ClientSampleId :
DFTPP

DDT Breakdown

Date	Instrument Name	DFTPP Data File
12/10/2021	BNA_N	<u>BN017893.D</u>
Compound Name	Response	Retention Time
DDT	2235560	20.586
DDD	87000	20.145
DDE	4495	19.639
SUM(DDD+DDE)	SUM(DDT+DDD+DDE)	% Breakdown Of DDT
91495	2327055	3.93

Instrument :
BNA_N
ClientSampleId :
DFTPP