
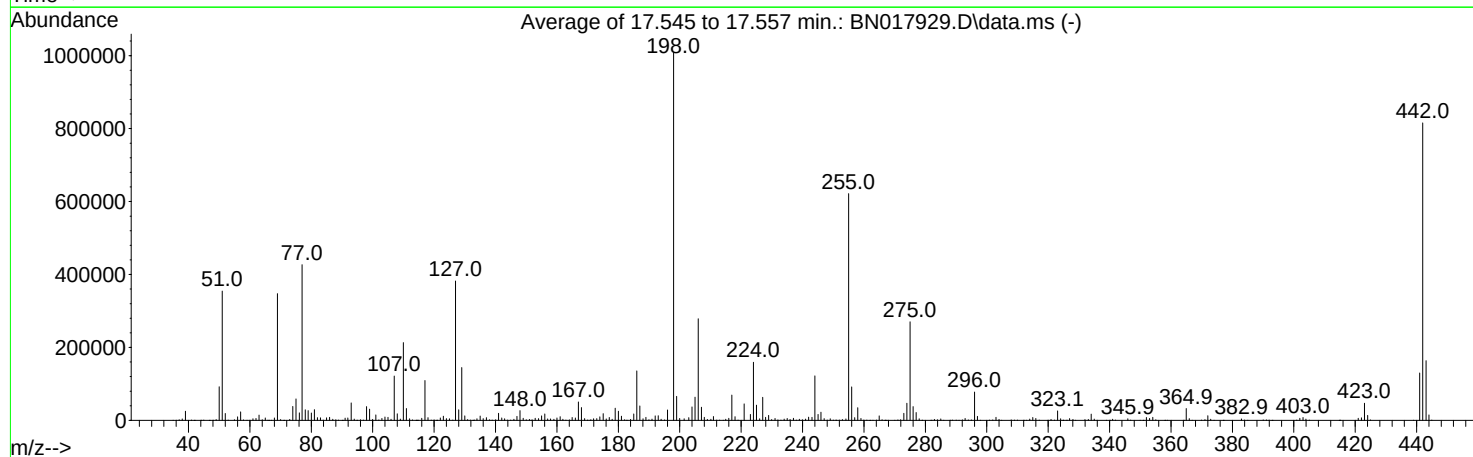


Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN121121\
 Data File : BN017929.D
 Acq On : 12 Dec 2021 07:05
 Operator : CG/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 53 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\8270-SIM-BN121121.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Sat Dec 11 00:01:30 2021

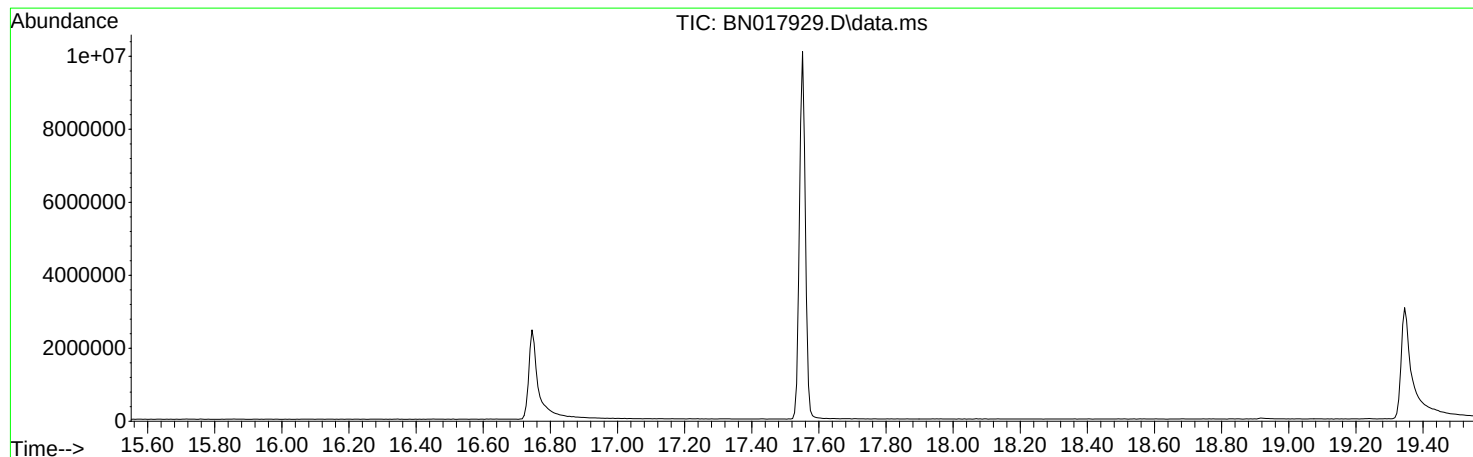




AutoFind: Scans 2475, 2476, 2477; Background Corrected with Scan 2468

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	35.2	354719	PASS
68	69	0.00	2	1.9	6436	PASS
69	198	0.00	100	34.4	347392	PASS
70	69	0.00	2	0.6	2198	PASS
127	198	10	80	37.9	382144	PASS
197	198	0.00	2	0.0	0	PASS
198	198	100	100	100.0	1008619	PASS
199	198	5	9	6.5	65931	PASS
275	198	10	60	26.8	270315	PASS
365	198	1	100	3.2	32568	PASS
441	198	0.01	100	12.9	130069	PASS
442	442	50	100	100.0	815445	PASS
443	442	15	24	20.1	163675	PASS

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN121121\
Data File : BN017929.D
Acq On : 12 Dec 2021 07:05
Operator : CG/JU
Sample : DFTPP
Misc :
ALS Vial : 53 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
DFTPP

Quant Time: Dec 13 03:16:47 2021
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\8270E-Tune.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Mon Dec 13 03:14:02 2021
Response via : Initial Calibration

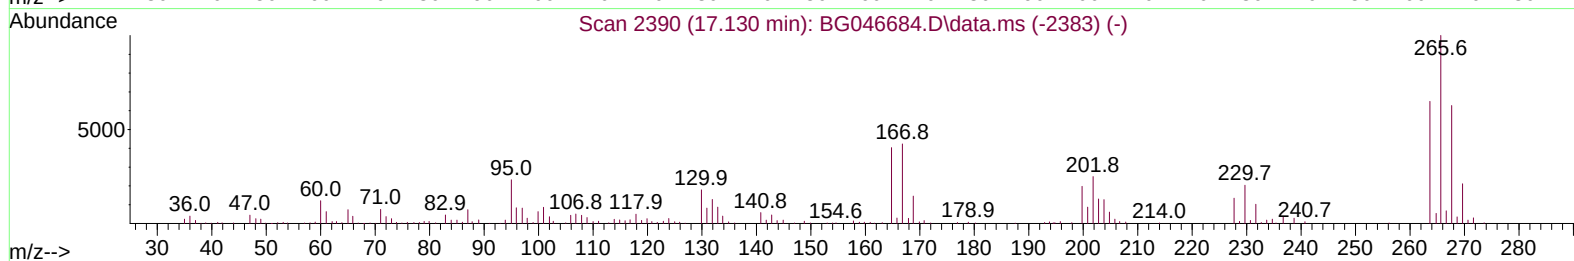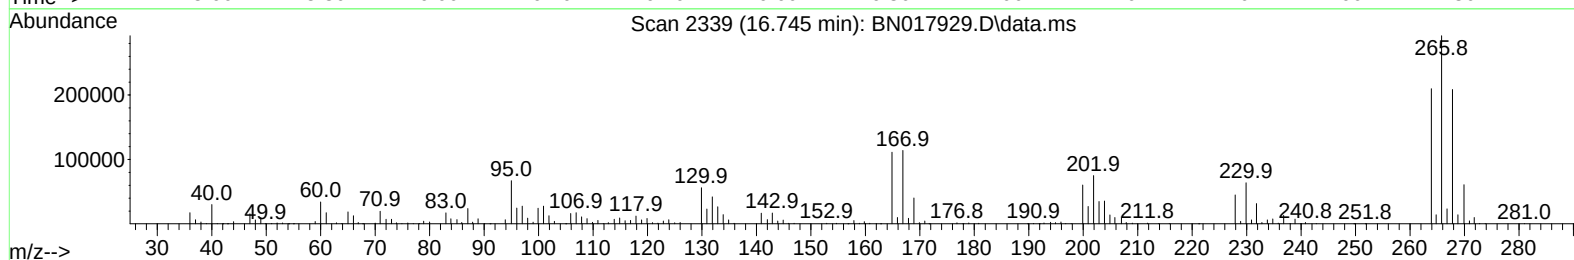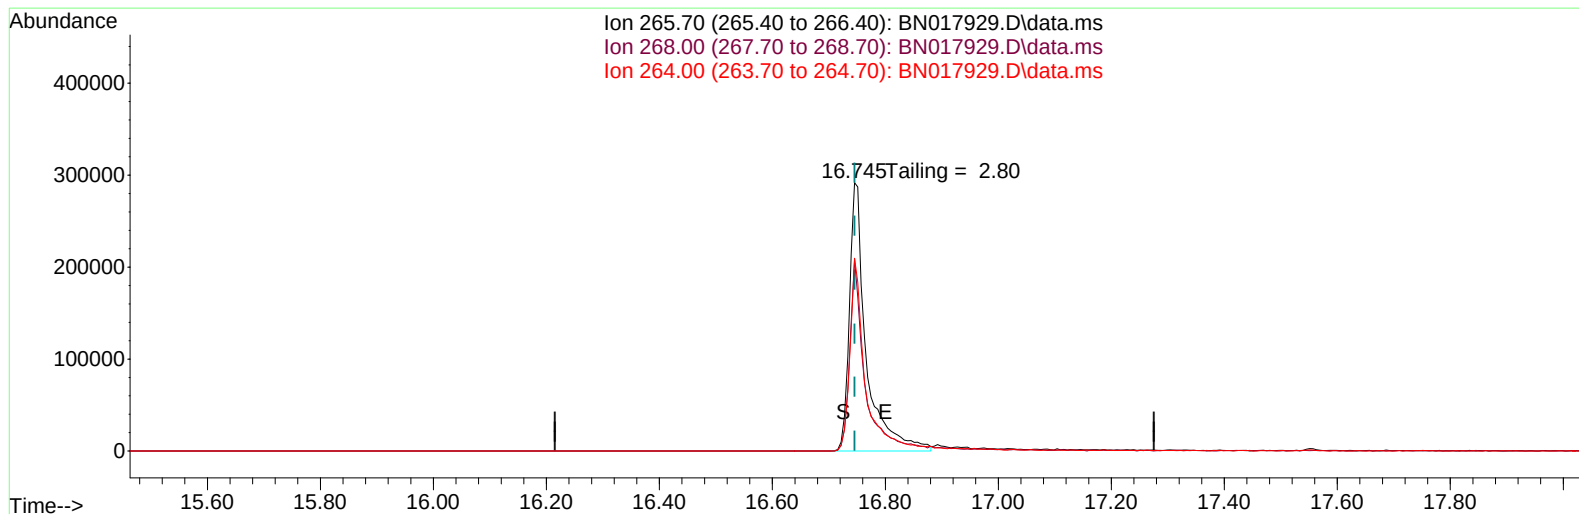

TIC: BN017929.D\data.ms

(70) Pentachlorophenol (C)

16.745min (+ 0.000) 11603.66 ng




response 610575

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	62.20	71.48
264.00	61.60	71.85
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN121121\
Data File : BN017929.D
Acq On : 12 Dec 2021 07:05
Operator : CG/JU
Sample : DFTPP
Misc :
ALS Vial : 53 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
DFTPP

Quant Time: Dec 13 03:16:47 2021
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\8270E-Tune.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Mon Dec 13 03:14:02 2021
Response via : Initial Calibration

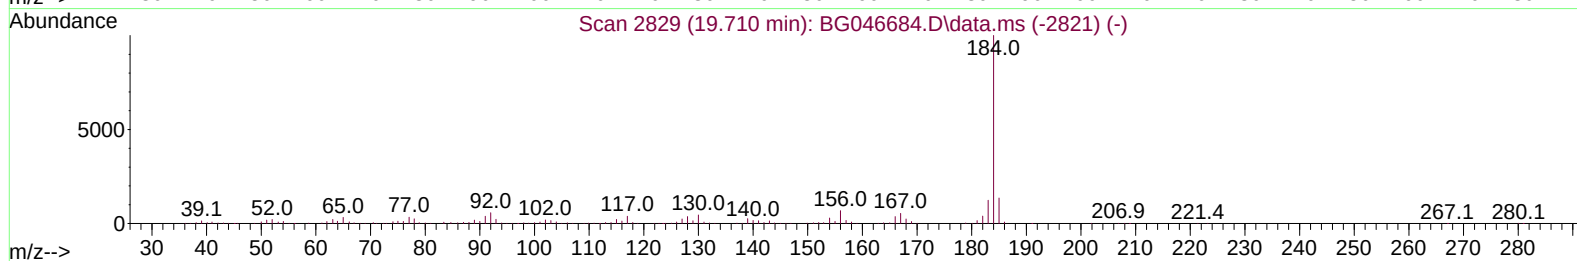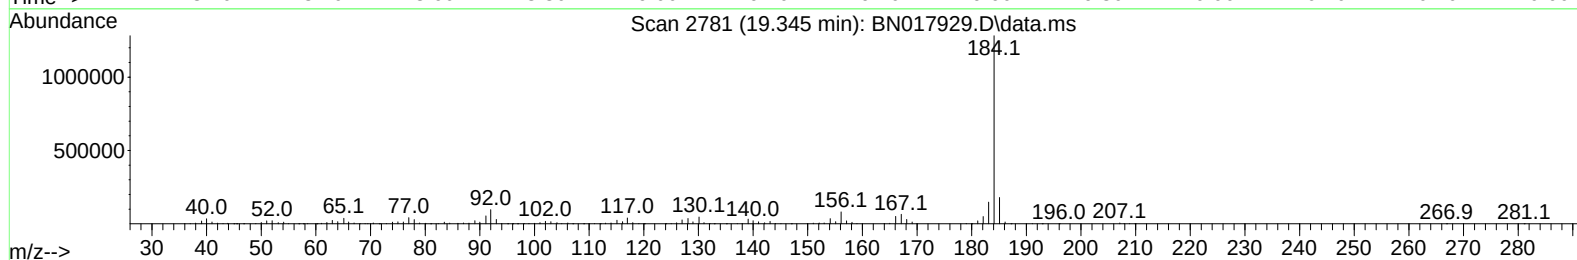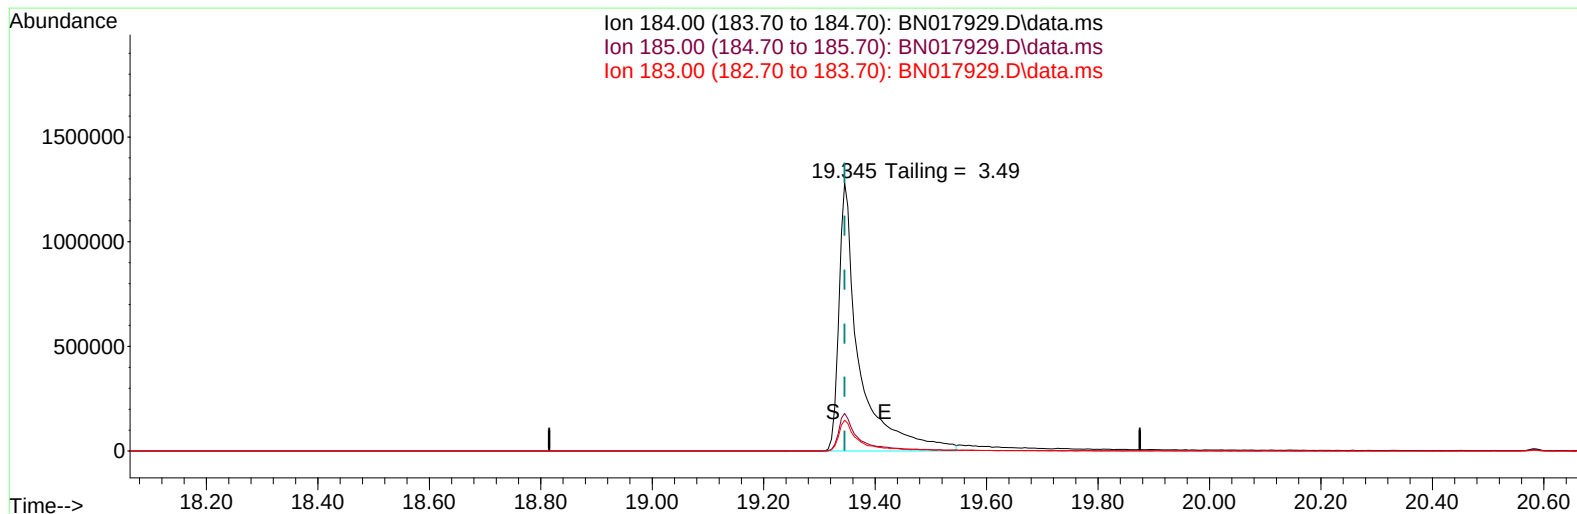

TIC: BN017929.D\data.ms

(77) Benzidine

19.345min (+ 0.000) 0.00 ng

response 3398259

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	15.50	14.02
183.00	13.20	11.53
0.00	0.00	0.00

Instrument :
BNA_N
ClientSampleId :
DFTPP

DDT Breakdown

Date	Instrument Name	DFTPP Data File
12/11/2021	BNA_N	<u>BN017929.D</u>
Compound Name	Response	Retention Time
DDT	2558662	20.586
DDD	105316	20.145
DDE	7041	19.639
SUM(DDD+DDE)	SUM(DDT+DDD+DDE)	% Breakdown Of DDT
112357	2671019	4.21

Instrument :
BNA_N
ClientSampleId :
DFTPP