
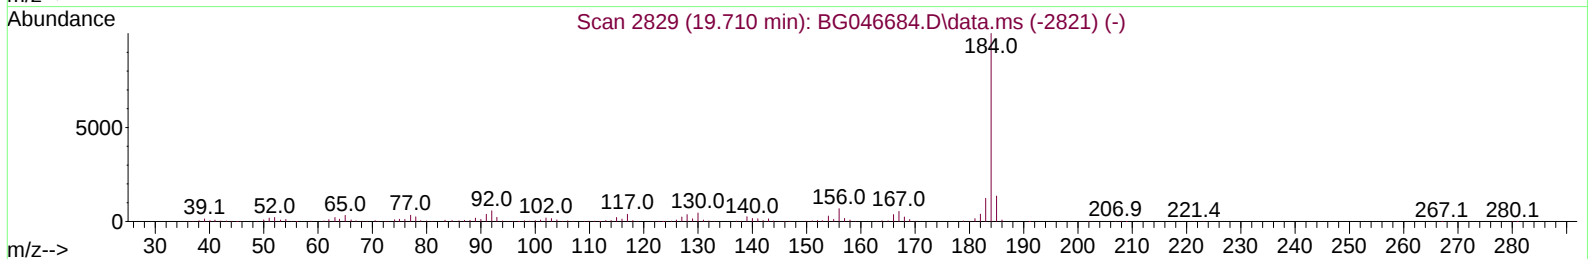
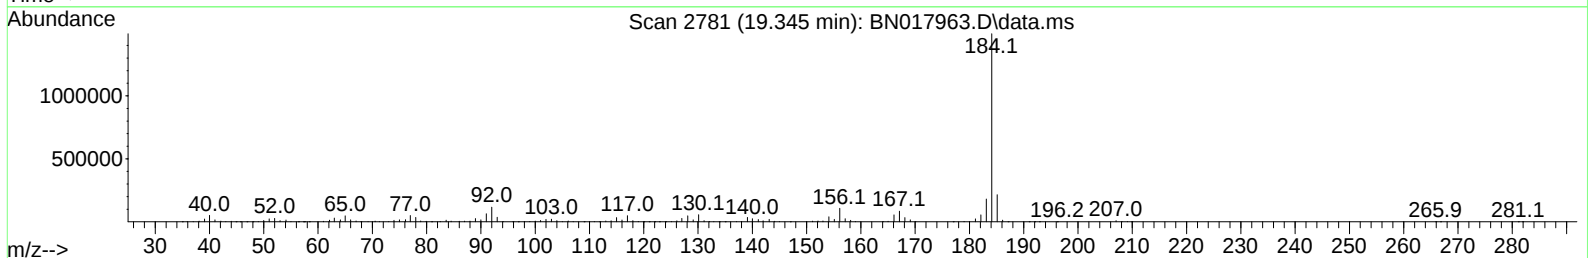


Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN121321\
 Data File : BN017963.D
 Acq On : 13 Dec 2021 09:23
 Operator : CG/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Quant Time: Dec 14 05:37:21 2021
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\8270E-Tune.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Tue Dec 14 05:37:16 2021
 Response via : Initial Calibration

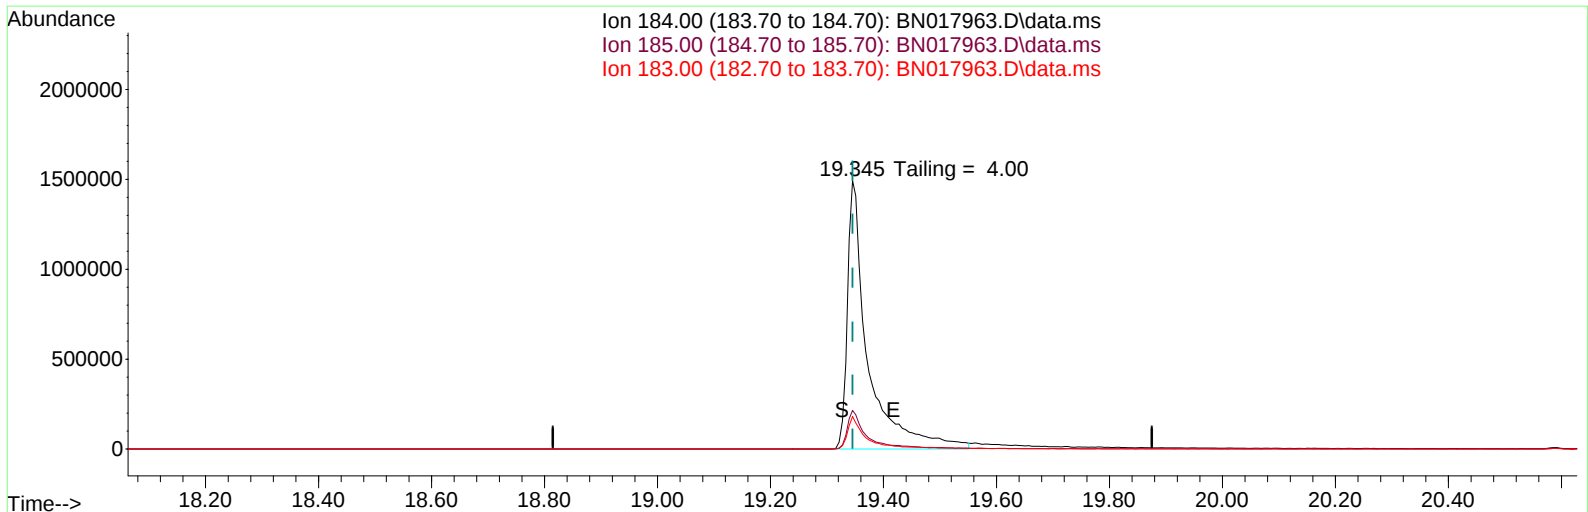

TIC: BN017963.D\data.ms

(77) Benzidine




19.345min (0.000) 0.00 ng

response 3902762

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	15.50	14.41
183.00	13.20	12.11
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN121321\
Data File : BN017963.D
Acq On : 13 Dec 2021 09:23
Operator : CG/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Dec 14 05:37:21 2021
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\8270E-Tune.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Dec 14 05:37:16 2021
Response via : Initial Calibration

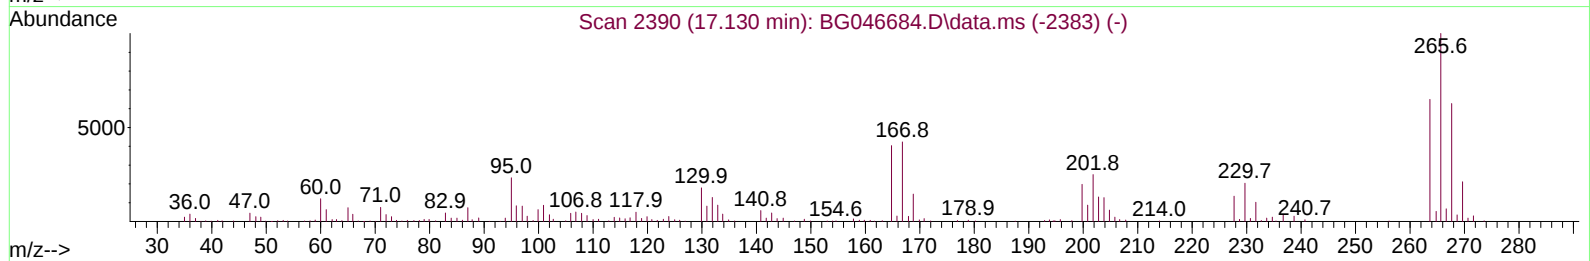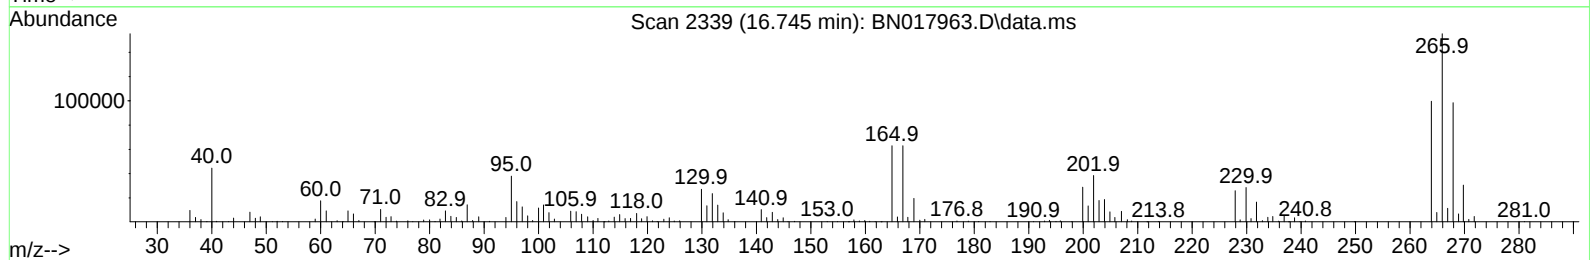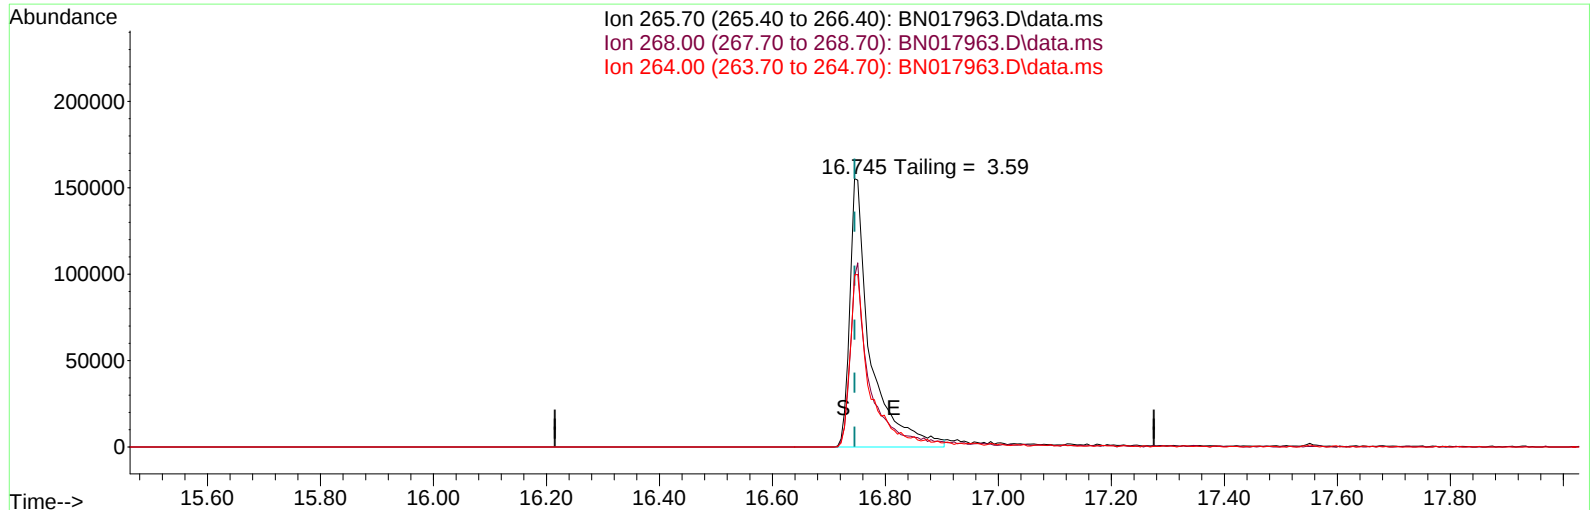

TIC: BN017963.D\data.ms

(70) Pentachlorophenol (C)

16.745min (0.000) 11598.31 ng

response 402220

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	62.20	63.41
264.00	61.60	64.14
0.00	0.00	0.00