

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN121321\
 Data File : BN017966.D
 Acq On : 13 Dec 2021 11:24
 Operator : CG/JU
 Sample : M4923-20
 Misc :
 ALS Vial : 4 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 RE105D1-20211202

Quant Time: Dec 14 03:40:21 2021
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\8270-SIM-BN121121.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Sat Dec 11 00:01:30 2021
 Response via : Initial Calibration

Manual Integrations
 APPROVED

Reviewed By :Christian Giraldo 12/14/2021
 Supervised By :Jagrut Upadhyay 12/14/2021

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.705	152	26109	0.400	ng	0.00
7) Naphthalene-d8	10.494	136	109386	0.400	ng	0.00
13) Acenaphthene-d10	14.334	164	65634	0.400	ng	0.00
19) Phenanthrene-d10	17.092	188	138693	0.400	ng	0.00
29) Chrysene-d12	21.293	240	86813	0.400	ng	0.00
35) Perylene-d12	23.599	264	43089	0.400	ng	0.01
System Monitoring Compounds						
4) 2-Fluorophenol	5.336	112	2843850	52.835	ng	0.00
5) Phenol-d6	6.903	99	1998132	37.383	ng	0.00
8) Nitrobenzene-d5	8.859	82	5957880	83.417	ng	0.00
11) 2-Methylnaphthalene-d10	12.089	152	47949	0.249	ng	0.00
14) 2,4,6-Tribromophenol	15.844	330	3478136	97.453	ng	0.00
15) 2-Fluorobiphenyl	12.977	172	11341503	49.106	ng	0.01
27) Fluoranthene-d10	19.129	212	144091	0.320	ng	0.00
31) Terphenyl-d14	19.745	244	12513423	58.461	ng	0.00
Target Compounds						
2) 1,4-Dioxane	3.270	88	47228m	5.961	ng	Qvalue
24) Pentachlorophenol	16.764	266	660	0.325	ng	96
34) Bis(2-ethylhexyl)phtha...	21.218	149	6222	0.067	ng	99

(#) = qualifier out of range (m) = manual integration (+) = signals summed


Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN121321\
Data File : BN017966.D
Acq On : 13 Dec 2021 11:24
Operator : CG/JU
Sample : M4923-20
Misc :
ALS Vial : 4 Sample Multiplier: 1


Instrument :
BNA_N
ClientSampleId :
RE105D1-20211202

Quant Time: Dec 14 03:40:21 2021
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\8270-SIM-BN121121.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Sat Dec 11 00:01:30 2021
Response via : Initial Calibration

Manual Integrations
APPROVED


Reviewed By :Christian Giraldo 12/14/2021
Supervised By :Jagrut Upadhyay 12/14/2021

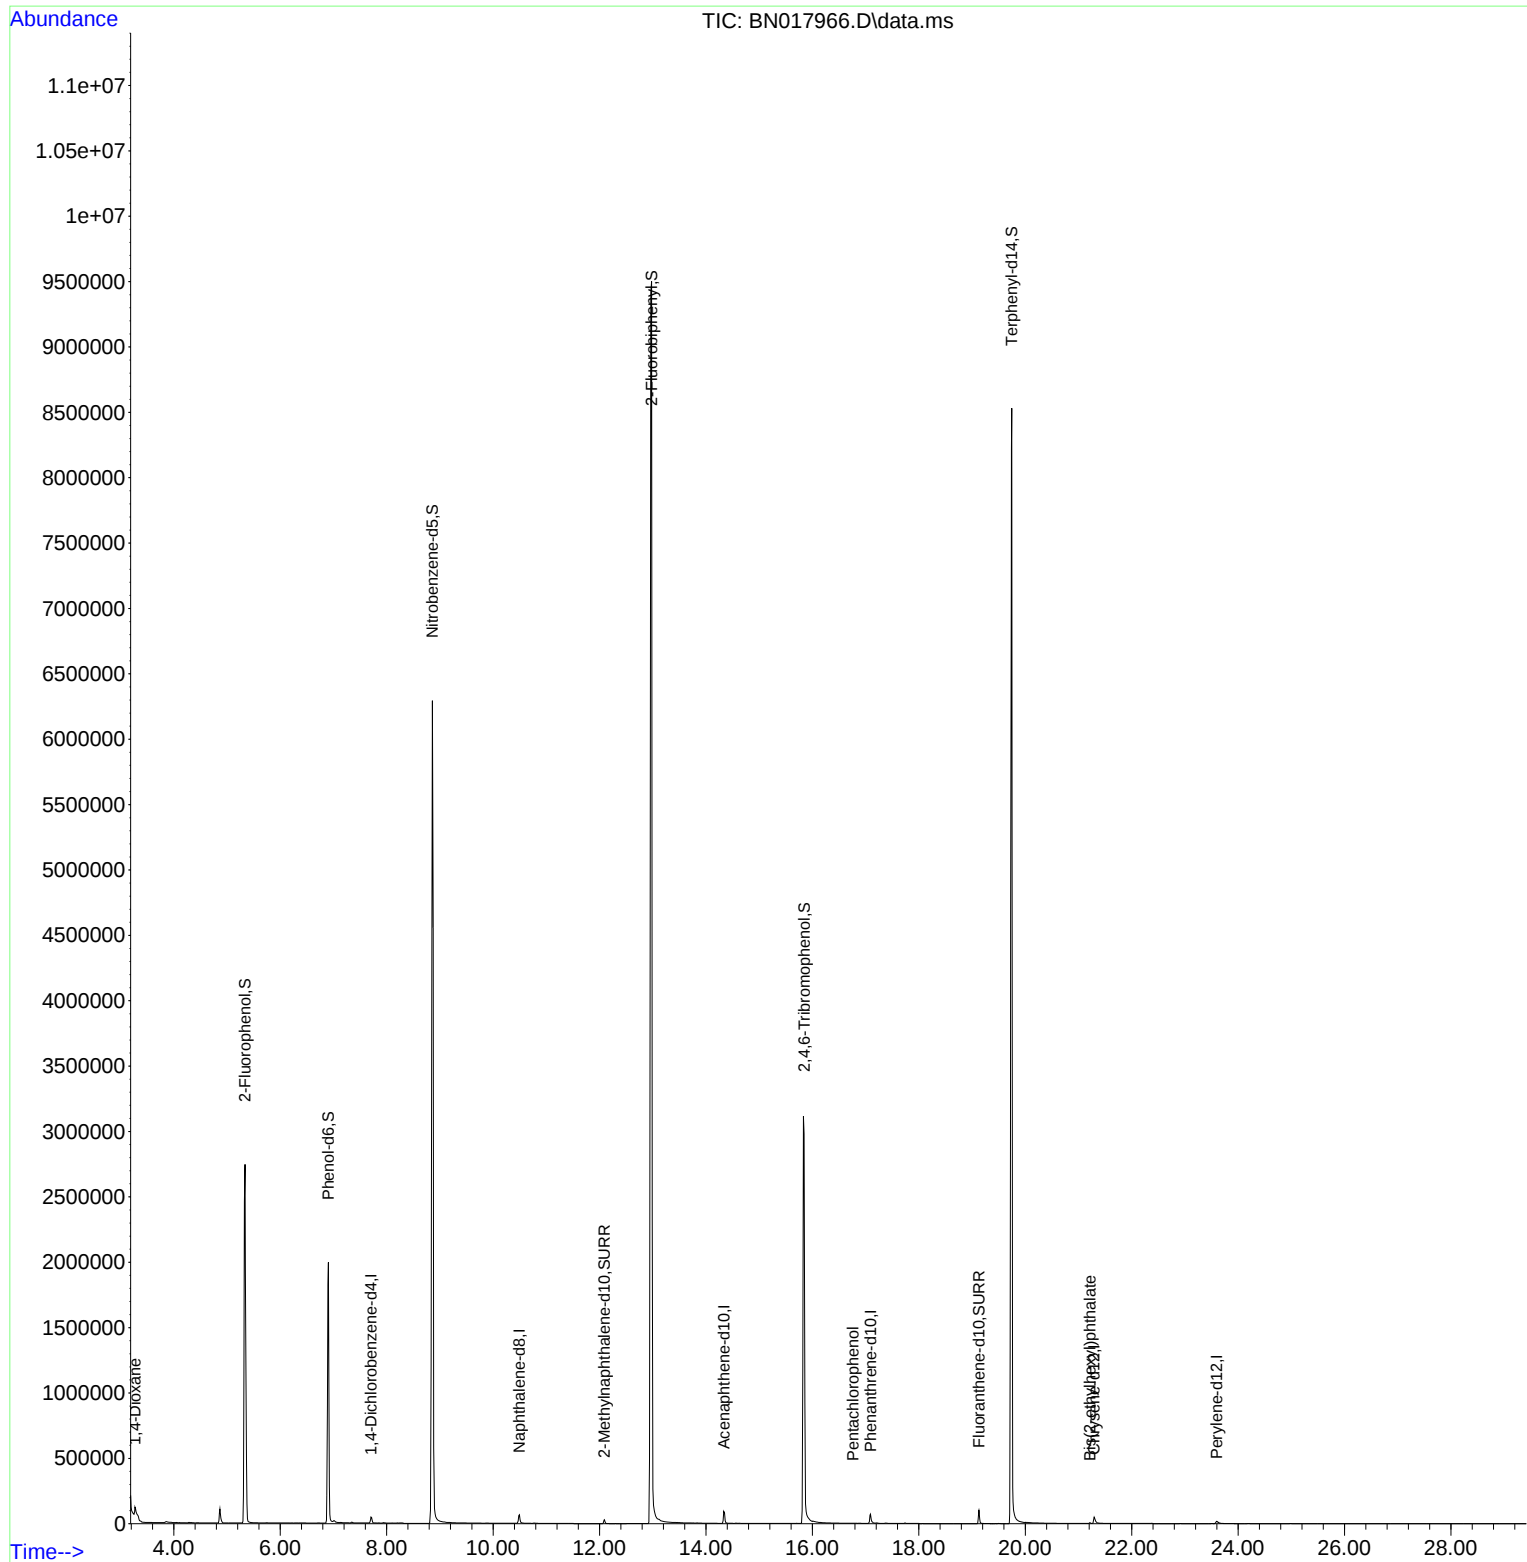



#1
1,4-Dichlorobenzene-d4
Concen: 0.400 ng
RT: 7.705 min Scan# 491
Delta R.T. -0.010 min
Lab File: BN017966.D
Acq: 13 Dec 2021 11:24




Instrument :
BNA_N
ClientSampleId :
RE105D1-20211202




Tgt Ion:152 Resp: 26109
Ion Ratio Lower Upper
152 100
150 157.9 121.9 182.9
115 57.6 44.1 66.1

Manual Integrations
APPROVED



Reviewed By :Christian Giraldo 12/14/2021
Supervised By :Jagrut Upadhyay 12/14/2021

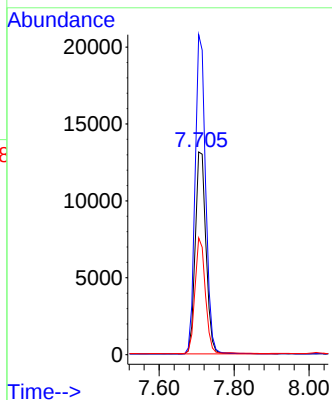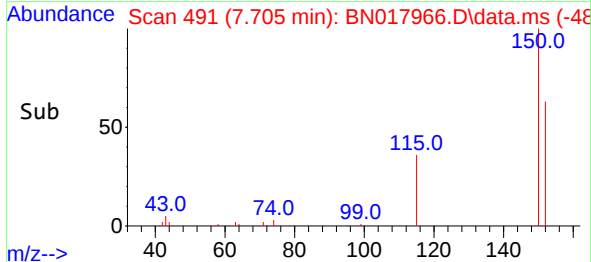


#2
1,4-Dioxane
Concen: 5.961 ng m
RT: 3.270 min Scan# 10
Delta R.T. -0.000 min
Lab File: BN017966.D
Acq: 13 Dec 2021 11:24

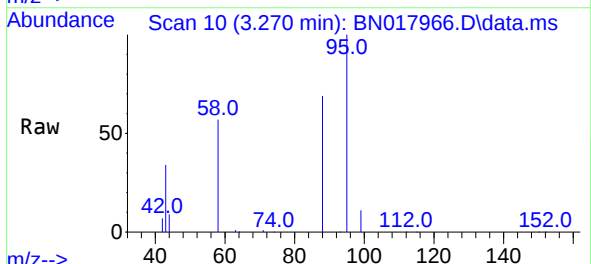


Tgt Ion: 88 Resp: 47228
Ion Ratio Lower Upper
88 100
43 33.7 28.0 42.0
58 86.6 65.4 98.0

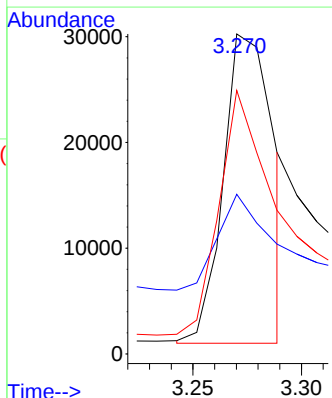



#4
2-Fluorophenol
Concen: 52.835 ng
RT: 5.336 min Scan# 21
Delta R.T. 0.009 min
Lab File: BN017966.D
Acq: 13 Dec 2021 11:24




Instrument :
BNA_N
ClientSampleId :
RE105D1-20211202




Tgt Ion:112 Resp: 2843850
Ion Ratio Lower Upper
112 100
64 60.4 49.0 73.4
63 31.6 26.2 39.2

Manual Integrations
APPROVED



Reviewed By :Christian Giraldo 12/14/2021
Supervised By :Jagrut Upadhyay 12/14/2021

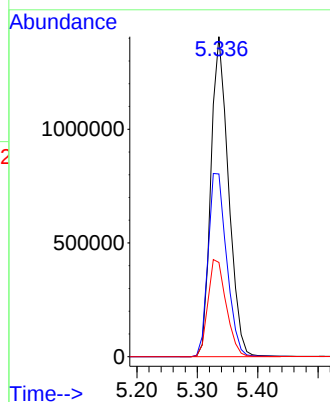


#5
Phenol-d6
Concen: 37.383 ng
RT: 6.903 min Scan# 404
Delta R.T. 0.009 min
Lab File: BN017966.D
Acq: 13 Dec 2021 11:24




Tgt Ion: 99 Resp: 1998132
Ion Ratio Lower Upper
99 100
42 19.8 17.0 25.4
71 33.9 28.0 42.0

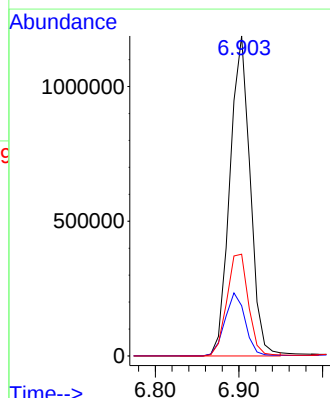

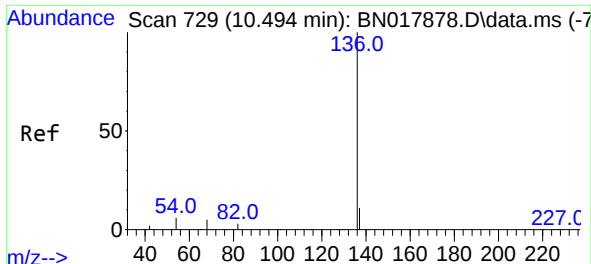

#7
Naphthalene-d8
Concen: 0.400 ng
RT: 10.494 min Scan# 729
Delta R.T. -0.000 min
Lab File: BN017966.D
Acq: 13 Dec 2021 11:24




Instrument :
BNA_N
ClientSampleId :
RE105D1-20211202



Tgt Ion:136 Resp: 109380
Ion Ratio Lower Upper
136 100
137 11.1 8.8 13.2
54 6.6 5.1 7.7
68 5.1 4.4 6.6




Manual Integrations
APPROVED


Reviewed By :Christian Giraldo 12/14/2021
Supervised By :Jagrut Upadhyay 12/14/2021



#8
Nitrobenzene-d5
Concen: 83.417 ng
RT: 8.859 min Scan# 600
Delta R.T. -0.000 min
Lab File: BN017966.D
Acq: 13 Dec 2021 11:24


Tgt Ion: 82 Resp: 5957880
Ion Ratio Lower Upper
82 100
128 39.3 32.2 48.4
54 51.7 37.6 56.4

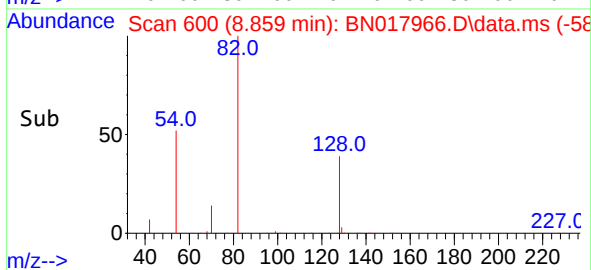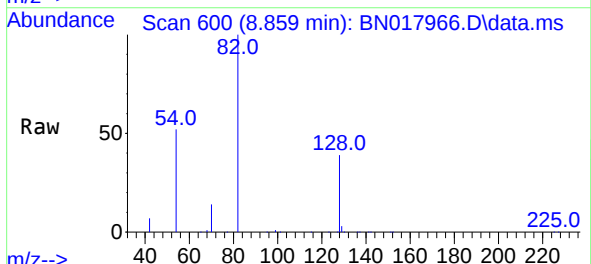



#11
2-Methylnaphthalene-d10
Concen: 0.249 ng
RT: 12.089 min Scan# 911
Delta R.T. -0.000 min
Lab File: BN017966.D
Acq: 13 Dec 2021 11:24




Instrument :
BNA_N
ClientSampleId :
RE105D1-20211202



Tgt Ion:152 Resp: 47949
Ion Ratio Lower Upper
152 100
151 20.4 16.4 24.6




Manual Integrations
APPROVED


Reviewed By :Christian Giraldo 12/14/2021
Supervised By :Jagrut Upadhyay 12/14/2021

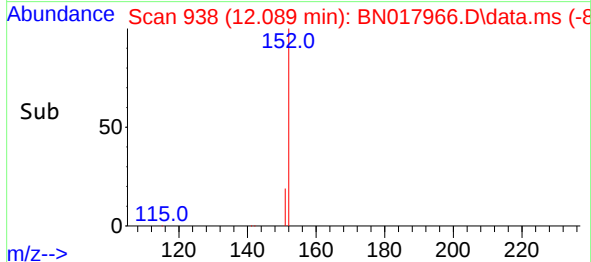

#13
Acenaphthene-d10
Concen: 0.400 ng
RT: 14.334 min Scan# 1176
Delta R.T. -0.000 min
Lab File: BN017966.D
Acq: 13 Dec 2021 11:24


Tgt Ion:164 Resp: 65634
Ion Ratio Lower Upper
164 100
162 102.3 82.1 123.1
160 48.3 38.2 57.2

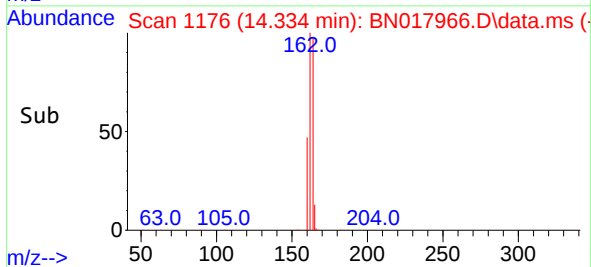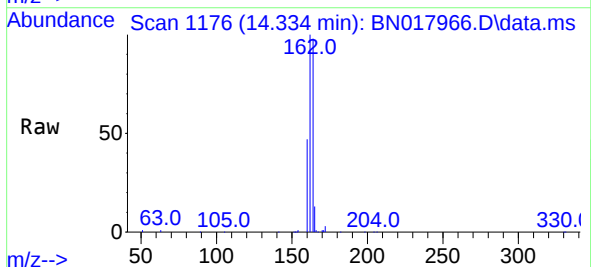



#14
2,4,6-Tribromophenol
Concen: 97.453 ng
RT: 15.844 min Scan# 1295
Delta R.T. 0.000 min
Lab File: BN017966.D
Acq: 13 Dec 2021 11:24




Instrument :
BNA_N
ClientSampleId :
RE105D1-20211202



Tgt Ion:330 Resp: 3478130
Ion Ratio Lower Upper
330 100
332 0.0 0.0 0.0
141 27.8 19.7 29.5




Manual Integrations
APPROVED


Reviewed By :Christian Giraldo 12/14/2021
Supervised By :Jagrut Upadhyay 12/14/2021

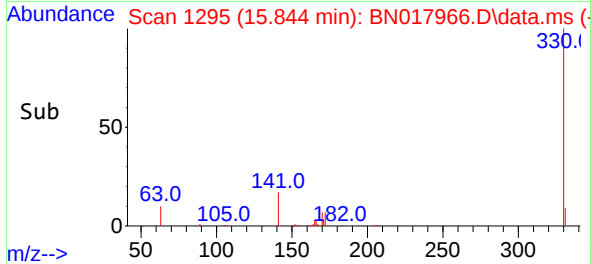

#15
2-Fluorobiphenyl
Concen: 49.106 ng
RT: 12.977 min Scan# 1069
Delta R.T. 0.013 min
Lab File: BN017966.D
Acq: 13 Dec 2021 11:24


Tgt Ion:172 Resp:11341503
Ion Ratio Lower Upper
172 100
171 34.3 28.3 42.5
170 23.1 19.1 28.7

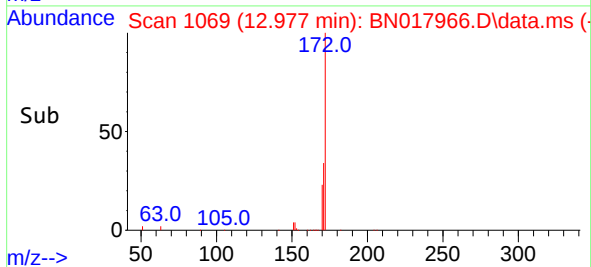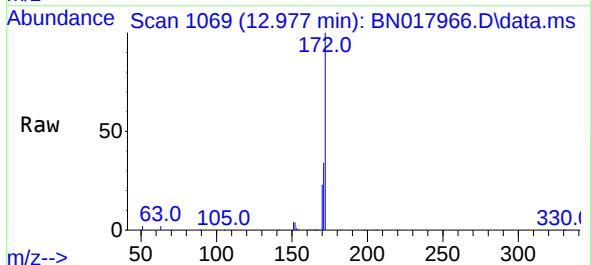

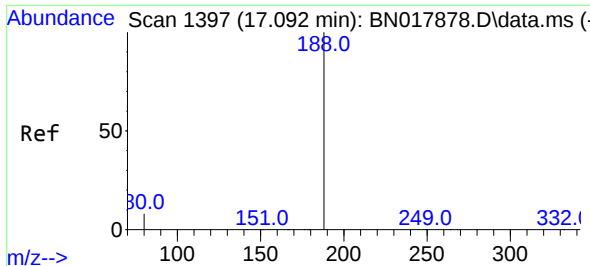

#19
Phenanthrene-d10
Concen: 0.400 ng
RT: 17.092 min Scan# 11
Delta R.T. -0.000 min
Lab File: BN017966.D
Acq: 13 Dec 2021 11:24




Instrument :
BNA_N
ClientSampleId :
RE105D1-20211202

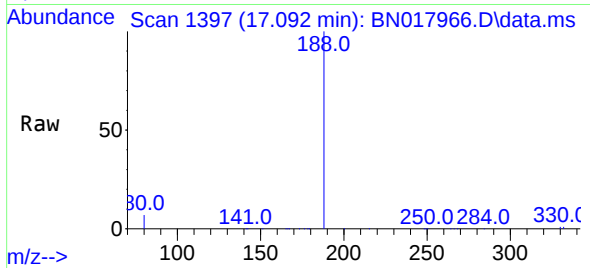

Tgt Ion:188 Resp: 13869
Ion Ratio Lower Upper
188 100
94 0.0 0.0 0.0
80 7.5 6.2 9.2




Manual Integrations
APPROVED


Reviewed By :Christian Giraldo 12/14/2021
Supervised By :Jagrut Upadhyay 12/14/2021

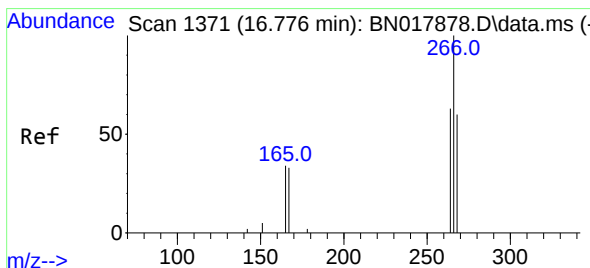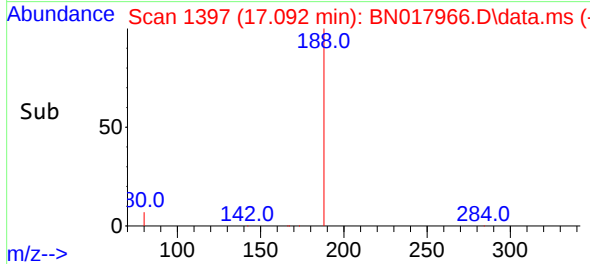

#24
Pentachlorophenol
Concen: 0.325 ng
RT: 16.764 min Scan# 1370
Delta R.T. -0.012 min
Lab File: BN017966.D
Acq: 13 Dec 2021 11:24


Tgt Ion:266 Resp: 660
Ion Ratio Lower Upper
266 100
264 63.6 50.6 76.0
268 72.4 53.7 80.5

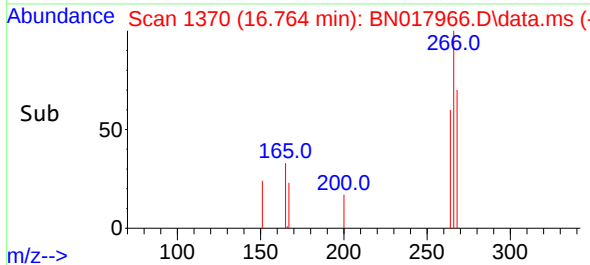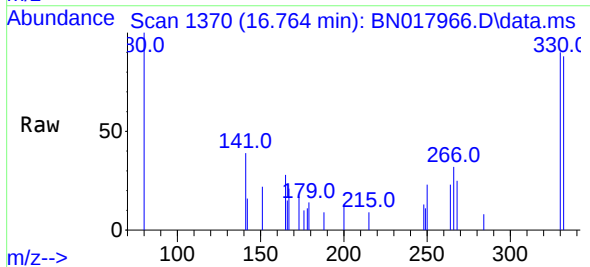



#27
Fluoranthene-d10
Concen: 0.320 ng
RT: 19.129 min Scan# 1697
Delta R.T. -0.000 min
Lab File: BN017966.D
Acq: 13 Dec 2021 11:24




Instrument :
BNA_N
ClientSampleId :
RE105D1-20211202




Tgt Ion:212 Resp: 14409
Ion Ratio Lower Upper
212 100
106 10.2 8.3 12.5
104 5.7 4.6 6.8

Manual Integrations
APPROVED



Reviewed By :Christian Giraldo 12/14/2021
Supervised By :Jagrut Upadhyay 12/14/2021

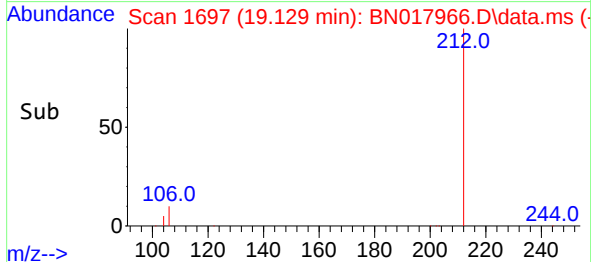


#29
Chrysene-d12
Concen: 0.400 ng
RT: 21.293 min Scan# 1995
Delta R.T. -0.000 min
Lab File: BN017966.D
Acq: 13 Dec 2021 11:24

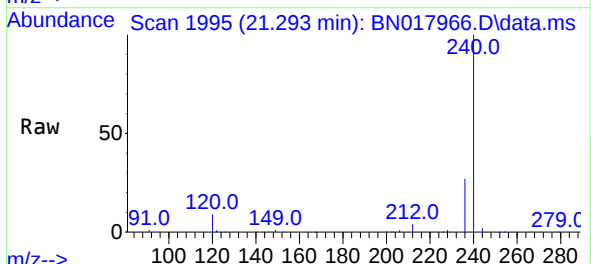


Tgt Ion:240 Resp: 86813
Ion Ratio Lower Upper
240 100
120 8.7 5.8 8.8
236 26.9 21.0 31.6

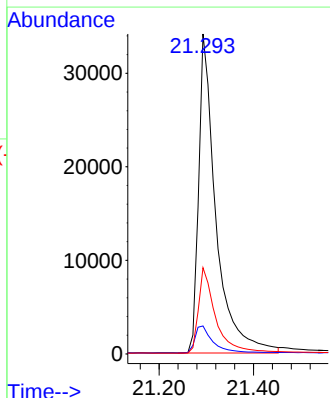



#31
Terphenyl-d14
Concen: 58.461 ng
RT: 19.745 min Scan# 1820
Delta R.T. 0.005 min
Lab File: BN017966.D
Acq: 13 Dec 2021 11:24




Instrument :
BNA_N
ClientSampleId :
RE105D1-20211202



Tgt Ion:244 Resp:1251342
Ion Ratio Lower Upper
244 100
212 8.8 6.2 9.2
122 9.4 7.5 11.3




Manual Integrations
APPROVED


Reviewed By :Christian Giraldo 12/14/2021
Supervised By :Jagrut Upadhyay 12/14/2021

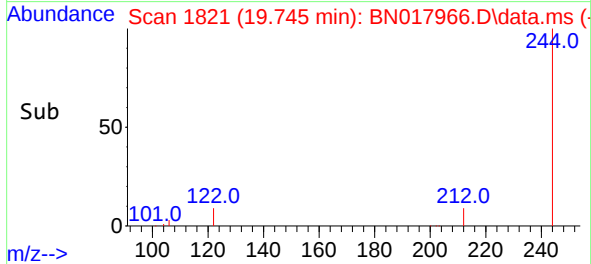

#34
Bis(2-ethylhexyl)phthalate
Concen: 0.067 ng
RT: 21.218 min Scan# 1988
Delta R.T. 0.010 min
Lab File: BN017966.D
Acq: 13 Dec 2021 11:24

Tgt Ion:149 Resp: 6222
Ion Ratio Lower Upper
149 100
167 28.8 23.4 35.0
279 4.3 3.6 5.4

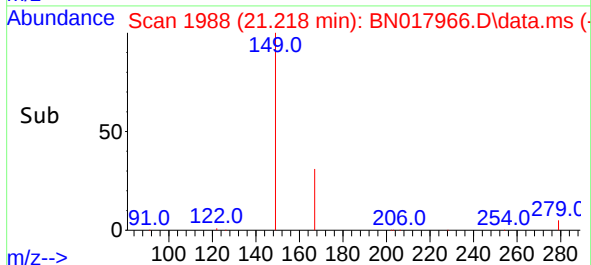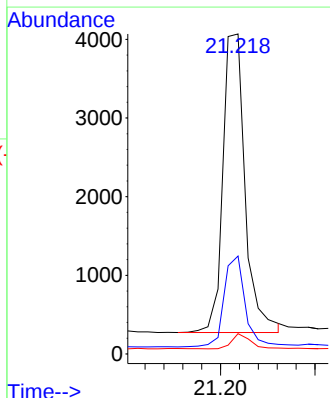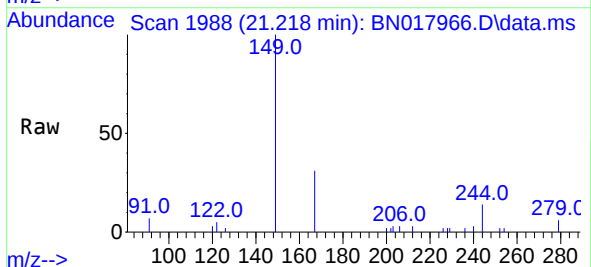

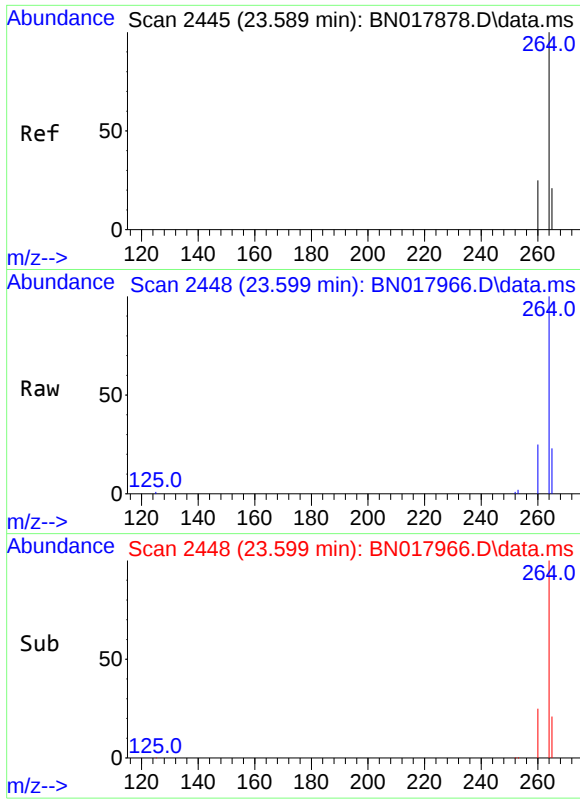

#35
 Perylene-d12
 Concen: 0.400 ng
 RT: 23.599 min Scan# 24
 Delta R.T. 0.010 min
 Lab File: BN017966.D
 Acq: 13 Dec 2021 11:24

Instrument :
 BNA_N
 ClientSampleId :
 RE105D1-20211202

Tgt Ion:264	Resp:	43089
Ion Ratio	Lower	Upper
264	100	
260	25.2	20.2 30.4
265	23.4	18.2 27.4

Manual Integrations
 APPROVED

Reviewed By :Christian Giraldo 12/14/2021
 Supervised By :Jagrut Upadhyay 12/14/2021

