


Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN121321\
 Data File : BN017963.D
 Acq On : 13 Dec 2021 09:23
 Operator : CG/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\8270-SIM-BN121121.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Sat Dec 11 00:01:30 2021

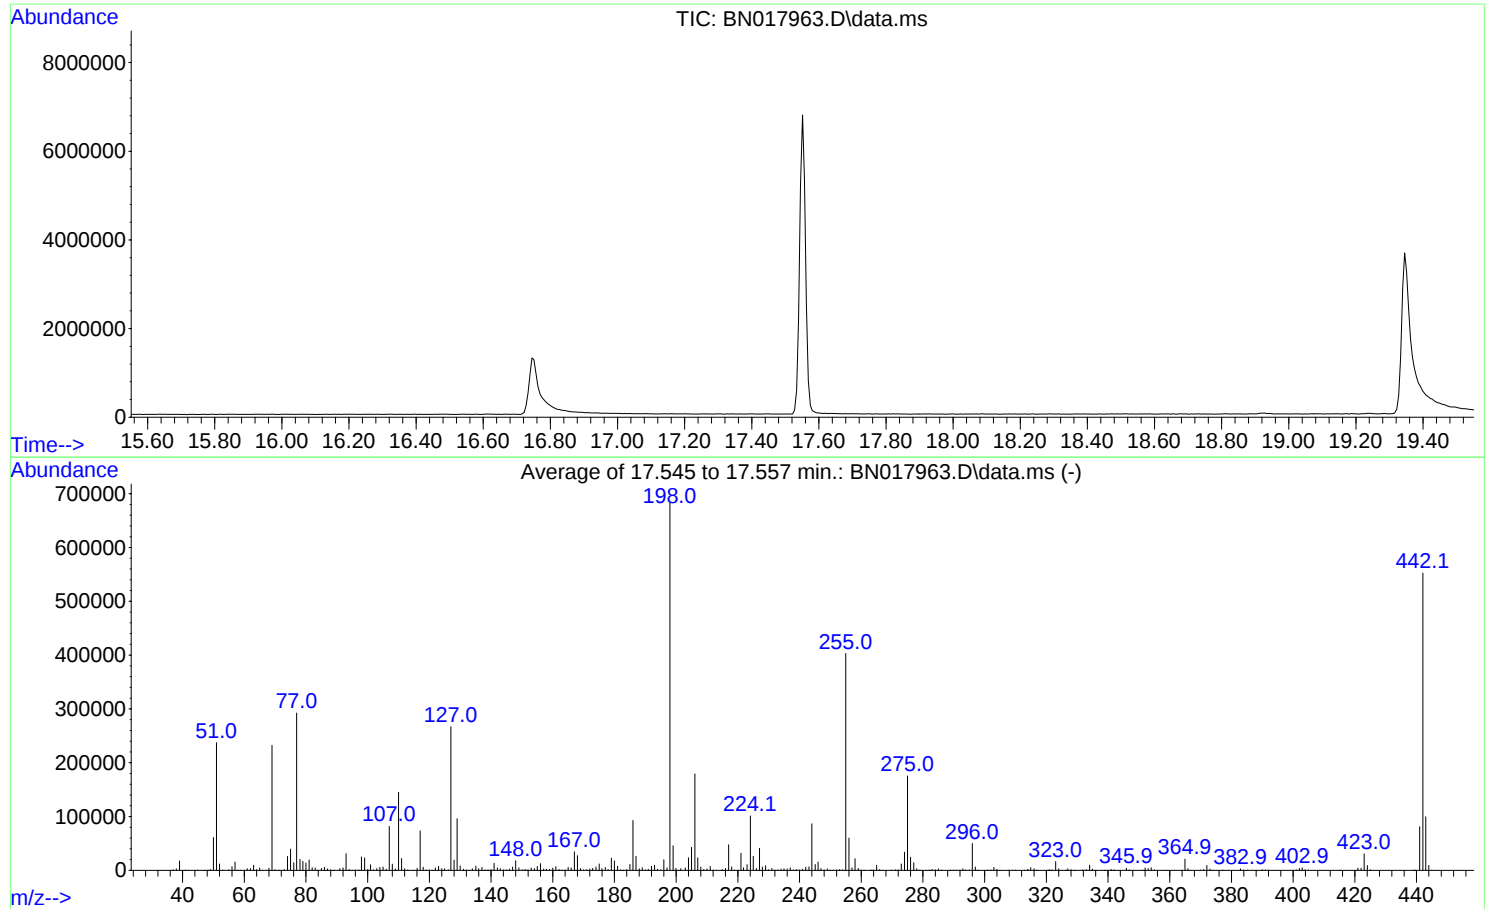




AutoFind: Scans 2475, 2476, 2477; Background Corrected with Scan 2468

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	34.7	237269	PASS
68	69	0.00	2	1.8	4218	PASS
69	198	0.00	100	34.0	232149	PASS
70	69	0.00	2	0.5	1170	PASS
127	198	10	80	39.1	266965	PASS
197	198	0.00	2	0.7	4708	PASS
198	198	100	100	100.0	683541	PASS
199	198	5	9	6.7	45669	PASS
275	198	10	60	25.7	175381	PASS
365	198	1	100	3.0	20787	PASS
441	198	0.01	100	11.9	81176	PASS
442	442	50	100	100.0	552491	PASS
443	442	15	24	18.0	99693	PASS

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN121321\
Data File : BN017963.D
Acq On : 13 Dec 2021 09:23
Operator : CG/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
DFTPP

Quant Time: Dec 14 05:37:21 2021
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\8270E-Tune.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Dec 14 05:37:16 2021
Response via : Initial Calibration

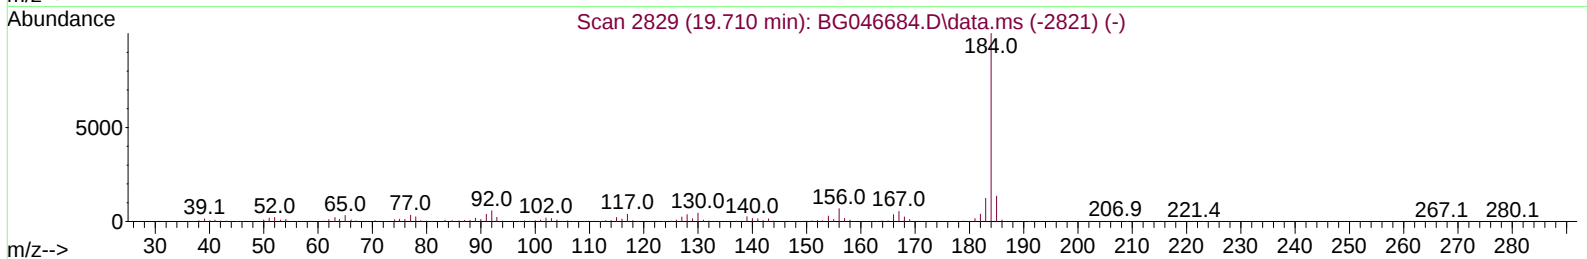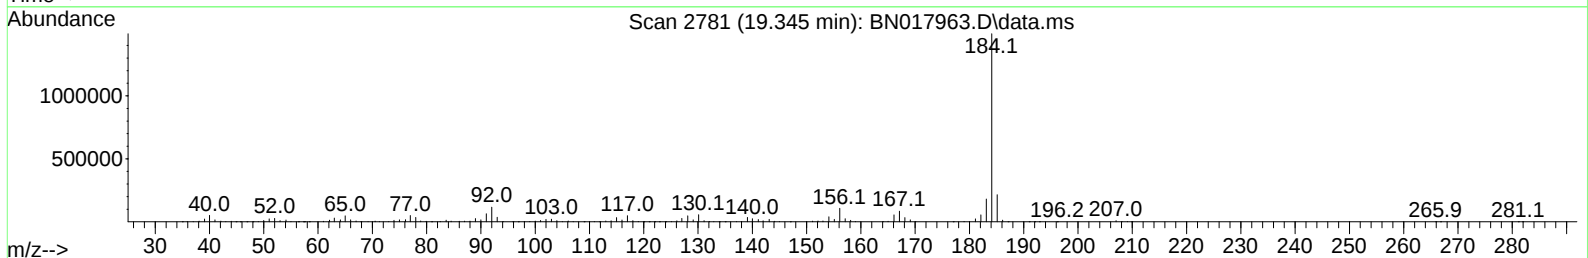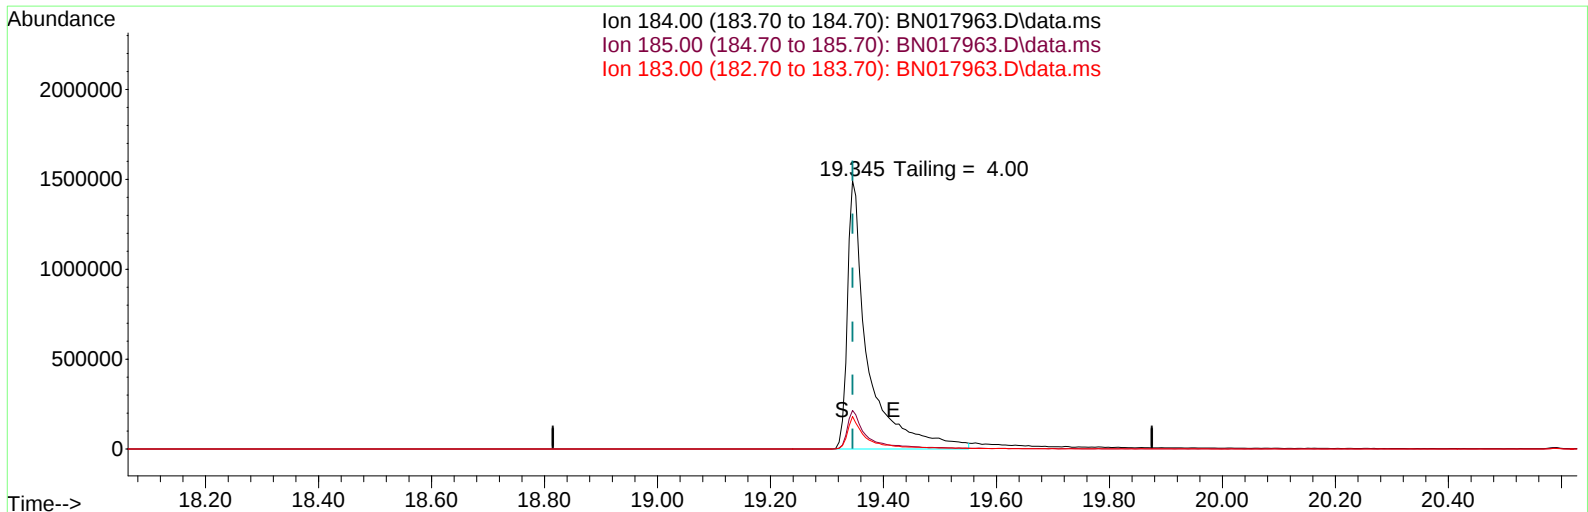

TIC: BN017963.D\data.ms

(77) Benzidine

19.345min (0.000) 0.00 ng




response 3902762

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	15.50	14.41
183.00	13.20	12.11
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN121321\
Data File : BN017963.D
Acq On : 13 Dec 2021 09:23
Operator : CG/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
DFTPP

Quant Time: Dec 14 05:37:21 2021
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\8270E-Tune.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Dec 14 05:37:16 2021
Response via : Initial Calibration

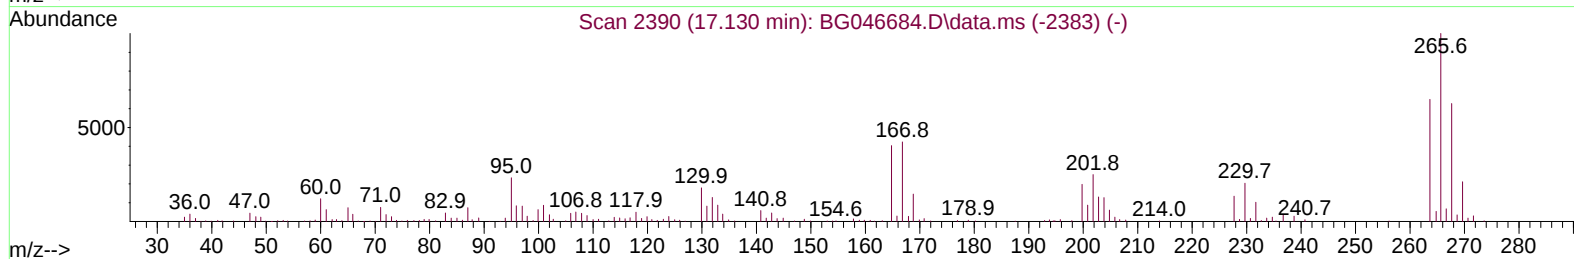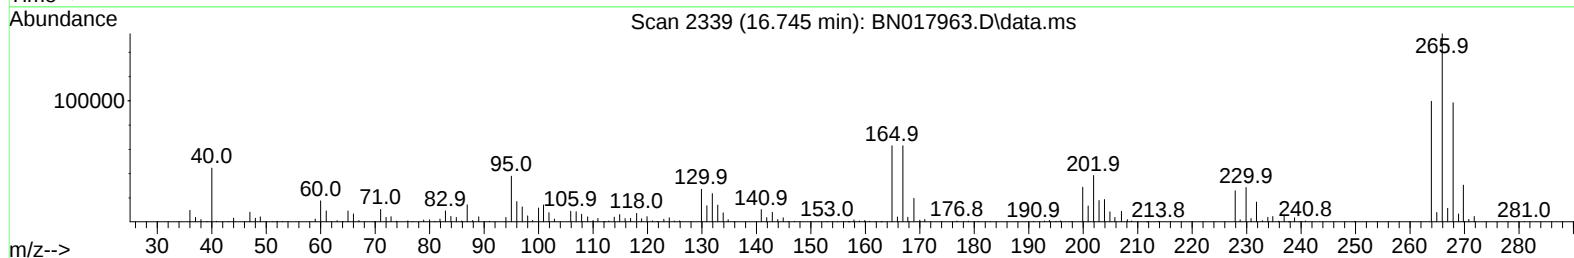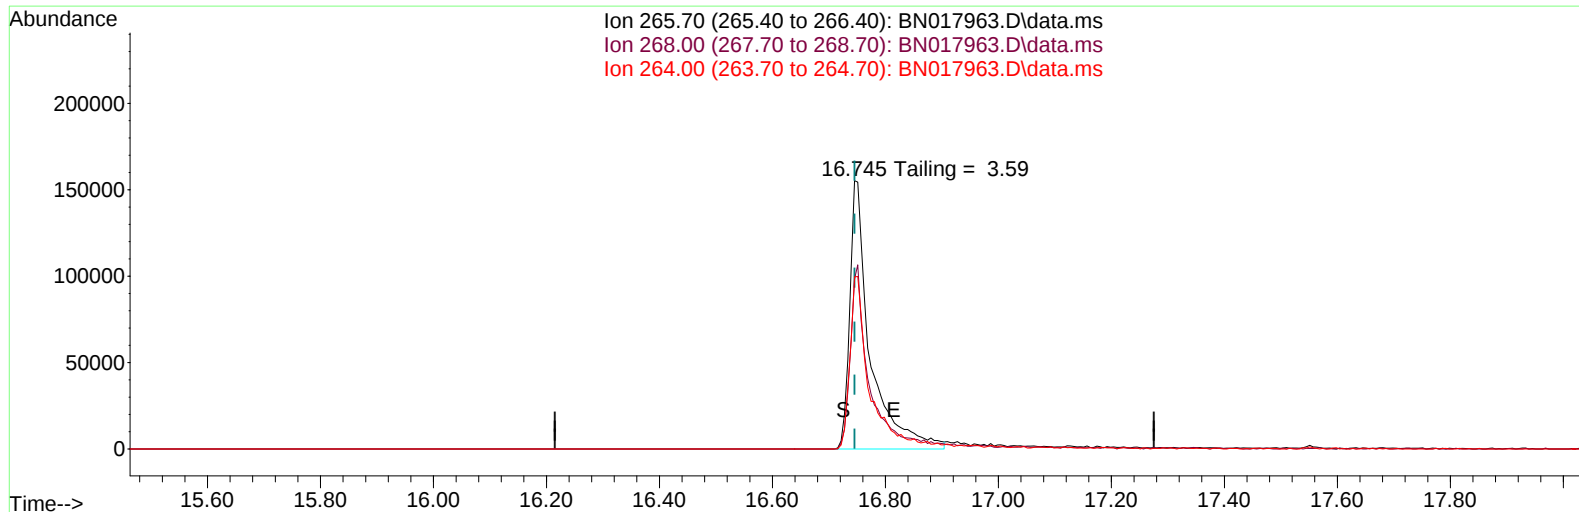

TIC: BN017963.D\data.ms

(70) Pentachlorophenol (C)

16.745min (0.000) 11598.31 ng

response 402220

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	62.20	63.41
264.00	61.60	64.14
0.00	0.00	0.00

DDT Breakdown

Date	Instrument Name	DFTPP Data File
12/13/2021	BNA_N	<u>BN017963.D</u>
Compound Name	Response	Retention Time
DDT	1915796	20.586
DDD	149979	20.151
DDE	9031	19.639
SUM(DDD+DDE)	SUM(DDT+DDD+DDE)	% Breakdown Of DDT
159010	2074806	7.66

Instrument :
BNA_N
ClientSampleId :
DFTPP