

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN121322\
 Data File : BN023158.D
 Acq On : 13 Dec 2022 10:58
 Operator : CG/JU
 Sample : PB149494BL
 Misc :
 ALS Vial : 3 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 SBLK494

Quant Time: Dec 13 23:58:19 2022
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SFAM-EPA-SIM-BN112622.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Tue Dec 13 23:52:47 2022
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Dichlorobenzene-d4	8.015	152	9196	0.400	ng/ul	0.00
4) Naphthalene-d8	10.836	136	30202	0.400	ng/ul	0.00
9) Acenaphthene-d10	14.662	164	18146	0.400	ng/ul	0.00
13) Phenanthrene-d10	17.406	188	41700	0.400	ng/ul	0.00
17) Chrysene-d12	21.590	240	34916	0.400	ng/ul	0.00
23) Perylene-d12	24.045	264	34026	0.400	ng/ul	# 0.00
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.361	96	48558	4.400	ng/ul	0.00
6) 2-Methylnaphthalene-d10	12.420	152	11997	0.261	ng/ul	0.00
18) Fluoranthene-d10	19.433	212	28725	0.223	ng/ul	0.00
Target Compounds						
					Qvalue	
5) Naphthalene	10.852	128	6867	0.075	ng/ul#	86
20) Pyrene	19.800	202	4811	0.027	ng/ul#	1
26) Benzo(a)pyrene	23.893	252	9576	0.073	ng/ul#	61


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN121322\
Data File : BN023158.D
Acq On : 13 Dec 2022 10:58
Operator : CG/JU
Sample : PB149494BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
SBLK494

Quant Time: Dec 13 23:58:19 2022
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SFAM-EPA-SIM-BN112622.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Dec 13 23:52:47 2022
Response via : Initial Calibration




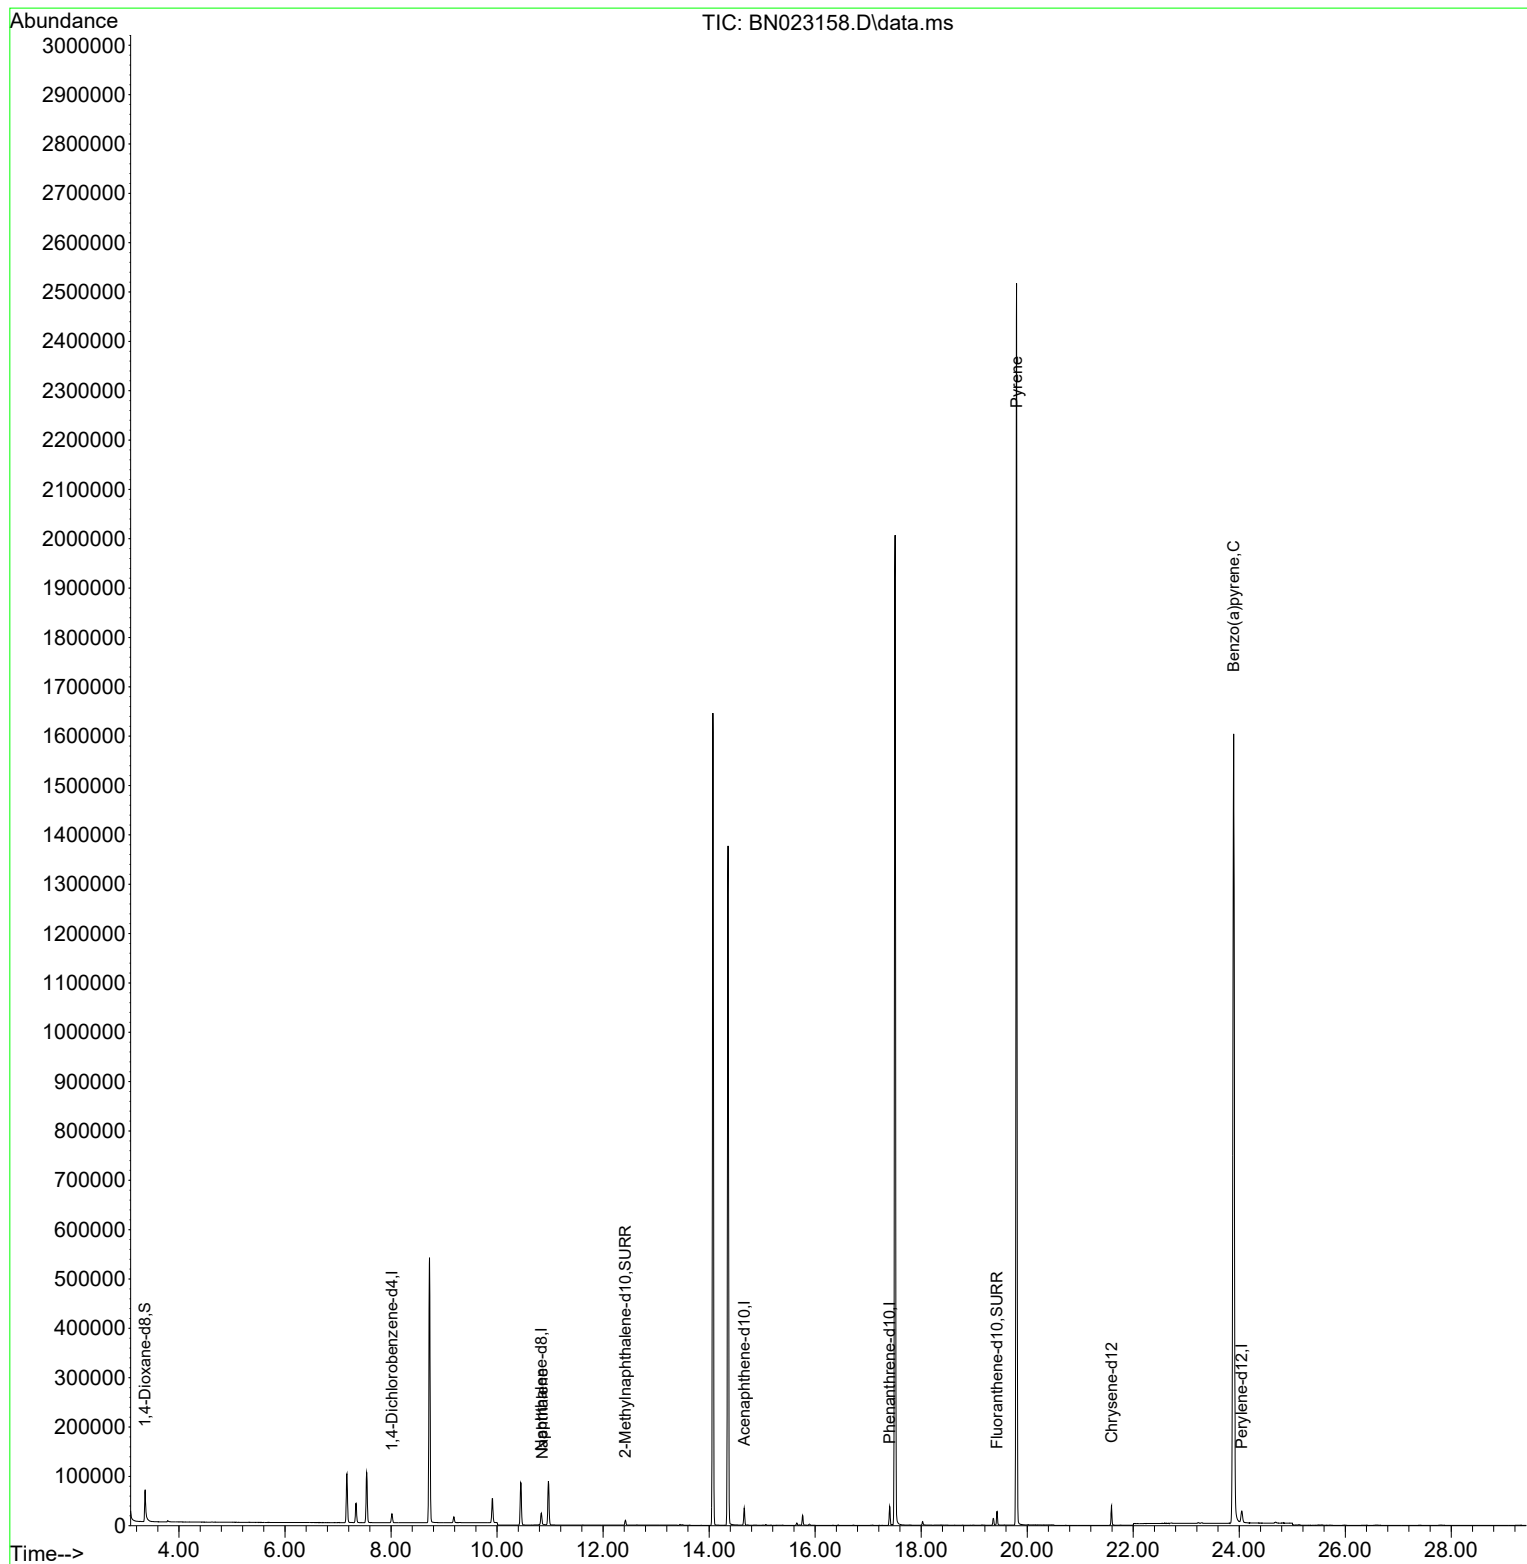


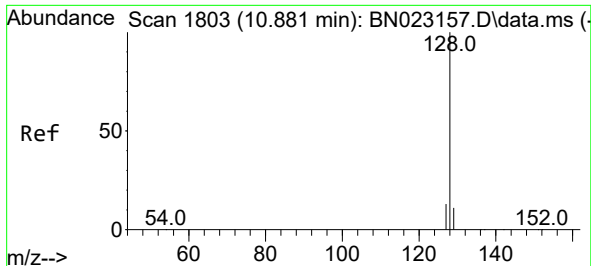

#5
Naphthalene
Concen: 0.075 ng/ul
RT: 10.852 min Scan# 11
Delta R.T. -0.029 min
Lab File: BN023158.D
Acq: 13 Dec 2022 10:58




Instrument :
BNA_N
ClientSampleId :
SBLK494


Tgt Ion:128 Resp: 6867
Ion Ratio Lower Upper
128 100
129 18.7 9.0 13.6#
127 17.1 10.6 16.0#

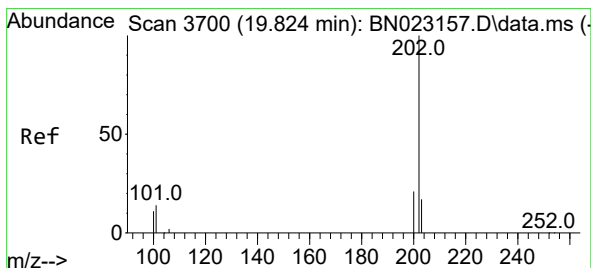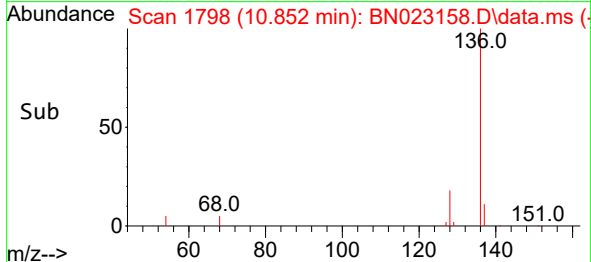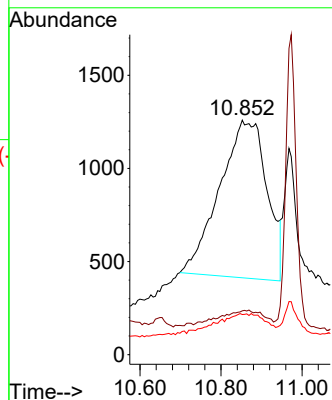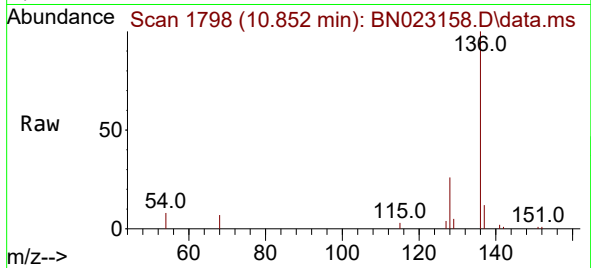

#20
Pyrene
Concen: 0.027 ng/ul
RT: 19.800 min Scan# 3695
Delta R.T. -0.024 min
Lab File: BN023158.D
Acq: 13 Dec 2022 10:58


Tgt Ion:202 Resp: 4811
Ion Ratio Lower Upper
202 100
101 159.0 10.6 16.0#
100 1132.2 8.2 12.4#

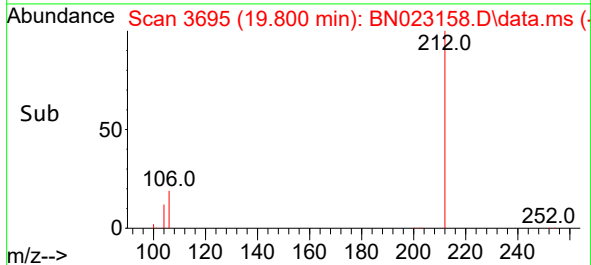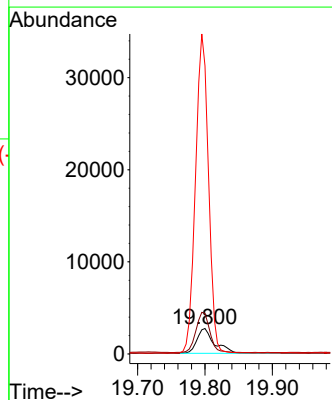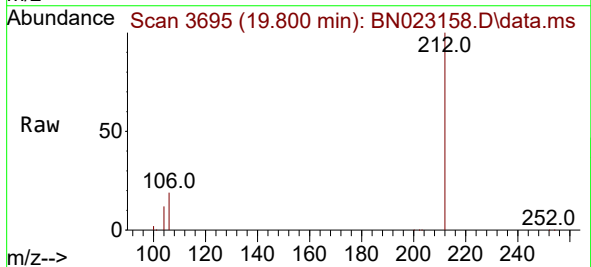

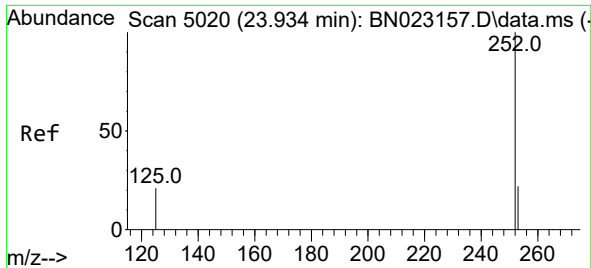

#26
 Benzo(a)pyrene
 Concen: 0.073 ng/ul
 RT: 23.893 min Scan# 50
 Delta R.T. -0.040 min
 Lab File: BN023158.D
 Acq: 13 Dec 2022 10:58

Instrument :
 BNA_N
 ClientSampleId :
 SBLK494

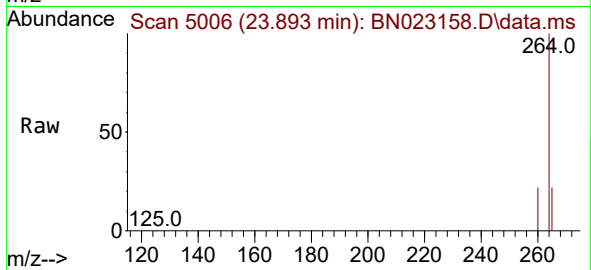

Tgt Ion:252 Resp: 9576
 Ion Ratio Lower Upper
 252 100
 253 41.9 19.7 29.5#
 125 36.6 13.7 20.5#

