

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN121322\
 Data File : BN023169.D
 Acq On : 13 Dec 2022 17:42
 Operator : CG/JU
 Sample : N5927-01
 Misc :
 ALS Vial : 14 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 EXZ85

Quant Time: Dec 13 23:59:40 2022
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SFAM-EPA-SIM-BN112622.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Tue Dec 13 23:52:47 2022
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Dichlorobenzene-d4	8.019	152	5872	0.400	ng/ul	0.00
4) Naphthalene-d8	10.837	136	19356	0.400	ng/ul	0.00
9) Acenaphthene-d10	14.664	164	11690	0.400	ng/ul	0.00
13) Phenanthrene-d10	17.407	188	27351	0.400	ng/ul	0.00
17) Chrysene-d12	21.590	240	24887	0.400	ng/ul	0.00
23) Perylene-d12	24.048	264	24016	0.400	ng/ul	0.00
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.357	96	22953	3.257	ng/ul	0.00
6) 2-Methylnaphthalene-d10	12.421	152	8014	0.272	ng/ul	0.00
18) Fluoranthene-d10	19.429	212	21651	0.235	ng/ul	0.00
Target Compounds						
					Qvalue	
2) 1,4-Dioxane	3.395	88	712	0.097	ng/ul#	36
20) Pyrene	19.797	202	3470	0.028	ng/ul#	1
26) Benzo(a)pyrene	23.893	252	7676	0.083	ng/ul#	57


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN121322\
Data File : BN023169.D
Acq On : 13 Dec 2022 17:42
Operator : CG/JU
Sample : N5927-01
Misc :
ALS Vial : 14 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
EXZ85

Quant Time: Dec 13 23:59:40 2022
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SFAM-EPA-SIM-BN112622.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Dec 13 23:52:47 2022
Response via : Initial Calibration




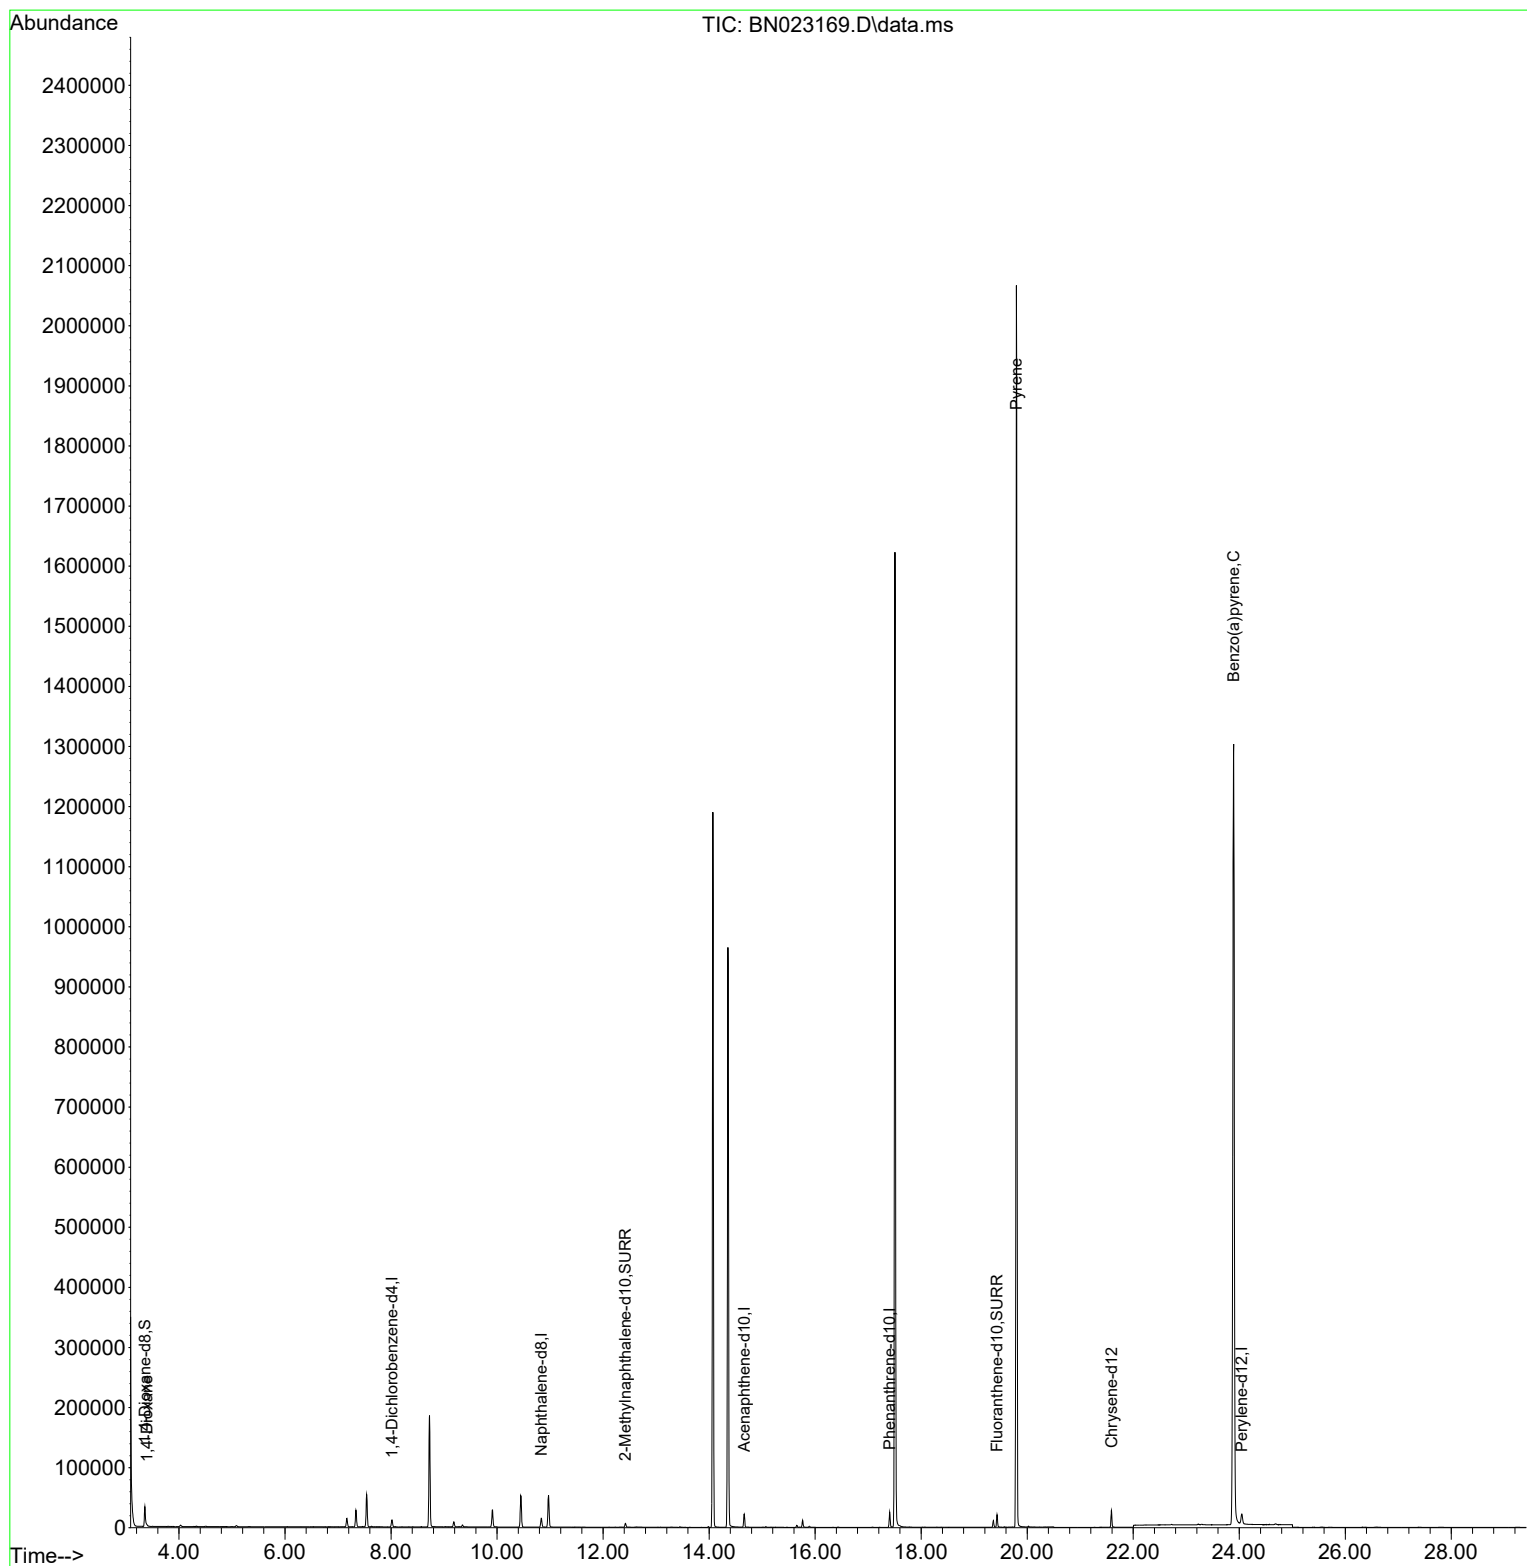


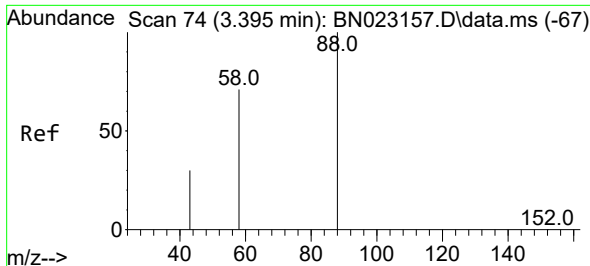

#2
1,4-Dioxane
Concen: 0.097 ng/ul
RT: 3.395 min Scan# 74
Delta R.T. 0.000 min
Lab File: BN023169.D
Acq: 13 Dec 2022 17:42




Instrument :
BNA_N
ClientSampleId :
EXZ85


Tgt Ion: 88 Resp: 712
Ion Ratio Lower Upper
88 100
43 124.1 26.2 39.4#
58 51.6 47.6 71.4

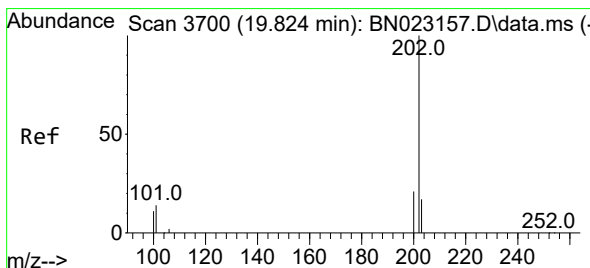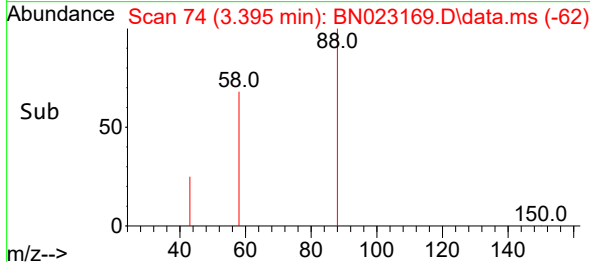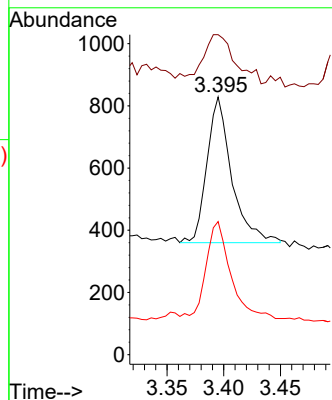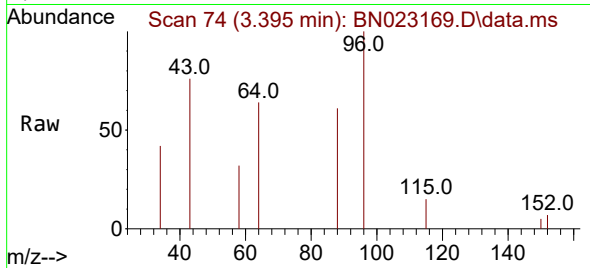

#20
Pyrene
Concen: 0.028 ng/ul
RT: 19.797 min Scan# 3694
Delta R.T. -0.028 min
Lab File: BN023169.D
Acq: 13 Dec 2022 17:42

Tgt Ion: 202 Resp: 3470
Ion Ratio Lower Upper
202 100
101 163.9 10.6 16.0#
100 1215.4 8.2 12.4#

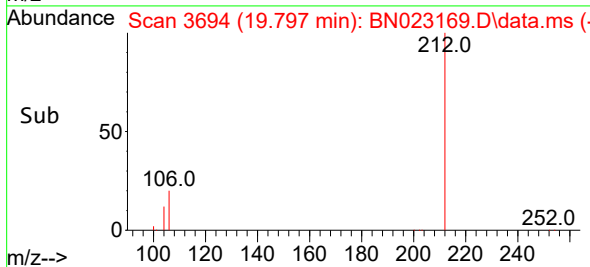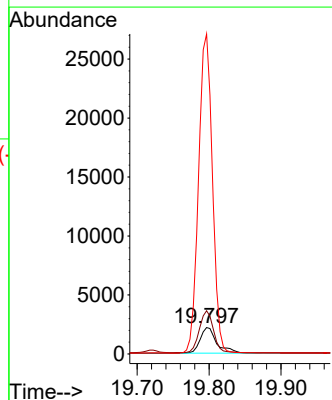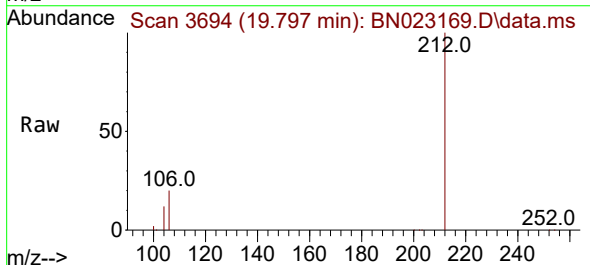

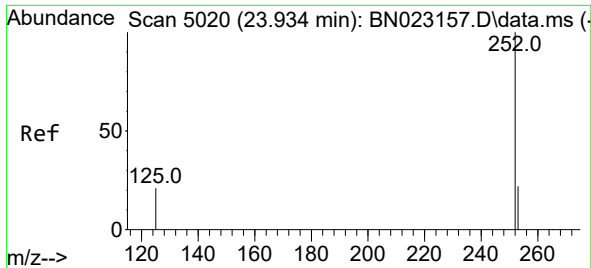

#26

Benzo(a)pyrene

Concen: 0.083 ng/ul

RT: 23.893 min Scan# 50

Delta R.T. -0.041 min

Lab File: BN023169.D


Acq: 13 Dec 2022 17:42

Instrument :

BNA_N

ClientSampleId :

EXZ85

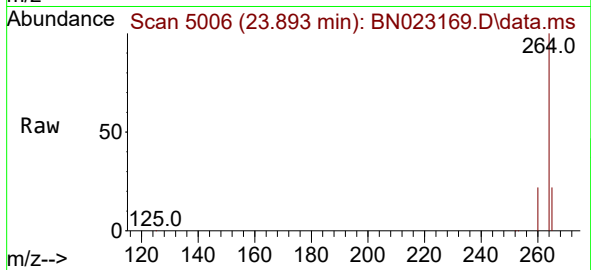

Tgt Ion:252 Resp: 7676

Ion Ratio Lower Upper

252 100

253 43.6 19.7 29.5#

125 38.5 13.7 20.5#

