

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN121322\
 Data File : BN023170.D
 Acq On : 13 Dec 2022 18:19
 Operator : CG/JU
 Sample : N5927-02
 Misc :
 ALS Vial : 15 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 EXZ87

Quant Time: Dec 13 23:59:45 2022
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SFAM-EPA-SIM-BN112622.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Tue Dec 13 23:52:47 2022
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Dichlorobenzene-d4	8.015	152	6836	0.400	ng/ul	0.00
4) Naphthalene-d8	10.836	136	22346	0.400	ng/ul	0.00
9) Acenaphthene-d10	14.662	164	13543	0.400	ng/ul	0.00
13) Phenanthrene-d10	17.406	188	30809	0.400	ng/ul	0.00
17) Chrysene-d12	21.590	240	27225	0.400	ng/ul	0.00
23) Perylene-d12	24.045	264	26050	0.400	ng/ul	0.00
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.357	96	23902	2.914	ng/ul	0.00
6) 2-Methylnaphthalene-d10	12.420	152	9066	0.266	ng/ul	0.00
18) Fluoranthene-d10	19.432	212	24933	0.248	ng/ul	0.00
Target Compounds						
					Qvalue	
2) 1,4-Dioxane	3.395	88	5496	0.642	ng/ul#	91
20) Pyrene	19.800	202	4191	0.030	ng/ul#	1
26) Benzo(a)pyrene	23.893	252	8776	0.087	ng/ul#	62


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN121322\
Data File : BN023170.D
Acq On : 13 Dec 2022 18:19
Operator : CG/JU
Sample : N5927-02
Misc :
ALS Vial : 15 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
EXZ87

Quant Time: Dec 13 23:59:45 2022
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SFAM-EPA-SIM-BN112622.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Dec 13 23:52:47 2022
Response via : Initial Calibration




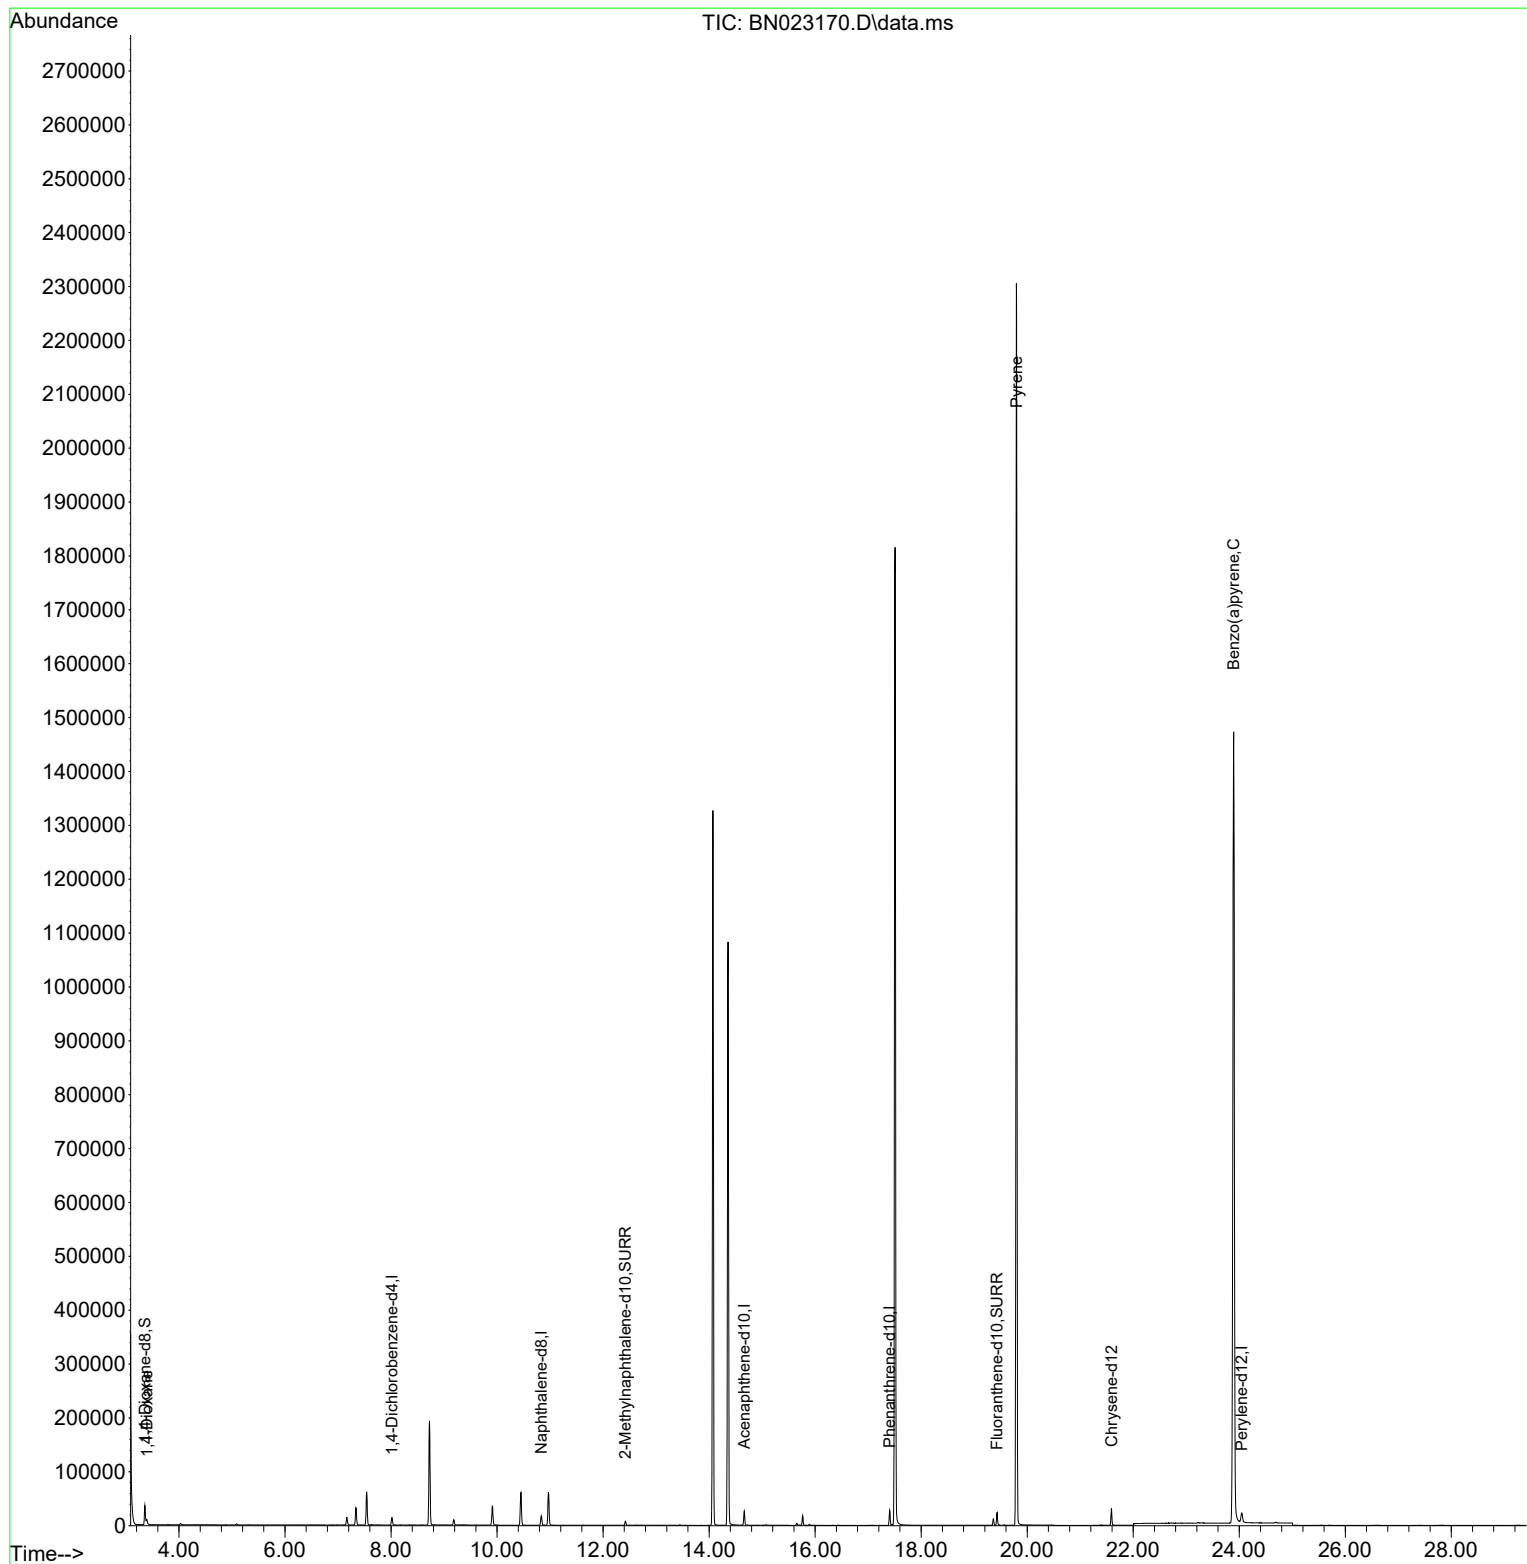


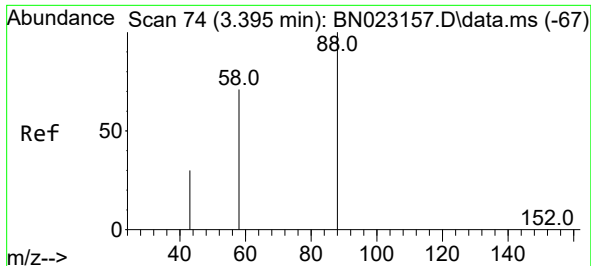

#2
1,4-Dioxane
Concen: 0.642 ng/ul
RT: 3.395 min Scan# 74
Delta R.T. 0.000 min
Lab File: BN023170.D
Acq: 13 Dec 2022 18:19




Instrument :
BNA_N
ClientSampleId :
EXZ87


Tgt Ion: 88 Resp: 5496
Ion Ratio Lower Upper
88 100
43 42.1 26.2 39.4#
58 63.6 47.6 71.4

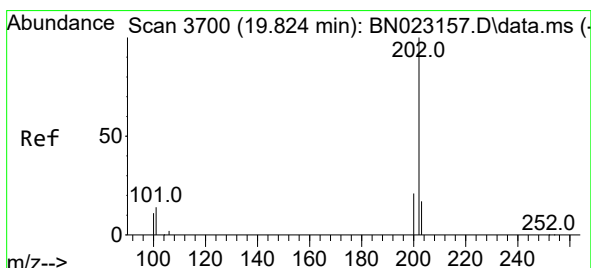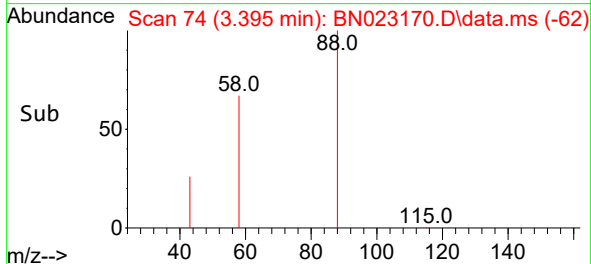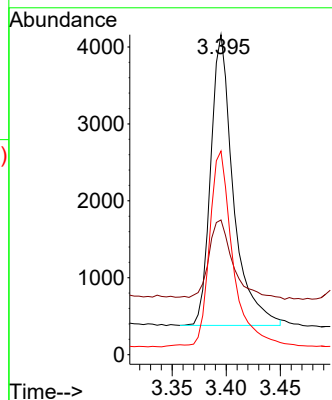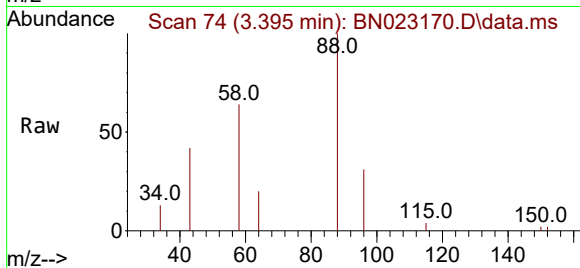

#20
Pyrene
Concen: 0.030 ng/ul
RT: 19.800 min Scan# 3695
Delta R.T. -0.025 min
Lab File: BN023170.D
Acq: 13 Dec 2022 18:19


Tgt Ion: 202 Resp: 4191
Ion Ratio Lower Upper
202 100
101 155.3 10.6 16.0#
100 1102.0 8.2 12.4#

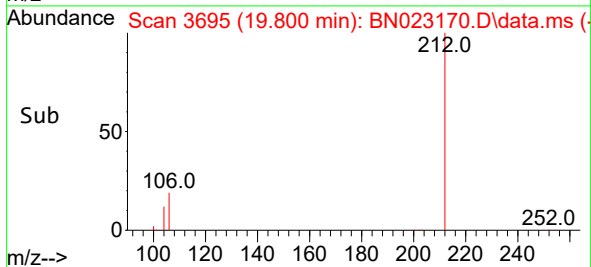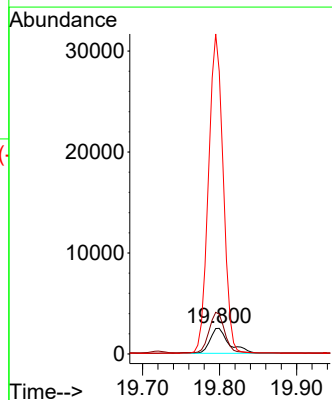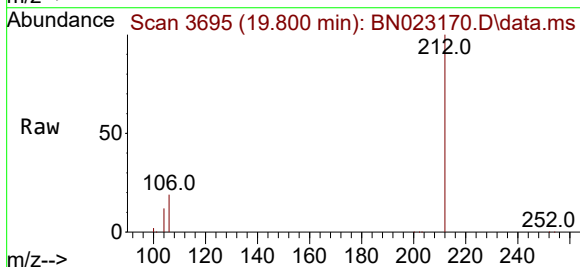

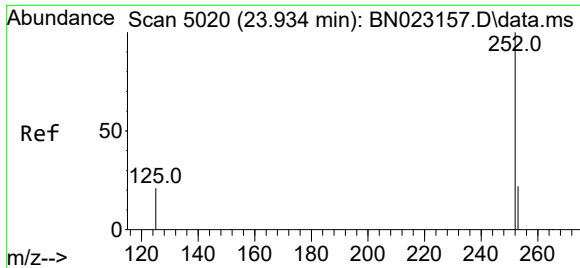

#26
Benzo(a)pyrene
Concen: 0.087 ng/ul
RT: 23.893 min Scan# 5006
Delta R.T. -0.041 min
Lab File: BN023170.D
Acq: 13 Dec 2022 18:19

Instrument :
BNA_N
ClientSampleId :
EXZ87

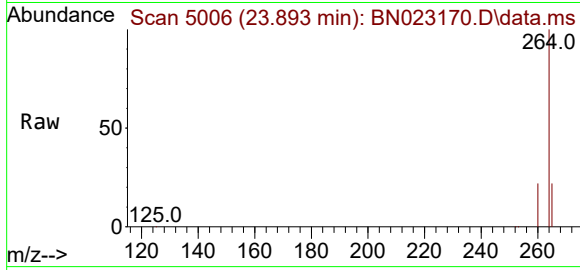

Tgt Ion:252 Resp: 8776
Ion Ratio Lower Upper
252 100
253 41.2 19.7 29.5#
125 36.9 13.7 20.5#

