

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN121322\
 Data File : BN023171.D
 Acq On : 13 Dec 2022 18:56
 Operator : CG/JU
 Sample : N5927-03
 Misc :
 ALS Vial : 16 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 EXZ88

Quant Time: Dec 13 23:59:51 2022
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SFAM-EPA-SIM-BN112622.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Tue Dec 13 23:52:47 2022
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Dichlorobenzene-d4	8.015	152	5604	0.400	ng/ul	0.00
4) Naphthalene-d8	10.837	136	18553	0.400	ng/ul	0.00
9) Acenaphthene-d10	14.660	164	11137	0.400	ng/ul	0.00
13) Phenanthrene-d10	17.404	188	26806	0.400	ng/ul	0.00
17) Chrysene-d12	21.590	240	24947	0.400	ng/ul	0.00
23) Perylene-d12	24.049	264	24288	0.400	ng/ul	0.00
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.357	96	23234	3.455	ng/ul	0.00
6) 2-Methylnaphthalene-d10	12.421	152	7989	0.283	ng/ul	0.00
18) Fluoranthene-d10	19.430	212	24292	0.264	ng/ul	0.00
Target Compounds						
					Qvalue	
2) 1,4-Dioxane	3.395	88	645	0.092	ng/ul#	43
20) Pyrene	19.797	202	3955	0.031	ng/ul#	1
26) Benzo(a)pyrene	23.894	252	8336	0.089	ng/ul#	60


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN121322\
Data File : BN023171.D
Acq On : 13 Dec 2022 18:56
Operator : CG/JU
Sample : N5927-03
Misc :
ALS Vial : 16 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
EXZ88

Quant Time: Dec 13 23:59:51 2022
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SFAM-EPA-SIM-BN112622.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Dec 13 23:52:47 2022
Response via : Initial Calibration




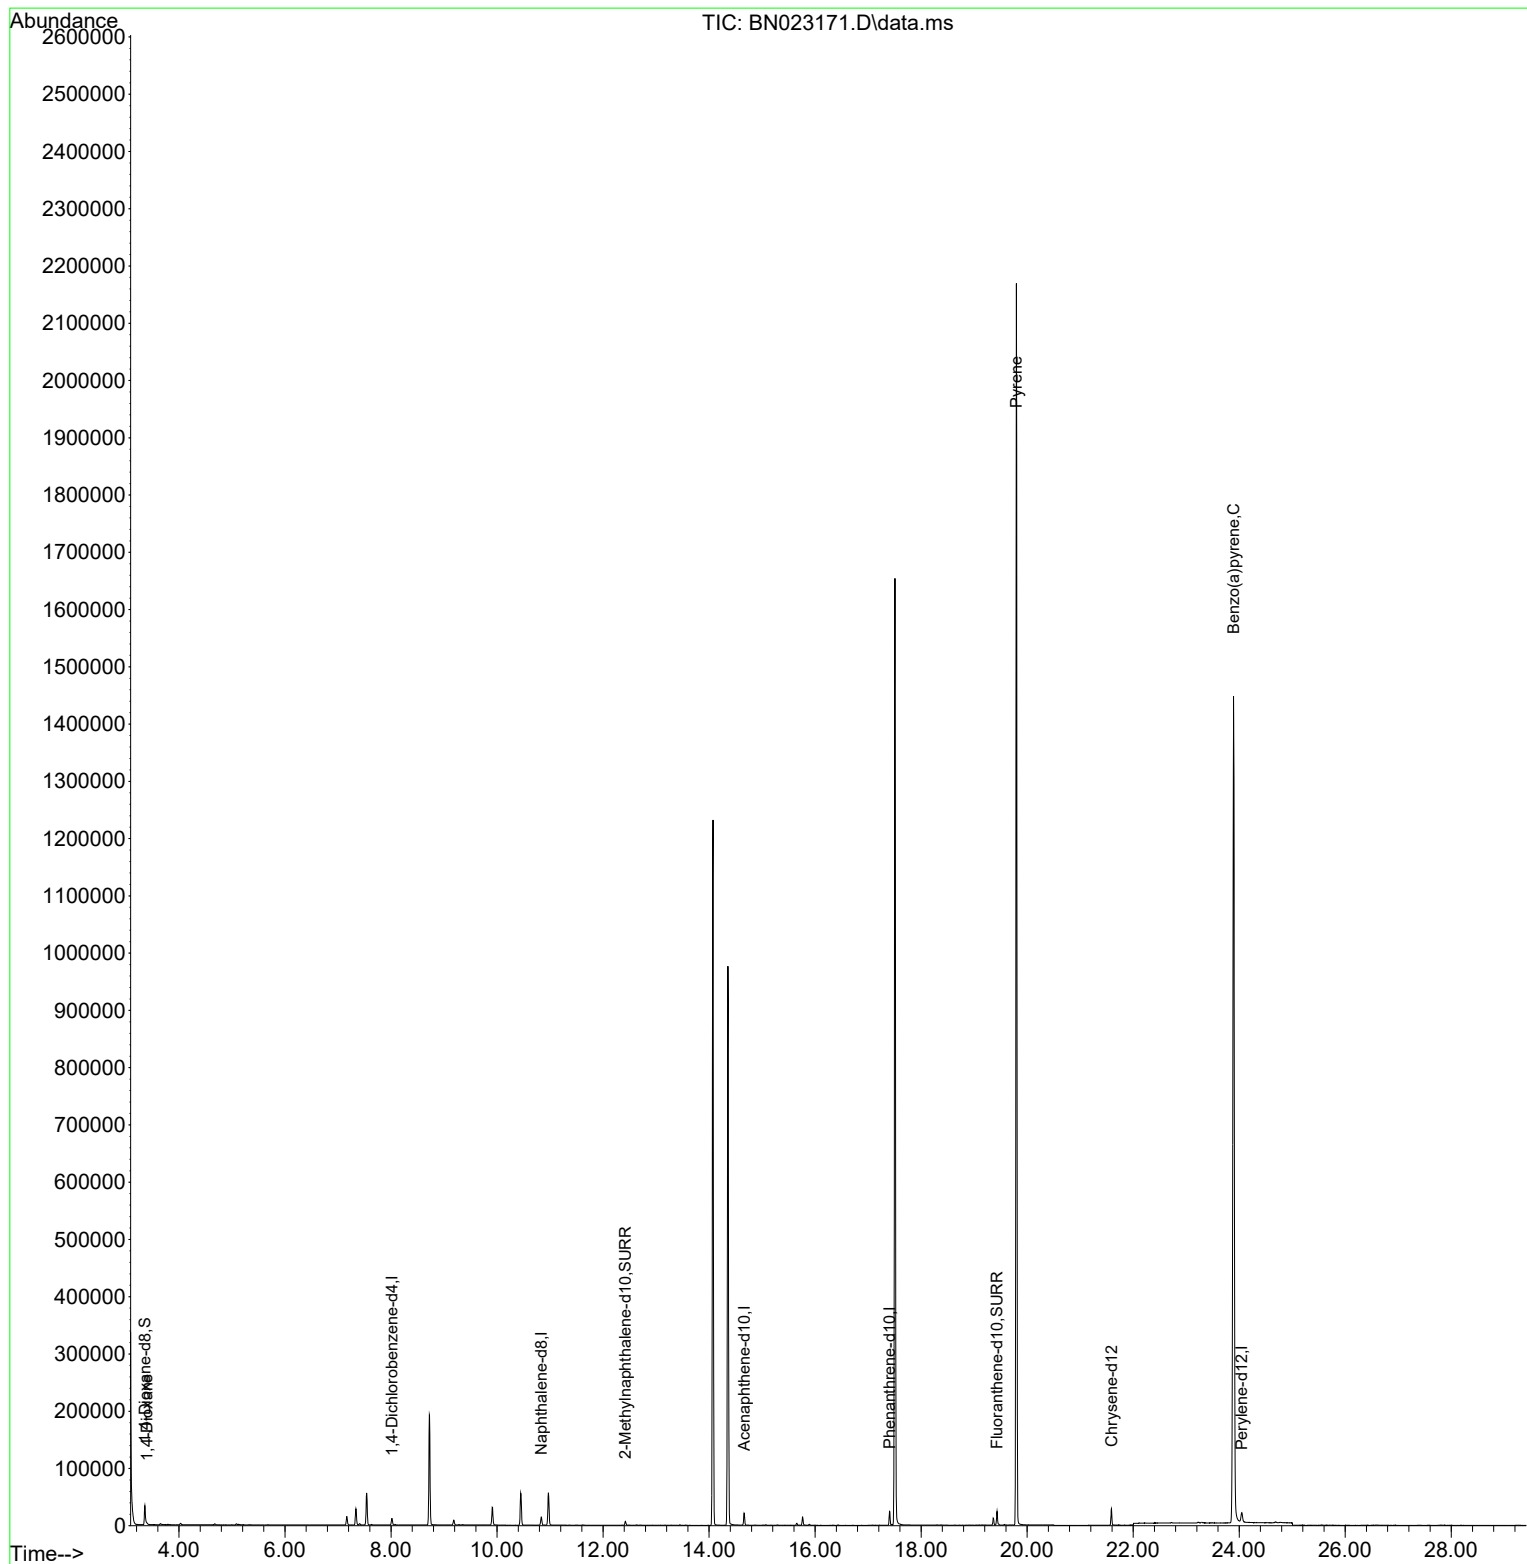


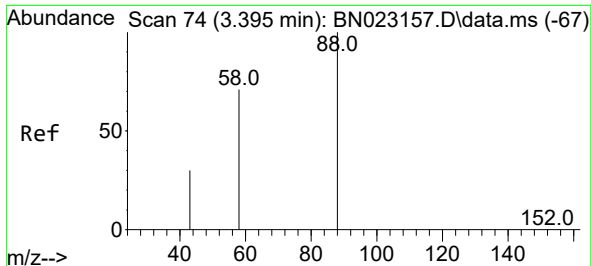

#2
1,4-Dioxane
Concen: 0.092 ng/ul
RT: 3.395 min Scan# 74
Delta R.T. 0.000 min
Lab File: BN023171.D
Acq: 13 Dec 2022 18:56




Instrument :
BNA_N
ClientSampleId :
EXZ88


Tgt Ion: 88 Resp: 645
Ion Ratio Lower Upper
88 100
43 109.4 26.2 39.4#
58 49.1 47.6 71.4

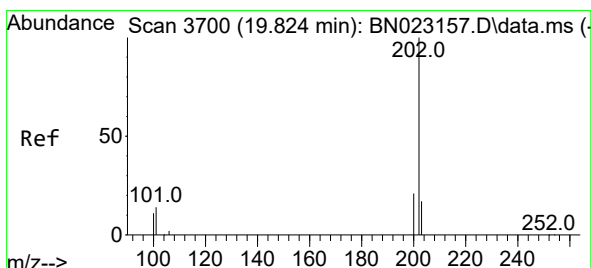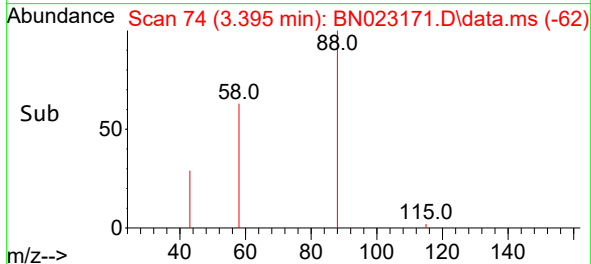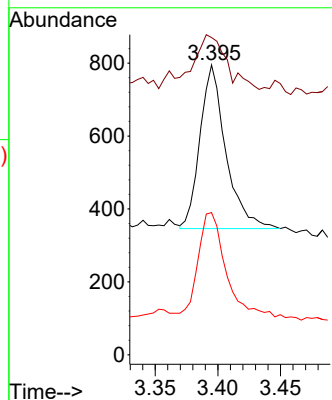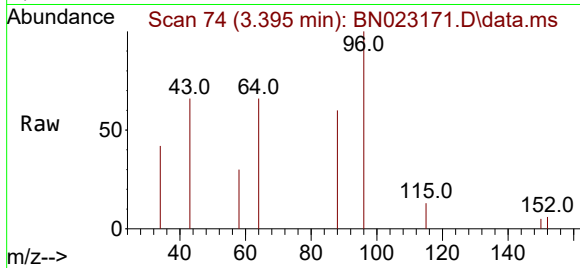

#20
Pyrene
Concen: 0.031 ng/ul
RT: 19.797 min Scan# 3694
Delta R.T. -0.027 min
Lab File: BN023171.D
Acq: 13 Dec 2022 18:56

Tgt Ion: 202 Resp: 3955
Ion Ratio Lower Upper
202 100
101 156.6 10.6 16.0#
100 1169.2 8.2 12.4#

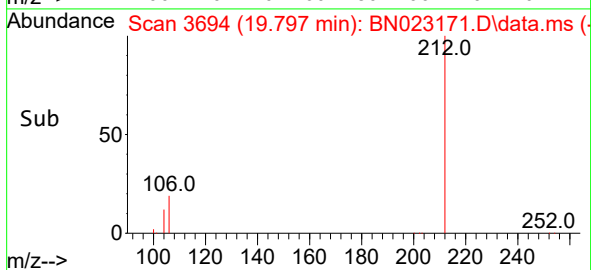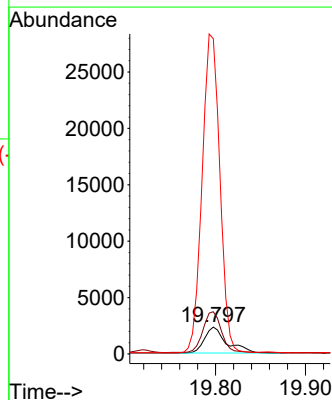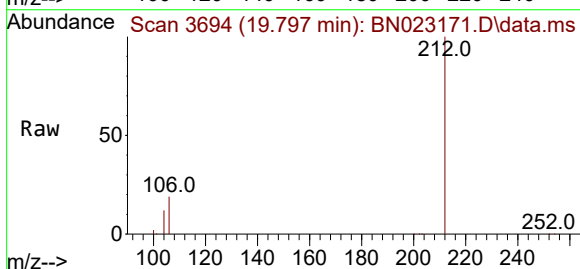

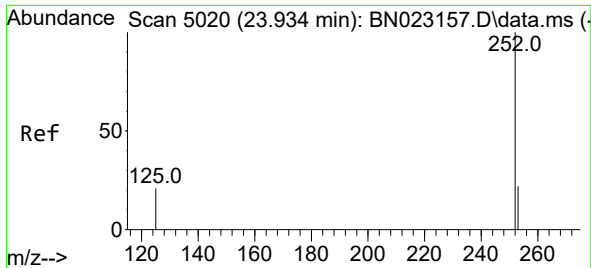

#26

Benzo(a)pyrene

Concen: 0.089 ng/ul

RT: 23.894 min Scan# 50

Delta R.T. -0.040 min

Lab File: BN023171.D


Acq: 13 Dec 2022 18:56

Instrument :

BNA_N

ClientSampleId :

EXZ88

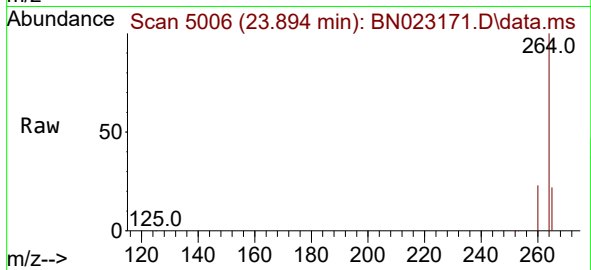

Tgt Ion:252 Resp: 8336

Ion Ratio Lower Upper

252 100

253 42.1 19.7 29.5#

125 37.6 13.7 20.5#

