

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN121322\
 Data File : BN023172.D
 Acq On : 13 Dec 2022 19:33
 Operator : CG/JU
 Sample : N5927-04
 Misc :
 ALS Vial : 17 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 EXZ90

Quant Time: Dec 13 23:59:57 2022
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SFAM-EPA-SIM-BN112622.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Tue Dec 13 23:52:47 2022
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Dichlorobenzene-d4	8.015	152	6326	0.400	ng/ul	0.00
4) Naphthalene-d8	10.837	136	21221	0.400	ng/ul	0.00
9) Acenaphthene-d10	14.660	164	12967	0.400	ng/ul	0.00
13) Phenanthrene-d10	17.408	188	31199	0.400	ng/ul	0.00
17) Chrysene-d12	21.587	240	28052	0.400	ng/ul	0.00
23) Perylene-d12	24.043	264	26425	0.400	ng/ul	0.00
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.357	96	20977	2.763	ng/ul	0.00
6) 2-Methylnaphthalene-d10	12.421	152	8597	0.266	ng/ul	0.00
18) Fluoranthene-d10	19.430	212	25599	0.247	ng/ul	0.00
Target Compounds						
					Qvalue	
2) 1,4-Dioxane	3.395	88	5794	0.732	ng/ul#	91
20) Pyrene	19.797	202	4529	0.032	ng/ul#	1
26) Benzo(a)pyrene	23.888	252	8510	0.083	ng/ul#	61


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN121322\
Data File : BN023172.D
Acq On : 13 Dec 2022 19:33
Operator : CG/JU
Sample : N5927-04
Misc :
ALS Vial : 17 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
EXZ90

Quant Time: Dec 13 23:59:57 2022
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SFAM-EPA-SIM-BN112622.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Dec 13 23:52:47 2022
Response via : Initial Calibration




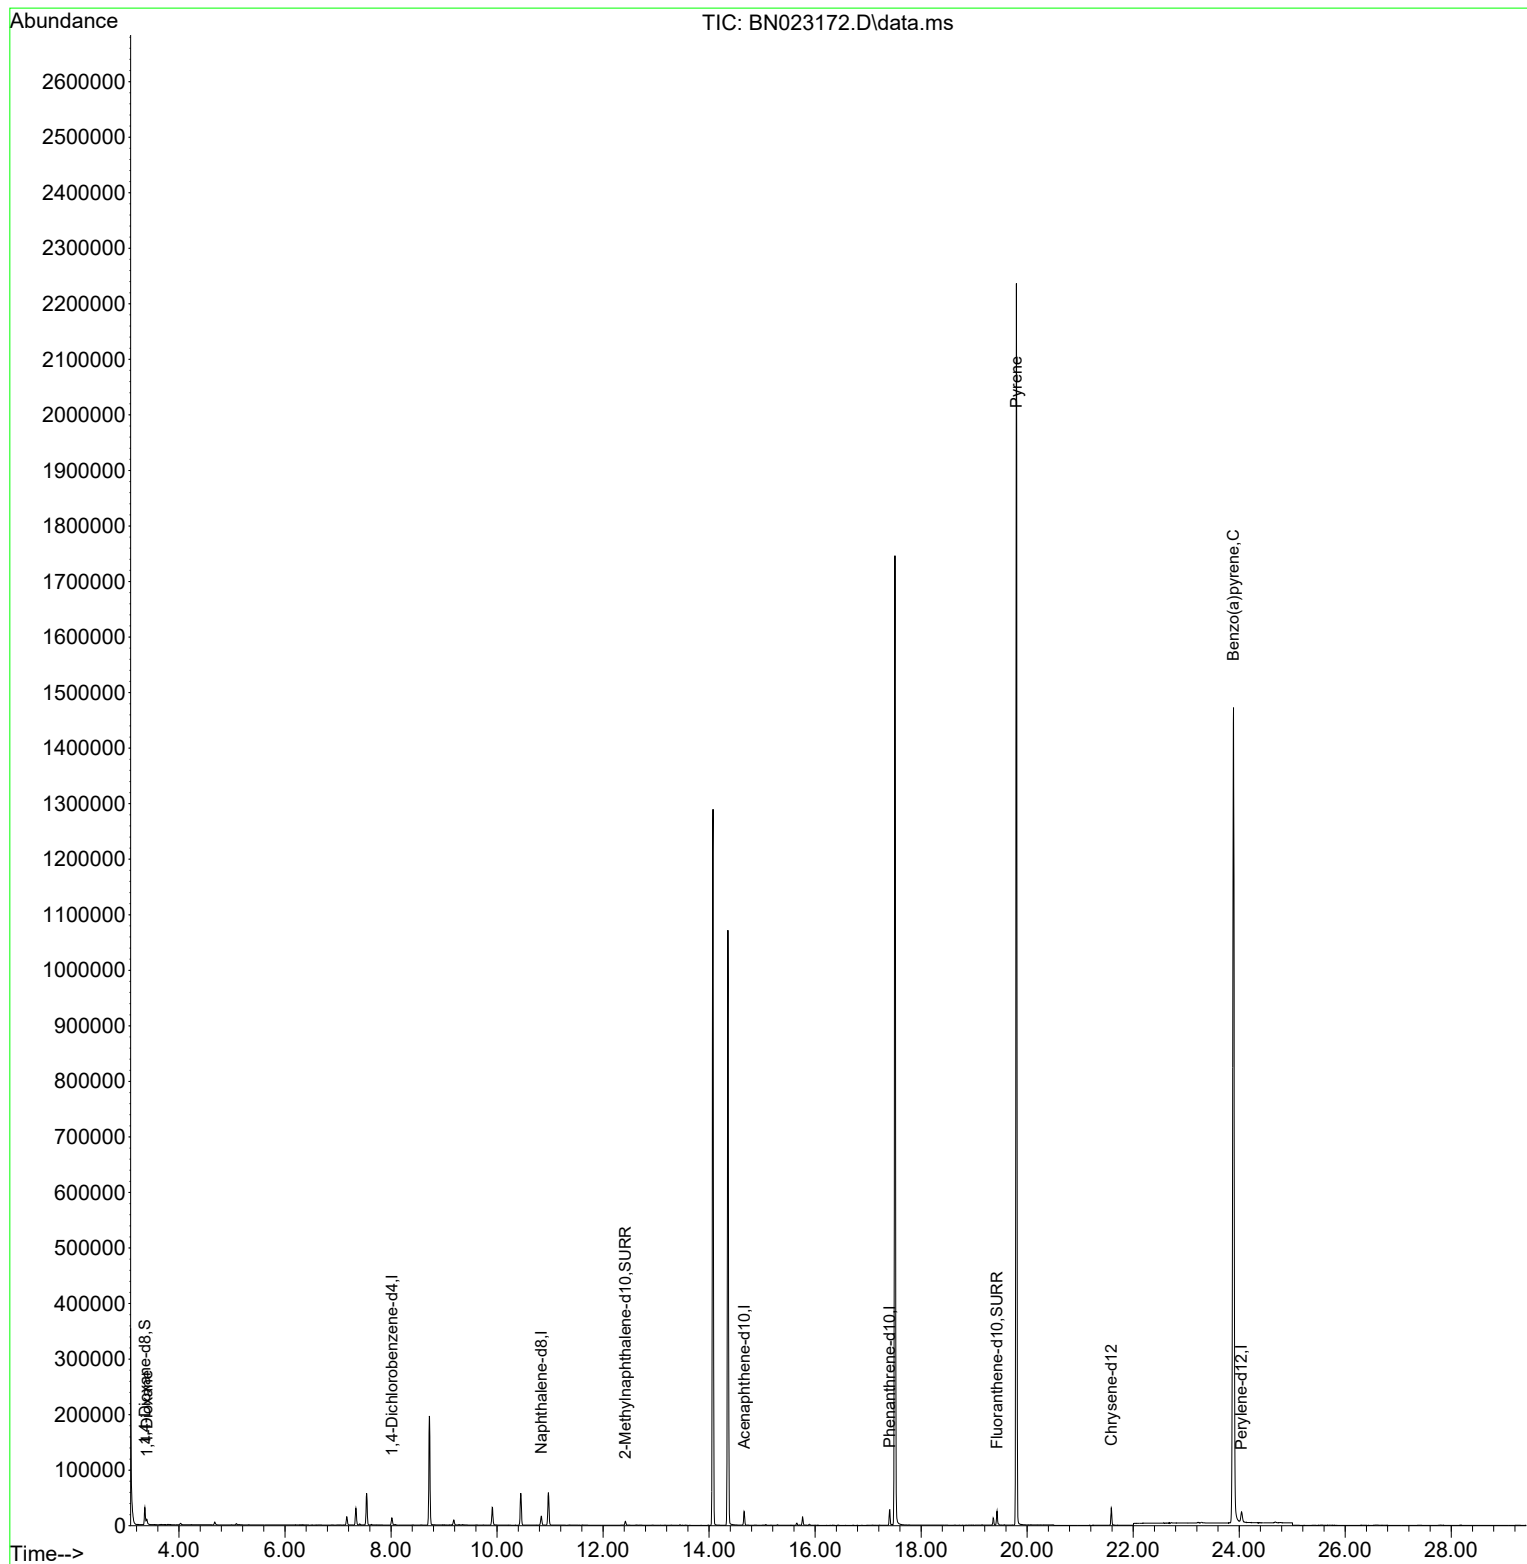


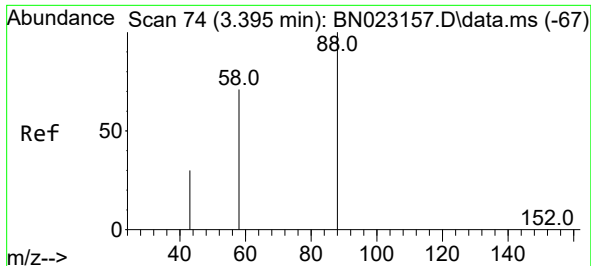

#2
1,4-Dioxane
Concen: 0.732 ng/ul
RT: 3.395 min Scan# 74
Delta R.T. 0.000 min
Lab File: BN023172.D
Acq: 13 Dec 2022 19:33




Instrument :
BNA_N
ClientSampleId :
EXZ90


Tgt Ion: 88 Resp: 5794
Ion Ratio Lower Upper
88 100
43 41.1 26.2 39.4#
58 63.6 47.6 71.4

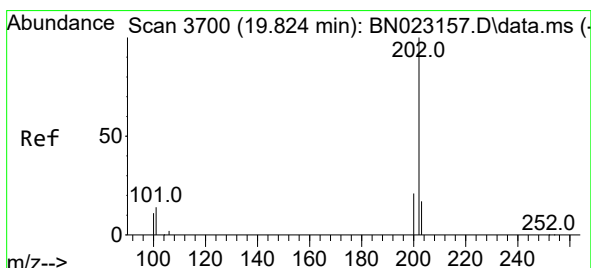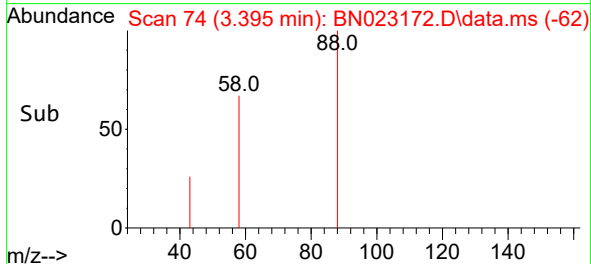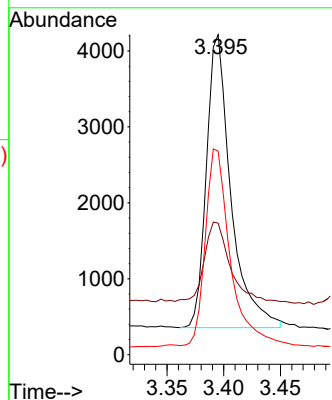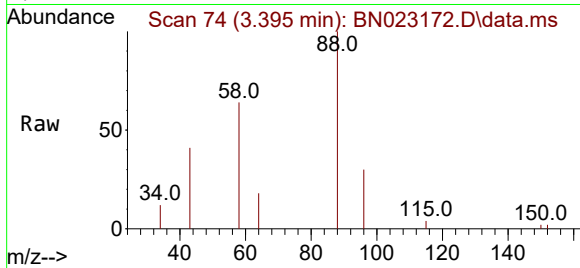

#20
Pyrene
Concen: 0.032 ng/ul
RT: 19.797 min Scan# 3694
Delta R.T. -0.027 min
Lab File: BN023172.D
Acq: 13 Dec 2022 19:33


Tgt Ion: 202 Resp: 4529
Ion Ratio Lower Upper
202 100
101 155.9 10.6 16.0#
100 1150.2 8.2 12.4#

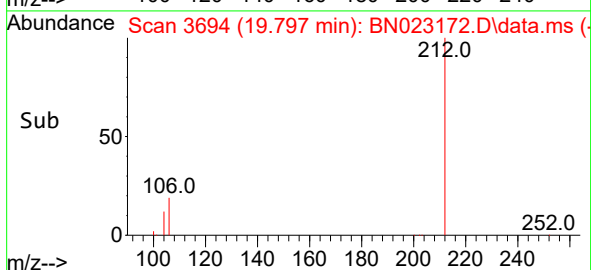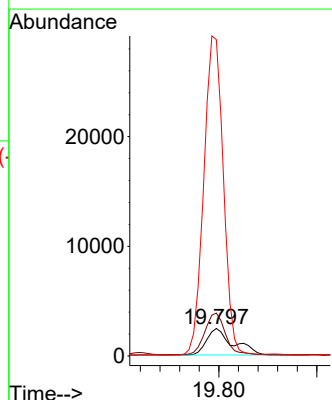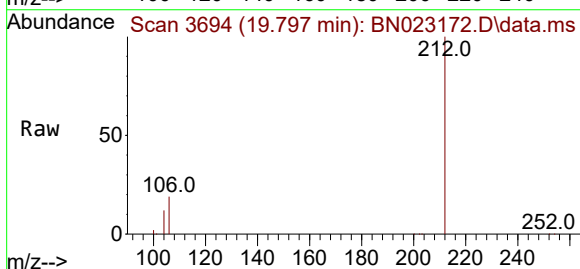

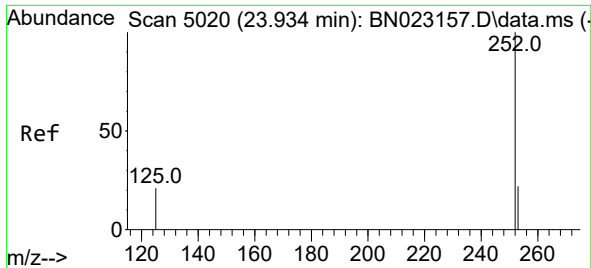

#26
 Benzo(a)pyrene
 Concen: 0.083 ng/ul
 RT: 23.888 min Scan# 50
 Delta R.T. -0.046 min
 Lab File: BN023172.D
 Acq: 13 Dec 2022 19:33

Instrument :
 BNA_N
 ClientSampleId :
 EXZ90

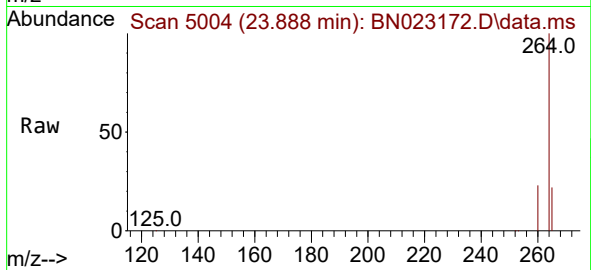

Tgt Ion:252 Resp: 8510
 Ion Ratio Lower Upper
 252 100
 253 41.2 19.7 29.5#
 125 38.0 13.7 20.5#

