

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN121322\
 Data File : BN023175.D
 Acq On : 13 Dec 2022 22:00
 Operator : CG/JU
 Sample : PB149499BL
 Misc :
 ALS Vial : 20 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 SBLK499

Quant Time: Dec 14 00:00:19 2022
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SFAM-EPA-SIM-BN112622.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Tue Dec 13 23:52:47 2022
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Dichlorobenzene-d4	8.015	152	6373	0.400	ng/ul	0.00
4) Naphthalene-d8	10.832	136	20933	0.400	ng/ul	0.00
9) Acenaphthene-d10	14.659	164	12400	0.400	ng/ul	0.00
13) Phenanthrene-d10	17.407	188	28275	0.400	ng/ul	0.00
17) Chrysene-d12	21.588	240	23499	0.400	ng/ul	0.00
23) Perylene-d12	24.044	264	22469	0.400	ng/ul	0.00
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.357	96	35318	4.618	ng/ul	0.00
6) 2-Methylnaphthalene-d10	12.421	152	8720	0.273	ng/ul	0.00
18) Fluoranthene-d10	19.430	212	20783	0.239	ng/ul	0.00
Target Compounds						
					Qvalue	
12) Fluorene	15.654	166	3134	0.057	ng/ul#	13
20) Pyrene	19.797	202	3136	0.026	ng/ul#	1
26) Benzo(a)pyrene	23.889	252	7525	0.087	ng/ul#	59


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN121322\
Data File : BN023175.D
Acq On : 13 Dec 2022 22:00
Operator : CG/JU
Sample : PB149499BL
Misc :
ALS Vial : 20 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
SBLK499

Quant Time: Dec 14 00:00:19 2022
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SFAM-EPA-SIM-BN112622.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Dec 13 23:52:47 2022
Response via : Initial Calibration




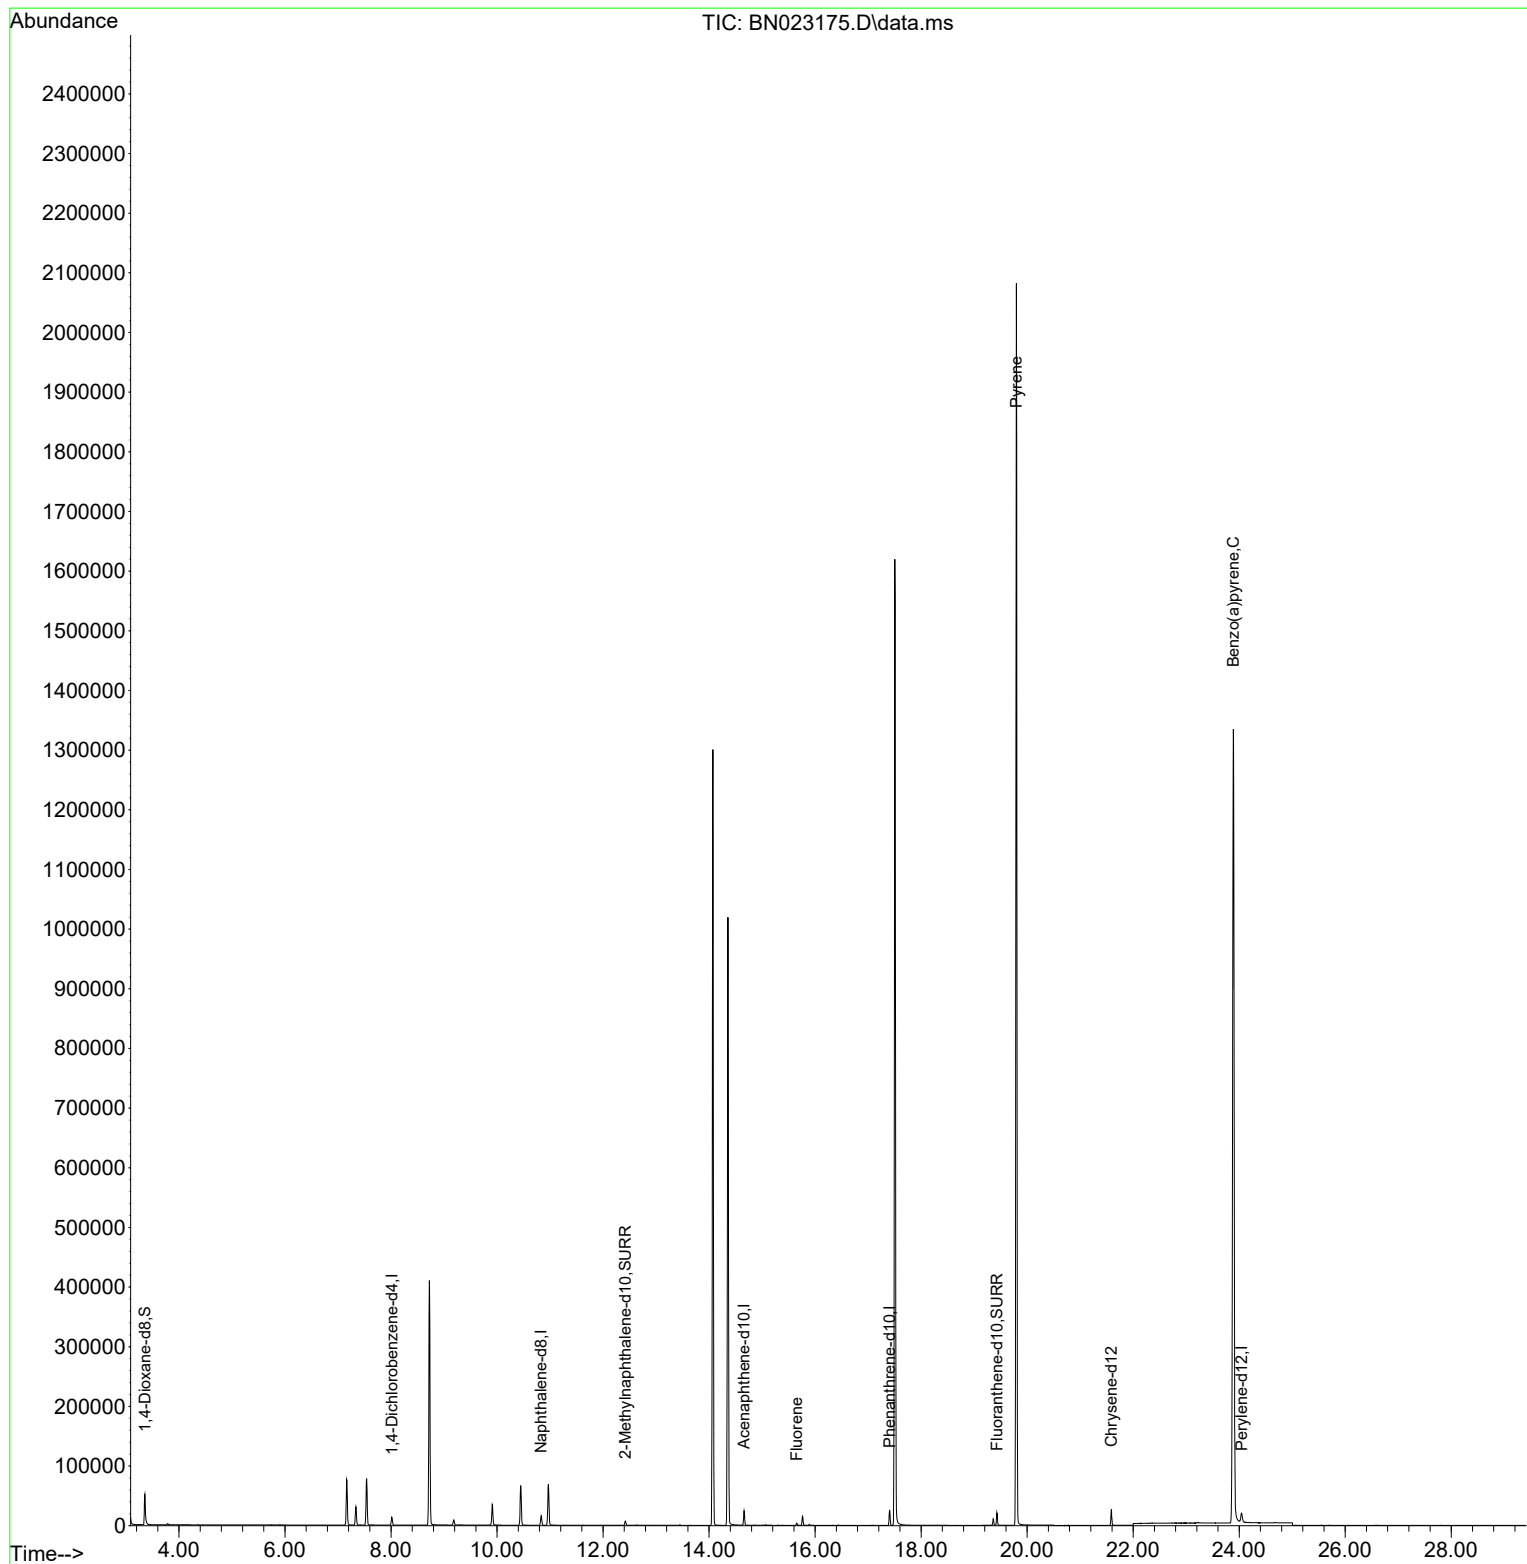


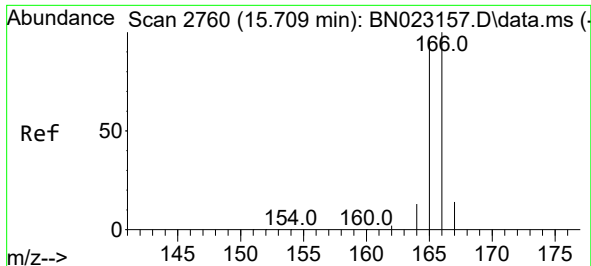

#12
Fluorene
Concen: 0.057 ng/ul
RT: 15.654 min Scan# 21
Delta R.T. -0.055 min
Lab File: BN023175.D
Acq: 13 Dec 2022 22:00




Instrument :
BNA_N
ClientSampleId :
SBLK499


Tgt Ion:166 Resp: 3134
Ion Ratio Lower Upper
166 100
165 6.9 78.7 118.1#
167 33.9 10.8 16.2#

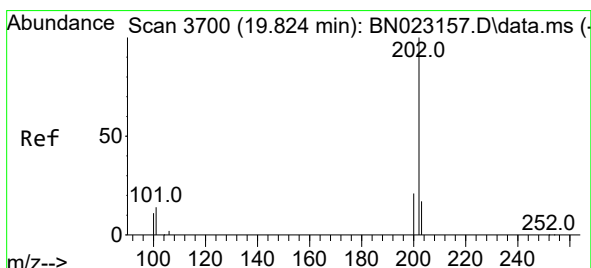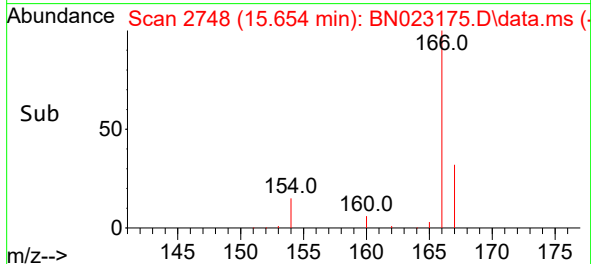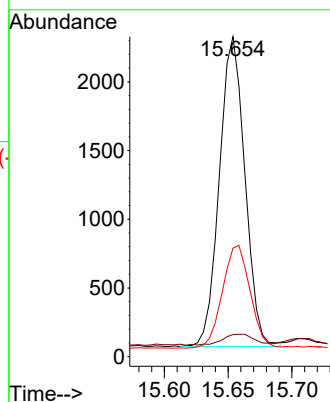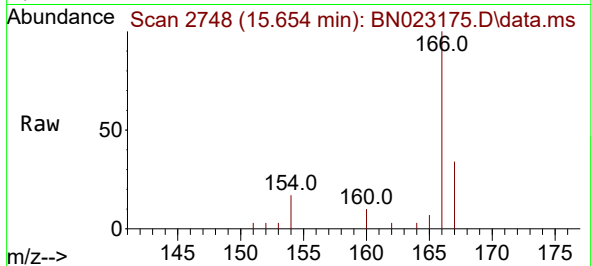

#20
Pyrene
Concen: 0.026 ng/ul
RT: 19.797 min Scan# 3694
Delta R.T. -0.028 min
Lab File: BN023175.D
Acq: 13 Dec 2022 22:00


Tgt Ion:202 Resp: 3136
Ion Ratio Lower Upper
202 100
101 163.1 10.6 16.0#
100 1214.6 8.2 12.4#

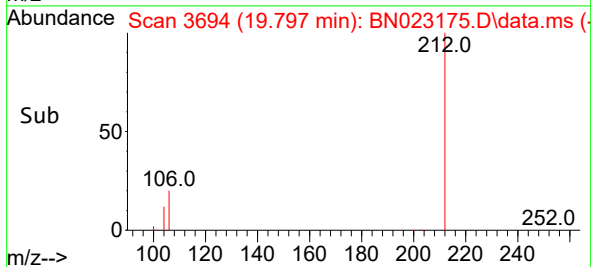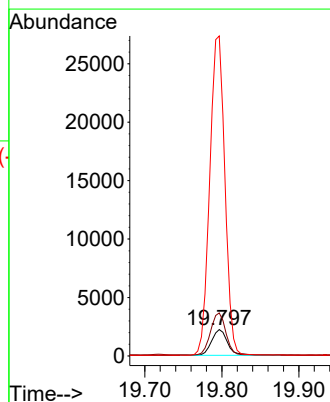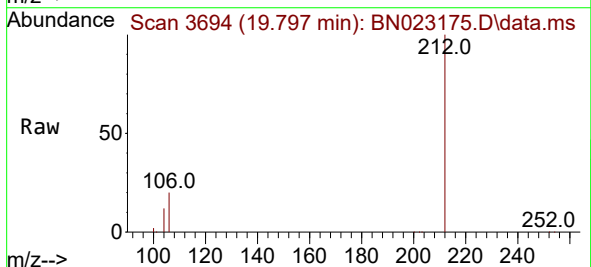

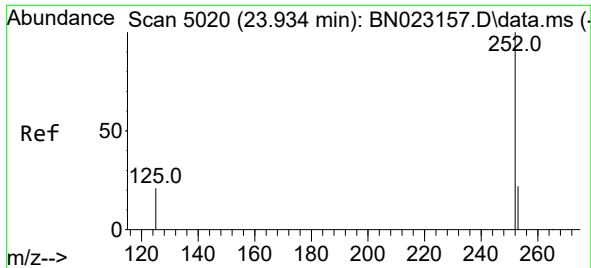

#26
Benzo(a)pyrene
Concen: 0.087 ng/ul
RT: 23.889 min Scan# 50
Delta R.T. -0.045 min
Lab File: BN023175.D
Acq: 13 Dec 2022 22:00

Instrument :
BNA_N
ClientSampleId :
SBLK499

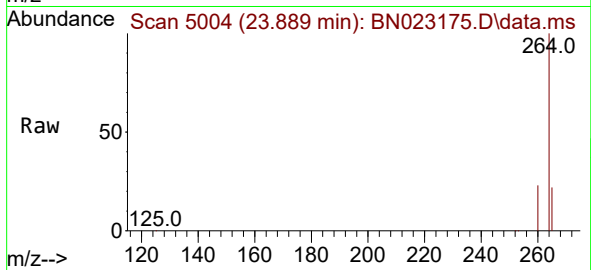

Tgt Ion:252 Resp: 7525
Ion Ratio Lower Upper
252 100
253 42.7 19.7 29.5#
125 37.8 13.7 20.5#

