

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN121322\
 Data File : BN023192.D
 Acq On : 14 Dec 2022 08:56
 Operator : CG/JU
 Sample : PB149529BL
 Misc :
 ALS Vial : 38 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :

Quant Time: Dec 14 23:18:55 2022
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SFAM-EPA-SIM-BN112622.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Tue Dec 13 23:52:47 2022
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Dichlorobenzene-d4	8.015	152	5749	0.400	ng/ul	0.00
4) Naphthalene-d8	10.832	136	19294	0.400	ng/ul	0.00
9) Acenaphthene-d10	14.660	164	11617	0.400	ng/ul	0.00
13) Phenanthrene-d10	17.404	188	26607	0.400	ng/ul	0.00
17) Chrysene-d12	21.587	240	24297	0.400	ng/ul	0.00
23) Perylene-d12	24.043	264	23183	0.400	ng/ul	0.00
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.353	96	35899	5.203	ng/ul	0.00
6) 2-Methylnaphthalene-d10	12.415	152	8416	0.286	ng/ul	0.00
18) Fluoranthene-d10	19.430	212	20388	0.227	ng/ul	0.00
Target Compounds						
					Qvalue	
12) Fluorene	15.650	166	3124	0.061	ng/ul#	13
20) Pyrene	19.797	202	3059	0.025	ng/ul#	1
26) Benzo(a)pyrene	23.888	252	7712	0.086	ng/ul#	63


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN121322\
Data File : BN023192.D
Acq On : 14 Dec 2022 08:56
Operator : CG/JU
Sample : PB149529BL
Misc :
ALS Vial : 38 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :


Quant Time: Dec 14 23:18:55 2022
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SFAM-EPA-SIM-BN112622.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Dec 13 23:52:47 2022
Response via : Initial Calibration

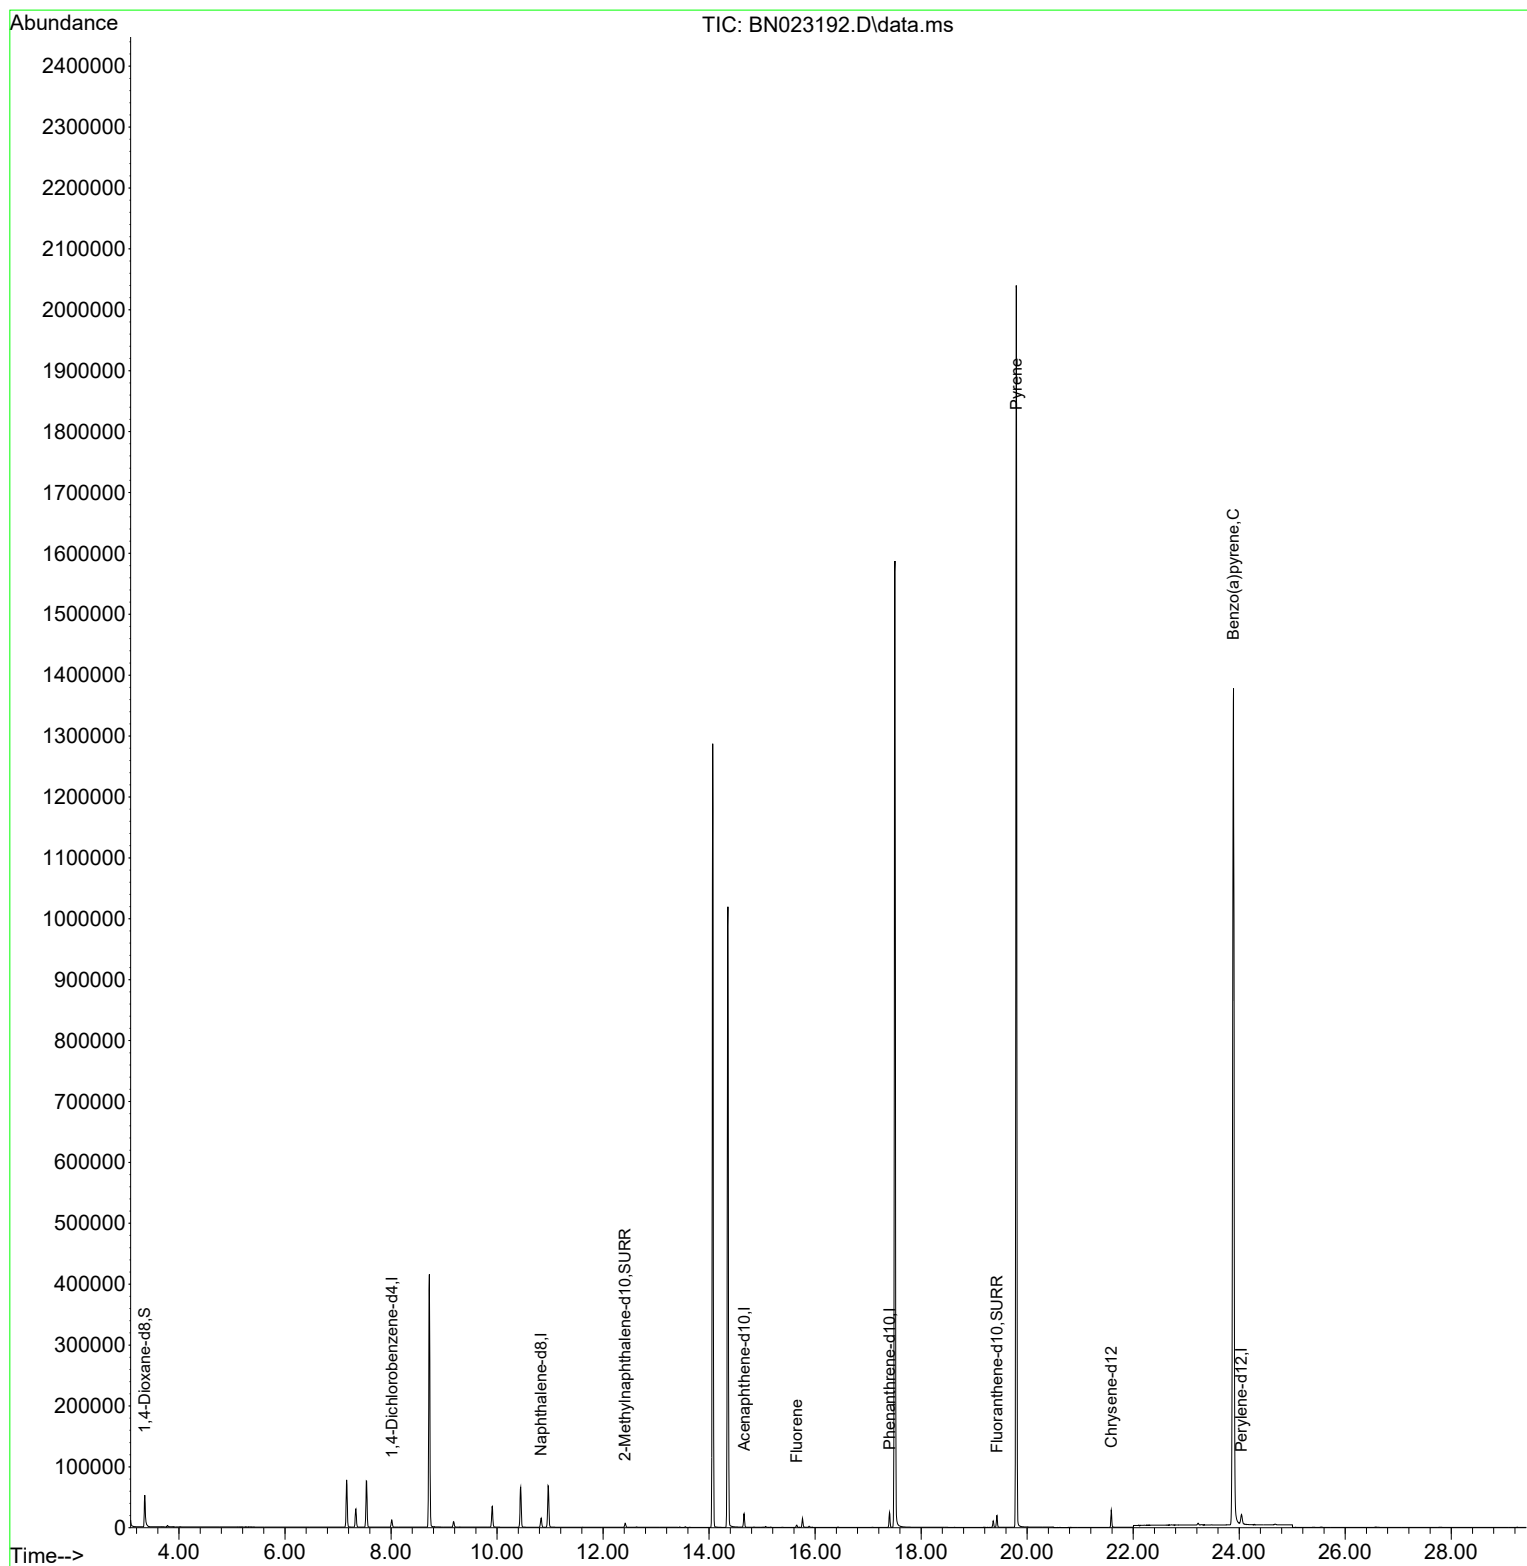



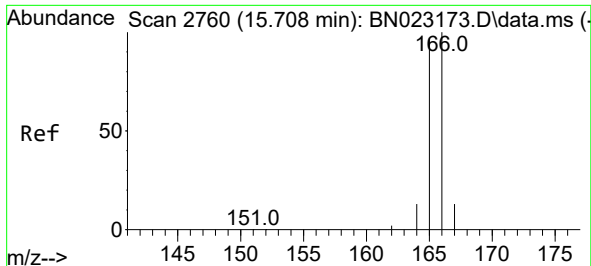


#12
Fluorene
Concen: 0.061 ng/ul
RT: 15.650 min Scan# 21
Delta R.T. -0.059 min
Lab File: BN023192.D
Acq: 14 Dec 2022 08:56

Instrument :
BNA_N
ClientSampleId :



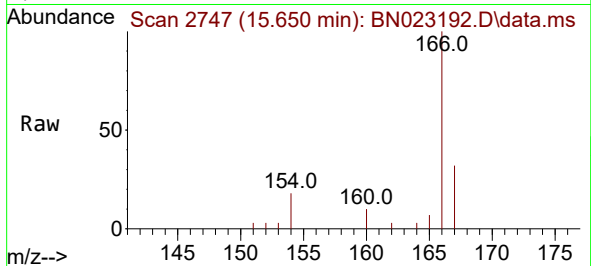



Tgt Ion:166 Resp: 3124
Ion Ratio Lower Upper
166 100
165 6.8 78.7 118.1#
167 31.5 10.8 16.2#

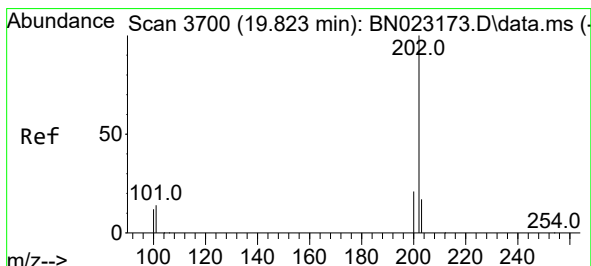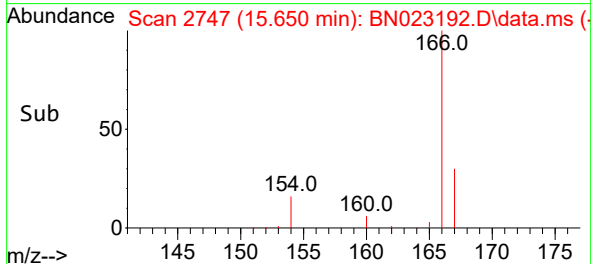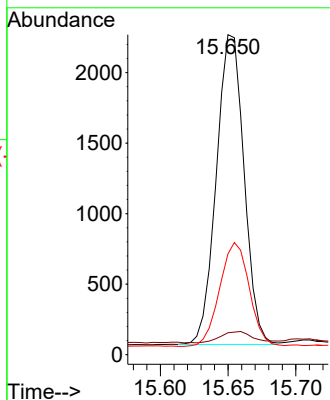

#20
Pyrene
Concen: 0.025 ng/ul
RT: 19.797 min Scan# 3694
Delta R.T. -0.027 min
Lab File: BN023192.D
Acq: 14 Dec 2022 08:56

Tgt Ion:202 Resp: 3059
Ion Ratio Lower Upper
202 100
101 154.6 10.6 16.0#
100 1098.9 8.2 12.4#

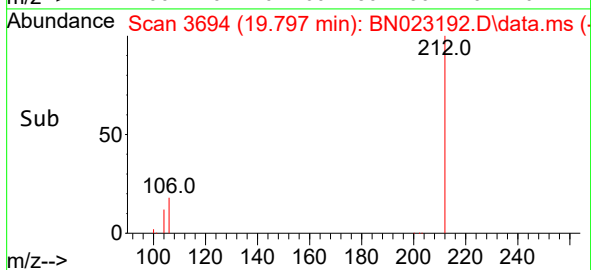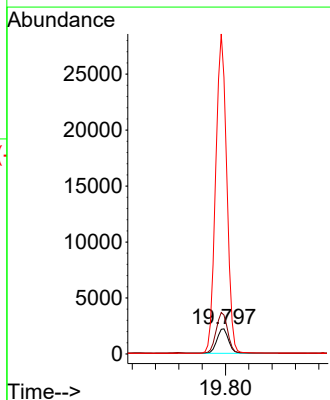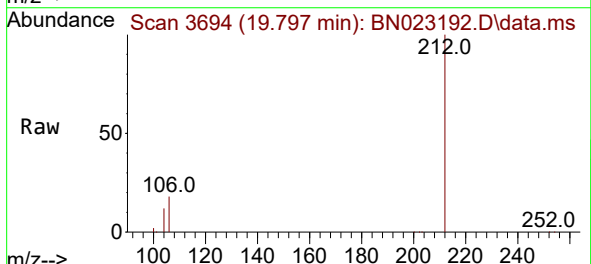

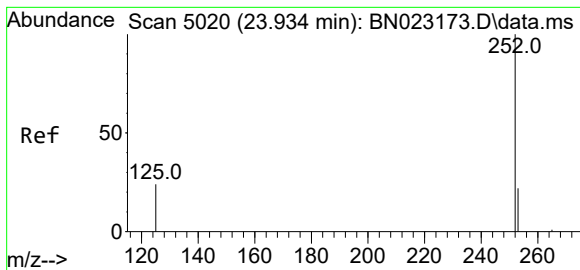

#26

Benzo(a)pyrene

Concen: 0.086 ng/ul

RT: 23.888 min Scan# 50

Delta R.T. -0.046 min


Lab File: BN023192.D

Acq: 14 Dec 2022 08:56

Instrument :

BNA_N

ClientSampleId :

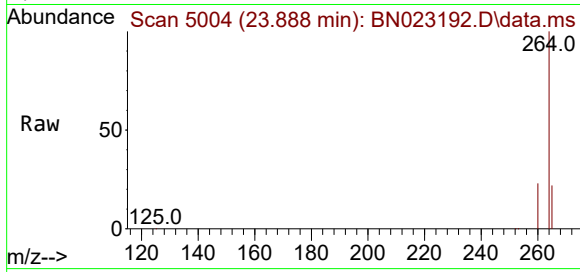

Tgt Ion:252 Resp: 7712

Ion Ratio Lower Upper

252 100

253 40.2 19.7 29.5#

125 36.6 13.7 20.5#

