

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN121322\
 Data File : BN023163.D
 Acq On : 13 Dec 2022 14:00
 Operator : CG/JU
 Sample : N5927-18
 Misc :
 ALS Vial : 8 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 EXZA3

Quant Time: Dec 13 23:58:52 2022
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SFAM-EPA-SIM-BN112622.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Tue Dec 13 23:52:47 2022
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Dichlorobenzene-d4	8.015	152	7179	0.400	ng/ul	0.00
4) Naphthalene-d8	10.837	136	23878	0.400	ng/ul	0.00
9) Acenaphthene-d10	14.659	164	14688	0.400	ng/ul	0.00
13) Phenanthrene-d10	17.407	188	34956	0.400	ng/ul	0.00
17) Chrysene-d12	21.590	240	31936	0.400	ng/ul	0.00
23) Perylene-d12	24.048	264	30610	0.400	ng/ul	# 0.00
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.357	96	34233	3.974	ng/ul	0.00
6) 2-Methylnaphthalene-d10	12.421	152	11346	0.312	ng/ul	0.00
18) Fluoranthene-d10	19.430	212	34242	0.290	ng/ul	0.00
Target Compounds						
						Qvalue
2) 1,4-Dioxane	3.395	88	8347	0.929	ng/ul#	88


(#) = qualifier out of range (m) = manual integration (+) = signals summed

```
Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN121322\  
Data File : BN023163.D  
Acq On    : 13 Dec 2022  14:00  
Operator  : CG/JU  
Sample    : N5927-18  
Misc      :  
ALS Vial  : 8      Sample Multiplier: 1
```

Instrument :
BNA_N
ClientSampleId :
EXZA3


Quant Time: Dec 13 23:58:52 2022
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SFAM-EPA-SIM-BN112622.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
Qlast Update : Tue Dec 13 23:52:47 2022
Response via : Initial Calibration

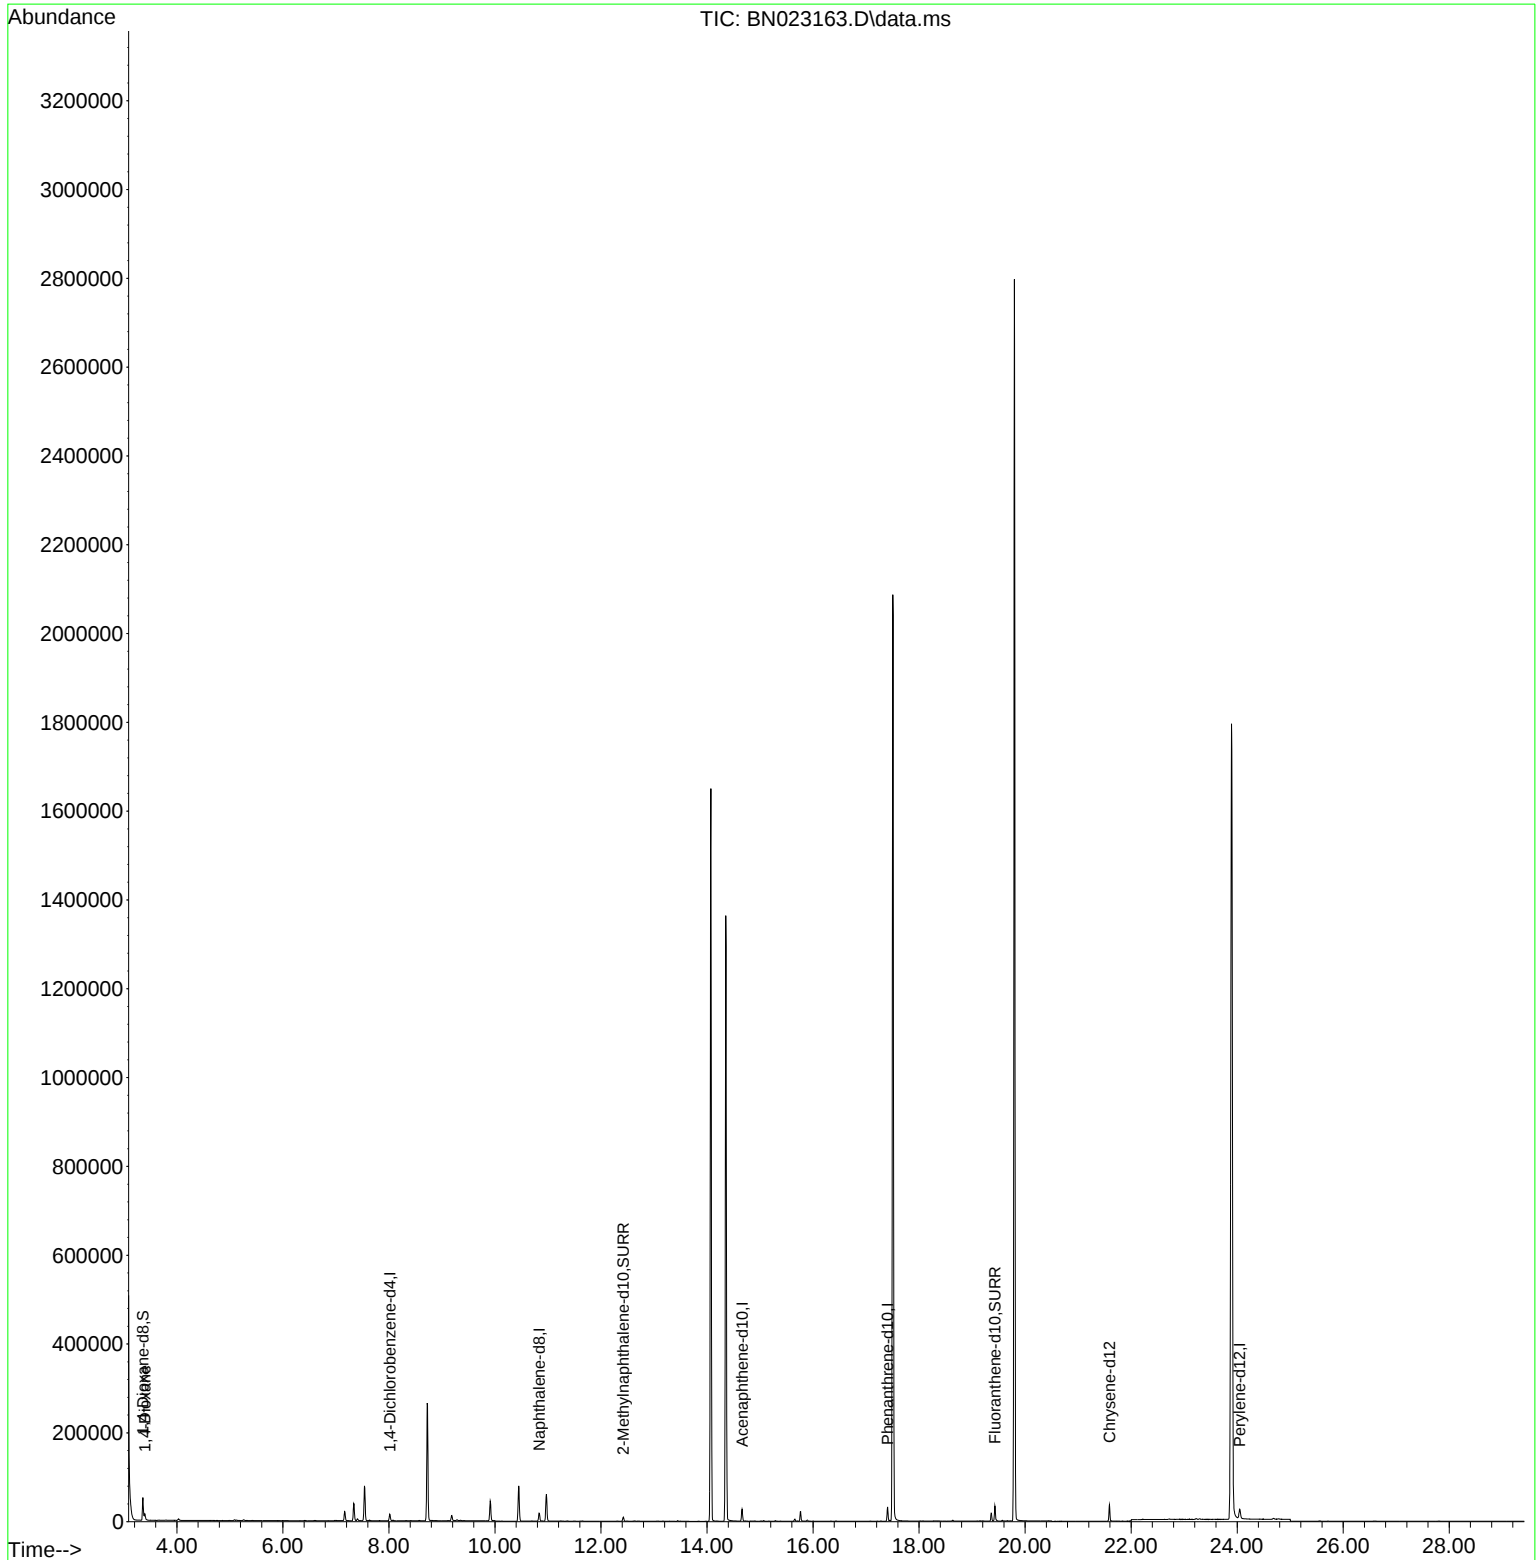

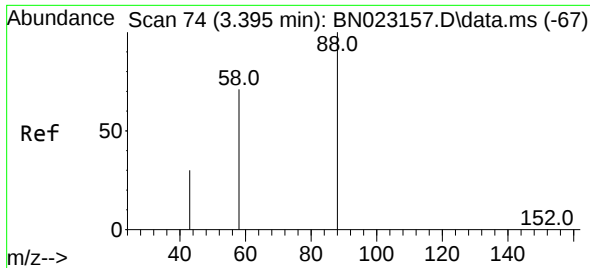

#2
 1,4-Dioxane
 Concen: 0.929 ng/ul
 RT: 3.395 min Scan# 74
 Delta R.T. 0.000 min
 Lab File: BN023163.D
 Acq: 13 Dec 2022 14:00

Instrument :
 BNA_N
 ClientSampleId :
 EXZA3

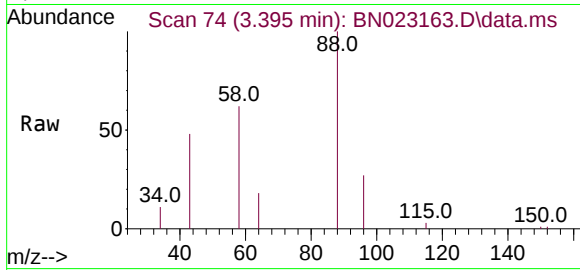

Tgt Ion: 88	Resp: 8347
Ion Ratio	Lower Upper
88	100
43	47.5 26.2 39.4#
58	62.1 47.6 71.4

