

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN121322\
 Data File : BN023167.D
 Acq On : 13 Dec 2022 16:28
 Operator : CG/JU
 Sample : N5927-21
 Misc :
 ALS Vial : 12 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 EXZA7

Quant Time: Dec 13 23:59:26 2022
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SFAM-EPA-SIM-BN112622.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Tue Dec 13 23:52:47 2022
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Dichlorobenzene-d4	8.019	152	7495	0.400	ng/ul	0.00
4) Naphthalene-d8	10.837	136	21035	0.400	ng/ul	0.00
9) Acenaphthene-d10	14.664	164	11746	0.400	ng/ul	0.00
13) Phenanthrene-d10	17.407	188	27989	0.400	ng/ul	0.00
17) Chrysene-d12	21.590	240	24981	0.400	ng/ul	0.00
23) Perylene-d12	24.051	264	23672	0.400	ng/ul	0.00
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.357	96	23993	2.668	ng/ul	0.00
6) 2-Methylnaphthalene-d10	12.421	152	9640	0.301	ng/ul	0.00
18) Fluoranthene-d10	19.430	212	27736	0.300	ng/ul	0.00
Target Compounds						
					Qvalue	
2) 1,4-Dioxane	3.395	88	1539	0.164	ng/ul#	56


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN121322\
Data File : BN023167.D
Acq On : 13 Dec 2022 16:28
Operator : CG/JU
Sample : N5927-21
Misc :
ALS Vial : 12 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
EXZA7

Quant Time: Dec 13 23:59:26 2022
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SFAM-EPA-SIM-BN112622.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Dec 13 23:52:47 2022
Response via : Initial Calibration

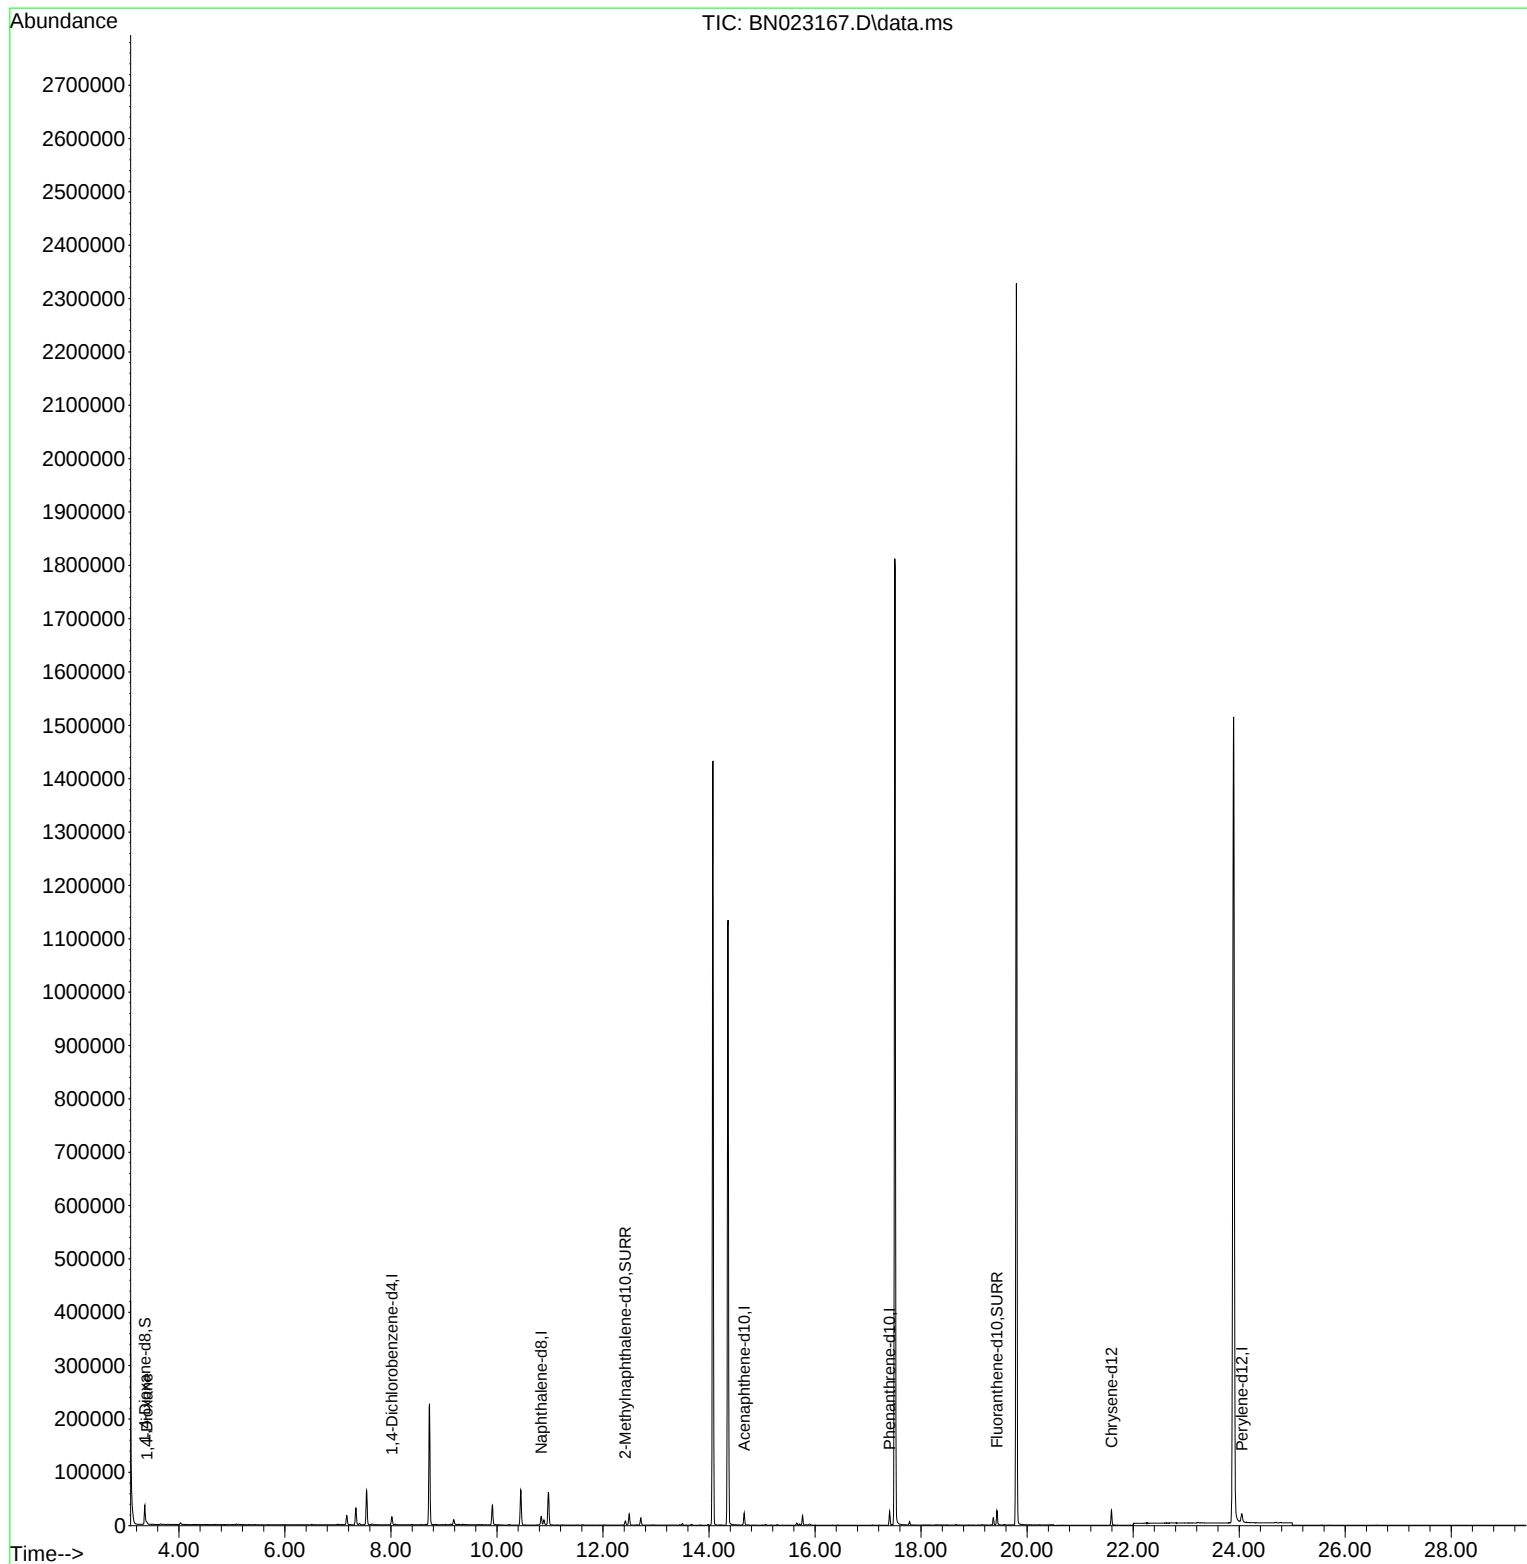

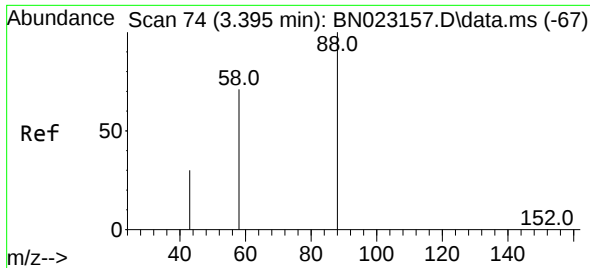

#2
 1,4-Dioxane
 Concen: 0.164 ng/ul
 RT: 3.395 min Scan# 74
 Delta R.T. 0.000 min
 Lab File: BN023167.D
 Acq: 13 Dec 2022 16:28

Instrument :
 BNA_N
 ClientSampleId :
 EXZA7

Tgt Ion:	88	Resp:	1539
Ion	Ratio	Lower	Upper
88	100		
43	101.9	26.2	39.4#
58	58.5	47.6	71.4

