

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN121322\
 Data File : BN023168.D
 Acq On : 13 Dec 2022 17:05
 Operator : CG/JU
 Sample : N5927-22
 Misc :
 ALS Vial : 13 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 EXZA8

Quant Time: Dec 13 23:59:33 2022
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SFAM-EPA-SIM-BN112622.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Tue Dec 13 23:52:47 2022
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Dichlorobenzene-d4	8.019	152	7410	0.400	ng/ul	0.00
4) Naphthalene-d8	10.837	136	24599	0.400	ng/ul	0.00
9) Acenaphthene-d10	14.664	164	15196	0.400	ng/ul	0.00
13) Phenanthrene-d10	17.407	188	35489	0.400	ng/ul	0.00
17) Chrysene-d12	21.588	240	31041	0.400	ng/ul	0.00
23) Perylene-d12	24.047	264	29489	0.400	ng/ul	# 0.00
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.361	96	27873	3.134	ng/ul	0.00
6) 2-Methylnaphthalene-d10	12.421	152	12793	0.341	ng/ul	0.00
18) Fluoranthene-d10	19.434	212	33702	0.294	ng/ul	0.00
Target Compounds						
						Qvalue
2) 1,4-Dioxane	3.399	88	915	0.099	ng/ul#	47


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN121322\
Data File : BN023168.D
Acq On : 13 Dec 2022 17:05
Operator : CG/JU
Sample : N5927-22
Misc :
ALS Vial : 13 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
EXZA8


Quant Time: Dec 13 23:59:33 2022
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SFAM-EPA-SIM-BN112622.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Dec 13 23:52:47 2022
Response via : Initial Calibration

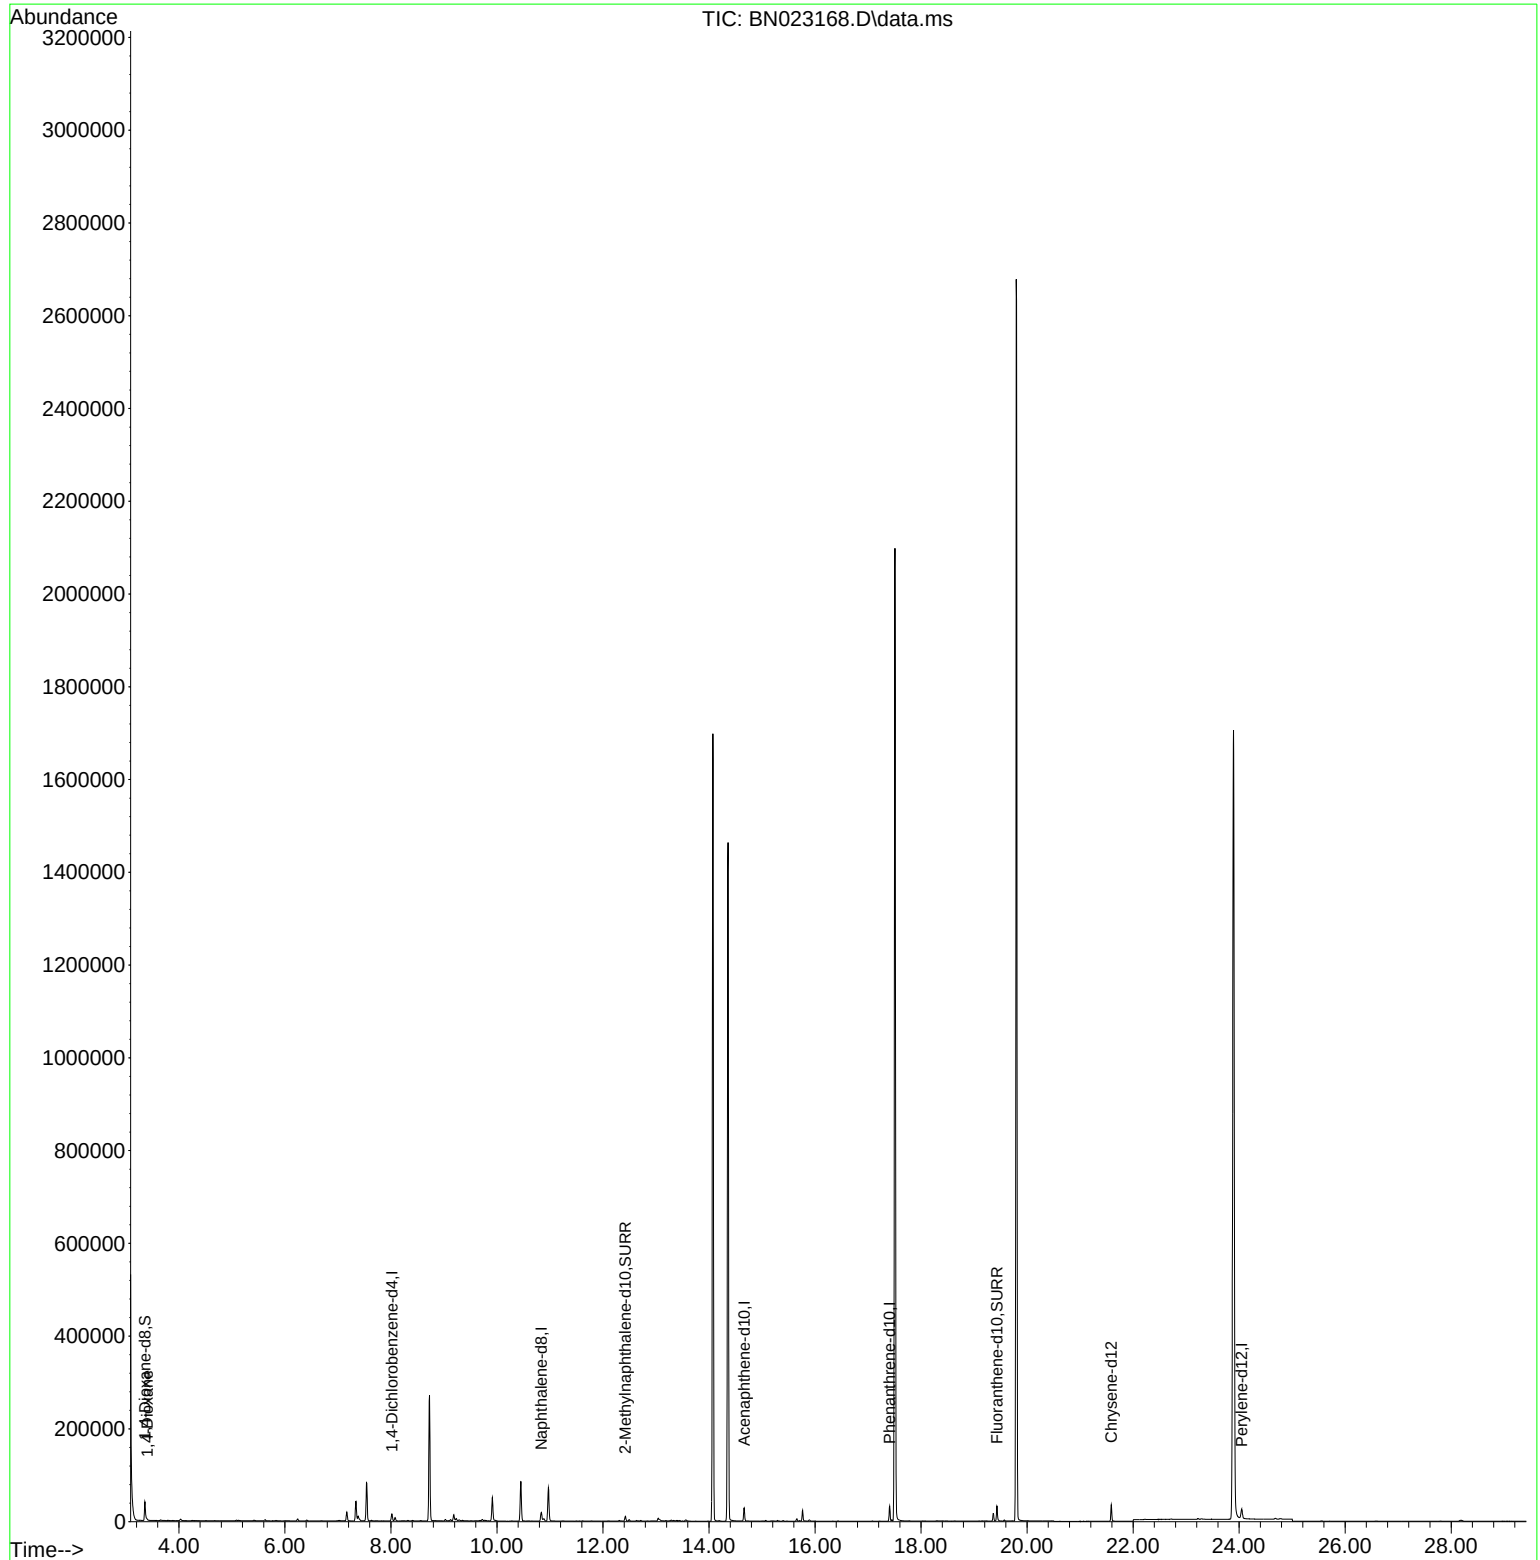

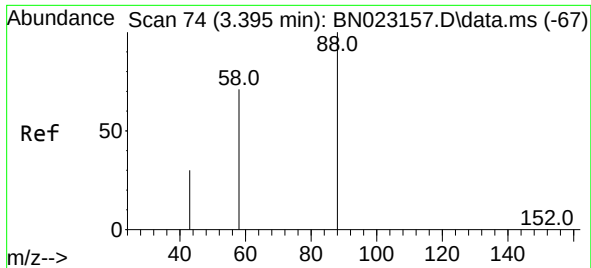

#2
 1,4-Dioxane
 Concen: 0.099 ng/ul
 RT: 3.399 min Scan# 74
 Delta R.T. 0.004 min
 Lab File: BN023168.D
 Acq: 13 Dec 2022 17:05

Instrument :
 BNA_N
 ClientSampleId :
 EXZA8

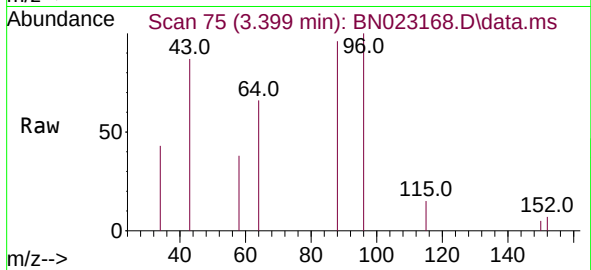

Tgt Ion: 88	Resp: 915
Ion Ratio	Lower Upper
88	100
43	91.3 26.2 39.4#
58	40.2 47.6 71.4#

