

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN121322\
 Data File : BN023184.D
 Acq On : 14 Dec 2022 03:28
 Operator : CG/JU
 Sample : N5927-07
 Misc :
 ALS Vial : 29 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 EXZ93

Quant Time: Dec 14 04:21:13 2022
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SFAM-EPA-SIM-BN112622.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Tue Dec 13 23:52:47 2022
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Dichlorobenzene-d4	8.015	152	6777	0.400	ng/ul	0.00
4) Naphthalene-d8	10.832	136	22444	0.400	ng/ul	0.00
9) Acenaphthene-d10	14.659	164	13364	0.400	ng/ul	0.00
13) Phenanthrene-d10	17.403	188	31831	0.400	ng/ul	0.00
17) Chrysene-d12	21.587	240	28508	0.400	ng/ul	0.00
23) Perylene-d12	24.042	264	26628	0.400	ng/ul	0.00
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.357	96	27562	3.389	ng/ul	0.00
6) 2-Methylnaphthalene-d10	12.415	152	9912	0.290	ng/ul	0.00
18) Fluoranthene-d10	19.429	212	28592	0.271	ng/ul	0.00
Target Compounds						
					Qvalue	
2) 1,4-Dioxane	3.395	88	1054	0.124	ng/ul#	65


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN121322\
Data File : BN023184.D
Acq On : 14 Dec 2022 03:28
Operator : CG/JU
Sample : N5927-07
Misc :
ALS Vial : 29 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
EXZ93

Quant Time: Dec 14 04:21:13 2022
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SFAM-EPA-SIM-BN112622.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Dec 13 23:52:47 2022
Response via : Initial Calibration

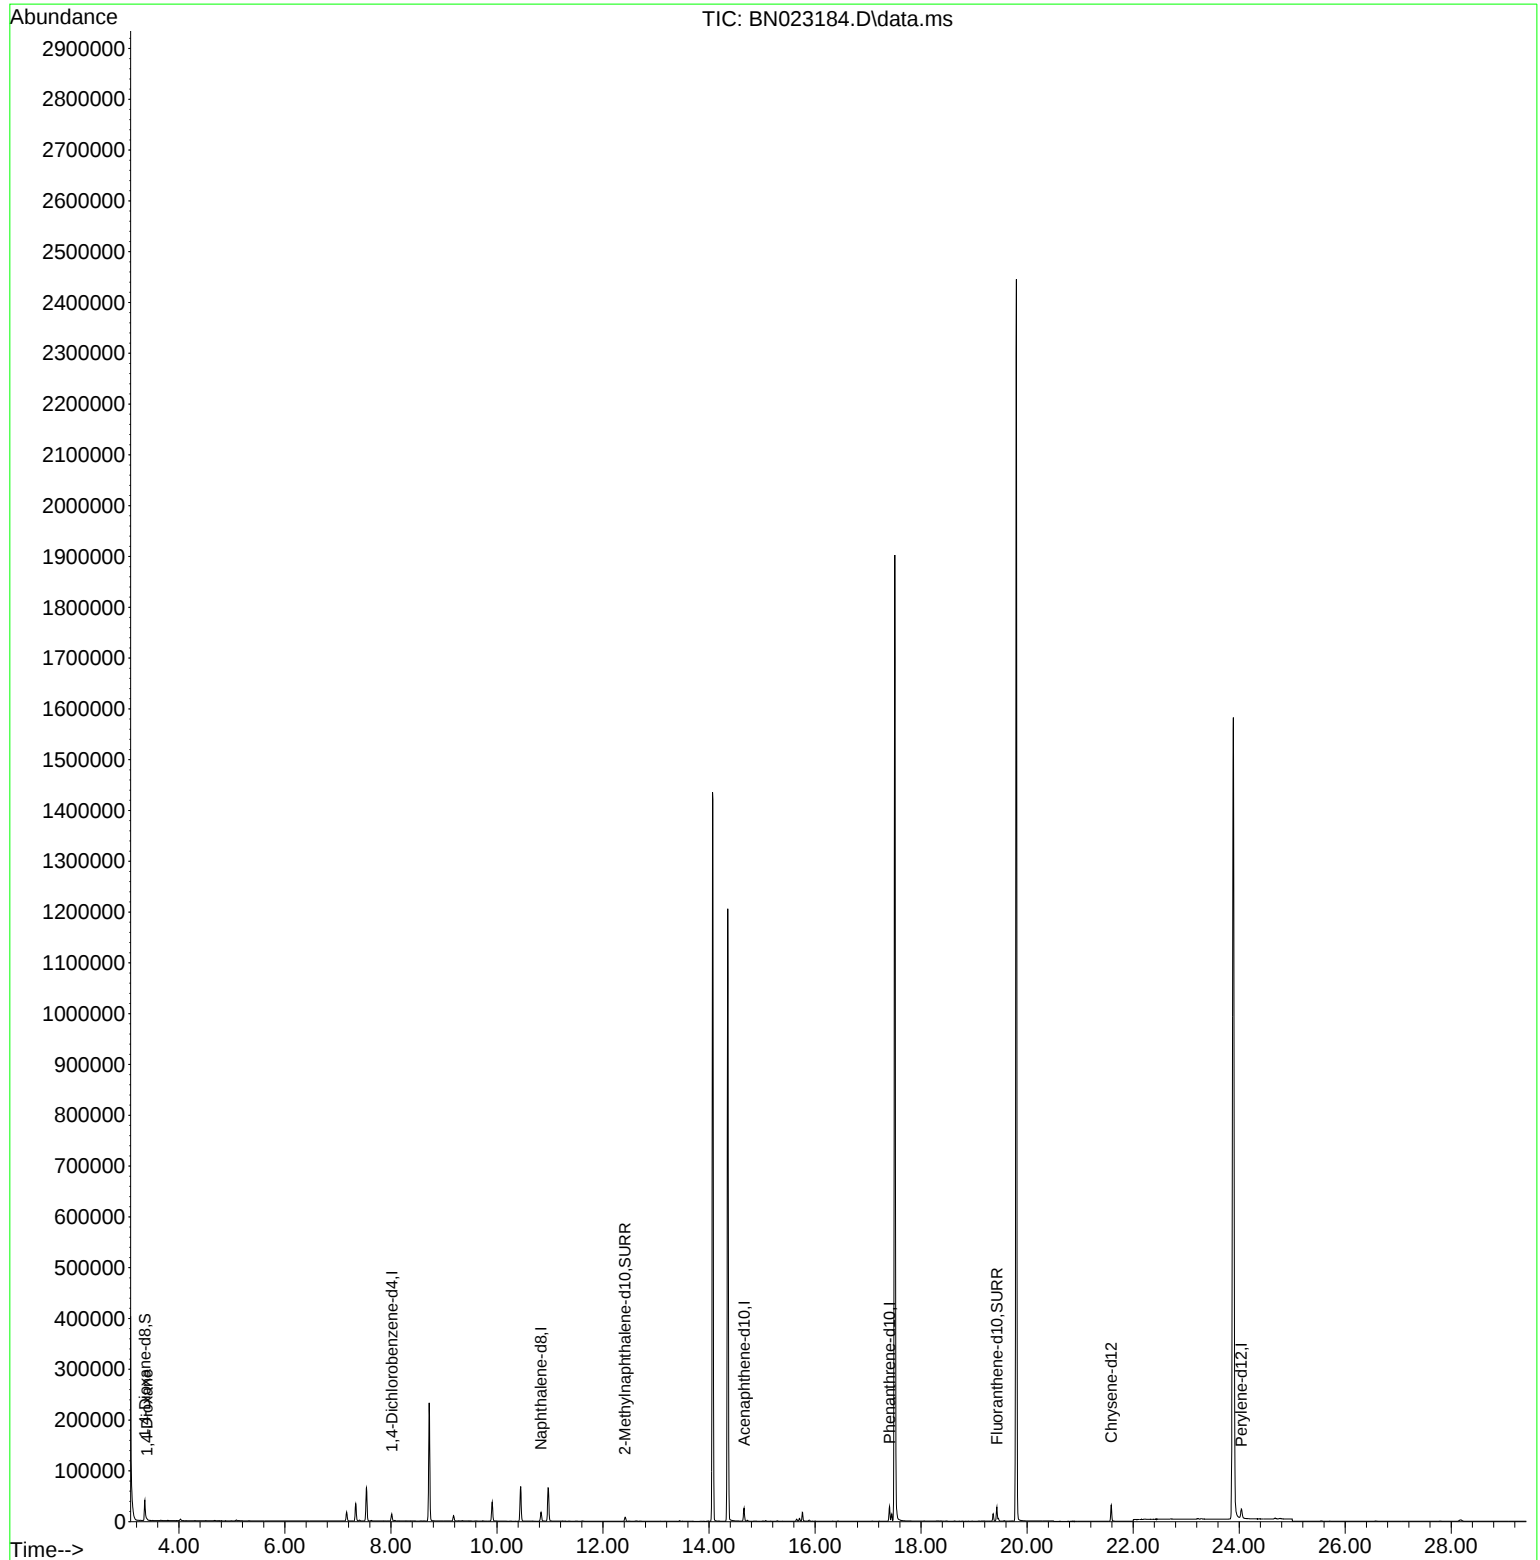

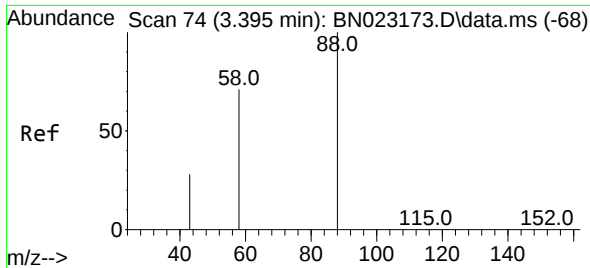

#2
 1,4-Dioxane
 Concen: 0.124 ng/ul
 RT: 3.395 min Scan# 74
 Delta R.T. 0.000 min
 Lab File: BN023184.D
 Acq: 14 Dec 2022 03:28

Instrument :
 BNA_N
 ClientSampleId :
 EXZ93

Tgt Ion: 88 Resp: 1054
 Ion Ratio Lower Upper
 88 100
 43 61.3 26.2 39.4#
 58 39.4 47.6 71.4#

