

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN121322\
 Data File : BN023185.D
 Acq On : 14 Dec 2022 04:05
 Operator : CG/JU
 Sample : N5927-08
 Misc :
 ALS Vial : 30 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 EXZ96

Quant Time: Dec 14 05:21:31 2022
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SFAM-EPA-SIM-BN112622.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Tue Dec 13 23:52:47 2022
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Dichlorobenzene-d4	8.015	152	6323	0.400	ng/u1	0.00
4) Naphthalene-d8	10.832	136	21302	0.400	ng/u1	0.00
9) Acenaphthene-d10	14.659	164	12978	0.400	ng/u1	0.00
13) Phenanthrene-d10	17.403	188	31422	0.400	ng/u1	0.00
17) Chrysene-d12	21.587	240	28177	0.400	ng/u1	0.00
23) Perylene-d12	24.045	264	25567	0.400	ng/u1	0.00
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.357	96	27518	3.627	ng/u1	0.00
6) 2-Methylnaphthalene-d10	12.416	152	9688	0.298	ng/u1	0.00
18) Fluoranthene-d10	19.430	212	30087	0.289	ng/u1	0.00
Target Compounds						
					Qvalue	
2) 1,4-Dioxane	3.391	88	7562	0.956	ng/u1	91


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN121322\
Data File : BN023185.D
Acq On : 14 Dec 2022 04:05
Operator : CG/JU
Sample : N5927-08
Misc :
ALS Vial : 30 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
EXZ96


Quant Time: Dec 14 05:21:31 2022
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SFAM-EPA-SIM-BN112622.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Dec 13 23:52:47 2022
Response via : Initial Calibration

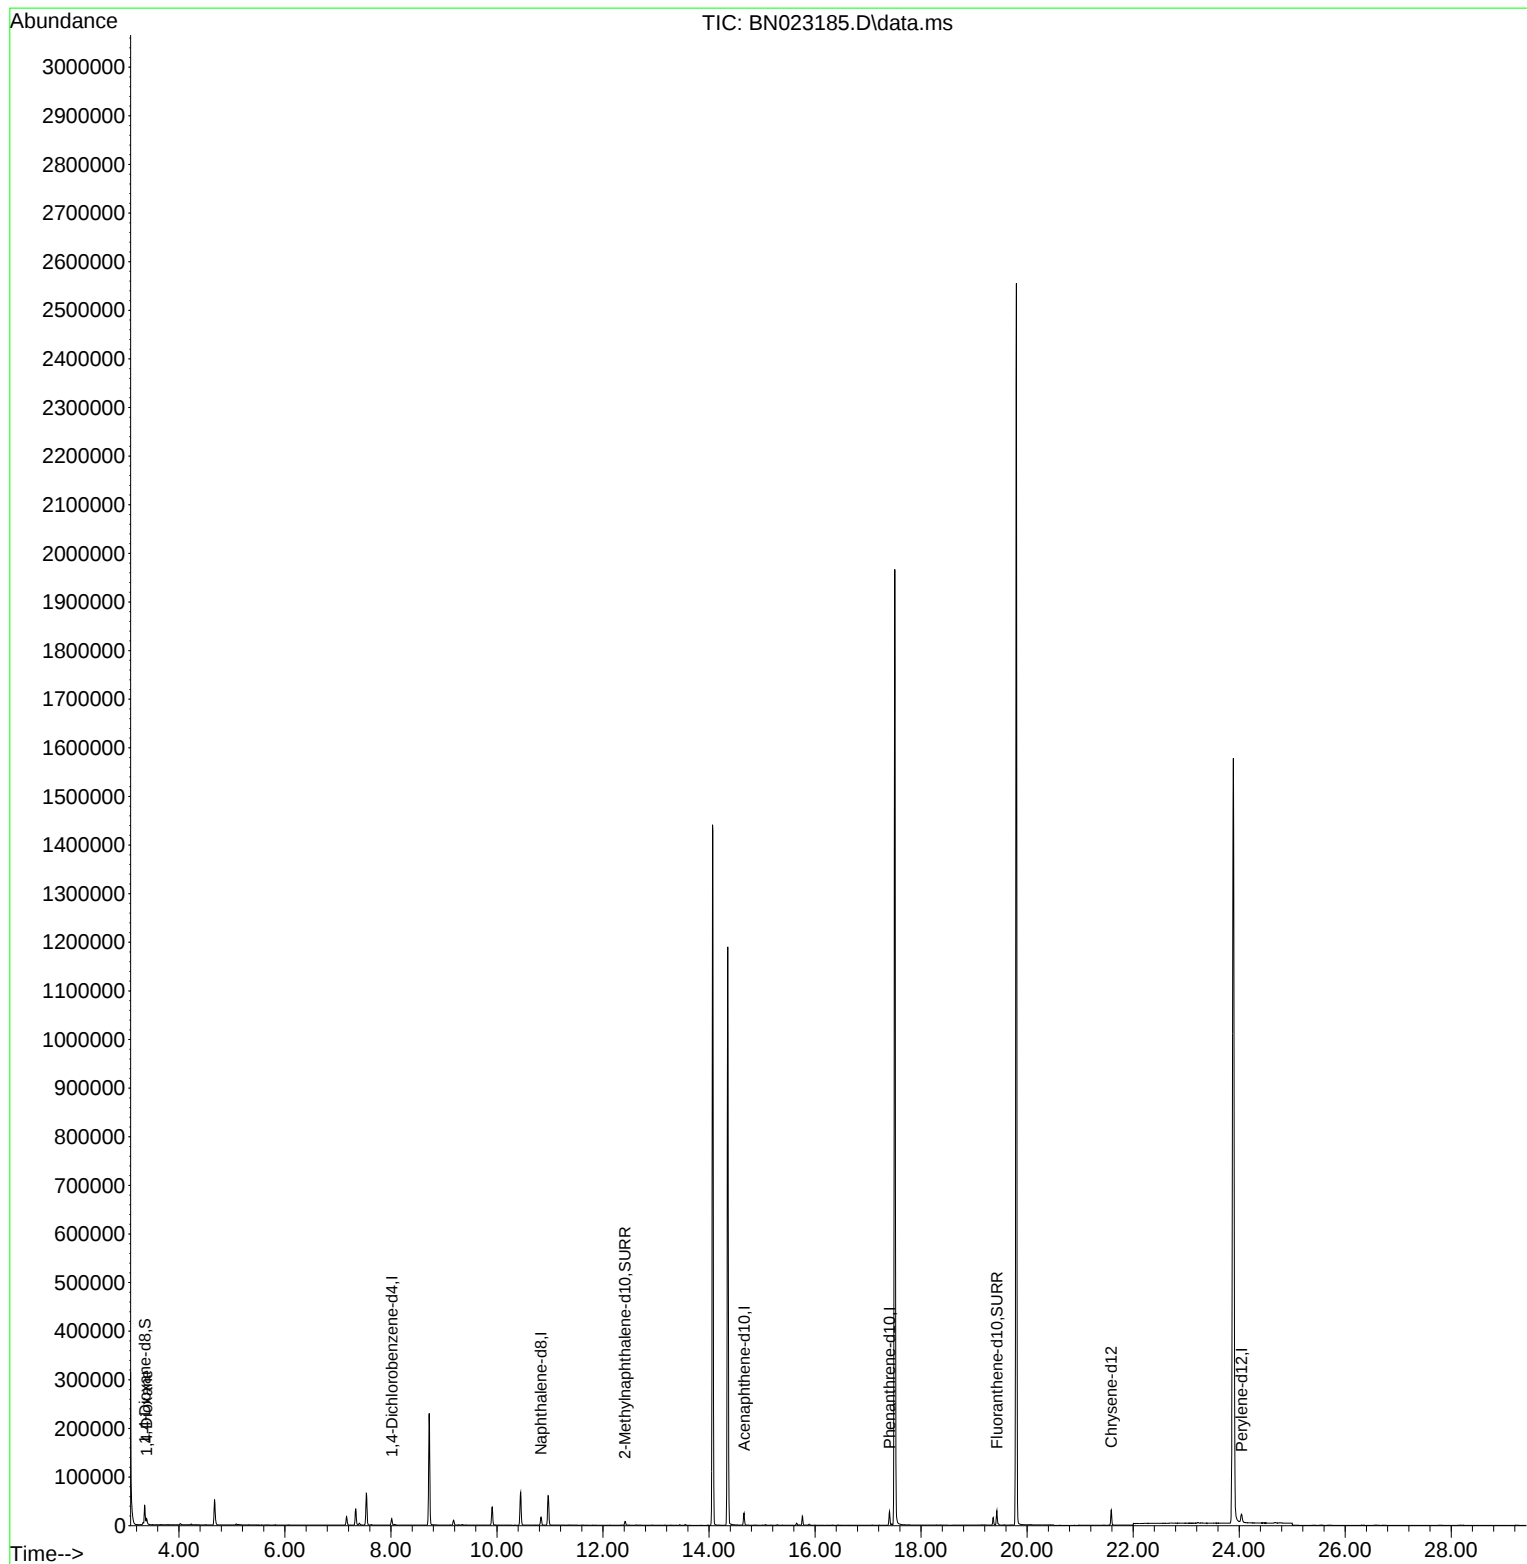

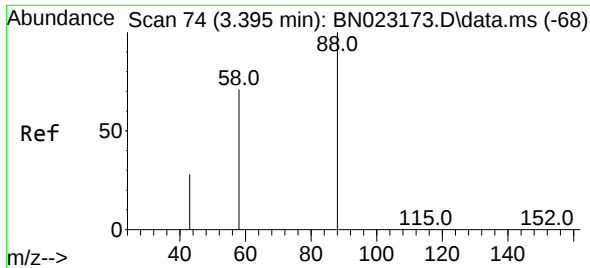

#2
 1,4-Dioxane
 Concen: 0.956 ng/ul
 RT: 3.391 min Scan# 74
 Delta R.T. -0.004 min
 Lab File: BN023185.D
 Acq: 14 Dec 2022 04:05

Instrument :
 BNA_N
 ClientSampleId :
 EXZ96

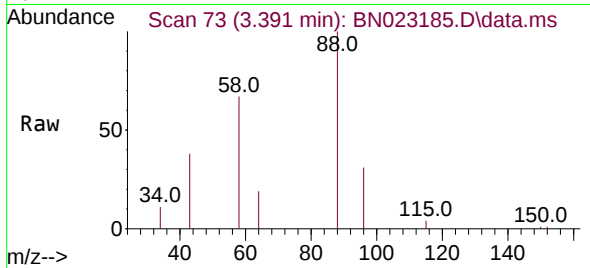

Tgt Ion:	88	Resp:	7562
Ion	Ratio	Lower	Upper
88	100		
43	37.6	26.2	39.4
58	66.7	47.6	71.4

