

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN121322\
 Data File : BN023188.D
 Acq On : 14 Dec 2022 05:54
 Operator : CG/JU
 Sample : N5948-02
 Misc :
 ALS Vial : 33 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 EXZB2

Quant Time: Dec 14 06:25:49 2022
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SFAM-EPA-SIM-BN112622.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Tue Dec 13 23:52:47 2022
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Dichlorobenzene-d4	8.015	152	6130	0.400	ng/ul	0.00
4) Naphthalene-d8	10.832	136	20585	0.400	ng/ul	0.00
9) Acenaphthene-d10	14.660	164	12610	0.400	ng/ul	0.00
13) Phenanthrene-d10	17.404	188	29220	0.400	ng/ul	0.00
17) Chrysene-d12	21.588	240	25983	0.400	ng/ul	0.00
23) Perylene-d12	24.043	264	24775	0.400	ng/ul	0.00
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.357	96	24796	3.371	ng/ul	0.00
6) 2-Methylnaphthalene-d10	12.416	152	9638	0.307	ng/ul	0.00
18) Fluoranthene-d10	19.430	212	25777	0.268	ng/ul	0.00
Target Compounds						
						Qvalue
2) 1,4-Dioxane	3.395	88	792	0.103	ng/ul#	66


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN121322\
Data File : BN023188.D
Acq On : 14 Dec 2022 05:54
Operator : CG/JU
Sample : N5948-02
Misc :
ALS Vial : 33 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
EXZB2

Quant Time: Dec 14 06:25:49 2022
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SFAM-EPA-SIM-BN112622.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Dec 13 23:52:47 2022
Response via : Initial Calibration

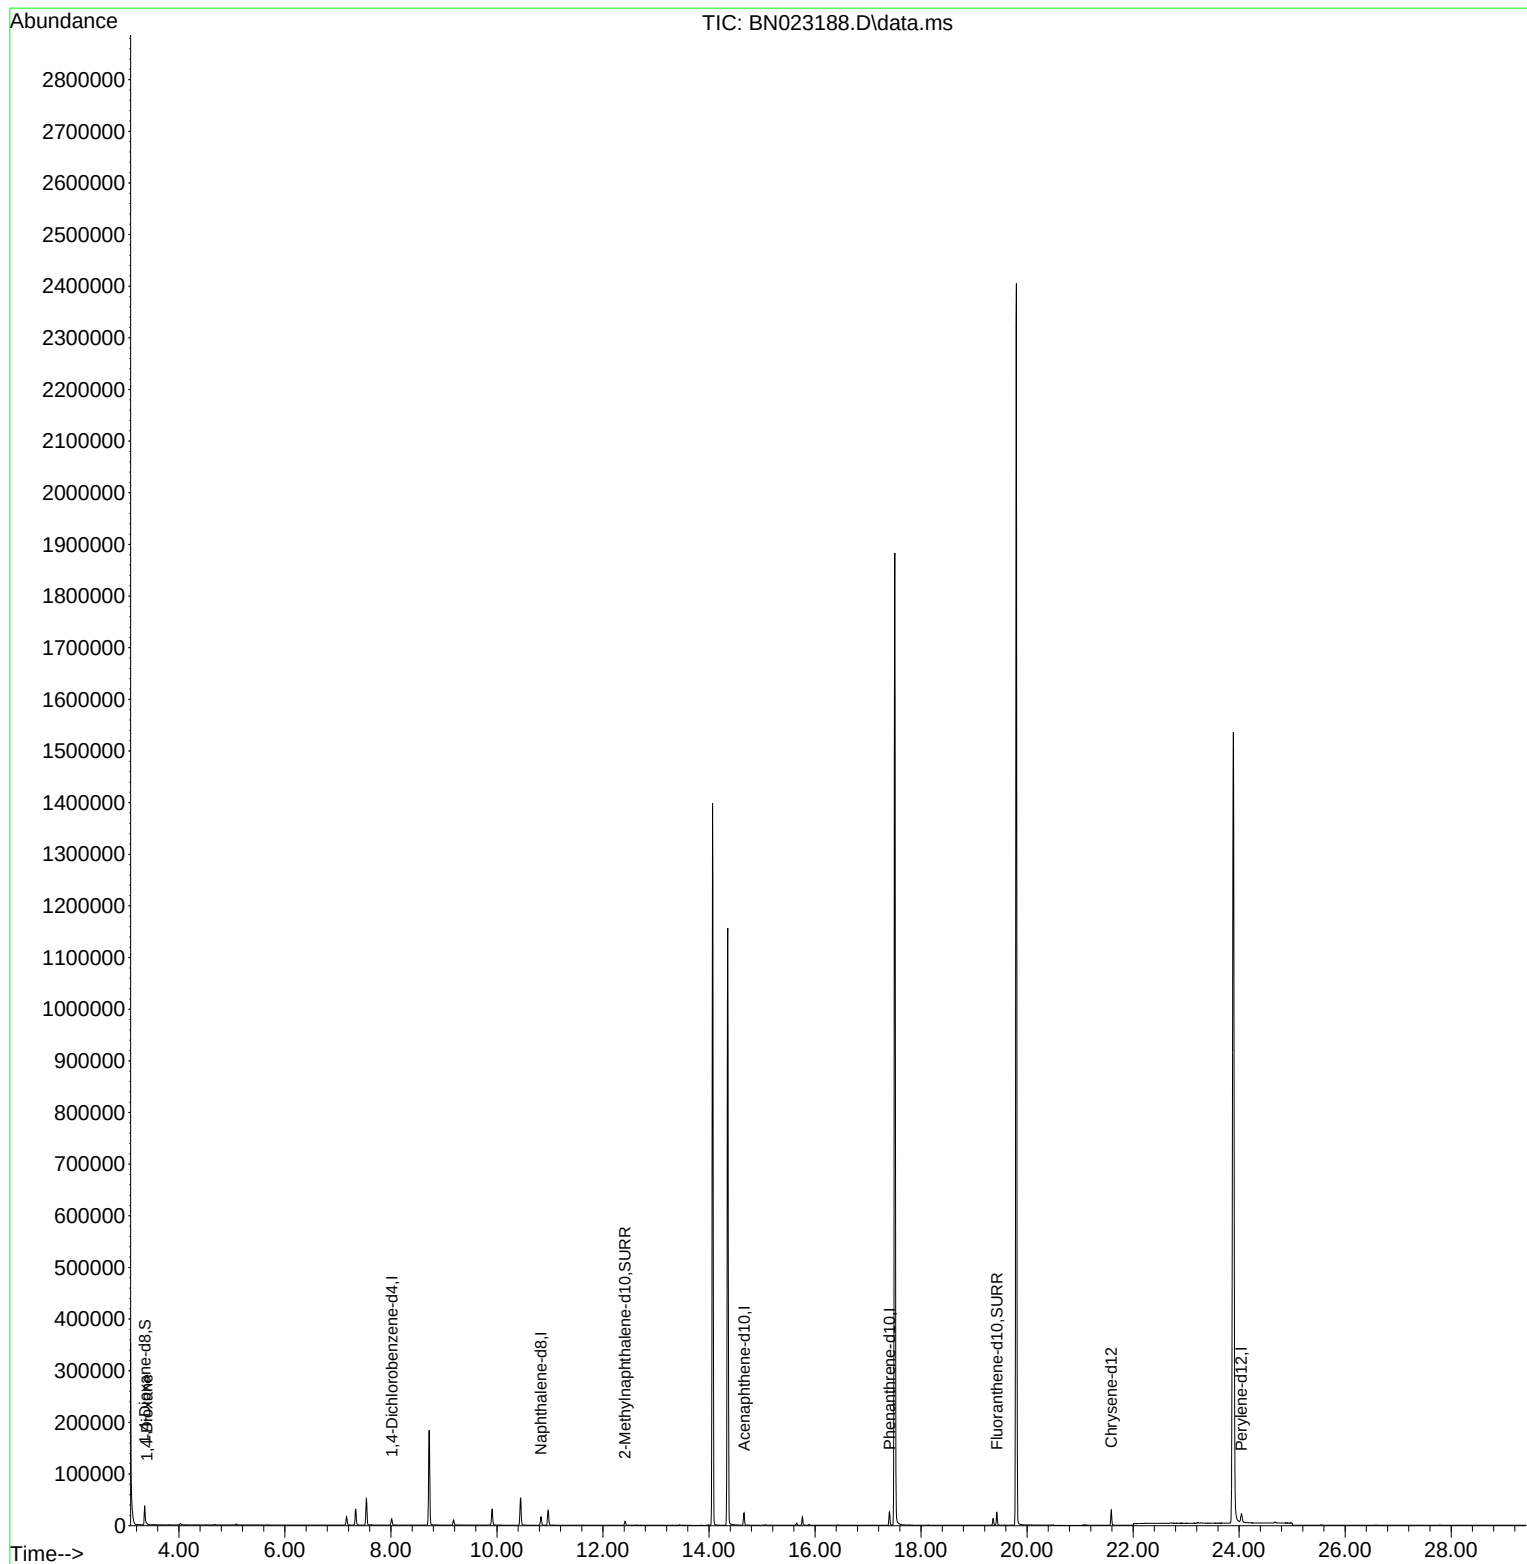

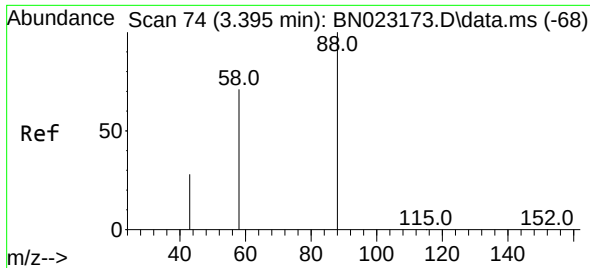

#2
 1,4-Dioxane
 Concen: 0.103 ng/ul
 RT: 3.395 min Scan# 74
 Delta R.T. 0.000 min
 Lab File: BN023188.D
 Acq: 14 Dec 2022 05:54

Instrument :
 BNA_N
 ClientSampleId :
 EXZB2

Tgt Ion: 88 Resp: 792
 Ion Ratio Lower Upper
 88 100
 43 73.1 26.2 39.4#
 58 50.0 47.6 71.4

