

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN121322\
 Data File : BN023189.D
 Acq On : 14 Dec 2022 06:30
 Operator : CG/JU
 Sample : N5948-03
 Misc :
 ALS Vial : 34 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 EXZB3

Quant Time: Dec 14 07:08:38 2022
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SFAM-EPA-SIM-BN112622.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Tue Dec 13 23:52:47 2022
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Dichlorobenzene-d4	8.015	152	5616	0.400	ng/ul	0.00
4) Naphthalene-d8	10.832	136	18436	0.400	ng/ul	0.00
9) Acenaphthene-d10	14.659	164	10989	0.400	ng/ul	0.00
13) Phenanthrene-d10	17.403	188	25502	0.400	ng/ul	0.00
17) Chrysene-d12	21.584	240	23705	0.400	ng/ul	0.00
23) Perylene-d12	24.039	264	22849	0.400	ng/ul	0.00
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.357	96	24841	3.686	ng/ul	0.00
6) 2-Methylnaphthalene-d10	12.416	152	8719	0.310	ng/ul	0.00
18) Fluoranthene-d10	19.430	212	23758	0.271	ng/ul	0.00
Target Compounds						
						Qvalue
2) 1,4-Dioxane	3.395	88	789	0.112	ng/ul#	69


(#) = qualifier out of range (m) = manual integration (+) = signals summed

```
Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN121322\  
Data File : BN023189.D  
Acq On    : 14 Dec 2022   06:30  
Operator  : CG/JU  
Sample    : N5948-03  
Misc      :  
ALS Vial  : 34    Sample Multiplier: 1
```

Instrument :
BNA_N
ClientSampleId :
EXZB3


Quant Time: Dec 14 07:08:38 2022
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SFAM-EPA-SIM-BN112622.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
Qlast Update : Tue Dec 13 23:52:47 2022
Response via : Initial Calibration

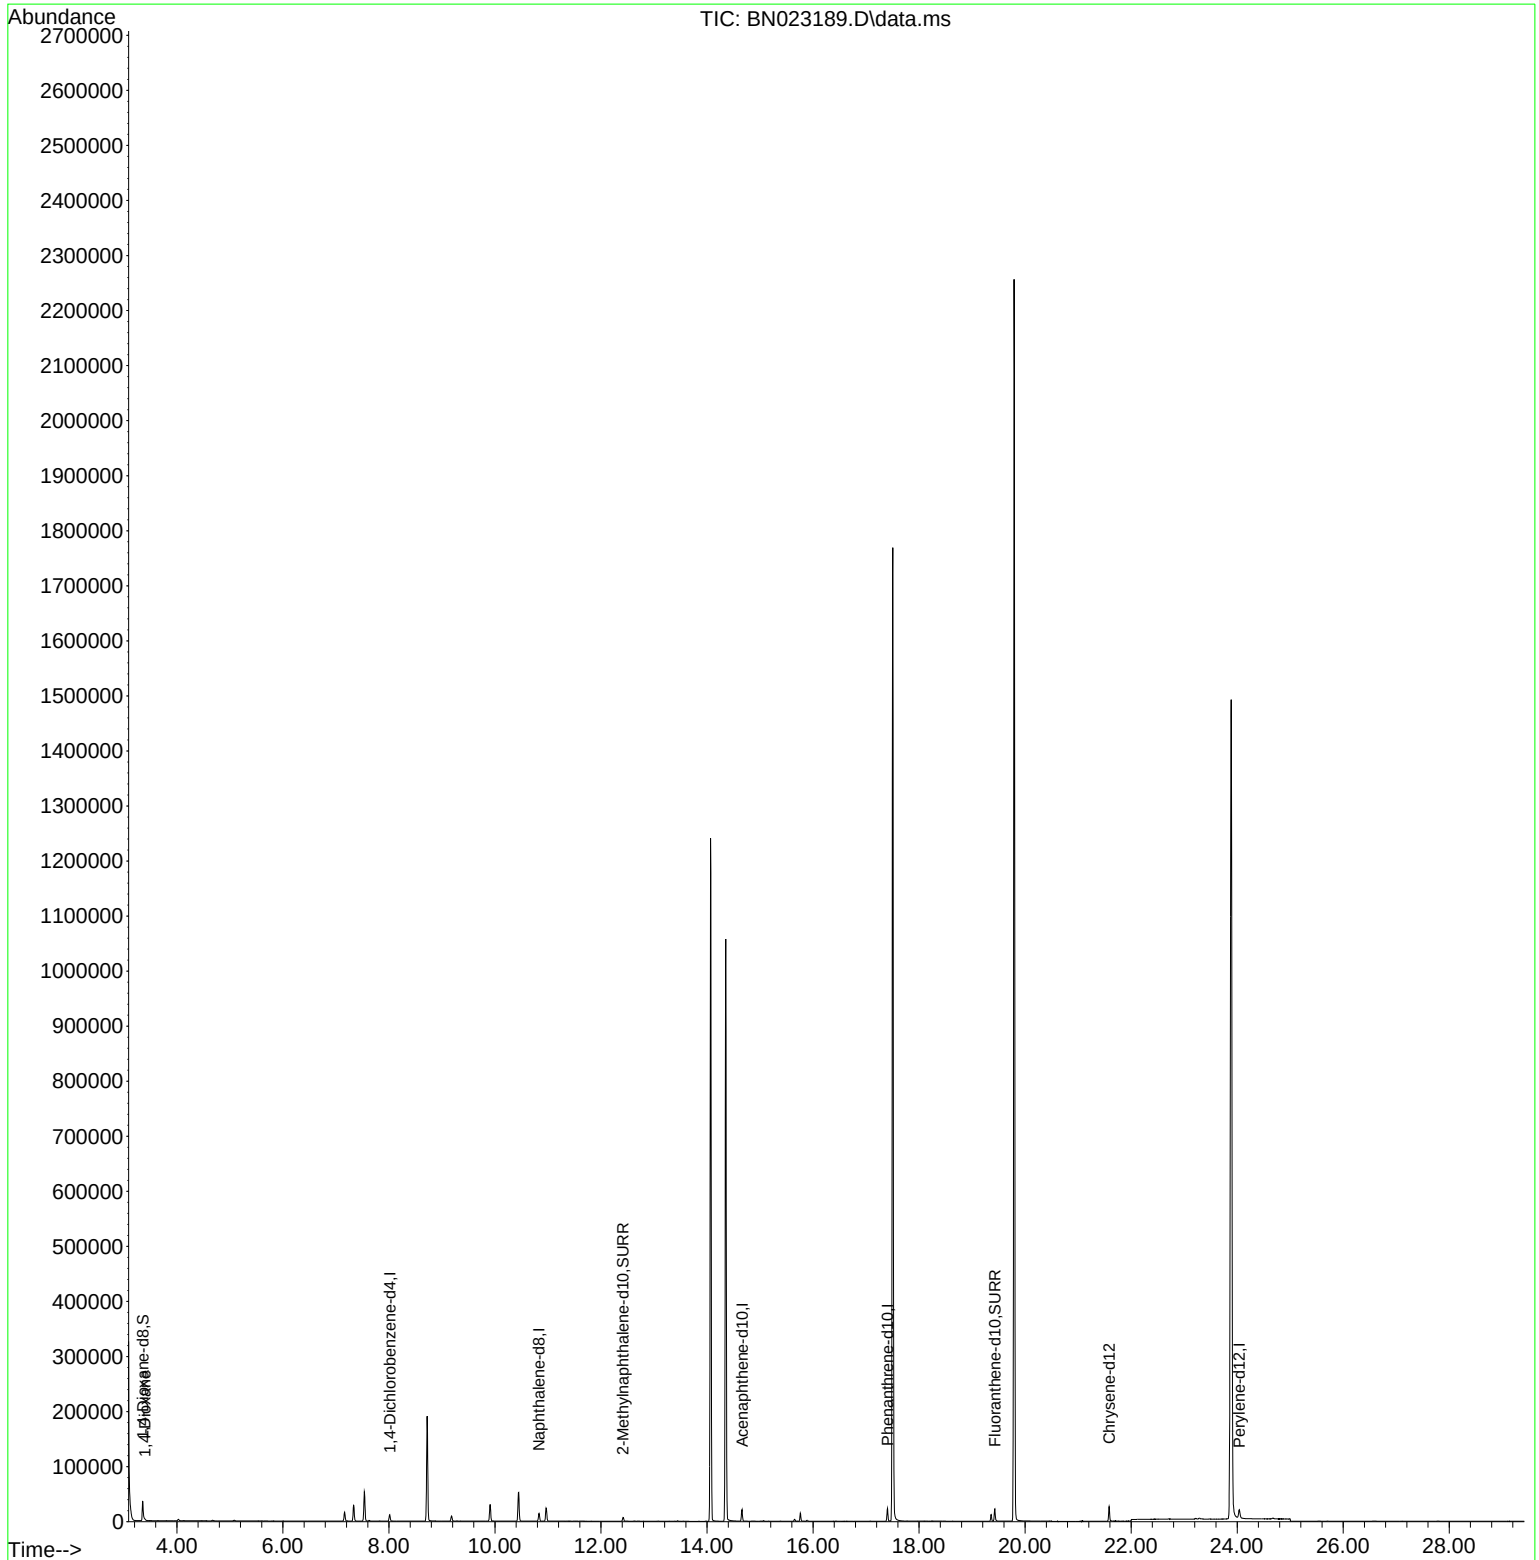

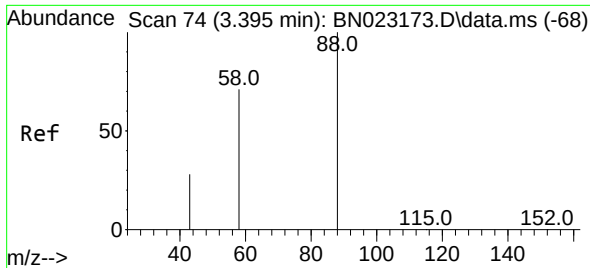

#2
 1,4-Dioxane
 Concen: 0.112 ng/ul
 RT: 3.395 min Scan# 74
 Delta R.T. 0.000 min
 Lab File: BN023189.D
 Acq: 14 Dec 2022 06:30

Instrument :
 BNA_N
 ClientSampleId :
 EXZB3

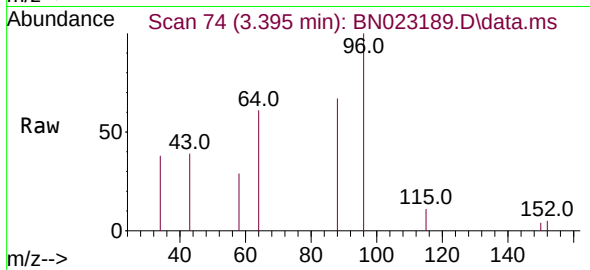

Tgt Ion:	88	Resp:	789
Ion	Ratio	Lower	Upper
88	100		
43	58.3	26.2	39.4#
58	42.5	47.6	71.4#

