

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN121322\
 Data File : BN023196.D
 Acq On : 14 Dec 2022 11:22
 Operator : CG/JU
 Sample : N5948-08
 Misc :
 ALS Vial : 42 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 EXZ94

Quant Time: Dec 14 23:19:34 2022
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SFAM-EPA-SIM-BN112622.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Tue Dec 13 23:52:47 2022
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Dichlorobenzene-d4	8.015	152	5069	0.400	ng/ul	0.00
4) Naphthalene-d8	10.832	136	16706	0.400	ng/ul	0.00
9) Acenaphthene-d10	14.659	164	9997	0.400	ng/ul	0.00
13) Phenanthrene-d10	17.403	188	23298	0.400	ng/ul	0.00
17) Chrysene-d12	21.585	240	21745	0.400	ng/ul	0.00
23) Perylene-d12	24.044	264	21051	0.400	ng/ul	0.00
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.357	96	23511	3.865	ng/ul	0.00
6) 2-Methylnaphthalene-d10	12.415	152	7821	0.307	ng/ul	0.00
18) Fluoranthene-d10	19.429	212	22253	0.277	ng/ul	0.00
Target Compounds						
					Qvalue	
2) 1,4-Dioxane	3.391	88	1261	0.199	ng/ul#	79


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN121322\
Data File : BN023196.D
Acq On : 14 Dec 2022 11:22
Operator : CG/JU
Sample : N5948-08
Misc :
ALS Vial : 42 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
EXZ94

Quant Time: Dec 14 23:19:34 2022
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SFAM-EPA-SIM-BN112622.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Dec 13 23:52:47 2022
Response via : Initial Calibration

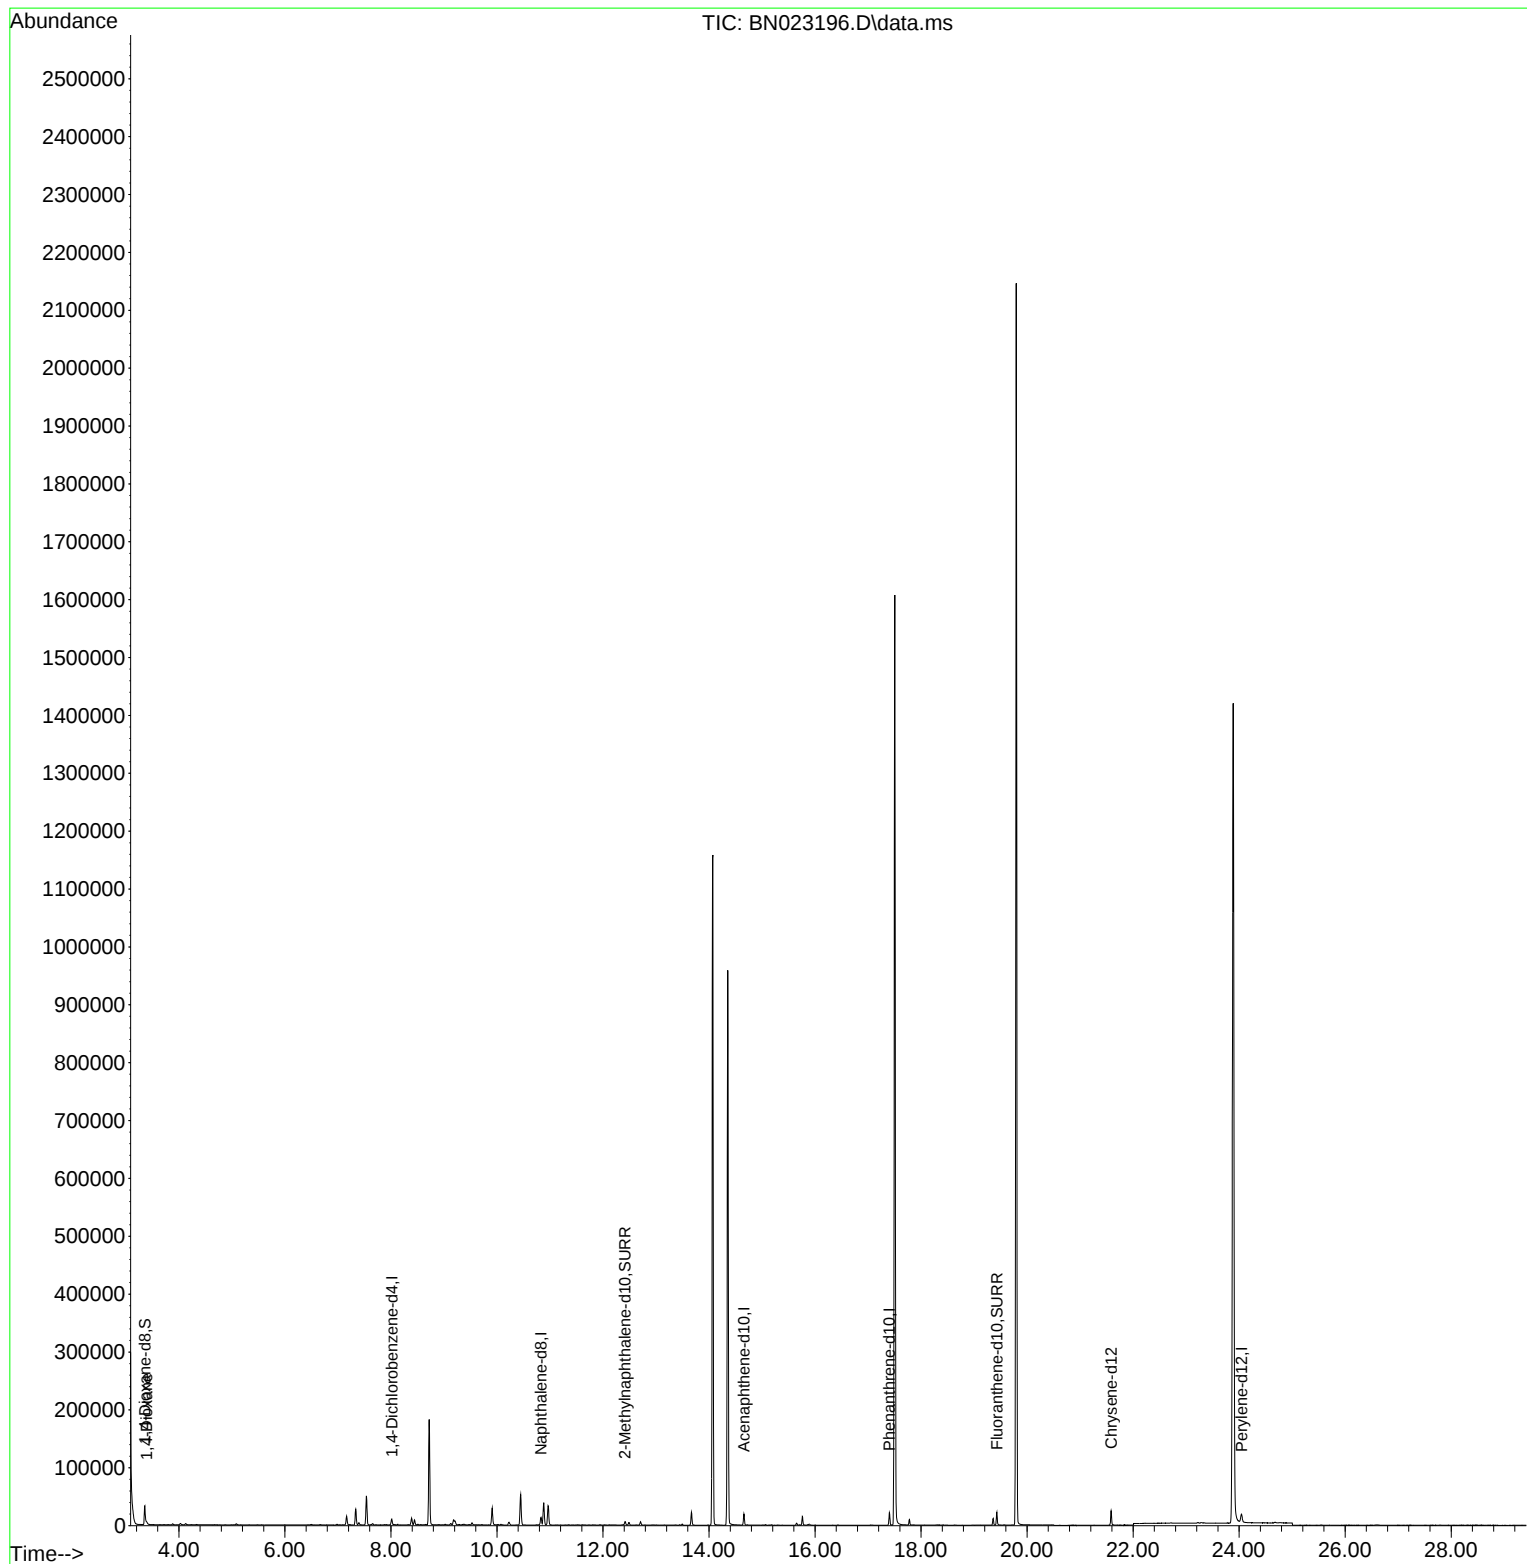

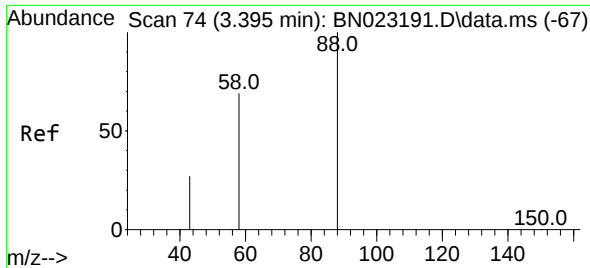

#2

1,4-Dioxane

Concen: 0.199 ng/ul

RT: 3.391 min Scan# 74

Delta R.T. -0.004 min

Lab File: BN023196.D


Acq: 14 Dec 2022 11:22

Instrument :

BNA_N

ClientSampleId :

EXZ94

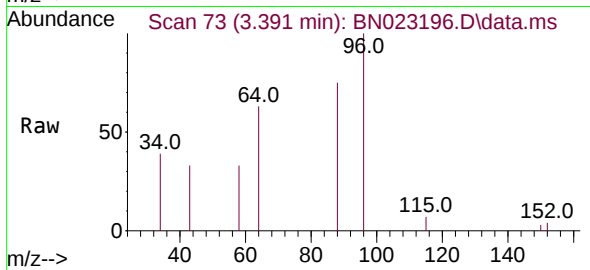

Tgt Ion: 88 Resp: 1261

Ion Ratio Lower Upper

88 100

43 43.4 26.2 39.4#

58 43.2 47.6 71.4#

