




Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN121324\
Data File : BN035589.D
Acq On : 13 Dec 2024 10:19
Operator : RC/JU
Sample : SSTDCCC0.4
Misc :
ALS Vial : 2 Sample Multiplier: 1

Instrument :
BNA_N
LabSampleId :
SSTDCCC0.4

Manual IntegrationsAPPROVED

Quant Time: Dec 13 11:32:39 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-SIM-BN111624.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Dec 10 16:10:57 2024
Response via : Initial Calibration

Reviewed By :Yogesh Patel 12/14/2024
Supervised By :mohammad ahmed 12/14/2024

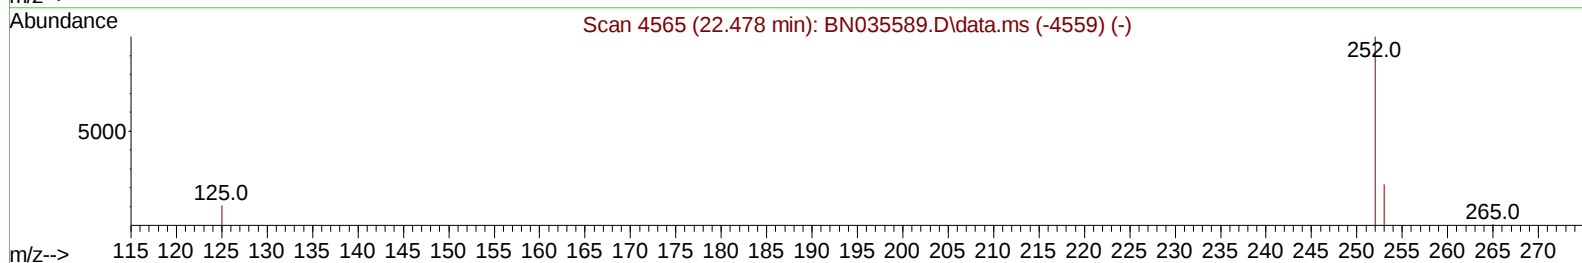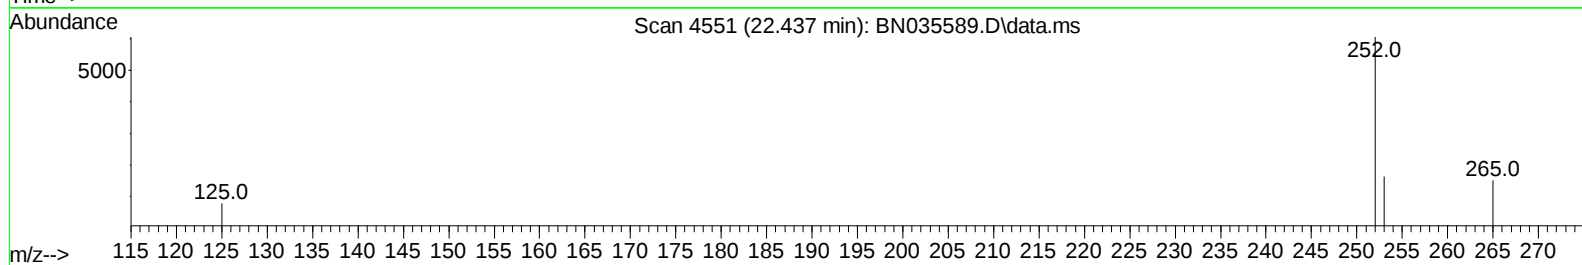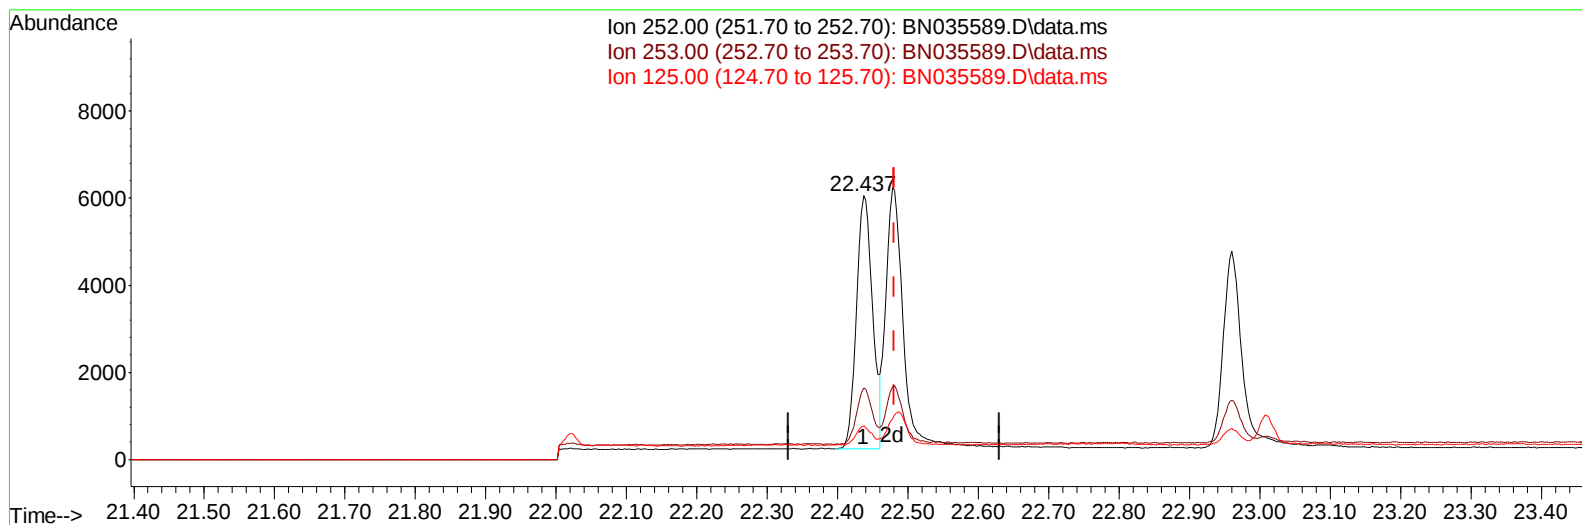

TIC: BN035589.D\data.ms

(25) Benzo(k)fluoranthene

22.437min (-0.044) 0.38 ng/u1

response 9290

Ion	Exp%	Act%
252.00	100.00	100.00
253.00	27.20	27.00
125.00	10.70	12.68
0.00	0.00	0.00




Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN121324\
Data File : BN035589.D
Acq On : 13 Dec 2024 10:19
Operator : RC/JU
Sample : SSTDCCC0.4
Misc :
ALS Vial : 2 Sample Multiplier: 1

Instrument :
BNA_N
LabSampleId :
SSTDCCC0.4

Manual IntegrationsAPPROVED

Quant Time: Dec 13 11:32:39 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-SIM-BN111624.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Dec 10 16:10:57 2024
Response via : Initial Calibration

Reviewed By :Yogesh Patel 12/14/2024
Supervised By :mohammad ahmed 12/14/2024

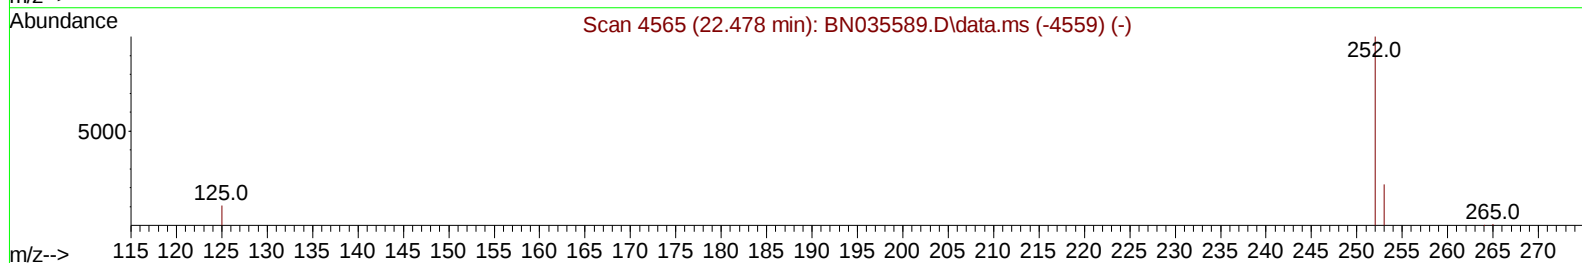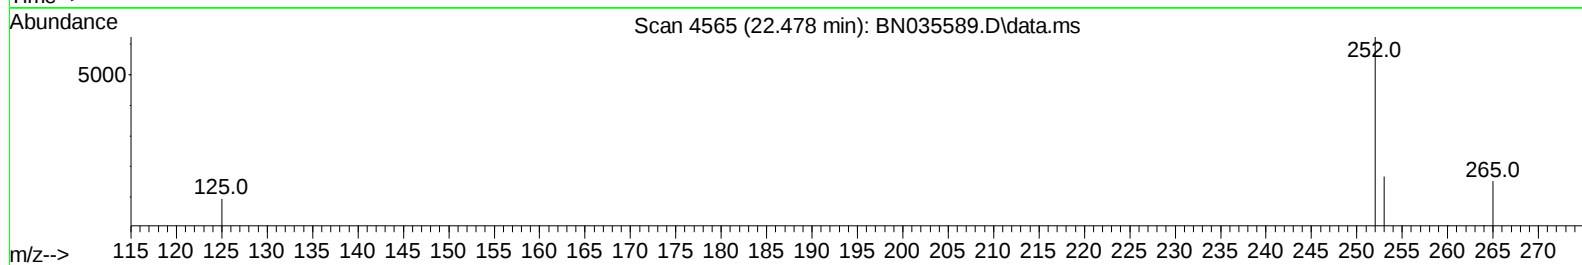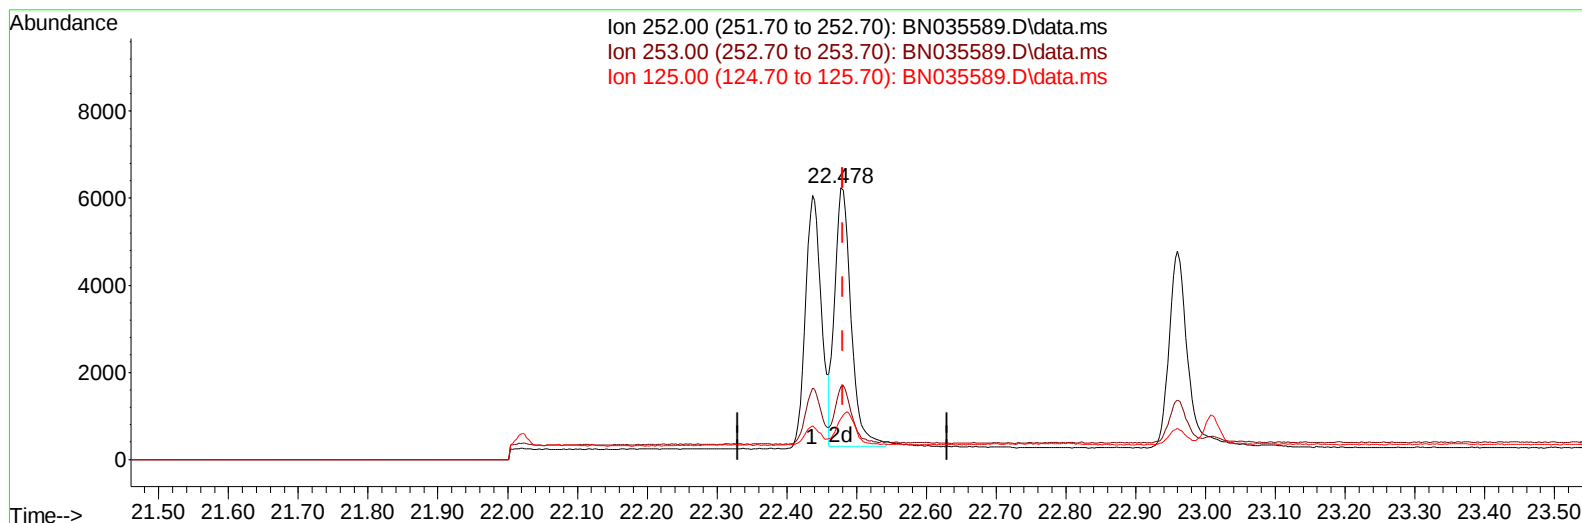

TIC: BN035589.D\data.ms

(25) Benzo(k)fluoranthene

22.478min (-0.003) 0.40 ng/u1 m

response 9711

Ion	Exp%	Act%
252.00	100.00	100.00
253.00	27.20	26.81
125.00	10.70	15.09#
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN121324\
 Data File : BN035589.D
 Acq On : 13 Dec 2024 10:19
 Operator : RC/JU
 Sample : SSTDCCC0.4
 Misc :
 ALS Vial : 2 Sample Multiplier: 1

Instrument :
 BNA_N
 LabSampleId :
 SSTDCCC0.4

Manual IntegrationsAPPROVED

Quant Time: Dec 13 11:32:39 2024
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-SIM-BN111624.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Tue Dec 10 16:10:57 2024
 Response via : Initial Calibration

Reviewed By :Yogesh Patel 12/14/2024
 Supervised By :mohammad ahmed 12/14/2024

Compound	R.T.	Q	Ion	Response	Conc	Units	Dev(Min)

Internal Standards							
1) 1,4-Dichlorobenzene-d4	7.289	152		1440	0.400	ng/ul	0.00
4) Naphthalene-d8	10.031	136		4210	0.400	ng/ul	# 0.00
9) Acenaphthene-d10	13.949	164		2854	0.400	ng/ul	0.00
13) Phenanthrene-d10	16.713	188		6686	0.400	ng/ul	# 0.00
17) Chrysene-d12	20.961	240		6808	0.400	ng/ul	# 0.00
23) Perylene-d12	23.051	264		7104	0.400	ng/ul	0.00
System Monitoring Compounds							
3) 1,4-Dioxane-d8	2.959	96		549	0.417	ng/ul	0.00
6) 2-Methylnaphthalene-d10	11.637	152		2462	0.399	ng/ul	0.00
18) Fluoranthene-d10	18.768	212		6887	0.367	ng/ul	0.00
Target Compounds							
						Qvalue	
2) 1,4-Dioxane	2.989	88		620	0.434	ng/ul#	84
5) Naphthalene	10.081	128		4663	0.440	ng/ul	97
7) 2-Methylnaphthalene	11.714	142		2882	0.392	ng/ul	98
8) 1-Methylnaphthalene	11.939	142		3022	0.407	ng/ul	98
10) Acenaphthylene	13.657	152		4694	0.415	ng/ul	98
11) Acenaphthene	14.009	153		3593	0.415	ng/ul	97
12) Fluorene	15.013	166		4171	0.410	ng/ul	99
14) Pentachlorophenol	16.380	266		912	0.586	ng/ul	98
15) Phenanthrene	16.755	178		7232	0.409	ng/ul	99
16) Anthracene	16.848	178		6471	0.394	ng/ul	99
19) Fluoranthene	18.796	202		8768	0.370	ng/ul#	96
20) Pyrene	19.163	202		9692	0.393	ng/ul#	94
21) Benzo(a)anthracene	20.947	228		9559	0.405	ng/ul	100
22) Chrysene	20.996	228		9950	0.419	ng/ul	100
24) Benzo(b)fluoranthene	22.437	252		9290	0.396	ng/ul	98
25) Benzo(k)fluoranthene	22.478	252		9711m	0.401	ng/ul	
26) Benzo(a)pyrene	22.960	252		8584	0.400	ng/ul#	97
27) Indeno(1,2,3-cd)pyrene	25.081	276		10573	0.365	ng/ul#	51
28) Dibenzo(a,h)anthracene	25.098	278		7947	0.350	ng/ul#	96
29) Benzo(g,h,i)perylene	25.691	276		8404	0.368	ng/ul#	95

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN121324\
Data File : BN035589.D
Acq On : 13 Dec 2024 10:19
Operator : RC/JU
Sample : SSTDCCC0.4
Misc :
ALS Vial : 2 Sample Multiplier: 1

Instrument :
BNA_N
LabSampleId :
SSTDCCC0.4

Manual IntegrationsAPPROVED

Quant Time: Dec 13 11:32:39 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-SIM-BN111624.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Dec 10 16:10:57 2024
Response via : Initial Calibration

Reviewed By :Yogesh Patel 12/14/2024
Supervised By :mohammad ahmed 12/14/2024

