




Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN121324\
Data File : BN035590.D
Acq On : 13 Dec 2024 10:55
Operator : RC/JU
Sample : PB165482BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
SBLK482

Manual IntegrationsAPPROVED

Quant Time: Dec 13 11:34:01 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-SIM-BN111624.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Dec 10 16:10:57 2024
Response via : Initial Calibration

Reviewed By :Yogesh Patel 12/14/2024
Supervised By :mohammad ahmed 12/14/2024

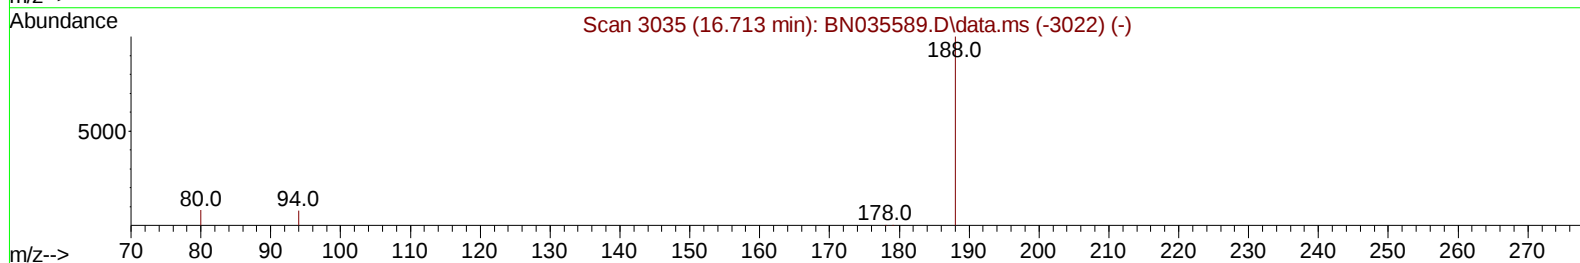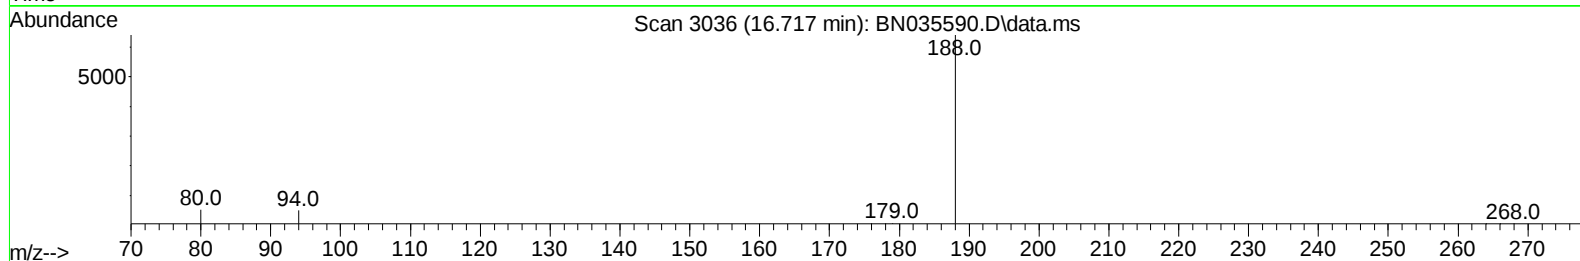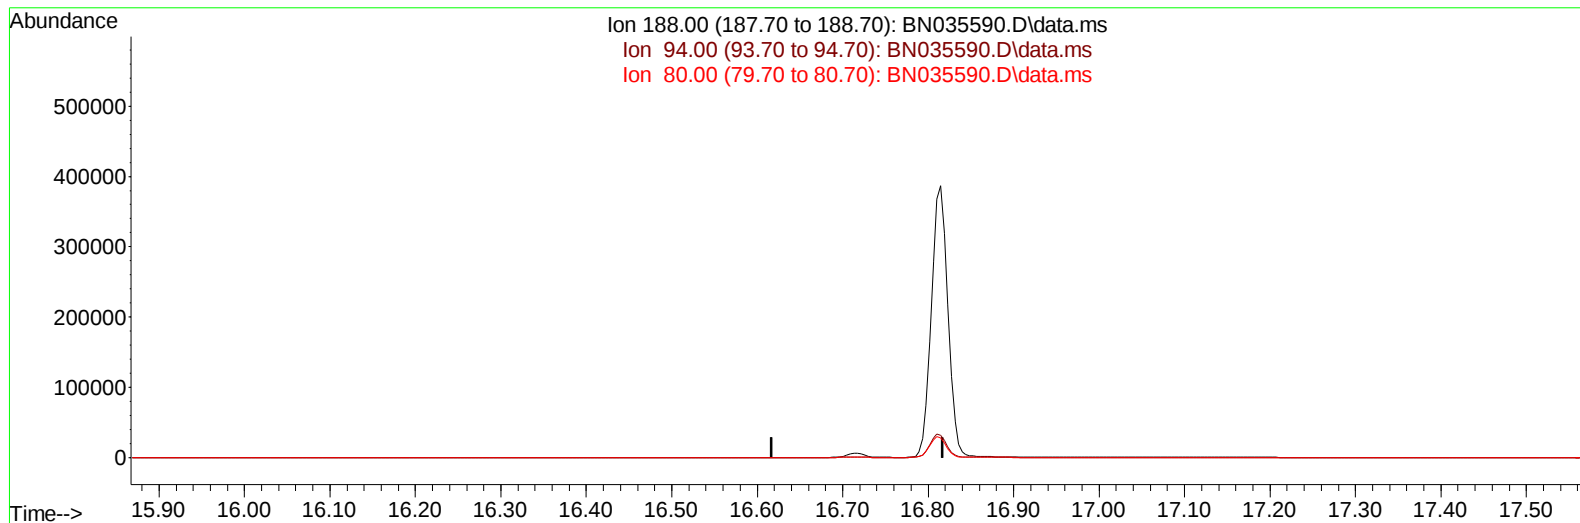

TIC: BN035590.D\data.ms

(13) Phenanthrene-d10 (I)

16.717min (-16.717) 0.00 ng/u1

response 0

Ion	Exp%	Act%
188.00	100.00	0.00
94.00	7.00	0.00#
80.00	7.60	0.00#
0.00	0.00	0.00




Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN121324\
Data File : BN035590.D
Acq On : 13 Dec 2024 10:55
Operator : RC/JU
Sample : PB165482BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
SBLK482

Manual IntegrationsAPPROVED

Quant Time: Dec 13 11:34:01 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-SIM-BN111624.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Dec 10 16:10:57 2024
Response via : Initial Calibration

Reviewed By :Yogesh Patel 12/14/2024
Supervised By :mohammad ahmed 12/14/2024

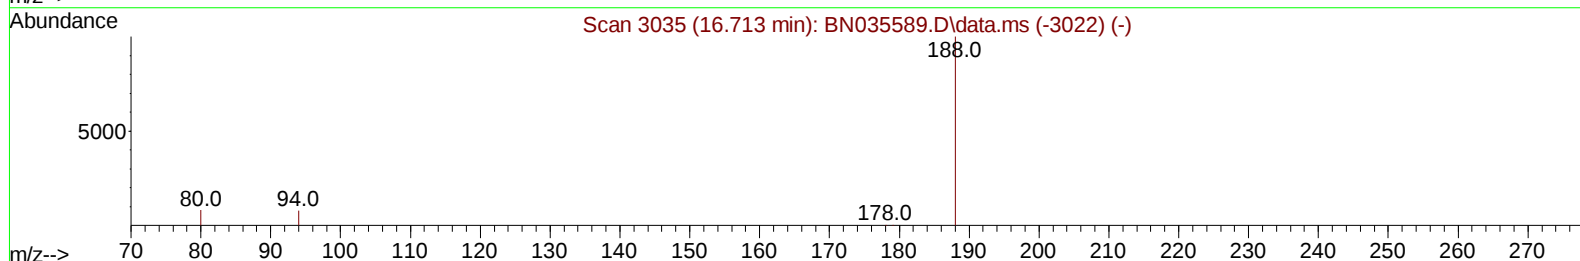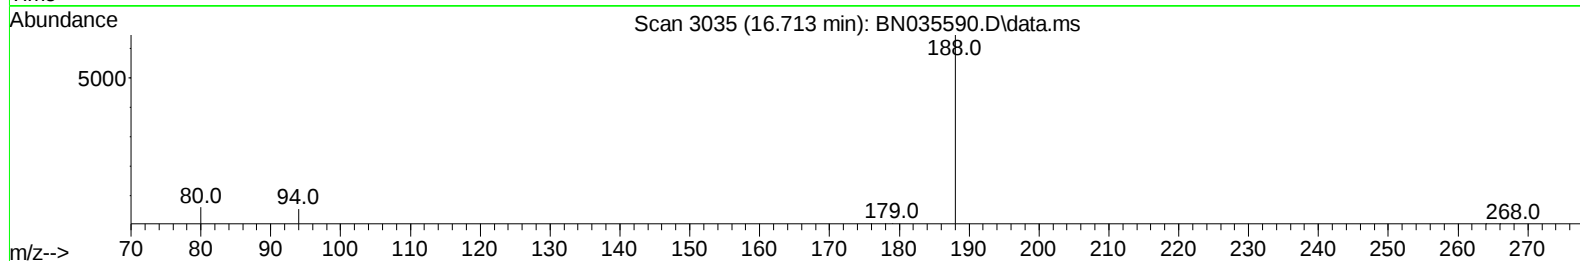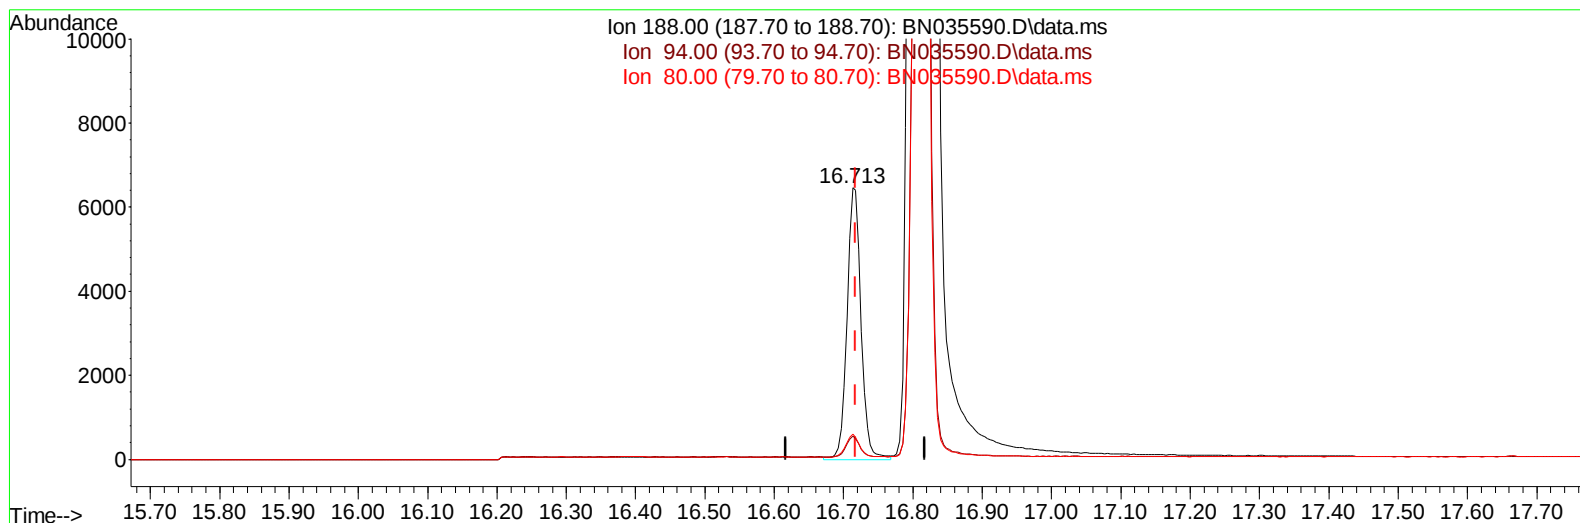

TIC: BN035590.D\data.ms

(13) Phenanthrene-d10 (I)

16.713min (-0.004) 0.40 ng/u1 m

response 9117

Ion	Exp%	Act%
188.00	100.00	100.00
94.00	7.00	8.58#
80.00	7.60	9.43#
0.00	0.00	0.00




Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN121324\
Data File : BN035590.D
Acq On : 13 Dec 2024 10:55
Operator : RC/JU
Sample : PB165482BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
SBLK482

Manual IntegrationsAPPROVED

Quant Time: Dec 13 11:34:01 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-SIM-BN111624.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Dec 10 16:10:57 2024
Response via : Initial Calibration

Reviewed By :Yogesh Patel 12/14/2024
Supervised By :mohammad ahmed 12/14/2024

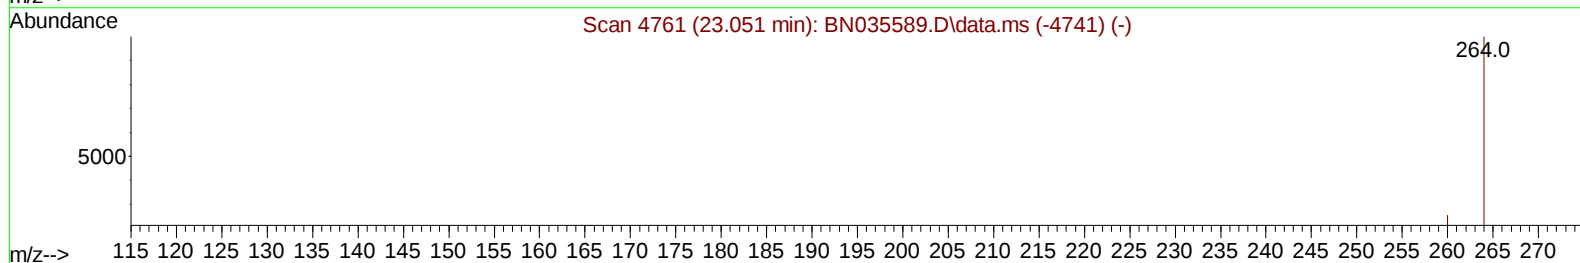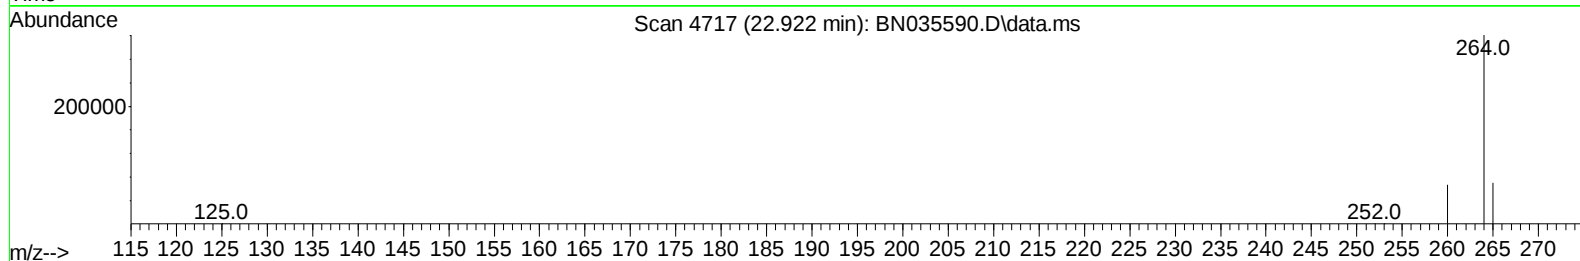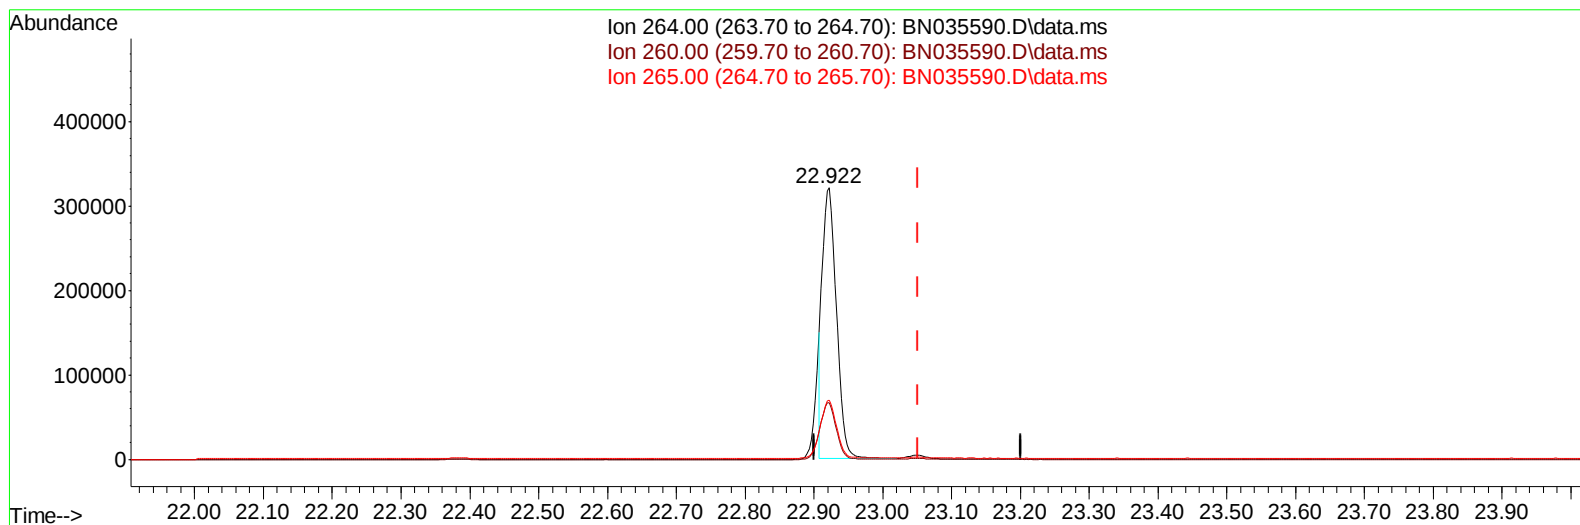

TIC: BN035590.D\data.ms

(23) Perylene-d12 (I)

22.922min (-0.128) 0.40 ng/u1

response 454763

Ion	Exp%	Act%
264.00	100.00	100.00
260.00	26.20	20.92#
265.00	75.50	21.78#
0.00	0.00	0.00




Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN121324\
Data File : BN035590.D
Acq On : 13 Dec 2024 10:55
Operator : RC/JU
Sample : PB165482BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
SBLK482

Manual IntegrationsAPPROVED

Quant Time: Dec 13 11:34:01 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-SIM-BN111624.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Dec 10 16:10:57 2024
Response via : Initial Calibration

Reviewed By :Yogesh Patel 12/14/2024
Supervised By :mohammad ahmed 12/14/2024

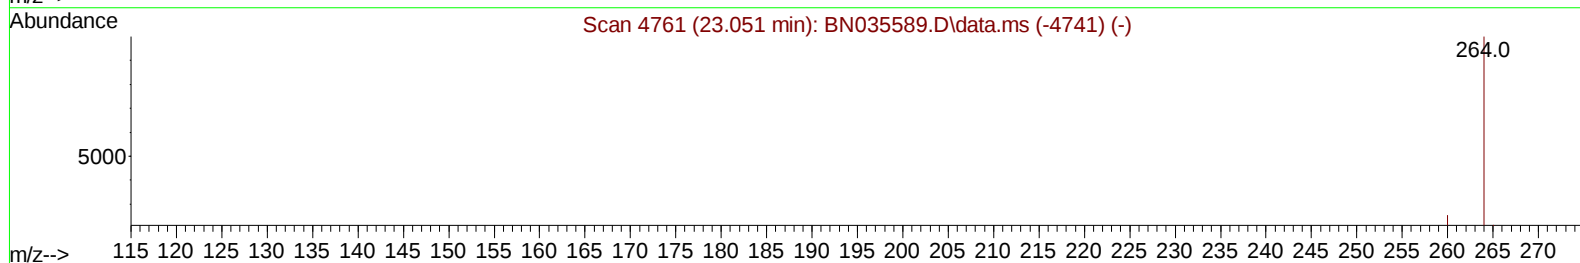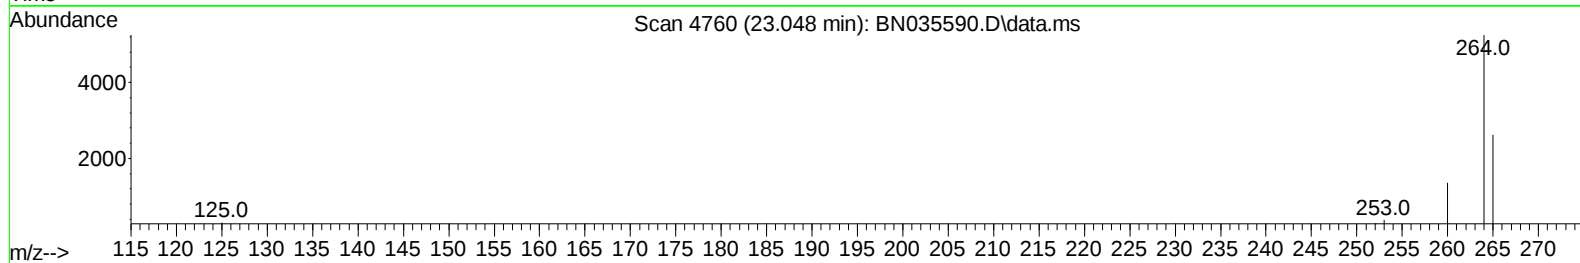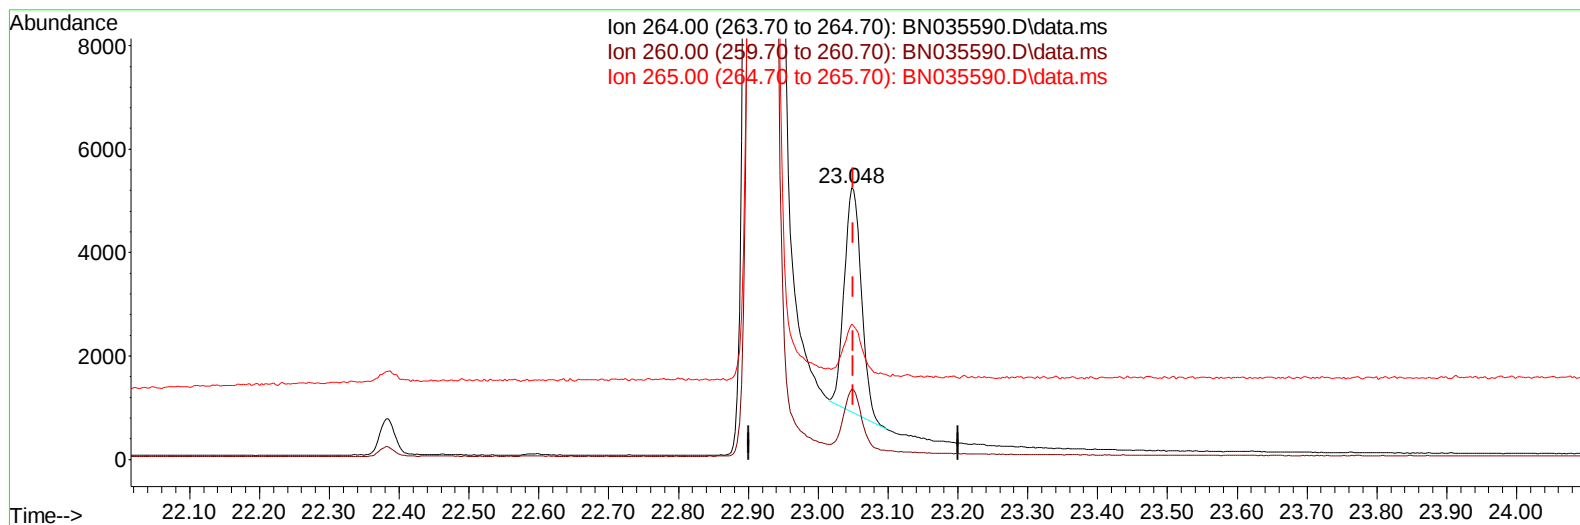

TIC: BN035590.D\data.ms

(23) Perylene-d12 (I)

23.048min (-0.003) 0.40 ng/ul m

response 7405

Ion	Exp%	Act%
264.00	100.00	100.00
260.00	26.20	25.81
265.00	75.50	49.96#
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN121324\
 Data File : BN035590.D
 Acq On : 13 Dec 2024 10:55
 Operator : RC/JU
 Sample : PB165482BL
 Misc :
 ALS Vial : 3 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 SBLK482

Manual IntegrationsAPPROVED

Reviewed By :Yogesh Patel 12/14/2024
 Supervised By :mohammad ahmed 12/14/2024

Quant Time: Dec 13 11:34:01 2024
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-SIM-BN111624.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Tue Dec 10 16:10:57 2024
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.289	152	1899	0.400	ng/ul	0.00
4) Naphthalene-d8	10.031	136	5500	0.400	ng/ul	0.00
9) Acenaphthene-d10	13.949	164	3874	0.400	ng/ul	0.00
13) Phenanthrene-d10	16.713	188	9117m	0.400	ng/ul	0.00
17) Chrysene-d12	20.961	240	7905	0.400	ng/ul	# 0.00
23) Perylene-d12	23.048	264	7405m	0.400	ng/ul	0.00
System Monitoring Compounds						
3) 1,4-Dioxane-d8	2.955	96	9252	5.331	ng/ul	0.00
6) 2-Methylnaphthalene-d10	11.637	152	2131	0.264	ng/ul	0.00
18) Fluoranthene-d10	18.768	212	5770	0.265	ng/ul	0.00

Target Compounds	Qvalue

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN121324\
Data File : BN035590.D
Acq On : 13 Dec 2024 10:55
Operator : RC/JU
Sample : PB165482BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
SBLK482

Manual IntegrationsAPPROVED

Quant Time: Dec 13 11:34:01 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-SIM-BN11624.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Dec 10 16:10:57 2024
Response via : Initial Calibration

Reviewed By :Yogesh Patel 12/14/2024
Supervised By :mohammad ahmed 12/14/2024

