

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN121324\
 Data File : BN035608.D
 Acq On : 13 Dec 2024 21:54
 Operator : RC/JU
 Sample : P5152-04
 Misc :
 ALS Vial : 20 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 BHK73

Manual Integrations
 APPROVED

Reviewed By :Yogesh Patel 12/14/2024
 Supervised By :mohammad ahmed 12/14/2024

Quant Time: Dec 13 22:32:45 2024
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-SIM-BN111624.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Tue Dec 10 16:10:57 2024
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.293	152	1855	0.400	ng/u1	0.00
4) Naphthalene-d8	10.036	136	5657	0.400	ng/u1	# 0.00
9) Acenaphthene-d10	13.953	164	3648	0.400	ng/u1	0.00
13) Phenanthrene-d10	16.721	188	6989m	0.400	ng/u1	0.00
17) Chrysene-d12	20.967	240	4872	0.400	ng/u1	# 0.00
23) Perylene-d12	23.056	264	5150m	0.400	ng/u1	0.00
System Monitoring Compounds						
3) 1,4-Dioxane-d8	2.959	96	7737	4.563	ng/u1	0.00
6) 2-Methylnaphthalene-d10	11.642	152	2507	0.302	ng/u1	0.00
18) Fluoranthene-d10	18.772	212	6055	0.451	ng/u1	0.00
Target Compounds						Qvalue
5) Naphthalene	10.086	128	503m	0.035	ng/u1	

(#) = qualifier out of range (m) = manual integration (+) = signals summed


Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN121324\
Data File : BN035608.D
Acq On : 13 Dec 2024 21:54
Operator : RC/JU
Sample : P5152-04
Misc :
ALS Vial : 20 Sample Multiplier: 1


Instrument :
BNA_N
ClientSampleId :
BHK73

Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 12/14/2024
Supervised By :mohammad ahmed 12/14/2024


Quant Time: Dec 13 22:32:45 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-SIM-BN111624.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Dec 10 16:10:57 2024
Response via : Initial Calibration

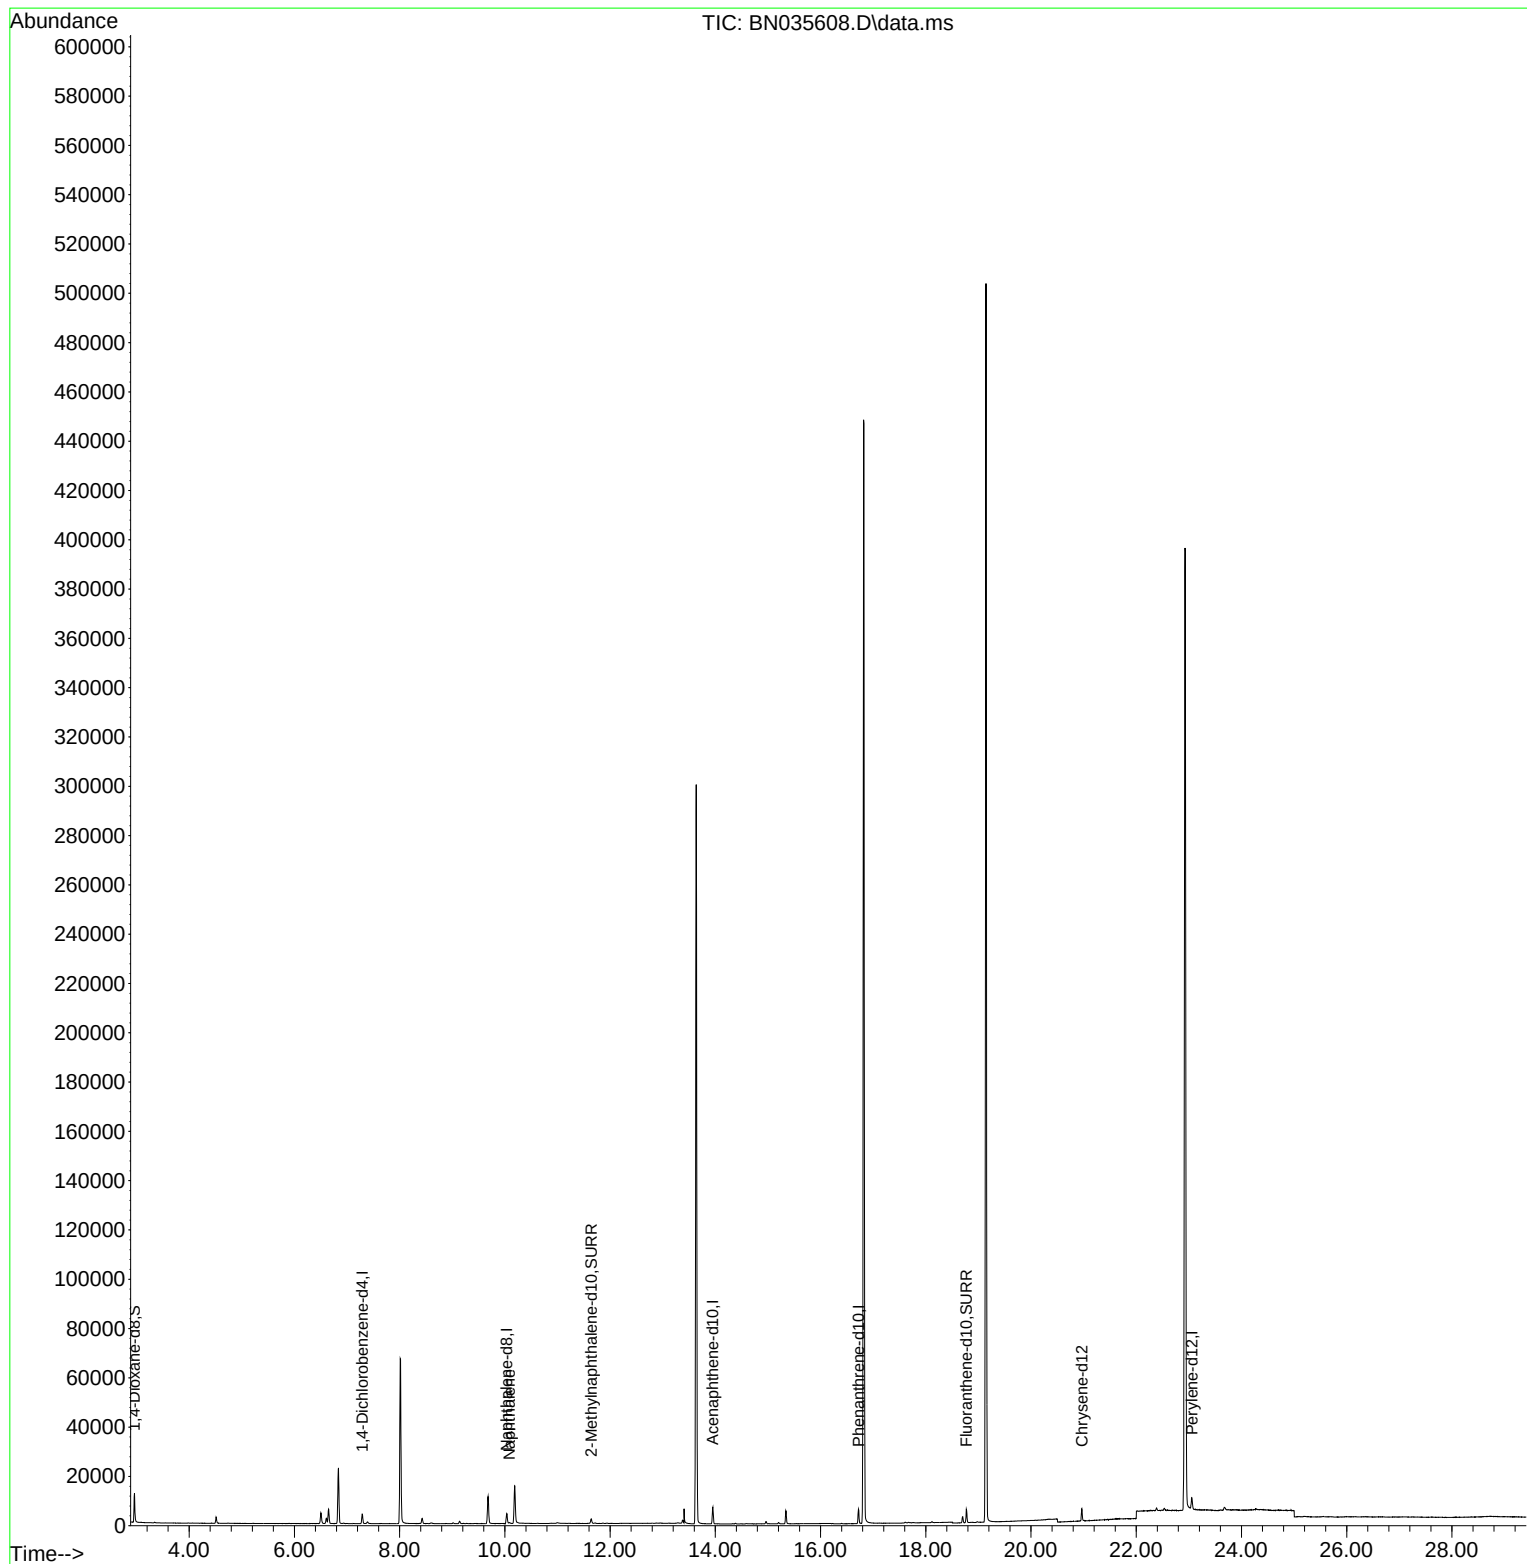

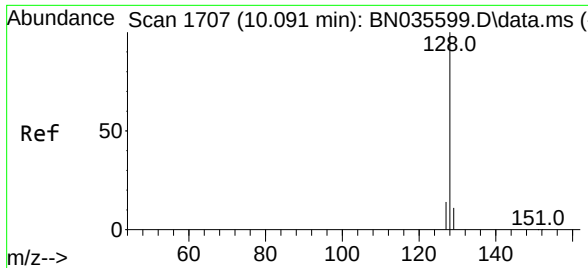

#5
Naphthalene
Concen: 0.035 ng/ul m
RT: 10.086 min Scan# 1
Delta R.T. -0.000 min
Lab File: BN035608.D
Acq: 13 Dec 2024 21:54

Instrument :
BNA_N
ClientSampleId :
BHK73

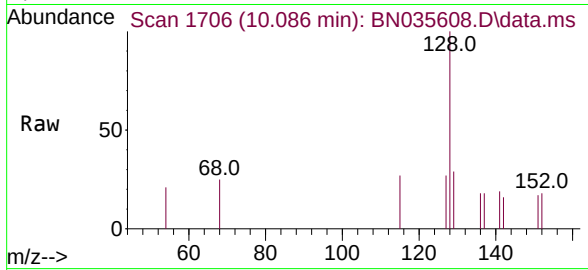

Tgt Ion:128 Resp: 500
Ion Ratio Lower Upper
128 100
129 29.4 9.9 14.9
127 27.4 11.4 17.2

Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 12/14/2024
Supervised By :mohammad ahmed 12/14/2024

