
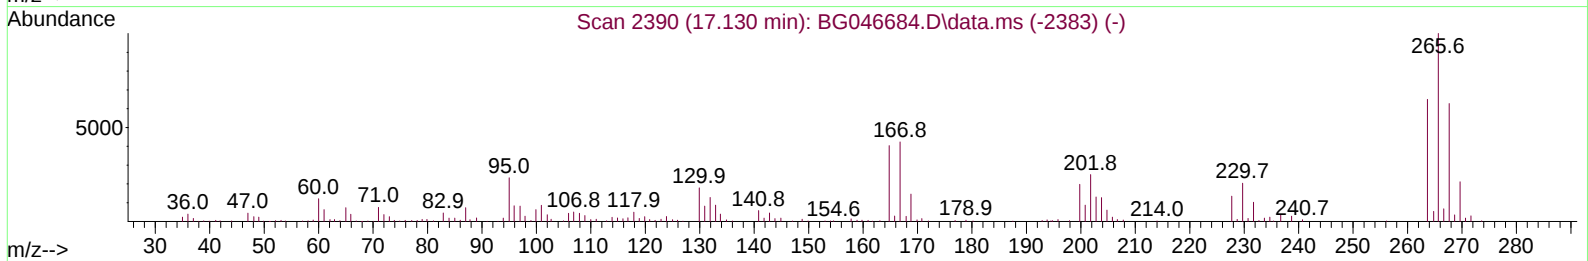
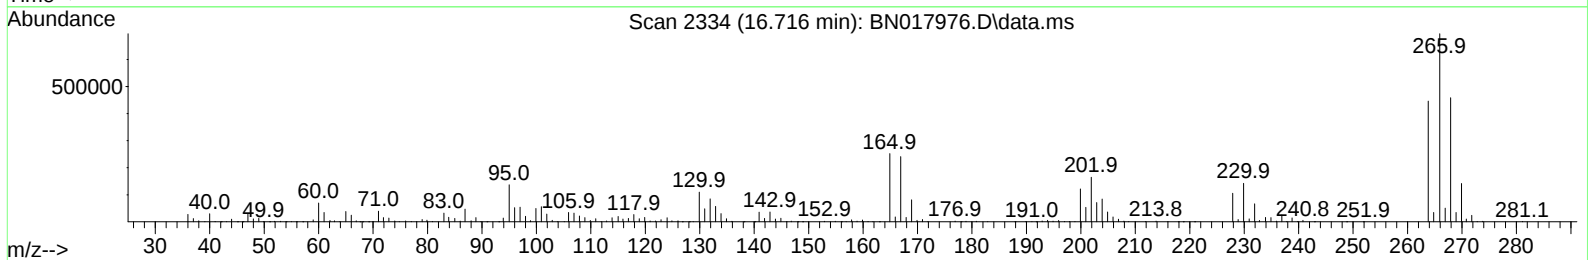


Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN121421\
 Data File : BN017976.D
 Acq On : 13 Dec 2021 19:23
 Operator : CG/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Quant Time: Dec 14 05:05:32 2021
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\8270E-Tune.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Tue Dec 14 05:05:27 2021
 Response via : Initial Calibration

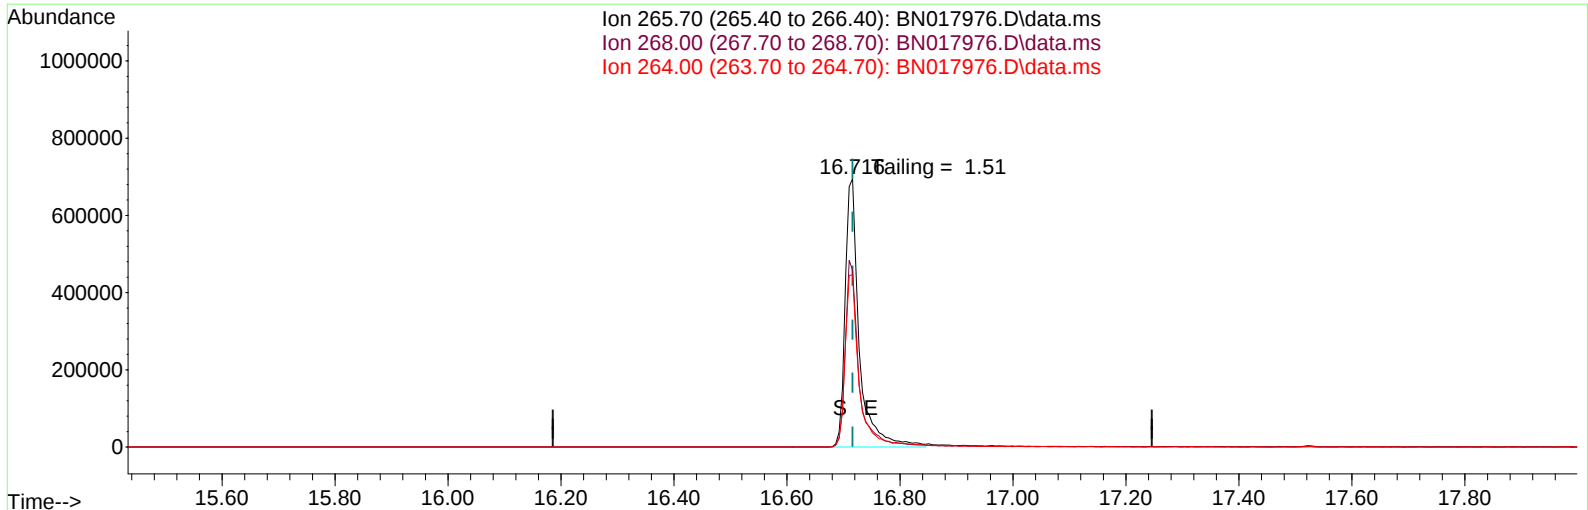

TIC: BN017976.D\data.ms

(70) Pentachlorophenol (C)




16.716min (0.000) 21628.39 ng

response 1233458

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	62.20	65.93
264.00	61.60	64.18
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN121421\
Data File : BN017976.D
Acq On : 13 Dec 2021 19:23
Operator : CG/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Dec 14 05:05:32 2021
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\8270E-Tune.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Dec 14 05:05:27 2021
Response via : Initial Calibration

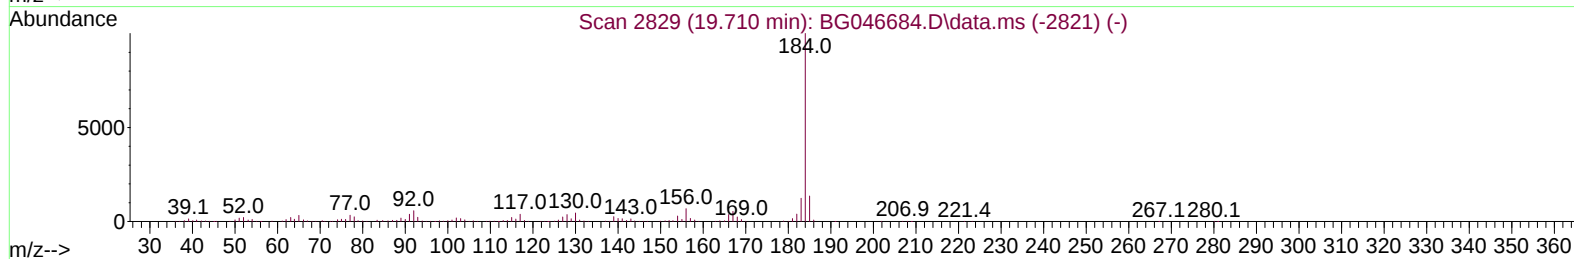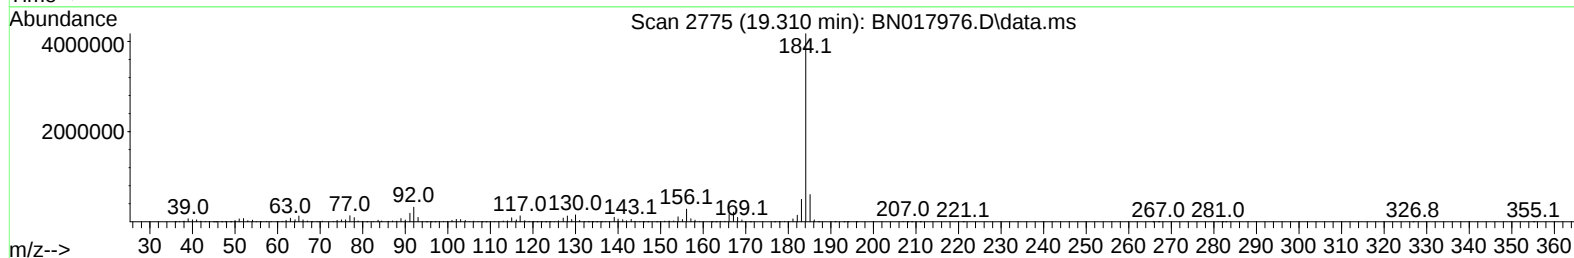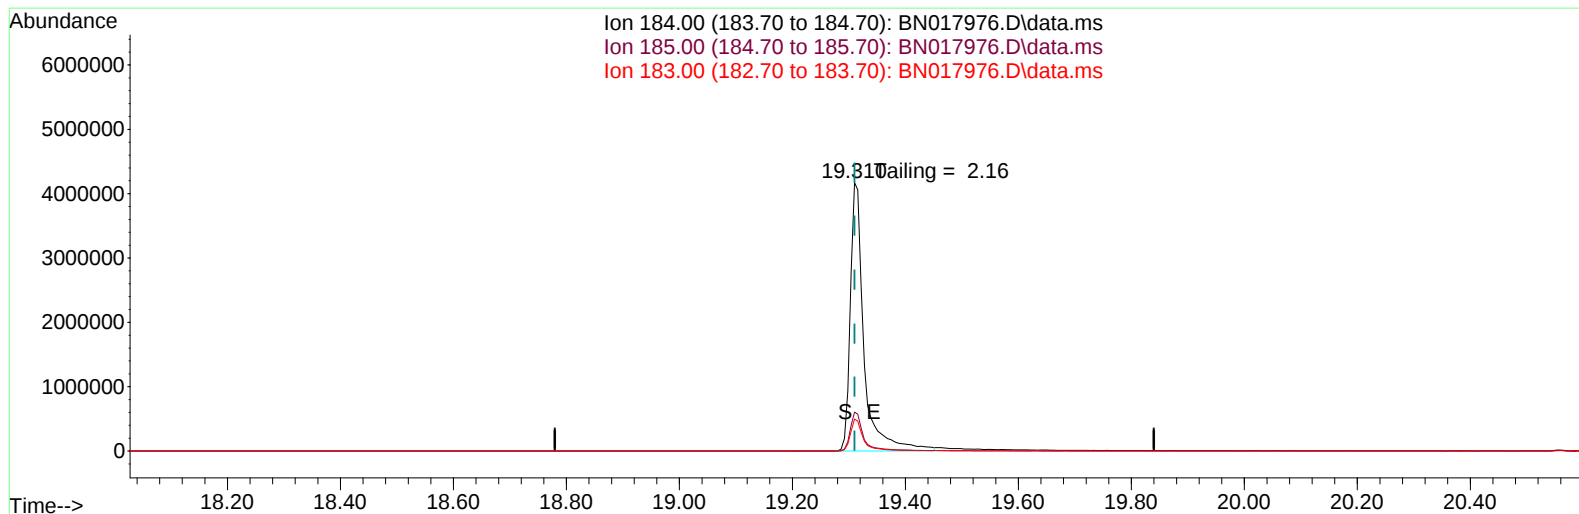

TIC: BN017976.D\data.ms

(77) Benzidine**19.310min (0.000) 2135094.19 ng****response 7305473**

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	15.50	14.49
183.00	13.20	11.92
0.00	0.00	0.00