
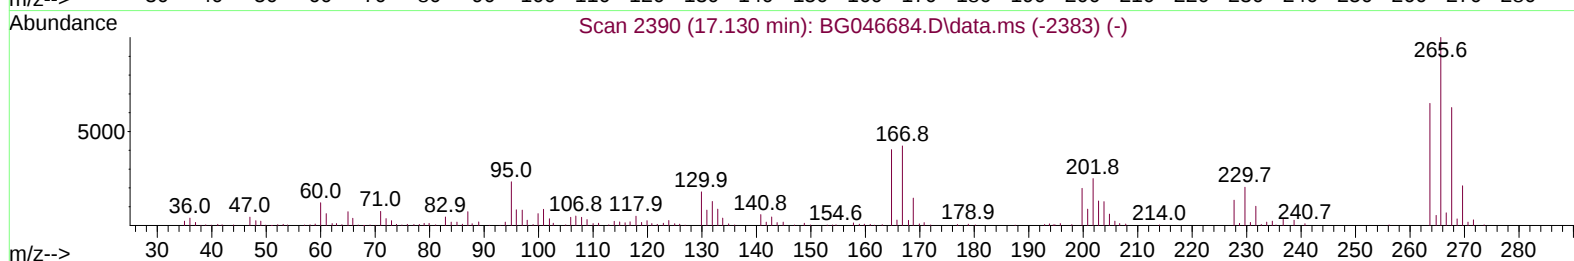
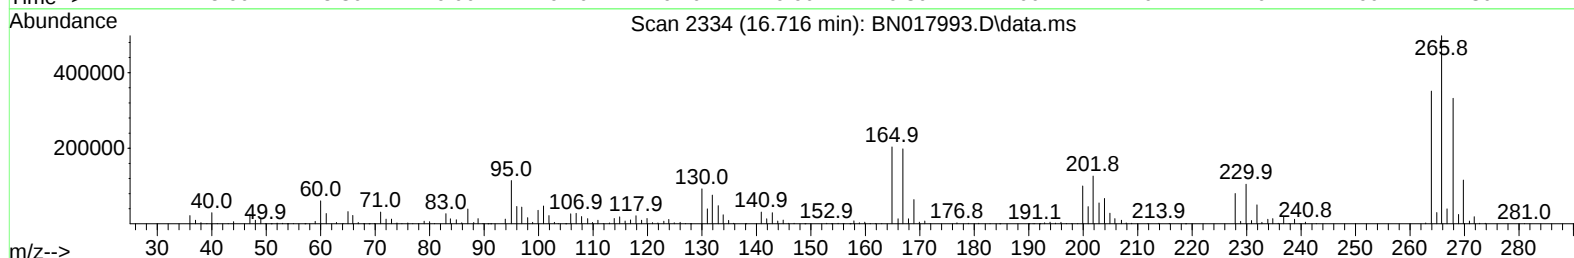


Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN121421\
 Data File : BN017993.D
 Acq On : 14 Dec 2021 07:23
 Operator : CG/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 20 Sample Multiplier: 1

Quant Time: Dec 14 08:18:53 2021
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\8270E-Tune.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Tue Dec 14 08:18:48 2021
 Response via : Initial Calibration

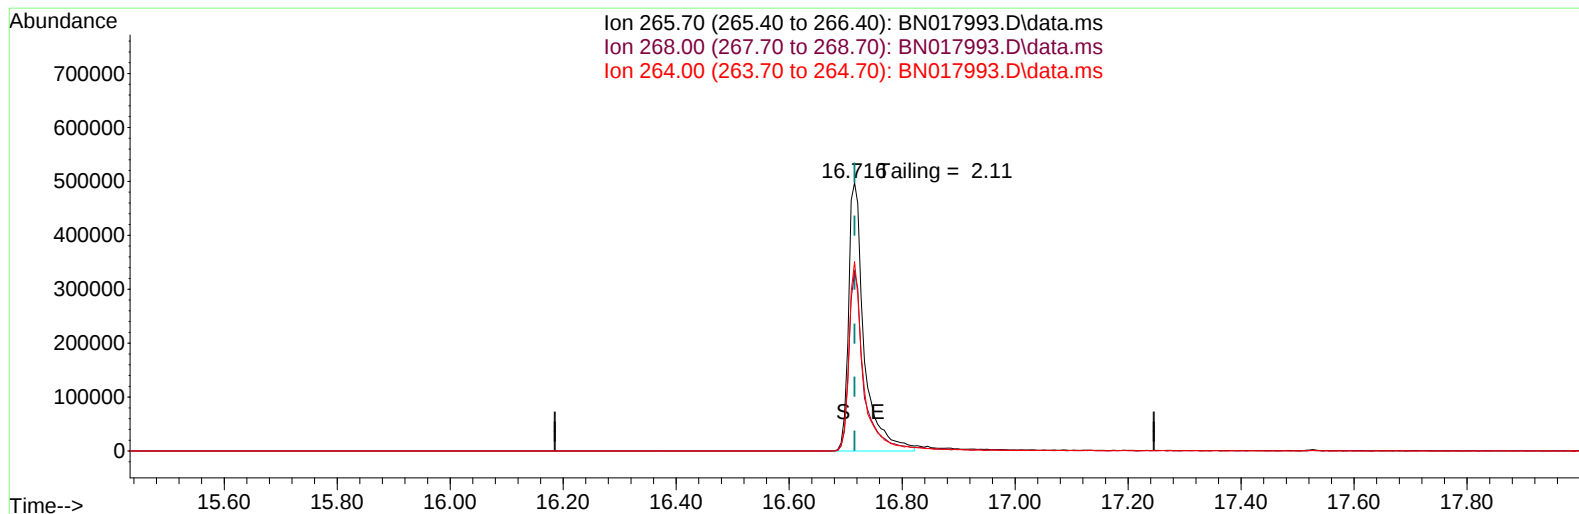

TIC: BN017993.D\data.ms

(70) Pentachlorophenol (C)




16.716min (0.000) 24474.91 ng

response 976691

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	62.20	66.76
264.00	61.60	70.56
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN121421\
Data File : BN017993.D
Acq On : 14 Dec 2021 07:23
Operator : CG/JU
Sample : DFTPP
Misc :
ALS Vial : 20 Sample Multiplier: 1

Quant Time: Dec 14 08:18:53 2021
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\8270E-Tune.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Dec 14 08:18:48 2021
Response via : Initial Calibration

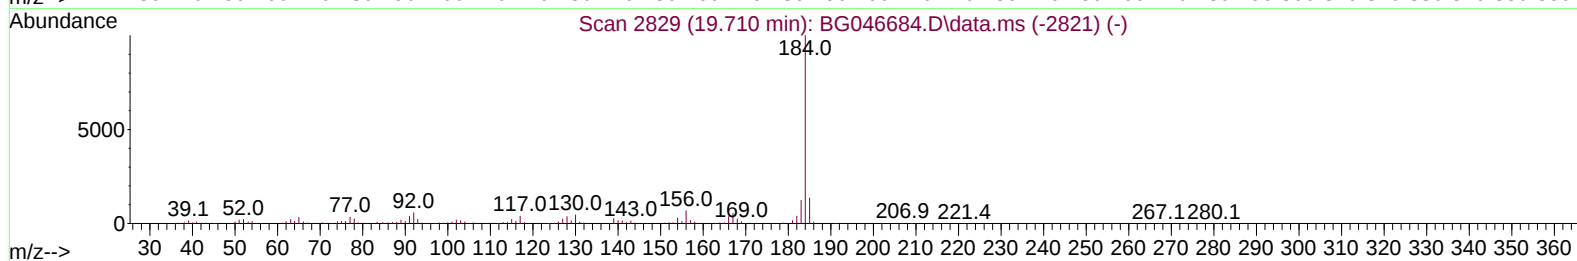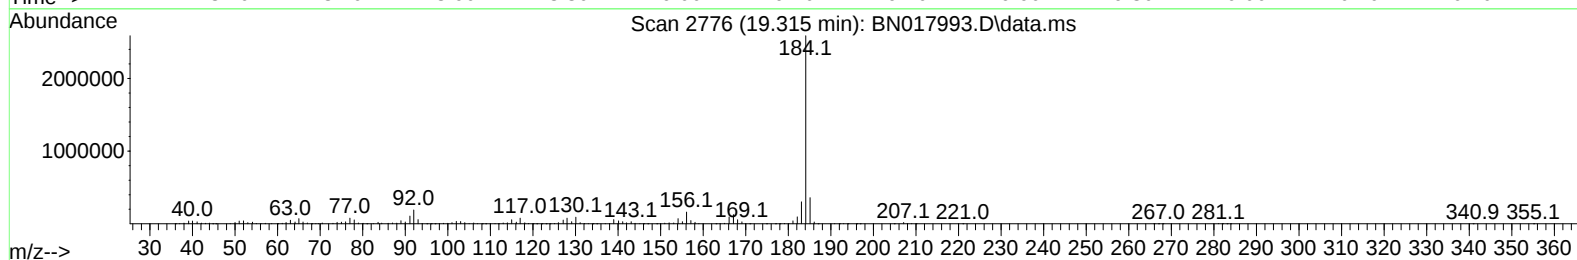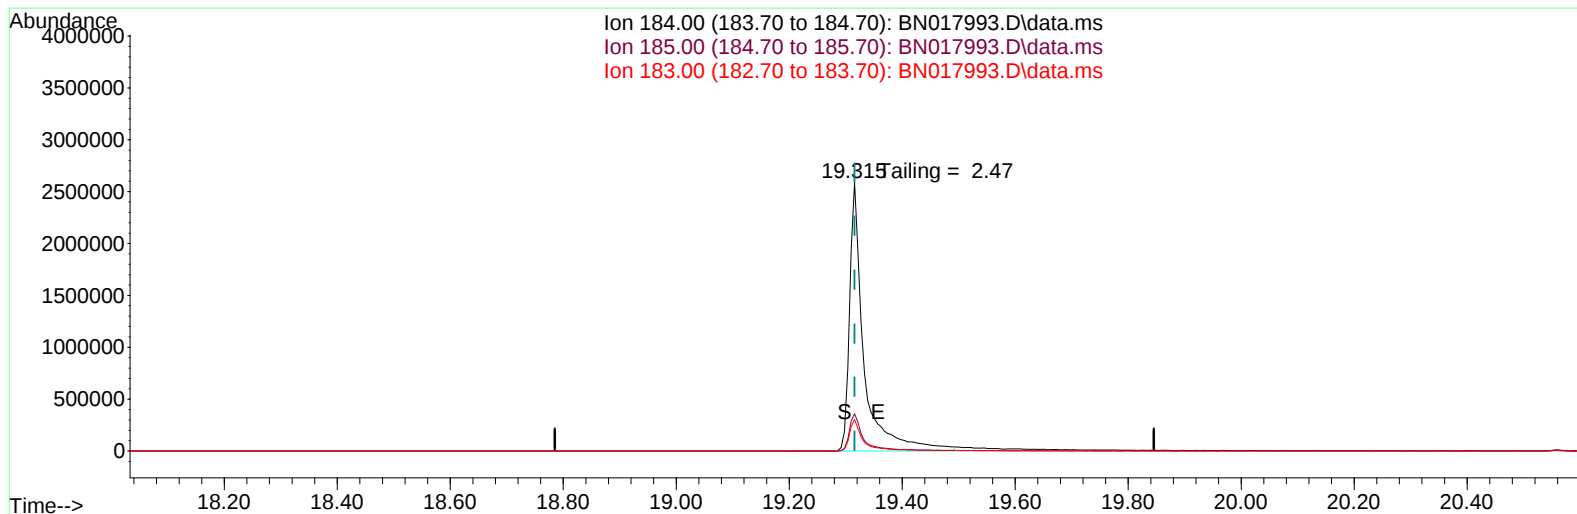

TIC: BN017993.D\data.ms

(77) Benzidine**19.315min (0.000) 1247100.05 ng****response 4766848**

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	15.50	13.88
183.00	13.20	11.70
0.00	0.00	0.00