
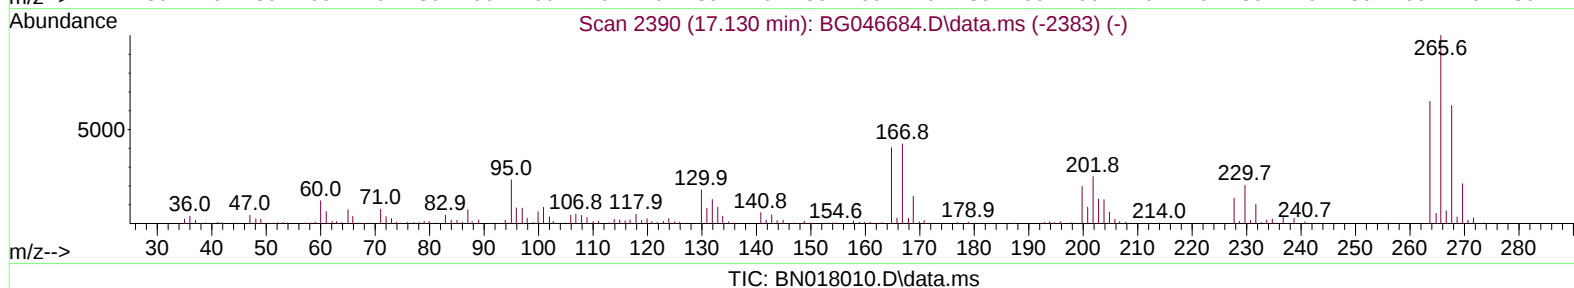
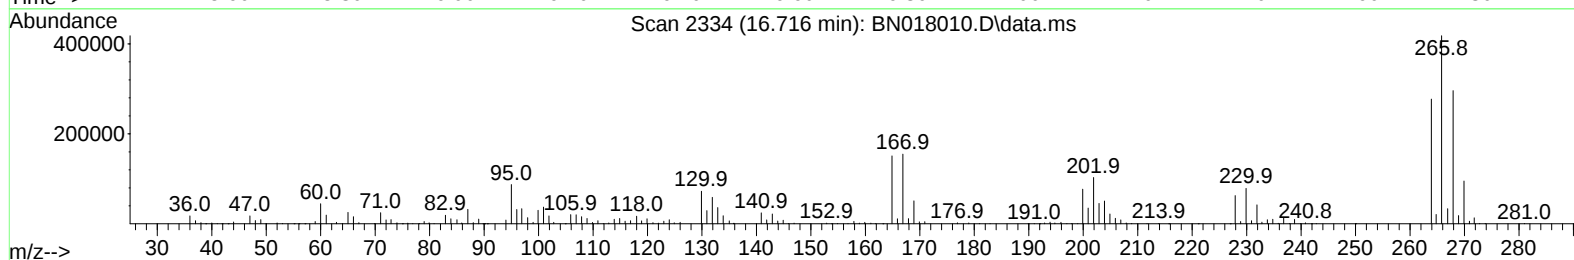


Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN121421\
Data File : BN018010.D
Acq On : 14 Dec 2021 19:31
Operator : CG/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Dec 15 05:00:09 2021
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\8270E-Tune.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Dec 15 05:00:04 2021
Response via : Initial Calibration

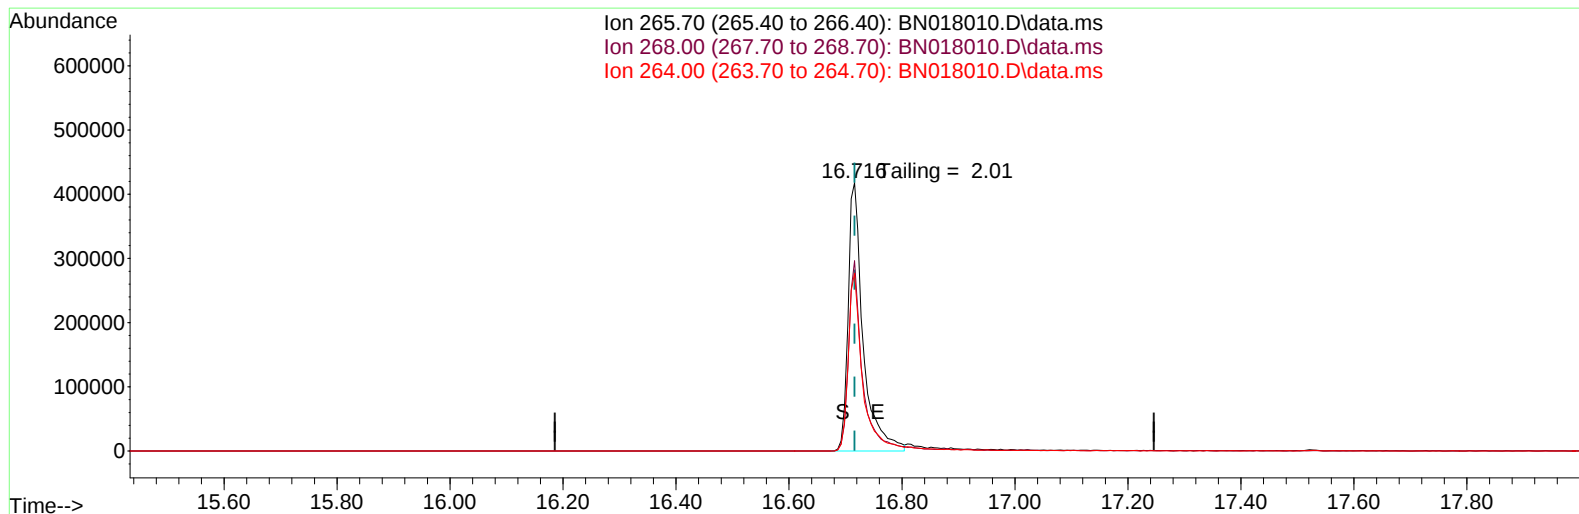

TIC: BN018010.D\data.ms

(70) Pentachlorophenol (C)




16.716min (0.000) 21375.88 ng

response 789611

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	62.20	70.87
264.00	61.60	66.32
0.00	0.00	0.00

```
Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN121421\  
Data File : BN018010.D  
Acq On    : 14 Dec 2021  19:31  
Operator  : CG/JU  
Sample    : DFTPP  
Misc      :  
ALS Vial  : 1    Sample Multiplier: 1
```

Quant Time: Dec 15 06:05:30 2021
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\8270E-Tune.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Dec 15 06:05:25 2021
Response via : Initial Calibration

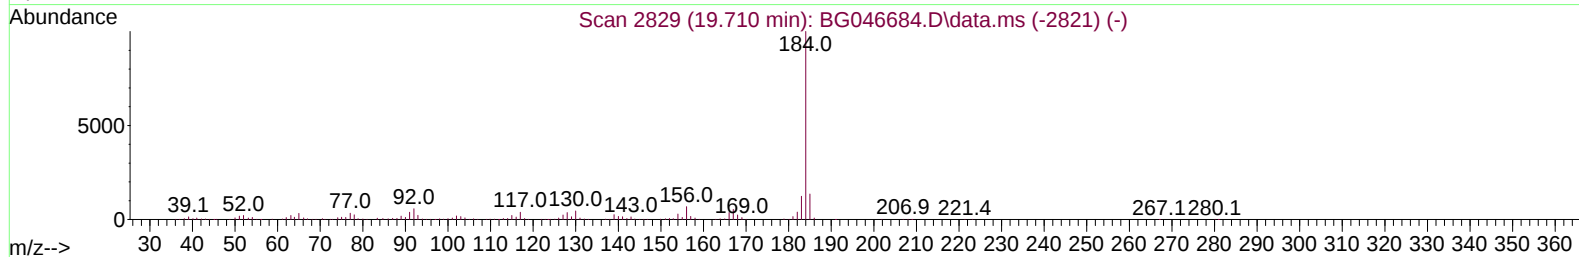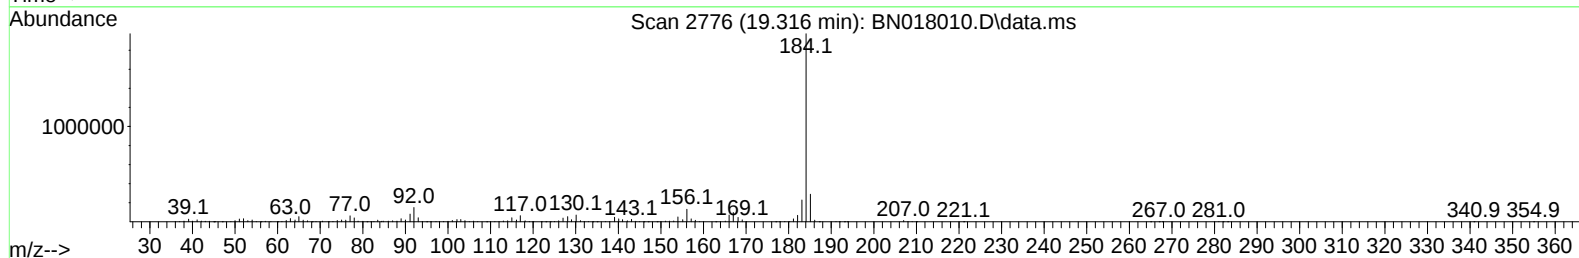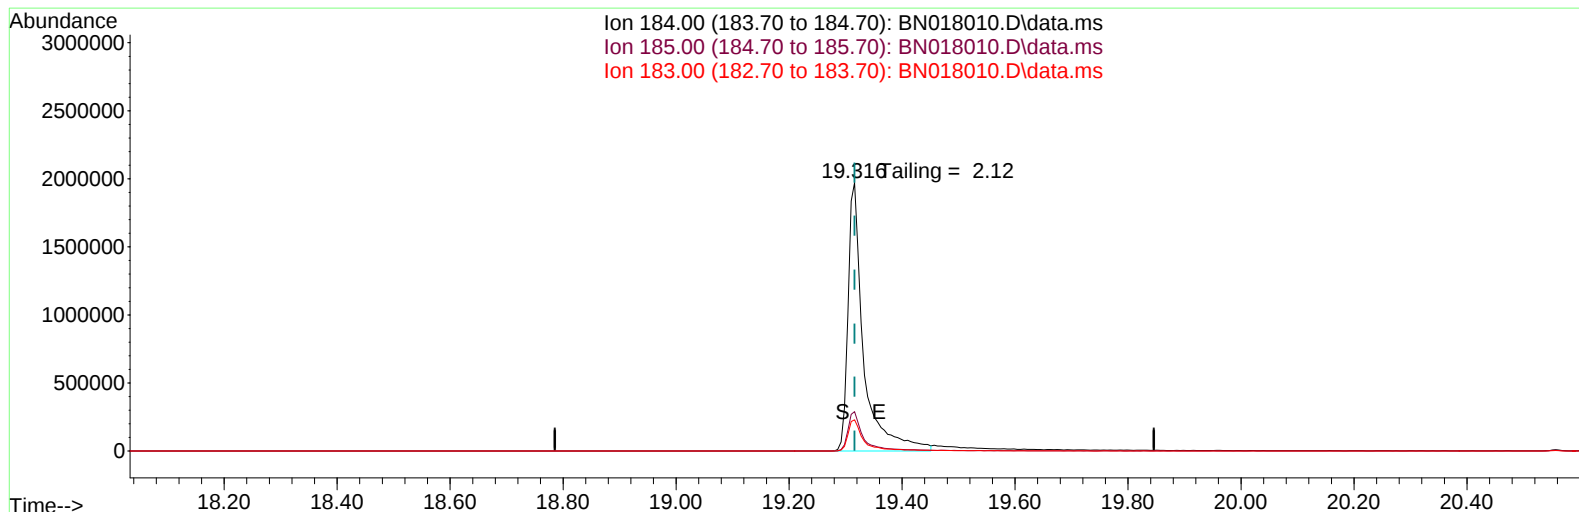

TIC: BN018010.D\data.ms

(77) Benzidine

19.316min (0.000) 1067300.47 ng

response **3980892**

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	15.50	14.68
183.00	13.20	11.63
0.00	0.00	0.00