

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN121421\
 Data File : BN017989.D
 Acq On : 14 Dec 2021 04:24
 Operator : CG/JU
 Sample : M4956-03DL 5X
 Misc :
 ALS Vial : 16 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 RE134D3-20211202DL

Quant Time: Dec 14 05:00:31 2021
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\8270-SIM-BN121421.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Tue Dec 14 01:08:04 2021
 Response via : Initial Calibration

Manual Integrations
 APPROVED

Reviewed By :Christian Giraldo 12/15/2021
 Supervised By :Jagrut Upadhyay 12/15/2021

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.689	152	33028	0.400	ng	0.00
7) Naphthalene-d8	10.470	136	119696	0.400	ng	0.00
13) Acenaphthene-d10	14.320	164	81263	0.400	ng	0.00
19) Phenanthrene-d10	17.078	188	153423	0.400	ng	0.01
29) Chrysene-d12	21.270	240	172198	0.400	ng	0.00
35) Perylene-d12	23.550	264	174025	0.400	ng	0.00
System Monitoring Compounds						
4) 2-Fluorophenol	5.300	112	1570	0.022	ng	0.00
5) Phenol-d6	6.877	99	673	0.009	ng	0.00
8) Nitrobenzene-d5	8.848	82	3496	0.041	ng	0.01
11) 2-Methylnaphthalene-d10	12.096	152	6625	0.033	ng	0.03
14) 2,4,6-Tribromophenol	15.842	330	1346m	0.215	ng	0.03
15) 2-Fluorobiphenyl	12.975	172	10111m	0.036	ng	0.03
27) Fluoranthene-d10	19.113	212	35159	0.069	ng	0.00
31) Terphenyl-d14	19.718	244	33836	0.094	ng	0.00
Target Compounds						
2) 1,4-Dioxane	3.235	88	25459m	1.237	ng	Qvalue
34) Bis(2-ethylhexyl)phtha...	21.196	149	7816	0.031	ng	# 99

(#) = qualifier out of range (m) = manual integration (+) = signals summed


Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN121421\
Data File : BN017989.D
Acq On : 14 Dec 2021 04:24
Operator : CG/JU
Sample : M4956-03DL 5X
Misc :
ALS Vial : 16 Sample Multiplier: 1


Instrument :
BNA_N
ClientSampleId :
RE134D3-20211202DL

Quant Time: Dec 14 05:00:31 2021
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\8270-SIM-BN121421.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Dec 14 01:08:04 2021
Response via : Initial Calibration

Manual Integrations
APPROVED


Reviewed By :Christian Giraldo 12/15/2021
Supervised By :Jagrut Upadhyay 12/15/2021

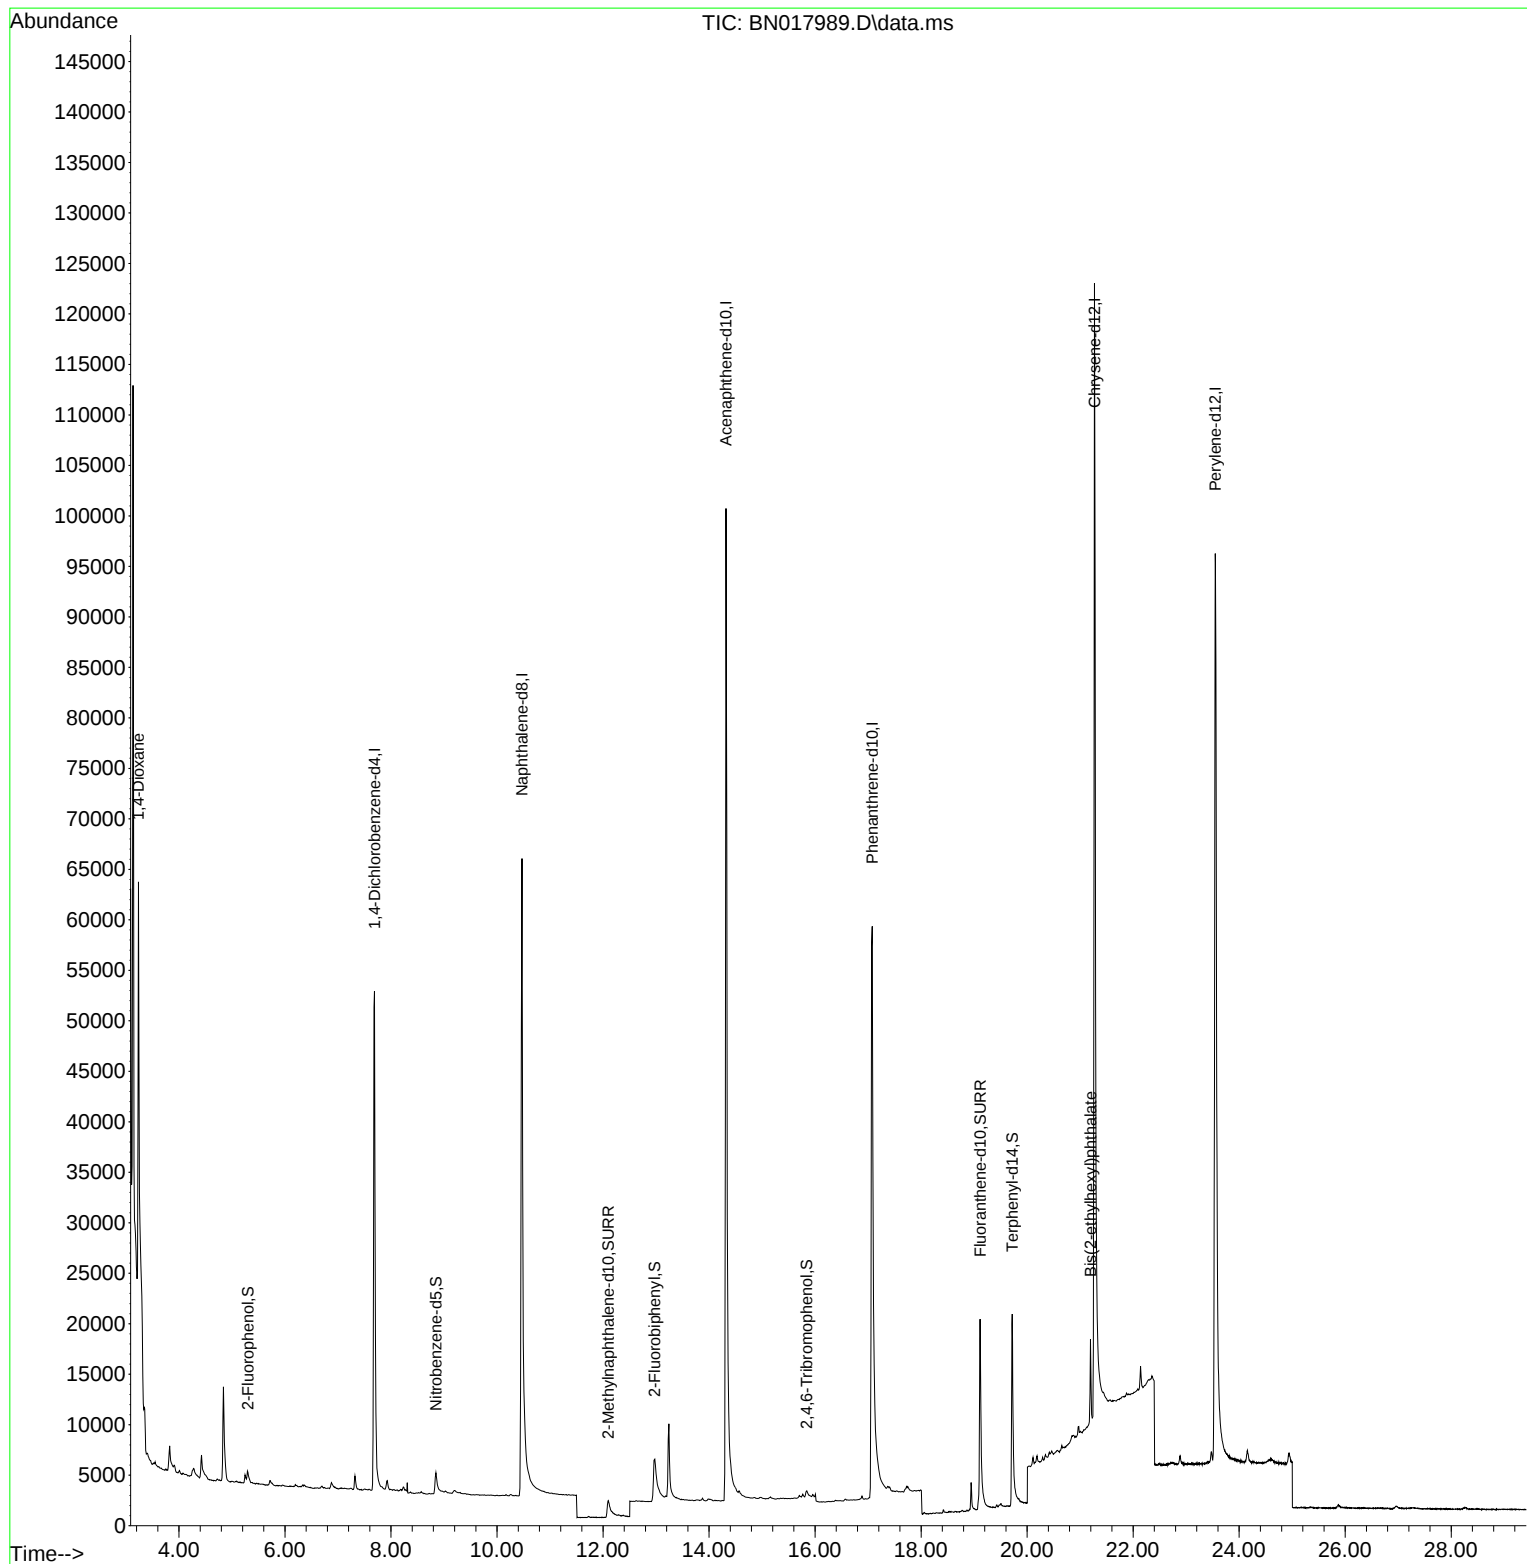

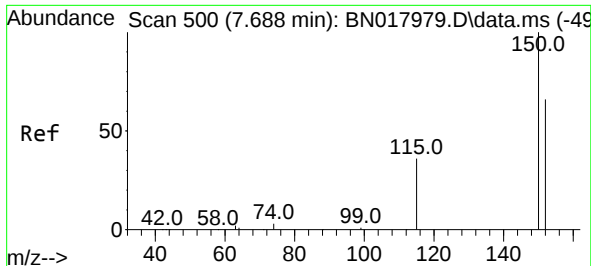

#1
 1,4-Dichlorobenzene-d4
 Concen: 0.400 ng
 RT: 7.689 min Scan# 500
 Delta R.T. 0.001 min
 Lab File: BN017989.D
 Acq: 14 Dec 2021 04:24




Instrument :
 BNA_N
 ClientSampleId :
 RE134D3-20211202DL

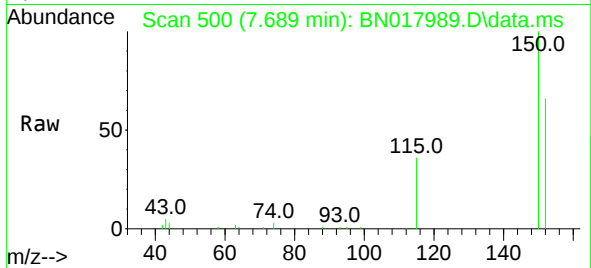


Tgt Ion: 152 Resp: 33028
 Ion Ratio Lower Upper
 152 100
 150 151.2 121.7 182.5
 115 53.8 43.8 65.8

Manual Integrations
 APPROVED



Reviewed By :Christian Giraldo 12/15/2021
 Supervised By :Jagrut Upadhyay 12/15/2021

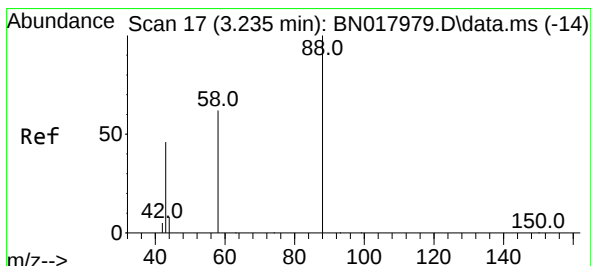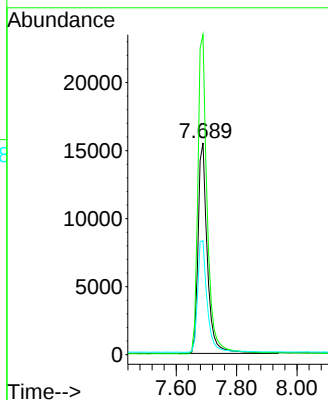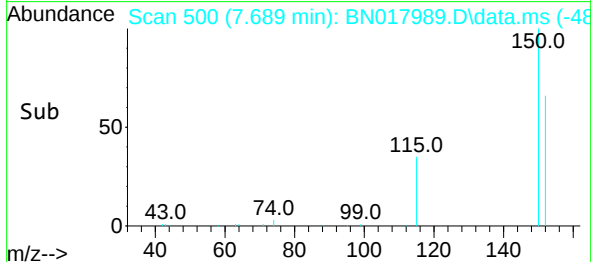


#2
 1,4-Dioxane
 Concen: 1.237 ng m
 RT: 3.235 min Scan# 17
 Delta R.T. 0.000 min
 Lab File: BN017989.D
 Acq: 14 Dec 2021 04:24

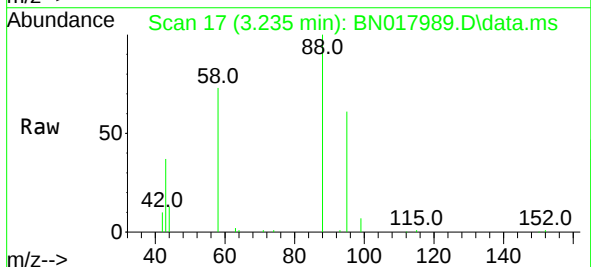


Tgt Ion: 88 Resp: 25459
 Ion Ratio Lower Upper
 88 100
 43 33.5 69.7 104.5#
 58 84.1 83.8 125.8

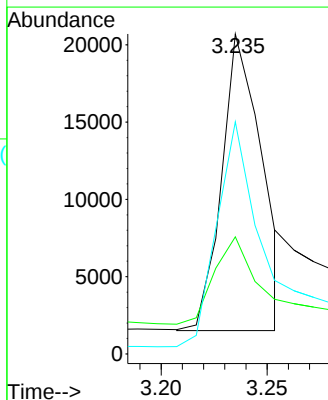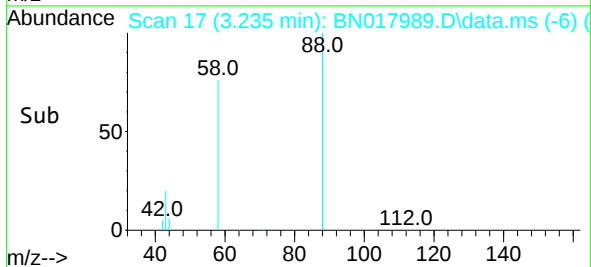

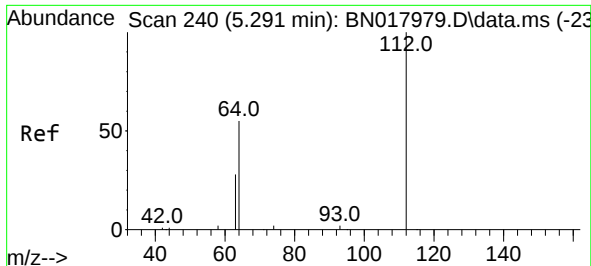

#4
2-Fluorophenol
Concen: 0.022 ng
RT: 5.300 min Scan# 241
Delta R.T. 0.010 min
Lab File: BN017989.D
Acq: 14 Dec 2021 04:24




Instrument :
BNA_N
ClientSampleId :
RE134D3-20211202DL

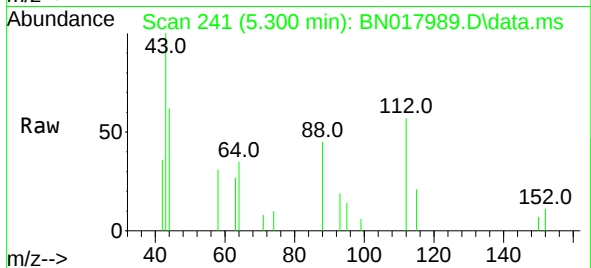


Tgt Ion: 112 Resp: 1570
Ion Ratio Lower Upper
112 100
64 61.5 48.0 72.0
63 31.0 25.3 37.9

Manual Integrations
APPROVED



Reviewed By :Christian Giraldo 12/15/2021
Supervised By :Jagrut Upadhyay 12/15/2021

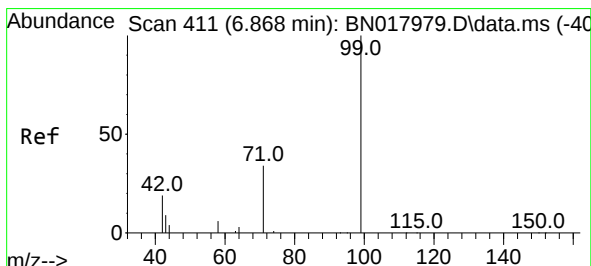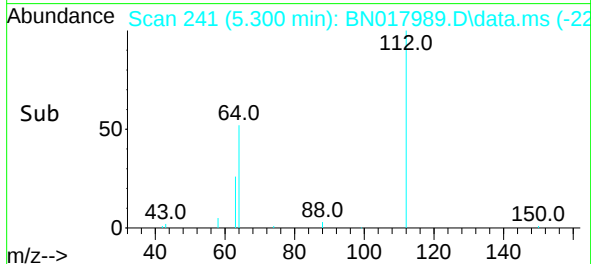


#5
Phenol-d6
Concen: 0.009 ng
RT: 6.877 min Scan# 412
Delta R.T. 0.010 min
Lab File: BN017989.D
Acq: 14 Dec 2021 04:24

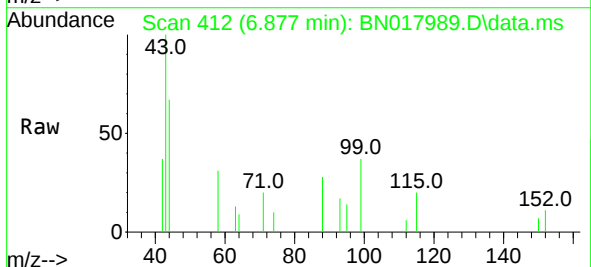


Tgt Ion: 99 Resp: 673
Ion Ratio Lower Upper
99 100
42 29.7 16.3 24.5#
71 47.0 26.8 40.2#

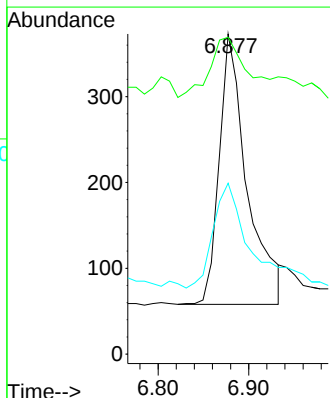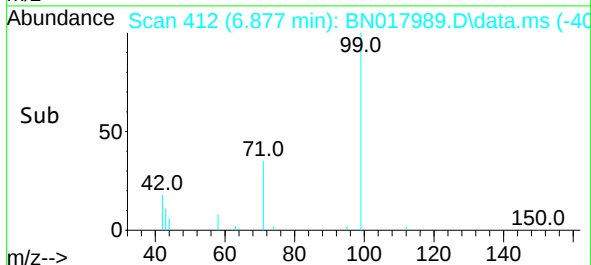

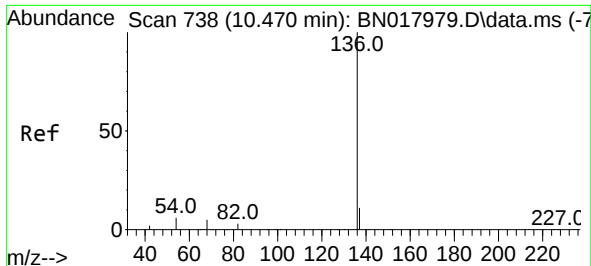

#7
Naphthalene-d8
Concen: 0.400 ng
RT: 10.470 min Scan# 71
Delta R.T. 0.000 min
Lab File: BN017989.D
Acq: 14 Dec 2021 04:24




Instrument :
BNA_N
ClientSampleId :
RE134D3-20211202DL

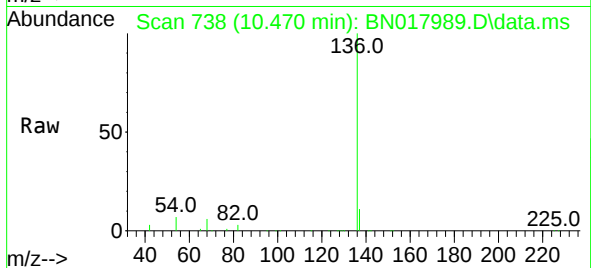

Tgt Ion: 136 Resp: 119690
Ion Ratio Lower Upper
136 100
137 11.1 8.8 13.2
54 6.7 5.0 7.6
68 5.7 4.4 6.6




Manual Integrations
APPROVED


Reviewed By :Christian Giraldo 12/15/2021
Supervised By :Jagrut Upadhyay 12/15/2021

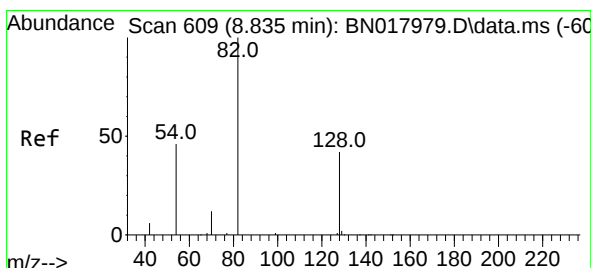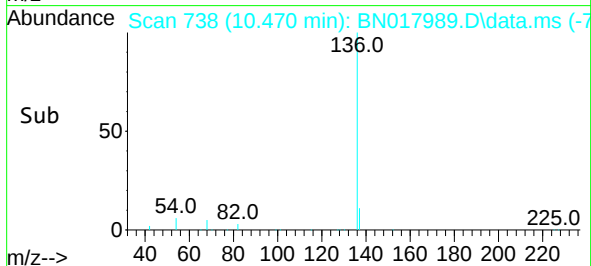

#8
Nitrobenzene-d5
Concen: 0.041 ng
RT: 8.848 min Scan# 610
Delta R.T. 0.013 min
Lab File: BN017989.D
Acq: 14 Dec 2021 04:24

Tgt Ion: 82 Resp: 3496
Ion Ratio Lower Upper
82 100
128 51.1 33.7 50.5#
54 53.5 36.6 55.0

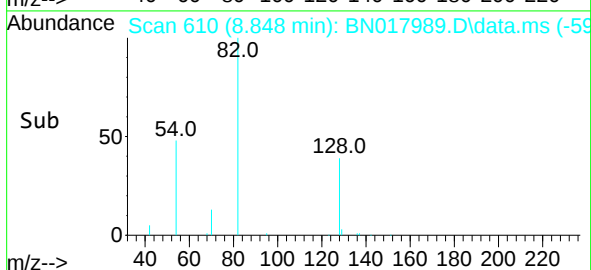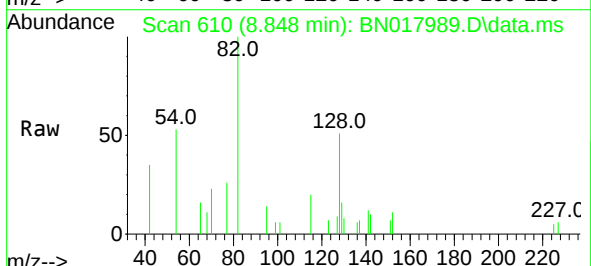

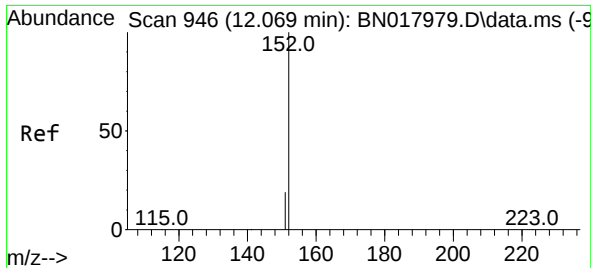

#11

2-Methylnaphthalene-d10

Concen: 0.033 ng

RT: 12.096 min Scan# 91

Delta R.T. 0.027 min

Lab File: BN017989.D

Acq: 14 Dec 2021 04:24

Instrument :

BNA_N

ClientSampleId :

RE134D3-20211202DL

Tgt Ion:152 Resp: 662

Ion Ratio Lower Upper

152 100





151 21.4 16.2 24.2

Manual Integrations

APPROVED

Reviewed By :Christian Giraldo 12/15/2021

Supervised By :Jagrut Upadhyay 12/15/2021

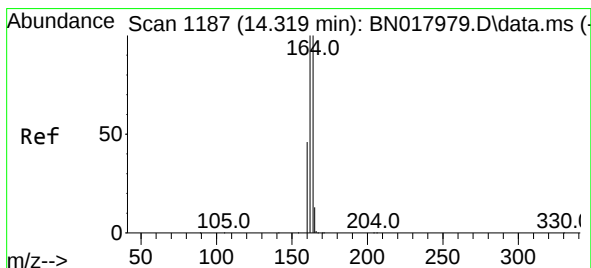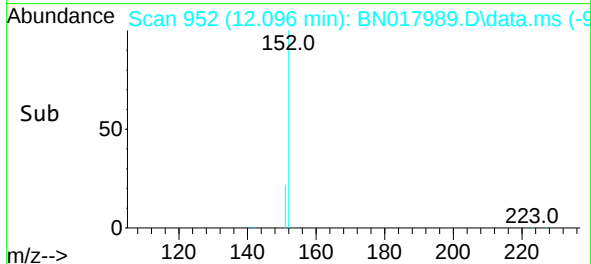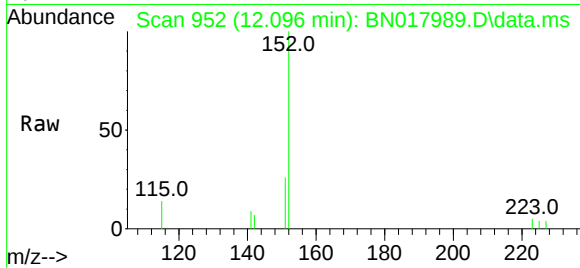

#13

Acenaphthene-d10

Concen: 0.400 ng

RT: 14.320 min Scan# 1187

Delta R.T. 0.000 min

Lab File: BN017989.D

Acq: 14 Dec 2021 04:24




Tgt Ion:164 Resp: 81263


Ion Ratio Lower Upper

164 100

162 100.6 80.2 120.2


160 46.7 36.9 55.3

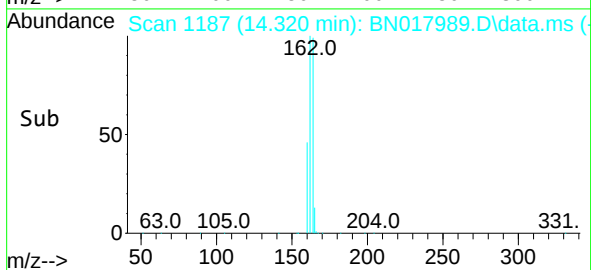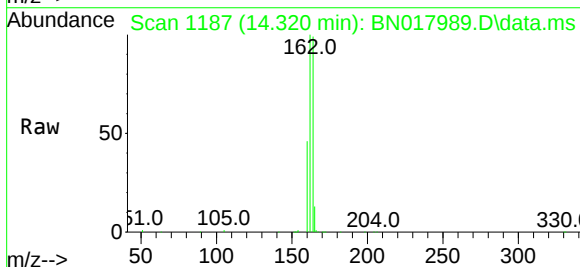

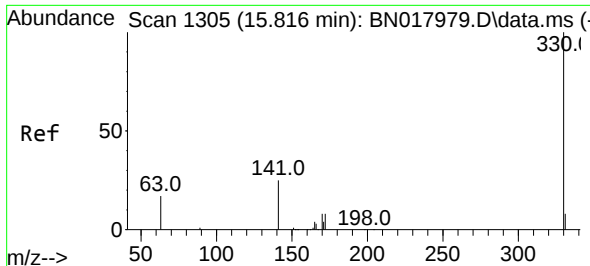

#14
2,4,6-Tribromophenol
Concen: 0.215 ng m
RT: 15.842 min Scan# 11
Delta R.T. 0.026 min
Lab File: BN017989.D
Acq: 14 Dec 2021 04:24




Instrument :
BNA_N
ClientSampleId :
RE134D3-20211202DL

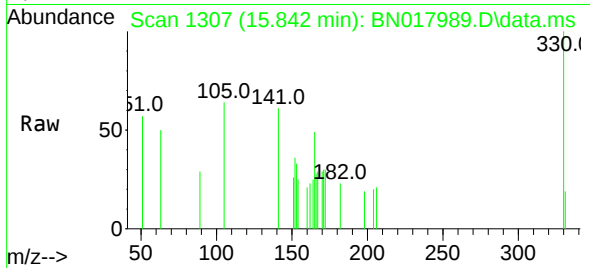


Tgt Ion:330 Resp: 1340
Ion Ratio Lower Upper
330 100
332 0.0 0.0 0.0
141 27.0 21.3 31.9

Manual Integrations
APPROVED



Reviewed By :Christian Giraldo 12/15/2021
Supervised By :Jagrut Upadhyay 12/15/2021

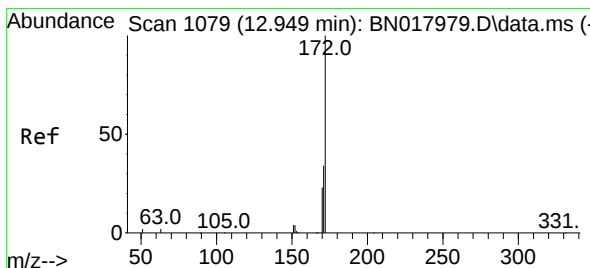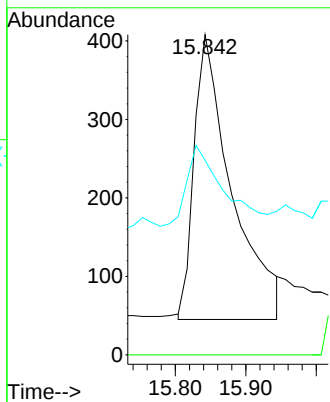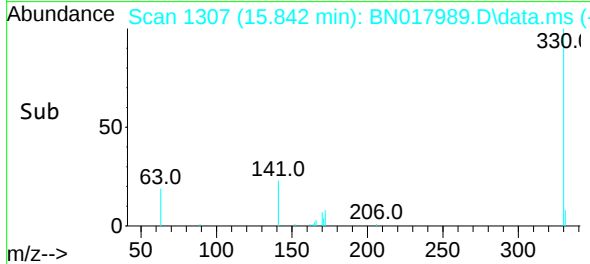


#15
2-Fluorobiphenyl
Concen: 0.036 ng m
RT: 12.975 min Scan# 1081
Delta R.T. 0.026 min
Lab File: BN017989.D
Acq: 14 Dec 2021 04:24

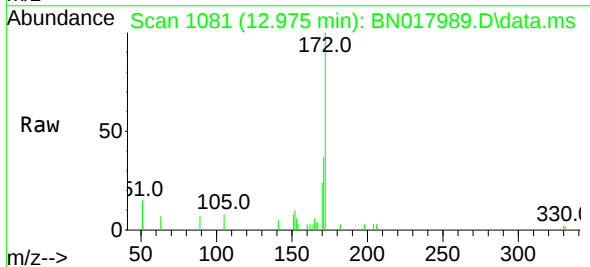


Tgt Ion:172 Resp: 10111
Ion Ratio Lower Upper
172 100
171 36.7 27.4 41.0
170 24.2 18.4 27.6

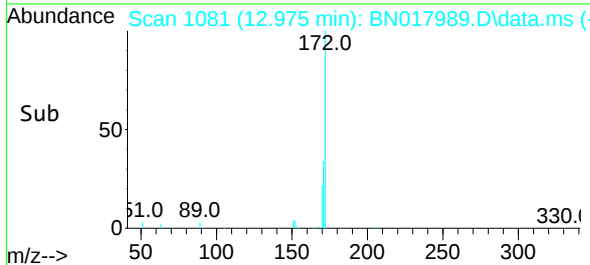

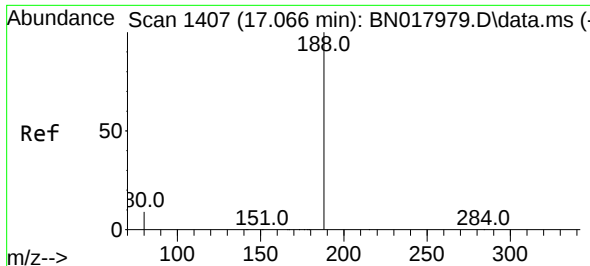

#19
Phenanthrene-d10
Concen: 0.400 ng
RT: 17.078 min Scan# 1408
Delta R.T. 0.012 min
Lab File: BN017989.D
Acq: 14 Dec 2021 04:24




Instrument :
BNA_N
ClientSampleId :
RE134D3-20211202DL

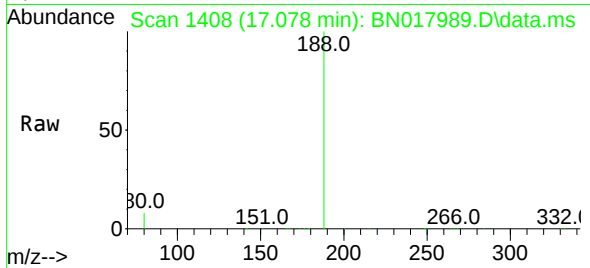

Tgt Ion:188 Resp: 15342
Ion Ratio Lower Upper
188 100
94 0.0 0.0 0.0
80 8.0 7.0 10.4




Manual Integrations
APPROVED


Reviewed By :Christian Giraldo 12/15/2021
Supervised By :Jagrut Upadhyay 12/15/2021

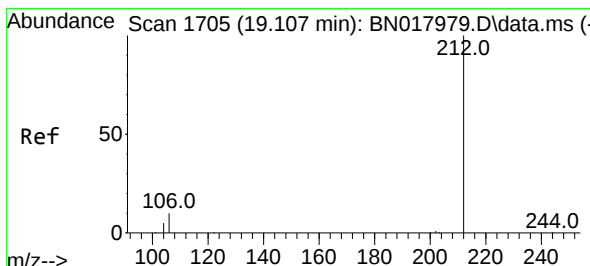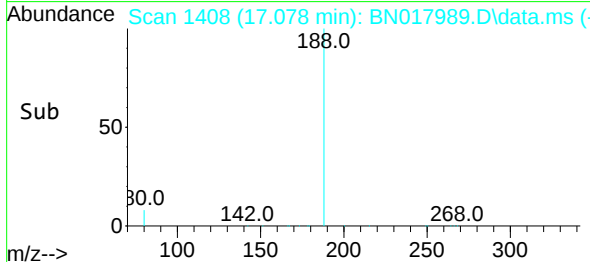

#27
Fluoranthene-d10
Concen: 0.069 ng
RT: 19.113 min Scan# 1706
Delta R.T. 0.005 min
Lab File: BN017989.D
Acq: 14 Dec 2021 04:24


Tgt Ion:212 Resp: 35159
Ion Ratio Lower Upper
212 100
106 10.5 8.4 12.6
104 5.7 4.5 6.7

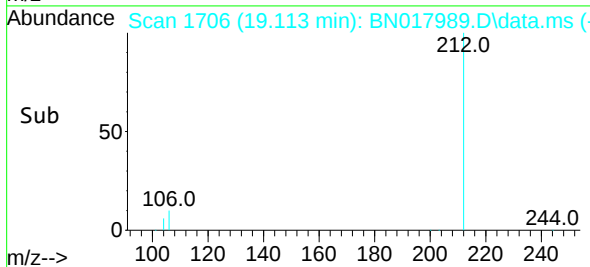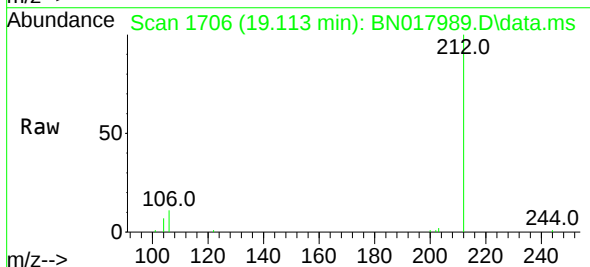

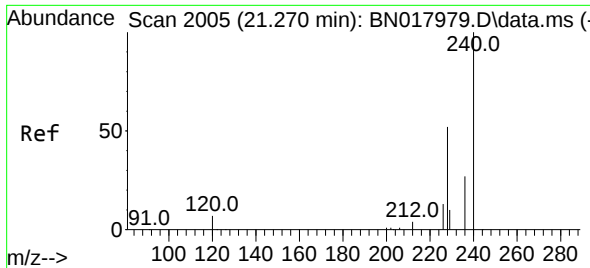

#29
Chrysene-d12
Concen: 0.400 ng
RT: 21.270 min Scan# 2005
Delta R.T. 0.000 min
Lab File: BN017989.D
Acq: 14 Dec 2021 04:24




Instrument :
BNA_N
ClientSampleId :
RE134D3-20211202DL

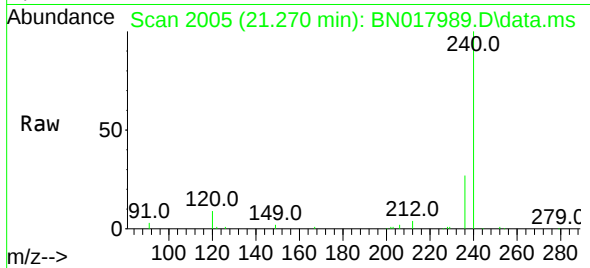


Tgt Ion:240 Resp: 172198
Ion Ratio Lower Upper
240 100
120 8.8 6.0 9.0
236 26.9 21.4 32.2

Manual Integrations
APPROVED



Reviewed By :Christian Giraldo 12/15/2021
Supervised By :Jagrut Upadhyay 12/15/2021

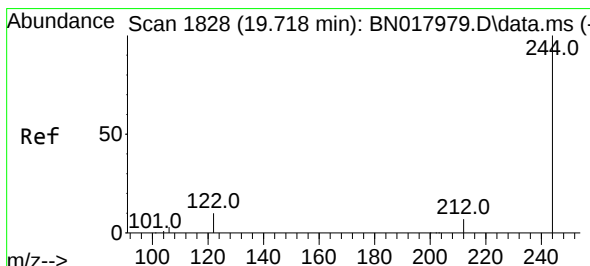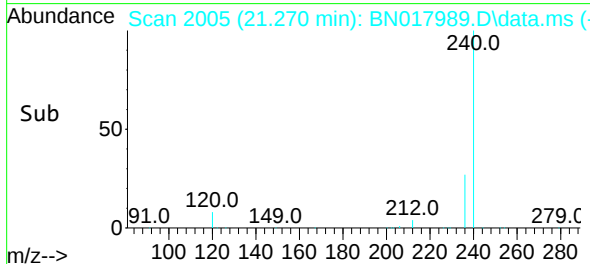


#31
Terphenyl-d14
Concen: 0.094 ng
RT: 19.718 min Scan# 1828
Delta R.T. 0.000 min
Lab File: BN017989.D
Acq: 14 Dec 2021 04:24

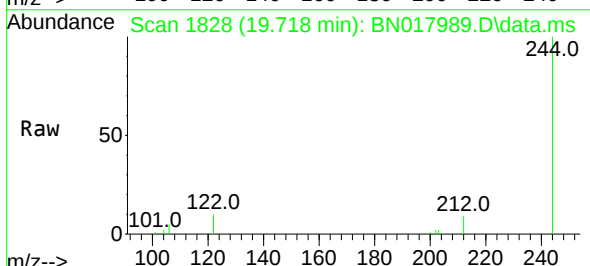


Tgt Ion:244 Resp: 33836
Ion Ratio Lower Upper
244 100
212 8.7 6.2 9.2
122 10.4 7.9 11.9

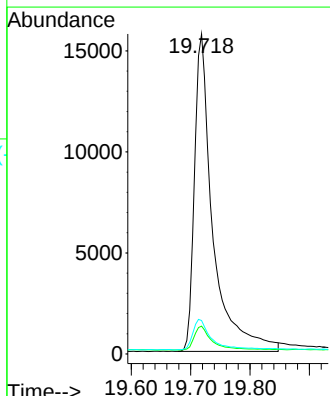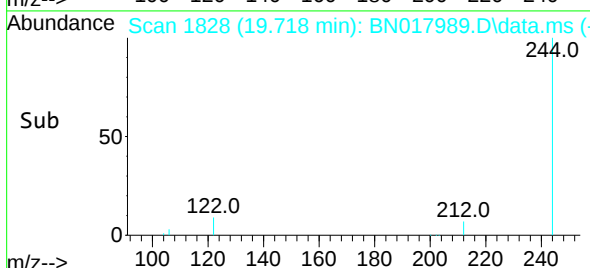

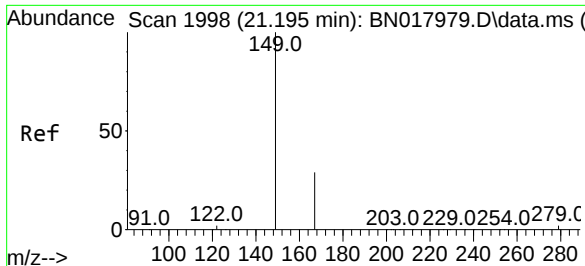

#34
Bis(2-ethylhexyl)phthalate
Concen: 0.031 ng
RT: 21.196 min Scan# 1998
Delta R.T. 0.000 min
Lab File: BN017989.D
Acq: 14 Dec 2021 04:24




Instrument :
BNA_N
ClientSampleId :
RE134D3-20211202DL

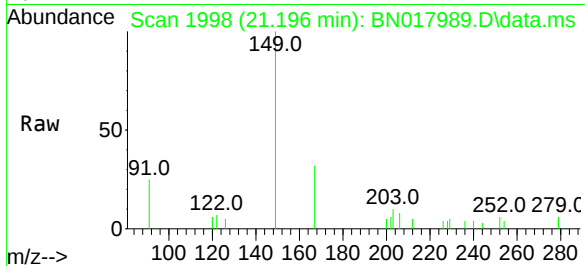

Tgt Ion:149 Resp: 7810
Ion Ratio Lower Upper
149 100
167 29.2 23.7 35.5
279 6.5 3.6 5.4

Manual Integrations
APPROVED

Reviewed By :Christian Giraldo 12/15/2021
Supervised By :Jagrut Upadhyay 12/15/2021

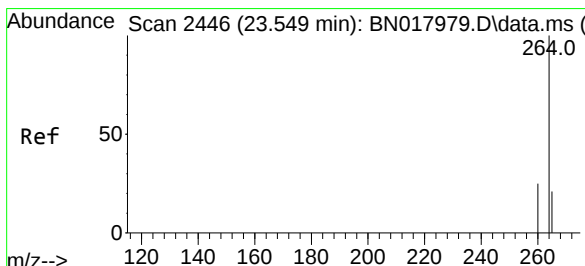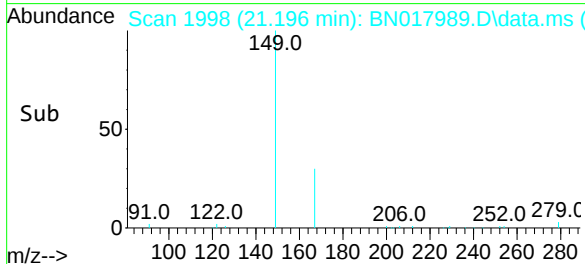

#35
Perylene-d12
Concen: 0.400 ng
RT: 23.550 min Scan# 2446
Delta R.T. 0.000 min
Lab File: BN017989.D
Acq: 14 Dec 2021 04:24

Tgt Ion:264 Resp: 174025
Ion Ratio Lower Upper
264 100
260 25.4 20.2 30.4
265 25.9 18.2 27.2

