

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN121421\
 Data File : BN017990.D
 Acq On : 14 Dec 2021 05:00
 Operator : CG/JU
 Sample : M4988-01DL 5X
 Misc :
 ALS Vial : 17 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 RE125D2-20211206DL

Manual Integrations
 APPROVED

Reviewed By : Christian Giraldo 12/15/2021
 Supervised By : Jagrut Upadhyay 12/15/2021

Quant Time: Dec 14 07:26:54 2021
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\8270-SIM-BN121421.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Tue Dec 14 01:08:04 2021
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.688	152	34583	0.400	ng	0.00
7) Naphthalene-d8	10.470	136	126621	0.400	ng	0.00
13) Acenaphthene-d10	14.319	164	86562	0.400	ng	0.00
19) Phenanthrene-d10	17.066	188	177931	0.400	ng	0.00
29) Chrysene-d12	21.270	240	189193	0.400	ng	0.00
35) Perylene-d12	23.546	264	193800	0.400	ng	0.00
System Monitoring Compounds						
4) 2-Fluorophenol	5.300	112	1398	0.019	ng	0.00
5) Phenol-d6	6.877	99	646	0.009	ng	0.00
8) Nitrobenzene-d5	8.835	82	3696	0.041	ng	0.00
11) 2-Methylnaphthalene-d10	12.087	152	6936	0.033	ng	0.02
14) 2,4,6-Tribromophenol	15.829	330	1078	0.208	ng	0.01
15) 2-Fluorobiphenyl	12.962	172	10015	0.033	ng	0.01
27) Fluoranthene-d10	19.108	212	34251	0.058	ng	0.00
31) Terphenyl-d14	19.713	244	29780	0.076	ng	0.00
Target Compounds						Qvalue
2) 1,4-Dioxane	3.235	88	30992m	1.438	ng	
34) Bis(2-ethylhexyl)phtha...	21.196	149	331712	1.187	ng	100

(#) = qualifier out of range (m) = manual integration (+) = signals summed


Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN121421\
Data File : BN017990.D
Acq On : 14 Dec 2021 05:00
Operator : CG/JU
Sample : M4988-01DL 5X
Misc :
ALS Vial : 17 Sample Multiplier: 1


Instrument :
BNA_N
ClientSampleId :
RE125D2-20211206DL

Quant Time: Dec 14 07:26:54 2021
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\8270-SIM-BN121421.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Dec 14 01:08:04 2021
Response via : Initial Calibration

Manual Integrations
APPROVED


Reviewed By : Christian Giraldo 12/15/2021
Supervised By : Jagrut Upadhyay 12/15/2021

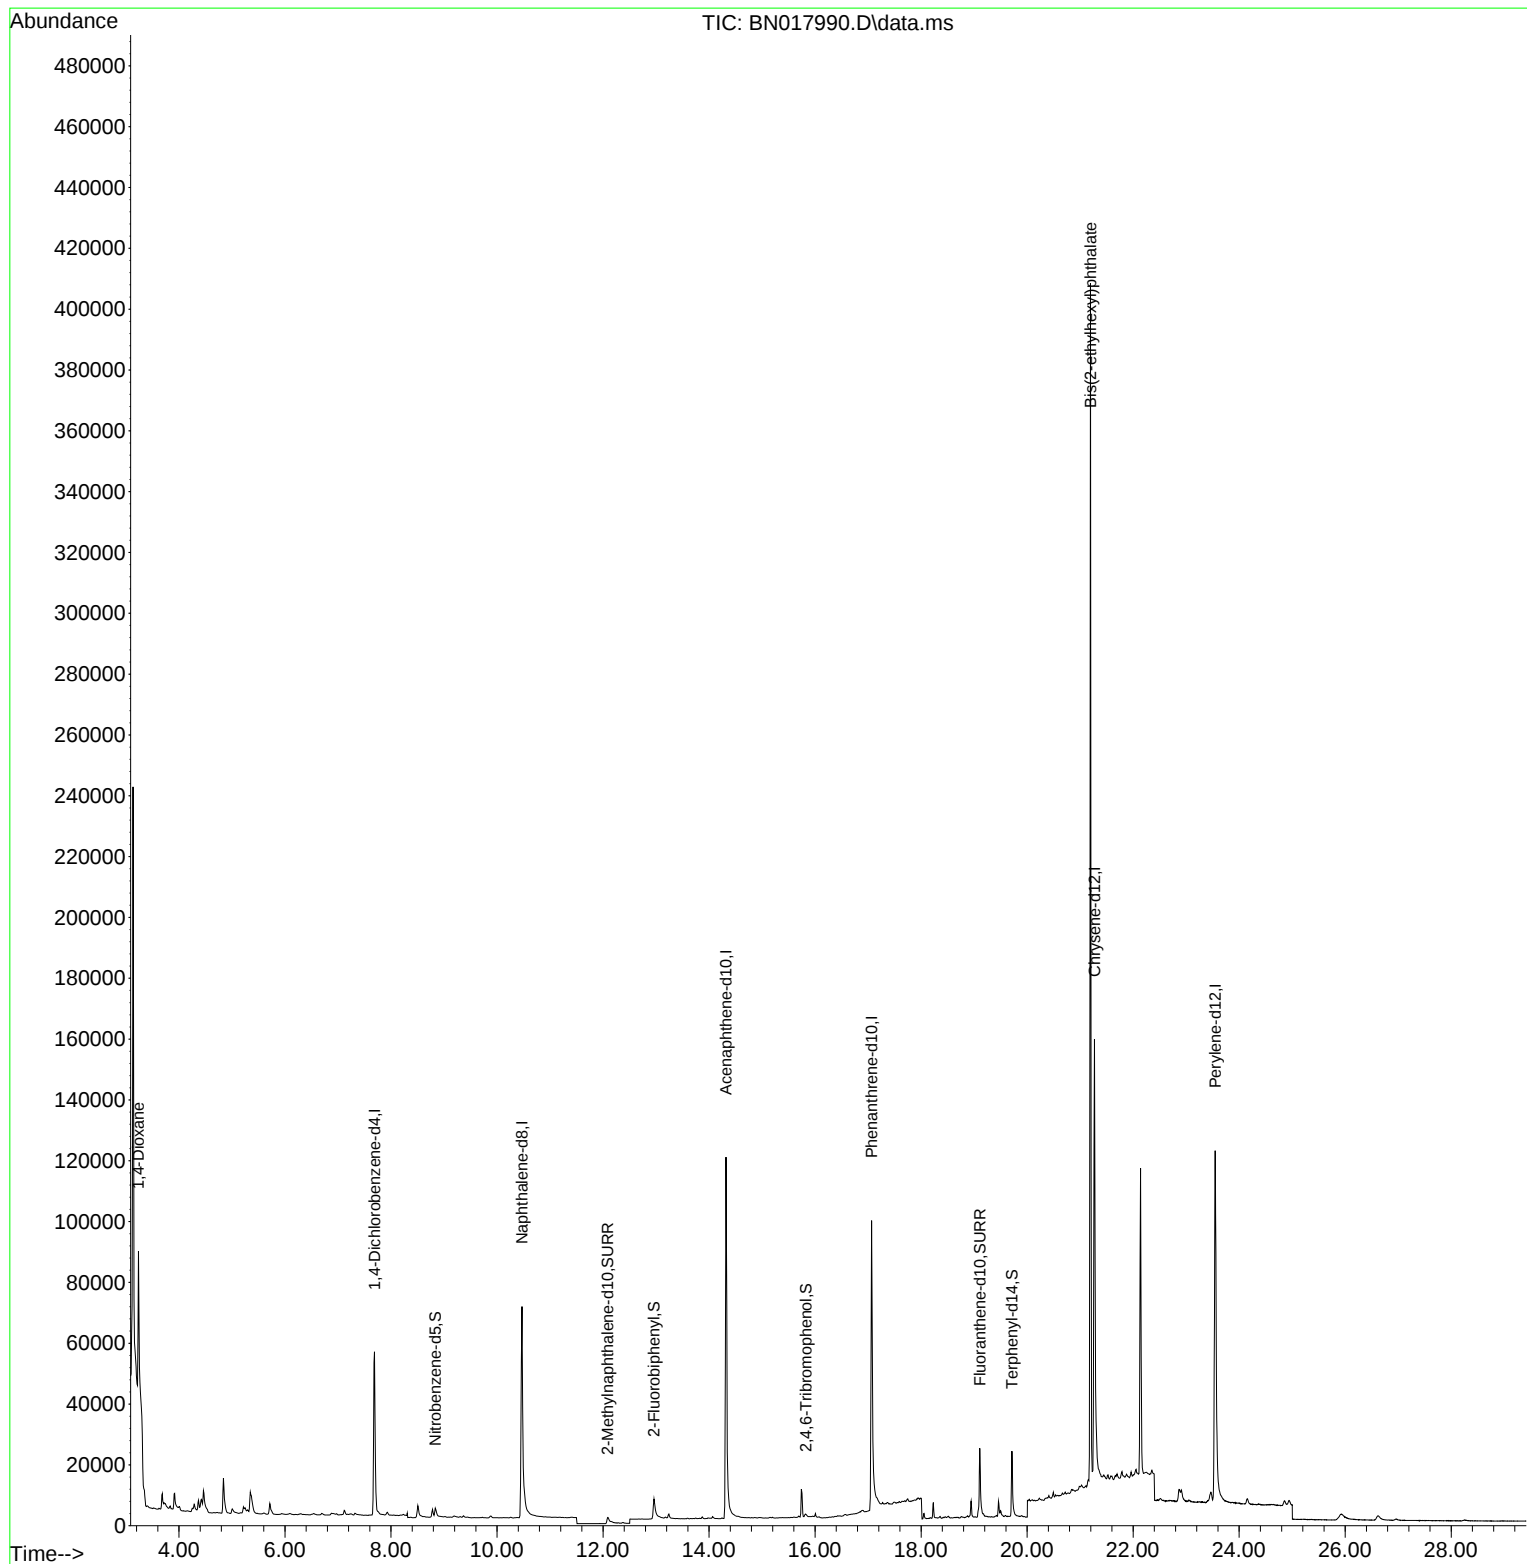

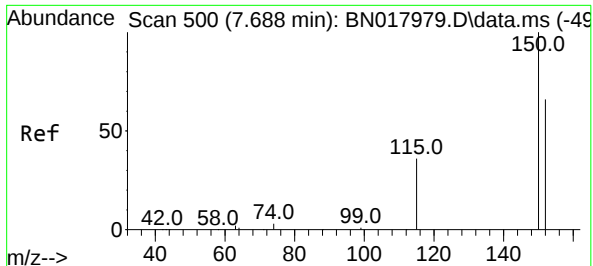

#1
 1,4-Dichlorobenzene-d4
 Concen: 0.400 ng
 RT: 7.688 min Scan# 50
 Delta R.T. 0.000 min
 Lab File: BN017990.D
 Acq: 14 Dec 2021 05:00




Instrument :
 BNA_N
 ClientSampleId :
 RE125D2-20211206DL

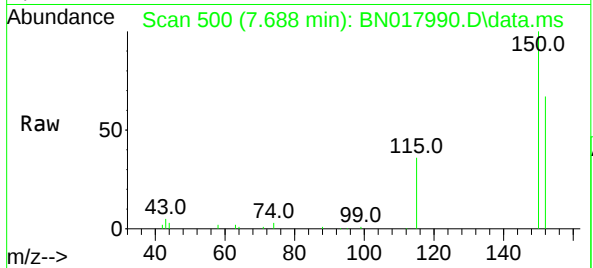


Tgt Ion: 152 Resp: 3458
 Ion Ratio Lower Upper
 152 100
 150 149.8 121.7 182.5
 115 53.7 43.8 65.8

Manual Integrations
 APPROVED



Reviewed By : Christian Giraldo 12/15/2021
 Supervised By : Jagrut Upadhyay 12/15/2021

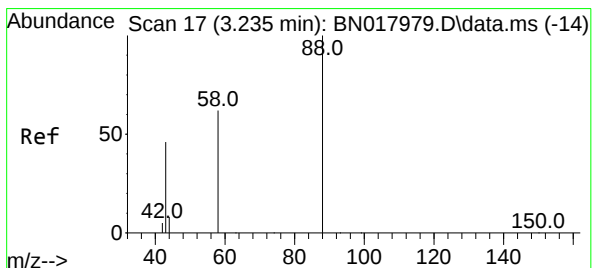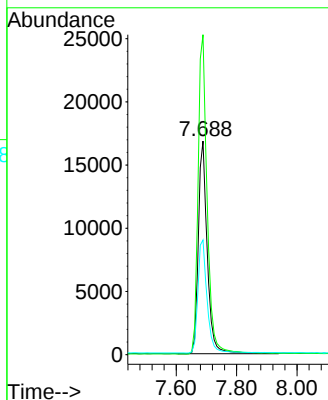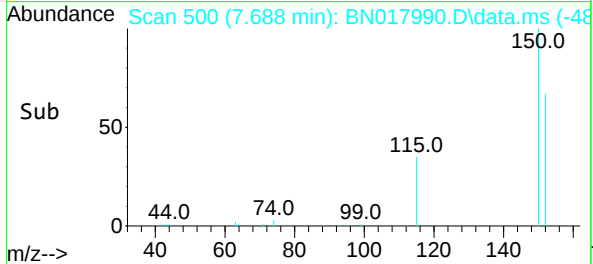


#2
 1,4-Dioxane
 Concen: 1.438 ng m
 RT: 3.235 min Scan# 17
 Delta R.T. 0.000 min
 Lab File: BN017990.D
 Acq: 14 Dec 2021 05:00

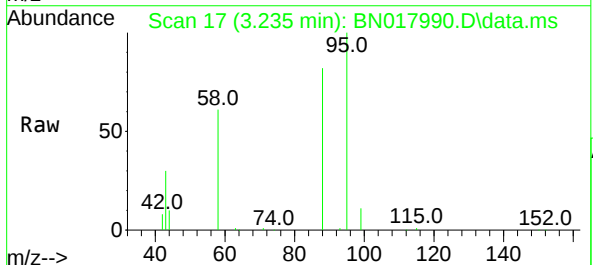


Tgt Ion: 88 Resp: 30992
 Ion Ratio Lower Upper
 88 100
 43 33.2 69.7 104.5#
 58 83.0 83.8 125.8#

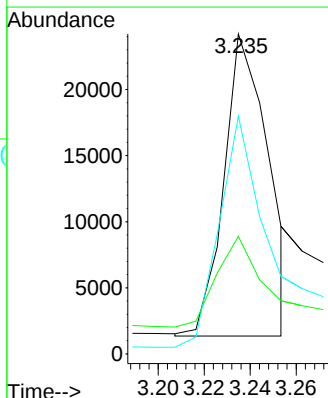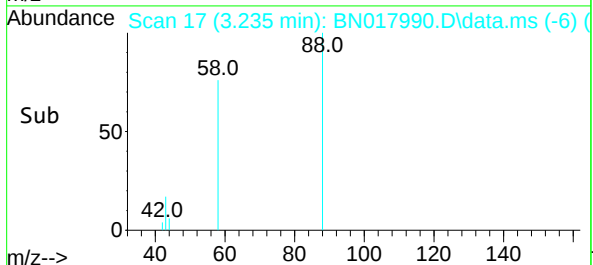

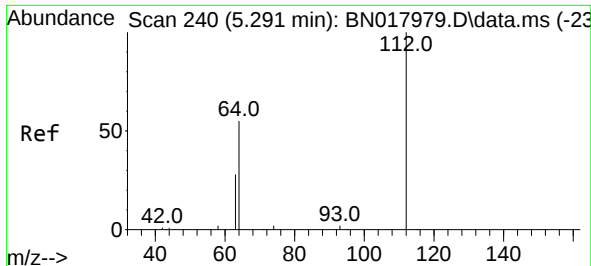

#4
2-Fluorophenol
Concen: 0.019 ng
RT: 5.300 min Scan# 241
Delta R.T. 0.009 min
Lab File: BN017990.D
Acq: 14 Dec 2021 05:00




Instrument :
BNA_N
ClientSampleId :
RE125D2-20211206DL

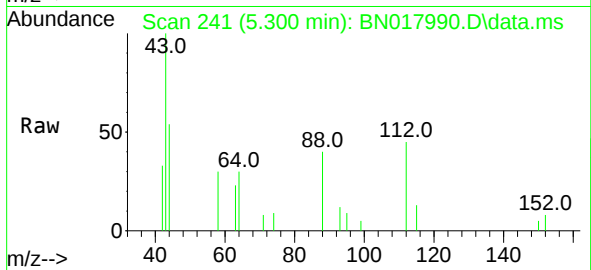

Tgt Ion: 112 Resp: 1398
Ion Ratio Lower Upper
112 100
64 34.0 48.0 72.0#
63 0.0 25.3 37.9#




Manual Integrations
APPROVED


Reviewed By :Christian Giraldo 12/15/2021
Supervised By :Jagrut Upadhyay 12/15/2021

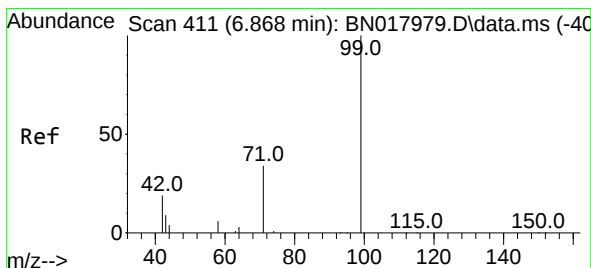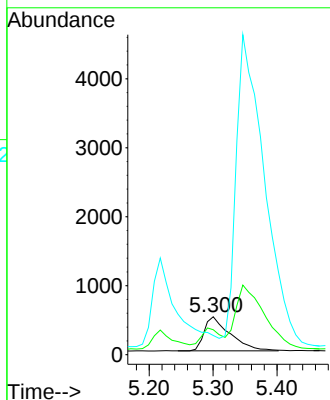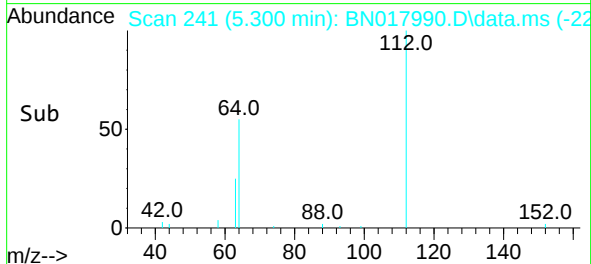

#5
Phenol-d6
Concen: 0.009 ng
RT: 6.877 min Scan# 412
Delta R.T. 0.009 min
Lab File: BN017990.D
Acq: 14 Dec 2021 05:00


Tgt Ion: 99 Resp: 646
Ion Ratio Lower Upper
99 100
42 31.6 16.3 24.5#
71 51.4 26.8 40.2#

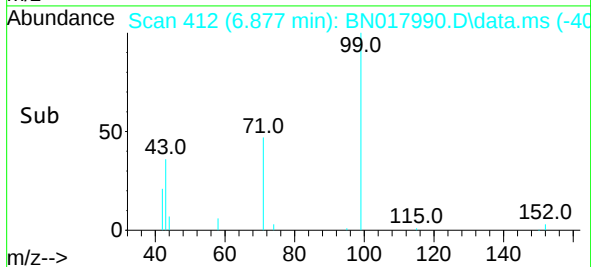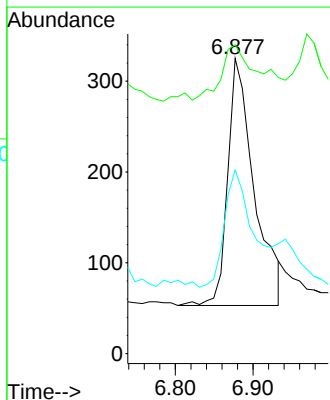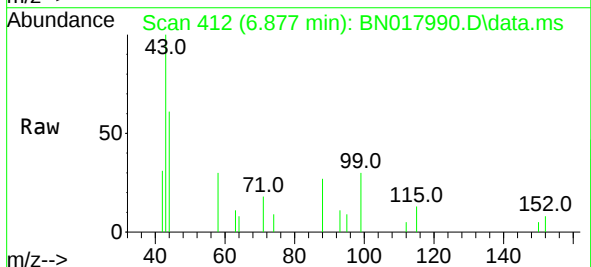

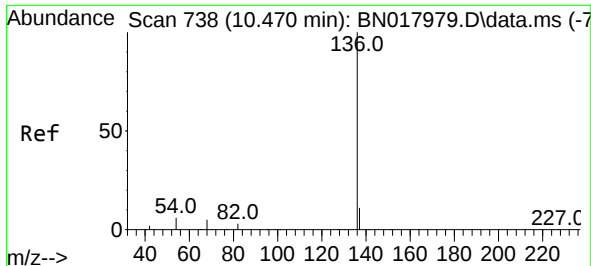

#7
Naphthalene-d8
Concen: 0.400 ng
RT: 10.470 min Scan# 738
Delta R.T. 0.000 min
Lab File: BN017990.D
Acq: 14 Dec 2021 05:00




Instrument :
BNA_N
ClientSampleId :
RE125D2-20211206DL

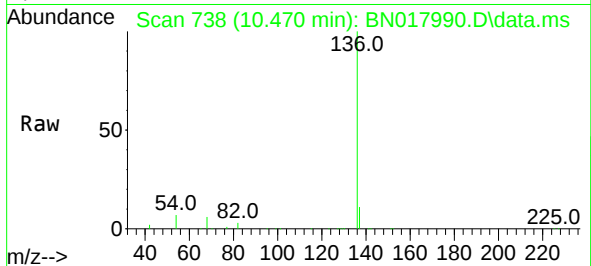

Tgt Ion:136 Resp: 12662
Ion Ratio Lower Upper
136 100
137 11.0 8.8 13.2
54 6.7 5.0 7.6
68 5.8 4.4 6.6




Manual Integrations
APPROVED


Reviewed By :Christian Giraldo 12/15/2021
Supervised By :Jagrut Upadhyay 12/15/2021

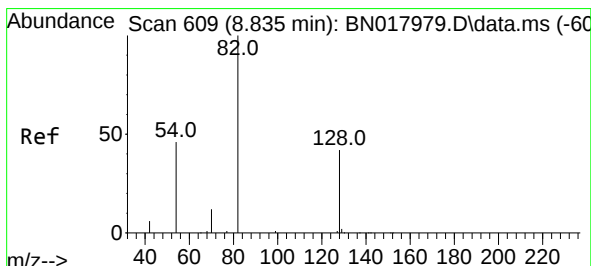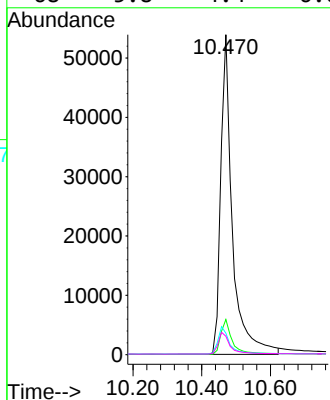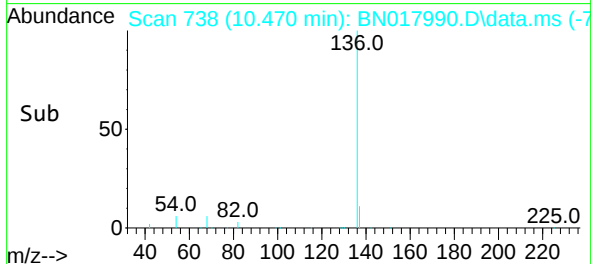

#8
Nitrobenzene-d5
Concen: 0.041 ng
RT: 8.835 min Scan# 609
Delta R.T. 0.000 min
Lab File: BN017990.D
Acq: 14 Dec 2021 05:00

Tgt Ion: 82 Resp: 3696
Ion Ratio Lower Upper
82 100
128 40.6 33.7 50.5
54 54.8 36.6 55.0

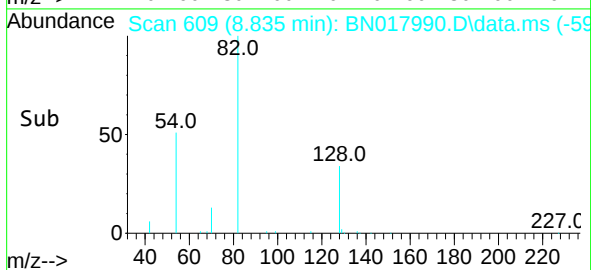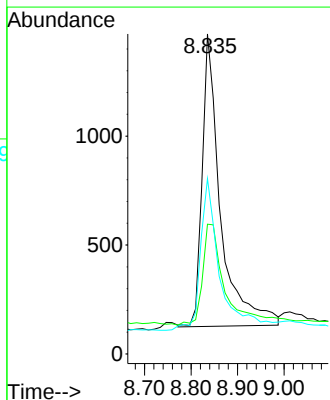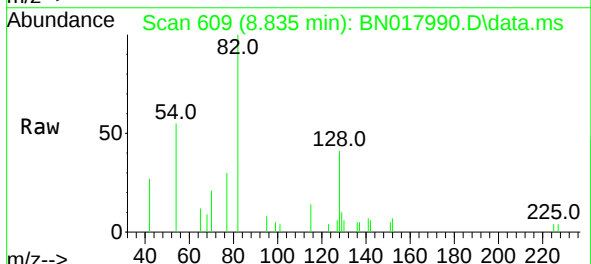

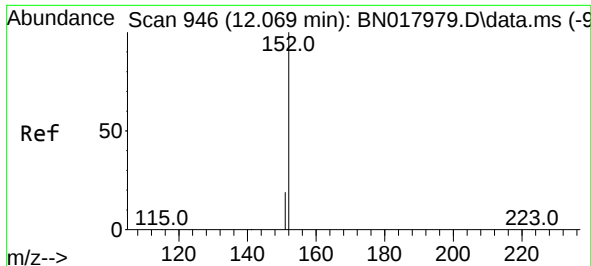

#11

2-Methylnaphthalene-d10

Concen: 0.033 ng

RT: 12.087 min Scan# 946

Delta R.T. 0.018 min

Lab File: BN017990.D

Acq: 14 Dec 2021 05:00

Instrument :

BNA_N

ClientSampleId :

RE125D2-20211206DL

Tgt Ion:152 Resp: 6930

Ion Ratio Lower Upper

152 100





151 18.7 16.2 24.2

Manual Integrations

APPROVED

Reviewed By :Christian Giraldo 12/15/2021

Supervised By :Jagrut Upadhyay 12/15/2021

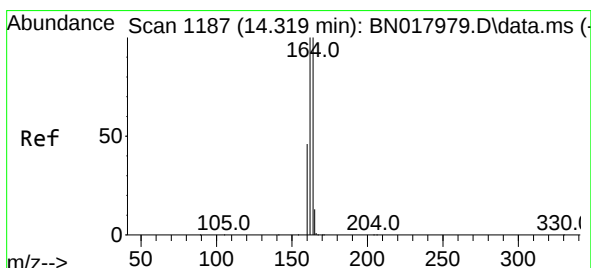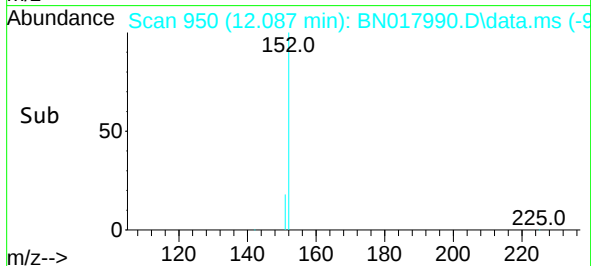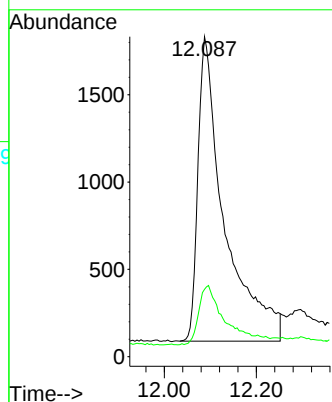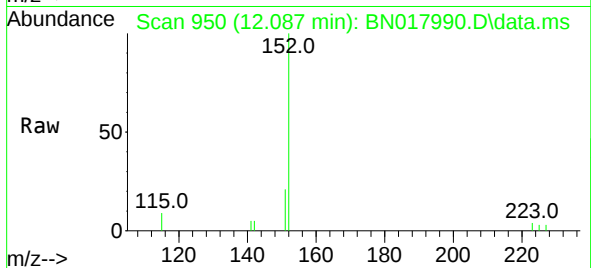

#13

Acenaphthene-d10

Concen: 0.400 ng

RT: 14.319 min Scan# 1187

Delta R.T. 0.000 min

Lab File: BN017990.D

Acq: 14 Dec 2021 05:00




Tgt Ion:164 Resp: 86562


Ion Ratio Lower Upper

164 100

162 99.8 80.2 120.2


160 46.2 36.9 55.3

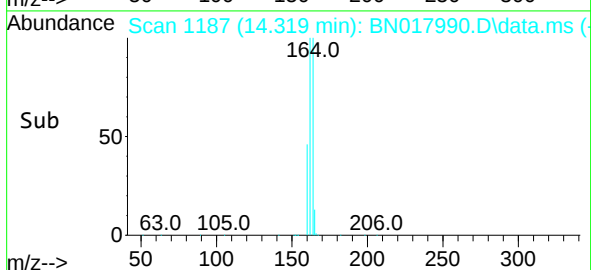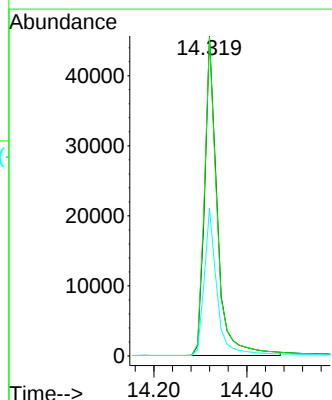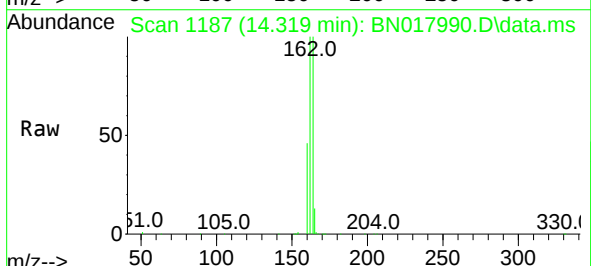

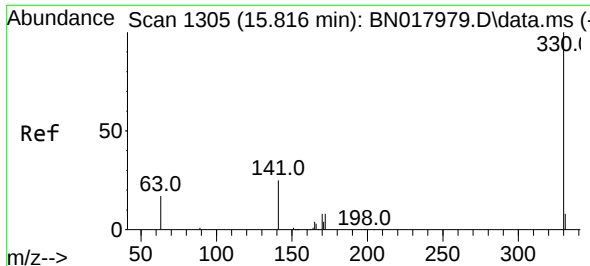

#14
2,4,6-Tribromophenol
Concen: 0.208 ng
RT: 15.829 min Scan# 11
Delta R.T. 0.013 min
Lab File: BN017990.D
Acq: 14 Dec 2021 05:00




Instrument :
BNA_N
ClientSampleId :
RE125D2-20211206DL

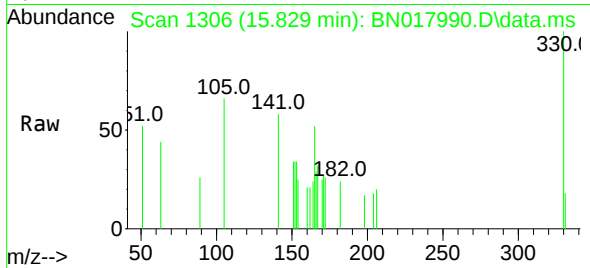

Tgt Ion:330 Resp: 1078
Ion Ratio Lower Upper
330 100
332 0.0 0.0 0.0
141 38.4 21.3 31.9




Manual Integrations
APPROVED


Reviewed By :Christian Giraldo 12/15/2021
Supervised By :Jagrut Upadhyay 12/15/2021

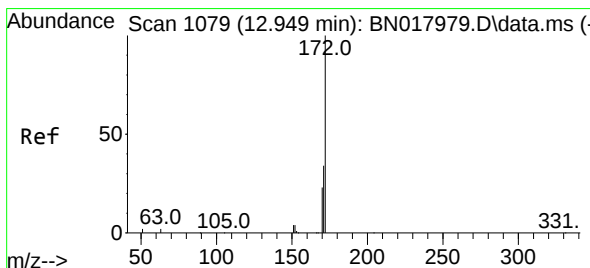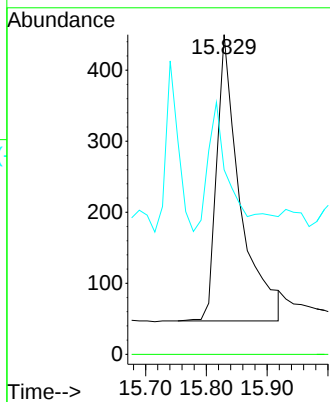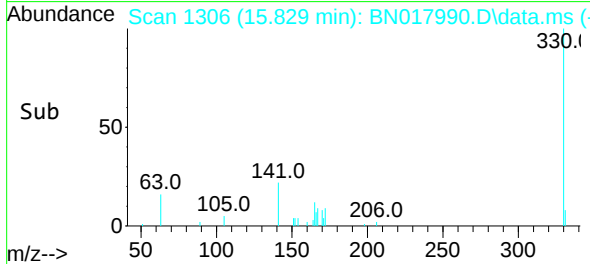

#15
2-Fluorobiphenyl
Concen: 0.033 ng
RT: 12.962 min Scan# 1080
Delta R.T. 0.013 min
Lab File: BN017990.D
Acq: 14 Dec 2021 05:00


Tgt Ion:172 Resp: 10015
Ion Ratio Lower Upper
172 100
171 35.8 27.4 41.0
170 24.4 18.4 27.6

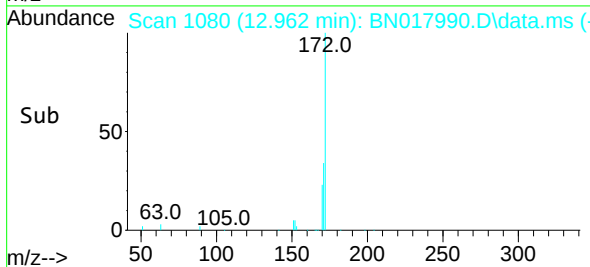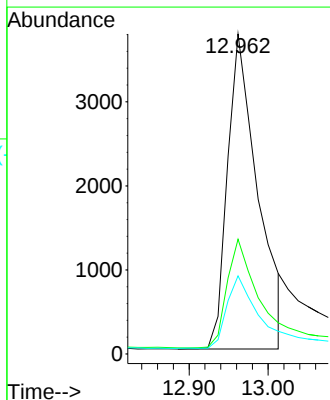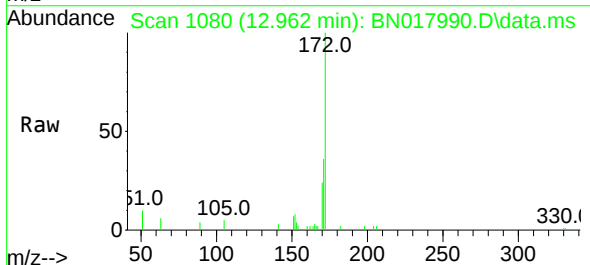

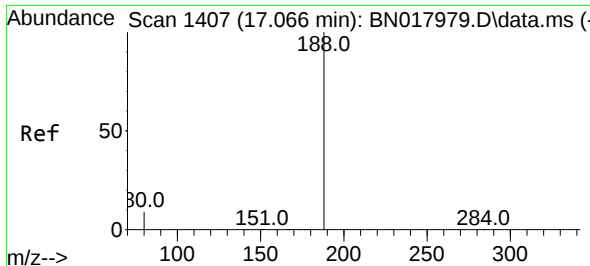

#19
Phenanthrene-d10
Concen: 0.400 ng
RT: 17.066 min Scan# 1407
Delta R.T. 0.000 min
Lab File: BN017990.D
Acq: 14 Dec 2021 05:00




Instrument :
BNA_N
ClientSampleId :
RE125D2-20211206DL

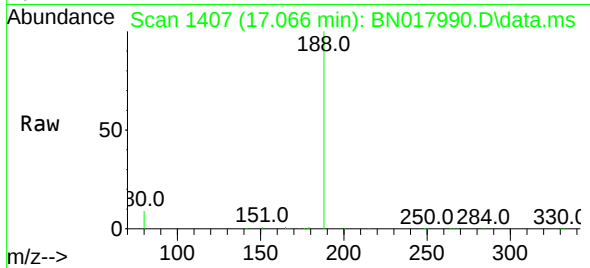


Tgt Ion:188 Resp: 17793
Ion Ratio Lower Upper
188 100
94 0.0 0.0 0.0
80 9.4 7.0 10.4

Manual Integrations
APPROVED



Reviewed By :Christian Giraldo 12/15/2021
Supervised By :Jagrut Upadhyay 12/15/2021

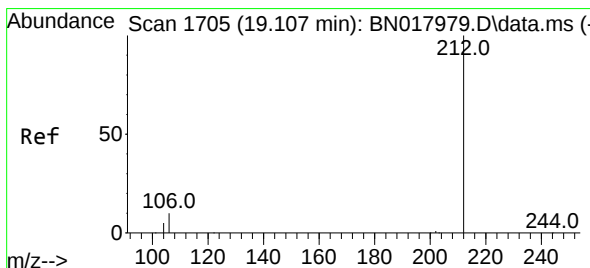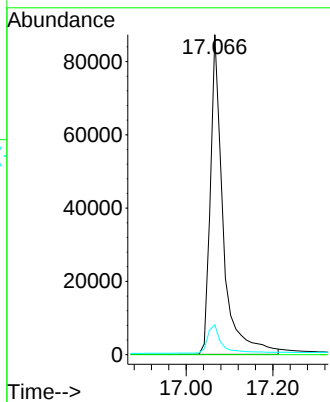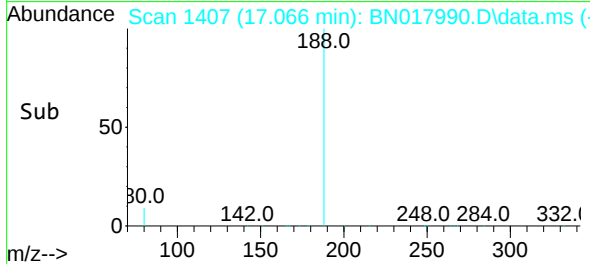


#27
Fluoranthene-d10
Concen: 0.058 ng
RT: 19.108 min Scan# 1705
Delta R.T. 0.000 min
Lab File: BN017990.D
Acq: 14 Dec 2021 05:00

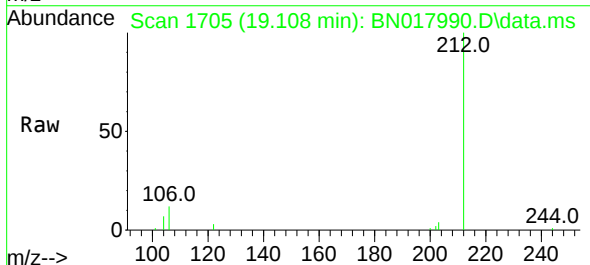


Tgt Ion:212 Resp: 34251
Ion Ratio Lower Upper
212 100
106 10.1 8.4 12.6
104 5.2 4.5 6.7

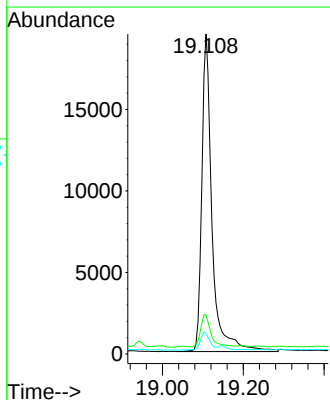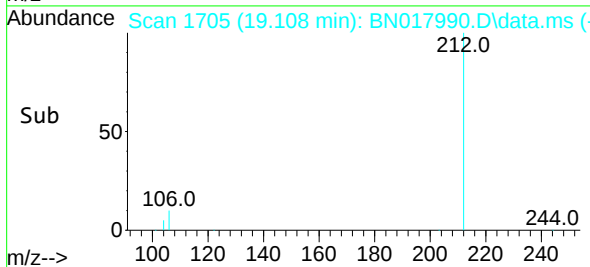

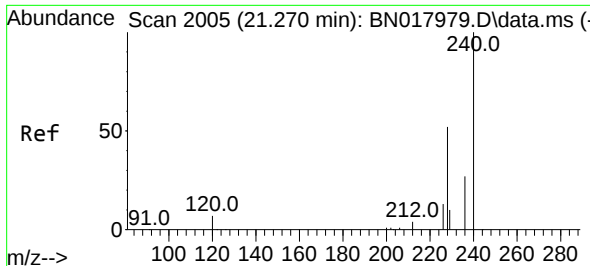

#29
Chrysene-d12
Concen: 0.400 ng
RT: 21.270 min Scan# 2005
Delta R.T. 0.000 min
Lab File: BN017990.D
Acq: 14 Dec 2021 05:00




Instrument :
BNA_N
ClientSampleId :
RE125D2-20211206DL

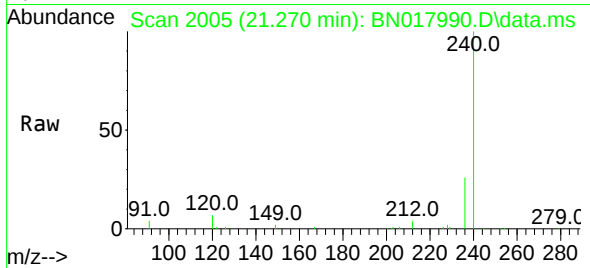

Tgt Ion:240 Resp: 18919
Ion Ratio Lower Upper
240 100
120 7.0 6.0 9.0
236 26.3 21.4 32.2




Manual Integrations
APPROVED


Reviewed By :Christian Giraldo 12/15/2021
Supervised By :Jagrut Upadhyay 12/15/2021

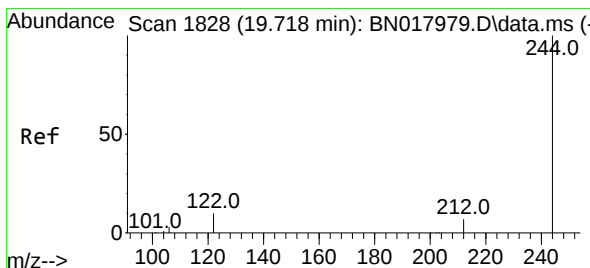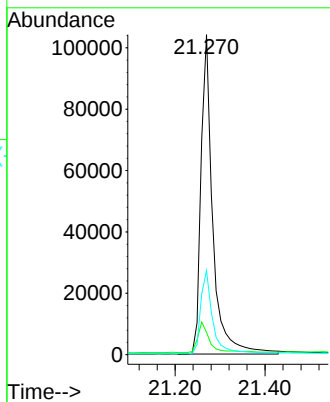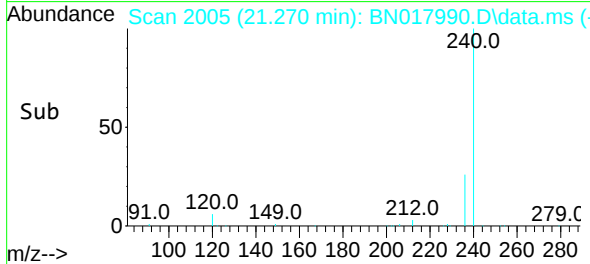

#31
Terphenyl-d14
Concen: 0.076 ng
RT: 19.713 min Scan# 1827
Delta R.T. -0.005 min
Lab File: BN017990.D
Acq: 14 Dec 2021 05:00


Tgt Ion:244 Resp: 29780
Ion Ratio Lower Upper
244 100
212 8.3 6.2 9.2
122 12.8 7.9 11.9#

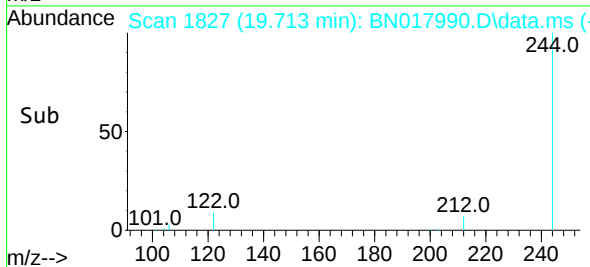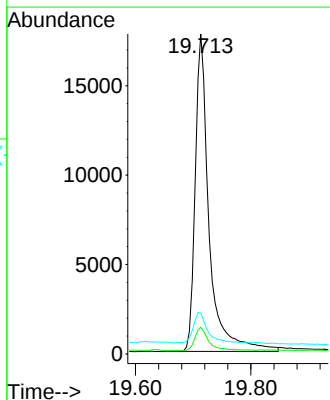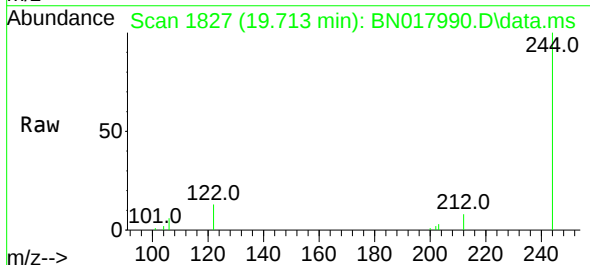

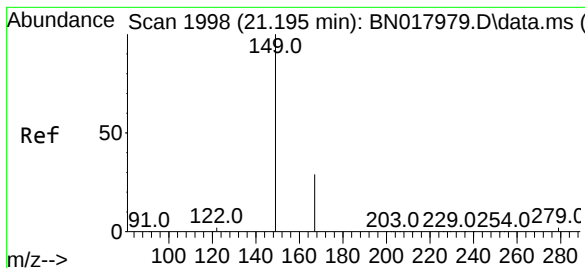

#34
Bis(2-ethylhexyl)phthalate
Concen: 1.187 ng
RT: 21.196 min Scan# 1998
Delta R.T. 0.000 min
Lab File: BN017990.D
Acq: 14 Dec 2021 05:00




Instrument :
BNA_N
ClientSampleId :
RE125D2-20211206DL

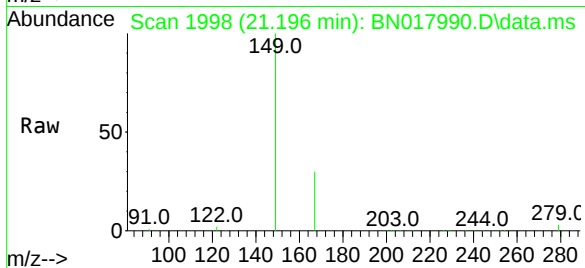


Tgt Ion:149 Resp: 33171
Ion Ratio Lower Upper
149 100
167 29.8 23.7 35.5
279 4.7 3.6 5.4

Manual Integrations
APPROVED

Reviewed By :Christian Giraldo 12/15/2021
Supervised By :Jagrut Upadhyay 12/15/2021

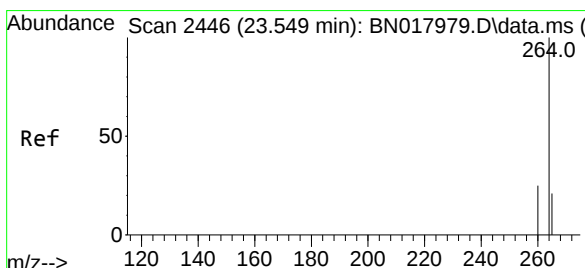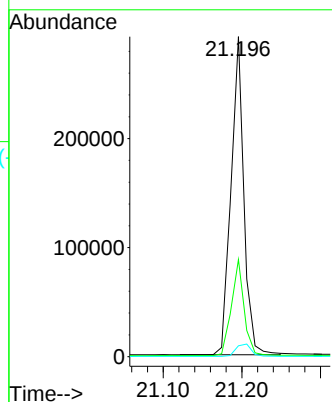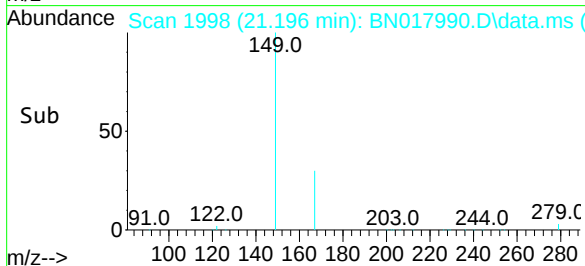

#35
Perylene-d12
Concen: 0.400 ng
RT: 23.546 min Scan# 2445
Delta R.T. -0.003 min
Lab File: BN017990.D
Acq: 14 Dec 2021 05:00

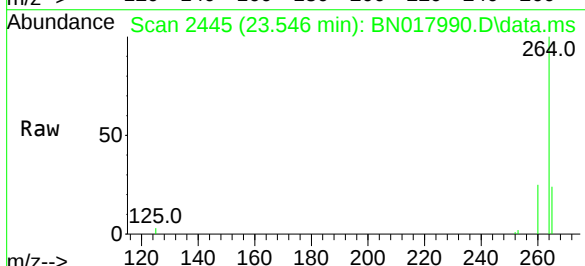

Tgt Ion:264 Resp: 193800
Ion Ratio Lower Upper
264 100
260 25.4 20.2 30.4
265 24.3 18.2 27.2

