
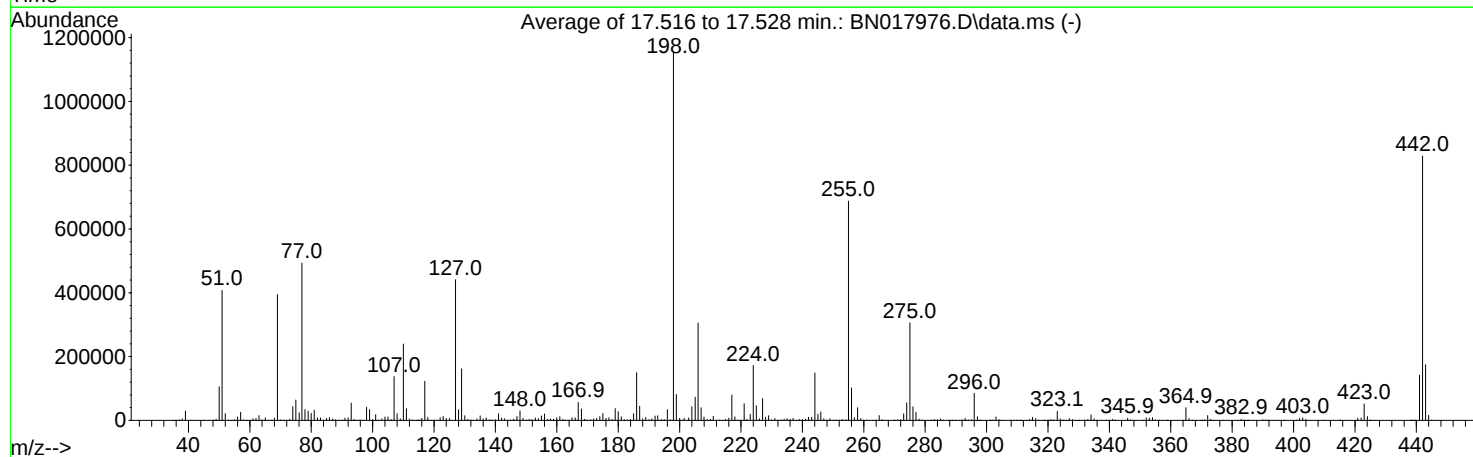


Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN121421\
 Data File : BN017976.D
 Acq On : 13 Dec 2021 19:23
 Operator : CG/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\8270-SIM-BN121421.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Tue Dec 14 01:08:04 2021

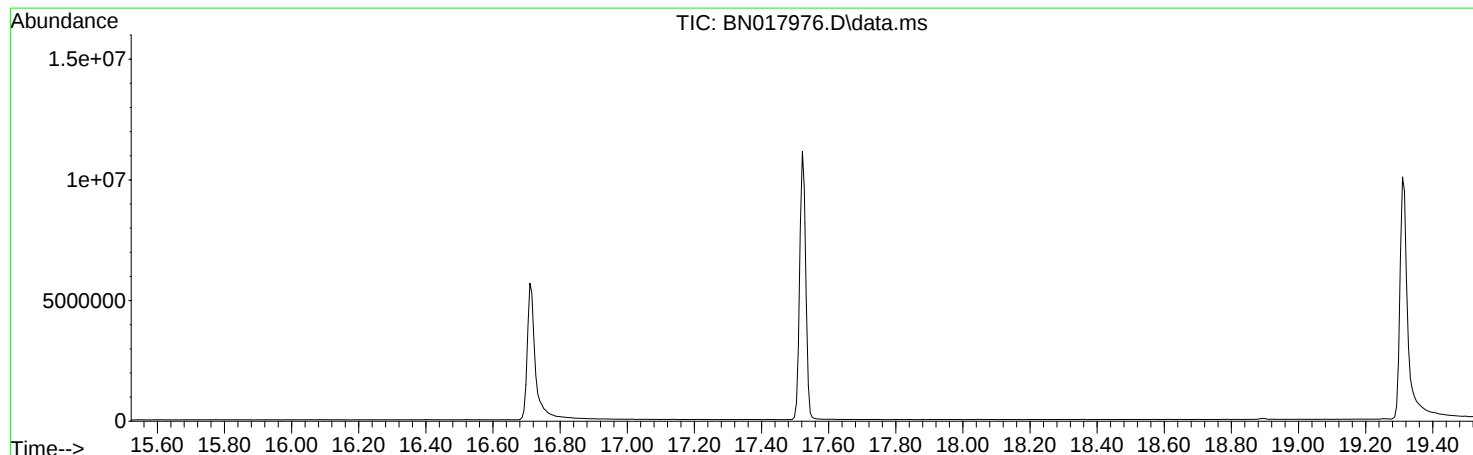

AutoFind: Scans 2470, 2471, 2472; Background Corrected with Scan 2463

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	35.3	407505	PASS
68	69	0.00	2	1.8	7025	PASS
69	198	0.00	100	34.2	394313	PASS
70	69	0.00	2	0.5	1902	PASS
127	198	10	80	38.2	441003	PASS
197	198	0.00	2	0.2	2294	PASS
198	198	100	100	100.0	1153280	PASS
199	198	5	9	7.0	81264	PASS
275	198	10	60	26.5	305813	PASS
365	198	1	100	3.4	39608	PASS
441	198	0.01	100	12.3	142155	PASS
442	442	50	100	100.0	828672	PASS
443	442	15	24	21.1	174456	PASS

Instrument :
 BNA_N
 ClientSampleId :
 DFTPP




DDT Breakdown

Date	Instrument Name	DFTPP Data File
12/14/2021	BNA_N	<u>BN017976.D</u>
Compound Name	Response	Retention Time
DDT	3687108	20.557
DDD	15602	20.169
DDE	1116	19.616
SUM(DDD+DDE)	SUM(DDT+DDD+DDE)	% Breakdown Of DDT
16718	3703826	0.45

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN121421\
 Data File : BN017976.D
 Acq On : 13 Dec 2021 19:23
 Operator : CG/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 DFTPP

Quant Time: Dec 14 05:05:32 2021
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\8270E-Tune.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Tue Dec 14 05:05:27 2021
 Response via : Initial Calibration

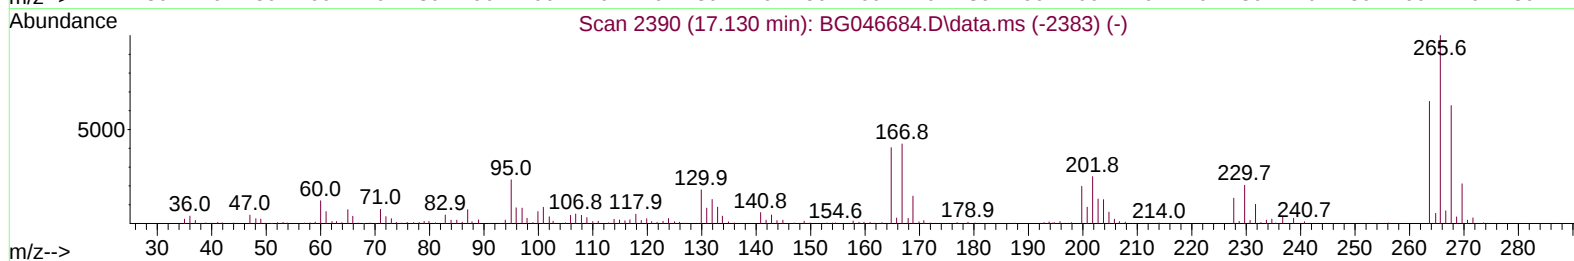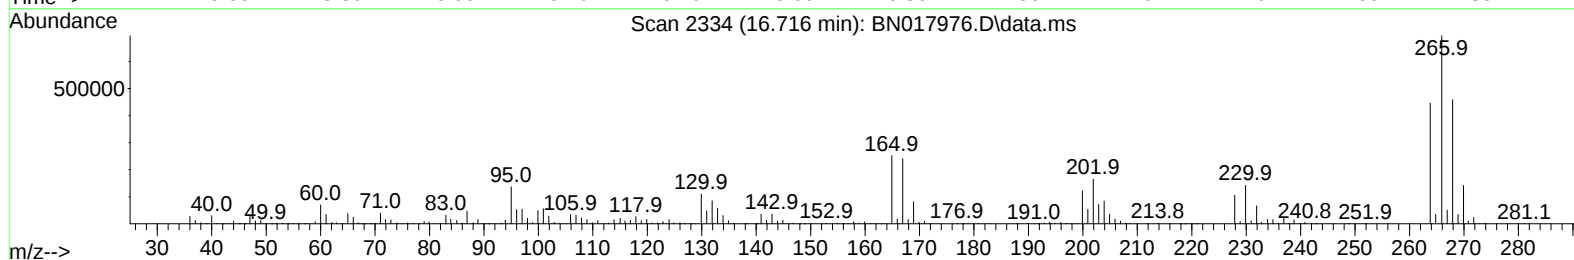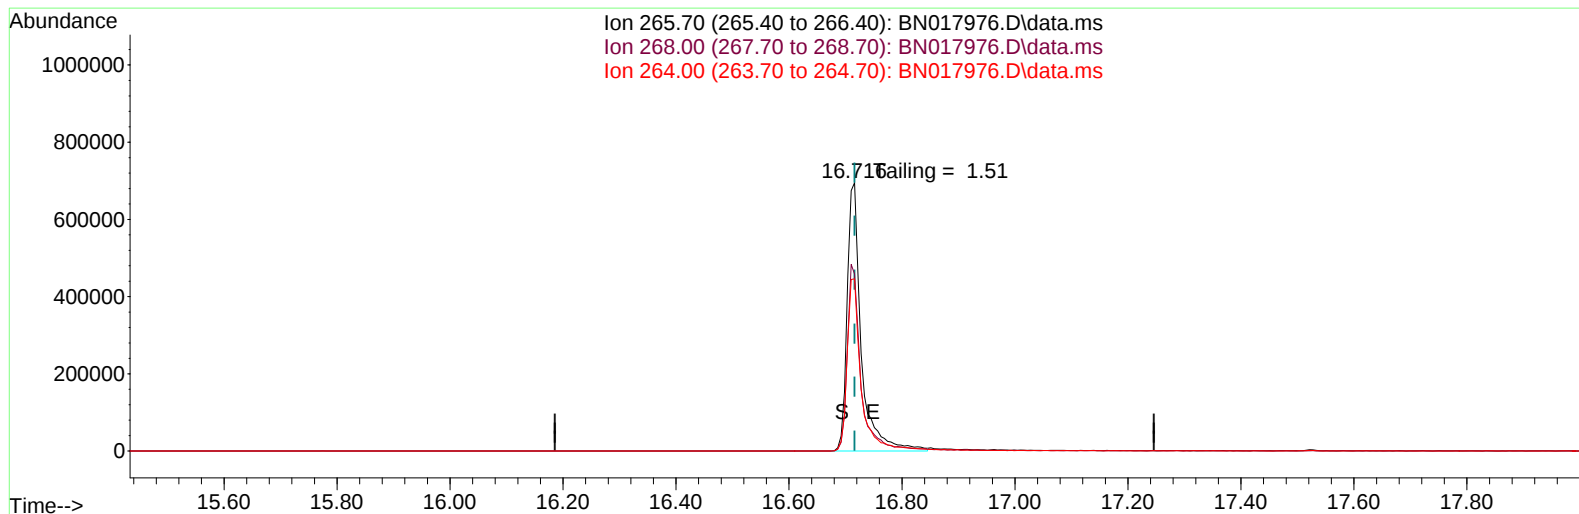

TIC: BN017976.D\data.ms

(70) Pentachlorophenol (C)

16.716min (0.000) 21628.39 ng




response 1233458

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	62.20	65.93
264.00	61.60	64.18
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN121421\
 Data File : BN017976.D
 Acq On : 13 Dec 2021 19:23
 Operator : CG/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 DFTPP

Quant Time: Dec 14 05:05:32 2021
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\8270E-Tune.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Tue Dec 14 05:05:27 2021
 Response via : Initial Calibration

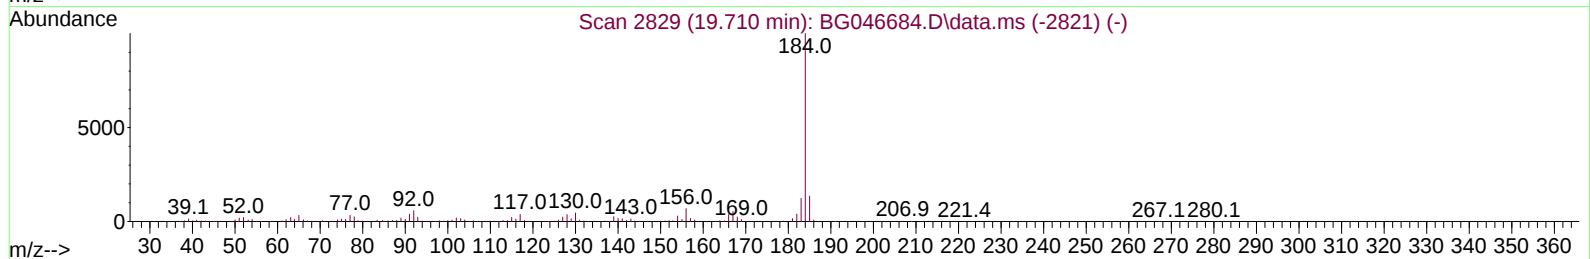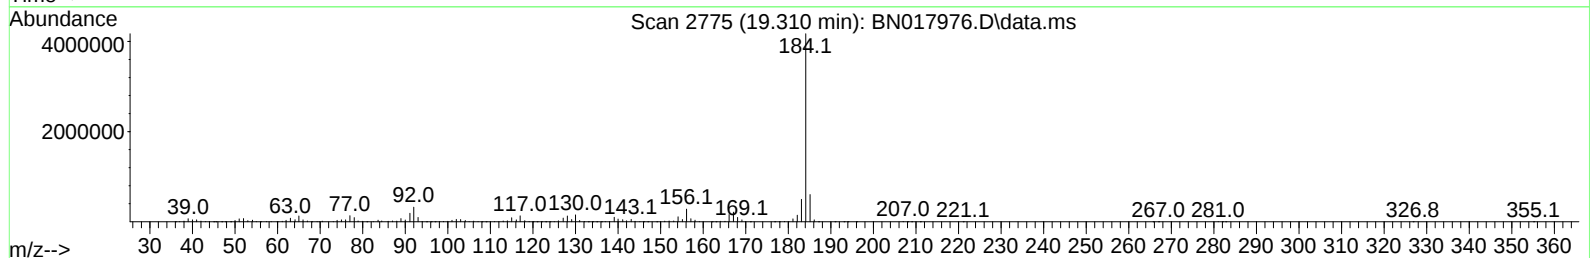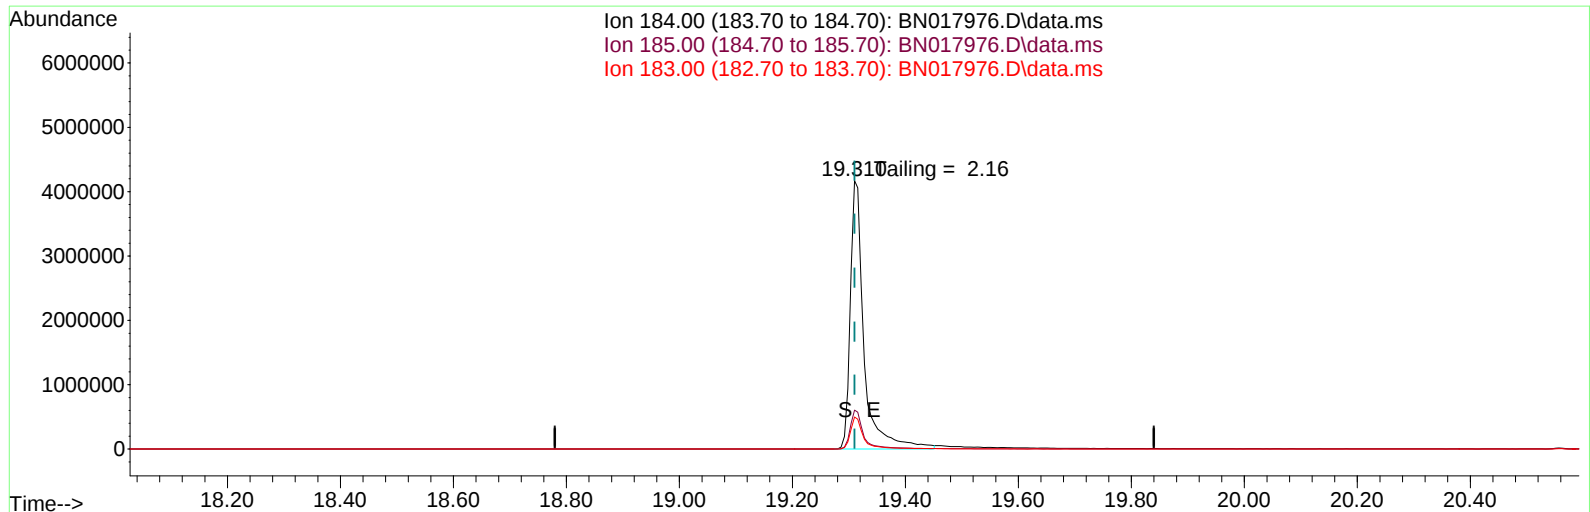

TIC: BN017976.D\data.ms

(77) Benzidine**19.310min (0.000) 2135094.19 ng****response 7305473**

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	15.50	14.49
183.00	13.20	11.92
0.00	0.00	0.00