
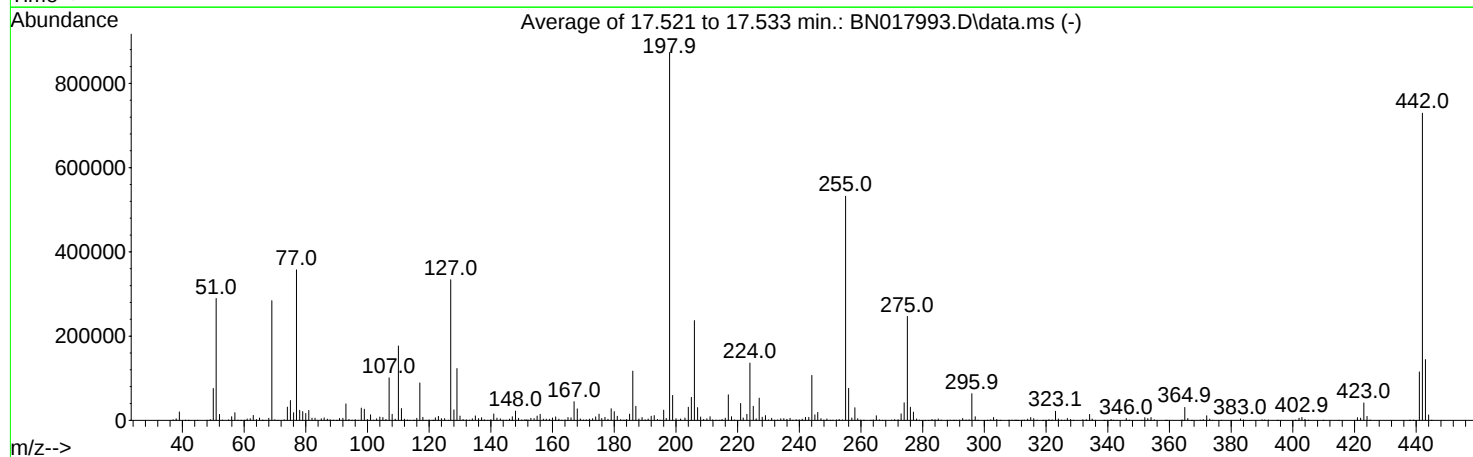


Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN121421\
 Data File : BN017993.D
 Acq On : 14 Dec 2021 07:23
 Operator : CG/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 20 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\8270-SIM-BN121421.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Tue Dec 14 01:08:04 2021

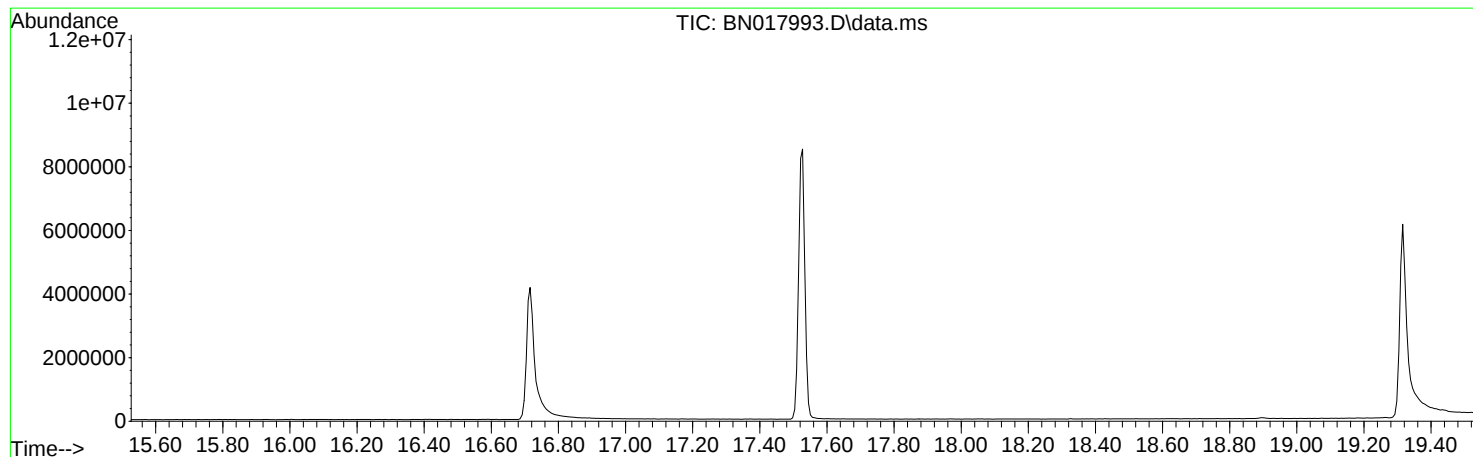




AutoFind: Scans 2471, 2472, 2473; Background Corrected with Scan 2464

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	33.1	289413	PASS
68	69	0.00	2	1.8	5102	PASS
69	198	0.00	100	32.6	284288	PASS
70	69	0.00	2	0.5	1475	PASS
127	198	10	80	38.2	334059	PASS
197	198	0.00	2	0.5	4761	PASS
198	198	100	100	100.0	873365	PASS
199	198	5	9	6.8	59323	PASS
275	198	10	60	28.3	246848	PASS
365	198	1	100	3.5	30885	PASS
441	198	0.01	100	13.2	115171	PASS
442	442	50	100	100.0	729237	PASS
443	442	15	24	19.8	144469	PASS

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN121421\
Data File : BN017993.D
Acq On : 14 Dec 2021 07:23
Operator : CG/JU
Sample : DFTPP
Misc :
ALS Vial : 20 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
DFTPP

Quant Time: Dec 14 08:18:53 2021
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\8270E-Tune.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Dec 14 08:18:48 2021
Response via : Initial Calibration

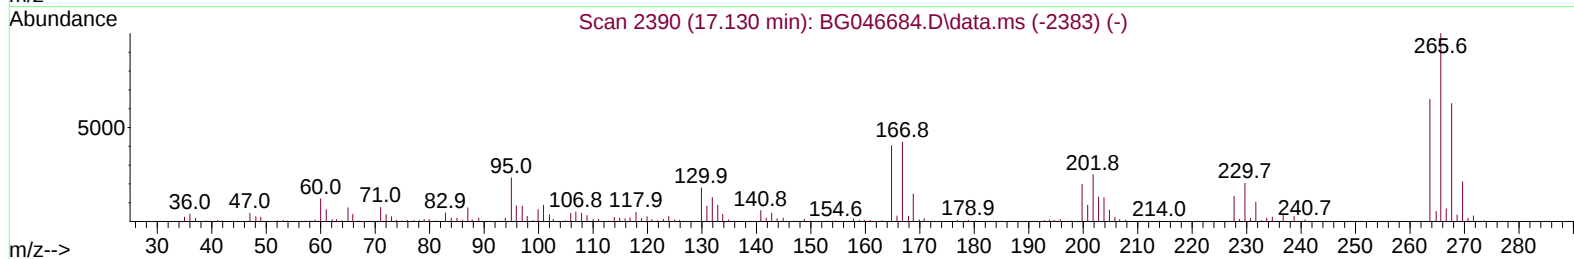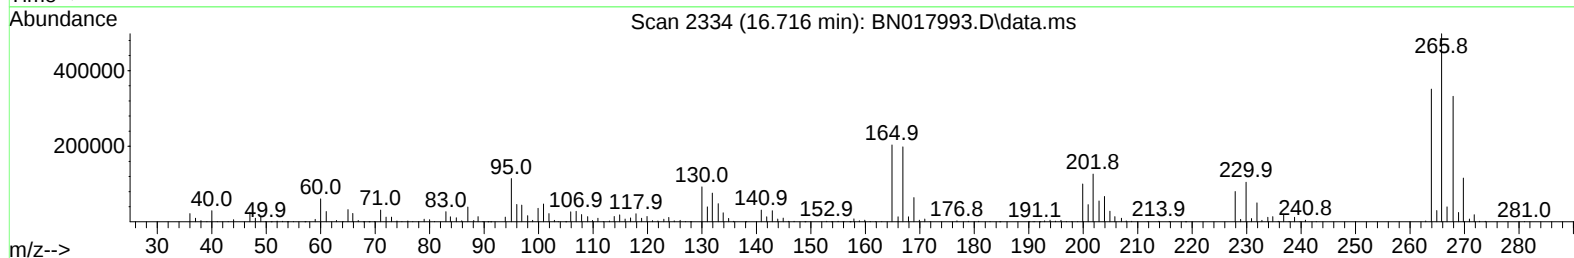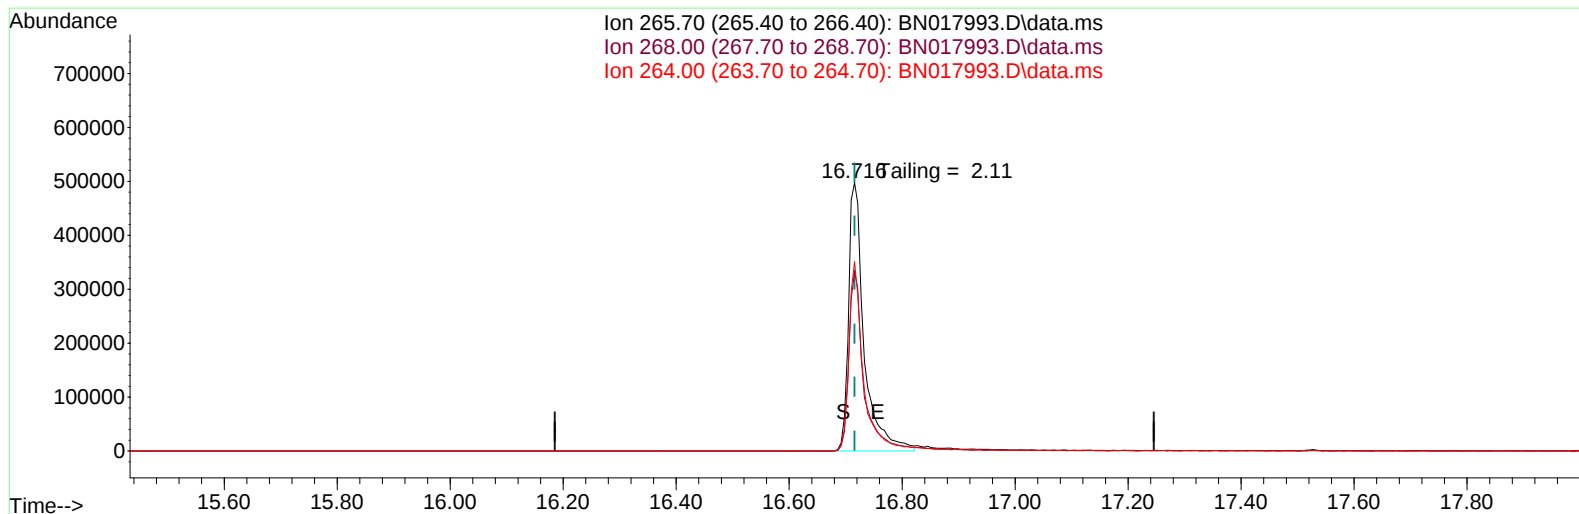

TIC: BN017993.D\data.ms

(70) Pentachlorophenol (C)

16.716min (0.000) 24474.91 ng

response 976691

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	62.20	66.76
264.00	61.60	70.56
0.00	0.00	0.00

Instrument :
 BNA_N
 ClientSampleId :
 DFTPP

DDT Breakdown

Date	Instrument Name	DFTPP Data File
12/14/2021	BNA_N	<u>BN017993.D</u>
Compound Name	Response	Retention Time
DDT	2971700	20.557
DDD	17622	20.168
DDE	1177	19.621
SUM(DDD+DDE)	SUM(DDT+DDD+DDE)	% Breakdown Of DDT
18799	2990499	0.63