


Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN121421\
 Data File : BN018010.D
 Acq On : 14 Dec 2021 19:31
 Operator : CG/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\8270-SIM-BN121421.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Tue Dec 14 01:08:04 2021

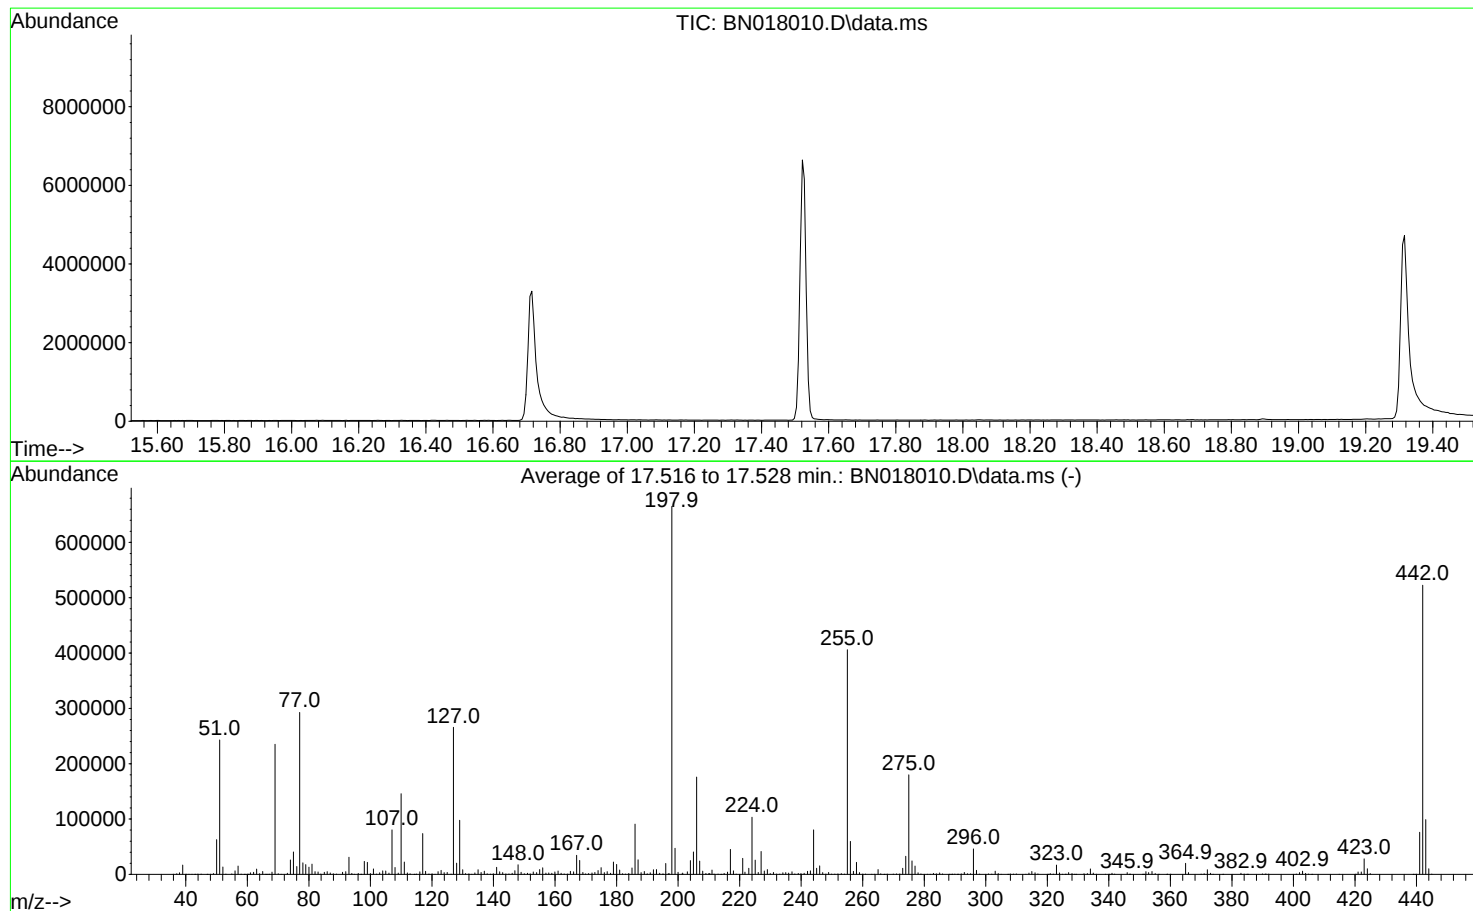




AutoFind: Scans 2470, 2471, 2472; Background Corrected with Scan 2464

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	36.5	242931	PASS
68	69	0.00	2	1.7	3977	PASS
69	198	0.00	100	35.4	235264	PASS
70	69	0.00	2	0.5	1217	PASS
127	198	10	80	40.0	265685	PASS
197	198	0.00	2	0.2	1478	PASS
198	198	100	100	100.0	664939	PASS
199	198	5	9	7.1	47088	PASS
275	198	10	60	27.1	179995	PASS
365	198	1	100	3.0	19846	PASS
441	198	0.01	100	11.4	76109	PASS
442	442	50	100	100.0	522752	PASS
443	442	15	24	18.9	99013	PASS

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN121421\
Data File : BN018010.D
Acq On : 14 Dec 2021 19:31
Operator : CG/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
DFTPP

Quant Time: Dec 15 05:00:09 2021
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\8270E-Tune.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Dec 15 05:00:04 2021
Response via : Initial Calibration

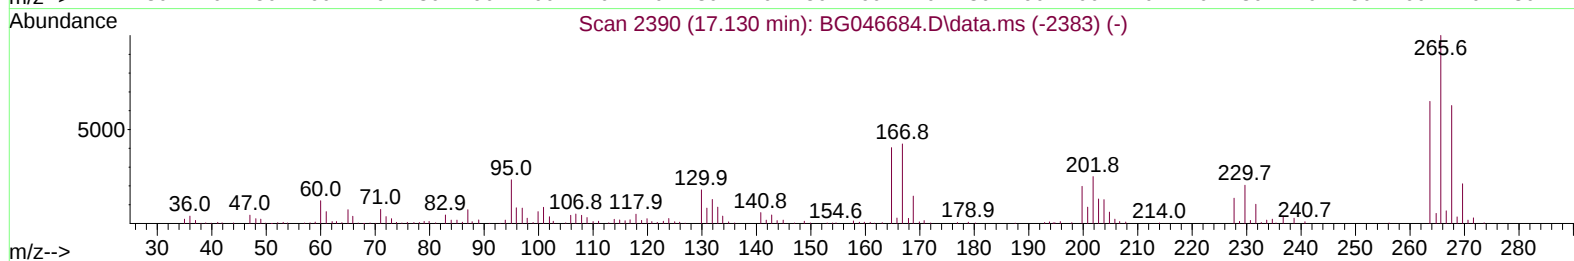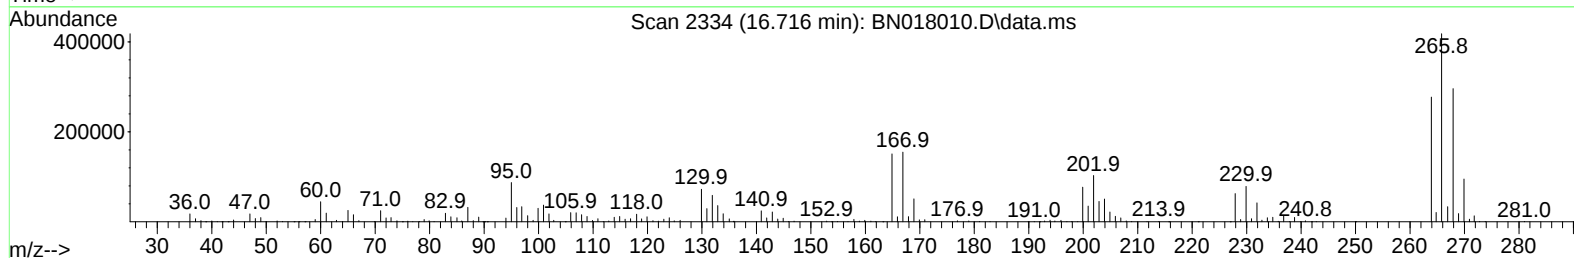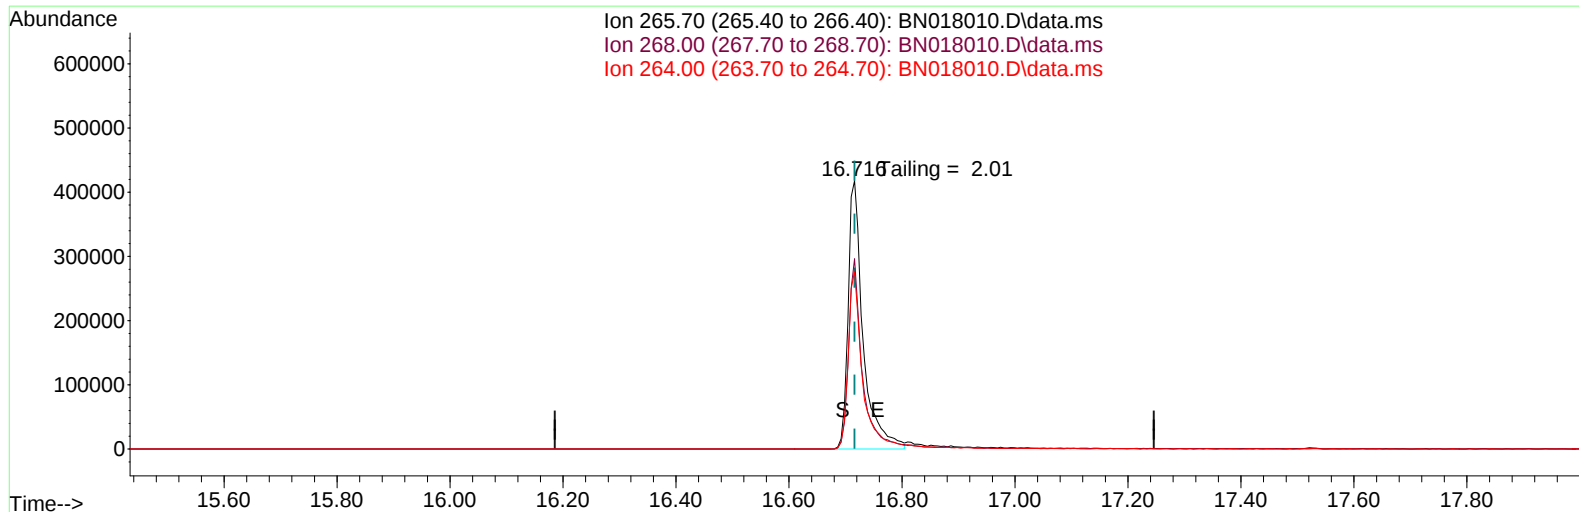

TIC: BN018010.D\data.ms

(70) Pentachlorophenol (C)

16.716min (0.000) 21375.88 ng




response 789611

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	62.20	70.87
264.00	61.60	66.32
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN121421\
 Data File : BN018010.D
 Acq On : 14 Dec 2021 19:31
 Operator : CG/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 DFTPP

Quant Time: Dec 15 06:05:30 2021
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\8270E-Tune.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Wed Dec 15 06:05:25 2021
 Response via : Initial Calibration

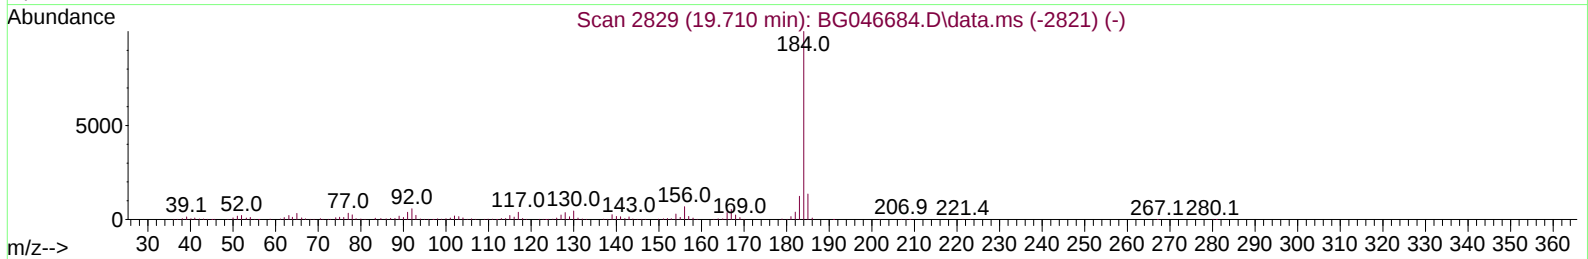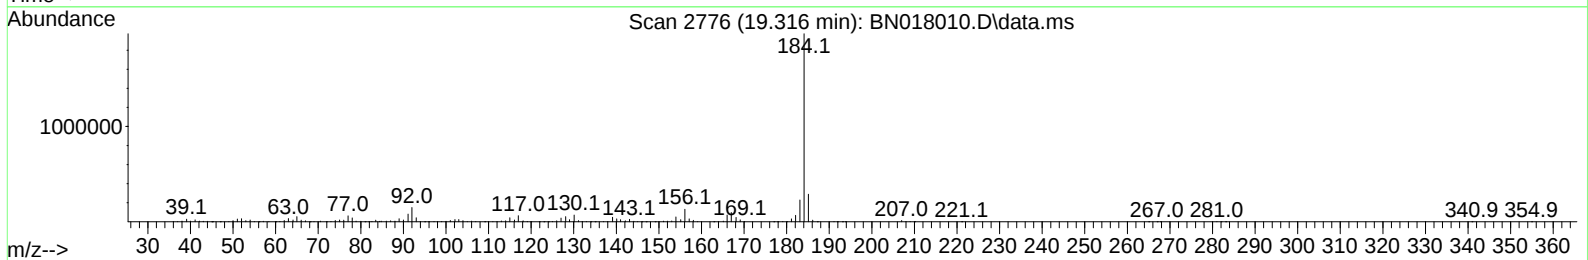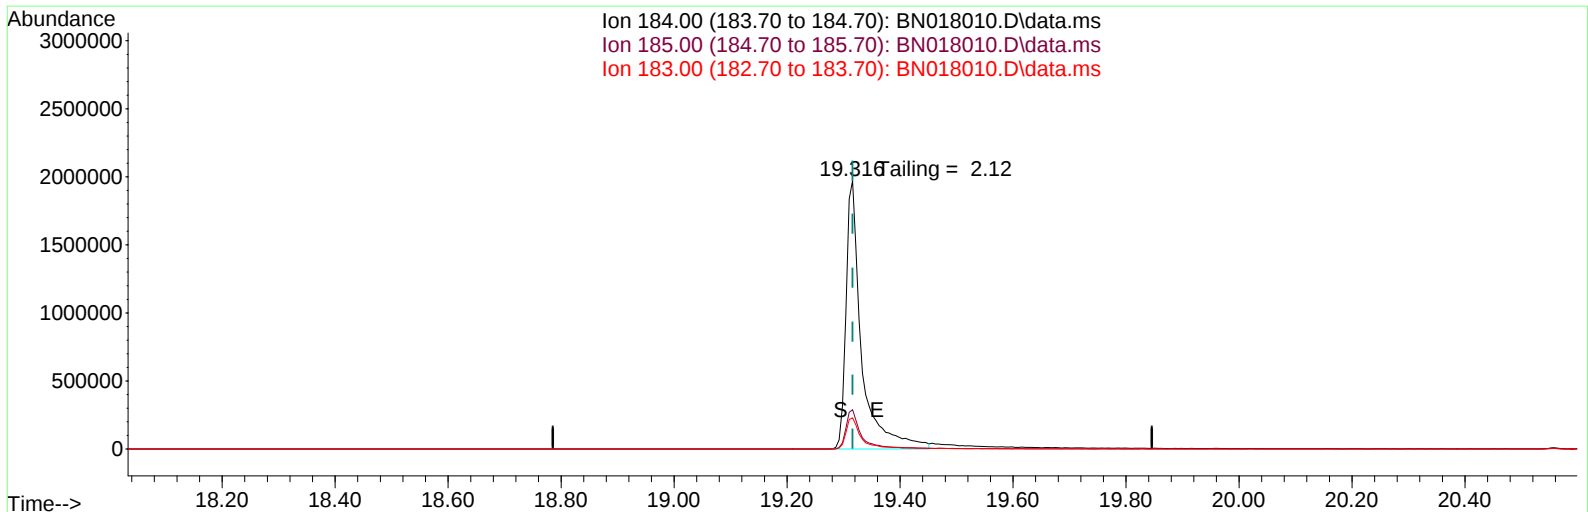

TIC: BN018010.D\data.ms

(77) Benzidine

19.316min (0.000) 1067300.47 ng

response 3980892

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	15.50	14.68
183.00	13.20	11.63
0.00	0.00	0.00

Instrument :
 BNA_N
 ClientSampleId :
 DFTPP

DDT Breakdown

Date	Instrument Name	DFTPP Data File
12/14/2021	BNA_N	<u>BN018010.D</u>
Compound Name	Response	Retention Time
DDT	2298780	20.557
DDD	36848	20.116
DDE	6630	19.61
SUM(DDD+DDE)	SUM(DDT+DDD+DDE)	% Breakdown Of DDT
43478	2342258	1.86