

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN121620\
 Data File : BN013174.D
 Acq On : 16 Dec 2020 20:20
 Operator : CG/JU
 Sample : L5053-07
 Misc :
 ALS Vial : 27 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 RE104D3-20201209

Quant Time: Dec 17 03:07:39 2020
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\8270-SIM-BN121620.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Tue Dec 15 16:49:20 2020
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.346	152	569	0.40	ng	0.00
7) Naphthalene-d8	10.137	136	1645	0.40	ng	# 0.03
13) Acenaphthene-d10	14.003	164	1085	0.40	ng	-0.01
19) Phenanthrene-d10	16.787	188	2257	0.40	ng	# 0.01
29) Chrysene-d12	21.016	240	2676	0.40	ng	# 0.01
36) Perylene-d12	23.106	264	3057	0.40	ng	# 0.00
System Monitoring Compounds						
4) 2-Fluorophenol	4.978	112	239	0.10	ng	0.00
5) Phenol-d6	6.548	99	115	0.05	ng	0.00
8) Nitrobenzene-d5	8.553	82	497	0.29	ng	0.04
11) 2-Methylnaphthalene-d10	11.742	152	810	0.28	ng	0.02
14) 2,4,6-Tribromophenol	15.539	330	162	0.24	ng	0.00
15) 2-Fluorobiphenyl	12.633	172	1255	0.28	ng	0.00
27) Fluoranthene-d10	18.826	212	3006	0.40	ng	0.00
31) Terphenyl-d14	19.441	244	2650	0.39	ng	0.00
Target Compounds						
						Qvalue
2) 1,4-Dioxane	3.029	88	20	0.02	ng	# 1
3) n-Nitrosodimethylamine	3.214	42	98	0.06	ng	# 42
12) 2-Methylnaphthalene	11.817	142	72	0.02	ng	# 65
20) 4,6-Dinitro-2-methylph...	15.247	198	1	0.19	ng	# 1
21) 4-Bromophenyl-phenylether	16.021	248	170	0.39	ng	# 72
23) Atrazine	16.021	200	171	0.13	ng	# 1
25) Phenanthrene	16.824	178	192	0.03	ng	# 89
34) Bis(2-ethylhexyl)phtha...	20.931	149	631	Below	Cal	97

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN121620\
Data File : BN013174.D
Acq On : 16 Dec 2020 20:20
Operator : CG/JU
Sample : L5053-07
Misc :
ALS Vial : 27 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
RE104D3-20201209

Quant Time: Dec 17 03:07:39 2020
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\8270-SIM-BN121620.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Dec 15 16:49:20 2020
Response via : Initial Calibration

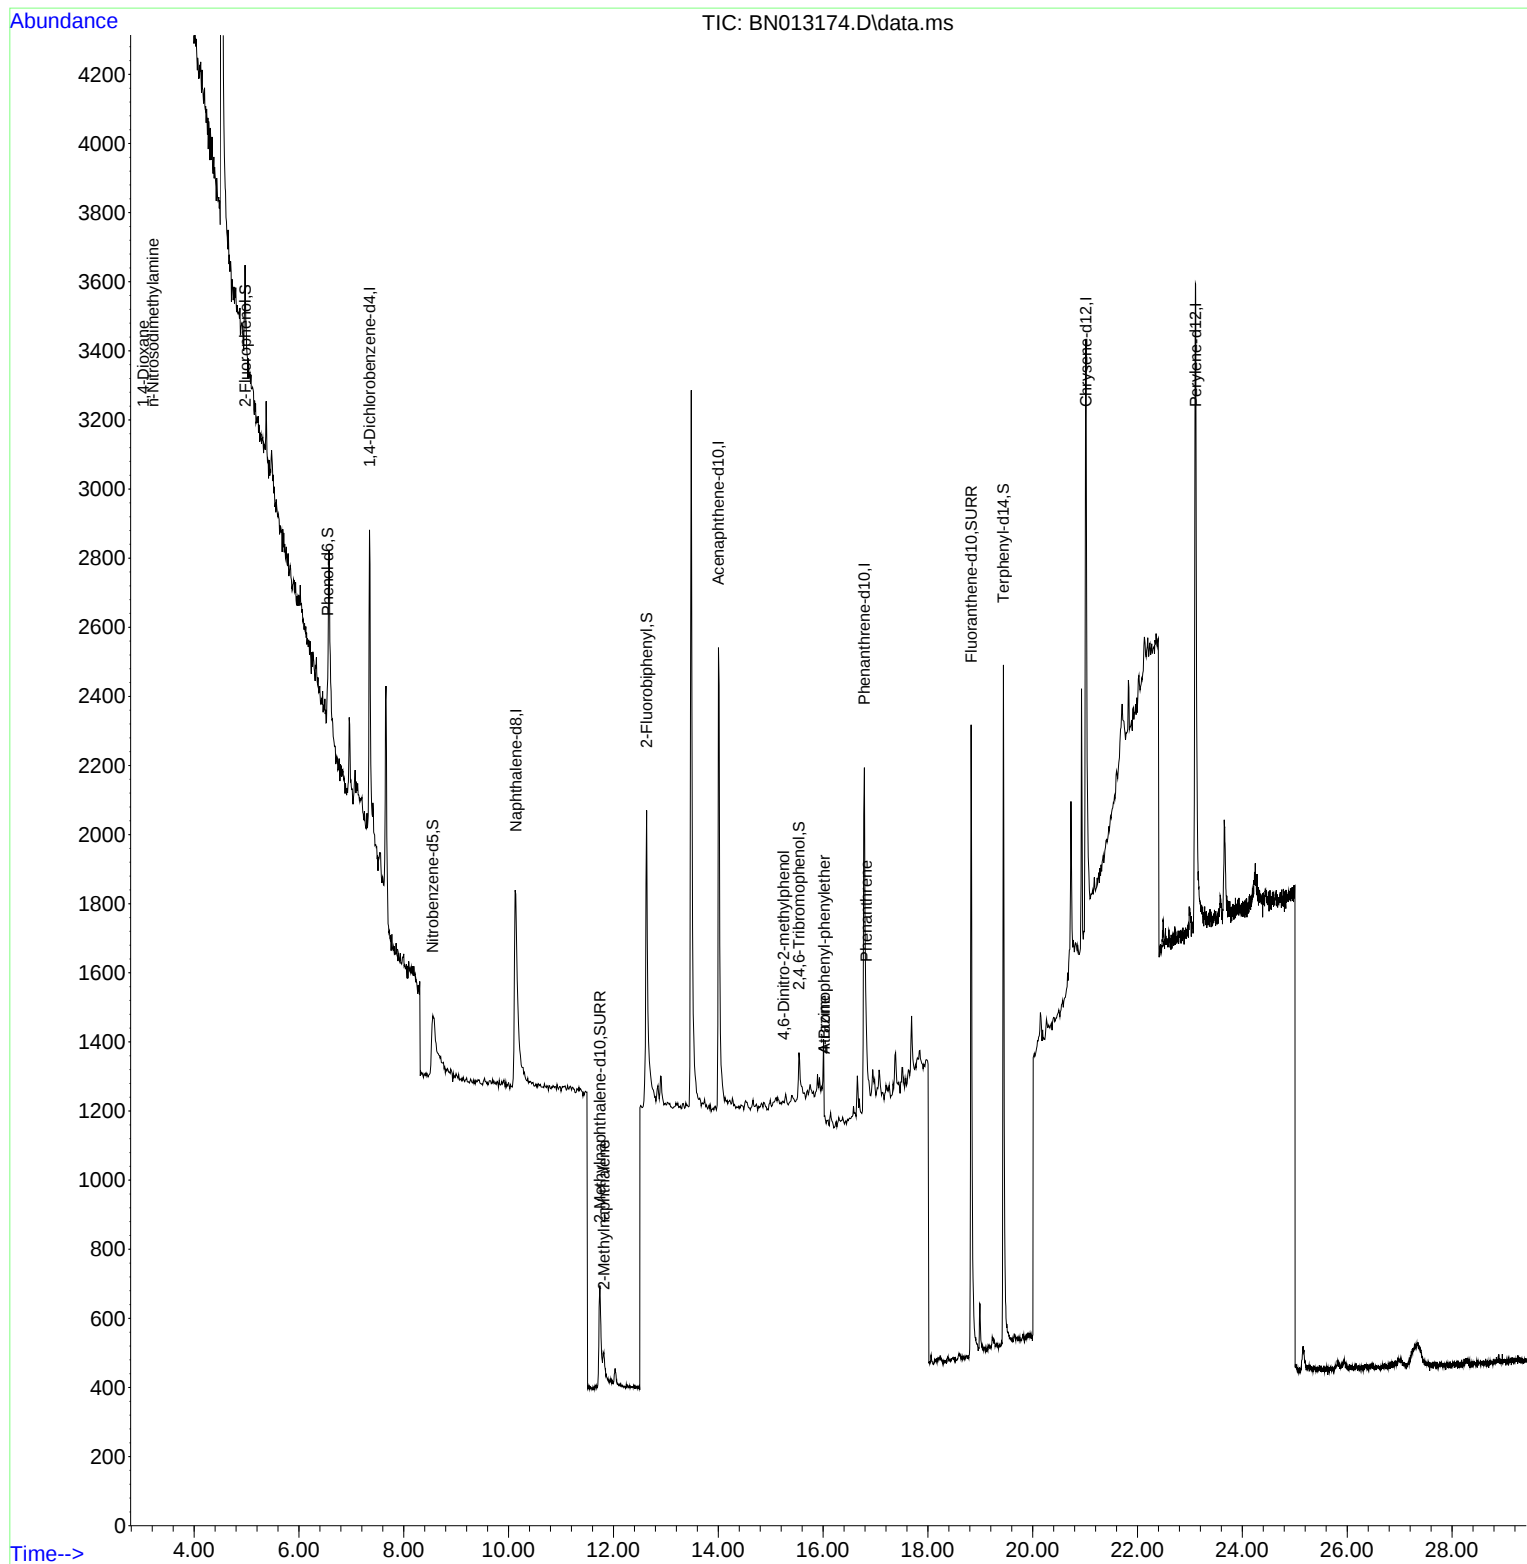






#1
1,4-Dichlorobenzene-d4
Concen: 0.40 ng
RT: 7.346 min Scan# 567
Delta R.T. -0.008 min
Lab File: BN013174.D
Acq: 16 Dec 2020 20:20

Instrument :
BNA_N
ClientSampleId :
RE104D3-20201209

Tgt Ion:152 Resp: 569




Ion	Ratio	Lower	Upper
152	100		
150	148.7	116.6	174.8
115	78.2	52.9	79.3

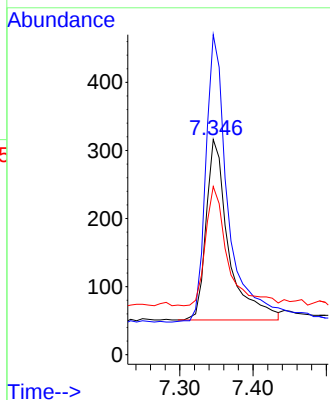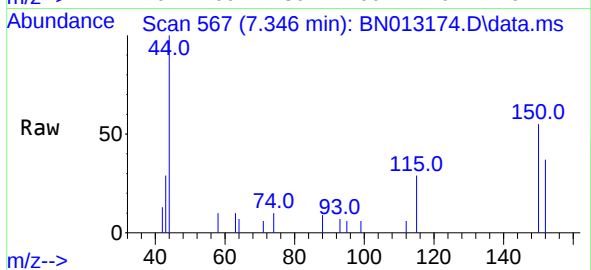


#2
1,4-Dioxane
Concen: 0.02 ng
RT: 3.029 min Scan# 31
Delta R.T. 0.088 min
Lab File: BN013174.D
Acq: 16 Dec 2020 20:20

Tgt Ion: 88 Resp: 20

Ion	Ratio	Lower	Upper
88	100		
58	0.0	59.4	89.2#
43	200.0	32.3	48.5#


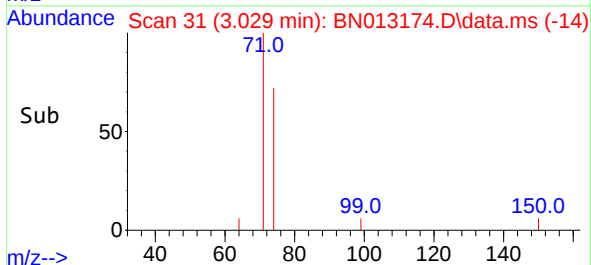
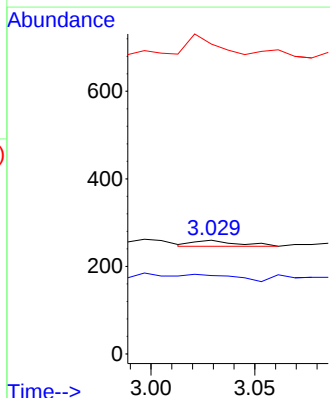
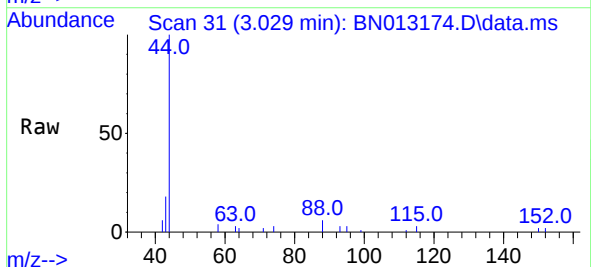




#3
n-Nitrosodimethylamine
Concen: 0.06 ng
RT: 3.214 min Scan# 54
Delta R.T. -0.065 min
Lab File: BN013174.D
Acq: 16 Dec 2020 20:20




Instrument :
BNA_N
ClientSampleId :
RE104D3-20201209

Tgt Ion: 42 Resp: 98
Ion Ratio Lower Upper
42 100
74 27.6 64.4 96.6#
44 0.0 2.8 4.2#

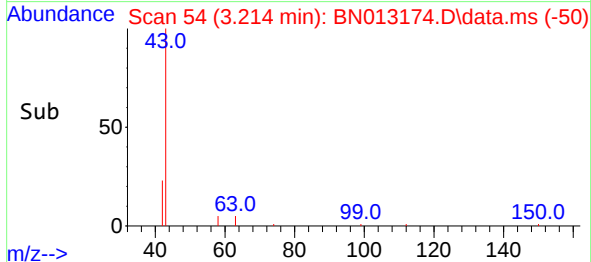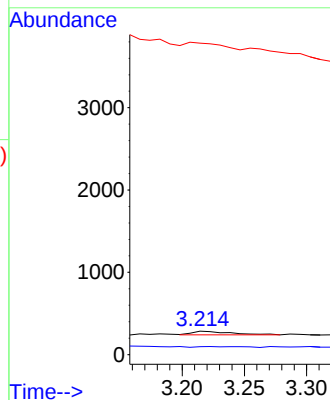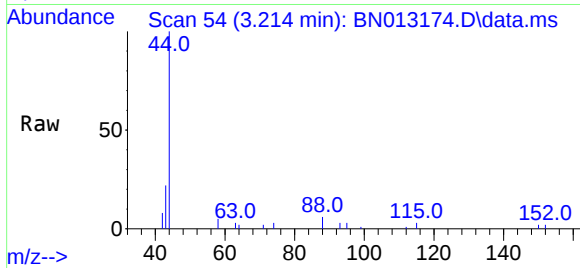

#4
2-Fluorophenol
Concen: 0.10 ng
RT: 4.978 min Scan# 273
Delta R.T. 0.008 min
Lab File: BN013174.D
Acq: 16 Dec 2020 20:20

Tgt Ion: 112 Resp: 239
Ion Ratio Lower Upper
112 100
64 69.5 49.5 74.3
63 45.2 32.0 48.0


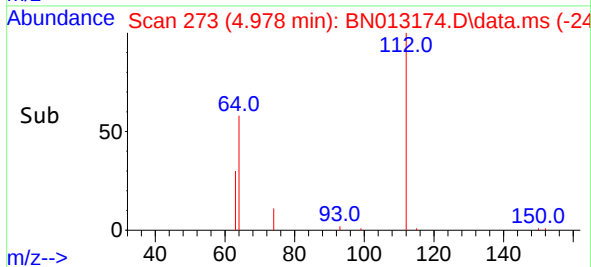
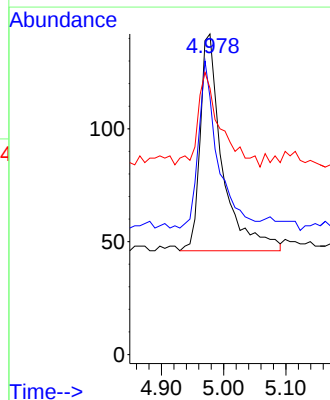
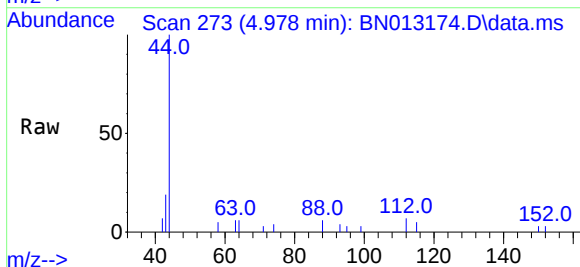




#5
Phenol-d6
Concen: 0.05 ng
RT: 6.548 min Scan# 468
Delta R.T. -0.008 min
Lab File: BN013174.D
Acq: 16 Dec 2020 20:20




Instrument :
BNA_N
ClientSampleId :
RE104D3-20201209


Tgt Ion: 99 Resp: 115
Ion Ratio Lower Upper
99 100
42 69.6 22.4 33.6#
71 45.2 37.8 56.6

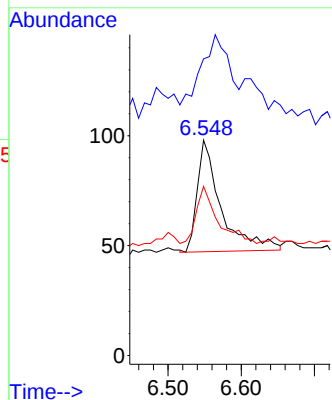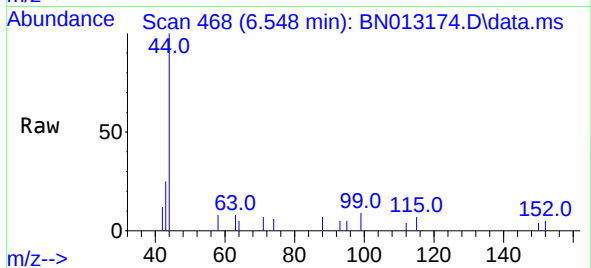

#7
Naphthalene-d8
Concen: 0.40 ng
RT: 10.137 min Scan# 831
Delta R.T. 0.025 min
Lab File: BN013174.D
Acq: 16 Dec 2020 20:20

Tgt Ion: 136 Resp: 1645
Ion Ratio Lower Upper
136 100
137 21.0 10.6 15.8#
54 19.9 8.6 12.8#
68 15.0 5.7 8.5#


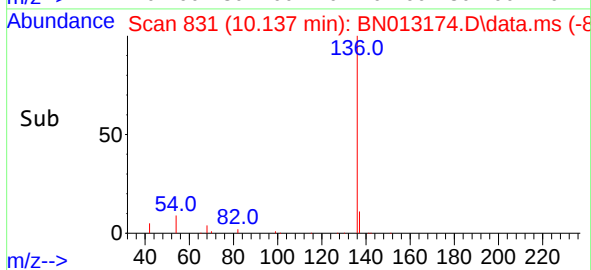
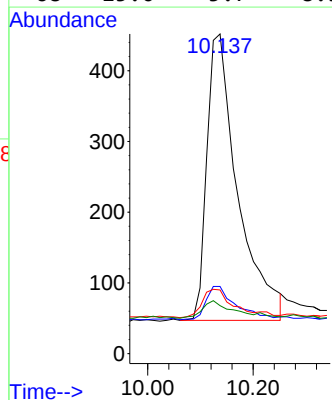





#8
Nitrobenzene-d5
Concen: 0.29 ng
RT: 8.553 min Scan# 706
Delta R.T. 0.038 min
Lab File: BN013174.D
Acq: 16 Dec 2020 20:20




Instrument :
BNA_N
ClientSampleId :
RE104D3-20201209


Tgt Ion: 82 Resp: 497
Ion Ratio Lower Upper
82 100
128 60.5 30.6 46.0#
54 79.8 48.3 72.5#

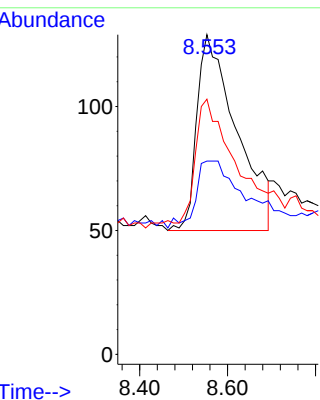

#11
2-Methylnaphthalene-d10
Concen: 0.28 ng
RT: 11.742 min Scan# 992
Delta R.T. 0.018 min
Lab File: BN013174.D
Acq: 16 Dec 2020 20:20

Tgt Ion: 152 Resp: 810
Ion Ratio Lower Upper
152 100
151 18.5 16.7 25.1

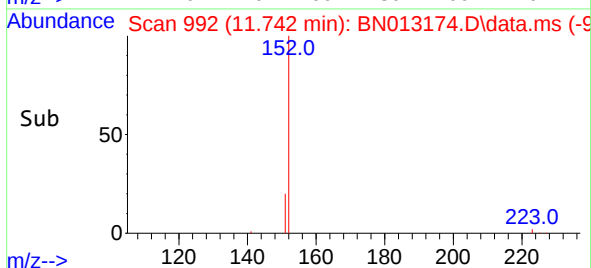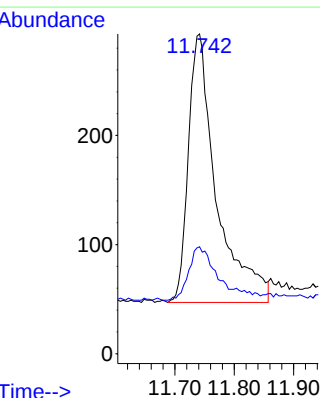







#12
2-Methylnaphthalene
Concen: 0.02 ng
RT: 11.817 min Scan# 1009
Delta R.T. 0.013 min
Lab File: BN013174.D
Acq: 16 Dec 2020 20:20

Instrument :
BNA_N
ClientSampleId :
RE104D3-20201209

Tgt Ion:142 Resp: 72




Ion	Ratio	Lower	Upper
142	100		
141	93.3	69.4	104.2
115	102.7	35.7	53.5

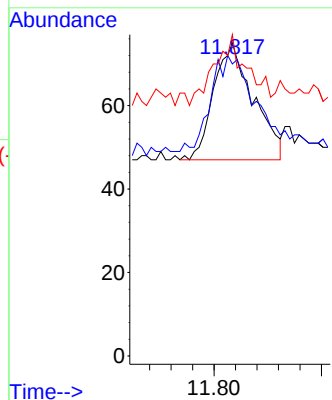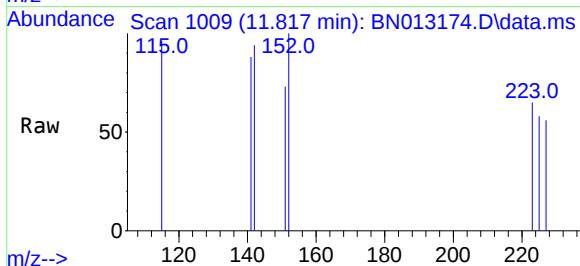


#13
Acenaphthene-d10
Concen: 0.40 ng
RT: 14.003 min Scan# 1282
Delta R.T. -0.013 min
Lab File: BN013174.D
Acq: 16 Dec 2020 20:20

Tgt Ion:164 Resp: 1085

Ion	Ratio	Lower	Upper
164	100		
162	106.8	80.6	120.8
160	55.6	39.5	59.3


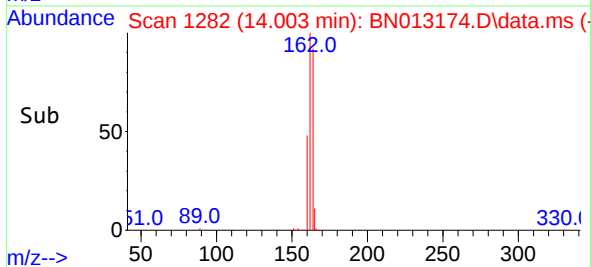
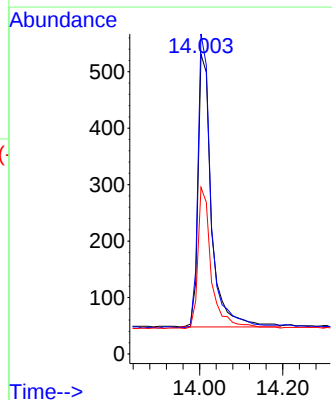
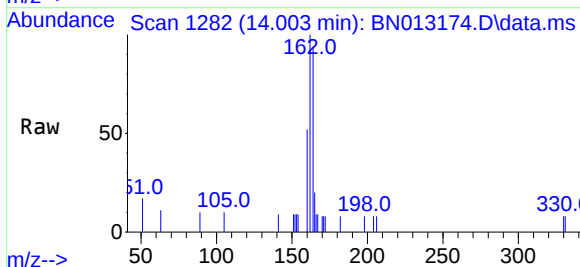




#14
2,4,6-Tribromophenol
Concen: 0.24 ng
RT: 15.539 min Scan# 1403
Delta R.T. -0.000 min
Lab File: BN013174.D
Acq: 16 Dec 2020 20:20




Instrument :
BNA_N
ClientSampleId :
RE104D3-20201209


Tgt Ion:330 Resp: 162
Ion Ratio Lower Upper
330 100
332 0.0 0.0 0.0
141 53.1 34.4 51.6#

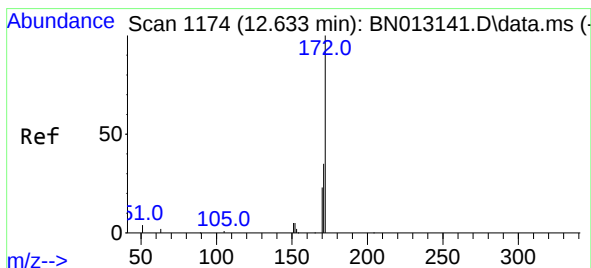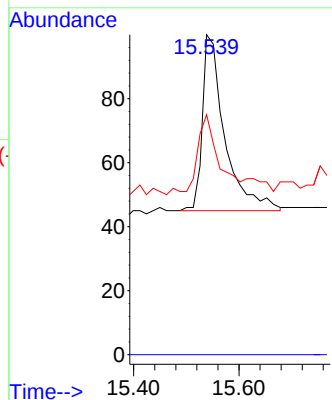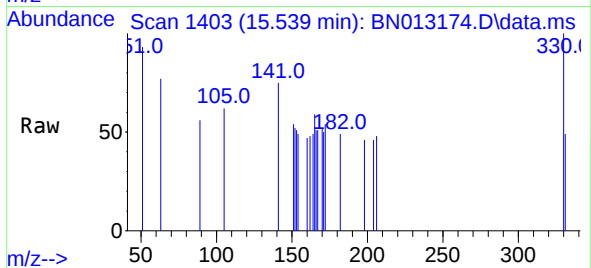

#15
2-Fluorobiphenyl
Concen: 0.28 ng
RT: 12.633 min Scan# 1174
Delta R.T. -0.000 min
Lab File: BN013174.D
Acq: 16 Dec 2020 20:20

Tgt Ion:172 Resp: 1255
Ion Ratio Lower Upper
172 100
171 42.1 28.2 42.4
170 30.3 20.0 30.0#


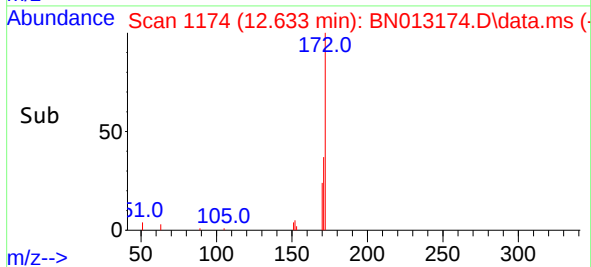
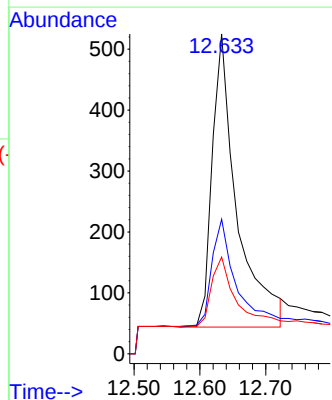
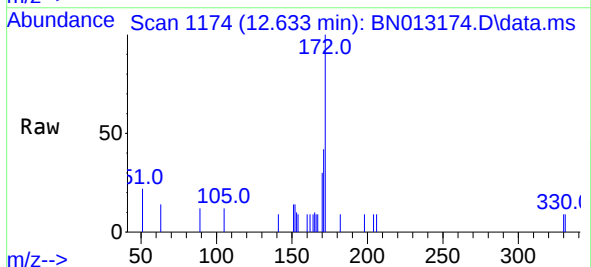




#19
Phenanthrene-d10
Concen: 0.40 ng
RT: 16.787 min Scan# 1504
Delta R.T. 0.012 min
Lab File: BN013174.D
Acq: 16 Dec 2020 20:20




Instrument :
BNA_N
ClientSampleId :
RE104D3-20201209


Tgt Ion:	188	Resp:	2257
Ion	Ratio	Lower	Upper
188	100		
94	0.0	0.0	0.0
80	10.9	5.0	7.4#

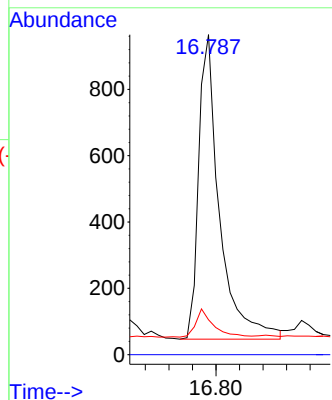

#20
4,6-Dinitro-2-methylphenol
Concen: 0.19 ng
RT: 15.247 min Scan# 1380
Delta R.T. 0.013 min
Lab File: BN013174.D
Acq: 16 Dec 2020 20:20

Tgt Ion:	198	Resp:	1
Ion	Ratio	Lower	Upper
198	100		
51	204.3	43.5	65.3#
105	128.3	27.2	40.8#


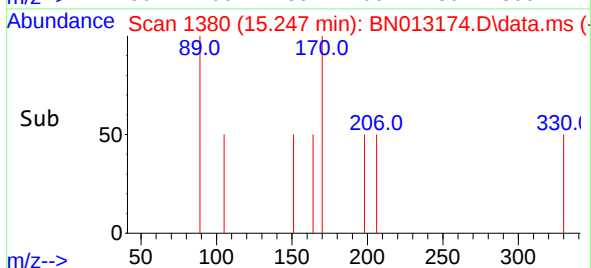
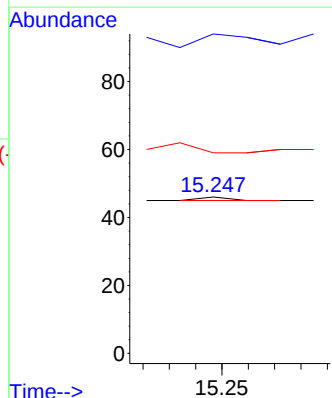





#21
4-Bromophenyl-phenylether
Concen: 0.39 ng
RT: 16.021 min Scan# 1441
Delta R.T. -0.000 min
Lab File: BN013174.D
Acq: 16 Dec 2020 20:20




Instrument :
BNA_N
ClientSampleId :
RE104D3-20201209


Tgt Ion:248 Resp: 170
Ion Ratio Lower Upper
248 100
250 104.3 77.3 115.9
141 117.4 57.8 86.8#

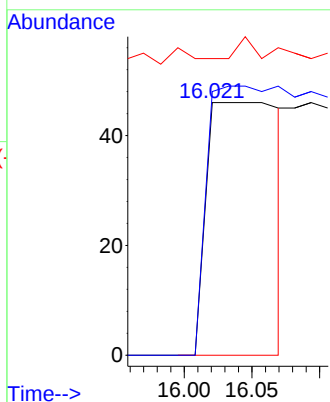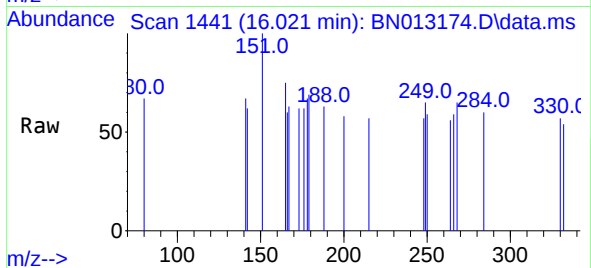

#23
Atrazine
Concen: 0.13 ng
RT: 16.021 min Scan# 1441
Delta R.T. -0.256 min
Lab File: BN013174.D
Acq: 16 Dec 2020 20:20

Tgt Ion:200 Resp: 171
Ion Ratio Lower Upper
200 100
173 106.4 22.8 34.2#
215 97.9 38.1 57.1#


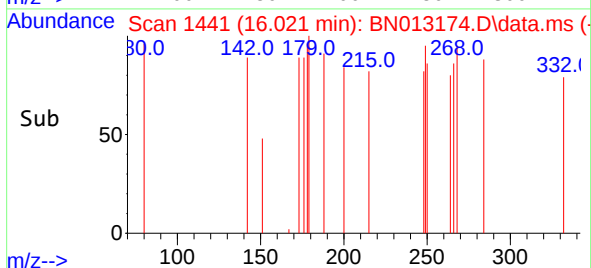
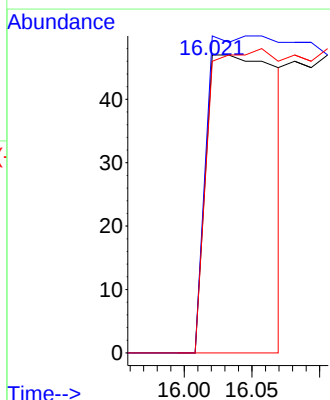





#25
Phenanthrene
Concen: 0.03 ng
RT: 16.824 min Scan# 1507
Delta R.T. -0.000 min
Lab File: BN013174.D
Acq: 16 Dec 2020 20:20




Instrument :
BNA_N
ClientSampleId :
RE104D3-20201209


Tgt Ion:	178	Resp:	192
Ion	Ratio	Lower	Upper
178	100		
176	21.9	14.8	22.2
179	21.9	12.4	18.6#

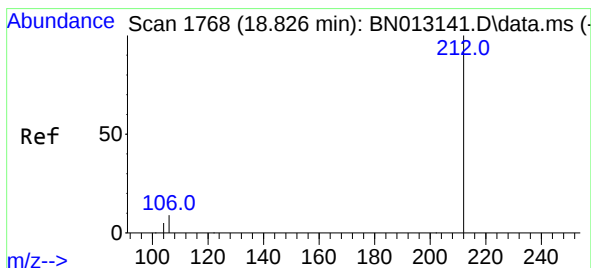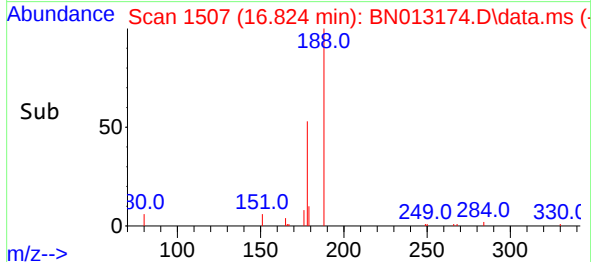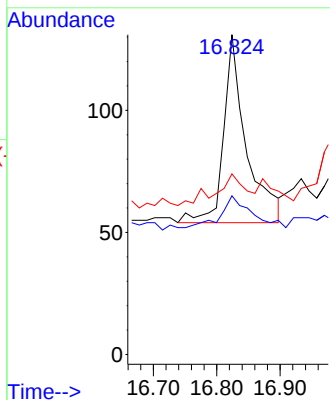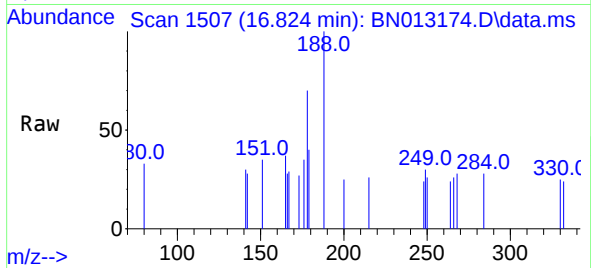

#27
Fluoranthene-d10
Concen: 0.40 ng
RT: 18.826 min Scan# 1768
Delta R.T. -0.000 min
Lab File: BN013174.D
Acq: 16 Dec 2020 20:20

Tgt Ion:	212	Resp:	3006
Ion	Ratio	Lower	Upper
212	100		
106	8.6	6.8	10.2
104	5.4	4.1	6.1


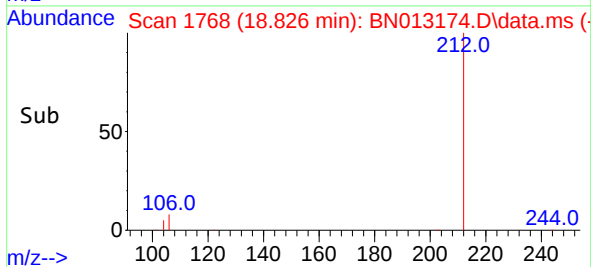
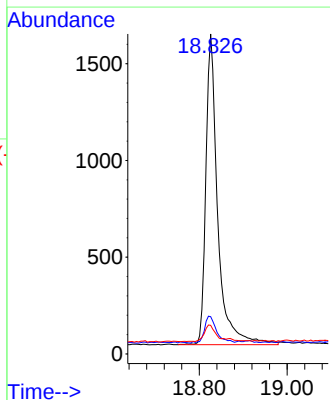
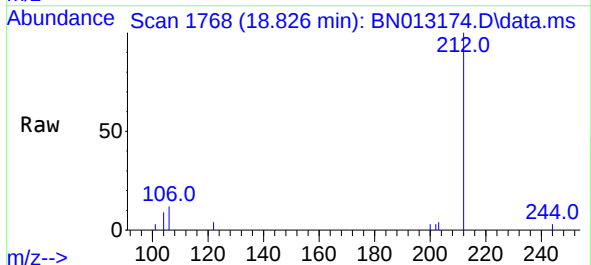




#29
Chrysene-d12
Concen: 0.40 ng
RT: 21.016 min Scan# 2101
Delta R.T. 0.010 min
Lab File: BN013174.D
Acq: 16 Dec 2020 20:20




Instrument :
BNA_N
ClientSampleId :
RE104D3-20201209


Tgt Ion:240 Resp: 2676
Ion Ratio Lower Upper
240 100
120 14.0 5.3 7.9#
236 30.2 21.8 32.8

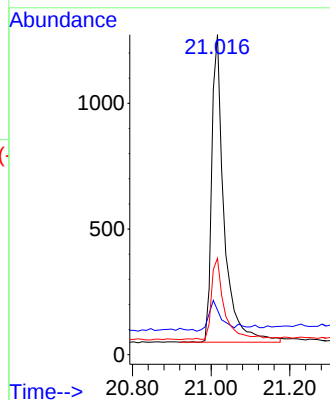

#31
Terphenyl-d14
Concen: 0.39 ng
RT: 19.441 min Scan# 1892
Delta R.T. -0.005 min
Lab File: BN013174.D
Acq: 16 Dec 2020 20:20

Tgt Ion:244 Resp: 2650
Ion Ratio Lower Upper
244 100
212 11.3 7.3 10.9#
122 11.6 7.3 10.9#

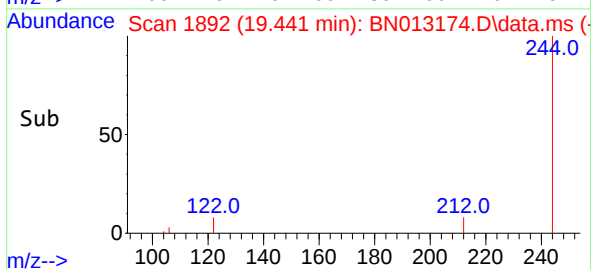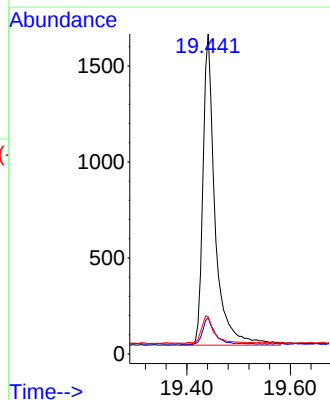




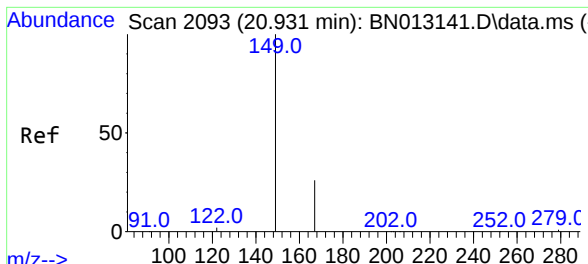


#34
 Bis(2-ethylhexyl)phthalate
 Concen: Below Cal
 RT: 20.931 min Scan# 2093
 Delta R.T. 0.000 min
 Lab File: BN013174.D
 Acq: 16 Dec 2020 20:20

Instrument :
 BNA_N
 ClientSampleId :
 RE104D3-20201209

Tgt Ion:149 Resp: 631

Ion	Ratio	Lower	Upper
149	100		
167	27.1	23.2	34.8
279	4.0	3.9	5.9

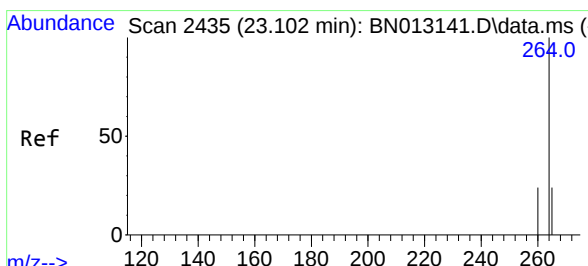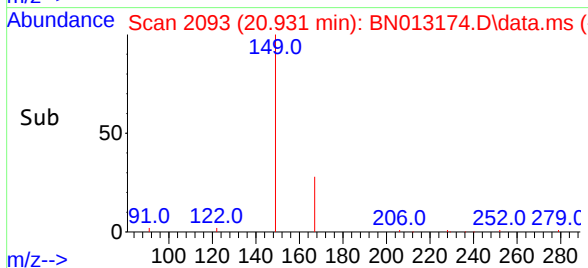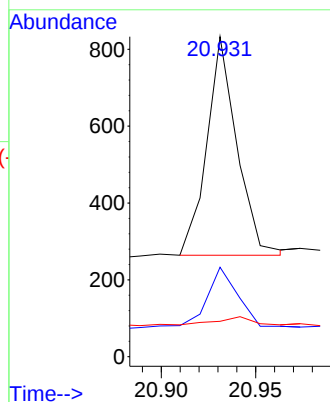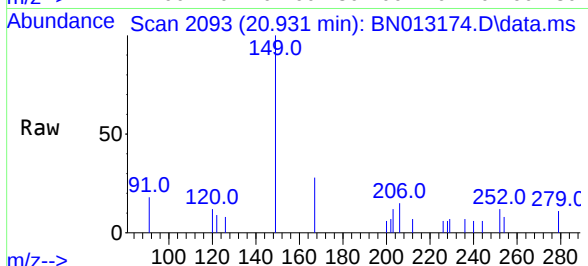

#36
 Perylene-d12
 Concen: 0.40 ng
 RT: 23.106 min Scan# 2436
 Delta R.T. 0.003 min
 Lab File: BN013174.D
 Acq: 16 Dec 2020 20:20

Tgt Ion:264 Resp: 3057

Ion	Ratio	Lower	Upper
264	100		
260	27.8	19.8	29.6
265	94.0	51.4	77.0#

