

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN121620\
 Data File : BN013176.D
 Acq On : 16 Dec 2020 21:32
 Operator : CG/JU
 Sample : L4960-03RE
 Misc :
 ALS Vial : 29 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 MW-5RE

Quant Time: Dec 17 03:08:10 2020
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\8270-SIM-BN121620.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Tue Dec 15 16:49:20 2020
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.346	152	882	0.40	ng	0.00
7) Naphthalene-d8	10.099	136	3502	0.40	ng	#-0.01
13) Acenaphthene-d10	14.004	164	4744	0.40	ng	-0.01
19) Phenanthrene-d10	16.763	188	5158	0.40	ng	#-0.01
29) Chrysene-d12	21.003	240	5296	0.40	ng	# 0.00
36) Perylene-d12	23.093	264	5187	0.40	ng	0.00
System Monitoring Compounds						
4) 2-Fluorophenol	4.970	112	386	0.11	ng	0.00
5) Phenol-d6	6.541	99	225	0.06	ng	-0.02
8) Nitrobenzene-d5	8.490	82	1087	0.30	ng	-0.03
11) 2-Methylnaphthalene-d10	11.697	152	2007	0.33	ng	-0.03
14) 2,4,6-Tribromophenol	15.513	330	266	0.09	ng	-0.03
15) 2-Fluorobiphenyl	12.608	172	3209	0.16	ng	-0.03
27) Fluoranthene-d10	18.818	212	6139	0.36	ng	0.00
31) Terphenyl-d14	19.439	244	6584	0.49	ng	0.00
Target Compounds						Qvalue
3) n-Nitrosodimethylamine	3.271	42	470	0.18	ng	# 16
6) bis(2-Chloroethyl)ether	6.814	93	200	0.09	ng	# 1
9) Naphthalene	10.150	128	10940	1.02	ng	# 1
17) Acenaphthene	14.067	154	873	0.06	ng	# 81
18) Fluorene	15.069	166	1089	0.05	ng	96
20) 4,6-Dinitro-2-methylph...	15.196	198	16	0.20	ng	# 1
23) Atrazine	16.033	200	282	0.09	ng	# 1
25) Phenanthrene	16.811	178	486	0.03	ng	# 89
28) Fluoranthene	18.848	202	455	0.02	ng	# 75
30) Pyrene	19.215	202	1187	0.06	ng	# 86
34) Bis(2-ethylhexyl)phtha...	20.929	149	3252	0.08	ng	96

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN121620\
Data File : BN013176.D
Acq On : 16 Dec 2020 21:32
Operator : CG/JU
Sample : L4960-03RE
Misc :
ALS Vial : 29 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
MW-5RE

Quant Time: Dec 17 03:08:10 2020
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\8270-SIM-BN121620.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Dec 15 16:49:20 2020
Response via : Initial Calibration




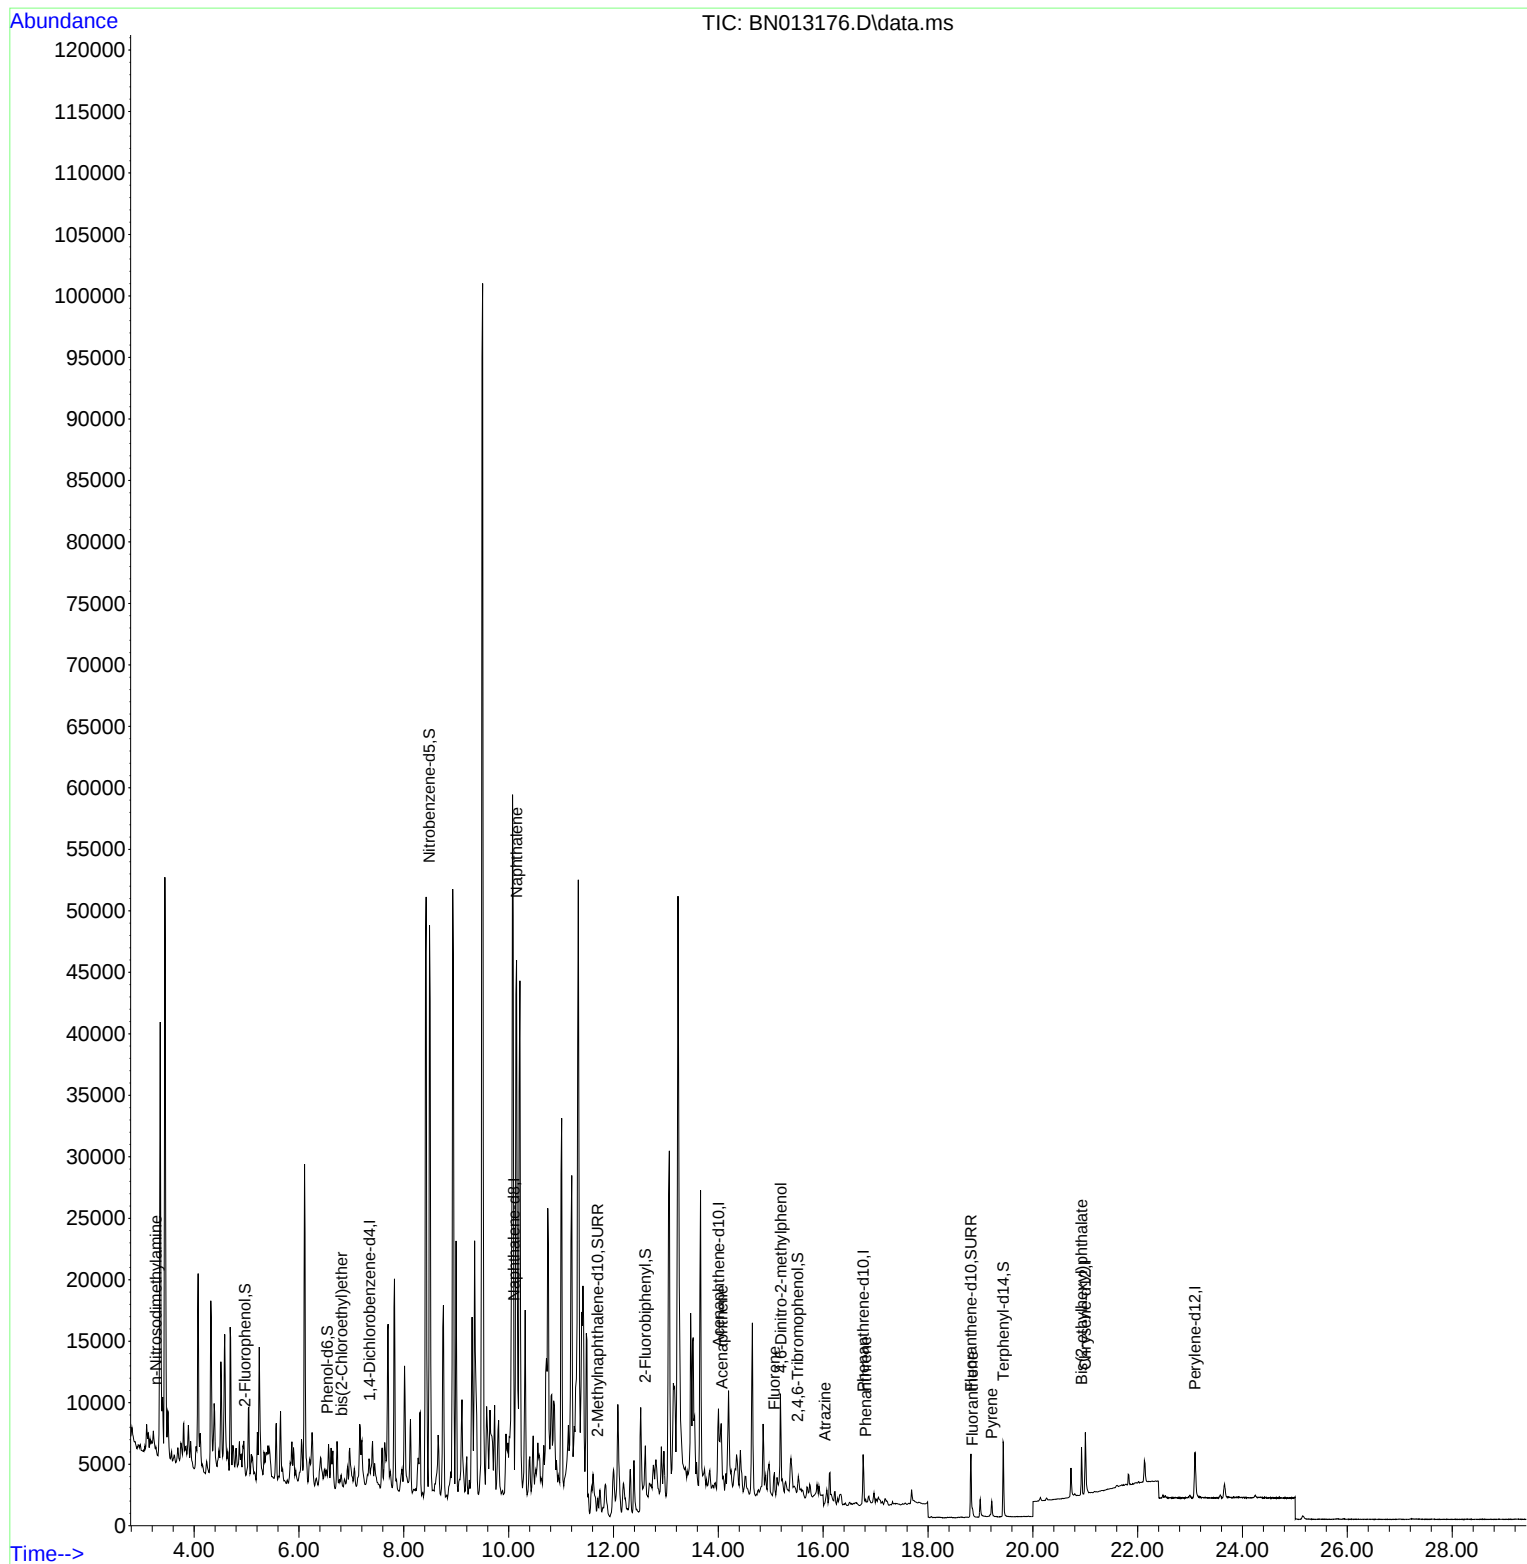




#1
1,4-Dichlorobenzene-d4
Concen: 0.40 ng
RT: 7.346 min Scan# 567
Delta R.T. -0.008 min
Lab File: BN013176.D
Acq: 16 Dec 2020 21:32




Instrument :
BNA_N
ClientSampled :
MW-5RE

Tgt Ion:152 Resp: 882
Ion Ratio Lower Upper
152 100
150 147.3 116.6 174.8
115 69.5 52.9 79.3

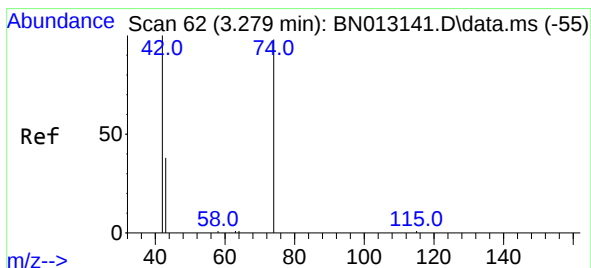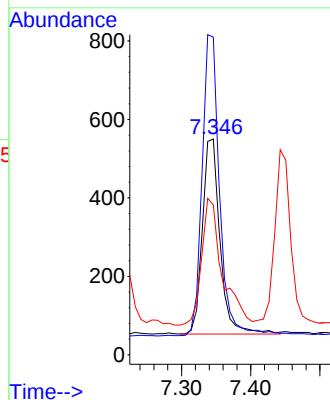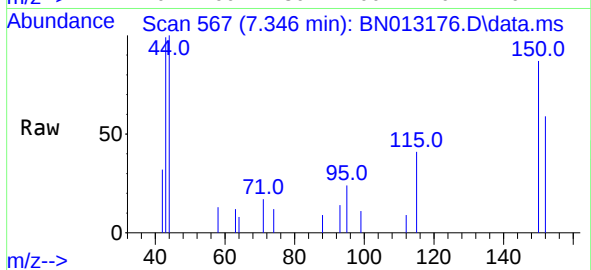

#3
n-Nitrosodimethylamine
Concen: 0.18 ng
RT: 3.271 min Scan# 61
Delta R.T. -0.008 min
Lab File: BN013176.D
Acq: 16 Dec 2020 21:32

Tgt Ion: 42 Resp: 470
Ion Ratio Lower Upper
42 100
74 3.0 64.4 96.6#
44 0.0 2.8 4.2#

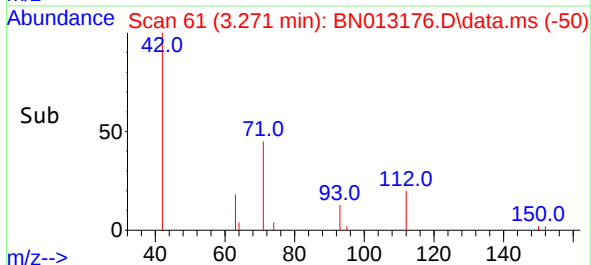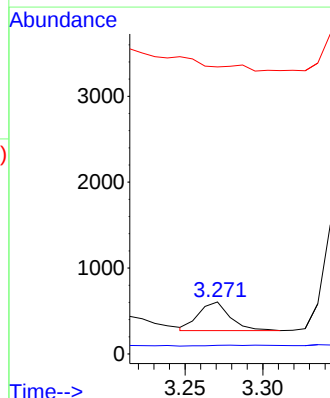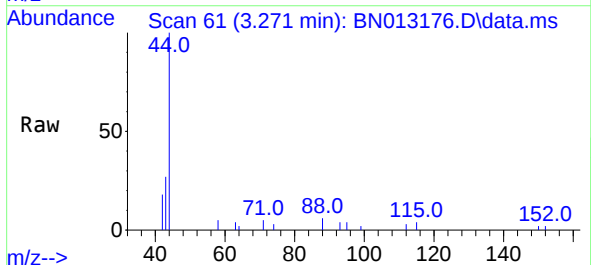






#4
2-Fluorophenol
Concen: 0.11 ng
RT: 4.970 min Scan# 272
Delta R.T. -0.000 min
Lab File: BN013176.D
Acq: 16 Dec 2020 21:32

Instrument :
BNA_N
ClientSampleId :
MW-5RE

Tgt Ion:112 Resp: 386




Ion	Ratio	Lower	Upper
112	100		
64	60.4	49.5	74.3
63	42.7	32.0	48.0

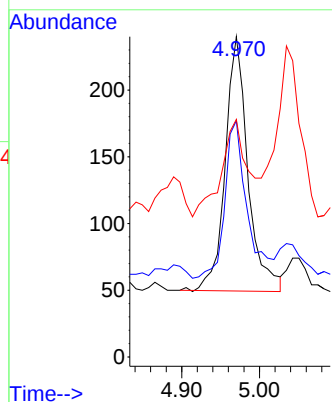


#5
Phenol-d6
Concen: 0.06 ng
RT: 6.541 min Scan# 467
Delta R.T. -0.016 min
Lab File: BN013176.D
Acq: 16 Dec 2020 21:32

Tgt Ion: 99 Resp: 225

Ion	Ratio	Lower	Upper
99	100		
42	0.0	22.4	33.6#
71	439.6	37.8	56.6#


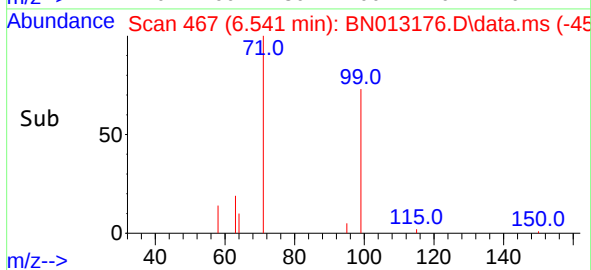
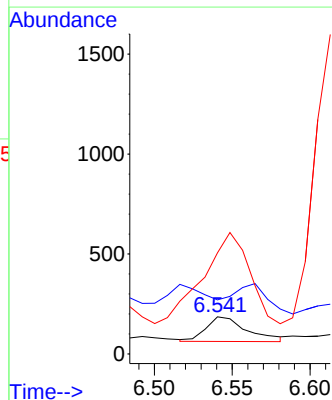





#6
bis(2-Chloroethyl)ether
Concen: 0.09 ng
RT: 6.814 min Scan# 501
Delta R.T. 0.008 min
Lab File: BN013176.D
Acq: 16 Dec 2020 21:32




Instrument :
BNA_N
ClientSampleId :
MW-5RE


Tgt Ion: 93 Resp: 200
Ion Ratio Lower Upper
93 100
63 0.0 63.1 94.7#
95 169.5 26.1 39.1#

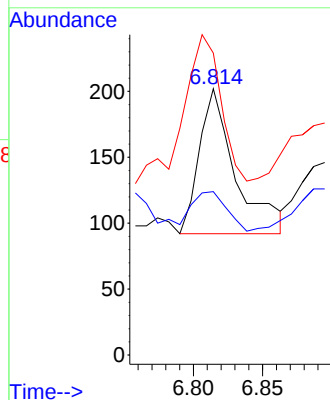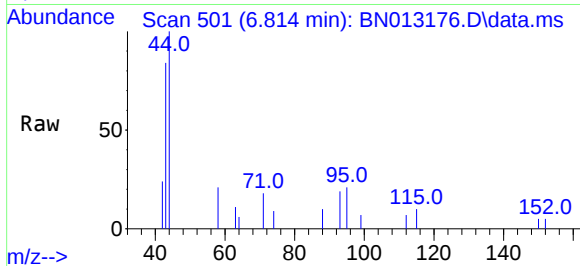

#7
Naphthalene-d8
Concen: 0.40 ng
RT: 10.099 min Scan# 828
Delta R.T. -0.013 min
Lab File: BN013176.D
Acq: 16 Dec 2020 21:32

Tgt Ion: 136 Resp: 3502
Ion Ratio Lower Upper
136 100
137 13.7 10.6 15.8
54 12.8 8.6 12.8
68 10.3 5.7 8.5#


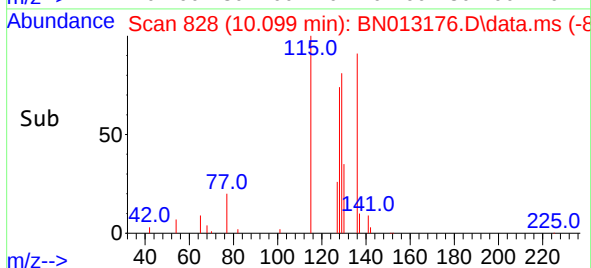
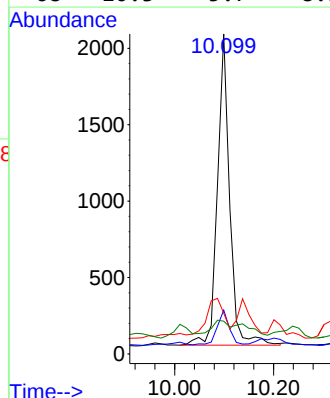
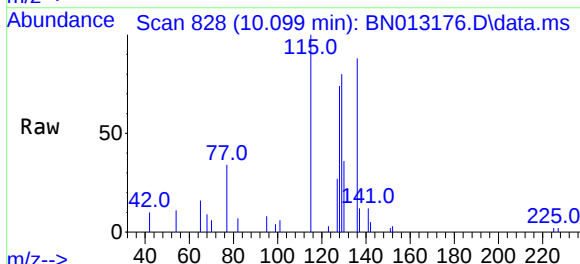




#8
Nitrobenzene-d5
Concen: 0.30 ng
RT: 8.490 min Scan# 701
Delta R.T. -0.025 min
Lab File: BN013176.D
Acq: 16 Dec 2020 21:32




Instrument :
BNA_N
ClientSampleId :
MW-5RE


Tgt Ion: 82 Resp: 1087
Ion Ratio Lower Upper
82 100
128 393.1 30.6 46.0#
54 89.2 48.3 72.5#

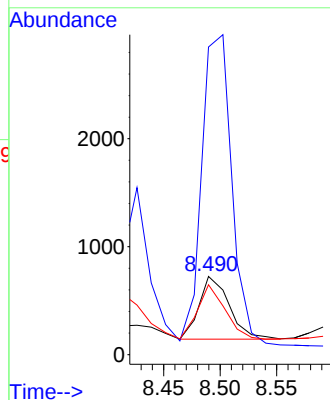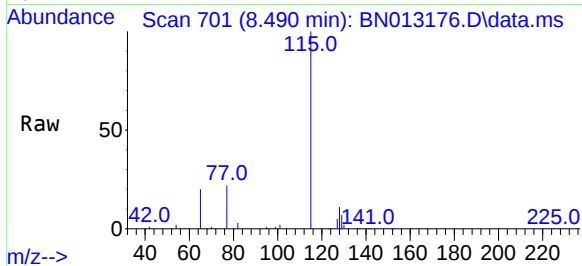

#9
Naphthalene
Concen: 1.02 ng
RT: 10.150 min Scan# 832
Delta R.T. -0.013 min
Lab File: BN013176.D
Acq: 16 Dec 2020 21:32

Tgt Ion: 128 Resp: 10940
Ion Ratio Lower Upper
128 100
129 95.6 9.8 14.8#
127 38.5 12.2 18.4#


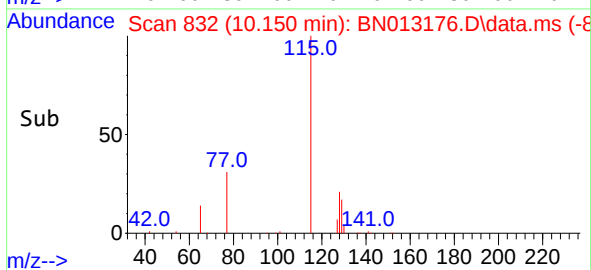
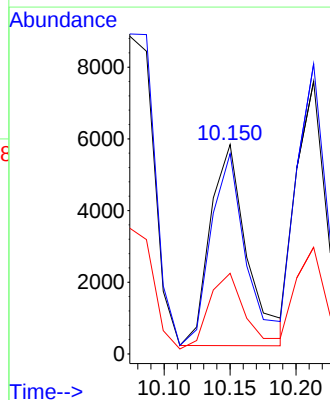
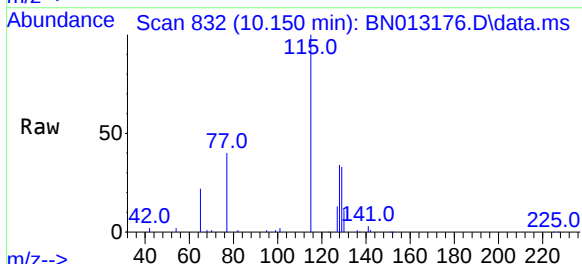


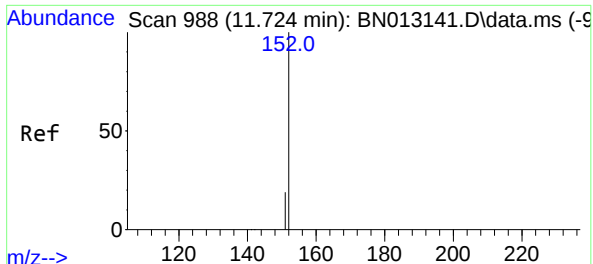

#11
2-Methylnaphthalene-d10
Concen: 0.33 ng
RT: 11.697 min Scan# 982
Delta R.T. -0.027 min
Lab File: BN013176.D
Acq: 16 Dec 2020 21:32




Instrument :
BNA_N
ClientSampleId :
MW-5RE


Tgt Ion:152 Resp: 2007
Ion Ratio Lower Upper
152 100
151 22.8 16.7 25.1

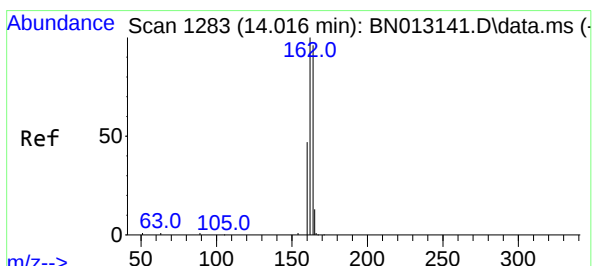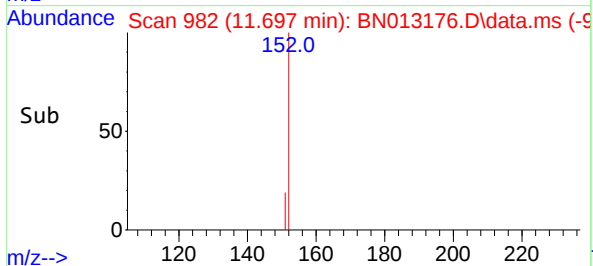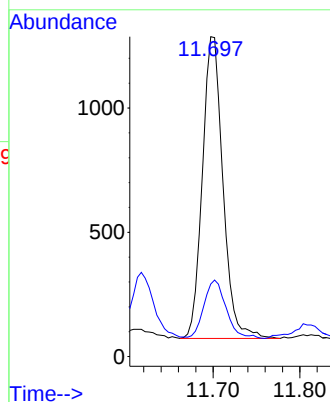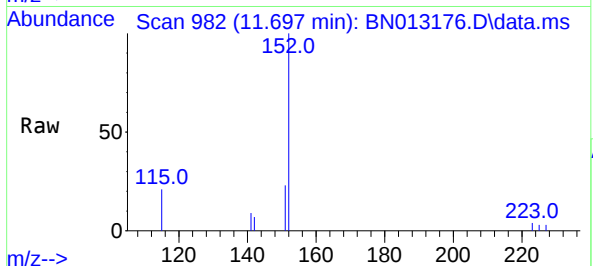

#13
Acenaphthene-d10
Concen: 0.40 ng
RT: 14.004 min Scan# 1282
Delta R.T. -0.012 min
Lab File: BN013176.D
Acq: 16 Dec 2020 21:32

Tgt Ion:164 Resp: 4744
Ion Ratio Lower Upper
164 100
162 88.2 80.6 120.8
160 40.2 39.5 59.3


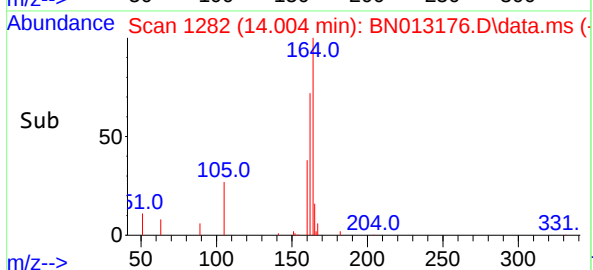
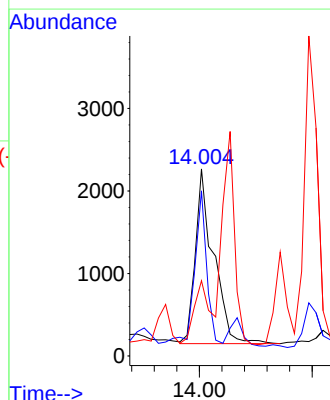
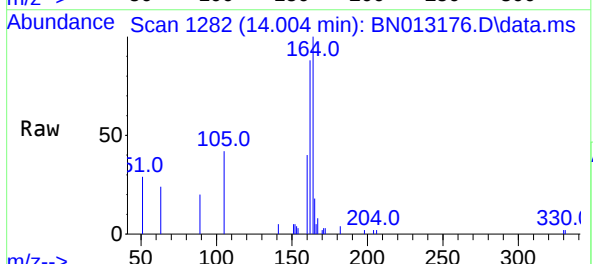




#14
2,4,6-Tribromophenol
Concen: 0.09 ng
RT: 15.513 min Scan# 1401
Delta R.T. -0.025 min
Lab File: BN013176.D
Acq: 16 Dec 2020 21:32




Instrument :
BNA_N
ClientSampleId :
MW-5RE


Tgt Ion: 330 Resp: 266
Ion Ratio Lower Upper
330 100
332 0.0 0.0 0.0
141 68.8 34.4 51.6#

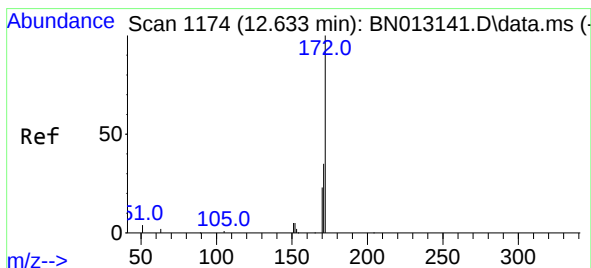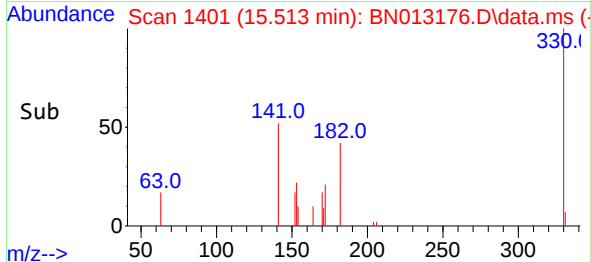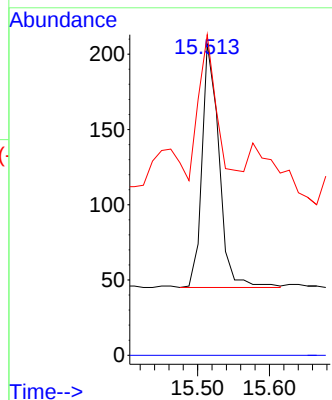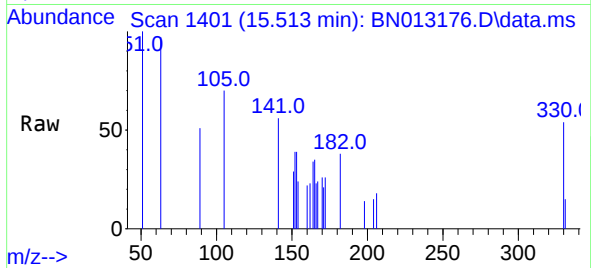

#15
2-Fluorobiphenyl
Concen: 0.16 ng
RT: 12.608 min Scan# 1172
Delta R.T. -0.025 min
Lab File: BN013176.D
Acq: 16 Dec 2020 21:32

Tgt Ion: 172 Resp: 3209
Ion Ratio Lower Upper
172 100
171 37.2 28.2 42.4
170 24.9 20.0 30.0


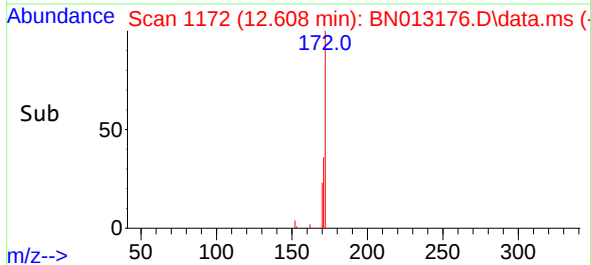
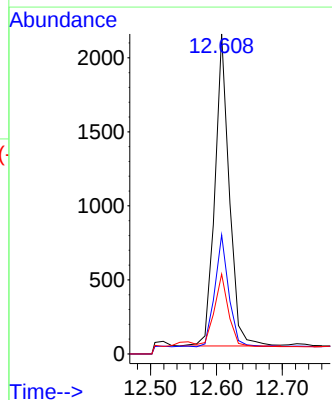
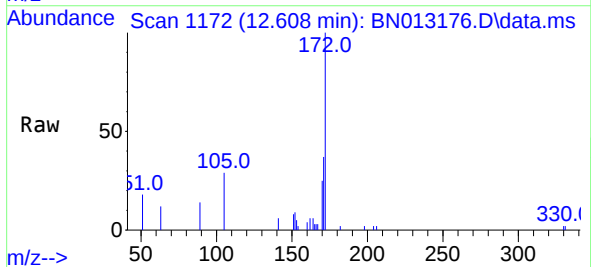




#17
Acenaphthene
Concen: 0.06 ng
RT: 14.067 min Scan# 1287
Delta R.T. -0.013 min
Lab File: BN013176.D
Acq: 16 Dec 2020 21:32




Instrument :
BNA_N
ClientSampleId :
MW-5RE


Tgt Ion:154 Resp: 873
Ion Ratio Lower Upper
154 100
153 129.4 83.6 125.4#
152 62.2 43.9 65.9

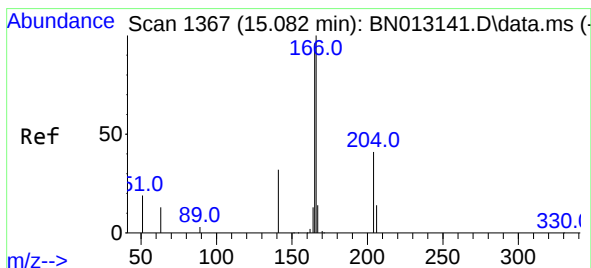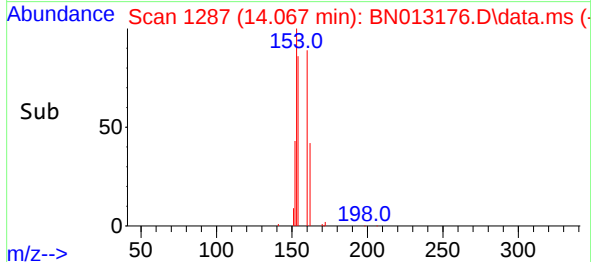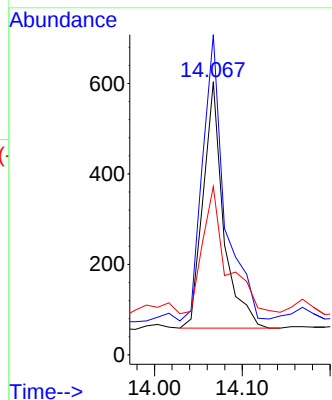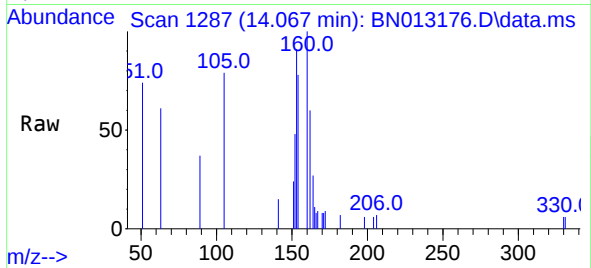

#18
Fluorene
Concen: 0.05 ng
RT: 15.069 min Scan# 1366
Delta R.T. -0.013 min
Lab File: BN013176.D
Acq: 16 Dec 2020 21:32

Tgt Ion:166 Resp: 1089
Ion Ratio Lower Upper
166 100
165 94.4 78.6 118.0
167 14.1 10.7 16.1


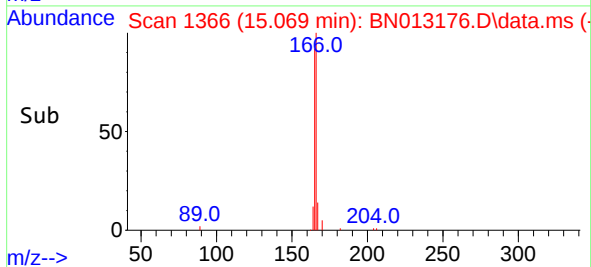
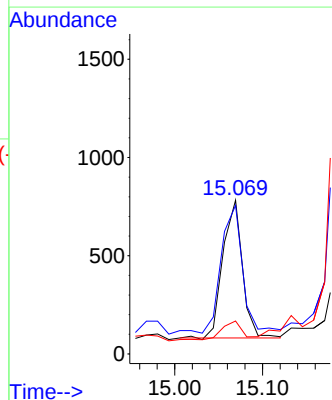
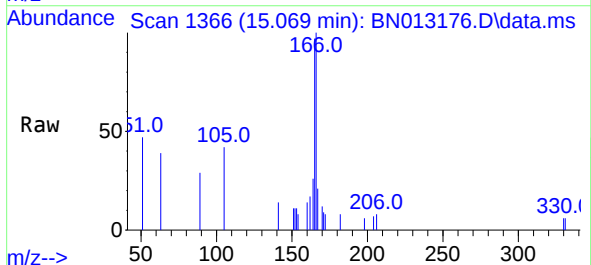




#19
Phenanthrene-d10
Concen: 0.40 ng
RT: 16.763 min Scan# 1502
Delta R.T. -0.012 min
Lab File: BN013176.D
Acq: 16 Dec 2020 21:32




Instrument :
BNA_N
ClientSampleId :
MW-5RE


Tgt Ion:188	Resp:	5158
Ion Ratio	Lower	Upper
188	100	
94	0.0	0.0
80	12.3	5.0

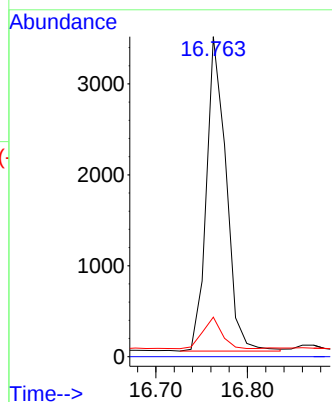

#20
4,6-Dinitro-2-methylphenol
Concen: 0.20 ng
RT: 15.196 min Scan# 1376
Delta R.T. -0.038 min
Lab File: BN013176.D
Acq: 16 Dec 2020 21:32

Tgt Ion:198	Resp:	16
Ion Ratio	Lower	Upper
198	100	
51	627.8	43.5
105	687.0	27.2


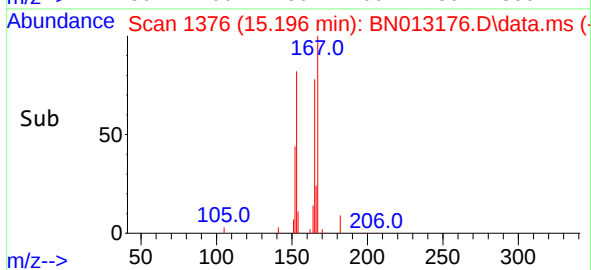
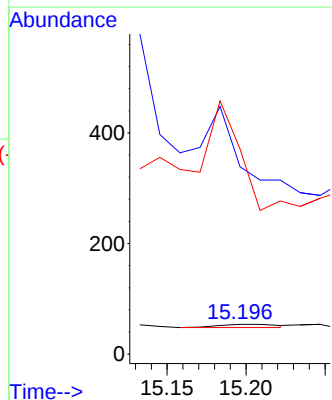





#23
Atrazine
Concen: 0.09 ng
RT: 16.033 min Scan# 1442
Delta R.T. -0.244 min
Lab File: BN013176.D
Acq: 16 Dec 2020 21:32




Instrument :
BNA_N
ClientSampleId :
MW-5RE


Tgt Ion:200 Resp: 282
Ion Ratio Lower Upper
200 100
173 129.8 22.8 34.2#
215 89.5 38.1 57.1#

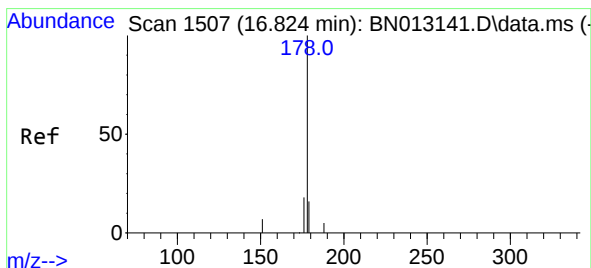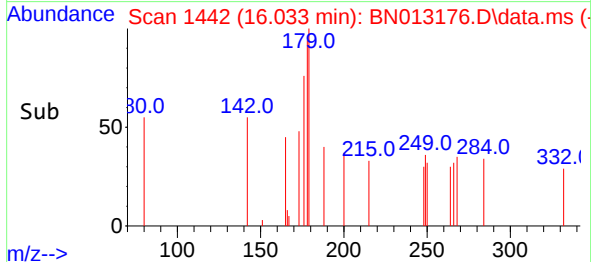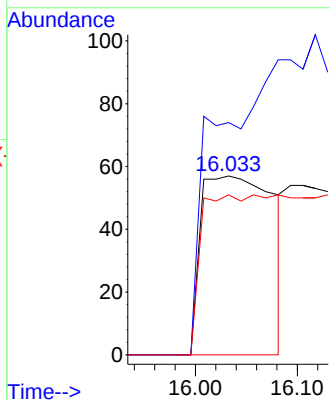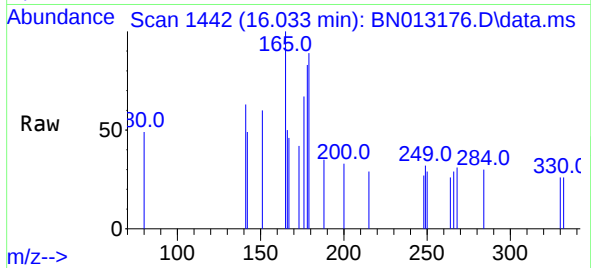

#25
Phenanthrene
Concen: 0.03 ng
RT: 16.811 min Scan# 1506
Delta R.T. -0.013 min
Lab File: BN013176.D
Acq: 16 Dec 2020 21:32

Tgt Ion:178 Resp: 486
Ion Ratio Lower Upper
178 100
176 15.2 14.8 22.2
179 8.6 12.4 18.6#


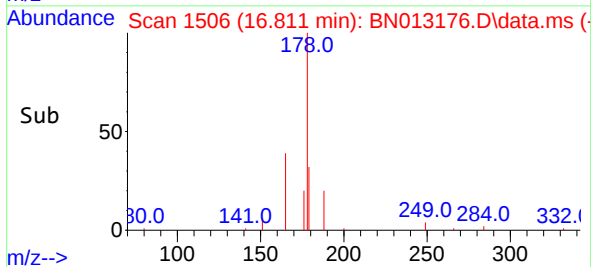
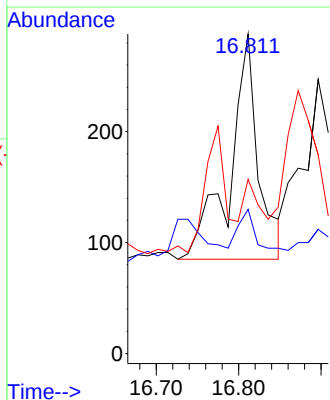
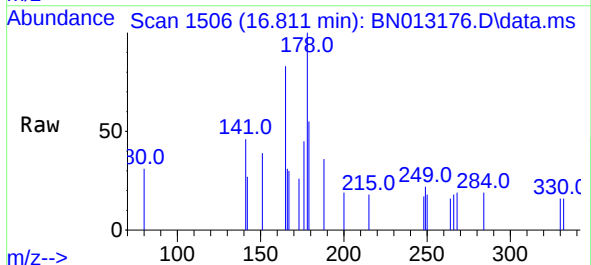




#27
Fluoranthene-d10
Concen: 0.36 ng
RT: 18.818 min Scan# 1768
Delta R.T. -0.008 min
Lab File: BN013176.D
Acq: 16 Dec 2020 21:32




Instrument :
BNA_N
ClientSampleId :
MW-5RE


Tgt Ion:212 Resp: 6139
Ion Ratio Lower Upper
212 100
106 10.9 6.8 10.2#
104 6.4 4.1 6.1#

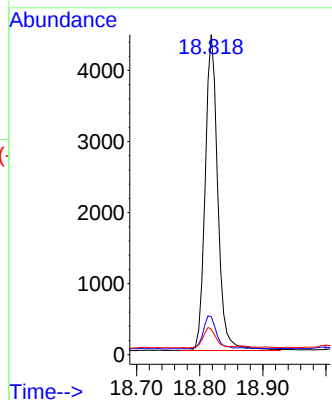

#28
Fluoranthene
Concen: 0.02 ng
RT: 18.848 min Scan# 1774
Delta R.T. -0.008 min
Lab File: BN013176.D
Acq: 16 Dec 2020 21:32

Tgt Ion:202 Resp: 455
Ion Ratio Lower Upper
202 100
101 0.0 5.8 8.6#
203 29.0 13.7 20.5#


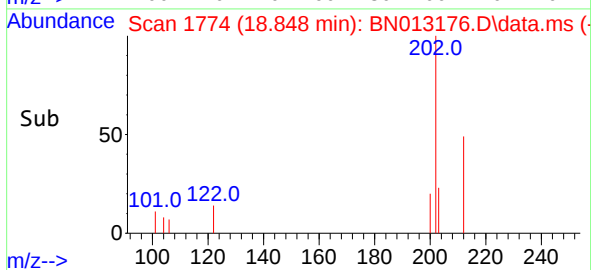
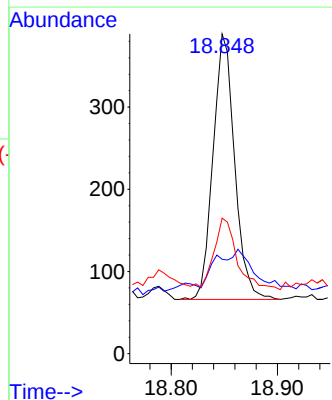





#29
Chrysene-d12
Concen: 0.40 ng
RT: 21.003 min Scan# 2101
Delta R.T. -0.003 min
Lab File: BN013176.D
Acq: 16 Dec 2020 21:32




Instrument :
BNA_N
ClientSampleId :
MW-5RE


Tgt Ion:240 Resp: 5296
Ion Ratio Lower Upper
240 100
120 11.3 5.3 7.9#
236 27.8 21.8 32.8

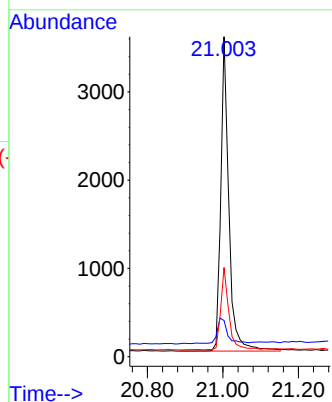

#30
Pyrene
Concen: 0.06 ng
RT: 19.215 min Scan# 1848
Delta R.T. -0.008 min
Lab File: BN013176.D
Acq: 16 Dec 2020 21:32

Tgt Ion:202 Resp: 1187
Ion Ratio Lower Upper
202 100
200 21.1 16.6 24.8
203 30.2 13.8 20.8#


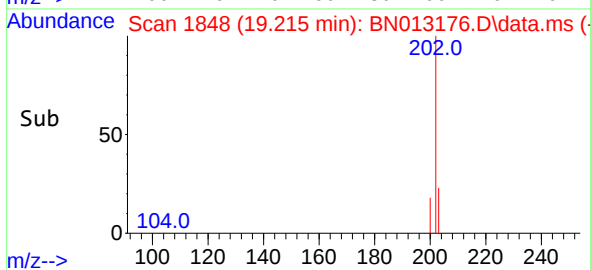
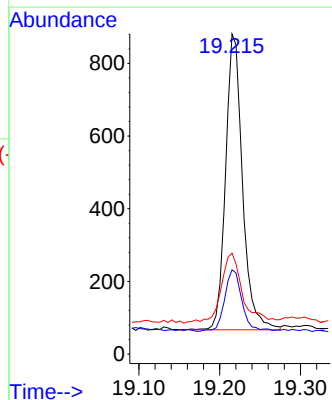





#31
 Terphenyl-d14
 Concen: 0.49 ng
 RT: 19.439 min Scan# 1893
 Delta R.T. -0.008 min
 Lab File: BN013176.D
 Acq: 16 Dec 2020 21:32




Instrument :
 BNA_N
 ClientSampleId :
 MW-5RE


Tgt Ion:244	Resp:	6584	
Ion	Ratio	Lower	Upper
244	100		
212	9.0	7.3	10.9
122	10.4	7.3	10.9

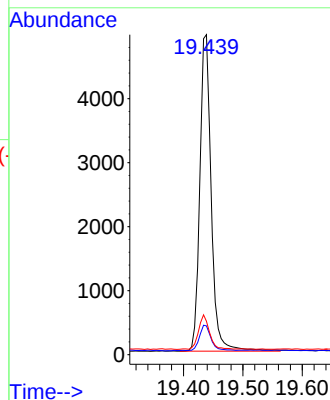

#34
 Bis(2-ethylhexyl)phthalate
 Concen: 0.08 ng
 RT: 20.929 min Scan# 2094
 Delta R.T. -0.002 min
 Lab File: BN013176.D
 Acq: 16 Dec 2020 21:32

Tgt Ion:149	Resp:	3252	
Ion	Ratio	Lower	Upper
149	100		
167	26.5	23.2	34.8
279	4.7	3.9	5.9

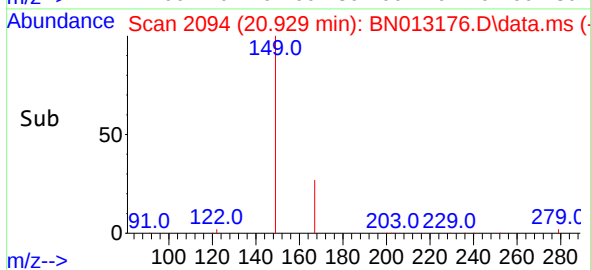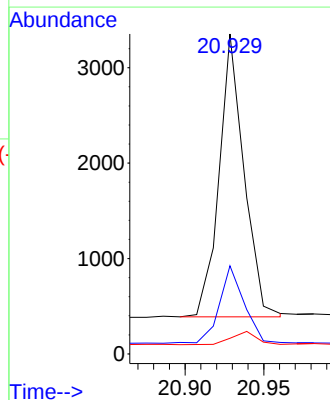

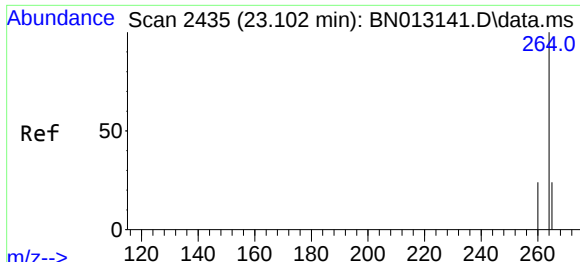

#36
Perylene-d12
Concen: 0.40 ng
RT: 23.093 min Scan# 2434
Delta R.T. -0.010 min
Lab File: BN013176.D
Acq: 16 Dec 2020 21:32

Instrument :
BNA_N
ClientSampleId :
MW-5RE

Tgt Ion:264	Resp:	5187
Ion	Ratio	Lower Upper
264	100	
260	25.9	19.8 29.6
265	68.5	51.4 77.0

