
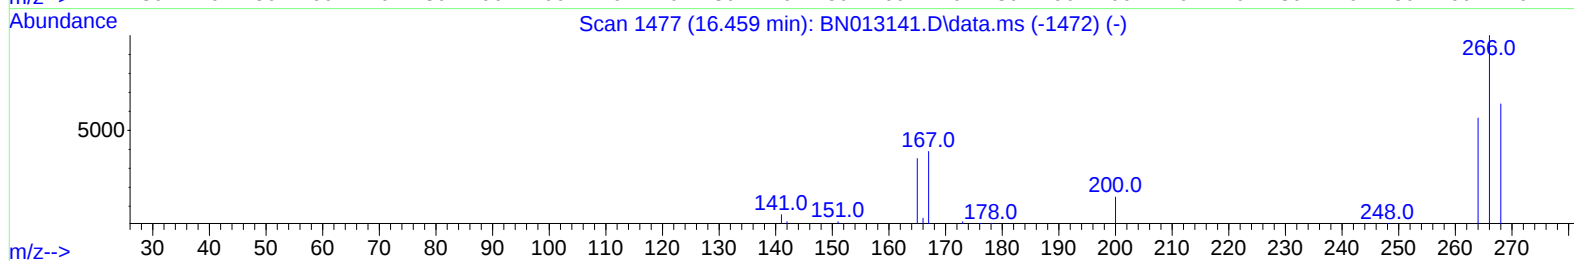
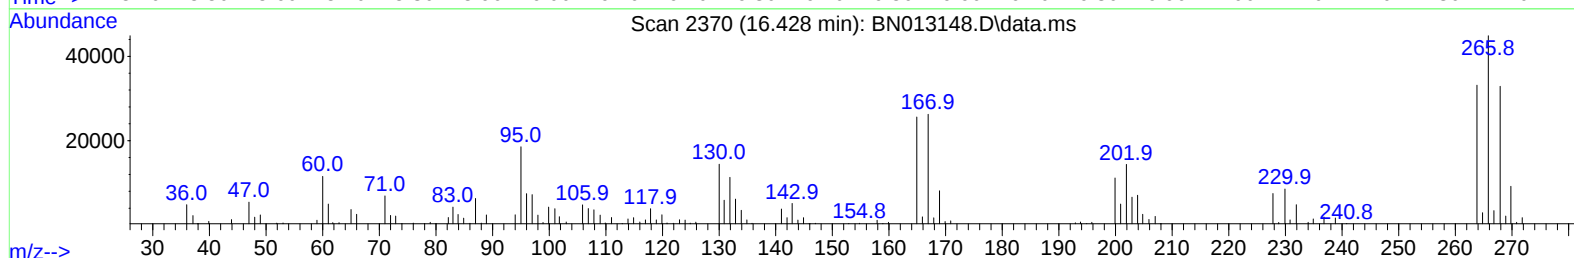


Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN121620\
Data File : BN013148.D
Acq On : 16 Dec 2020 01:35
Operator : CG/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Dec 16 06:51:10 2020
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\8270-SIM-BN121620.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Dec 15 16:49:20 2020
Response via : Initial Calibration

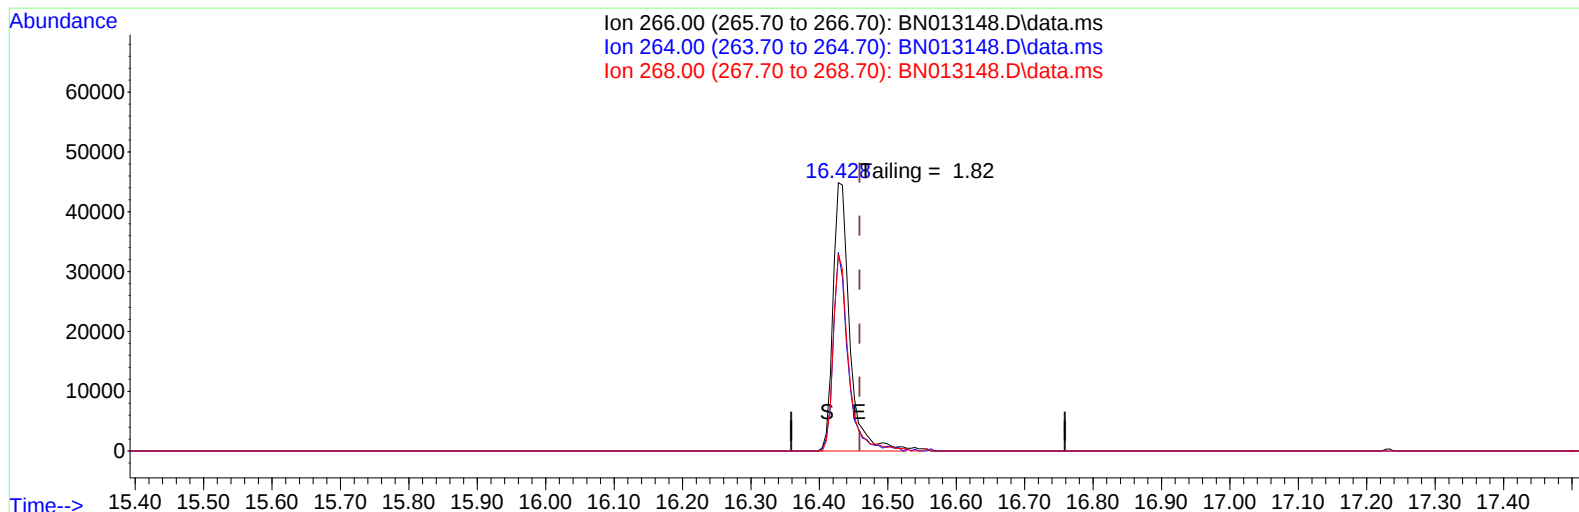

TIC: BN013148.D\data.ms

(24) Pentachlorophenol

16.428min (-0.031) 0.00 ng

response 73744

Ion	Exp%	Act%
266.00	100.00	100.00
264.00	63.60	68.47
268.00	64.40	70.10
0.00	0.00	0.00