

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN121620\
 Data File : BN013156.D
 Acq On : 16 Dec 2020 07:07
 Operator : CG/JU
 Sample : L4996-15
 Misc :
 ALS Vial : 9 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 RE132D6-20201207

Quant Time: Dec 16 08:09:20 2020
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\8270-SIM-BN121620.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Tue Dec 15 16:49:20 2020
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.354	152	735	0.40	ng	0.00
7) Naphthalene-d8	10.125	136	2560	0.40	ng	# 0.01
13) Acenaphthene-d10	14.016	164	1558	0.40	ng	0.00
19) Phenanthrene-d10	16.787	188	3390	0.40	ng	# 0.01
29) Chrysene-d12	21.003	240	3748	0.40	ng	# 0.00
36) Perylene-d12	23.100	264	4227	0.40	ng	# 0.00
System Monitoring Compounds						
4) 2-Fluorophenol	4.978	112	293	0.10	ng	0.00
5) Phenol-d6	6.557	99	176	0.06	ng	0.00
8) Nitrobenzene-d5	8.540	82	708	0.27	ng	0.03
11) 2-Methylnaphthalene-d10	11.737	152	1136	0.25	ng	0.01
14) 2,4,6-Tribromophenol	15.539	330	234	0.24	ng	0.00
15) 2-Fluorobiphenyl	12.633	172	1685	0.26	ng	0.00
27) Fluoranthene-d10	18.823	212	4102	0.37	ng	0.00
31) Terphenyl-d14	19.439	244	3647	0.38	ng	0.00
Target Compounds						Qvalue
2) 1,4-Dioxane	2.933	88	5860	4.57	ng	# 90


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN121620\
Data File : BN013156.D
Acq On : 16 Dec 2020 07:07
Operator : CG/JU
Sample : L4996-15
Misc :
ALS Vial : 9 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
RE132D6-20201207

Quant Time: Dec 16 08:09:20 2020
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\8270-SIM-BN121620.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Dec 15 16:49:20 2020
Response via : Initial Calibration

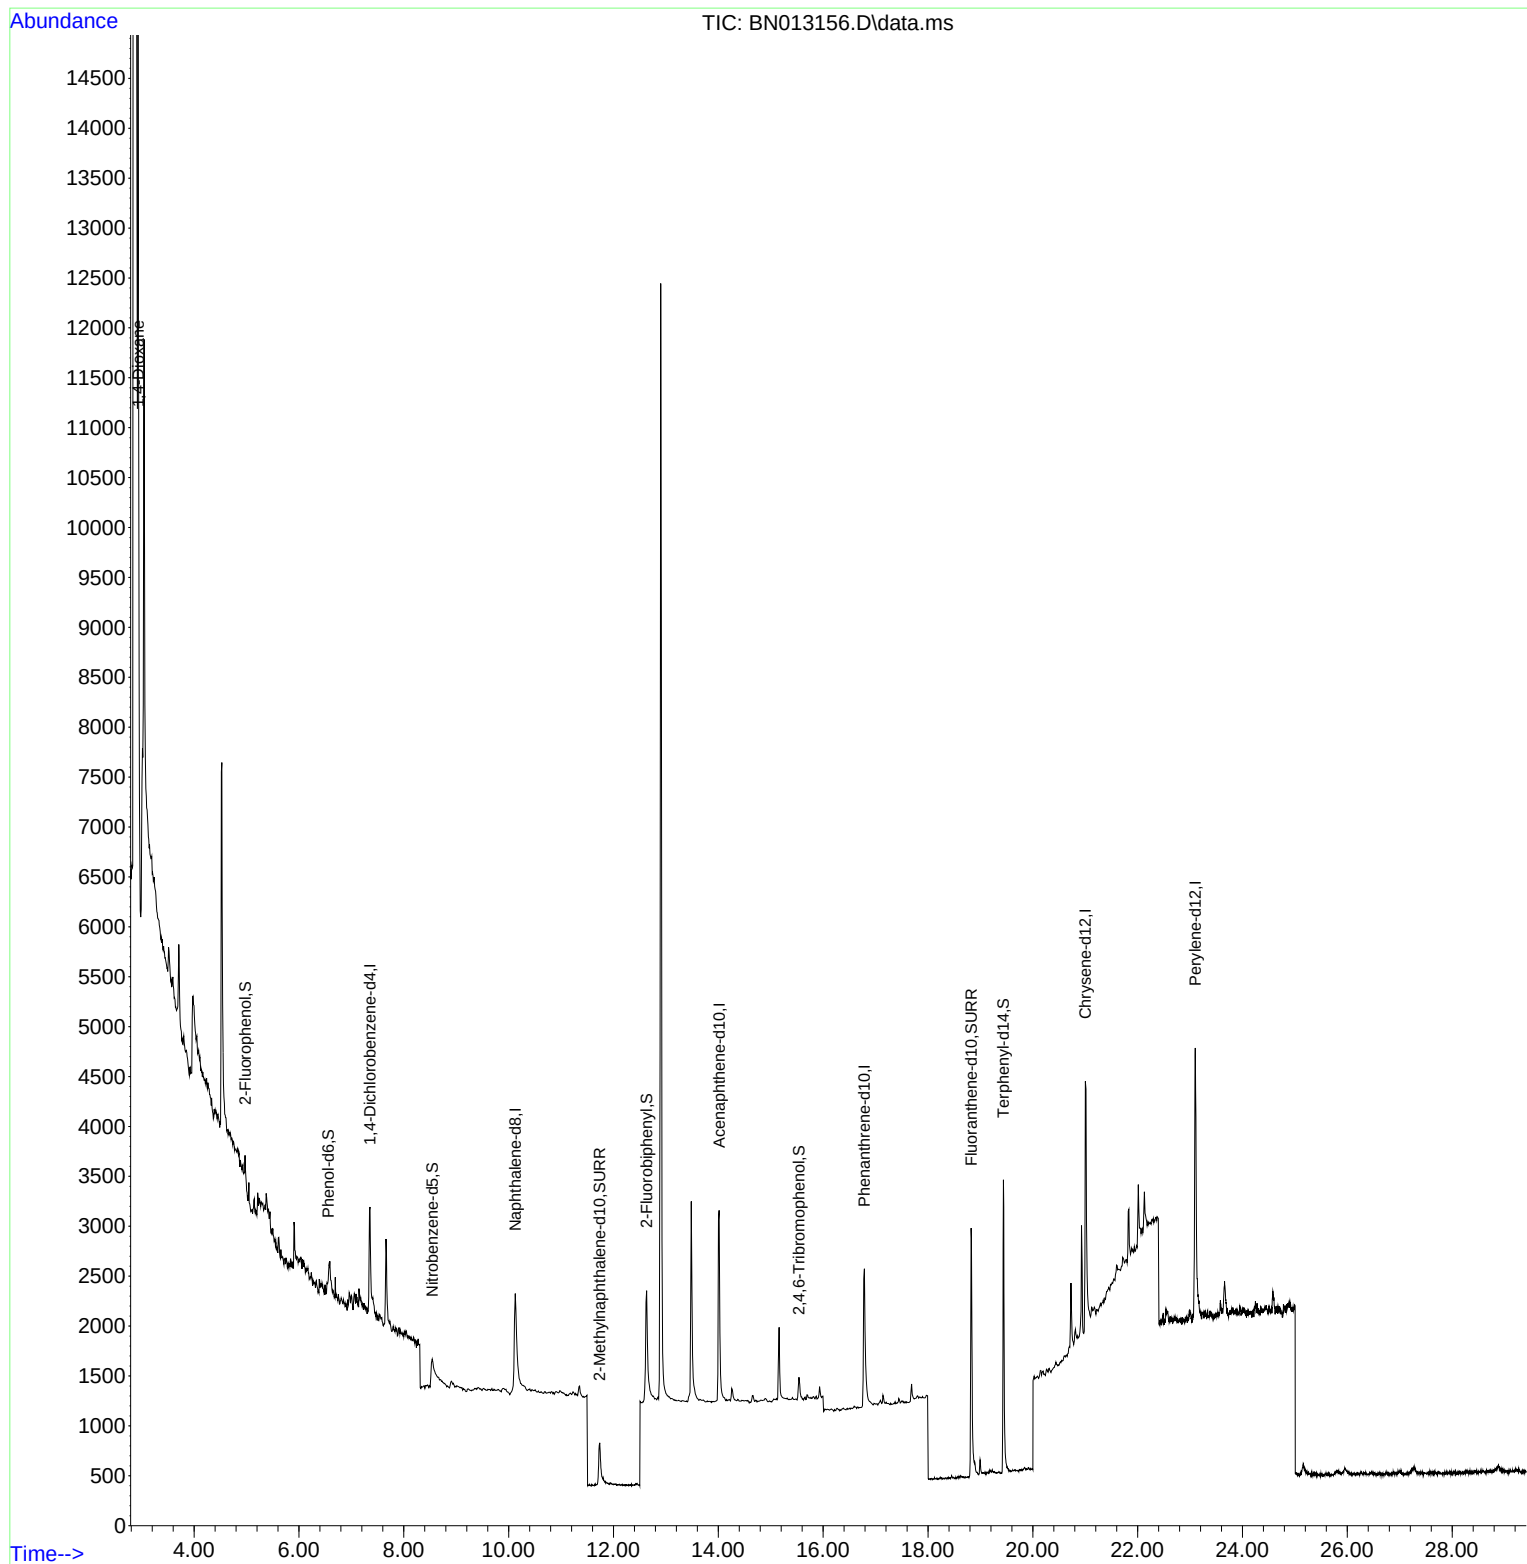




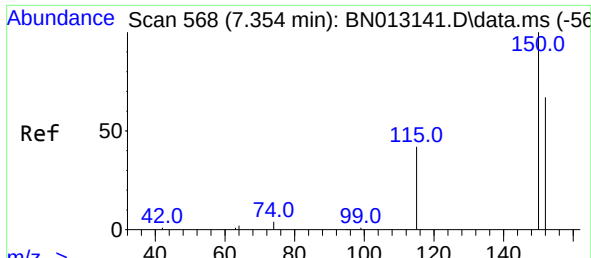


#1
1,4-Dichlorobenzene-d4
Concen: 0.40 ng
RT: 7.354 min Scan# 568
Delta R.T. -0.000 min
Lab File: BN013156.D
Acq: 16 Dec 2020 07:07

Instrument :
BNA_N
ClientSampleId :
RE132D6-20201207

Tgt Ion: 152 Resp: 735




Ion	Ratio	Lower	Upper
152	100		
150	144.3	116.6	174.8
115	75.3	52.9	79.3

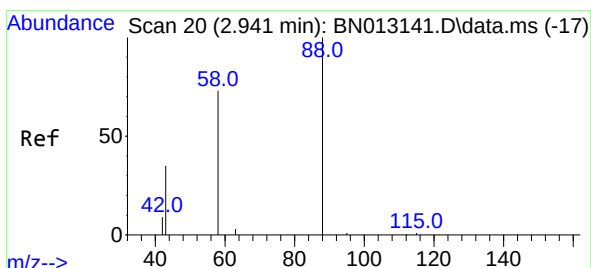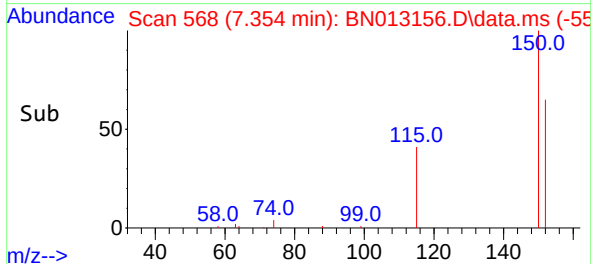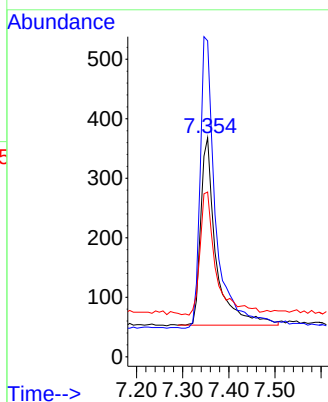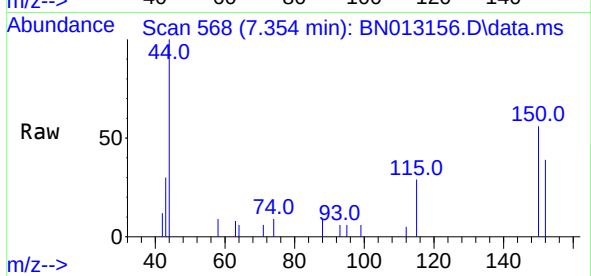


#2
1,4-Dioxane
Concen: 4.57 ng
RT: 2.933 min Scan# 19
Delta R.T. -0.008 min
Lab File: BN013156.D
Acq: 16 Dec 2020 07:07

Tgt Ion: 88 Resp: 5860

Ion	Ratio	Lower	Upper
88	100		
58	68.5	59.4	89.2
43	29.8	32.3	48.5


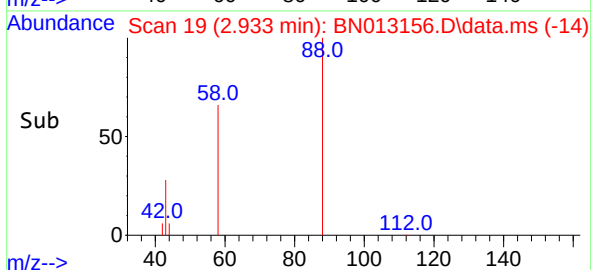
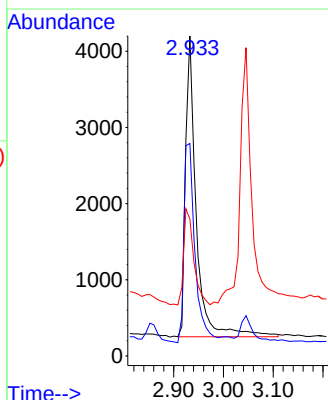
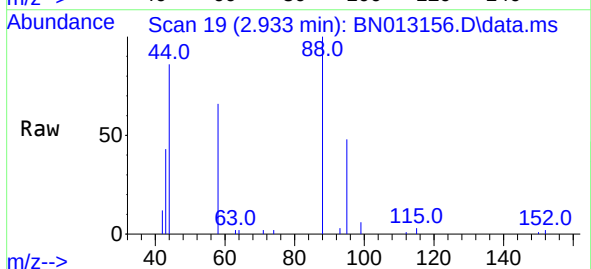




#4
2-Fluorophenol
Concen: 0.10 ng
RT: 4.978 min Scan# 273
Delta R.T. 0.008 min
Lab File: BN013156.D
Acq: 16 Dec 2020 07:07




Instrument :
BNA_N
ClientSampleId :
RE132D6-20201207


Tgt Ion:	112	Resp:	293
Ion	Ratio	Lower	Upper
112	100		
64	66.2	49.5	74.3
63	35.5	32.0	48.0

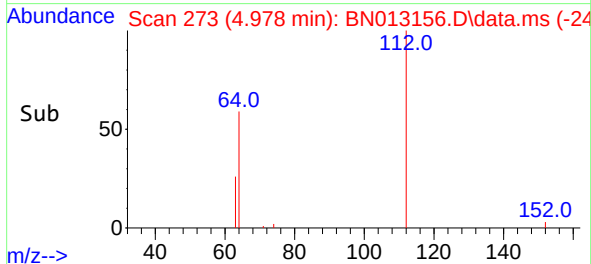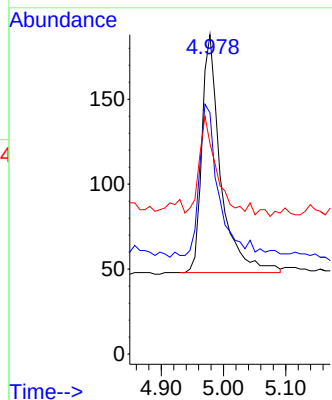

#5
Phenol-d6
Concen: 0.06 ng
RT: 6.557 min Scan# 469
Delta R.T. -0.000 min
Lab File: BN013156.D
Acq: 16 Dec 2020 07:07

Tgt Ion:	99	Resp:	176
Ion	Ratio	Lower	Upper
99	100		
42	24.4	22.4	33.6
71	44.3	37.8	56.6


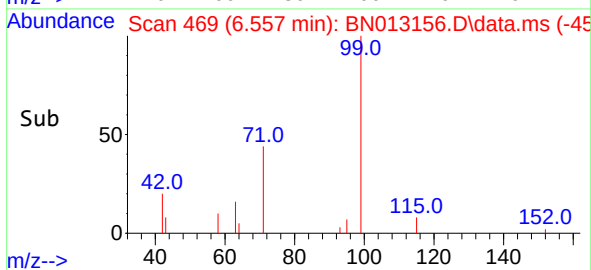
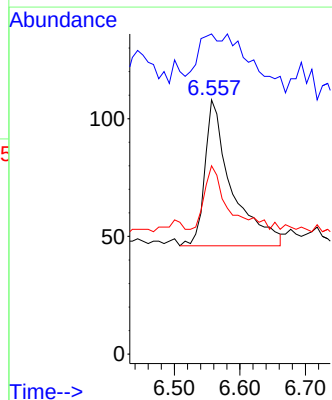
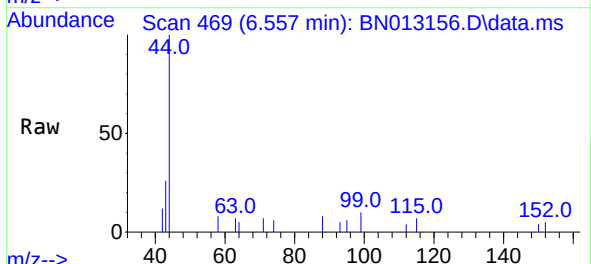




#7
Naphthalene-d8
Concen: 0.40 ng
RT: 10.125 min Scan# 830
Delta R.T. 0.013 min
Lab File: BN013156.D
Acq: 16 Dec 2020 07:07




Instrument :
BNA_N
ClientSampleId :
RE132D6-20201207


Tgt Ion:	136	Resp:	2560
Ion	Ratio	Lower	Upper
136	100		
137	17.1	10.6	15.8#
54	15.1	8.6	12.8#
68	11.4	5.7	8.5#

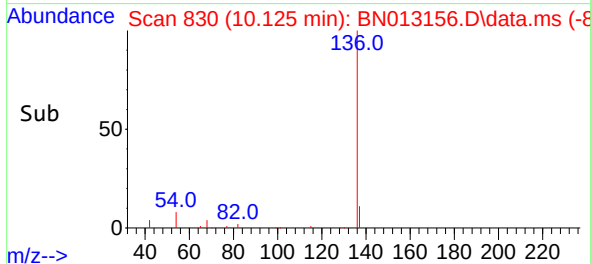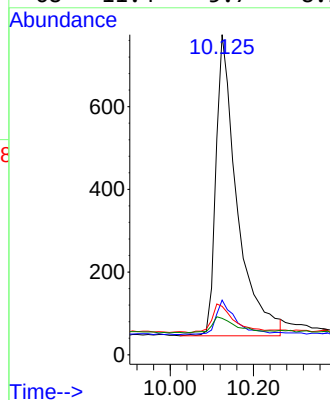

#8
Nitrobenzene-d5
Concen: 0.27 ng
RT: 8.540 min Scan# 705
Delta R.T. 0.025 min
Lab File: BN013156.D
Acq: 16 Dec 2020 07:07

Tgt Ion:	82	Resp:	708
Ion	Ratio	Lower	Upper
82	100		
128	60.3	30.6	46.0#
54	75.4	48.3	72.5#


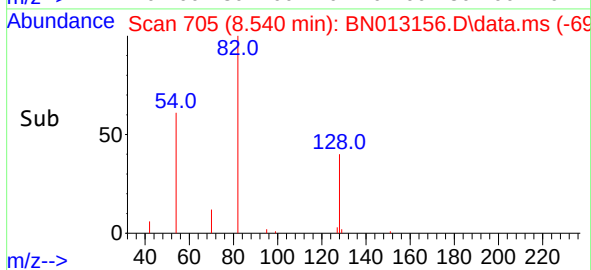
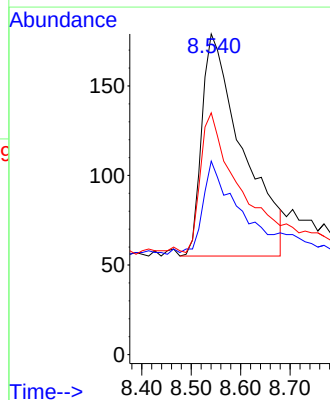
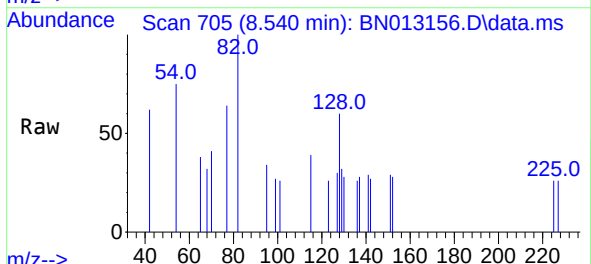


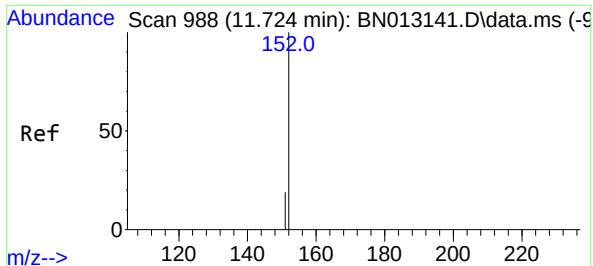

#11
2-Methylnaphthalene-d10
Concen: 0.25 ng
RT: 11.737 min Scan# 991
Delta R.T. 0.013 min
Lab File: BN013156.D
Acq: 16 Dec 2020 07:07




Instrument :
BNA_N
ClientSampleId :
RE132D6-20201207


Tgt Ion:152 Resp: 1136
Ion Ratio Lower Upper
152 100
151 25.2 16.7 25.1#

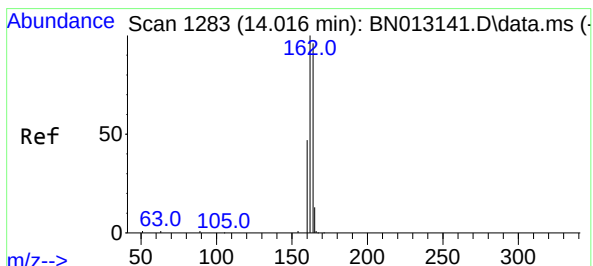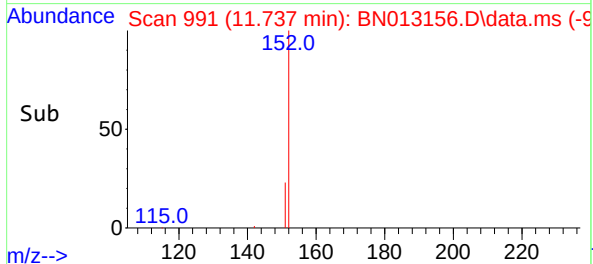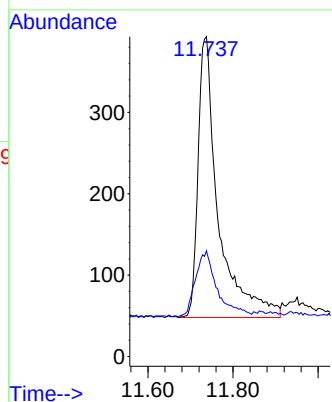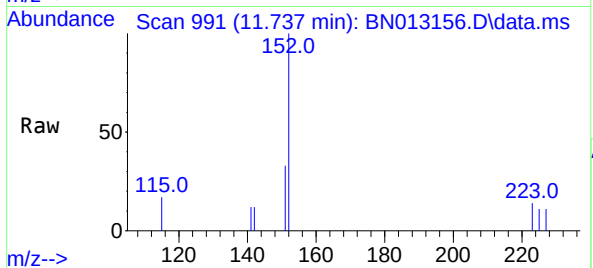

#13
Acenaphthene-d10
Concen: 0.40 ng
RT: 14.016 min Scan# 1283
Delta R.T. 0.000 min
Lab File: BN013156.D
Acq: 16 Dec 2020 07:07

Tgt Ion:164 Resp: 1558
Ion Ratio Lower Upper
164 100
162 102.6 80.6 120.8
160 49.7 39.5 59.3


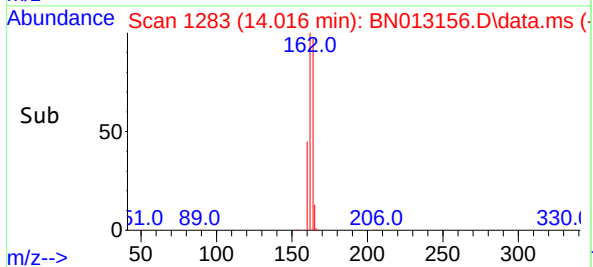
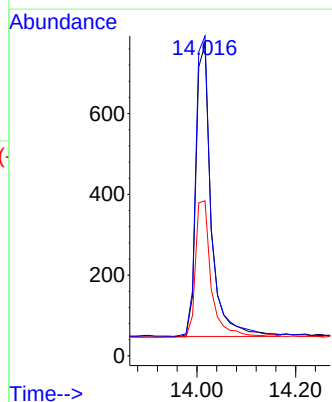
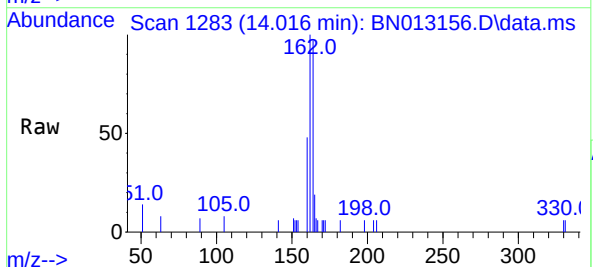




#14
2,4,6-Tribromophenol
Concen: 0.24 ng
RT: 15.539 min Scan# 1403
Delta R.T. -0.000 min
Lab File: BN013156.D
Acq: 16 Dec 2020 07:07




Instrument :
BNA_N
ClientSampleId :
RE132D6-20201207


Tgt Ion:330 Resp: 234
Ion Ratio Lower Upper
330 100
332 0.0 0.0 0.0
141 47.9 34.4 51.6

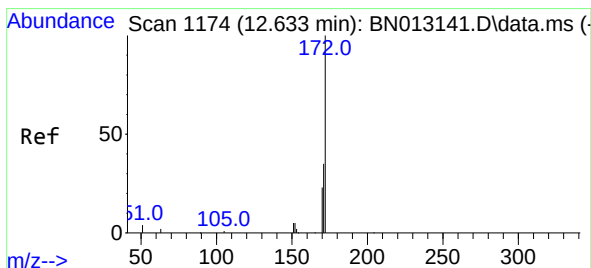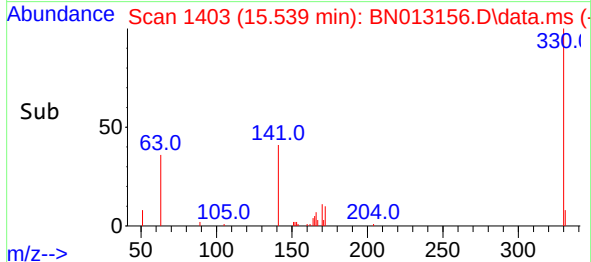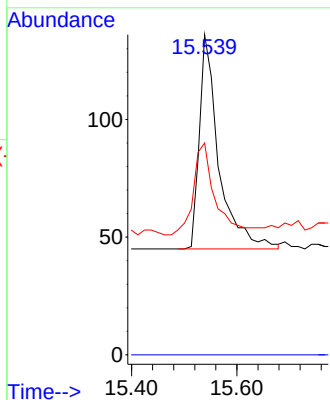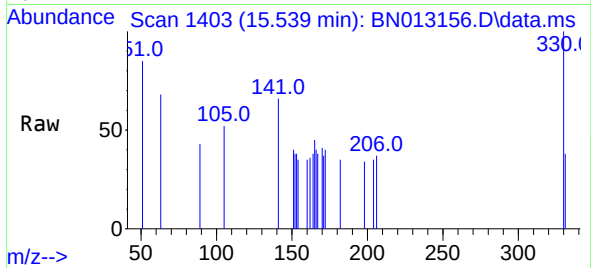

#15
2-Fluorobiphenyl
Concen: 0.26 ng
RT: 12.633 min Scan# 1174
Delta R.T. -0.000 min
Lab File: BN013156.D
Acq: 16 Dec 2020 07:07

Tgt Ion:172 Resp: 1685
Ion Ratio Lower Upper
172 100
171 40.1 28.2 42.4
170 27.0 20.0 30.0


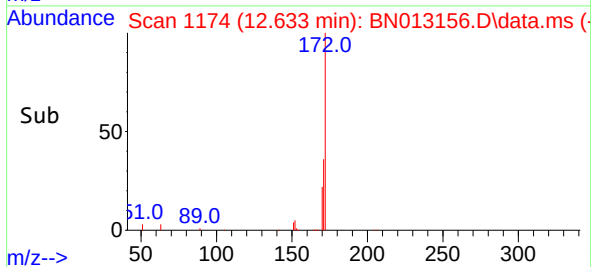
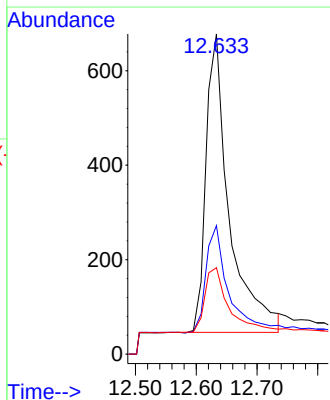
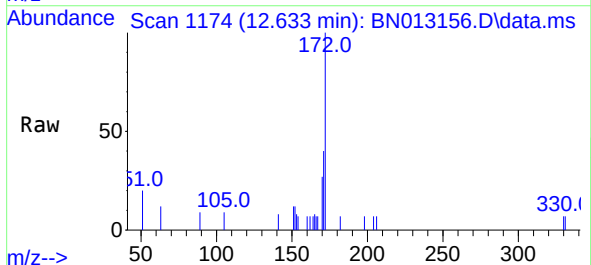




#19
Phenanthrene-d10
Concen: 0.40 ng
RT: 16.787 min Scan# 1504
Delta R.T. 0.012 min
Lab File: BN013156.D
Acq: 16 Dec 2020 07:07




Instrument :
BNA_N
ClientSampleId :
RE132D6-20201207


Tgt Ion:188 Resp: 3390
Ion Ratio Lower Upper
188 100
94 0.0 0.0 0.0
80 11.2 5.0 7.4#

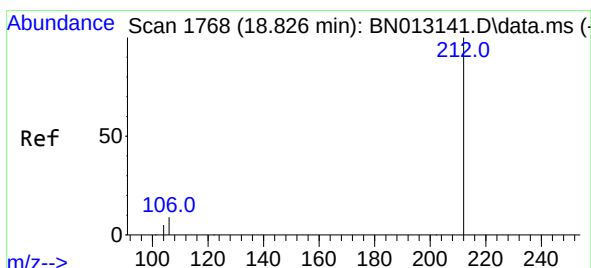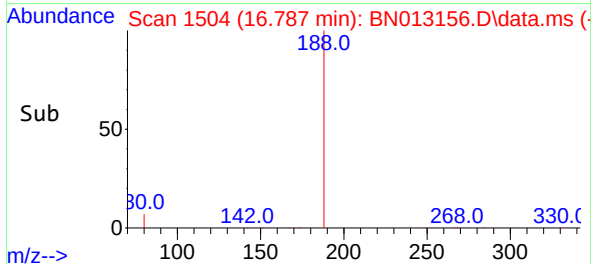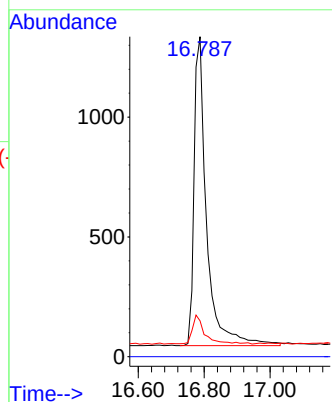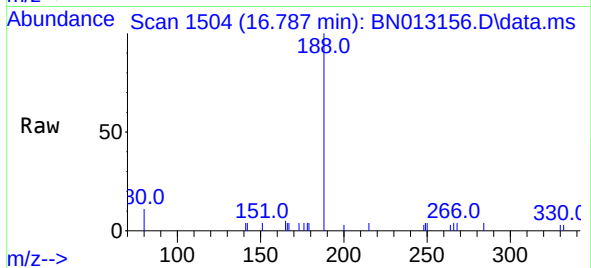

#27
Fluoranthene-d10
Concen: 0.37 ng
RT: 18.823 min Scan# 1769
Delta R.T. -0.003 min
Lab File: BN013156.D
Acq: 16 Dec 2020 07:07

Tgt Ion:212 Resp: 4102
Ion Ratio Lower Upper
212 100
106 10.6 6.8 10.2#
104 5.5 4.1 6.1


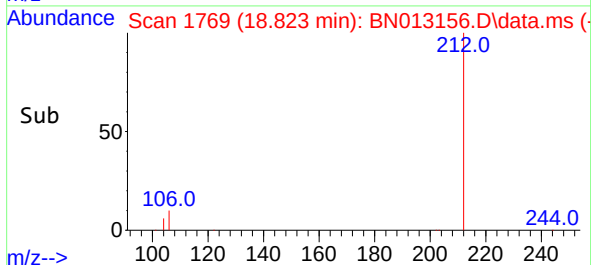
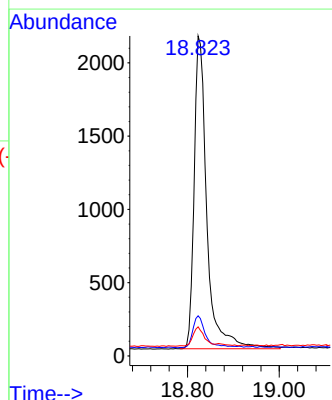
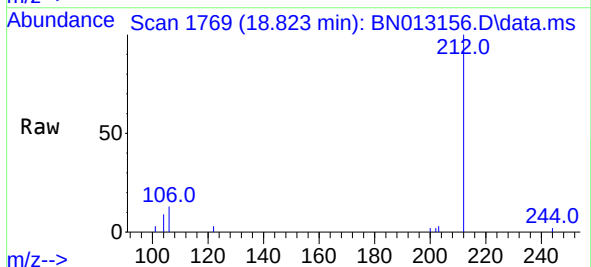




#29
Chrysene-d12
Concen: 0.40 ng
RT: 21.003 min Scan# 2101
Delta R.T. -0.003 min
Lab File: BN013156.D
Acq: 16 Dec 2020 07:07




Instrument :
BNA_N
ClientSampleId :
RE132D6-20201207


Tgt Ion:240 Resp: 3748
Ion Ratio Lower Upper
240 100
120 17.0 5.3 7.9#
236 29.4 21.8 32.8

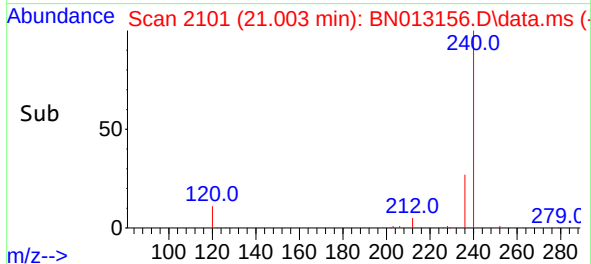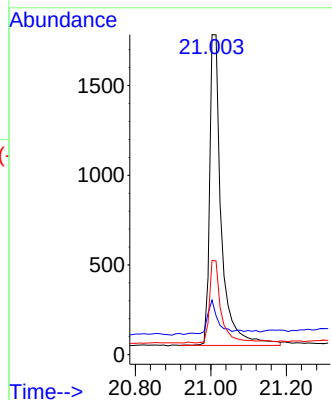

#31
Terphenyl-d14
Concen: 0.38 ng
RT: 19.439 min Scan# 1893
Delta R.T. -0.008 min
Lab File: BN013156.D
Acq: 16 Dec 2020 07:07

Tgt Ion:244 Resp: 3647
Ion Ratio Lower Upper
244 100
212 10.2 7.3 10.9
122 12.6 7.3 10.9#

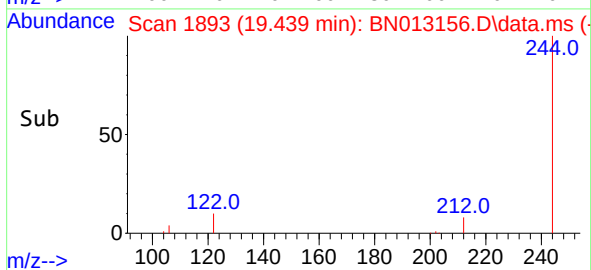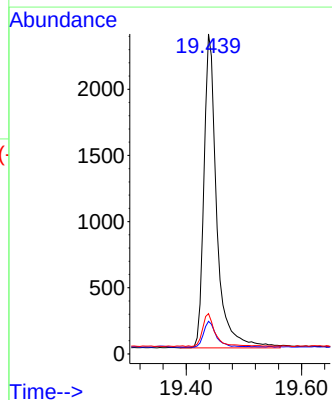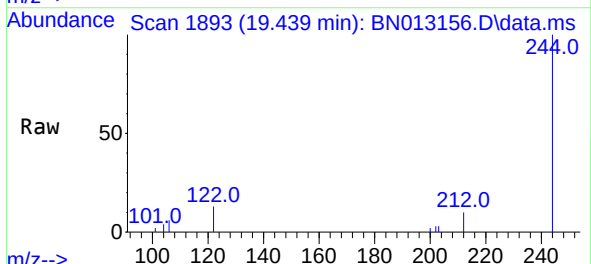

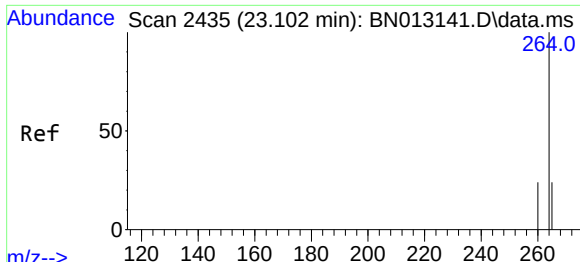

#36
 Perylene-d12
 Concen: 0.40 ng
 RT: 23.100 min Scan# 2436
 Delta R.T. -0.003 min
 Lab File: BN013156.D
 Acq: 16 Dec 2020 07:07

Instrument :
 BNA_N
 ClientSampleId :
 RE132D6-20201207

Tgt Ion:264 Resp: 4227

Ion	Ratio	Lower	Upper
264	100		
260	26.4	19.8	29.6
265	84.5	51.4	77.0#

