


Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN121620\
 Data File : BN013137.D
 Acq On : 15 Dec 2020 09:51
 Operator : CG/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\8270-SIM-BN121620.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Thu Dec 17 12:34:52 2020

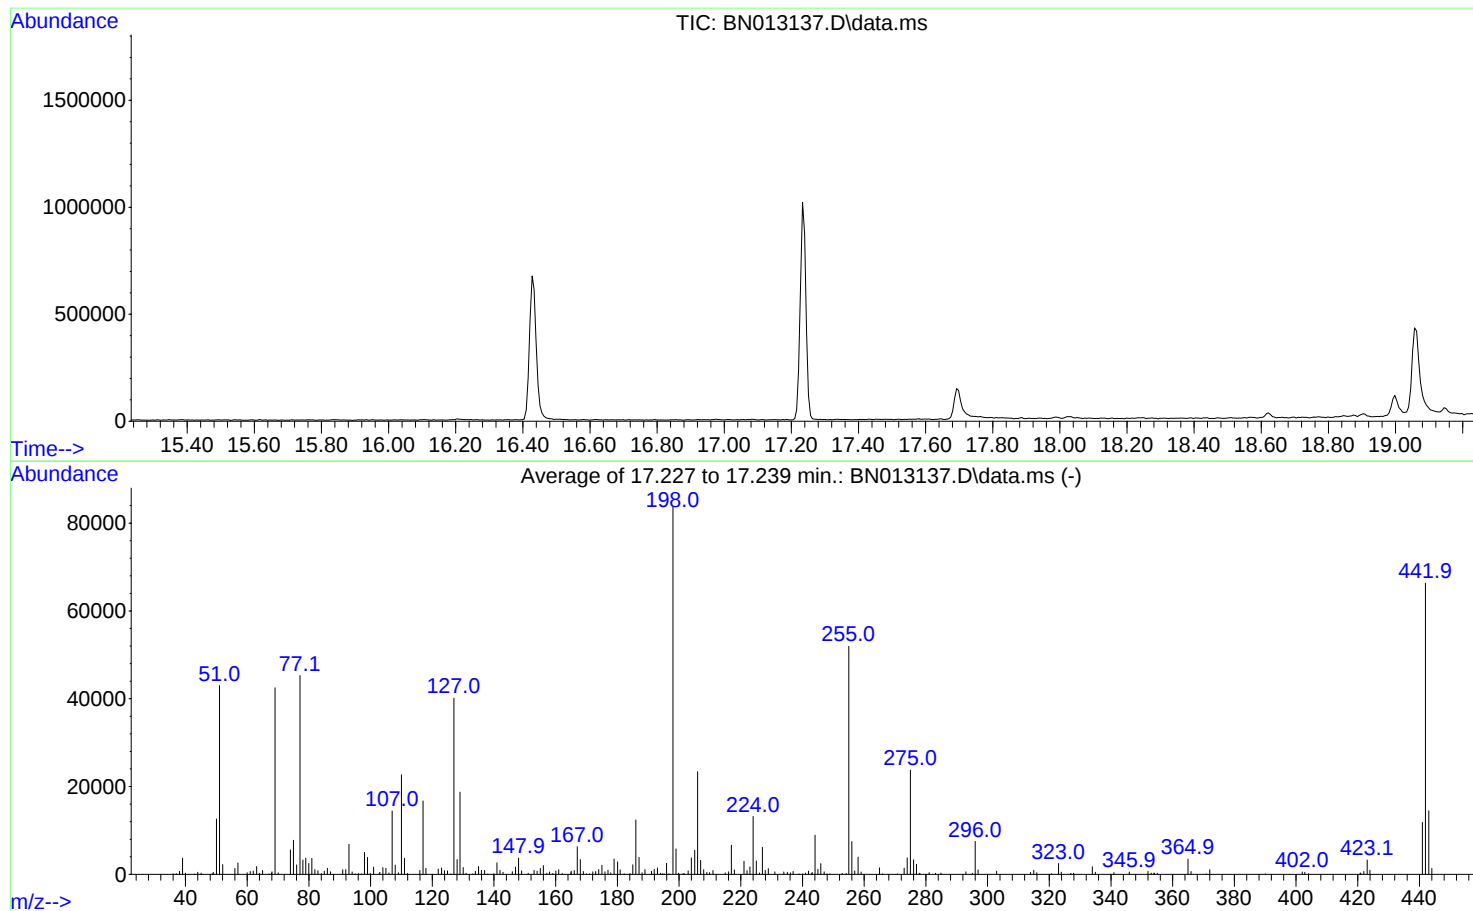

AutoFind: Scans 2506, 2507, 2508; Background Corrected with Scan 2500

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	51.3	43021	PASS
68	69	0.00	2	1.4	596	PASS
69	198	0.00	100	50.7	42480	PASS
70	69	0.00	2	0.8	357	PASS
127	198	10	80	47.9	40123	PASS
197	198	0.00	2	0.2	152	PASS
198	198	100	100	100.0	83787	PASS
199	198	5	9	6.9	5794	PASS
275	198	10	60	28.4	23774	PASS
365	198	1	100	4.1	3450	PASS
441	198	0.01	100	14.1	11799	PASS
442	442	50	100	100.0	66347	PASS
443	442	15	24	21.8	14480	PASS