
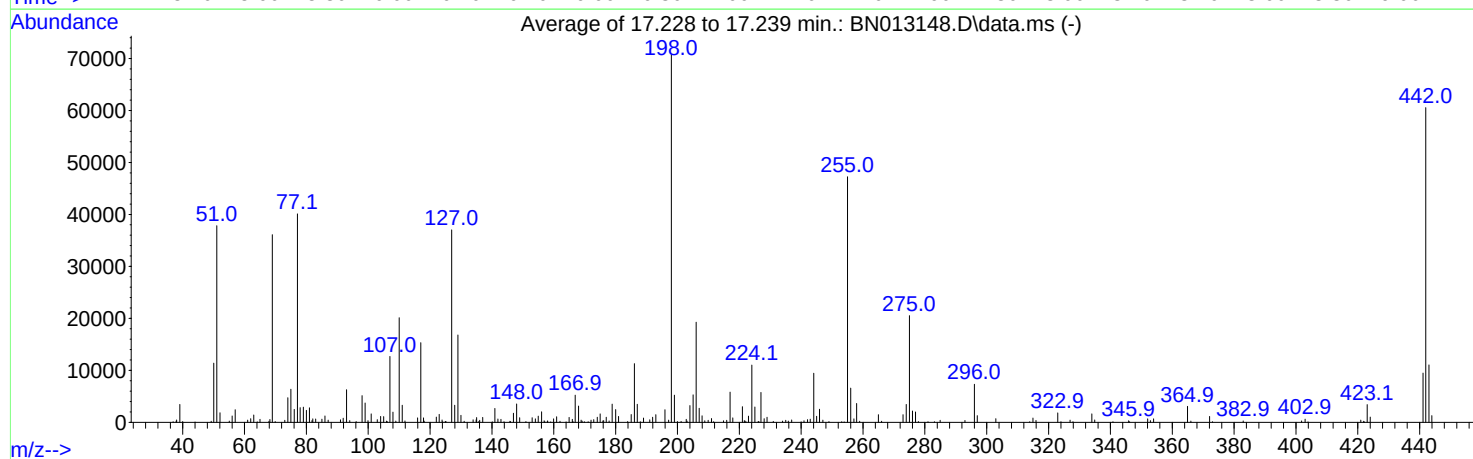


Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN121620\
 Data File : BN013148.D
 Acq On : 16 Dec 2020 01:35
 Operator : CG/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\8270-SIM-BN121620.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Thu Dec 17 12:34:52 2020

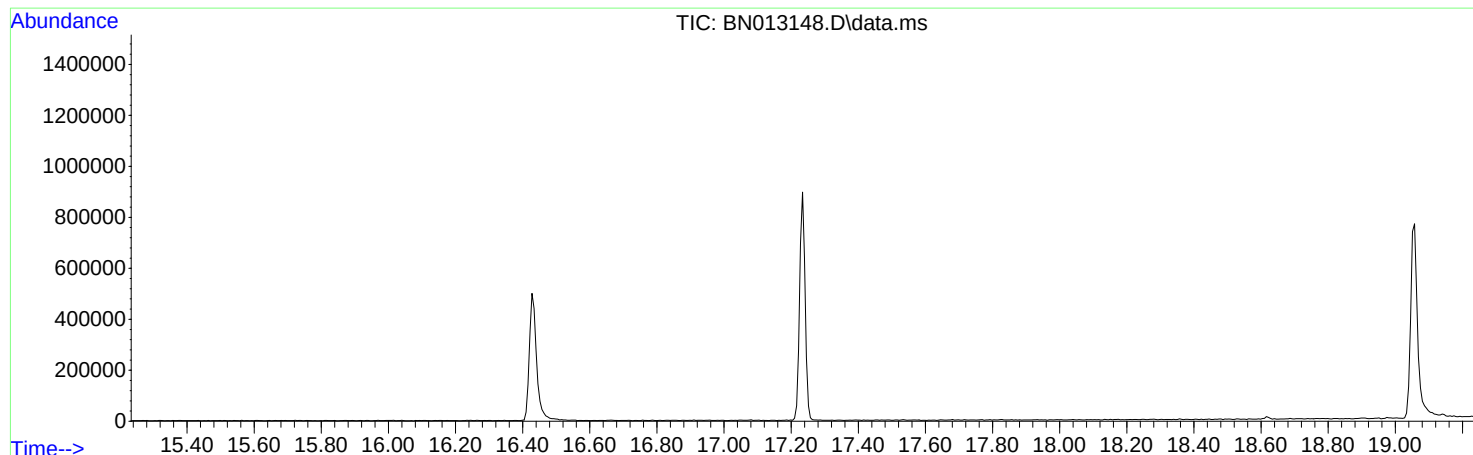

AutoFind: Scans 2506, 2507, 2508; Background Corrected with Scan 2500

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	53.4	37821	PASS
68	69	0.00	2	1.5	559	PASS
69	198	0.00	100	51.0	36096	PASS
70	69	0.00	2	0.4	152	PASS
127	198	10	80	52.3	37027	PASS
197	198	0.00	2	0.6	426	PASS
198	198	100	100	100.0	70768	PASS
199	198	5	9	7.4	5251	PASS
275	198	10	60	29.0	20528	PASS
365	198	1	100	4.3	3077	PASS
441	198	0.01	100	13.4	9484	PASS
442	442	50	100	100.0	60557	PASS
443	442	15	24	18.2	11049	PASS