


Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN121620\
 Data File : BN013166.D
 Acq On : 16 Dec 2020 14:56
 Operator : CG/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\8270-SIM-BN121620.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Thu Dec 17 12:34:52 2020

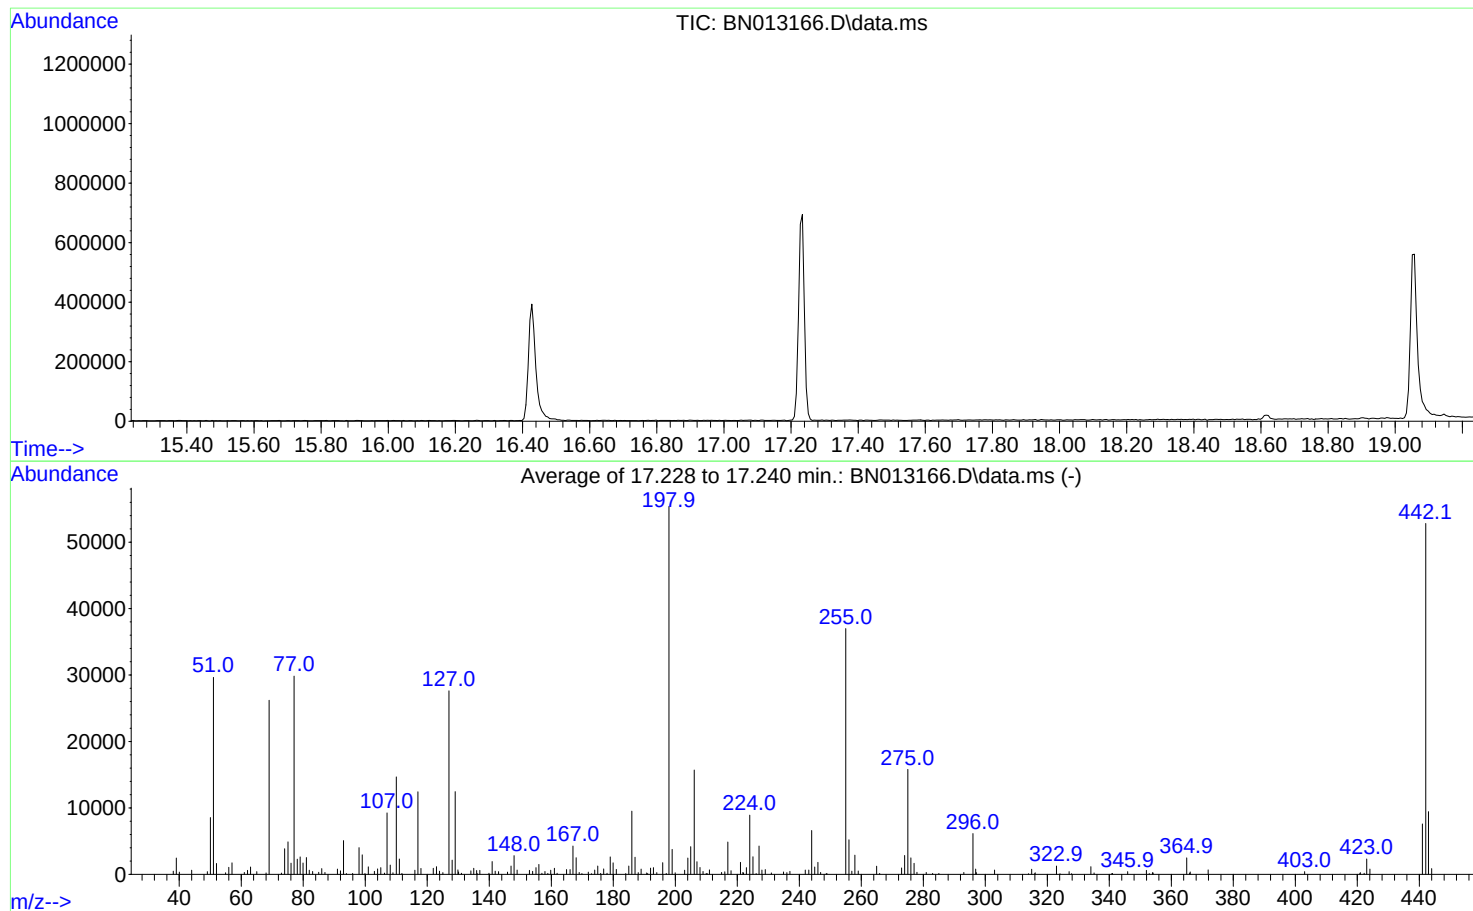

AutoFind: Scans 2506, 2507, 2508; Background Corrected with Scan 2500

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	53.6	29658	PASS
68	69	0.00	2	0.8	220	PASS
69	198	0.00	100	47.3	26195	PASS
70	69	0.00	2	0.0	0	PASS
127	198	10	80	49.9	27621	PASS
197	198	0.00	2	0.2	136	PASS
198	198	100	100	100.0	55368	PASS
199	198	5	9	6.8	3766	PASS
275	198	10	60	28.5	15788	PASS
365	198	1	100	4.5	2487	PASS
441	198	0.01	100	13.7	7598	PASS
442	442	50	100	100.0	52805	PASS
443	442	15	24	17.9	9452	PASS