

Data Path : Z:\SVOASRV\HPCHEM1\BNA N\DATA\BN121719\  
 Data File : BN009013.D  
 Acq On : 17 Dec 2019 13:04  
 Operator : JU  
 Sample : K6237-03  
 Misc :  
 ALS Vial : 7 Sample Multiplier: 1

Instrument :  
 BNA\_N  
 ClientSampleId :  
 KY038PS037-191209

Quant Time: Dec 18 12:31:03 2019  
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA N\METHODS\8270-SIM-BN120919.M  
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION  
 QLast Update : Mon Dec 09 17:02:53 2019  
 Response via : Initial Calibration


| Internal Standards             | R.T.  | QIon | Response | Conc  | Units | Dev(Min) |
|--------------------------------|-------|------|----------|-------|-------|----------|
| 1) 1,4-Dichlorobenzene-d4      | 7.55  | 152  | 2836     | 0.40  | ng    | -0.02    |
| 7) Naphthalene-d8              | 10.30 | 136  | 12227    | 0.40  | ng    | -0.01    |
| 13) Acenaphthene-d10           | 14.17 | 164  | 9070     | 0.40  | ng    | -0.01    |
| 19) Phenanthrene-d10           | 16.92 | 188  | 21864    | 0.40  | ng    | -0.01    |
| 27) Chrysene-d12               | 21.13 | 240  | 20852    | 0.40  | ng    | 0.00     |
| 34) Perylene-d12               | 23.27 | 264  | 19124    | 0.40  | ng    | -0.01    |
| System Monitoring Compounds    |       |      |          |       |       |          |
| 4) 2-Fluorophenol              | 5.19  | 112  | 1245     | 0.17  | ng    | 0.00     |
| 5) Phenol-d6                   | 6.74  | 99   | 1110     | 0.11  | ng    | -0.02    |
| 8) Nitrobenzene-d5             | 8.68  | 82   | 3731     | 0.36  | ng    | -0.01    |
| 11) 2-Methylnaphthalene-d10    | 11.90 | 152  | 8124     | 0.39  | ng    | -0.01    |
| 14) 2,4,6-Tribromophenol       | 15.67 | 330  | 1757     | 0.40  | ng    | -0.01    |
| 15) 2-Fluorobiphenyl           | 12.79 | 172  | 12360    | 0.36  | ng    | -0.02    |
| 25) Fluoranthene-d10           | 18.96 | 212  | 25856    | 0.39  | ng    | 0.00     |
| 29) Terphenyl-d14              | 19.57 | 244  | 19240    | 0.40  | ng    | 0.00     |
| Target Compounds               |       |      |          |       |       | Qvalue   |
| 32) Bis(2-ethylhexyl)phthalate | 21.07 | 149  | 3305     | 0.095 | ng    | 99       |


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\SVOASRV\HPCHEM1\BNA N\DATA\BN121719\  
Data File : BN009013.D  
Acq On : 17 Dec 2019 13:04  
Operator : JU  
Sample : K6237-03  
Misc :  
ALS Vial : 7 Sample Multiplier: 1

Instrument :  
BNA\_N  
ClientSampleId :  
KY038PS037-191209

Quant Time: Dec 18 12:31:03 2019  
Quant Method : Z:\SVOASRV\HPCHEM1\BNA N\METHODS\8270-SIM-BN120919.M  
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION  
QLast Update : Mon Dec 09 17:02:53 2019  
Response via : Initial Calibration

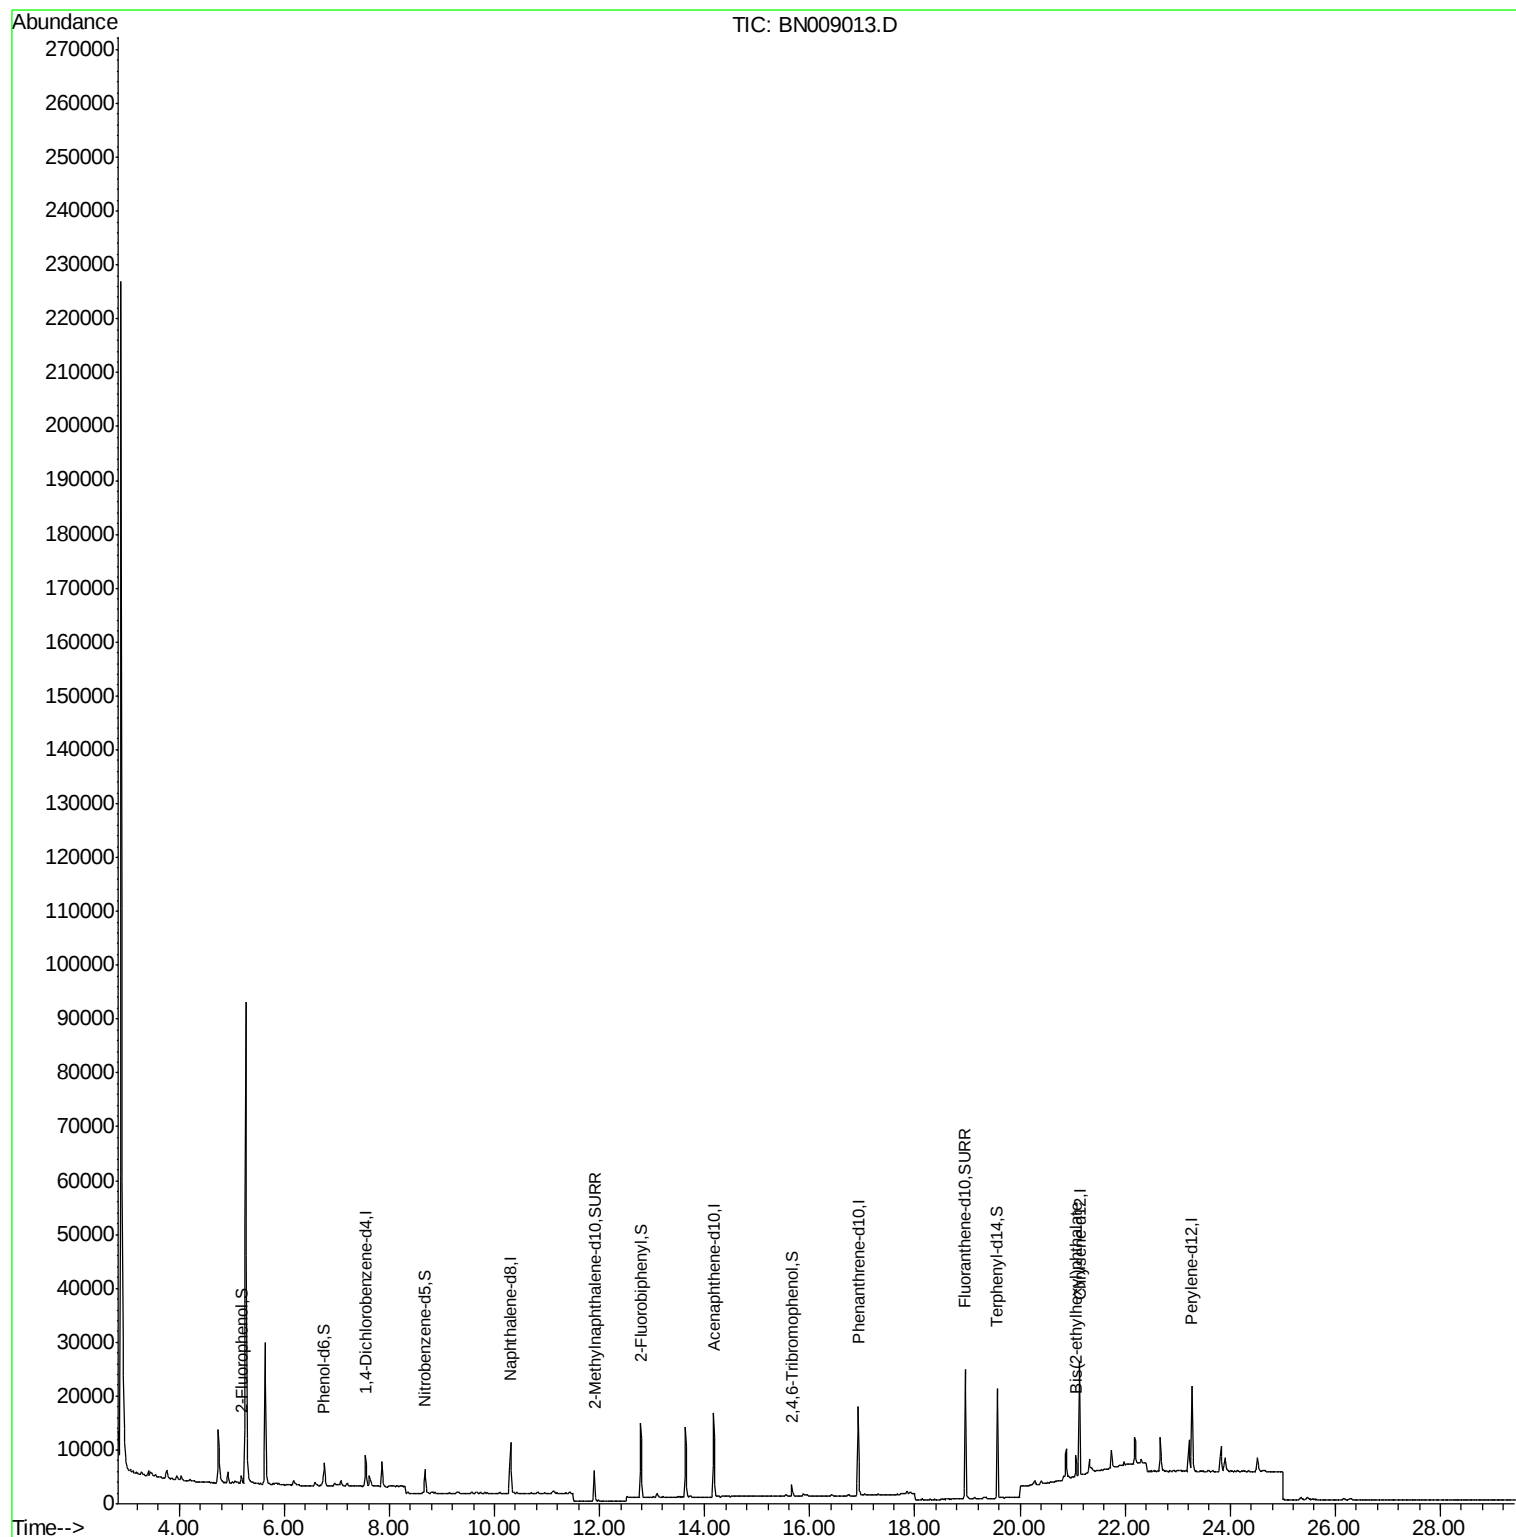

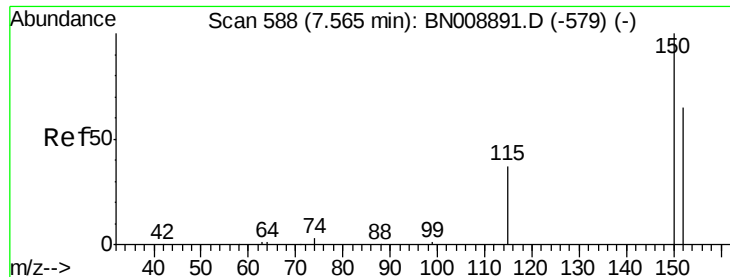


#1




1,4-Dichlorobenzene-d4  
Concen: 0.400 ng  
RT: 7.55 min Scan# 586  
Delta R.T. -0.02 min  
Lab File: BN009013.D  
Acq: 17 Dec 2019 13:04

Instrument :  
BNA\_N  
ClientSampleId :  
KY038PS037-191209

Tot Ion:152 Resp: 2836  
Ion Ratio Lower Upper  
152 100  
150 153.3 122.3 183.5  
115 61.9 48.4 72.6

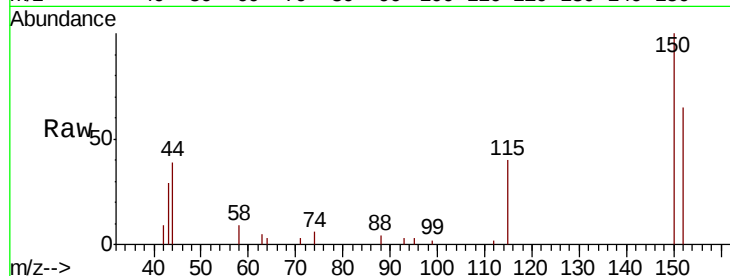


Abundance Ion 152.00 (151.70 to 152.70): E  
Ion 150.00 (149.70 to 150.70): E  
Ion 115.00 (114.70 to 115.70): E

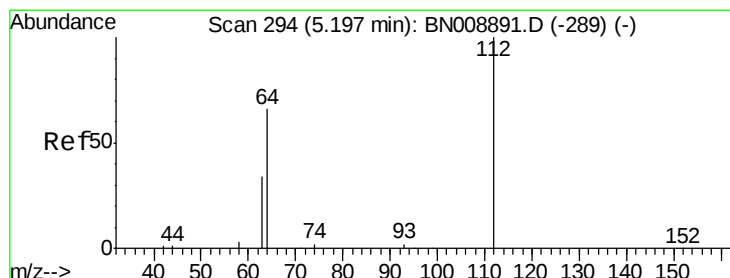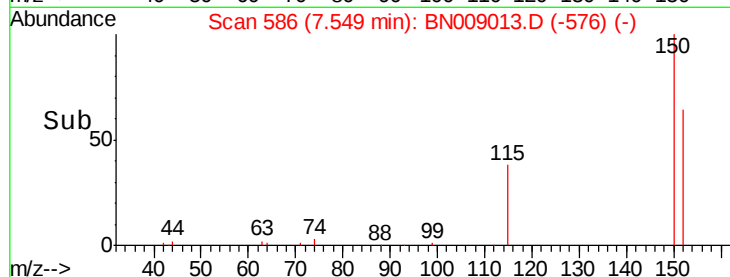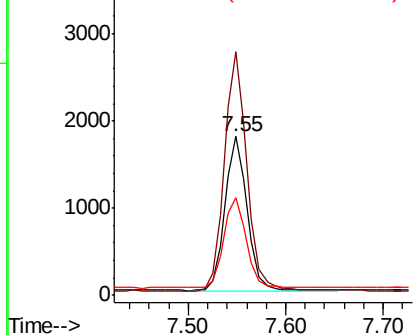



#4


2-Fluorophenol  
Concen: 0.173 ng  
RT: 5.19 min Scan# 293  
Delta R.T. -0.01 min  
Lab File: BN009013.D  
Acq: 17 Dec 2019 13:04

Tgt Ion:112 Resp: 1245  
Ion Ratio Lower Upper  
112 100  
64 68.8 57.7 86.5  
63 35.8 29.6 44.4

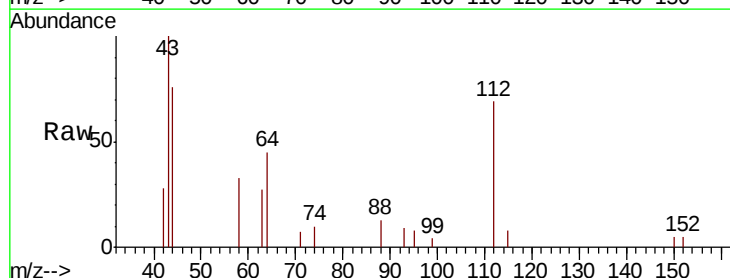

Abundance Ion 112.00 (111.70 to 112.70): E  
Ion 64.00 (63.70 to 64.70): BNC  
Ion 63.00 (62.70 to 63.70): BNC

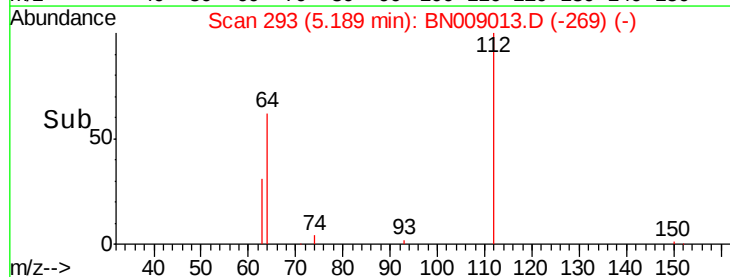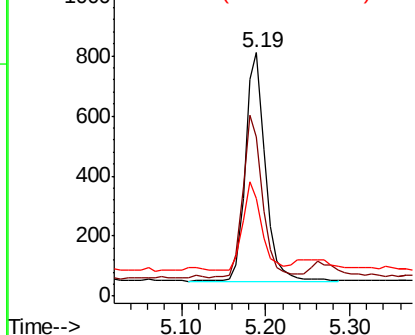

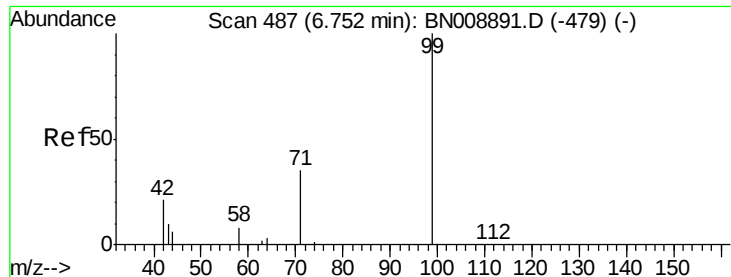

#5

Phenol-d6

Concen: 0.111 ng

RT: 6.74 min Scan# 485

Delta R.T. -0.02 min

Lab File: BN009013.D

Acq: 17 Dec 2019 13:04

Instrument :

BNA\_N

ClientSampleId :

KY038PS037-191209


Tot Ion: 99 Resp: 1110

Ion Ratio Lower Upper

99 100

42 0.0 20.1 30.1#




71 41.7 28.2 42.2

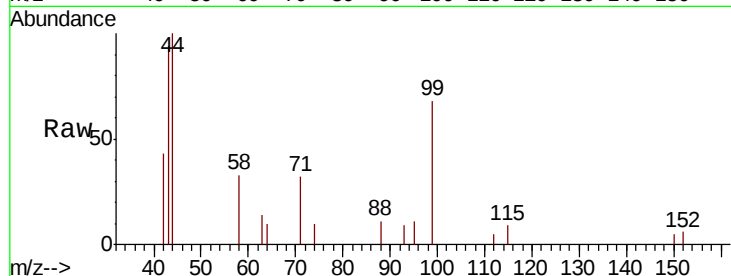

Abundance Ion 99.00 (98.70 to 99.70): BN008891.D (-479) (-)

Ion 42.00 (41.70 to 42.70): BN008891.D (-479) (-)

Ion 71.00 (70.70 to 71.70): BN008891.D (-479) (-)

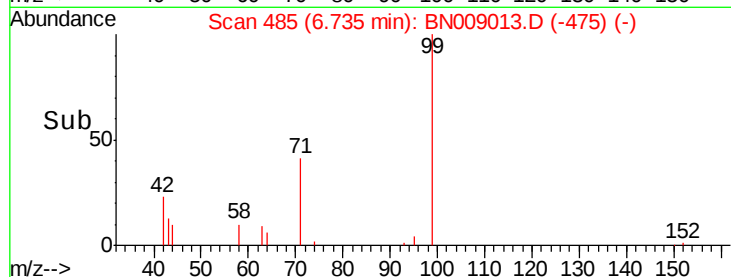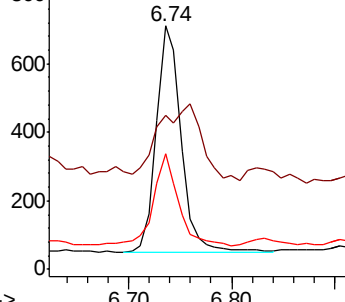

#7

Naphthalene-d8

Concen: 0.400 ng

RT: 10.30 min Scan# 838

Delta R.T. -0.01 min

Lab File: BN009013.D

Acq: 17 Dec 2019 13:04

Tgt Ion: 136 Resp: 12227


Ion Ratio Lower Upper

136 100

137 11.3 9.2 13.8

54 11.3 9.6 14.4

68 6.3 5.6 8.4






Abundance Ion 136.00 (135.70 to 136.70): BN008891.D (-834) (-)

Ion 137.00 (136.70 to 137.70): BN008891.D (-834) (-)

Ion 54.00 (53.70 to 54.70): BN008891.D (-834) (-)

Ion 68.00 (67.70 to 68.70): BN008891.D (-834) (-)

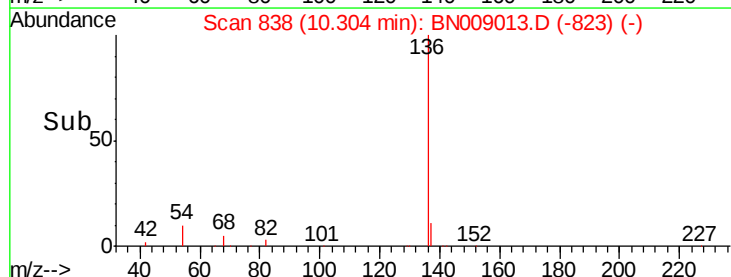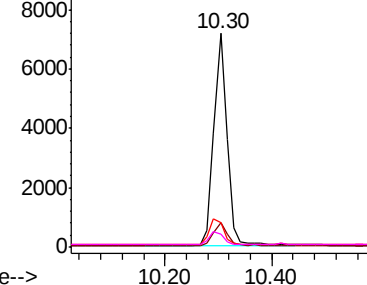

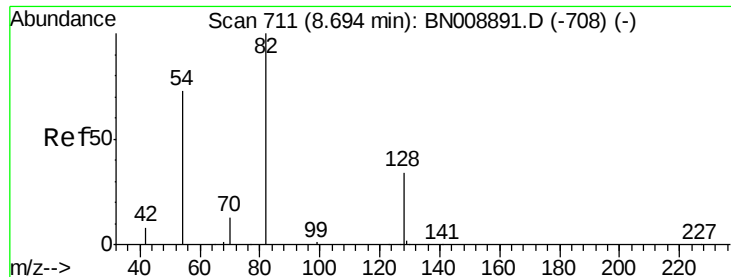

#8

Nitrobenzene-d5

Concen: 0.360 ng

RT: 8.68 min Scan# 710

Delta R.T. -0.01 min

Lab File: BN009013.D

Acq: 17 Dec 2019 13:04

Instrument :

BNA\_N

ClientSampleId :

KY038PS037-191209


Tot Ion: 82 Resp: 3731

Ion Ratio Lower Upper

82 100

128 38.2 29.1 43.7




54 69.7 59.7 89.5

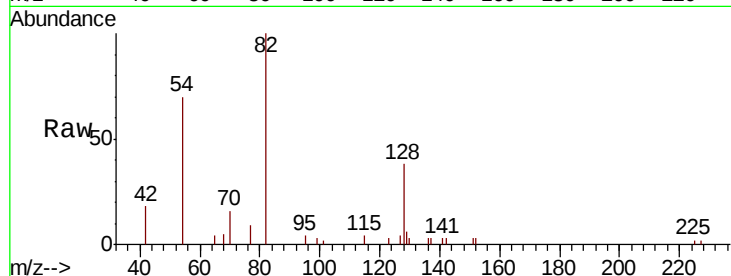

Abundance Ion 82.00 (81.70 to 82.70): BN008891.D (-708) (-)

Ion 128.00 (127.70 to 128.70): BN008891.D (-708) (-)

Ion 54.00 (53.70 to 54.70): BN008891.D (-708) (-)

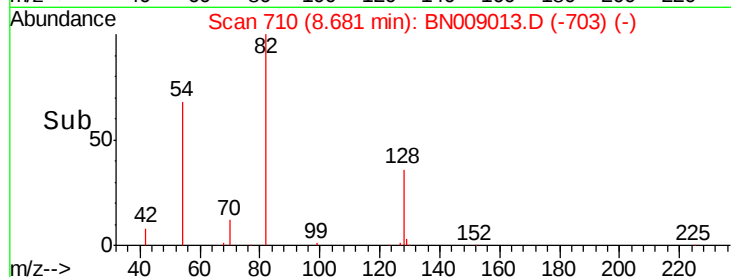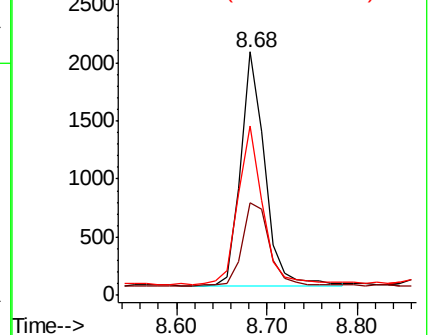

#11

2-Methylnaphthalene-d10

Concen: 0.389 ng

RT: 11.90 min Scan# 1021

Delta R.T. -0.01 min

Lab File: BN009013.D


Acq: 17 Dec 2019 13:04

Tgt Ion: 152 Resp: 8124

Ion Ratio Lower Upper



152 100


151 19.0 15.2 22.8



Abundance Ion 152.00 (151.70 to 152.70): BN008891.D (-1013) (-)

Ion 151.00 (150.70 to 151.70): BN008891.D (-1013) (-)

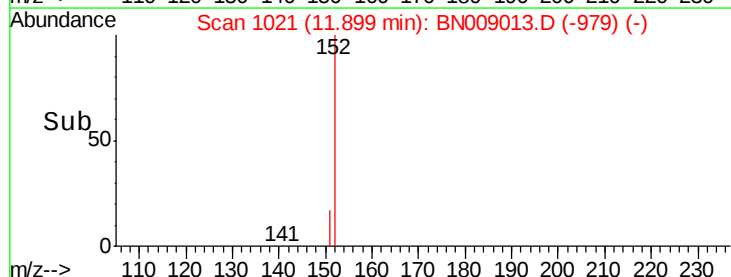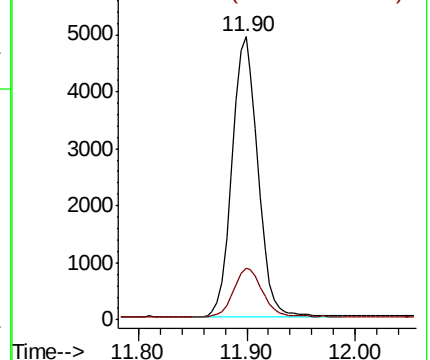

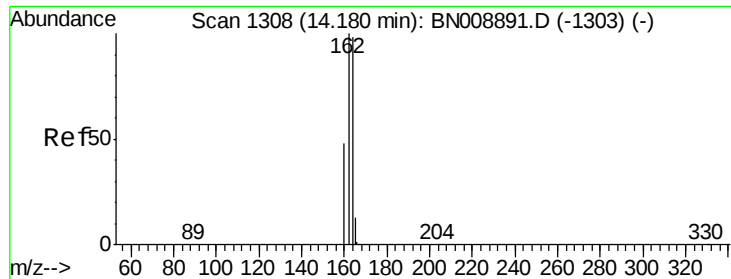

#13

Acenaphthene-d10

Concen: 0.400 ng

RT: 14.17 min Scan# 1307

Delta R.T. -0.01 min

Lab File: BN009013.D

Acq: 17 Dec 2019 13:04

Instrument :

BNA\_N

ClientSampleId :

KY038PS037-191209


Tot Ion:164 Resp: 9070

Ion Ratio Lower Upper

164 100

162 101.9 81.9 122.9




160 46.8 39.3 58.9



Abundance Ion 164.00 (163.70 to 164.70): E

Ion 162.00 (161.70 to 162.70): E

Ion 160.00 (159.70 to 160.70): E

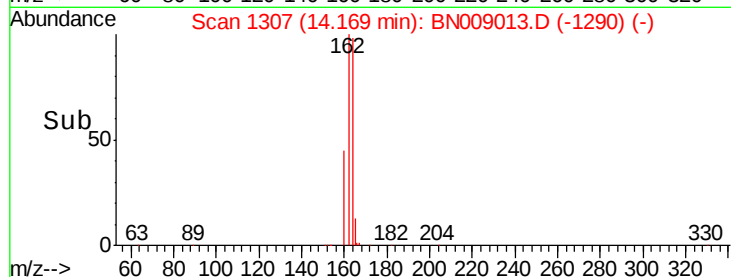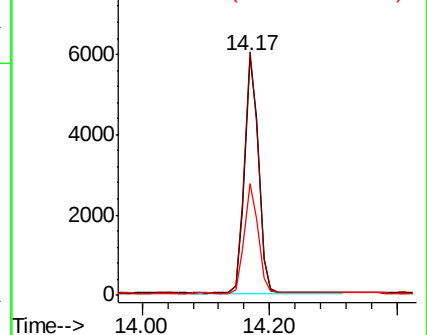

#14

2,4,6-Tribromophenol

Concen: 0.404 ng

RT: 15.67 min Scan# 1442

Delta R.T. -0.01 min

Lab File: BN009013.D

Acq: 17 Dec 2019 13:04


Tgt Ion:330 Resp: 1757

Ion Ratio Lower Upper

330 100

332 0.0 0.0 0.0



141 35.1 29.6 44.4




Abundance Ion 330.00 (329.70 to 330.70): E

Ion 331.80 (331.50 to 332.50): E

Ion 141.00 (140.70 to 141.70): E

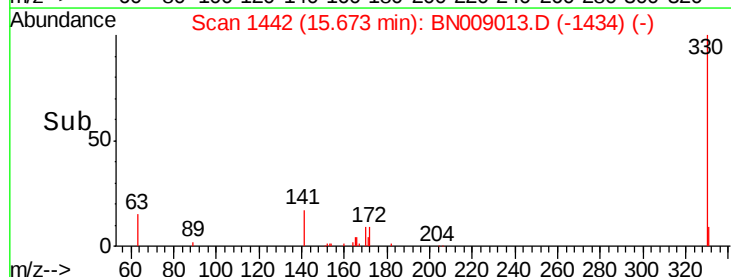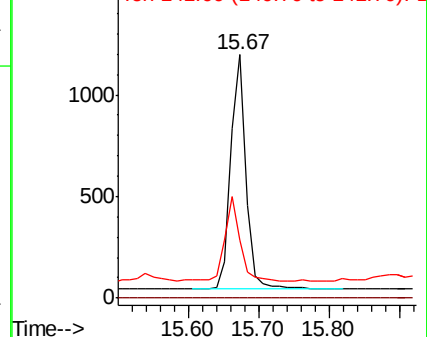

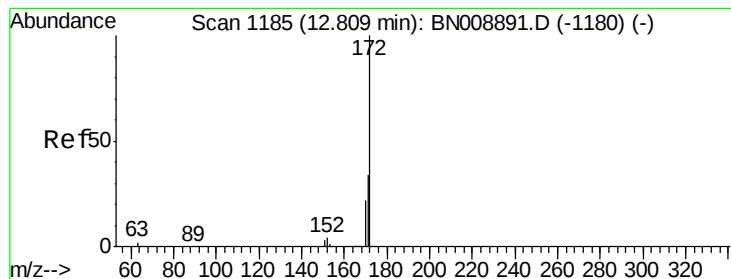

#15

2-Fluorobiphenyl

Concen: 0.359 ng

RT: 12.79 min Scan# 1183

Delta R.T. -0.02 min

Lab File: BN009013.D

Acq: 17 Dec 2019 13:04

Instrument :

BNA\_N

ClientSampleId :

KY038PS037-191209


Tot Ion:172 Resp: 12360

Ion Ratio Lower Upper

172 100

171 35.8 27.1 40.7




170 24.0 17.7 26.5



Abundance Ion 172.00 (171.70 to 172.70): E

Ion 171.00 (170.70 to 171.70): E

Ion 170.00 (169.70 to 170.70): E

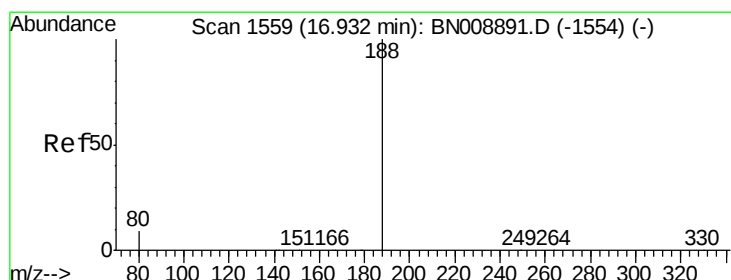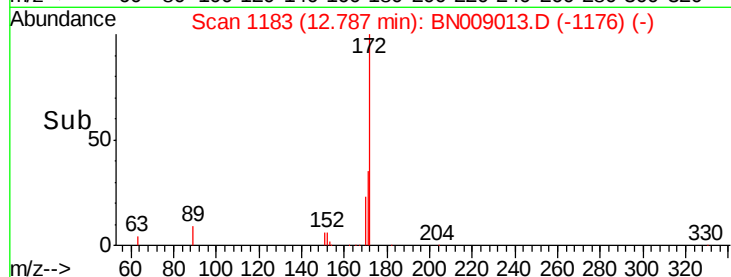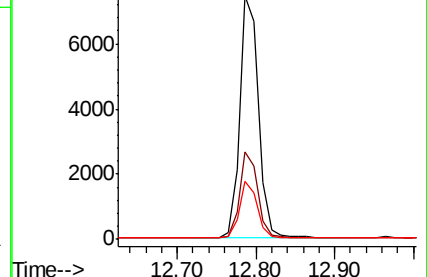

#19

Phenanthrene-d10

Concen: 0.400 ng

RT: 16.92 min Scan# 1558

Delta R.T. -0.01 min

Lab File: BN009013.D

Acq: 17 Dec 2019 13:04


Tgt Ion:188 Resp: 21864

Ion Ratio Lower Upper

188 100

94 0.0 0.0 0.0



80 8.9 7.3 10.9




Abundance Ion 188.00 (187.70 to 188.70): E

Ion 94.00 (93.70 to 94.70): BNC

Ion 80.00 (79.70 to 80.70): BNC

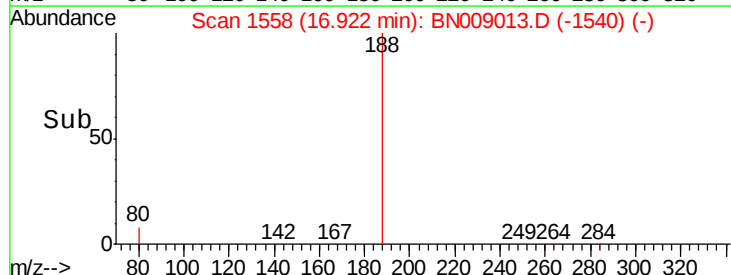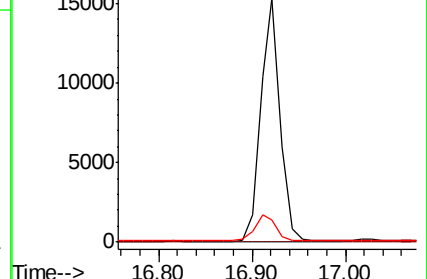

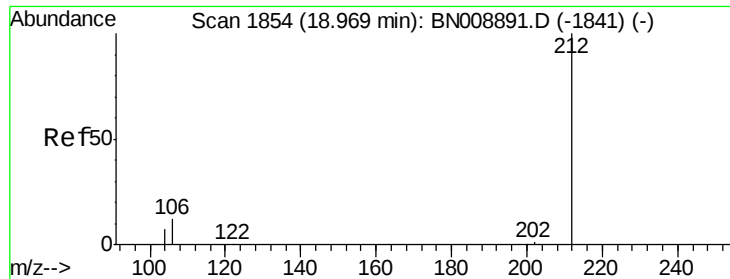

#25

Fluoranthene-d10

Concen: 0.391 ng

RT: 18.96 min Scan# 1852

Delta R.T. -0.01 min

Lab File: BN009013.D

Acq: 17 Dec 2019 13:04

Instrument :

BNA\_N

ClientSampleId :

KY038PS037-191209





Tot Ion:212 Resp: 25856

Ion Ratio Lower Upper

212 100

106 12.9 10.4 15.6

104 7.3 5.9 8.9

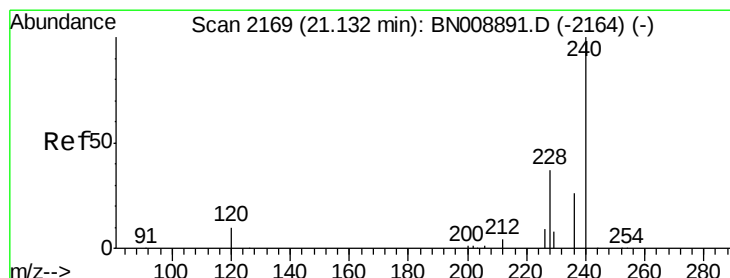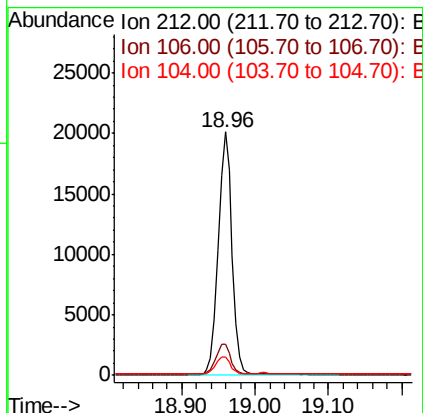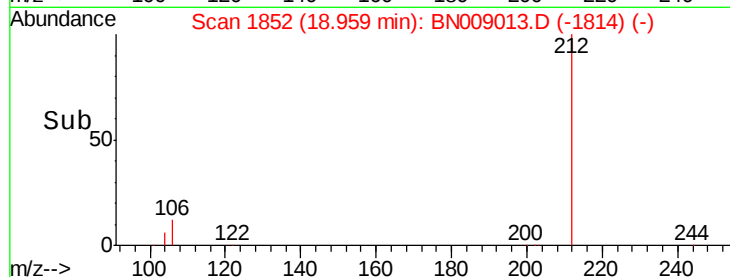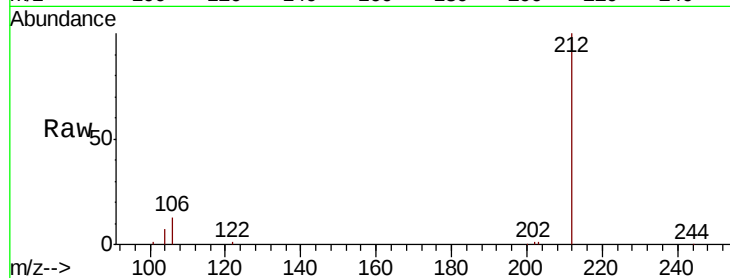

#27

Chrysene-d12

Concen: 0.400 ng

RT: 21.13 min Scan# 2169

Delta R.T. -0.00 min

Lab File: BN009013.D

Acq: 17 Dec 2019 13:04




Tgt Ion:240 Resp: 20852


Ion Ratio Lower Upper

240 100

120 7.5 9.1 13.7#

236 25.9 21.5 32.3

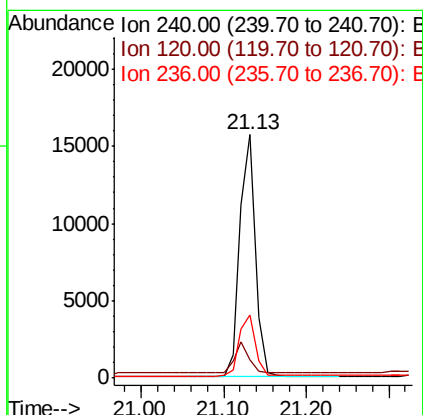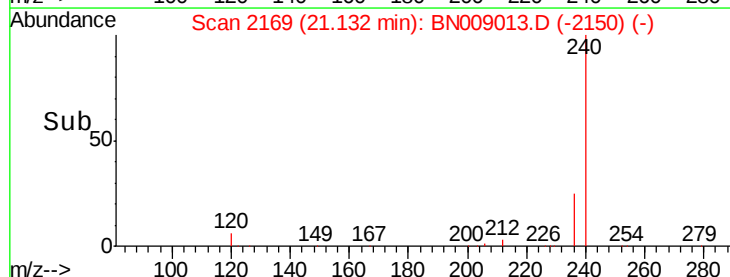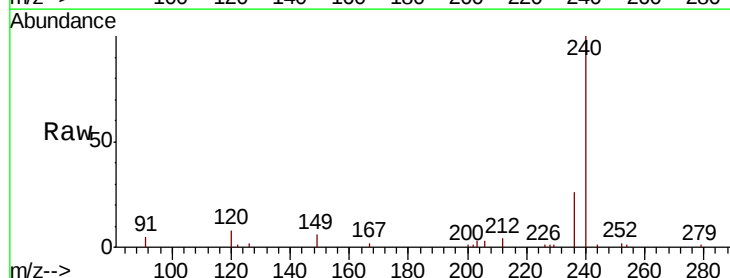

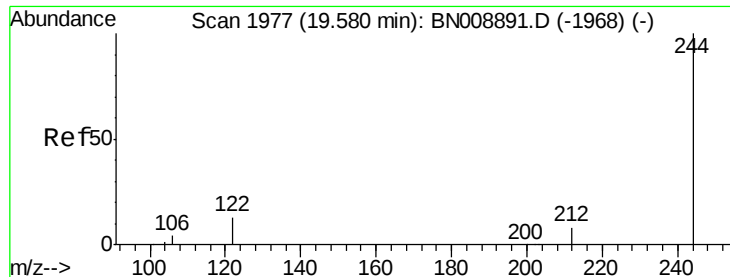

#29

Terphenyl-d14

Concen: 0.404 ng

RT: 19.57 min Scan# 1975

Delta R.T. -0.01 min

Lab File: BN009013.D

Acq: 17 Dec 2019 13:04

Instrument :

BNA\_N

ClientSampleId :

KY038PS037-191209


Tot Ion:244 Resp: 19240

Ion Ratio Lower Upper

244 100

212 8.0 6.5 9.7




122 13.5 10.4 15.6

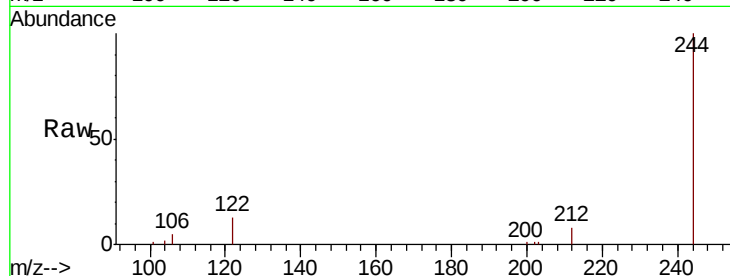

Abundance Ion 244.00 (243.70 to 244.70): E

Ion 212.00 (211.70 to 212.70): E

Ion 122.00 (121.70 to 122.70): E

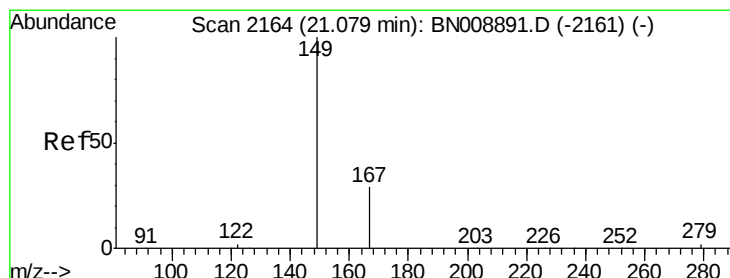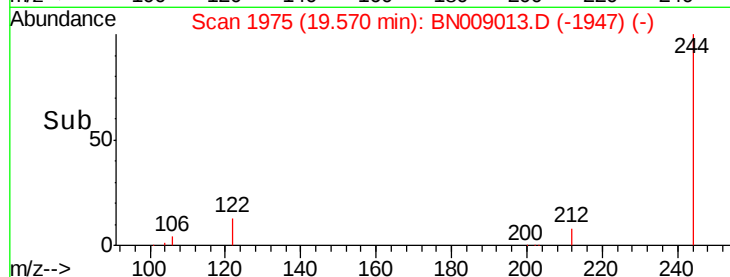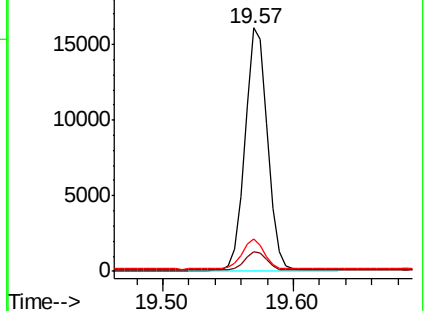

#32

Bis(2-ethylhexyl)phthalate

Concen: 0.095 ng

RT: 21.07 min Scan# 2163

Delta R.T. -0.01 min

Lab File: BN009013.D

Acq: 17 Dec 2019 13:04


Tgt Ion:149 Resp: 3305

Ion Ratio Lower Upper

149 100

167 28.0 22.7 34.1



279 4.1 3.3 4.9



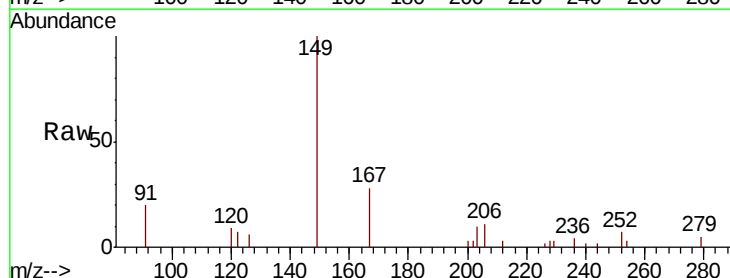


Abundance Ion 149.00 (148.70 to 149.70): E

Ion 167.00 (166.70 to 167.70): E

Ion 279.00 (278.70 to 279.70): E

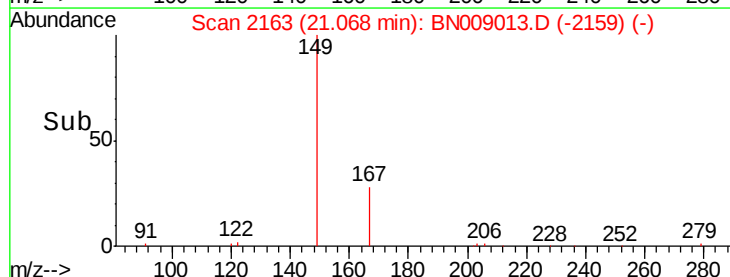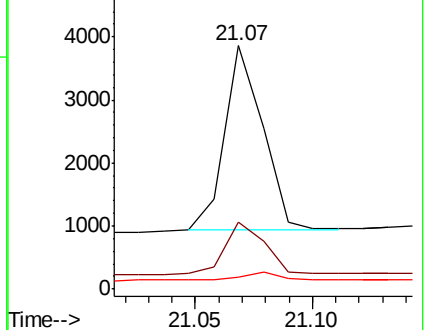

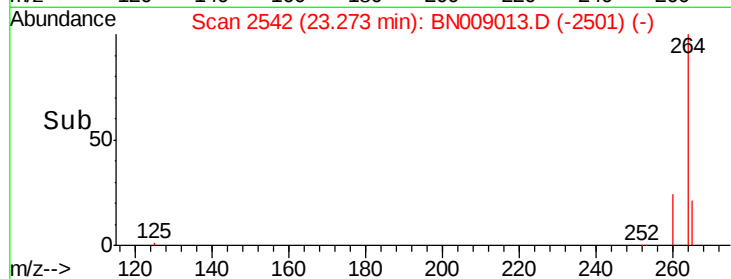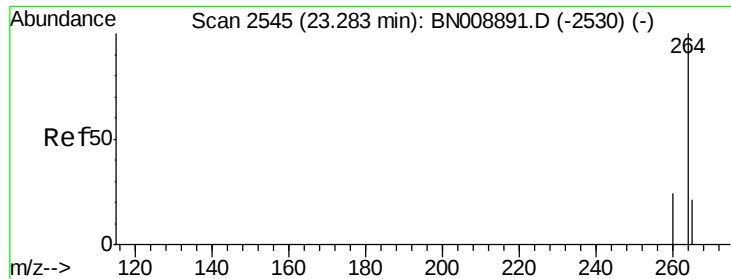

#34

Pervlene-d12

Concen: 0.400 ng

RT: 23.27 min Scan# 2542

Delta R.T. -0.01 min

Lab File: BN009013.D

Acq: 17 Dec 2019 13:04

Instrument :

BNA\_N

ClientSampleId :

KY038PS037-191209

Tot Ion: 264 Resp: 19124

Ion Ratio Lower Upper

264 100

260 24.3 19.4 29.0

265 54.8 47.5 71.3

