


Data Path : Z:\SVOASRV\HPCHEM1\BNA_N\DATA\BN121719\
 Data File : BN009007.D
 Acq On : 17 Dec 2019 09:30
 Operator : JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\8270-SIM-BN120919.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Mon Dec 09 17:02:53 2019

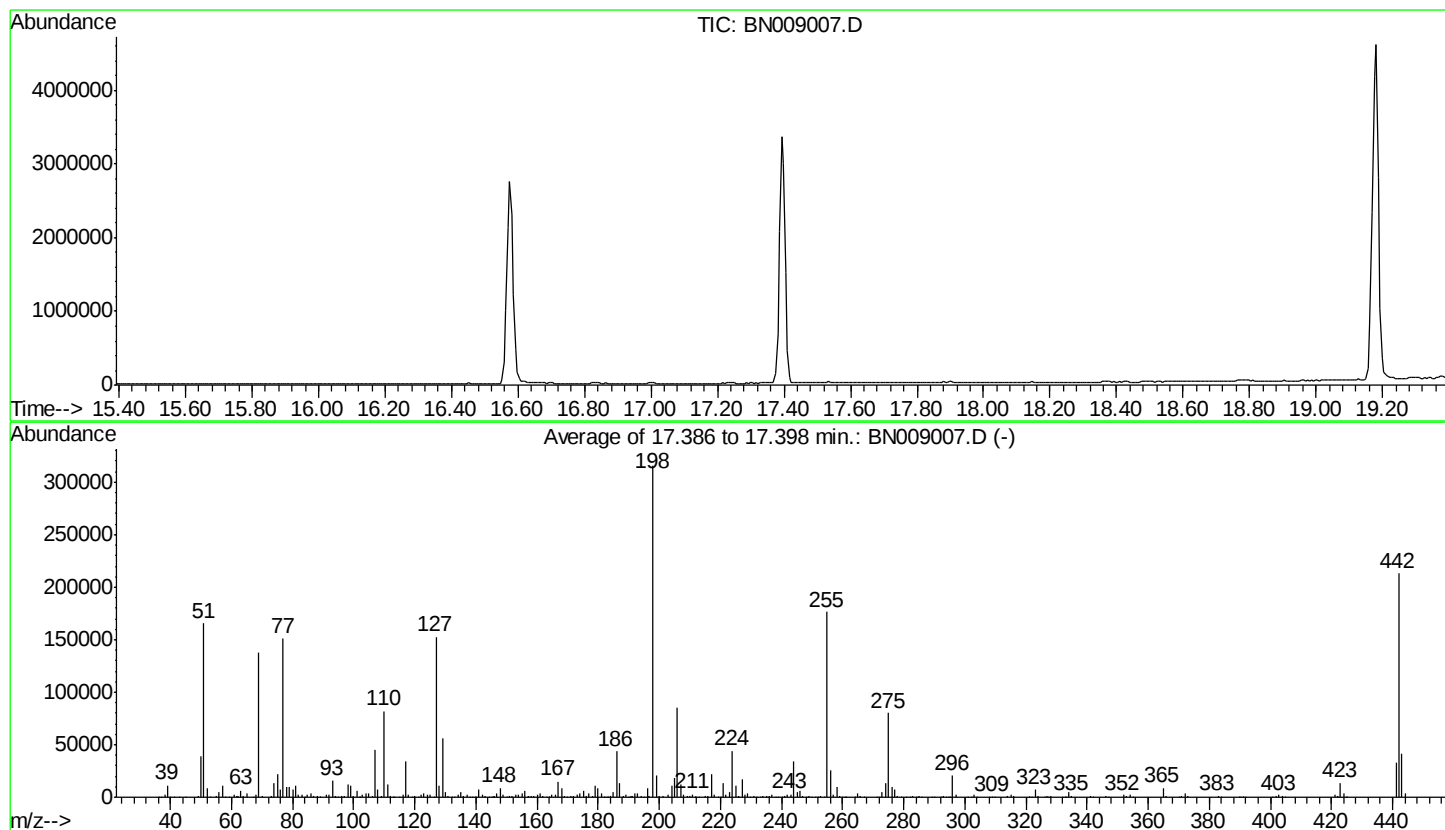

AutoFind: Scans 2448, 2449, 2450; Background Corrected with Scan 2441

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	52.4	165482	PASS
68	69	0.00	2	1.8	2501	PASS
69	198	0.00	100	43.7	137969	PASS
70	69	0.00	2	0.6	880	PASS
127	198	10	80	48.5	152973	PASS
197	198	0.00	2	0.6	1808	PASS
198	198	100	100	100.0	315690	PASS
199	198	5	9	6.6	20789	PASS
275	198	10	60	25.3	79906	PASS
365	198	1	100	2.9	9104	PASS
441	198	0.01	100	10.5	33274	PASS
442	198	50	100	67.5	212944	PASS
443	442	15	24	19.4	41224	PASS