

Data File : BN004074.D
Acq On : 18 Dec 2018 13:47
Operator : JU/SJ
Sample : J6270-16
Misc :
ALS Vial : 6 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
F9E15

Quant Time: Dec 19 01:57:52 2018
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SOM-EPA-SIM-BN111918.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Dec 19 01:54:36 2018
Response via : Initial Calibration


Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	7.84	152	1673	0.40	ng/ul	0.00
2) Naphthalene-d8	10.63	136	8281	0.40	ng/ul	0.00
6) Acenaphthene-d10	14.47	164	5126	0.40	ng/ul	0.00
10) Phenanthrene-d10	17.31	188	882967	0.40	ng/ul	0.10
16) Chrysene-d12	0.00	240	0	0.00	ng/ul	-21.41
20) Perylene-d12	23.72	264	13903	0.40	ng/ul	0.00
System Monitoring Compounds						
4) 2-Methylnaphthalene-d10	12.22	152	3603	0.28	ng/ul	0.00
14) Fluoranthene-d10	0.00	212	0	0.00	ng/ul	
Target Compounds						
21) Benzo(b)fluoranthene	23.02	252	2752	0.048	ng/ul#	24
22) Benzo(k)fluoranthene	23.02	252	2745	0.049	ng/ul#	25


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data File : BN004074.D
Acq On : 18 Dec 2018 13:47
Operator : JU/SJ
Sample : J6270-16
Misc :
ALS Vial : 6 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
F9E15

Quant Time: Dec 19 01:57:52 2018
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SOM-EPA-SIM-BN111918.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Dec 19 01:54:36 2018
Response via : Initial Calibration

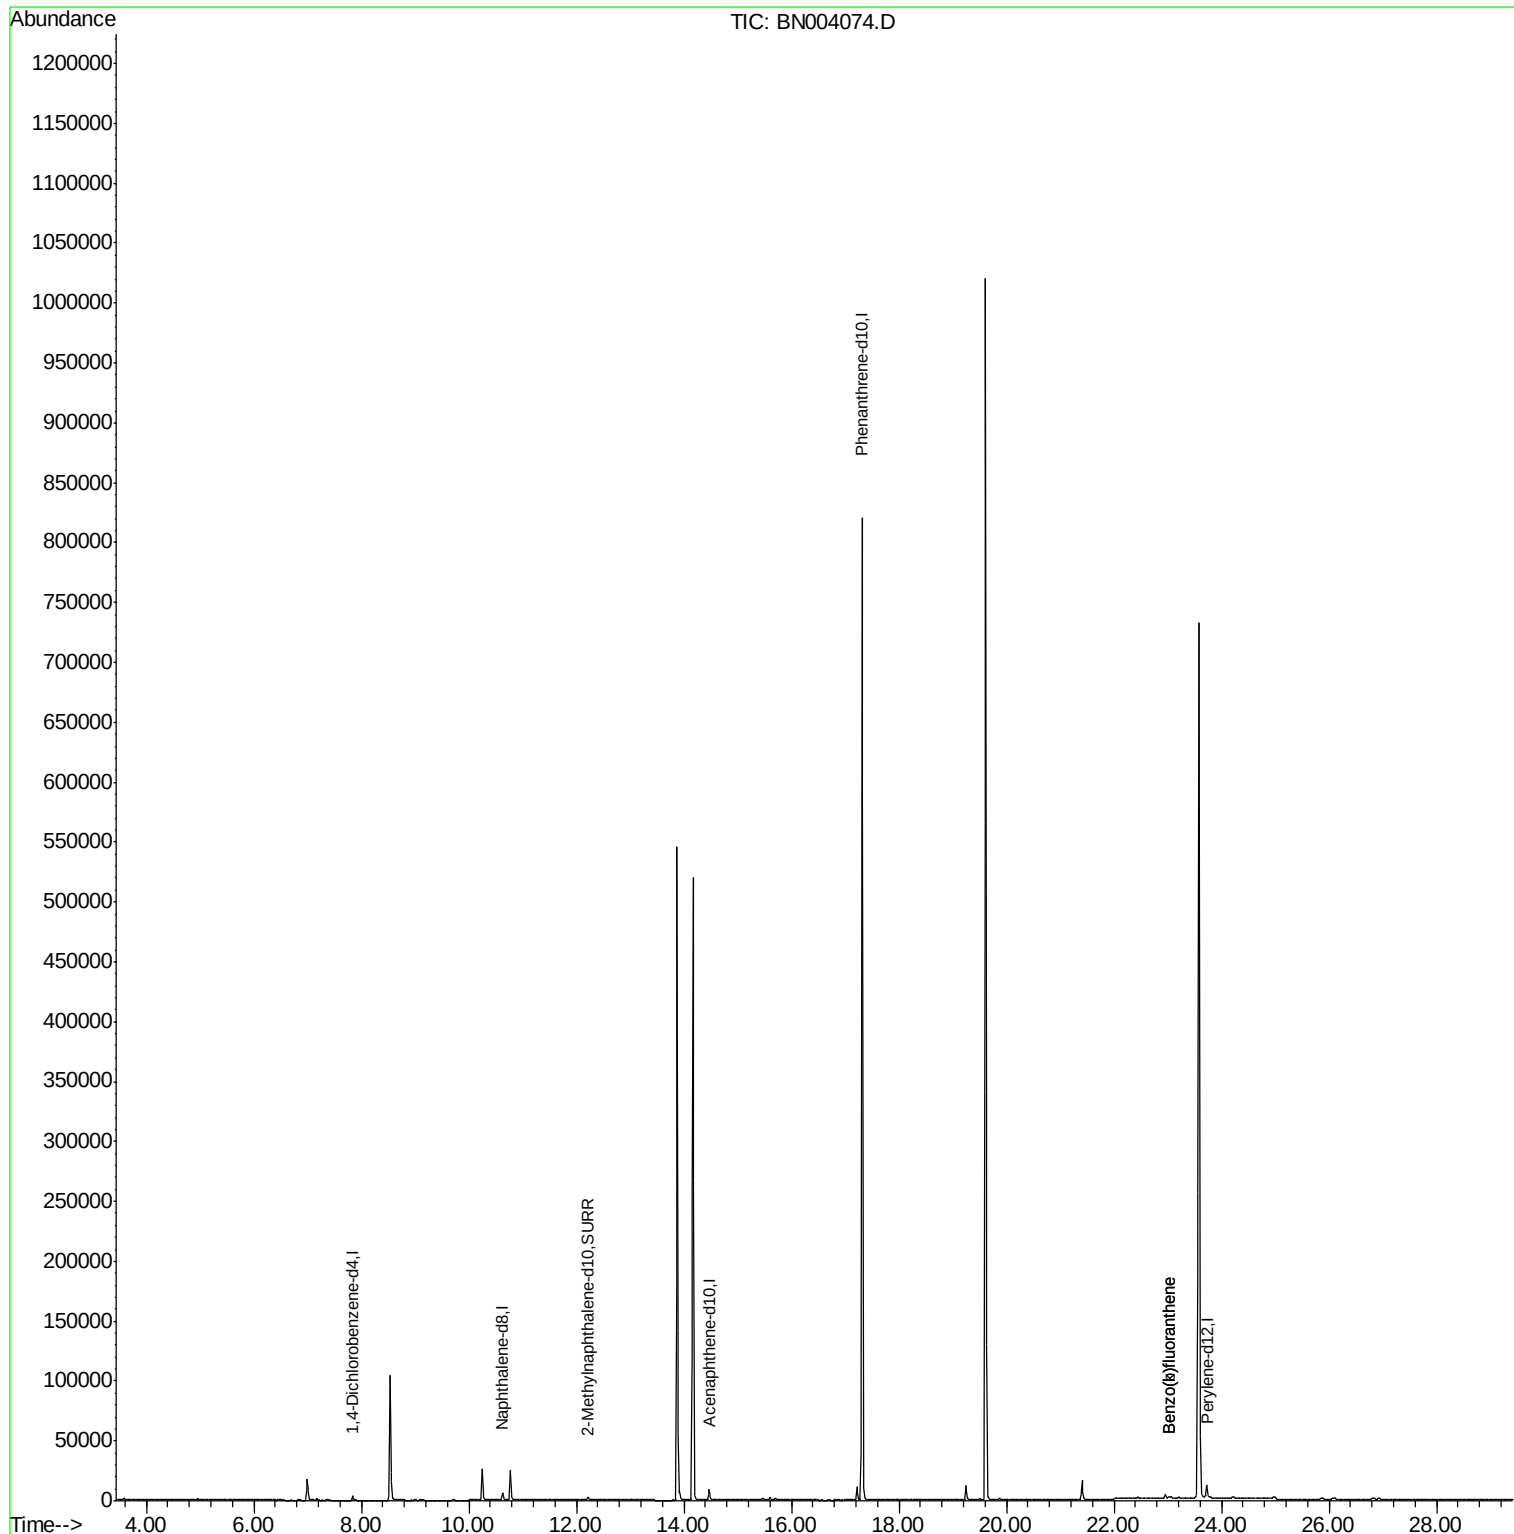

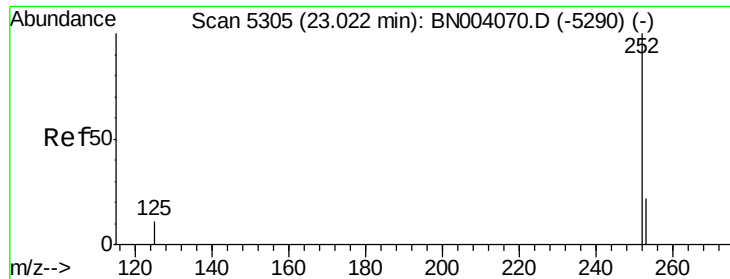

#21

Benzo(b)fluoranthene

Concen: 0.048 ng/ul

RT: 23.02 min Scan# 5305

Delta R.T. -0.00 min

Lab File: BN004074.D

Acq: 18 Dec 2018 13:47

Instrument :

BNA_N

ClientSampleId :

F9E15


Tgt Ion:252 Resp: 2752

Ion Ratio Lower Upper

252 100

253 52.2 0.0 46.0#




125 52.3 0.0 22.4#

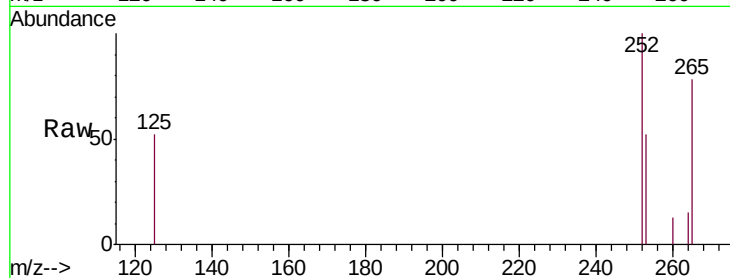

Abundance Ion 252.00 (251.70 to 252.70): E

Ion 253.00 (252.70 to 253.70): E

Ion 125.00 (124.70 to 125.70): E

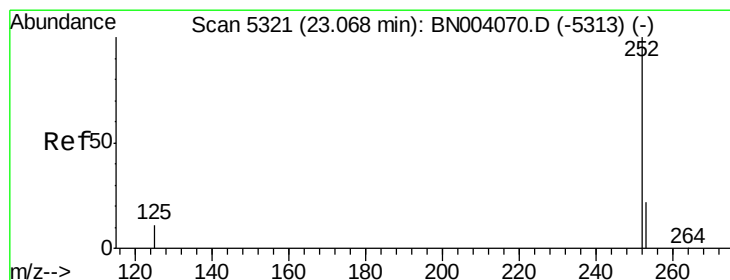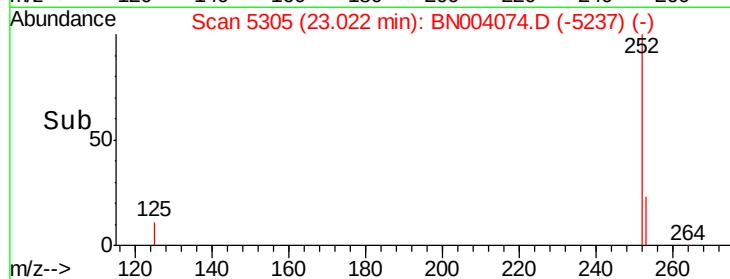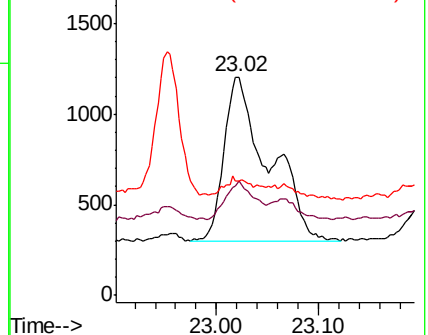

#22

Benzo(k)fluoranthene

Concen: 0.049 ng/ul

RT: 23.02 min Scan# 5305

Delta R.T. -0.05 min

Lab File: BN004074.D

Acq: 18 Dec 2018 13:47


Tgt Ion:252 Resp: 2745

Ion Ratio Lower Upper

252 100

253 52.2 18.5 27.7#

125 52.3 9.0 13.6#

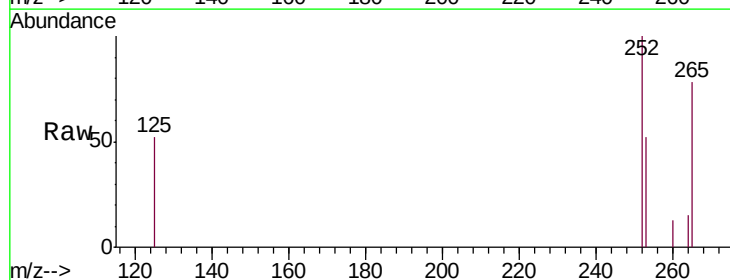

Abundance Ion 252.00 (251.70 to 252.70): E

Ion 253.00 (252.70 to 253.70): E

Ion 125.00 (124.70 to 125.70): E

