

Data Path : Z:\SVOASRV\HPCHEM1\BNA_N\DATA\BN121818\
Quantitation Report (Not Reviewed)

Data File : BN004075.D
Acq On : 18 Dec 2018 14:22
Operator : JU/SJ
Sample : J6270-17
Misc :
ALS Vial : 7 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
F9F45

Quant Time: Dec 19 01:57:58 2018
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SOM-EPA-SIM-BN111918.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Dec 19 01:54:36 2018
Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	7.83	152	1827	0.40	ng/ul	0.00
2) Naphthalene-d8	10.63	136	8932	0.40	ng/ul	0.00
6) Acenaphthene-d10	14.47	164	5405	0.40	ng/ul	0.00
10) Phenanthrene-d10	17.31	188	608635	0.40	ng/ul	0.10
16) Chrysene-d12	0.00	240	0	0.00	ng/ul	-21.41
20) Perylene-d12	23.72	264	13834	0.40	ng/ul	0.00
System Monitoring Compounds						
4) 2-Methylnaphthalene-d10	12.22	152	2645	0.19	ng/ul	0.00
14) Fluoranthene-d10	0.00	212	0	0.00	ng/ul	
Target Compounds						
23) Benzo(a)pyrene	23.58	252	2557	0.052	ng/ul#	Qvalue 42

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data File : BN004075.D

Acq On : 18 Dec 2018 14:22

Operator : JU/SJ

Sample : J6270-17

Misc :

ALS Vial : 7 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
F9F45


Quant Time: Dec 19 01:57:58 2018


Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SOM-EPA-SIM-BN111918.M

Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

QLast Update : Wed Dec 19 01:54:36 2018

Response via : Initial Calibration

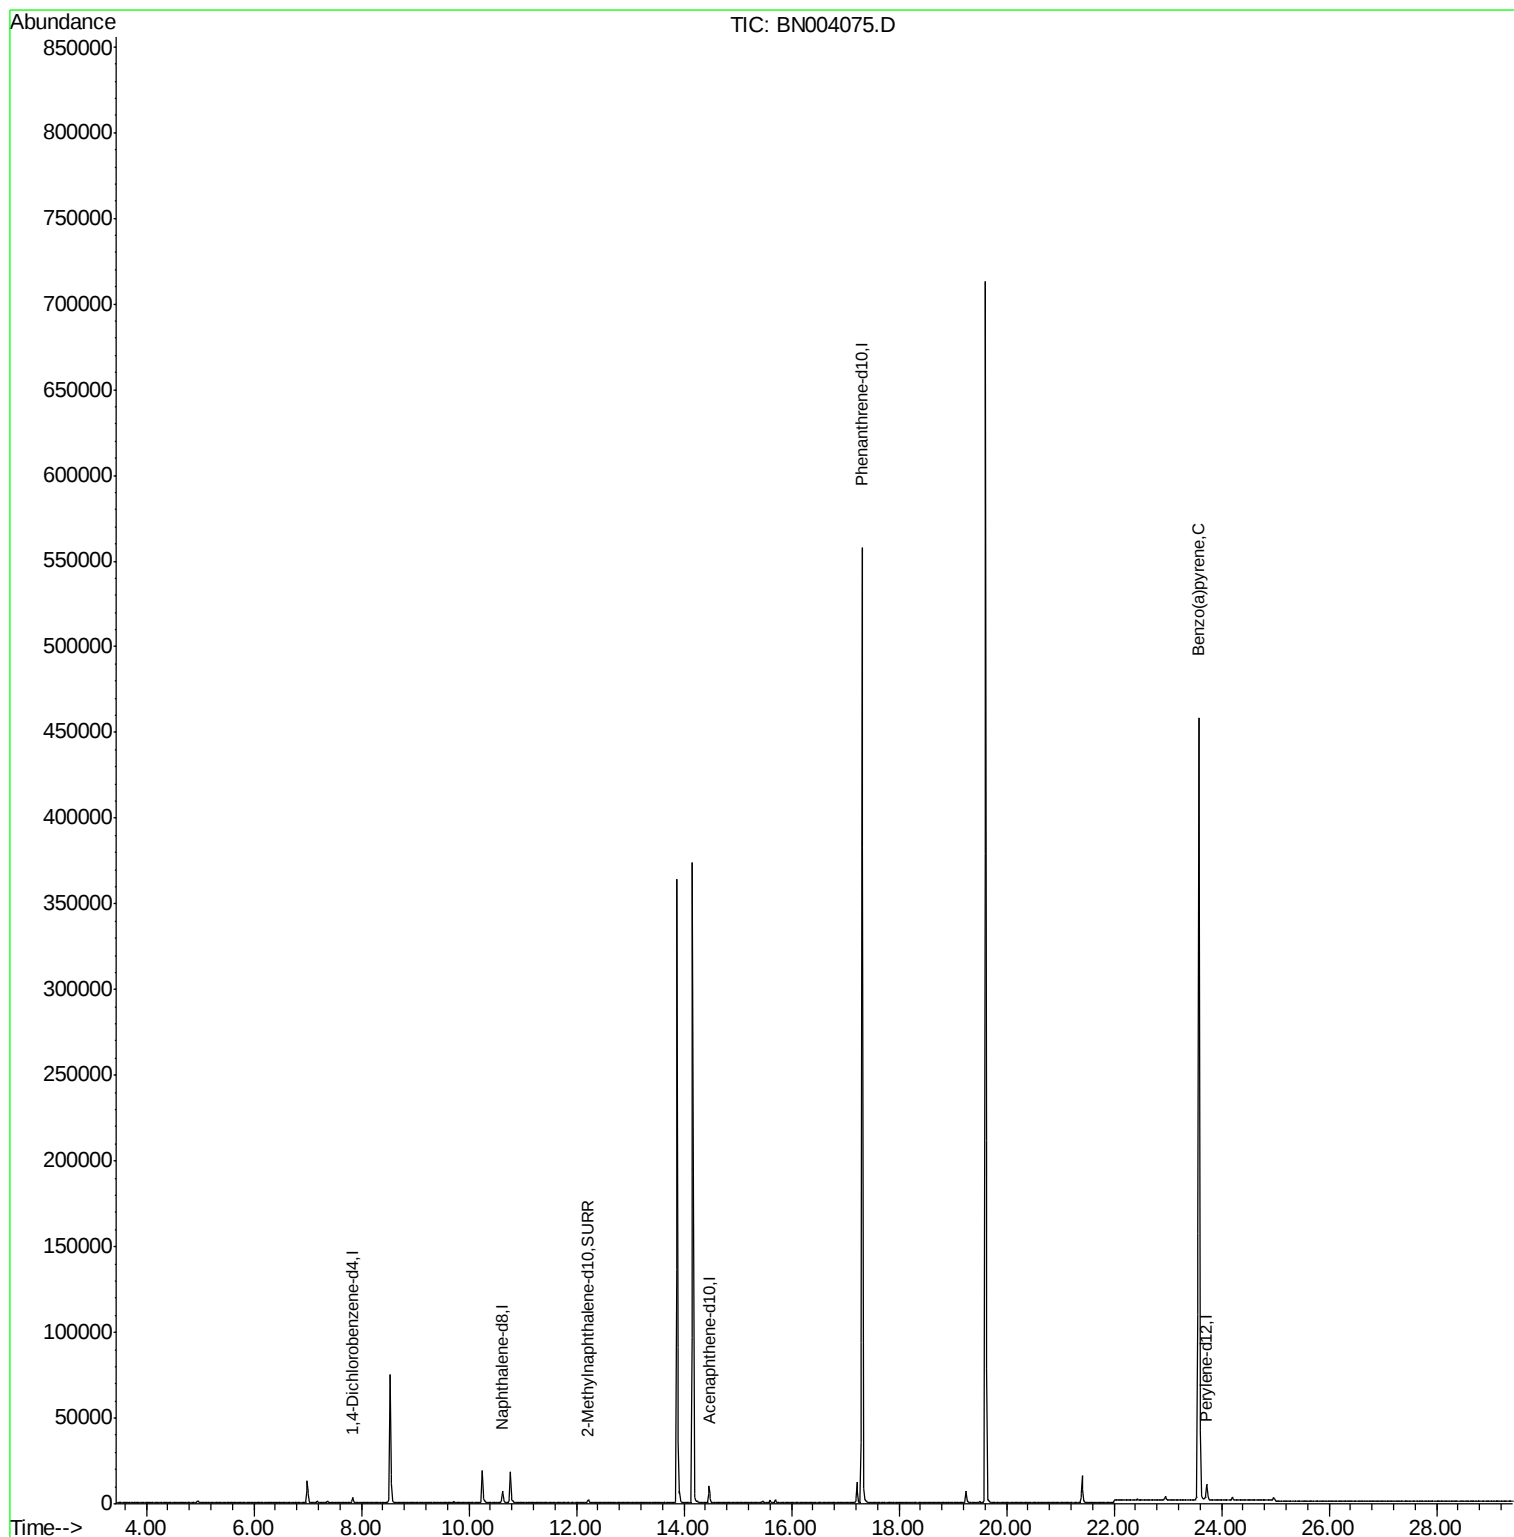

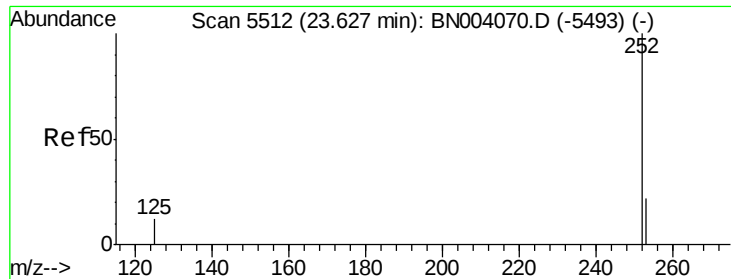

#23

Benzo(a)pyrene

Concen: 0.052 ng/ul

RT: 23.58 min Scan# 5495

Delta R.T. -0.05 min

Lab File: BN004075.D


Acq: 18 Dec 2018 14:22

Instrument :

BNA_N

ClientSampleId :

F9F45

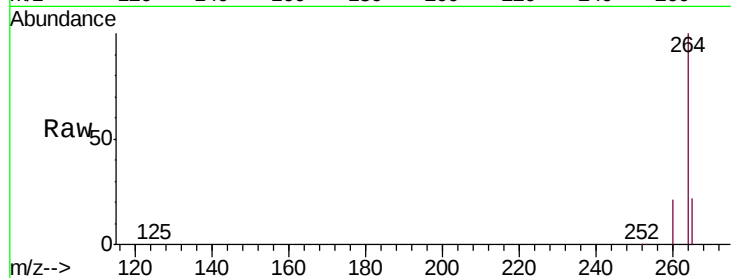

Tgt Ion:	252	Resp:	2557
Ion Ratio	Lower	Upper	
252	100		
253	46.6	19.0	28.4#
125	44.3	10.2	15.4#

