

Data Path : Z:\SVOASRV\HPCHEM1\BNA_N\DATA\BN121818\
Quantitation Report (Not Reviewed)

Data File : BN004078.D
Acq On : 18 Dec 2018 16:08
Operator : JU/SJ
Sample : PB115555BL
Misc :
ALS Vial : 10 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
SBLK55

Quant Time: Dec 19 01:58:16 2018
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SOM-EPA-SIM-BN111918.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Dec 19 01:54:36 2018
Response via : Initial Calibration


Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	7.83	152	1438	0.40	ng/ul	0.00
2) Naphthalene-d8	10.63	136	7278	0.40	ng/ul	0.00
6) Acenaphthene-d10	14.47	164	4769	0.40	ng/ul	0.00
10) Phenanthrene-d10	17.31	188	815214	0.40	ng/ul	0.10
16) Chrysene-d12	0.00	240	0	0.00	ng/ul	-21.41
20) Perylene-d12	23.73	264	14214	0.40	ng/ul	0.00
System Monitoring Compounds						
4) 2-Methylnaphthalene-d10	12.22	152	2935	0.26	ng/ul	0.00
14) Fluoranthene-d10	0.00	212	0	0.00	ng/ul	
Target Compounds						
					Qvalue	
9) Fluorene	15.46	166	1233	0.056	ng/ul#	17
23) Benzo(a)pyrene	23.58	252	3430	0.067	ng/ul#	44


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data File : BN004078.D
Acq On : 18 Dec 2018 16:08
Operator : JU/SJ
Sample : PB115555BL
Misc :
ALS Vial : 10 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
SBLK55

Quant Time: Dec 19 01:58:16 2018
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SOM-EPA-SIM-BN111918.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Dec 19 01:54:36 2018
Response via : Initial Calibration

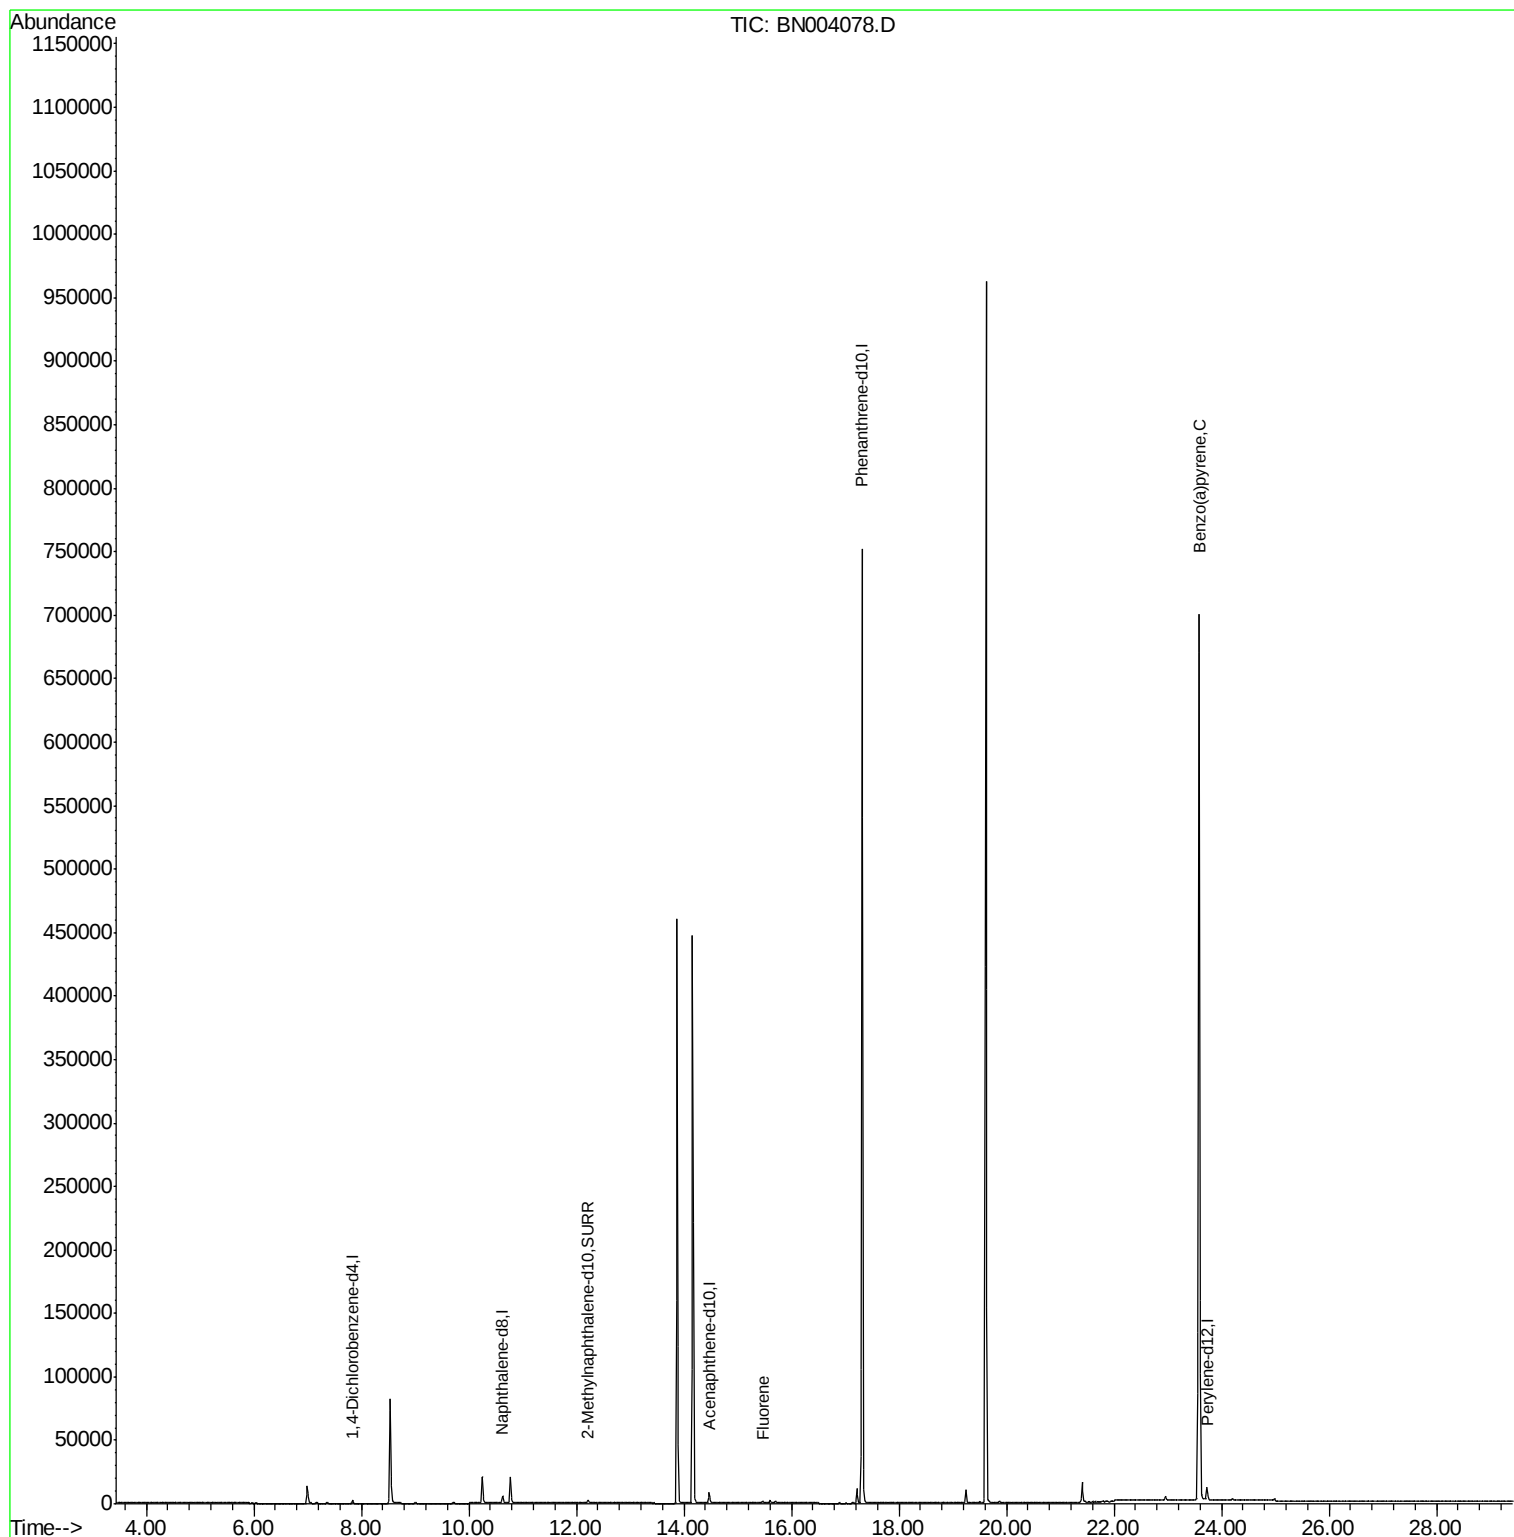

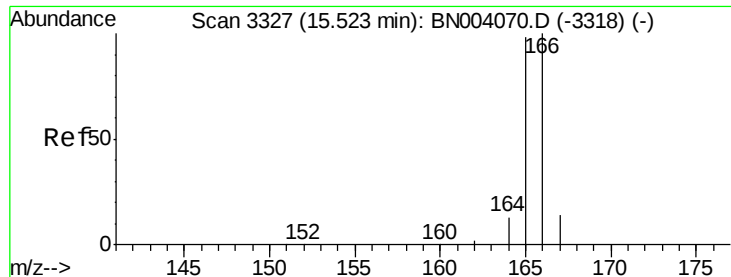

#9

Fluorene

Concen: 0.056 ng/ul

RT: 15.46 min Scan# 3314

Delta R.T. -0.06 min

Lab File: BN004078.D

Acq: 18 Dec 2018 16:08

Instrument :

BNA_N

ClientSampleId :

SBLK55


Tgt Ion:166 Resp: 1233

Ion Ratio Lower Upper




166 100

165 10.8 78.3 117.5#

167 33.8 11.3 16.9#

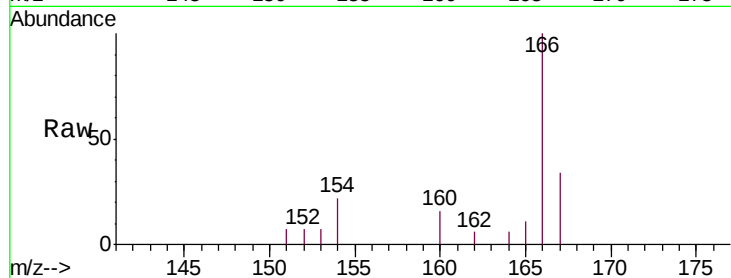

Abundance Ion 166.00 (165.70 to 166.70): E
Ion 165.00 (164.70 to 165.70): E
Ion 167.00 (166.70 to 167.70): E

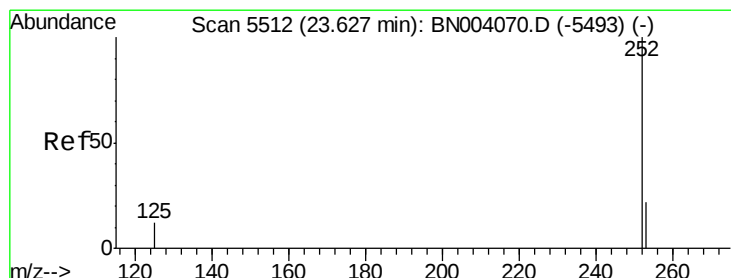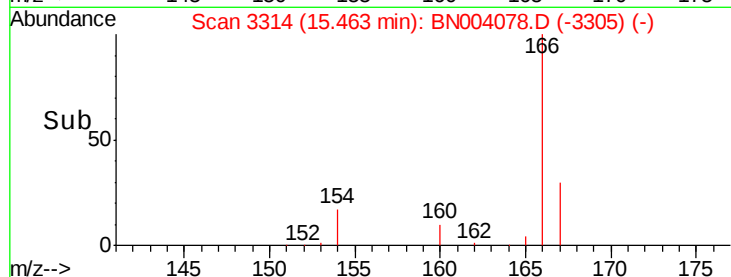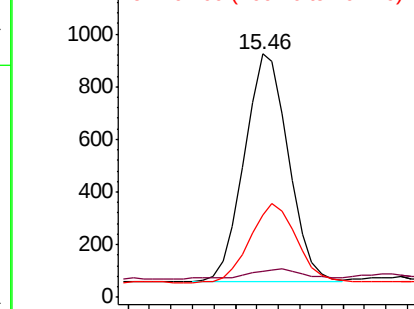

#23

Benzo(a)pyrene

Concen: 0.067 ng/ul

RT: 23.58 min Scan# 5497

Delta R.T. -0.04 min

Lab File: BN004078.D

Acq: 18 Dec 2018 16:08


Tgt Ion:252 Resp: 3430

Ion Ratio Lower Upper

252 100

253 42.5 19.0 28.4#

125 47.8 10.2 15.4#

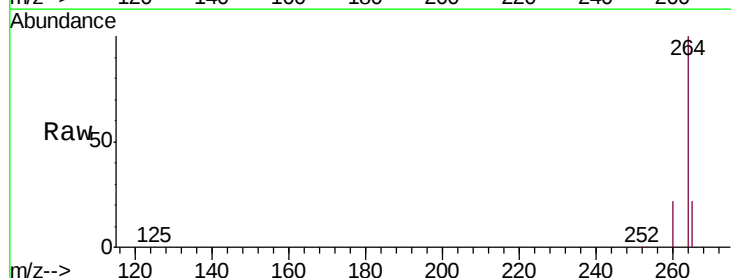

Abundance Ion 252.00 (251.70 to 252.70): E
Ion 253.00 (252.70 to 253.70): E
Ion 125.00 (124.70 to 125.70): E

