

Data Path : Z:\SVOASRV\HPCHEM1\BNA_N\DATA\BN121818\
Quantitation Report (Not Reviewed)

Data File : BN004083.D
Acq On : 18 Dec 2018 19:04
Operator : JU/SJ
Sample : J6271-07
Misc :
ALS Vial : 15 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
F9F14

Quant Time: Dec 19 01:58:53 2018
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SOM-EPA-SIM-BN111918.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Dec 19 01:54:36 2018
Response via : Initial Calibration


Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	7.83	152	1705	0.40	ng/ul	0.00
2) Naphthalene-d8	10.63	136	8494	0.40	ng/ul	0.00
6) Acenaphthene-d10	14.47	164	5295	0.40	ng/ul	0.00
10) Phenanthrene-d10	17.31	188	768547	0.40	ng/ul	0.10
16) Chrysene-d12	0.00	240	0	0.00	ng/ul	-21.41
20) Perylene-d12	23.73	264	13769	0.40	ng/ul	0.00
System Monitoring Compounds						
4) 2-Methylnaphthalene-d10	12.21	152	3202	0.25	ng/ul	0.00
14) Fluoranthene-d10	0.00	212	0	0.00	ng/ul	
Target Compounds						
23) Benzo(a)pyrene	23.58	252	2501	0.051	ng/ul#	Qvalue 54


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data File : BN004083.D
Acq On : 18 Dec 2018 19:04
Operator : JU/SJ
Sample : J6271-07
Misc :
ALS Vial : 15 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
F9F14

Quant Time: Dec 19 01:58:53 2018
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SOM-EPA-SIM-BN111918.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Dec 19 01:54:36 2018
Response via : Initial Calibration

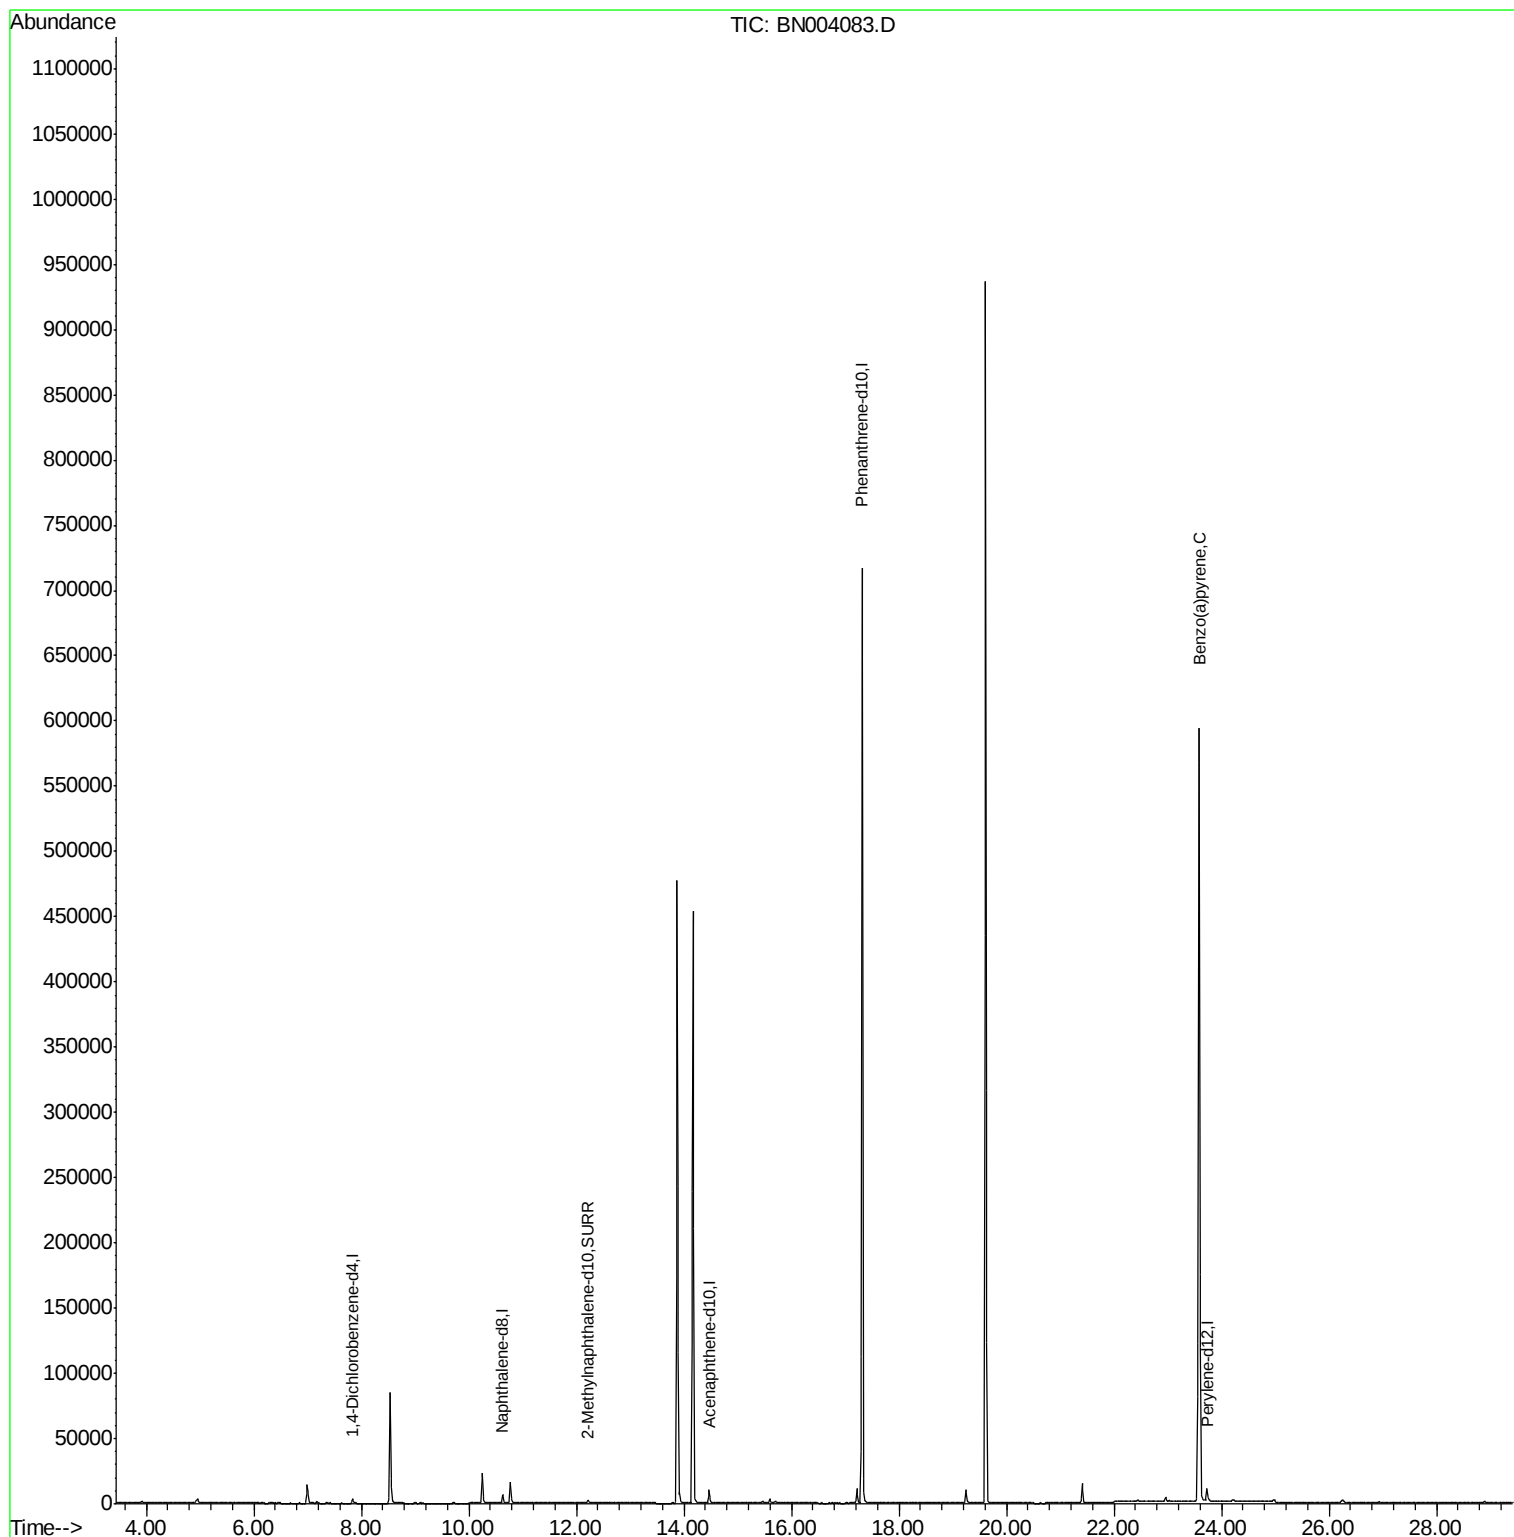

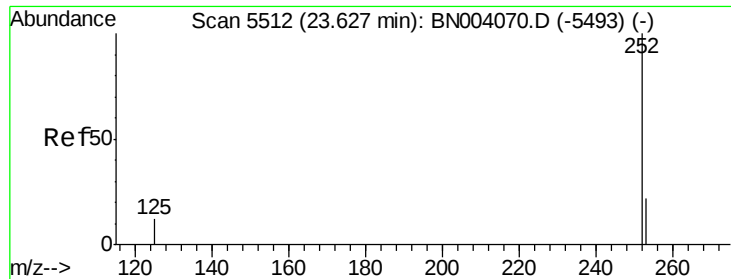

#23

Benzo(a)pyrene

Concen: 0.051 ng/ul

RT: 23.58 min Scan# 5496

Delta R.T. -0.05 min

Lab File: BN004083.D


Acq: 18 Dec 2018 19:04

Instrument :

BNA_N

ClientSampleId :

F9F14

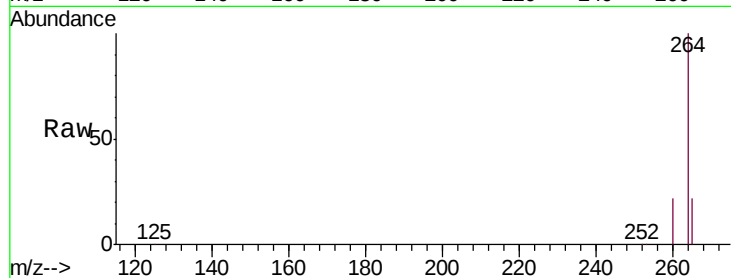


Tgt Ion: 252 Resp: 2501

Ion Ratio Lower Upper

252 100

253 41.3 19.0 28.4#

125 38.7 10.2 15.4#

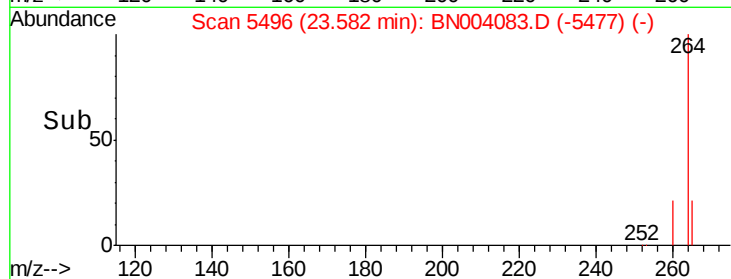

Abundance Ion 252.00 (251.70 to 252.70): E

Ion 253.00 (252.70 to 253.70): E

Ion 125.00 (124.70 to 125.70): E

