

Data File : BN004090.D
Acq On : 18 Dec 2018 23:09
Operator : JU/SJ
Sample : J6271-11
Misc :
ALS Vial : 21 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
F9E26

Quant Time: Dec 19 04:12:42 2018
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SOM-EPA-SIM-BN111918.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Dec 19 04:08:55 2018
Response via : Initial Calibration


Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	7.83	152	1721	0.40	ng/ul	0.00
2) Naphthalene-d8	10.63	136	8398	0.40	ng/ul	0.00
6) Acenaphthene-d10	14.47	164	5199	0.40	ng/ul	0.00
10) Phenanthrene-d10	17.31	188	754441	0.40	ng/ul	0.10
16) Chrysene-d12	0.00	240	0	0.00	ng/ul	-21.40
20) Perylene-d12	23.72	264	14087	0.40	ng/ul	0.00
System Monitoring Compounds						
4) 2-Methylnaphthalene-d10	12.22	152	3093	0.24	ng/ul	0.00
14) Fluoranthene-d10	0.00	212	0	0.00	ng/ul	
Target Compounds						
21) Benzo(b)fluoranthene	23.02	252	1264	0.022	ng/ul#	8
26) Benzo(g,h,i)perylene	26.82	276	1138	0.023	ng/ul#	28


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data File : BN004090.D
Acq On : 18 Dec 2018 23:09
Operator : JU/SJ
Sample : J6271-11
Misc :
ALS Vial : 21 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
F9E26

Quant Time: Dec 19 04:12:42 2018
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SOM-EPA-SIM-BN111918.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Dec 19 04:08:55 2018
Response via : Initial Calibration

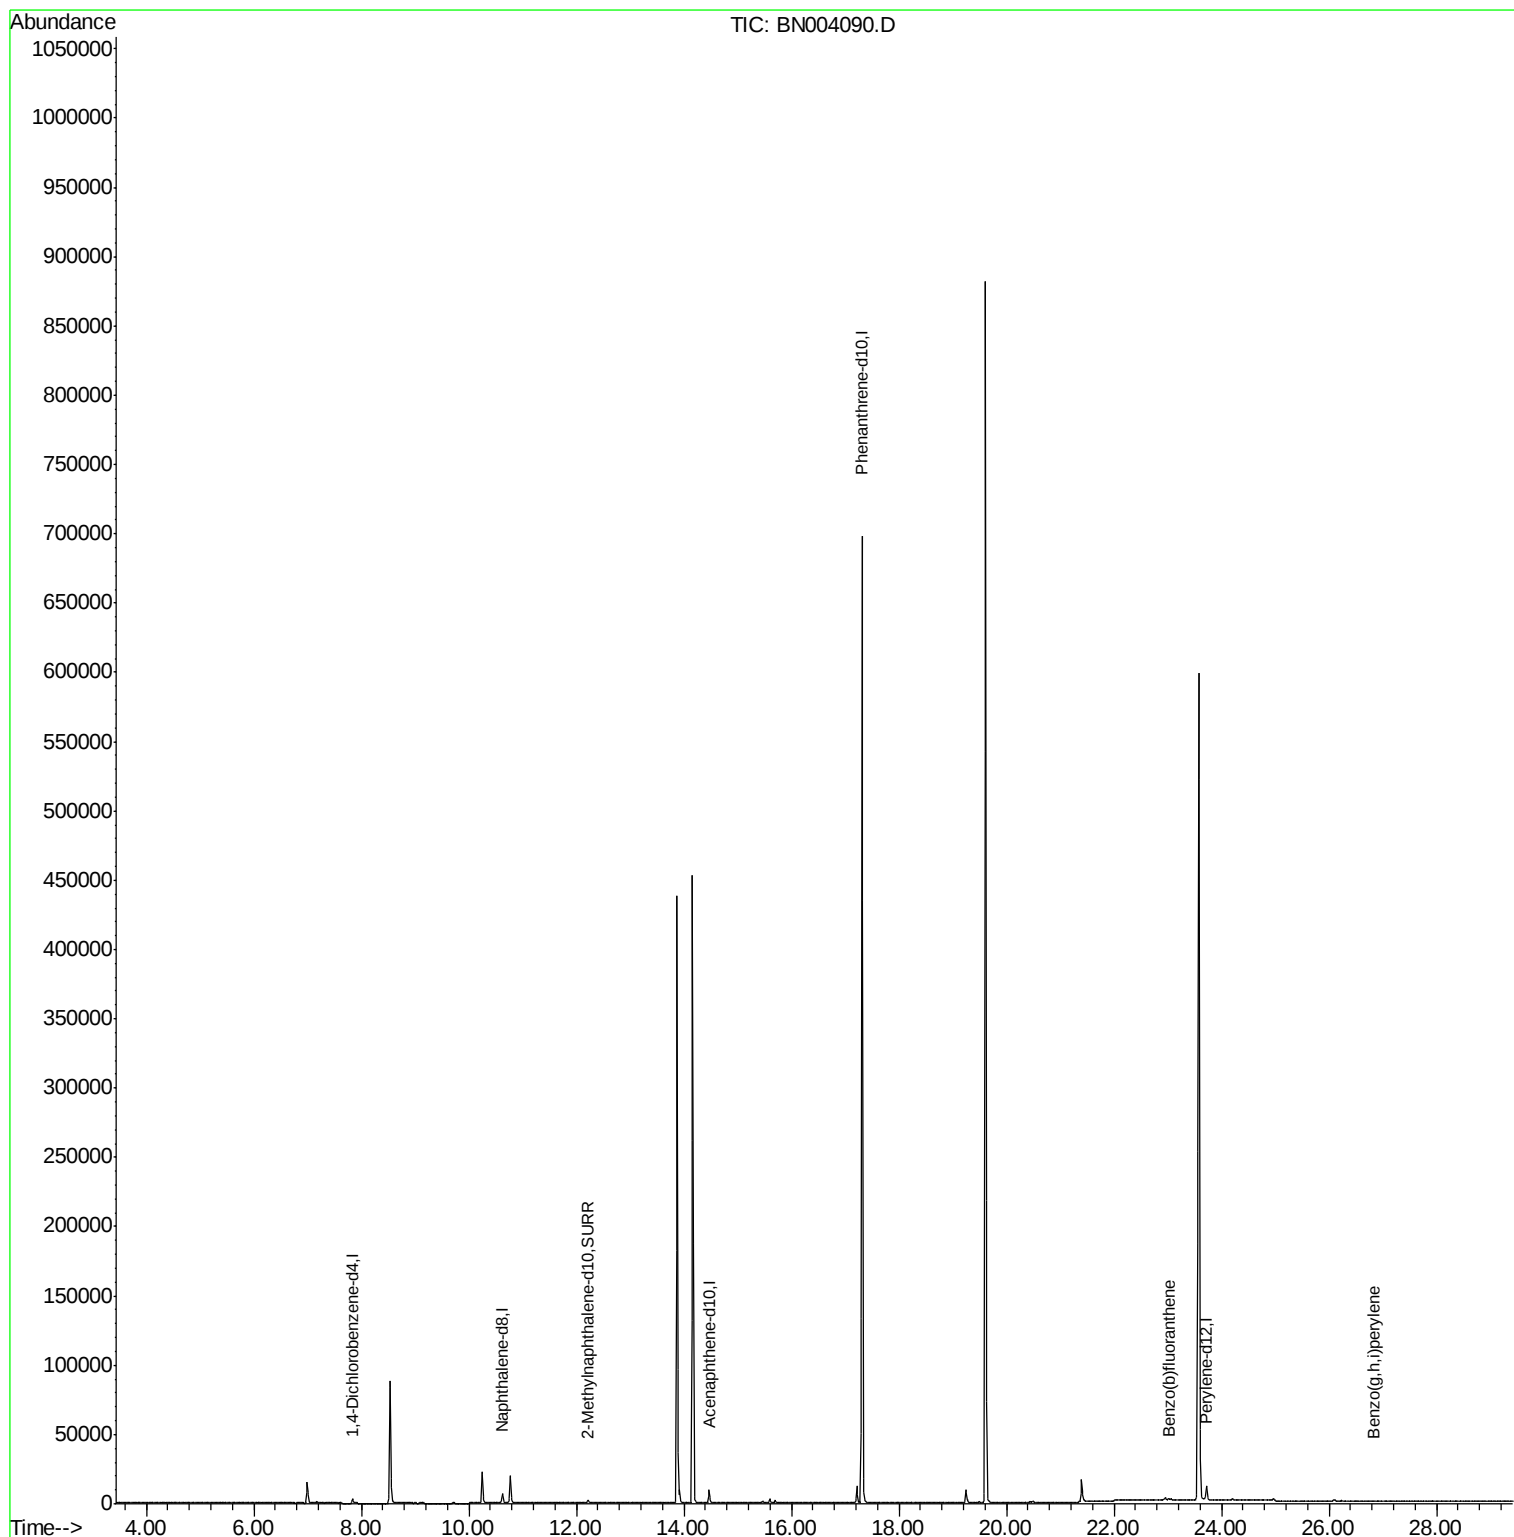

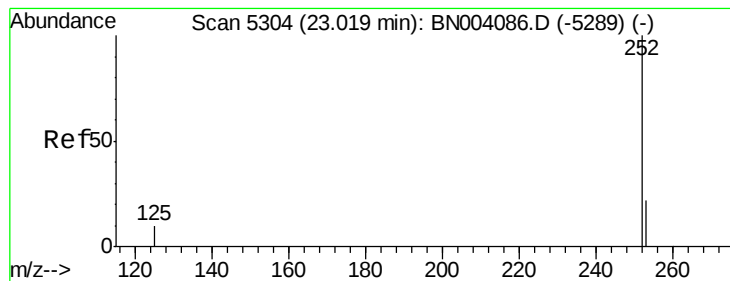

#21

Benzo(b)fluoranthene

Concen: 0.022 ng/u1

RT: 23.02 min Scan# 5303

Delta R.T. -0.00 min

Lab File: BN004090.D

Acq: 18 Dec 2018 23:09

Instrument :

BNA_N

ClientSampleId :

F9E26


Tgt Ion:252 Resp: 1264

Ion Ratio Lower Upper

252 100

253 57.8 0.0 46.0#




125 62.5 0.0 22.4#

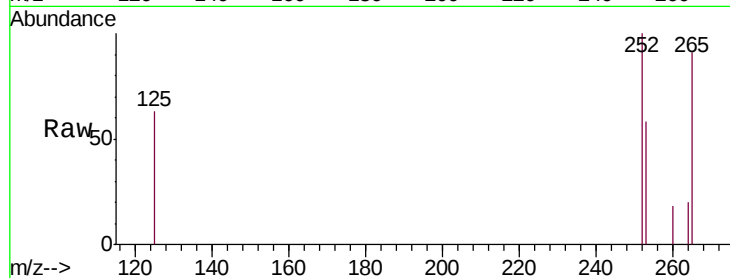

Abundance Ion 252.00 (251.70 to 252.70): E

Ion 253.00 (252.70 to 253.70): E

Ion 125.00 (124.70 to 125.70): E

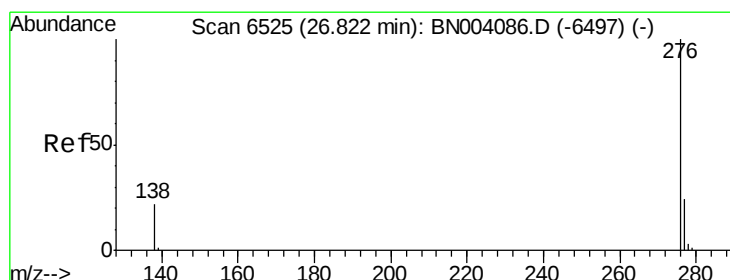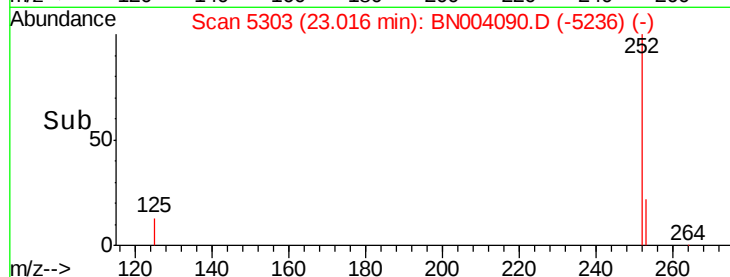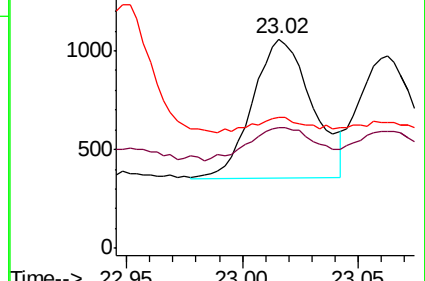

#26

Benzo(g,h,i)perylene

Concen: 0.023 ng/u1

RT: 26.82 min Scan# 6524

Delta R.T. -0.00 min

Lab File: BN004090.D

Acq: 18 Dec 2018 23:09


Tgt Ion:276 Resp: 1138

Ion Ratio Lower Upper

276 100

138 61.9 17.7 26.5#

277 54.5 19.3 28.9#

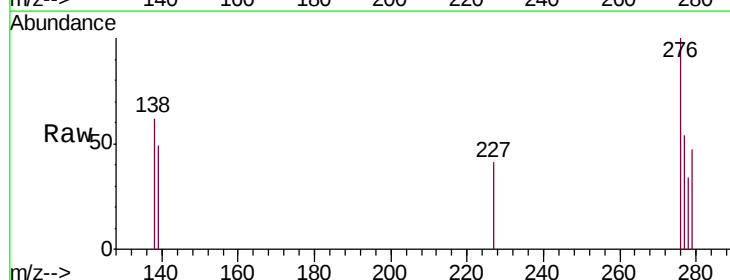

Abundance Ion 276.00 (275.70 to 276.70): E

Ion 138.00 (137.70 to 138.70): E

Ion 277.00 (276.70 to 277.70): E

