

Data Path : Z:\SVOASRV\HPCHEM1\BNA_N\DATA\BN121818\
Quantitation Report (Not Reviewed)

Data File : BN004098.D
Acq On : 19 Dec 2018 03:49
Operator : JU/SJ
Sample : J6271-19
Misc :
ALS Vial : 29 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
F9E34

Quant Time: Dec 19 04:58:44 2018
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SOM-EPA-SIM-BN111918.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Dec 19 04:08:55 2018
Response via : Initial Calibration


Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	7.83	152	2121	0.40	ng/ul	0.00
2) Naphthalene-d8	10.63	136	10188	0.40	ng/ul	0.00
6) Acenaphthene-d10	14.47	164	6066	0.40	ng/ul	0.00
10) Phenanthrene-d10	17.31	188	665858	0.40	ng/ul	0.10
16) Chrysene-d12	0.00	240	0	0.00	ng/ul	-21.40
20) Perylene-d12	23.72	264	14702	0.40	ng/ul	0.00
System Monitoring Compounds						
4) 2-Methylnaphthalene-d10	12.22	152	2888	0.18	ng/ul	0.00
14) Fluoranthene-d10	0.00	212	0	0.00	ng/ul	
Target Compounds						
23) Benzo(a)pyrene	23.57	252	2635	0.050	ng/ul#	Qvalue 52


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data File : BN004098.D
Acq On : 19 Dec 2018 03:49
Operator : JU/SJ
Sample : J6271-19
Misc :
ALS Vial : 29 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
F9E34

Quant Time: Dec 19 04:58:44 2018
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SOM-EPA-SIM-BN111918.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Dec 19 04:08:55 2018
Response via : Initial Calibration

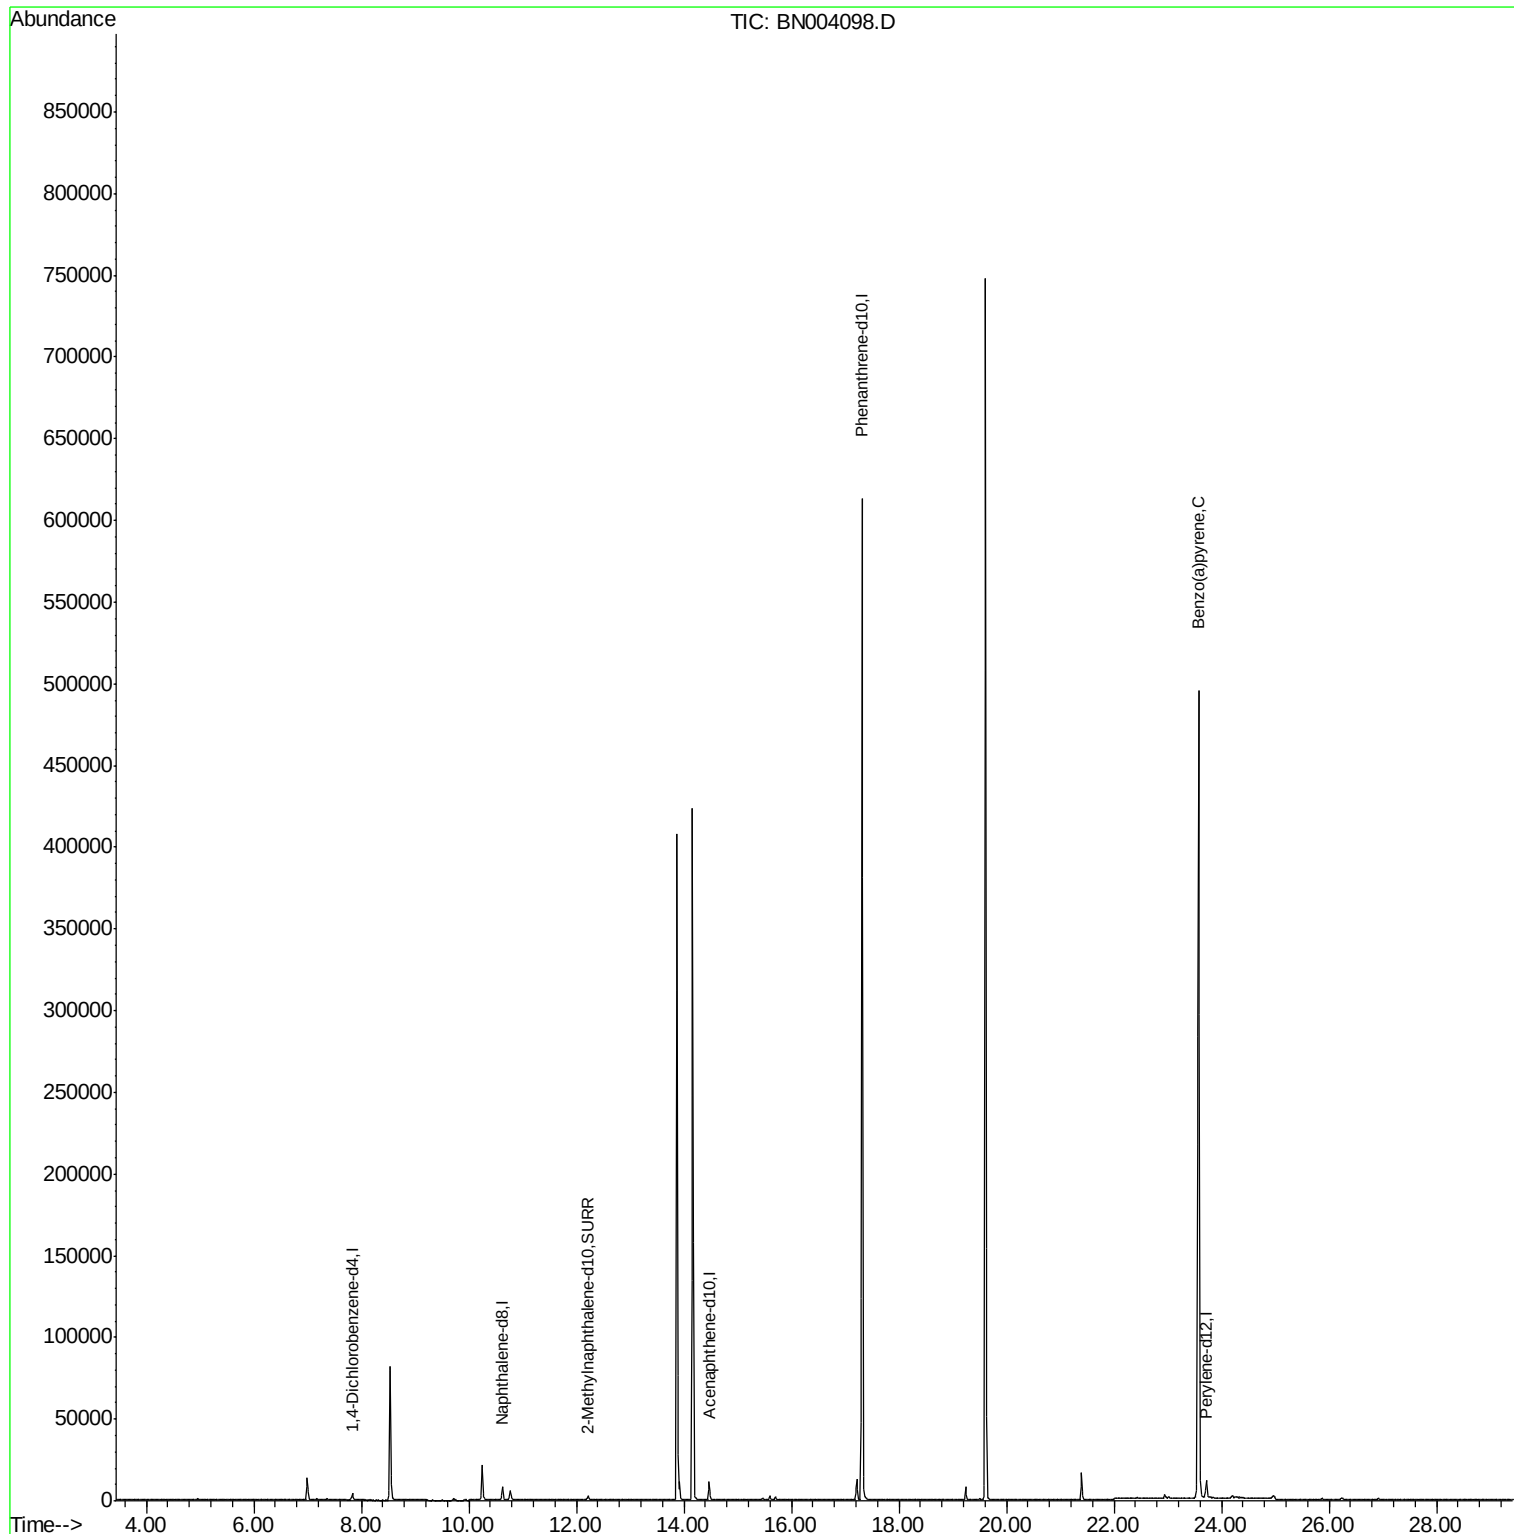

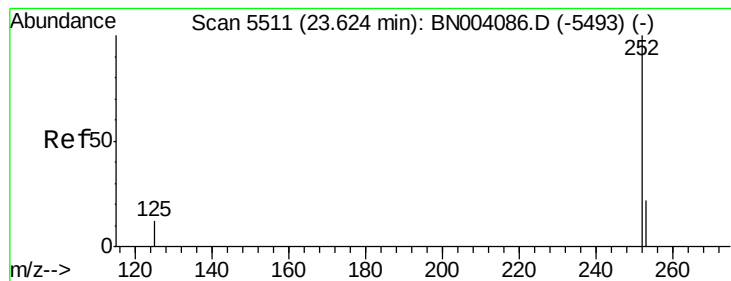

#23

Benzo(a)pyrene

Concen: 0.050 ng/ul

RT: 23.57 min Scan# 5492

Delta R.T. -0.05 min

Lab File: BN004098.D


Acq: 19 Dec 2018 03:49

Instrument :

BNA_N

ClientSampleId :

F9E34

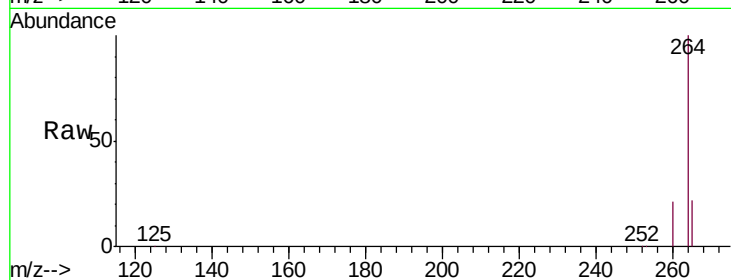


Tgt Ion: 252 Resp: 2635

Ion Ratio Lower Upper

252 100

253 43.1 19.0 28.4#

125 37.7 10.2 15.4#

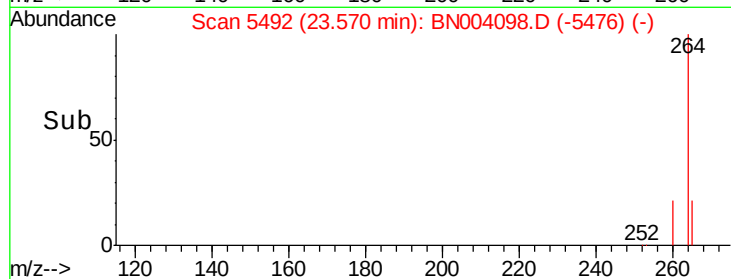

Abundance Ion 252.00 (251.70 to 252.70): E

2000 Ion 253.00 (252.70 to 253.70): E

Ion 125.00 (124.70 to 125.70): E

