

Data Path : Z:\SVOASRV\HPCHEM1\BNA_N\DATA\BN121818\
Quantitation Report (Not Reviewed)

Data File : BN004099.D
Acq On : 19 Dec 2018 04:24
Operator : JU/SJ
Sample : J6271-20
Misc :
ALS Vial : 30 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
F9E35

Quant Time: Dec 19 04:58:49 2018
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SOM-EPA-SIM-BN111918.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Dec 19 04:08:55 2018
Response via : Initial Calibration


Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	7.83	152	1969	0.40	ng/ul	0.00
2) Naphthalene-d8	10.63	136	9476	0.40	ng/ul	0.00
6) Acenaphthene-d10	14.47	164	5882	0.40	ng/ul	0.00
10) Phenanthrene-d10	17.31	188	1177414	0.40	ng/ul	0.10
16) Chrysene-d12	0.00	240	0	0.00	ng/ul	-21.40
20) Perylene-d12	23.72	264	14839	0.40	ng/ul	0.00
System Monitoring Compounds						
4) 2-Methylnaphthalene-d10	12.22	152	4989	0.34	ng/ul	0.00
14) Fluoranthene-d10	0.00	212	0	0.00	ng/ul	
Target Compounds						
23) Benzo(a)pyrene	23.58	252	4727	0.089	ng/ul#	Qvalue 71


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data File : BN004099.D
Acq On : 19 Dec 2018 04:24
Operator : JU/SJ
Sample : J6271-20
Misc :
ALS Vial : 30 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
F9E35

Quant Time: Dec 19 04:58:49 2018
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SOM-EPA-SIM-BN111918.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Dec 19 04:08:55 2018
Response via : Initial Calibration

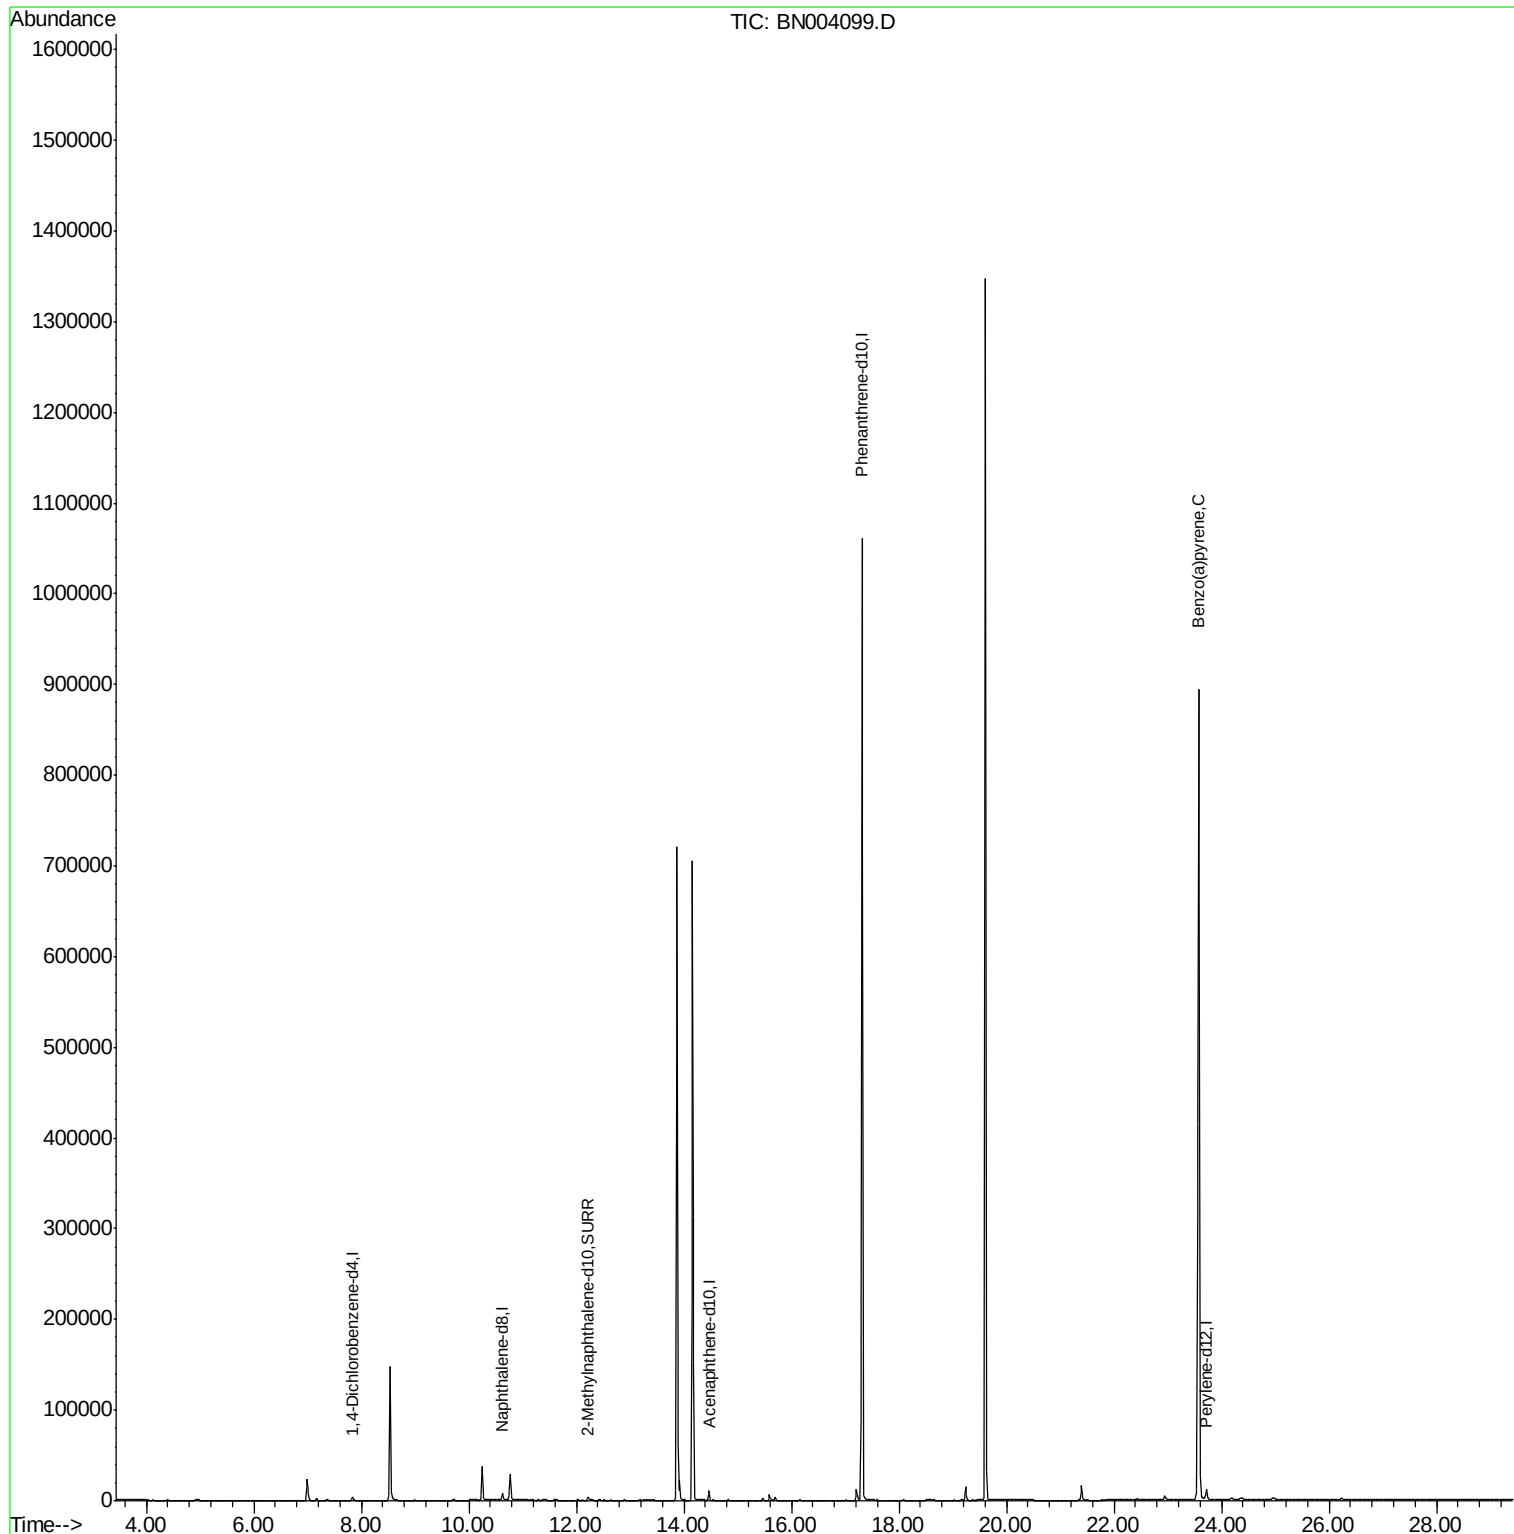

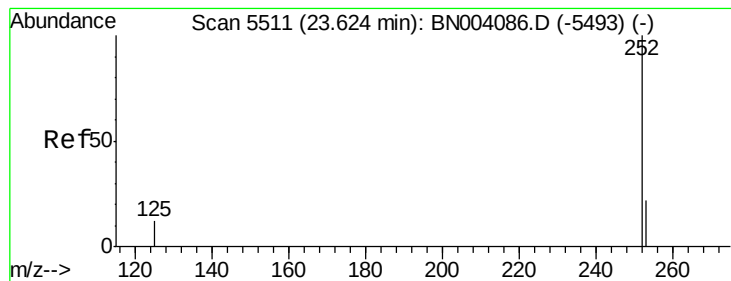

#23

Benzo(a)pyrene

Concen: 0.089 ng/ul

RT: 23.58 min Scan# 5495

Delta R.T. -0.05 min

Lab File: BN004099.D


Acq: 19 Dec 2018 04:24

Instrument :

BNA_N

ClientSampleId :

F9E35

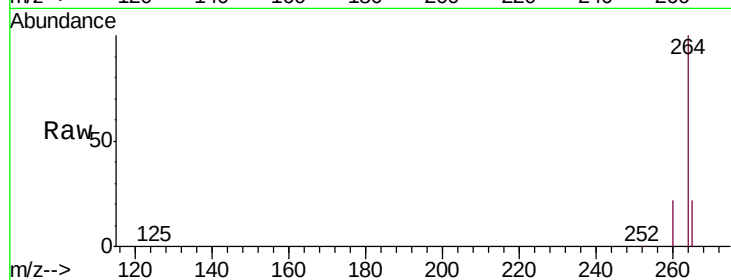

Tgt Ion: 252 Resp: 4727

Ion Ratio Lower Upper

252 100

253 35.1 19.0 28.4#

125 28.9 10.2 15.4#

