

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN121818\
Quantitation Report (QT Reviewed)


Data File : BN004078.D
Acq On : 18 Dec 2018 16:08
Operator : JU/SJ
Sample : PB115555BL
Misc :
ALS Vial : 10 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
SBLK55

Manual Integrations
APPROVED

Sohil
12/19/2018 4:16:01 PM

Quant Time: Dec 19 03:22:29 2018
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SOM-EPA-SIM-BN111918.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Dec 19 01:54:36 2018
Response via : Initial Calibration

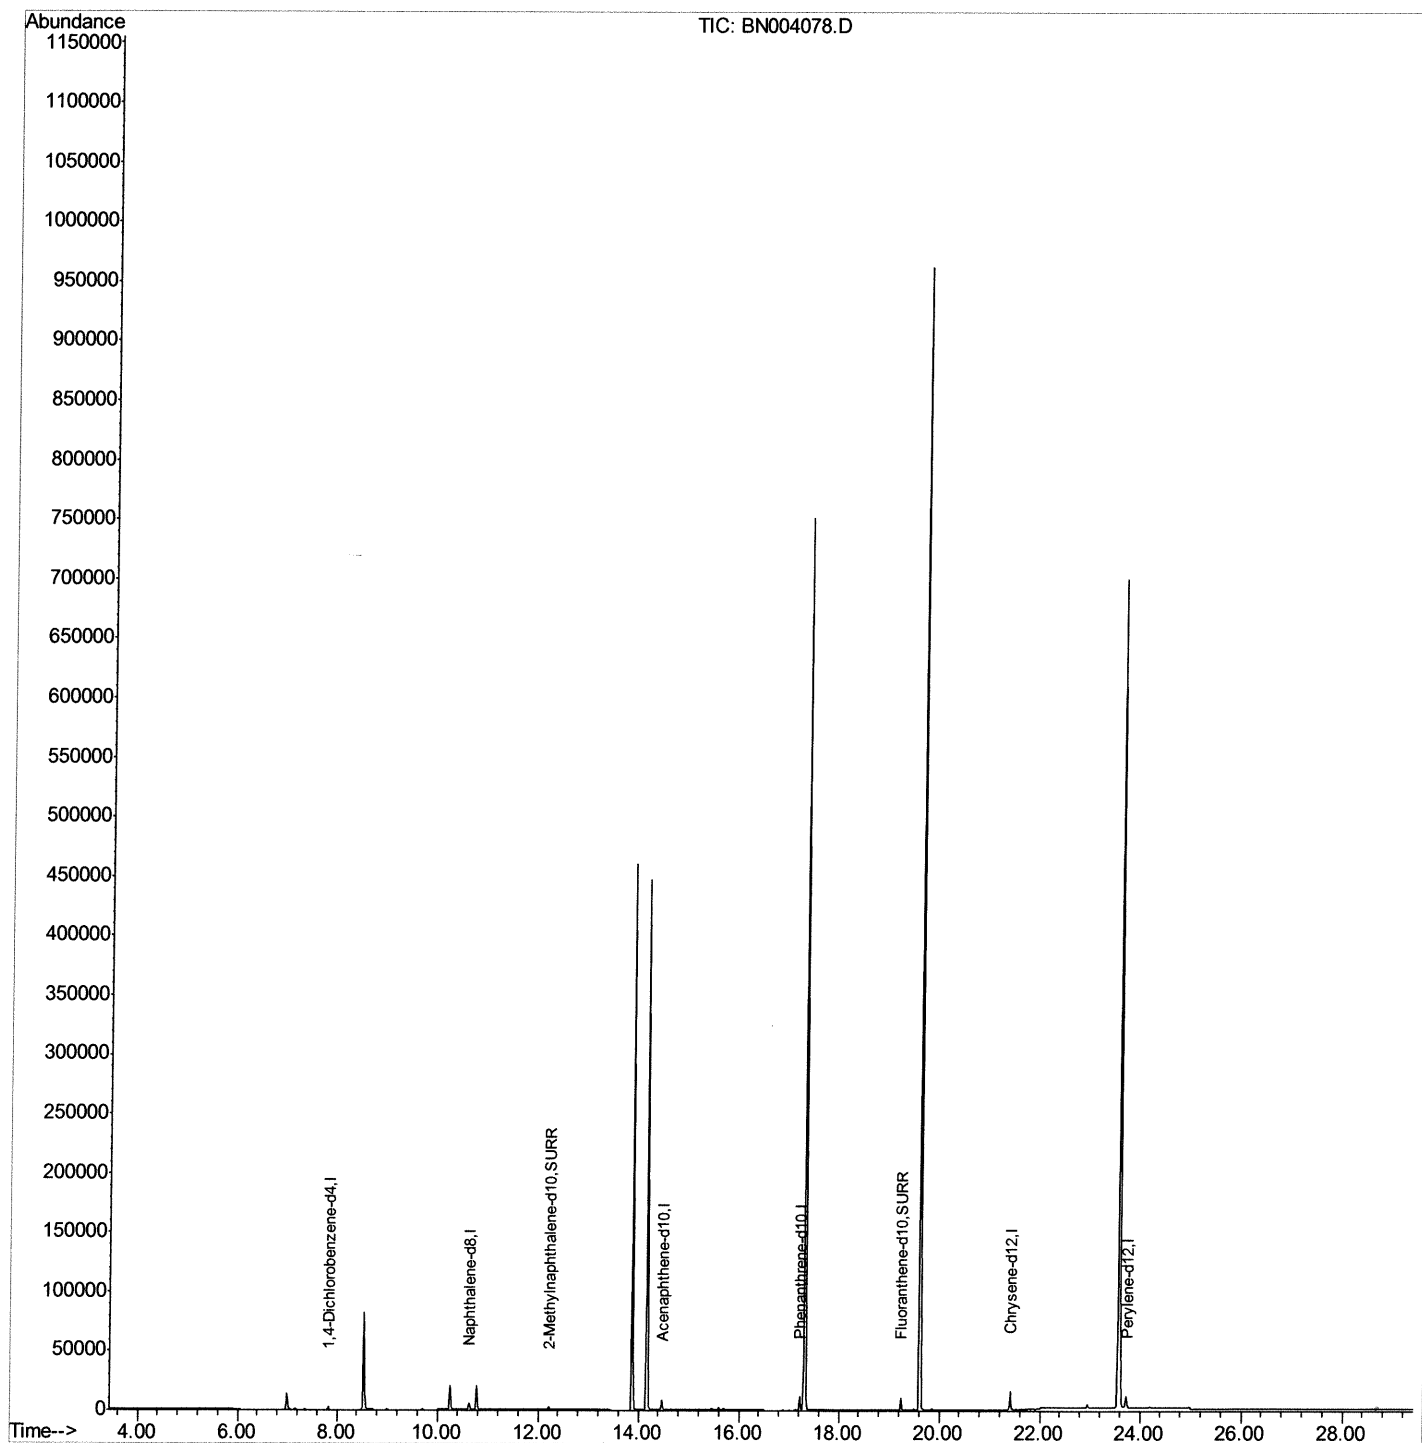

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN121818\
Quantitation Report (Qedit)




Data File : BN004078.D
Acq On : 18 Dec 2018 16:08
Operator : JU/SJ
Sample : PB115555BL
Misc :
ALS Vial : 10 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
SBLK55

Manual Integrations
APPROVED

Sohil
12/19/2018 4:16:01 PM

Quant Time: Dec 19 01:58:16 2018
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SOM-EPA-SIM-BN111918.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Dec 19 01:54:36 2018
Response via : Initial Calibration

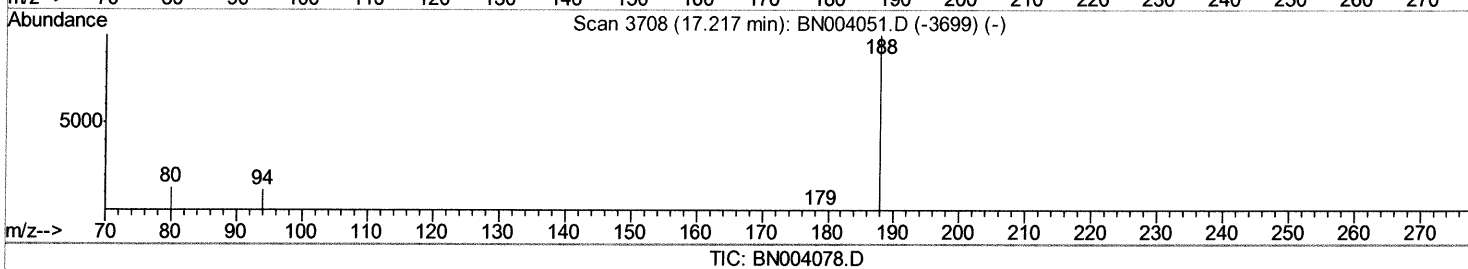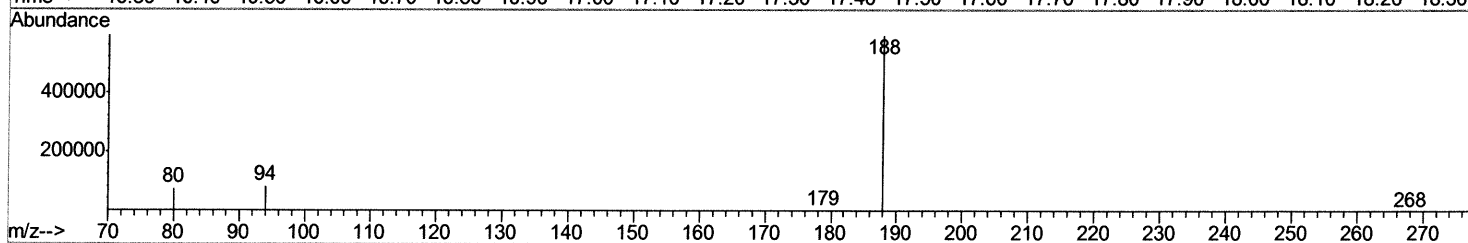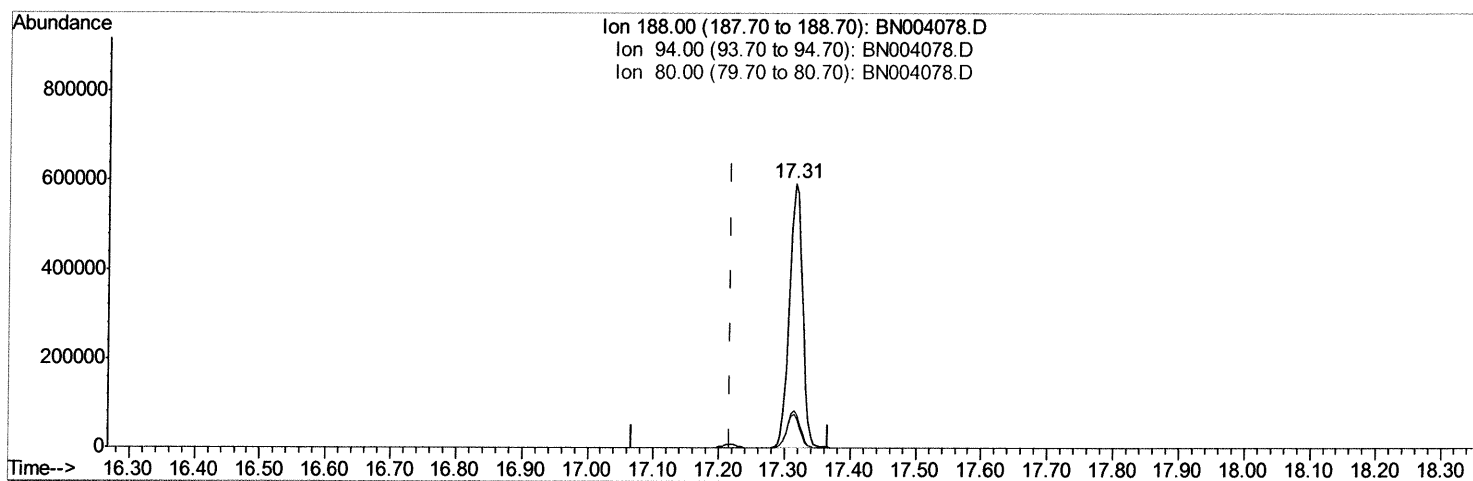

(10) Phenanthrene-d10 (I)

17.314min (+0.097) 0.40ng/ul

response 815214

Ion	Exp%	Act%
188.00	100	100
94.00	10.40	13.98#
80.00	11.60	12.66
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN121818\
Quantitation Report (Qedit)




Data File : BN004078.D
Acq On : 18 Dec 2018 16:08
Operator : JU/SJ
Sample : PB115555BL
Misc :
ALS Vial : 10 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
SBLK55

Manual Integrations
APPROVED

Sohil
12/19/2018 4:16:01 PM

Quant Time: Dec 19 01:58:16 2018
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SOM-EPA-SIM-BN111918.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Dec 19 01:54:36 2018
Response via : Initial Calibration

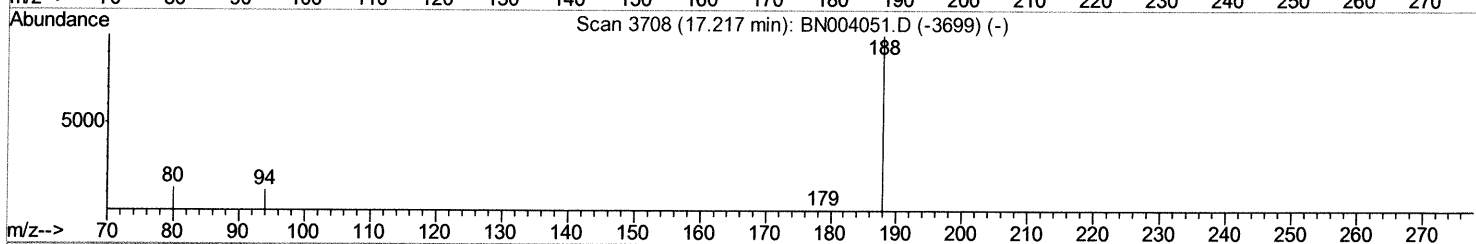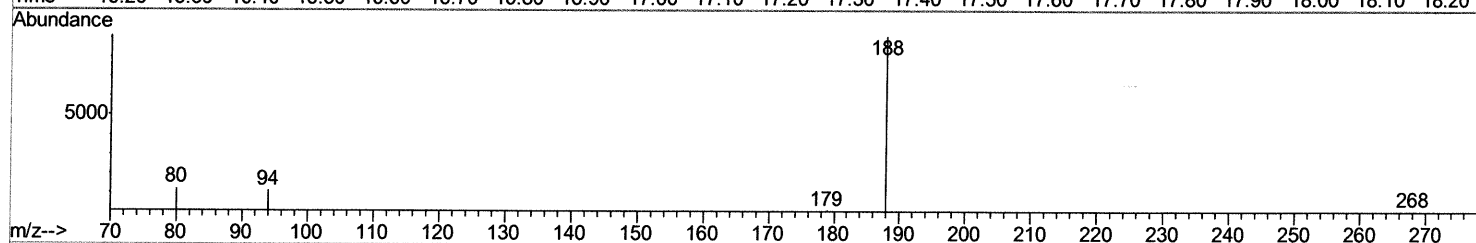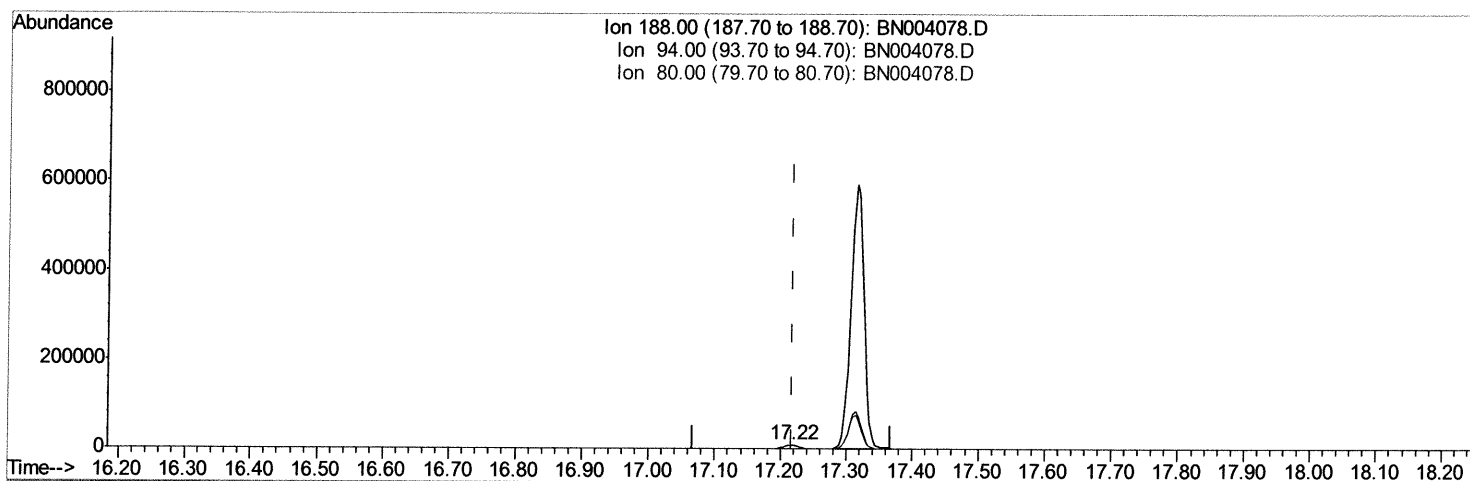

TIC: BN004078.D

(10) Phenanthrene-d10 (I)

17.217min (-0.000) 0.40ng/ul m

response 12538

Ion	Exp%	Act%
188.00	100	100
94.00	10.40	12.02
80.00	11.60	13.13
0.00	0.00	0.00

> SJ
12/19/18

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN121818\
Quantitation Report (Qedit)




Data File : BN004078.D
Acq On : 18 Dec 2018 16:08
Operator : JU/SJ
Sample : PB115555BL
Misc :
ALS Vial : 10 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
SBLK55

Manual Integrations
APPROVED

Sohil
12/19/2018 4:16:01 PM

Quant Time: Dec 19 03:21:01 2018
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SOM-EPA-SIM-BN111918.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Dec 19 01:54:36 2018
Response via : Initial Calibration

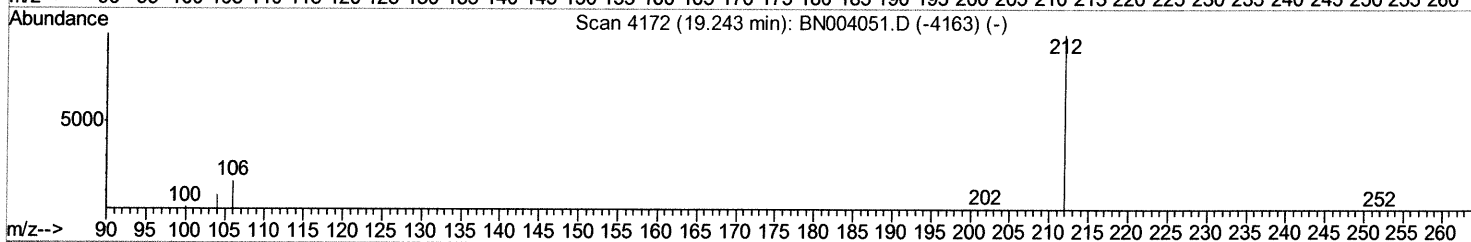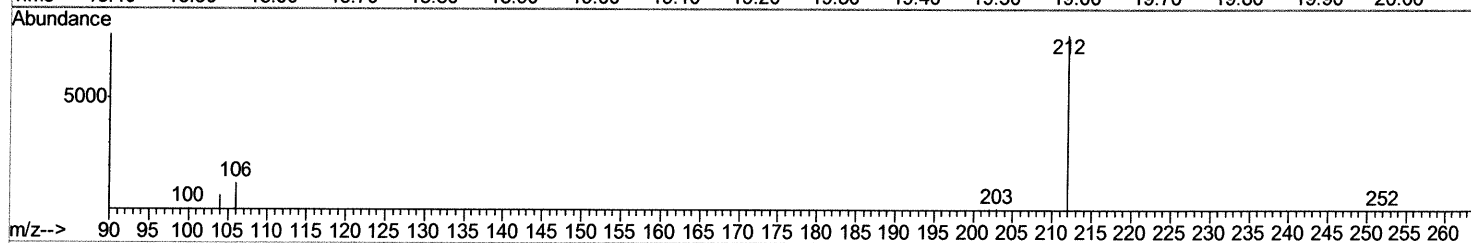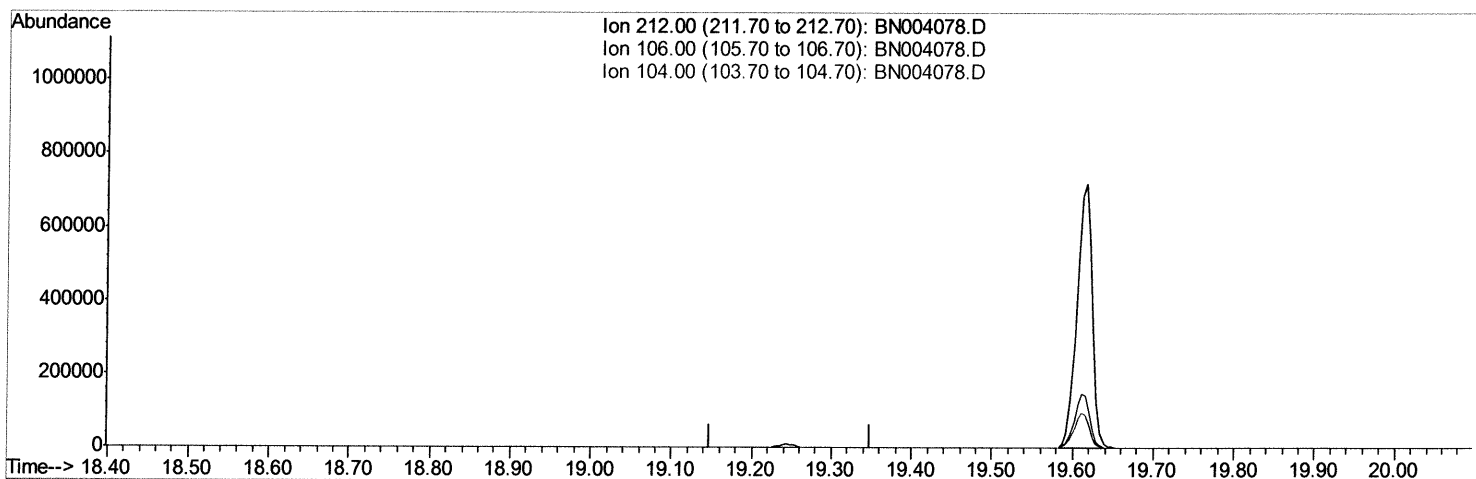

TIC: BN004078.D

(14) Fluoranthene-d10 (SURR)

19.248min (-19.248) 0.00ng/ul

response 0

Ion	Exp%	Act%
212.00	100	0.00
106.00	14.20	0.00#
104.00	8.00	0.00#
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN121818\
Quantitation Report (Qedit)




Data File : BN004078.D
Acq On : 18 Dec 2018 16:08
Operator : JU/SJ
Sample : PB115555BL
Misc :
ALS Vial : 10 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
SBLK55

Manual Integrations
APPROVED

Sohil
12/19/2018 4:16:01 PM

Quant Time: Dec 19 03:21:01 2018
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SOM-EPA-SIM-BN111918.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Dec 19 01:54:36 2018
Response via : Initial Calibration

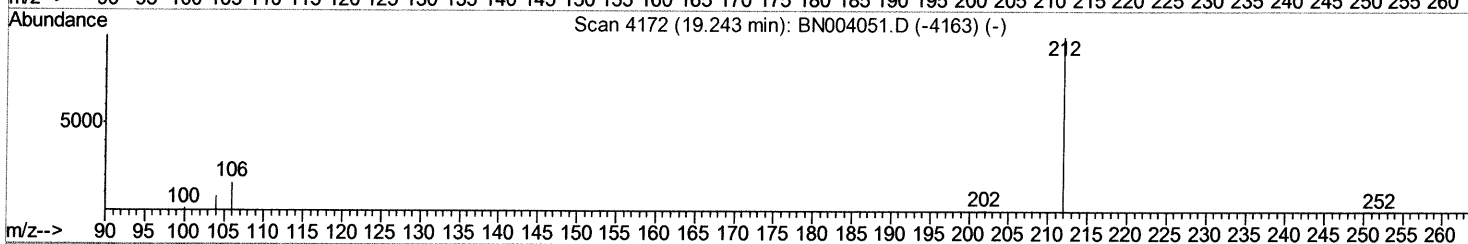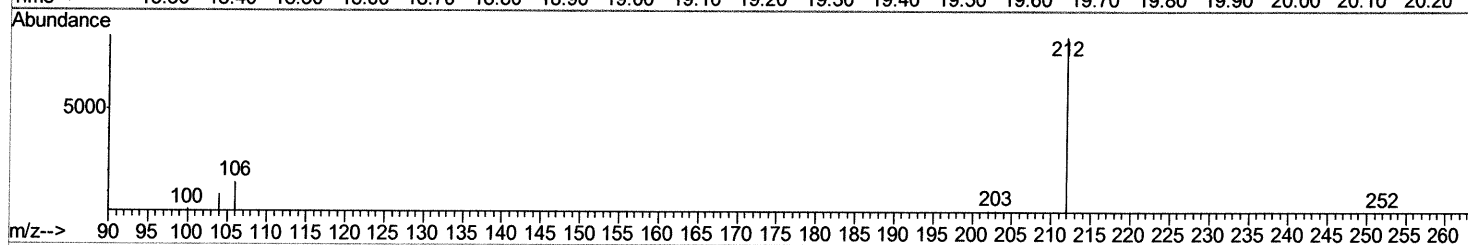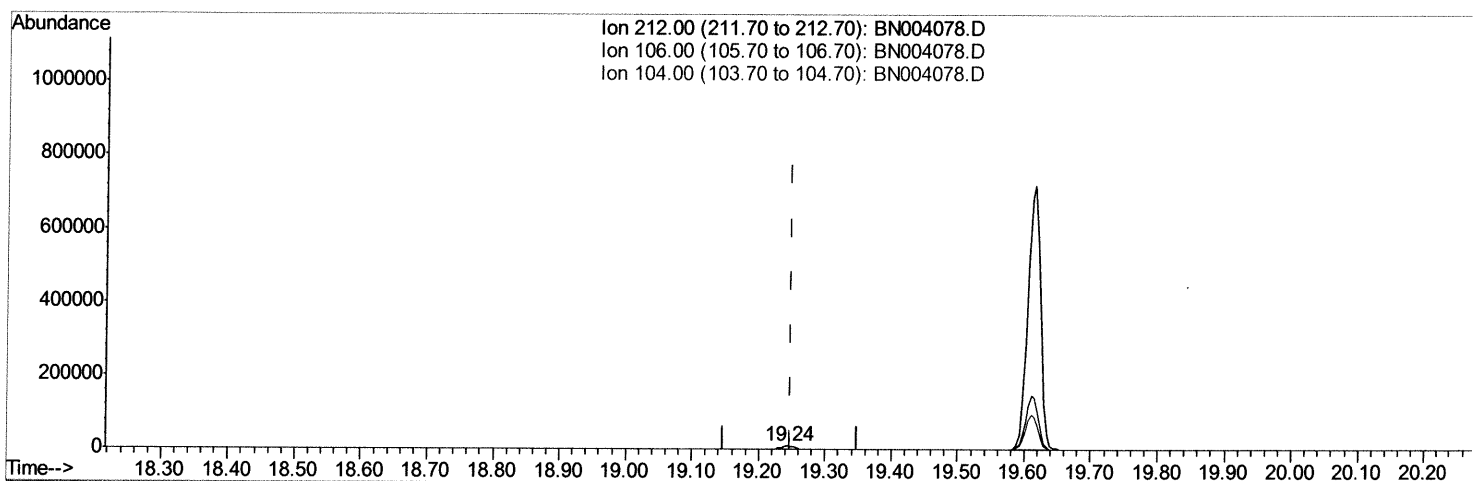

TIC: BN004078.D

(14) Fluoranthene-d10 (SURR)

19.244min (-0.005) 0.30ng/ul m

response 11012

Ion	Exp%	Act%
212.00	100	100
106.00	14.20	0.00#
104.00	8.00	0.00#
0.00	0.00	0.00

> SJ
12/19/18

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN121818\
Quantitation Report (Qedit)




Data File : BN004078.D
Acq On : 18 Dec 2018 16:08
Operator : JU/SJ
Sample : PB115555BL
Misc :
ALS Vial : 10 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
SBLK55

Manual Integrations
APPROVED

Sohil
12/19/2018 4:16:01 PM

Quant Time: Dec 19 03:21:01 2018
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SOM-EPA-SIM-BN111918.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Dec 19 01:54:36 2018
Response via : Initial Calibration

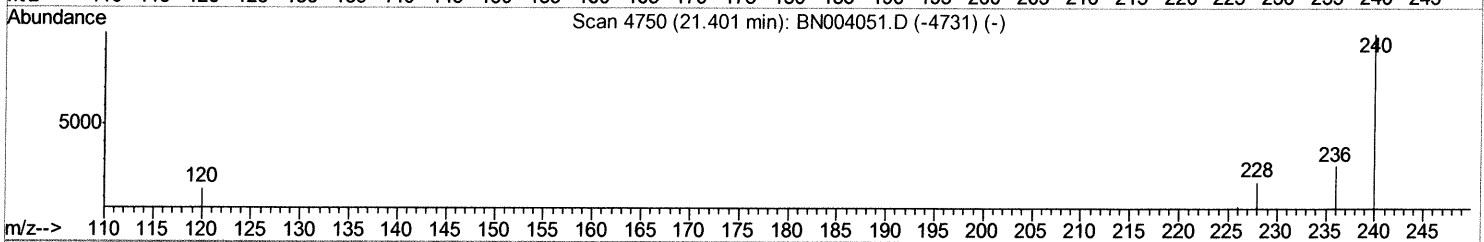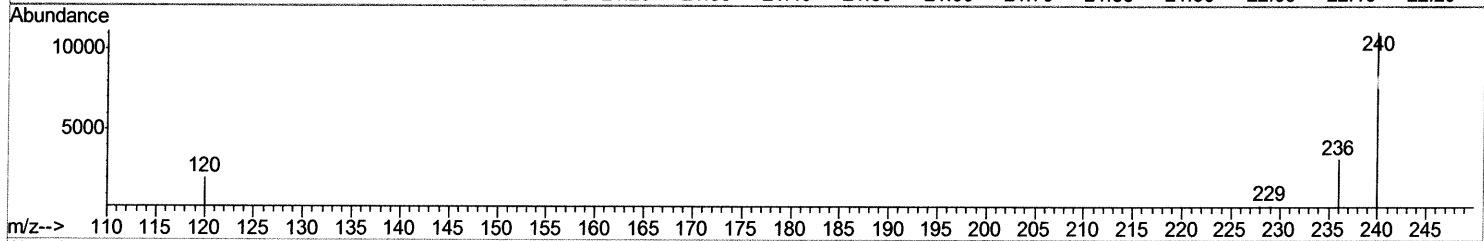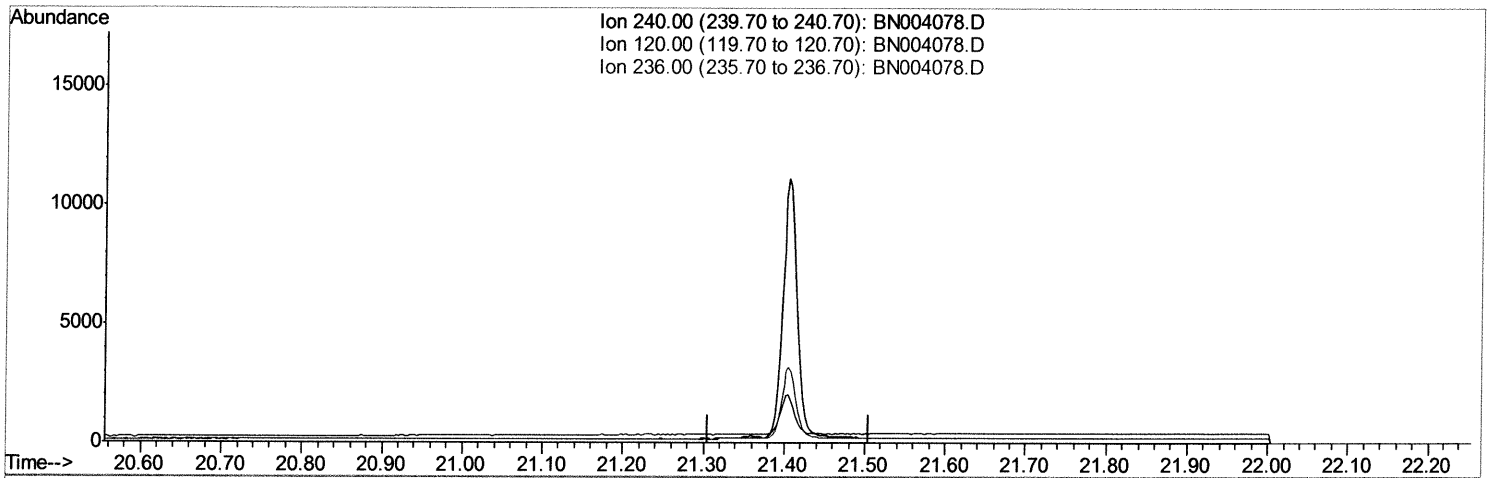

TIC: BN004078.D

(16) Chrysene-d12 (I)

21.406min (-21.406) 0.00ng/ul

response 0

Ion	Exp%	Act%
240.00	100	0.00
120.00	14.00	0.00#
236.00	27.60	0.00#
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN121818\
Quantitation Report (Qedit)




Data File : BN004078.D
Acq On : 18 Dec 2018 16:08
Operator : JU/SJ
Sample : PB115555BL
Misc :
ALS Vial : 10 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
SBLK55

Manual Integrations
APPROVED

Sohil
12/19/2018 4:16:01 PM

Quant Time: Dec 19 03:21:01 2018
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SOM-EPA-SIM-BN111918.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Dec 19 01:54:36 2018
Response via : Initial Calibration

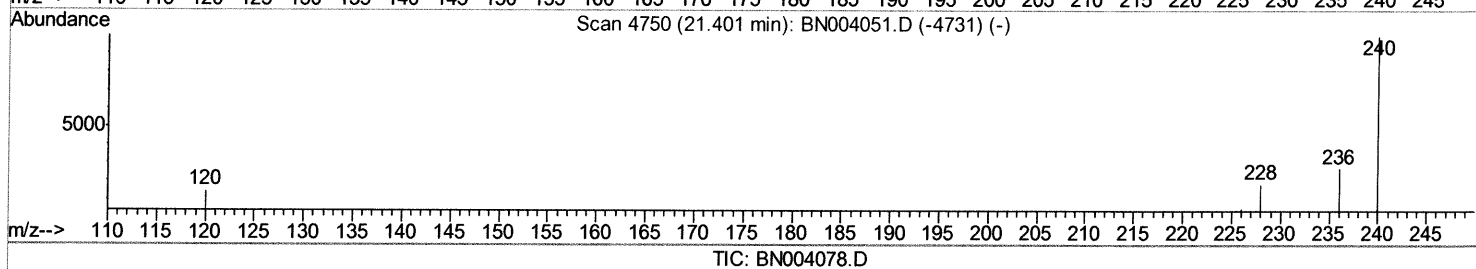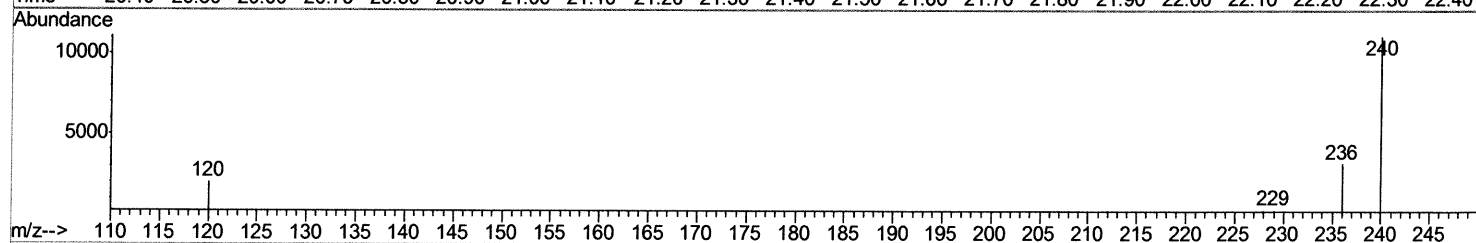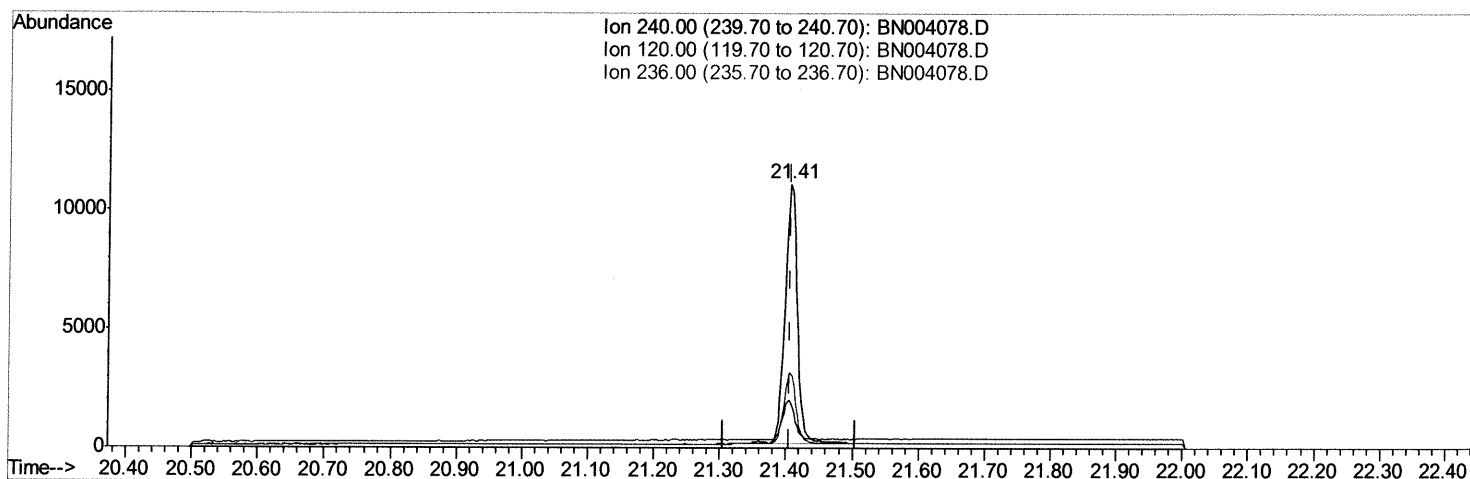

(16) Chrysene-d12 (I)

21.405min (-0.000) 0.40ng/ul m

response 13900

Ion	Exp%	Act%
240.00	100	100
120.00	14.00	18.03#
236.00	27.60	28.82
0.00	0.00	0.00

> SJ
12/19/18

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN121818\
Quantitation Report (Qedit)




Data File : BN004078.D
Acq On : 18 Dec 2018 16:08
Operator : JU/SJ
Sample : PB115555BL
Misc :
ALS Vial : 10 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
SBLK55

Manual Integrations
APPROVED

Sohil
12/19/2018 4:16:01 PM

Quant Time: Dec 19 03:21:42 2018
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SOM-EPA-SIM-BN111918.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Dec 19 01:54:36 2018
Response via : Initial Calibration

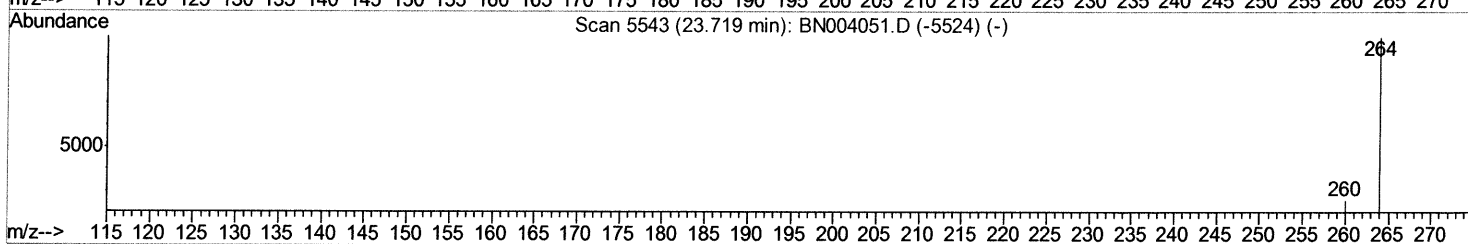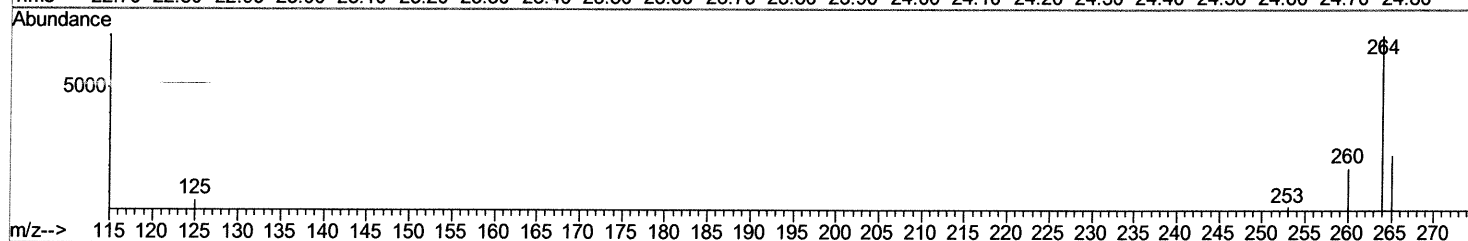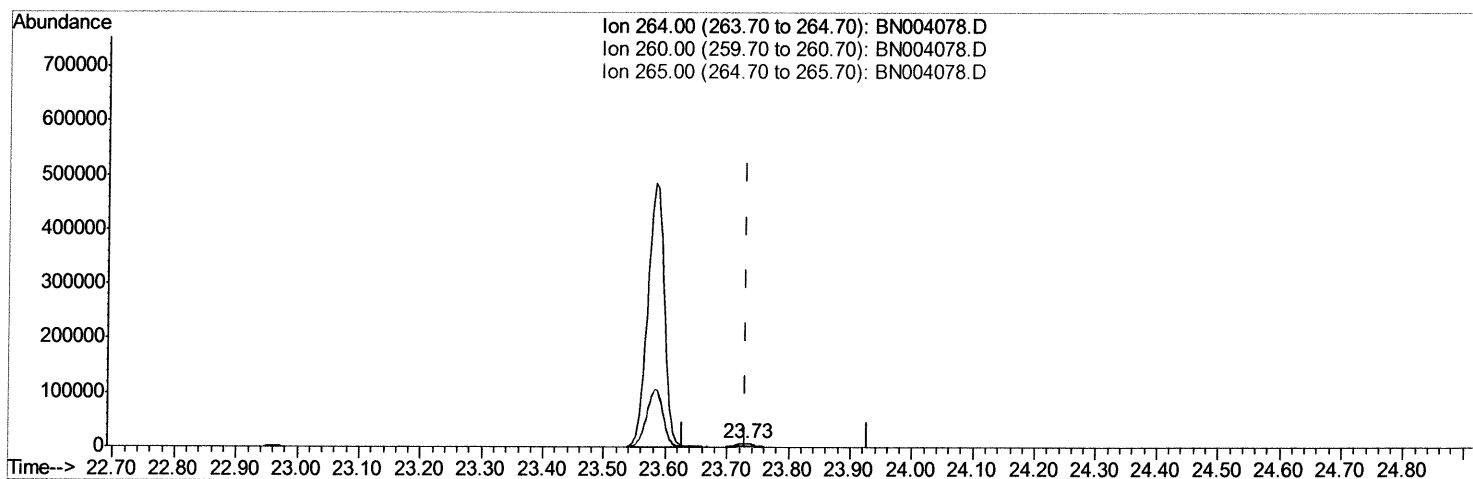

TIC: BN004078.D

(20) Perylene-d12 (I)

23.729min (-0.000) 0.40ng/ul

response 14214

Ion	Exp%	Act%
264.00	100	100
260.00	26.20	27.94
265.00	33.50	34.81
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN121818\
Quantitation Report (Qedit)




Data File : BN004078.D
Acq On : 18 Dec 2018 16:08
Operator : JU/SJ
Sample : PB115555BL
Misc :
ALS Vial : 10 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
SBLK55

Manual Integrations
APPROVED

Sohil
12/19/2018 4:16:01 PM

Quant Time: Dec 19 03:21:42 2018
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SOM-EPA-SIM-BN111918.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Dec 19 01:54:36 2018
Response via : Initial Calibration

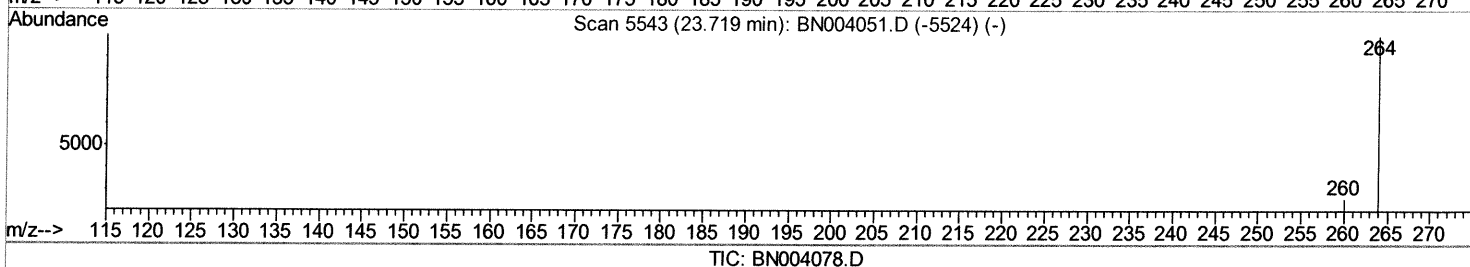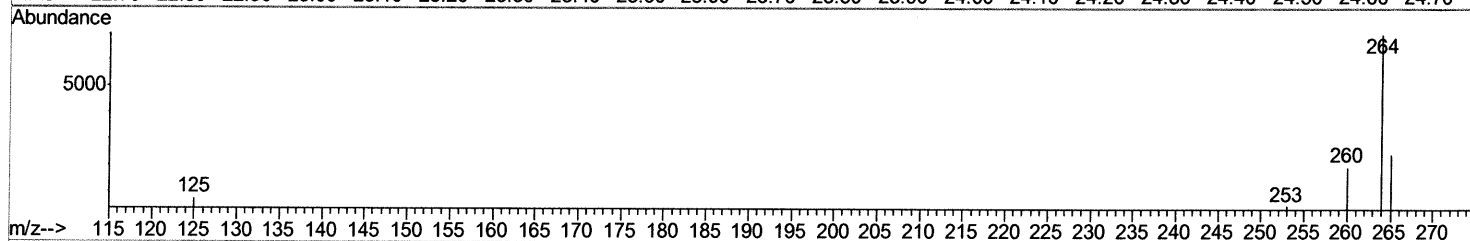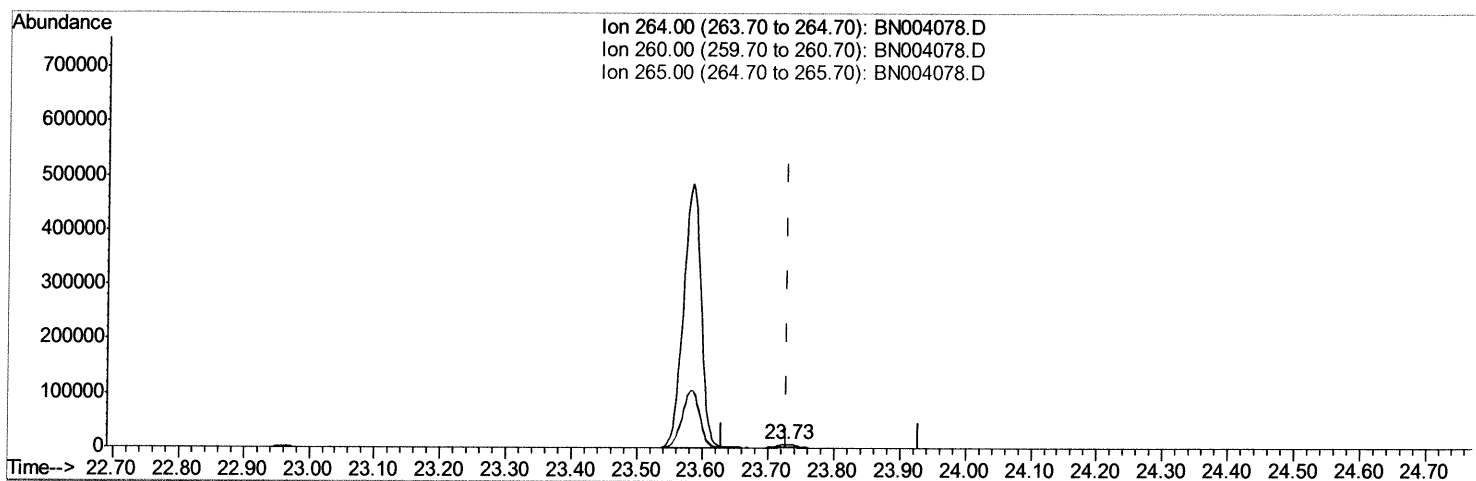

(20) Perylene-d12 (I)

23.729min (-0.000) 0.40ng/ul m

response 12352

Ion	Exp%	Act%
264.00	100	100
260.00	26.20	27.94
265.00	33.50	34.81
0.00	0.00	0.00

> SJ
12/19/18

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN121818\
Quantitation Report (QT Reviewed)

Data File : BN004078.D
Acq On : 18 Dec 2018 16:08
Operator : JU/SJ
Sample : PB115555BL
Misc :
ALS Vial : 10 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
SBLK55

Manual Integrations
APPROVED

Sohil
12/19/2018 4:16:01 PM

Quant Time: Dec 19 03:22:29 2018
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SOM-EPA-SIM-BN111918.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Dec 19 01:54:36 2018
Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	7.83	152	1438	0.40	ng/ul	0.00
2) Naphthalene-d8	10.63	136	7278	0.40	ng/ul	0.00
6) Acenaphthene-d10	14.47	164	4769	0.40	ng/ul	0.00
10) Phenanthrene-d10	17.22	188	12538m	0.40	ng/ul	0.00
16) Chrysene-d12	21.41	240	13900m	0.40	ng/ul	0.00
20) Perylene-d12	23.73	264	12352m	0.40	ng/ul	0.00

System Monitoring Compounds	R.T.	QIon	Response	Conc	Units	Dev(Min)
4) 2-Methylnaphthalene-d10	12.22	152	2935	0.26	ng/ul	0.00
14) Fluoranthene-d10	19.24	212	11012m	0.30	ng/ul	0.00

Target Compounds	Qvalue
------------------	--------

(#) = qualifier out of range (m) = manual integration (+) = signals summed

SJ
12/19/18