

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN121818\
Quantitation Report (QT Reviewed)


Data File : BN004083.D
Acq On : 18 Dec 2018 19:04
Operator : JU/SJ
Sample : J6271-07
Misc :
ALS Vial : 15 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
F9F14

Manual Integrations
APPROVED

Sohil
12/19/2018 4:16:05 PM

Quant Time: Dec 19 04:00:57 2018
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SOM-EPA-SIM-BN111918.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Dec 19 01:54:36 2018
Response via : Initial Calibration

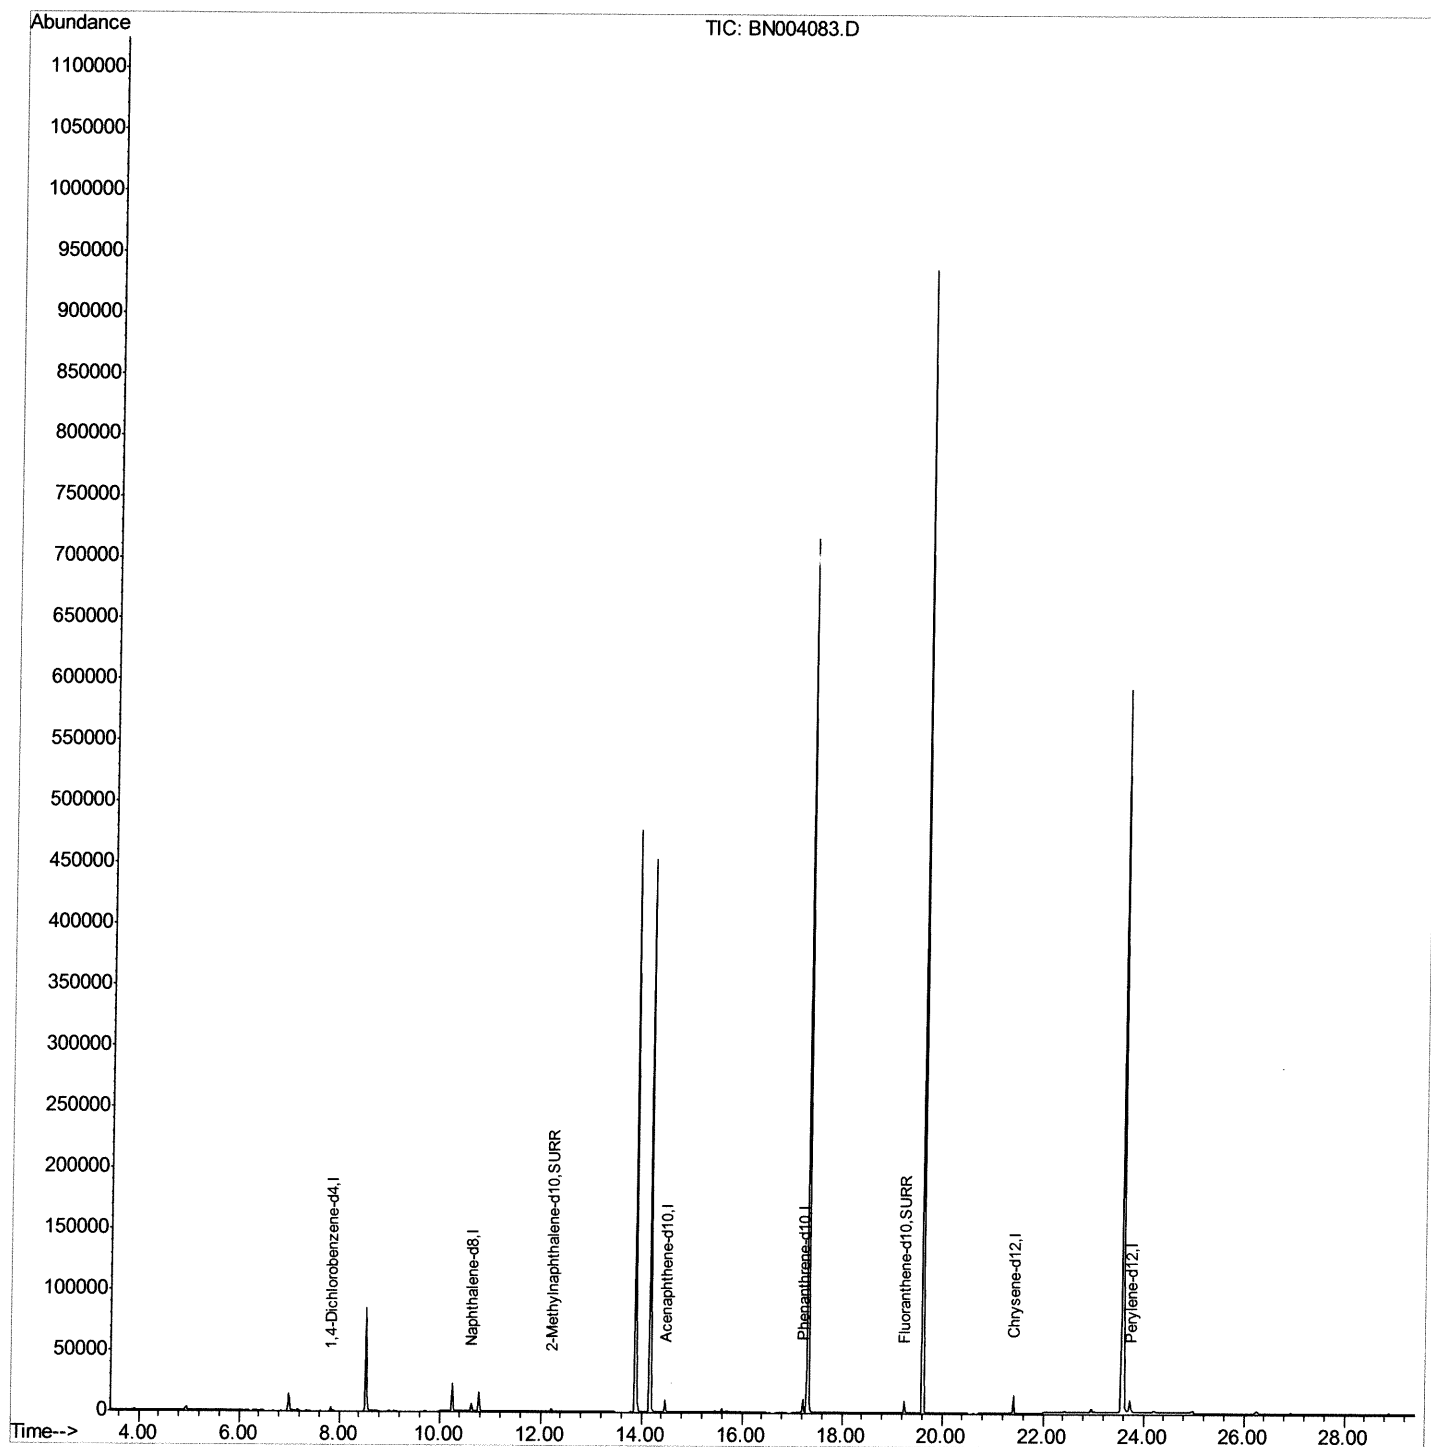

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN121818\
Quantitation Report (Qedit)




Data File : BN004083.D
Acq On : 18 Dec 2018 19:04
Operator : JU/SJ
Sample : J6271-07
Misc :
ALS Vial : 15 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
F9F14

Manual Integrations
APPROVED

Sohil
12/19/2018 4:16:05 PM

Quant Time: Dec 19 01:58:53 2018
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SOM-EPA-SIM-BN111918.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Dec 19 01:54:36 2018
Response via : Initial Calibration

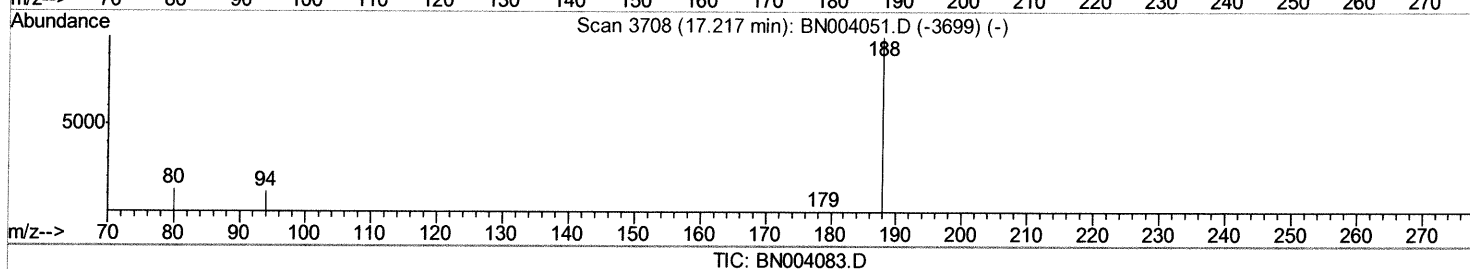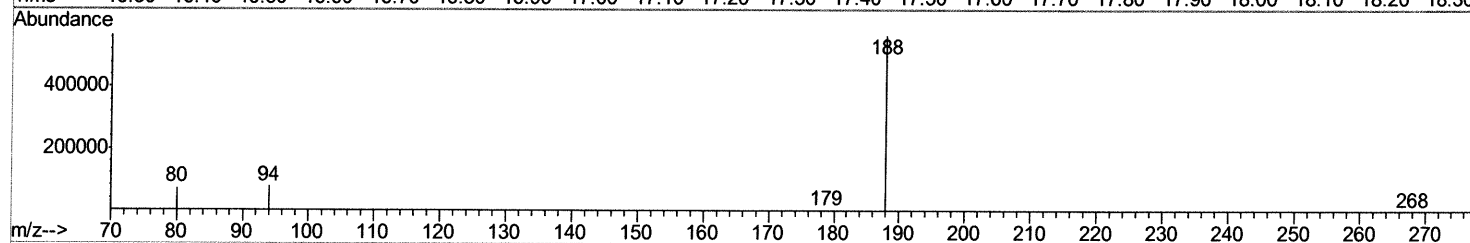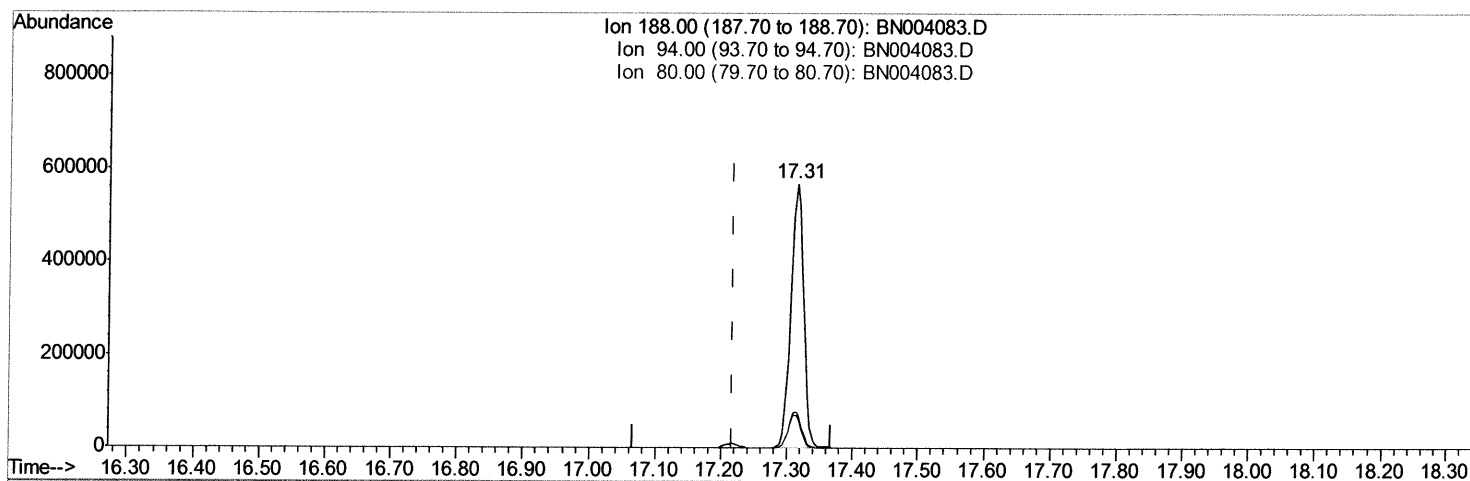

(10) Phenanthrene-d10 (I)
17.314min (+0.097) 0.40ng/ul
response 768547

Ion	Exp%	Act%
188.00	100	100
94.00	10.40	13.65#
80.00	11.60	12.37
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN121818\
Quantitation Report (Qedit)




Data File : BN004083.D
Acq On : 18 Dec 2018 19:04
Operator : JU/SJ
Sample : J6271-07
Misc :
ALS Vial : 15 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
F9F14

Manual Integrations
APPROVED

Sohil
12/19/2018 4:16:05 PM

Quant Time: Dec 19 01:58:53 2018
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SOM-EPA-SIM-BN111918.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Dec 19 01:54:36 2018
Response via : Initial Calibration

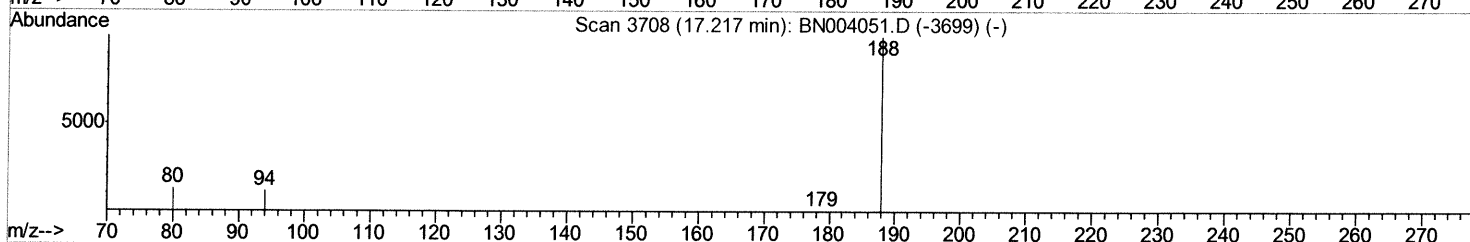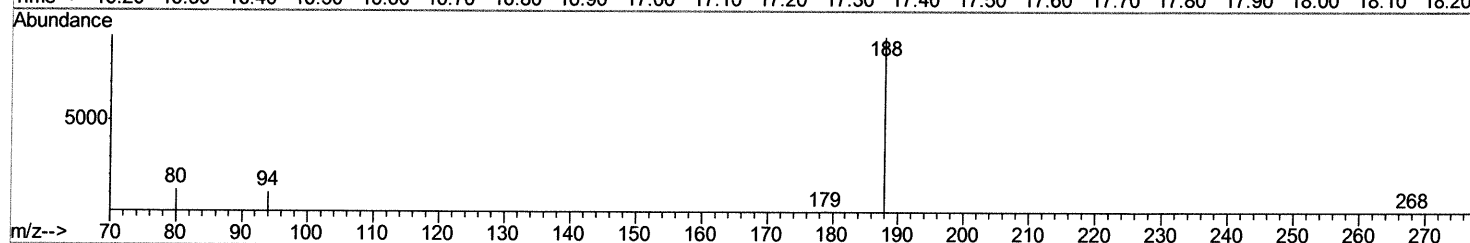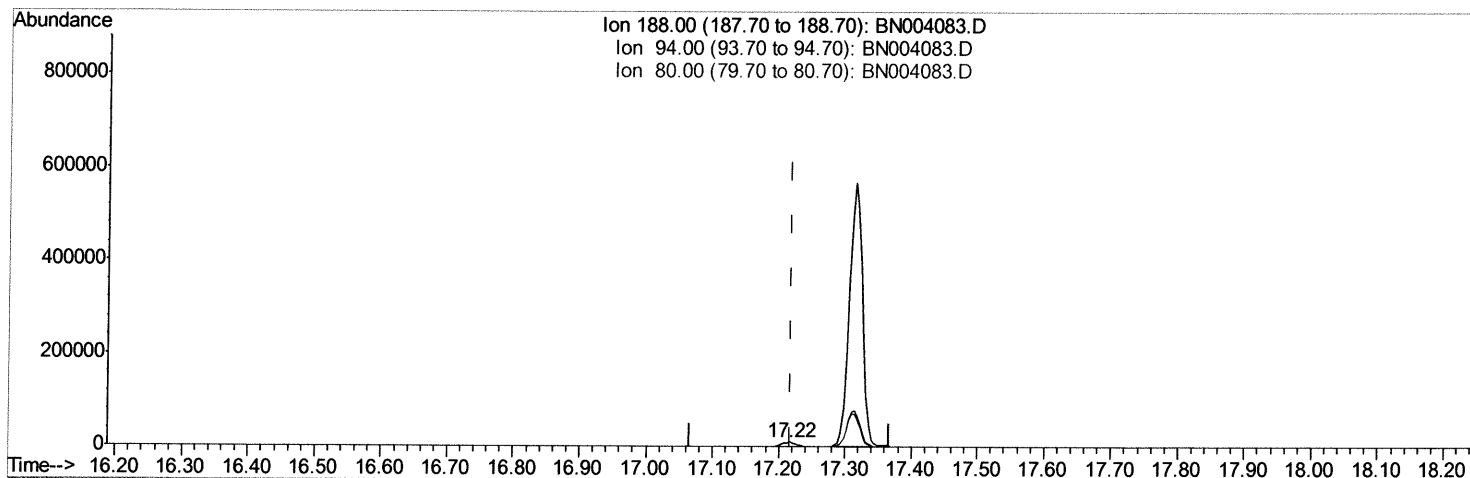

TIC: BN004083.D

(10) Phenanthrene-d10 (I)

17.217min (-0.000) 0.40ng/ul m

response 13297

Ion	Exp%	Act%
188.00	100	100
94.00	10.40	11.73
80.00	11.60	12.88
0.00	0.00	0.00

> SJ
12/19/18

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN121818\
Quantitation Report (Qedit)




Data File : BN004083.D
Acq On : 18 Dec 2018 19:04
Operator : JU/SJ
Sample : J6271-07
Misc :
ALS Vial : 15 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
F9F14

Manual Integrations
APPROVED

Sohil
12/19/2018 4:16:05 PM

Quant Time: Dec 19 03:59:36 2018
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SOM-EPA-SIM-BN111918.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Dec 19 01:54:36 2018
Response via : Initial Calibration

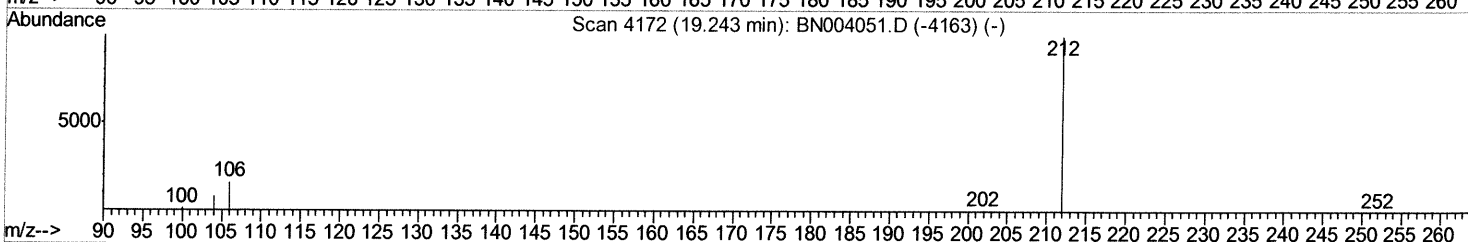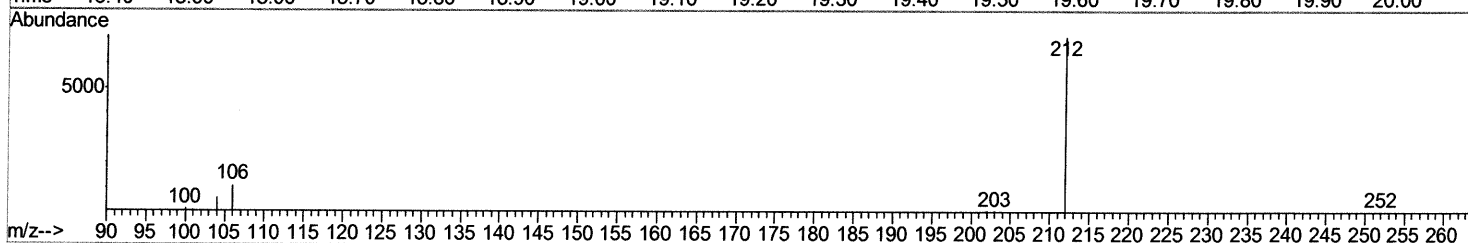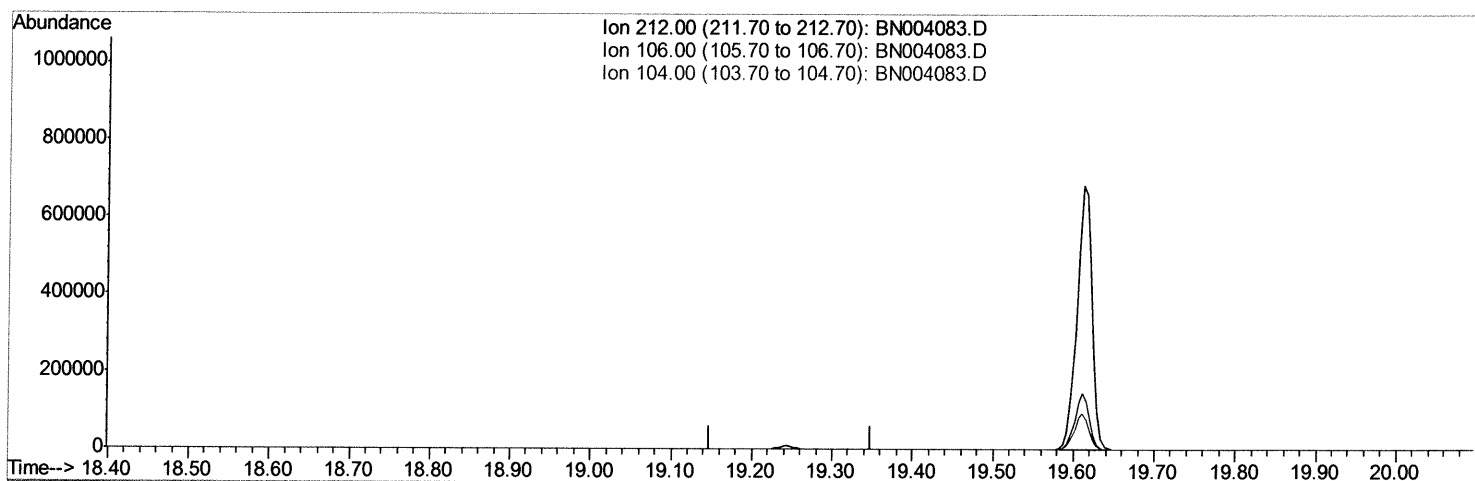

TIC: BN004083.D

(14) Fluoranthene-d10 (SURR)

19.248min (-19.248) 0.00ng/ul

response 0

Ion	Exp%	Act%
212.00	100	0.00
106.00	14.20	0.00#
104.00	8.00	0.00#
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN121818\
Quantitation Report (Qedit)




Data File : BN004083.D
Acq On : 18 Dec 2018 19:04
Operator : JU/SJ
Sample : J6271-07
Misc :
ALS Vial : 15 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
F9F14

Manual Integrations
APPROVED

Sohil
12/19/2018 4:16:05 PM

Quant Time: Dec 19 03:59:36 2018
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SOM-EPA-SIM-BN111918.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Dec 19 01:54:36 2018
Response via : Initial Calibration

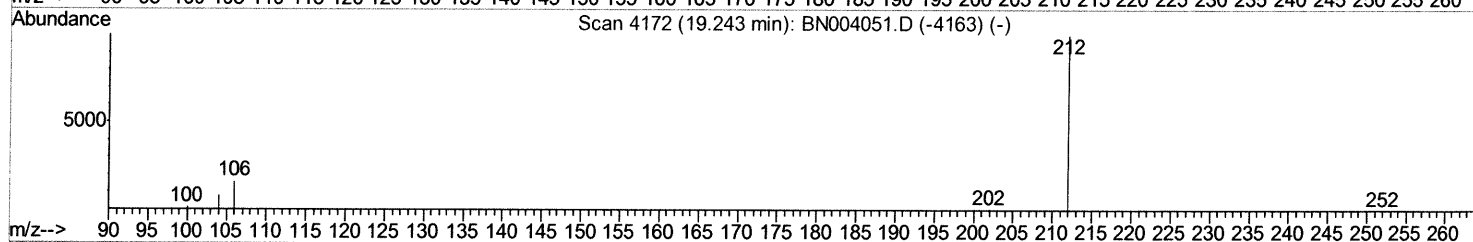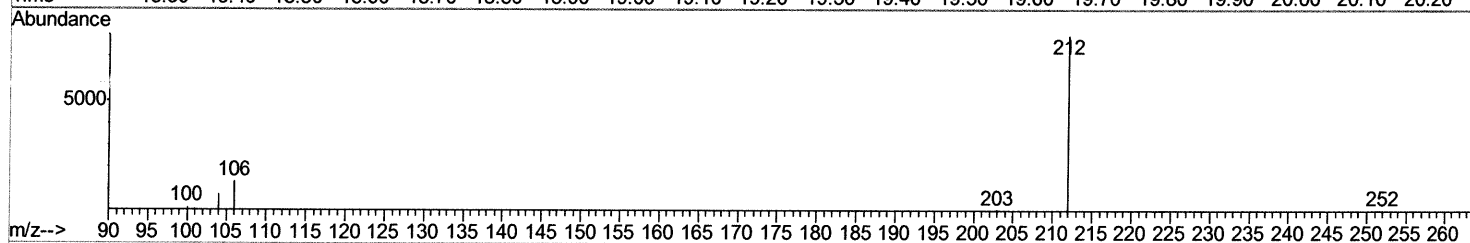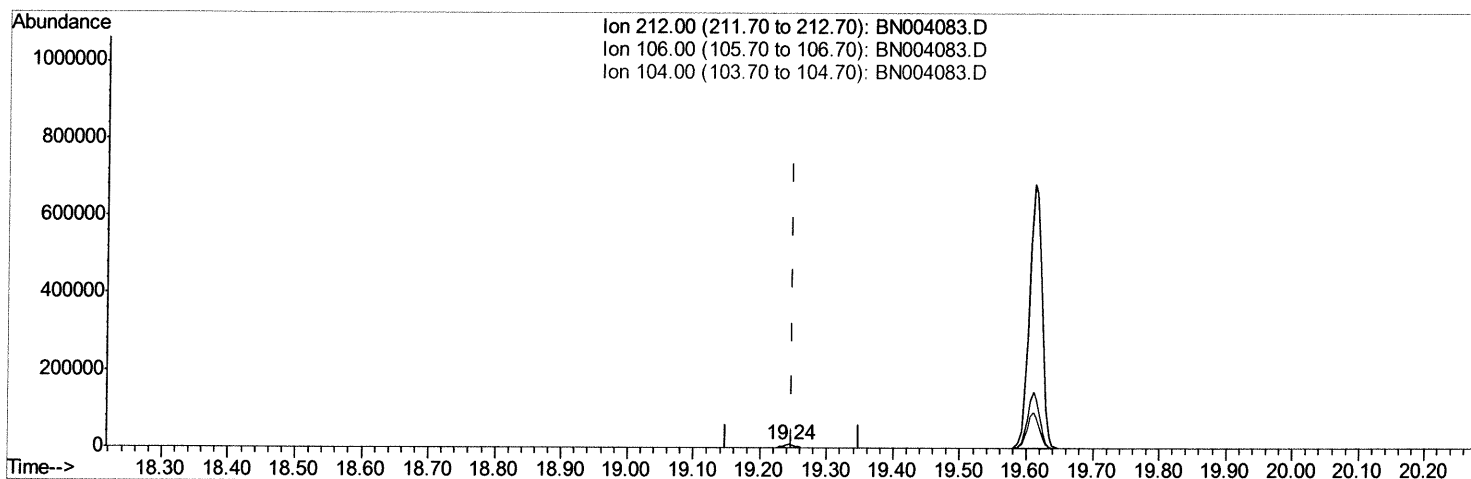

TIC: BN004083.D

(14) Fluoranthene-d10 (SURR)

19.243min (-0.005) 0.27ng/ul m

response 10343

Ion	Exp%	Act%
212.00	100	100
106.00	14.20	0.00#
104.00	8.00	0.00#
0.00	0.00	0.00

> SJ
12/19/18

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN121818\
Quantitation Report (Qedit)




Data File : BN004083.D
Acq On : 18 Dec 2018 19:04
Operator : JU/SJ
Sample : J6271-07
Misc :
ALS Vial : 15 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
F9F14

Manual Integrations
APPROVED

Sohil
12/19/2018 4:16:05 PM

Quant Time: Dec 19 03:59:36 2018
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SOM-EPA-SIM-BN111918.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Dec 19 01:54:36 2018
Response via : Initial Calibration

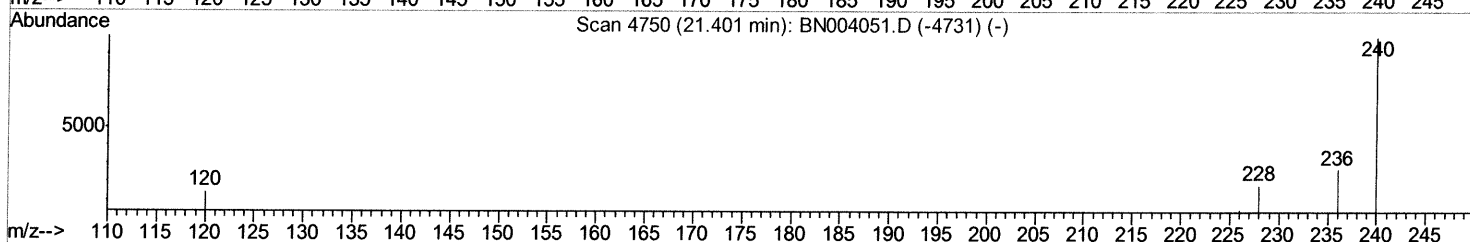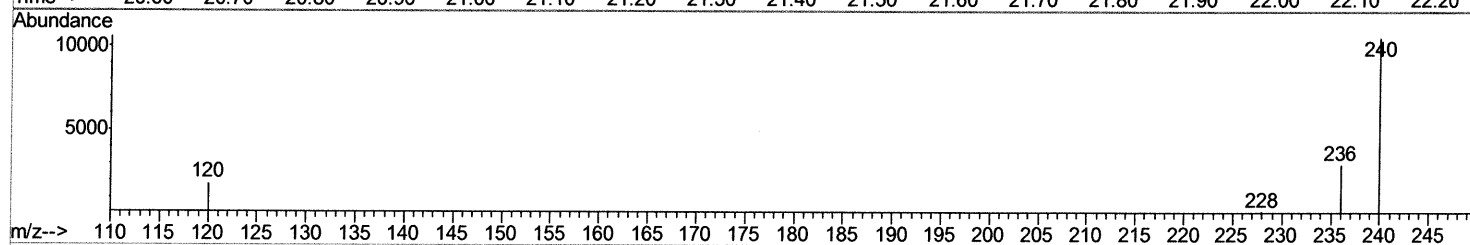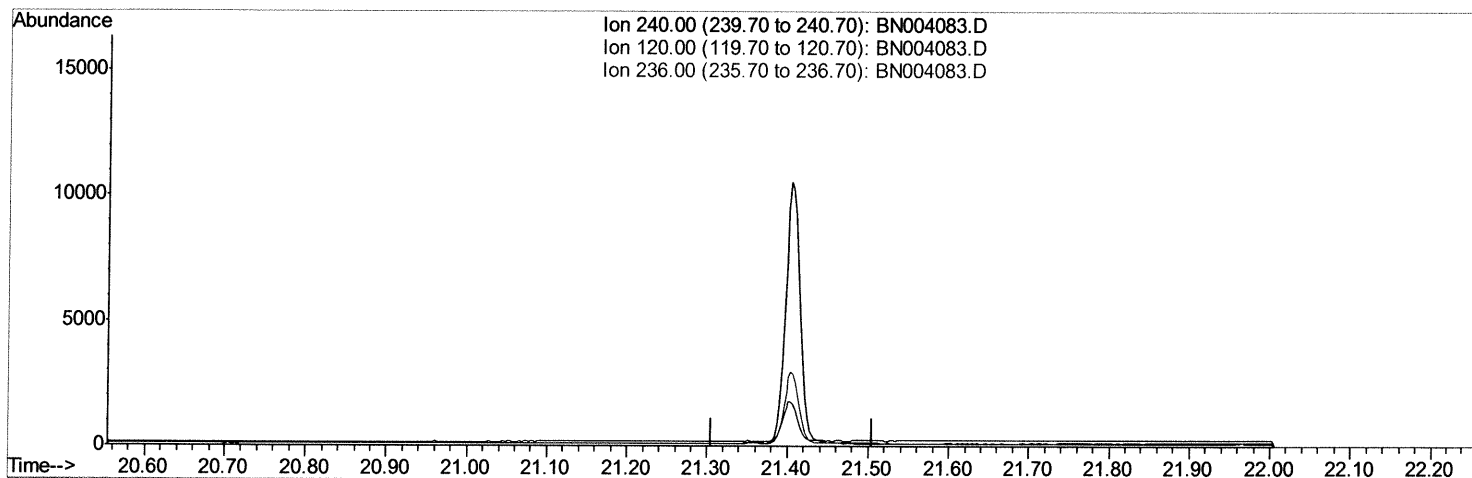

TIC: BN004083.D

(16) Chrysene-d12 (I)

21.406min (-21.406) 0.00ng/ul

response 0

Ion	Exp%	Act%
240.00	100	0.00
120.00	14.00	0.00#
236.00	27.60	0.00#
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN121818\
Quantitation Report (Qedit)




Data File : BN004083.D
Acq On : 18 Dec 2018 19:04
Operator : JU/SJ
Sample : J6271-07
Misc :
ALS Vial : 15 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
F9F14

Manual Integrations
APPROVED

Sohil
12/19/2018 4:16:05 PM

Quant Time: Dec 19 03:59:36 2018
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SOM-EPA-SIM-BN111918.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Dec 19 01:54:36 2018
Response via : Initial Calibration

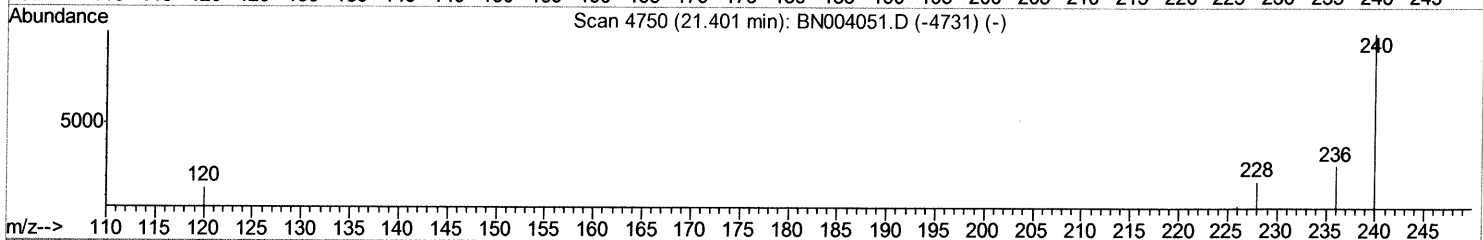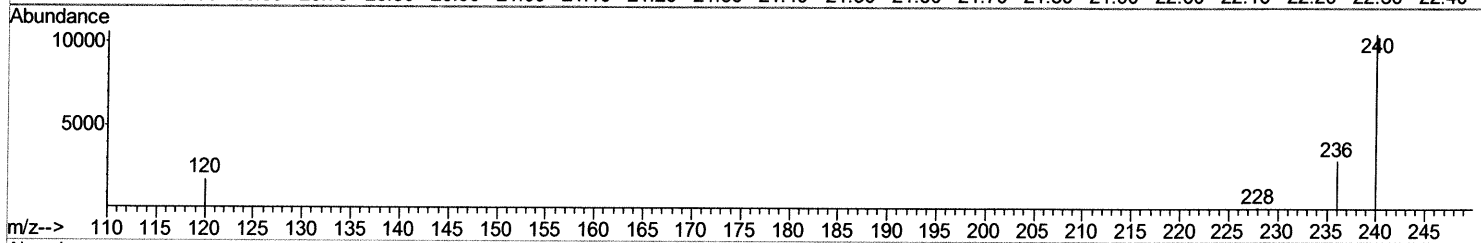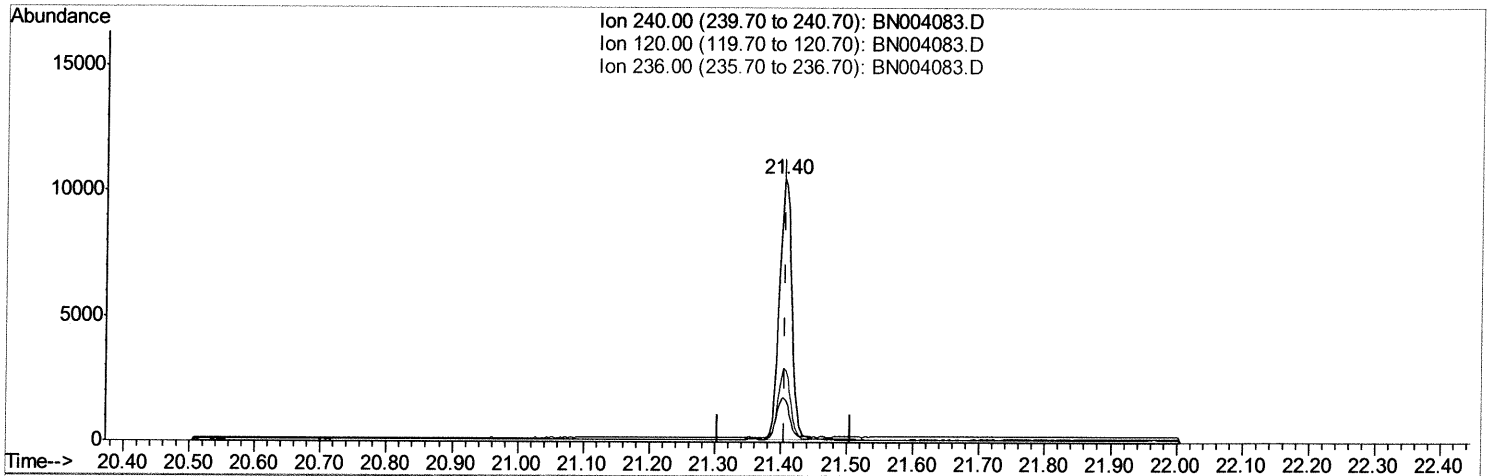

TIC: BN004083.D

(16) Chrysene-d12 (I)

21.404min (-0.001) 0.40ng/ul m

response 13517

Ion	Exp%	Act%
240.00	100	100
120.00	14.00	17.04#
236.00	27.60	28.30
0.00	0.00	0.00

> SJ
12/19/18

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN121818\
Quantitation Report (Qedit)




Data File : BN004083.D
Acq On : 18 Dec 2018 19:04
Operator : JU/SJ
Sample : J6271-07
Misc :
ALS Vial : 15 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
F9F14

Manual Integrations
APPROVED

Sohil
12/19/2018 4:16:05 PM

Quant Time: Dec 19 04:00:15 2018
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SOM-EPA-SIM-BN111918.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Dec 19 01:54:36 2018
Response via : Initial Calibration

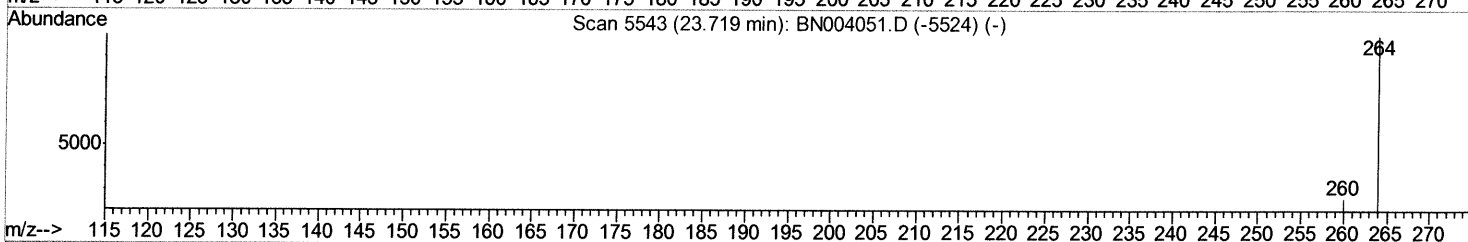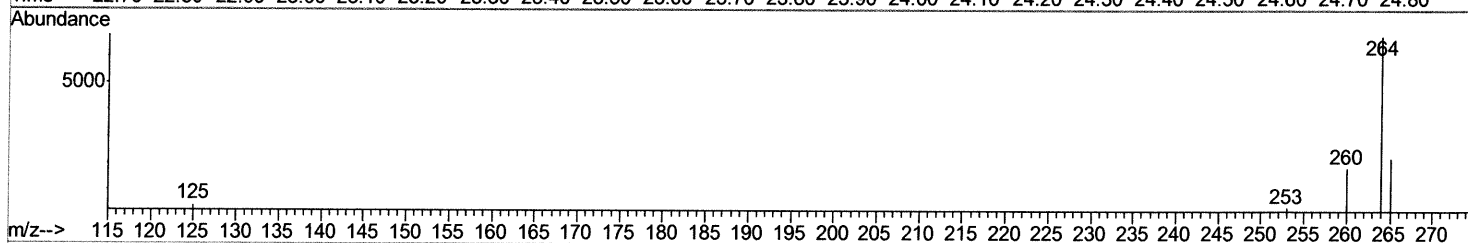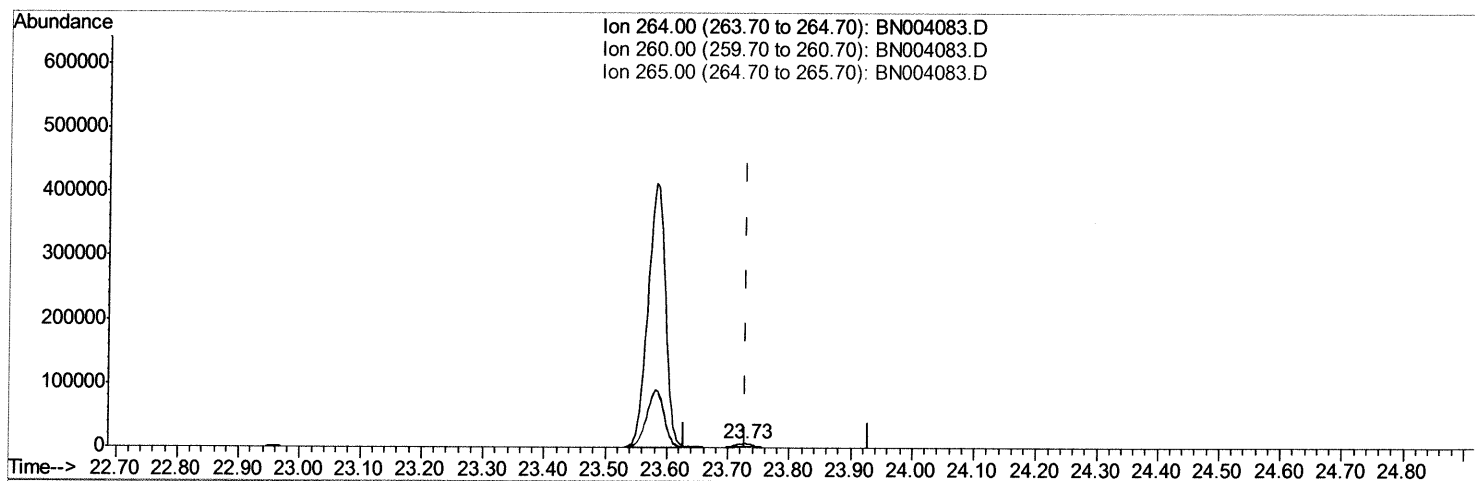

TIC: BN004083.D

(20) Perylene-d12 (I)

23.728min (-0.001) 0.40ng/ul

response 13769

Ion	Exp%	Act%
264.00	100	100
260.00	26.20	27.30
265.00	33.50	32.86
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN121818\
Quantitation Report (Qedit)




Data File : BN004083.D
Acq On : 18 Dec 2018 19:04
Operator : JU/SJ
Sample : J6271-07
Misc :
ALS Vial : 15 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
F9F14

Manual Integrations
APPROVED

Sohil
12/19/2018 4:16:05 PM

Quant Time: Dec 19 04:00:15 2018
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SOM-EPA-SIM-BN111918.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Dec 19 01:54:36 2018
Response via : Initial Calibration

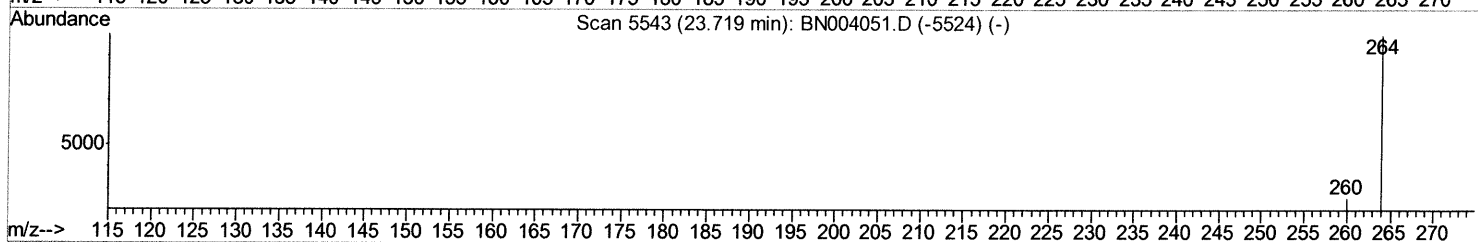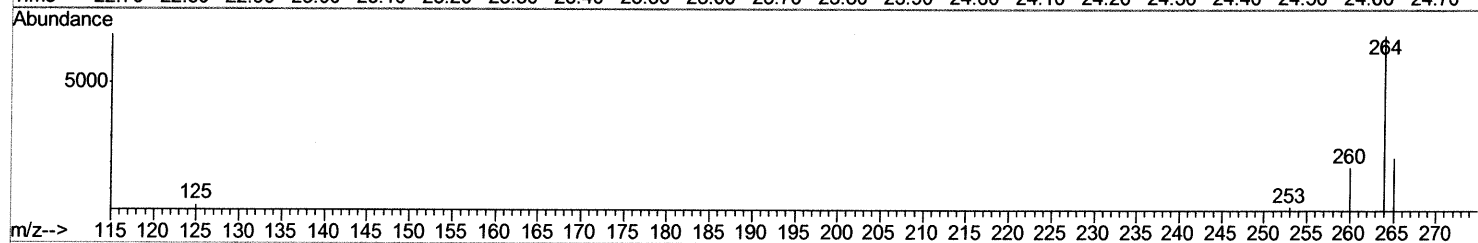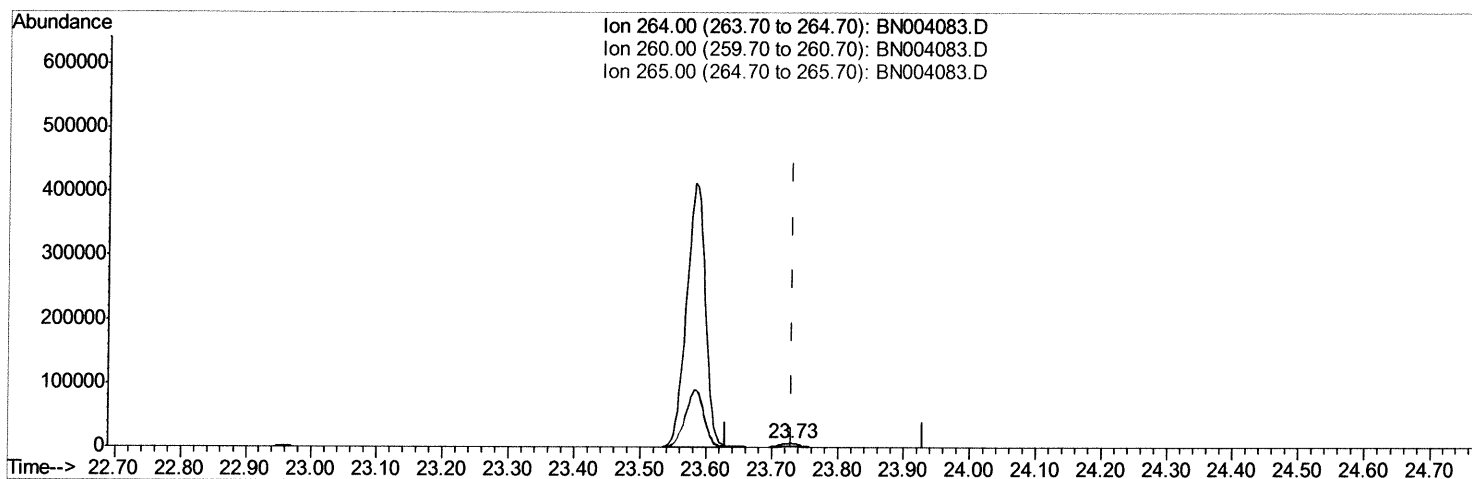

TIC: BN004083.D

(20) Perylene-d12 (I)

23.728min (-0.001) 0.40ng/ul m

response 12061

Ion	Exp%	Act%
264.00	100	100
260.00	26.20	27.30
265.00	33.50	32.86
0.00	0.00	0.00

> SJ
12/19/18

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN121818\
 Quantitation Report (QT Reviewed)
 Data File : BN004083.D
 Acq On : 18 Dec 2018 19:04
 Operator : JU/SJ
 Sample : J6271-07
 Misc :
 ALS Vial : 15 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 F9F14

Manual Integrations
 APPROVED

Sohil
 12/19/2018 4:16:05 PM

Quant Time: Dec 19 04:00:57 2018
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SOM-EPA-SIM-BN111918.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Wed Dec 19 01:54:36 2018
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	7.83	152	1705	0.40	ng/ul	0.00
2) Naphthalene-d8	10.63	136	8494	0.40	ng/ul	0.00
6) Acenaphthene-d10	14.47	164	5295	0.40	ng/ul	0.00
10) Phenanthrene-d10	17.22	188	13297m	0.40	ng/ul	0.00
16) Chrysene-d12	21.40	240	13517m	0.40	ng/ul	0.00
20) Perylene-d12	23.73	264	12061m	0.40	ng/ul	0.00

System Monitoring Compounds	R.T.	QIon	Response	Conc	Units	Dev(Min)
4) 2-Methylnaphthalene-d10	12.21	152	3202	0.25	ng/ul	0.00
14) Fluoranthene-d10	19.24	212	10343m	0.27	ng/ul	0.00

Target Compounds	Qvalue

(#) = qualifier out of range (m) = manual integration (+) = signals summed

SJ
 12/19/18