

Data Path : Z:\SVOASRV\HPCHEM1\BNA_N\DATA\BN121818\
Quantitation Report (QT Reviewed)


Data File : BN004096.D
Acq On : 19 Dec 2018 02:39
Operator : JU/SJ
Sample : J6271-17
Misc :
ALS Vial : 27 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
F9E32

Manual Integrations
APPROVED

Sohil
12/19/2018 4:16:53 PM

Quant Time: Dec 19 04:54:57 2018
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SOM-EPA-SIM-BN111918.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Dec 19 04:08:55 2018
Response via : Initial Calibration

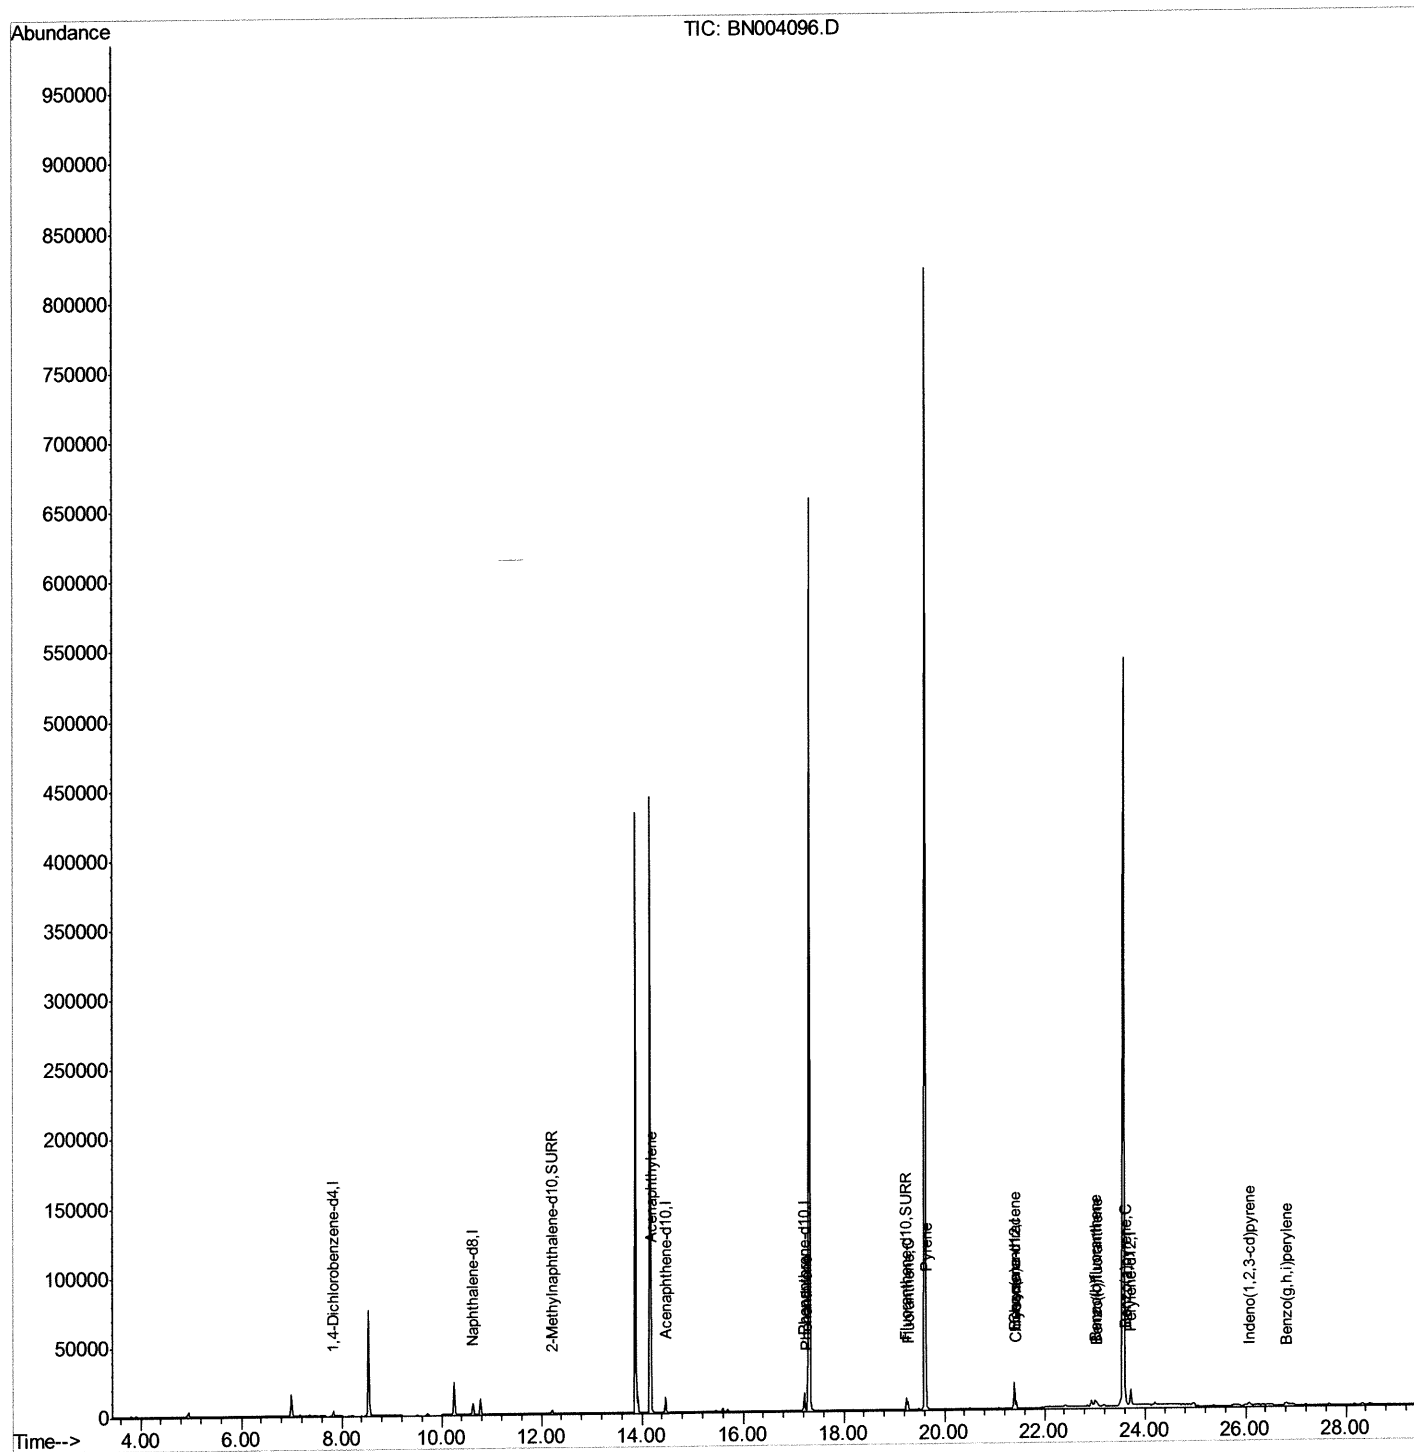

Data Path : Z:\SVOASRV\HPCHEM1\BNA_N\DATA\BN121818\
Quantitation Report (Qedit)




Data File : BN004096.D
Acq On : 19 Dec 2018 02:39
Operator : JU/SJ
Sample : J6271-17
Misc :
ALS Vial : 27 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
F9E32

Manual Integrations
APPROVED

Sohil
12/19/2018 4:16:53 PM

Quant Time: Dec 19 04:13:24 2018
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SOM-EPA-SIM-BN111918.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Dec 19 04:08:55 2018
Response via : Initial Calibration

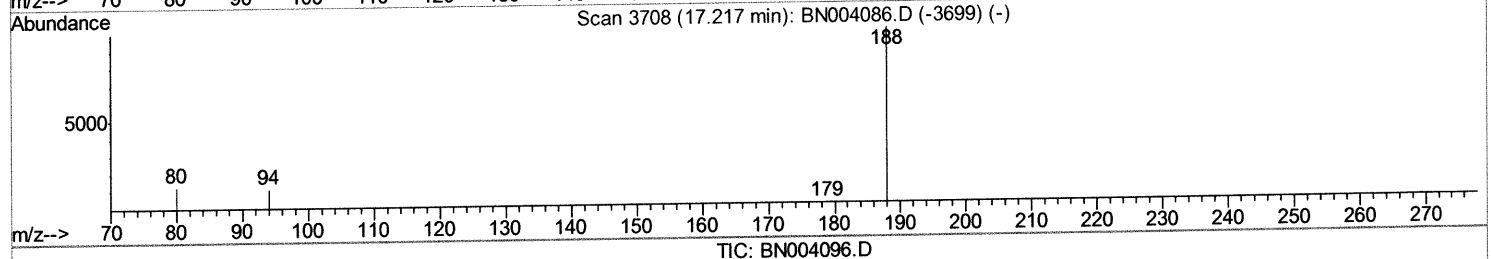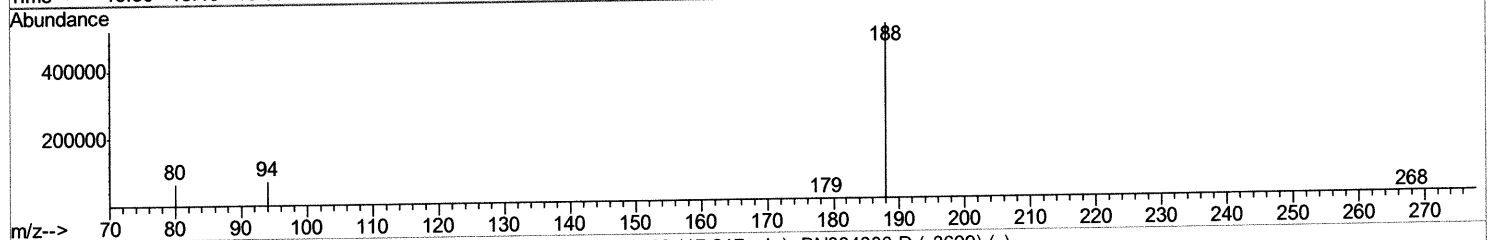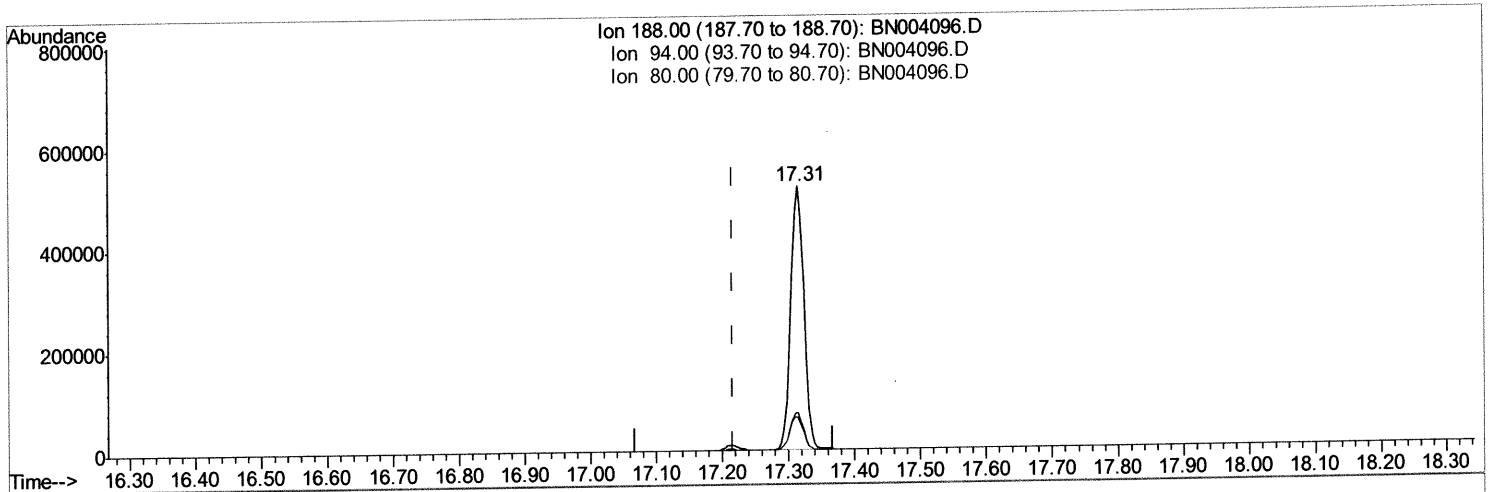

TIC: BN004096.D

(10) Phenanthrene-d10 (I)
17.314min (+0.097) 0.40ng/ul
response 703155

Ion	Exp%	Act%
188.00	100	100
94.00	10.40	13.89#
80.00	11.60	12.46
0.00	0.00	0.00

Data Path : Z:\SVOASRV\HPCHEM1\BNA_N\DATA\BN121818\
Quantitation Report (Qedit)




Data File : BN004096.D
Acq On : 19 Dec 2018 02:39
Operator : JU/SJ
Sample : J6271-17
Misc :
ALS Vial : 27 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
F9E32

Manual Integrations
APPROVED

Sohil
12/19/2018 4:16:53 PM

Quant Time: Dec 19 04:13:24 2018
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SOM-EPA-SIM-BN111918.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Dec 19 04:08:55 2018
Response via : Initial Calibration

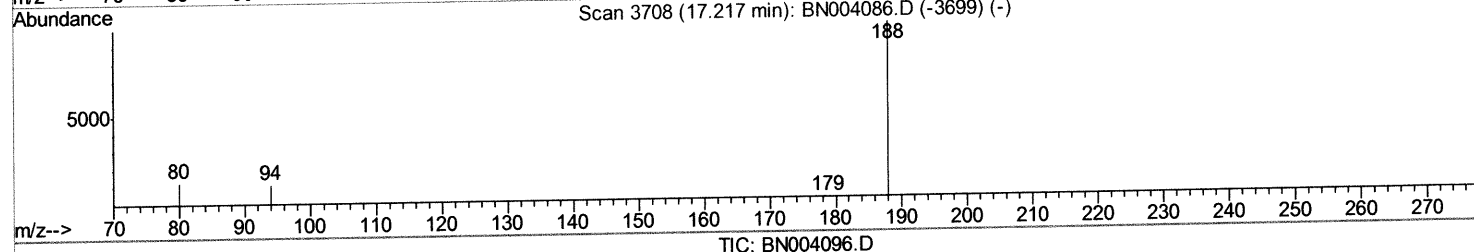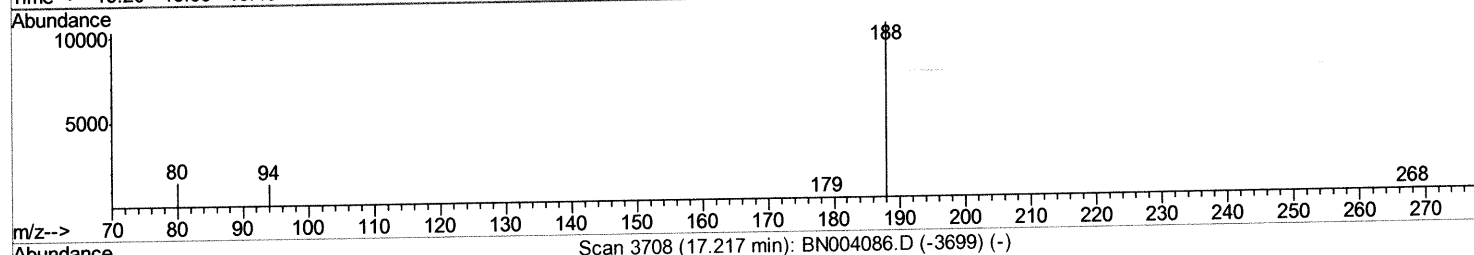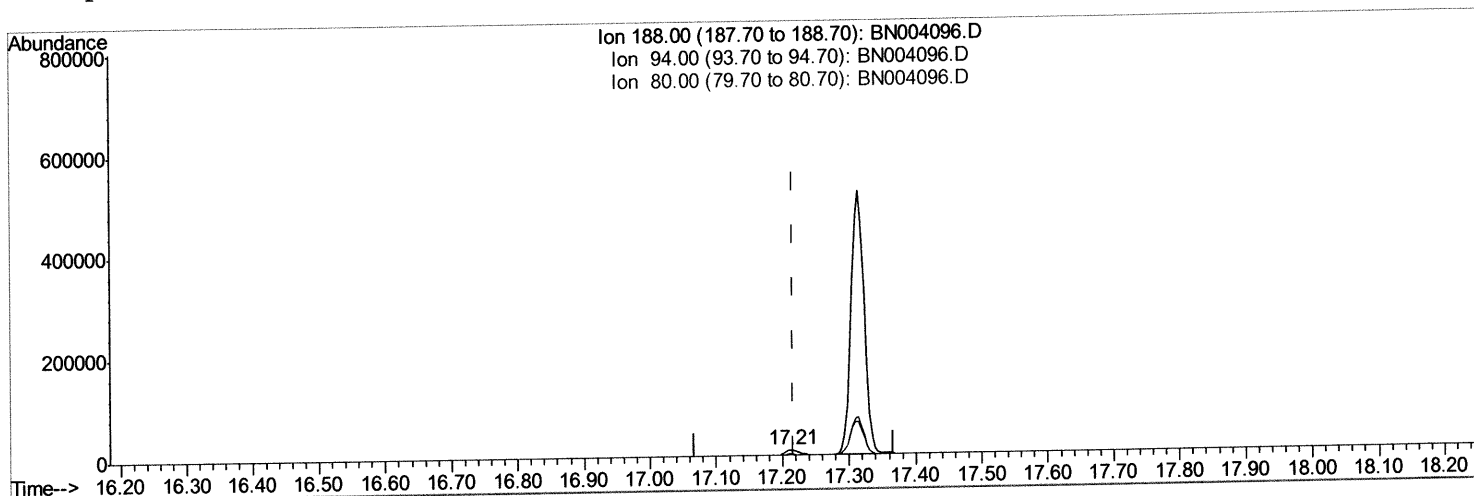

(10) Phenanthrene-d10 (I)

17.213min (-0.004) 0.40ng/ul m

response 14900

Ion	Exp%	Act%
188.00	100	100
94.00	10.40	12.65#
80.00	11.60	13.96#
0.00	0.00	0.00

> SJ
12/19/18

Data Path : Z:\SVOASRV\HPCHEM1\BNA_N\DATA\BN121818\
Quantitation Report (Qedit)




Data File : BN004096.D
Acq On : 19 Dec 2018 02:39
Operator : JU/SJ
Sample : J6271-17
Misc :
ALS Vial : 27 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
F9E32

Manual Integrations
APPROVED

Sohil
12/19/2018 4:16:53 PM

Quant Time: Dec 19 04:51:49 2018
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SOM-EPA-SIM-BN111918.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Dec 19 04:08:55 2018
Response via : Initial Calibration

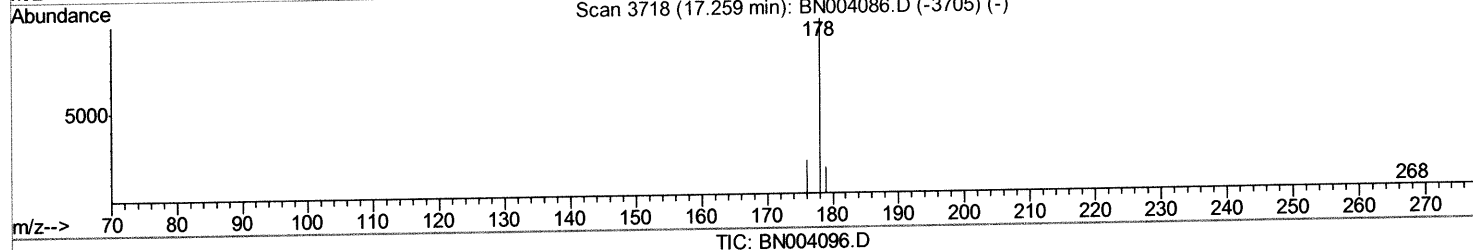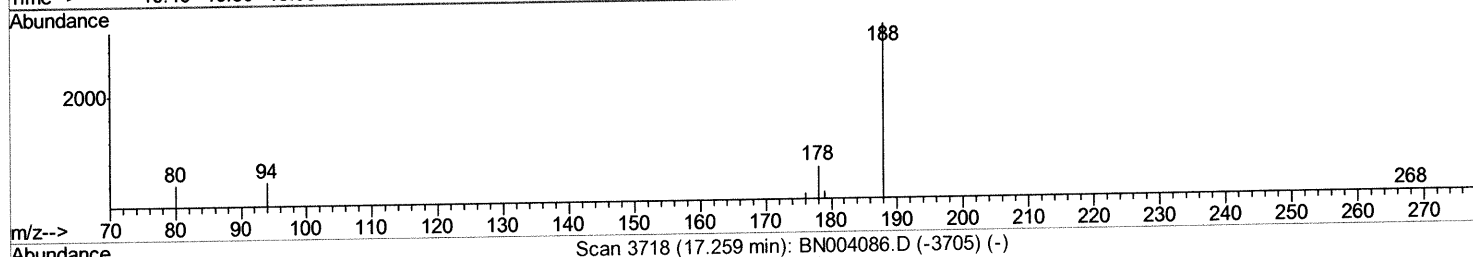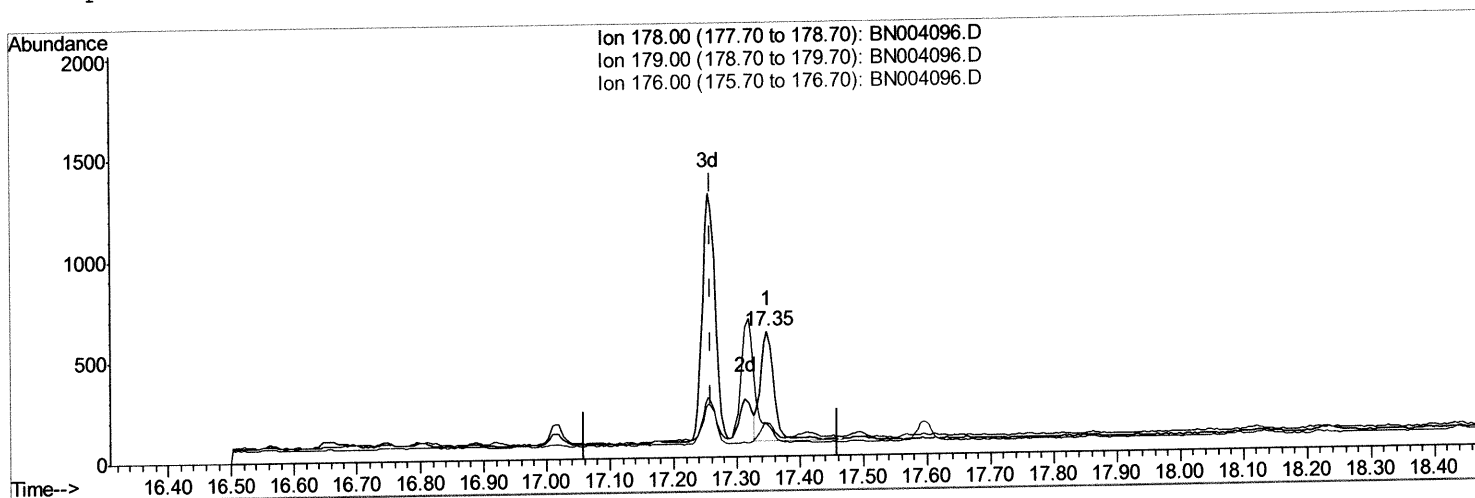

(12) Phenanthrene
17.348min (+0.089) 0.02ng/ul
response 833

Ion	Exp%	Act%
178.00	100	100
179.00	15.60	26.94#
176.00	18.70	25.48#
0.00	0.00	0.00

Data Path : Z:\SVOASRV\HPCHEM1\BNA_N\DATA\BN121818\
Quantitation Report (Qedit)




Data File : BN004096.D
Acq On : 19 Dec 2018 02:39
Operator : JU/SJ
Sample : J6271-17
Misc :
ALS Vial : 27 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
F9E32

Manual Integrations
APPROVED

Sohil
12/19/2018 4:16:53 PM

Quant Time: Dec 19 04:51:49 2018
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SOM-EPA-SIM-BN111918.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Dec 19 04:08:55 2018
Response via : Initial Calibration

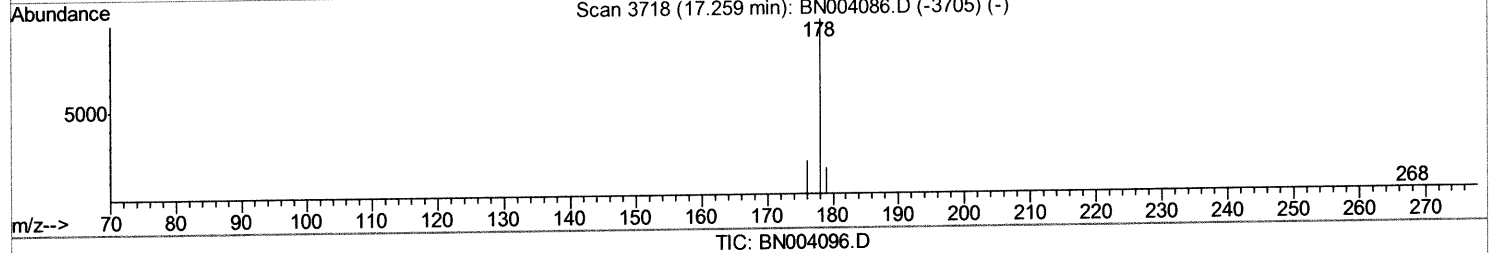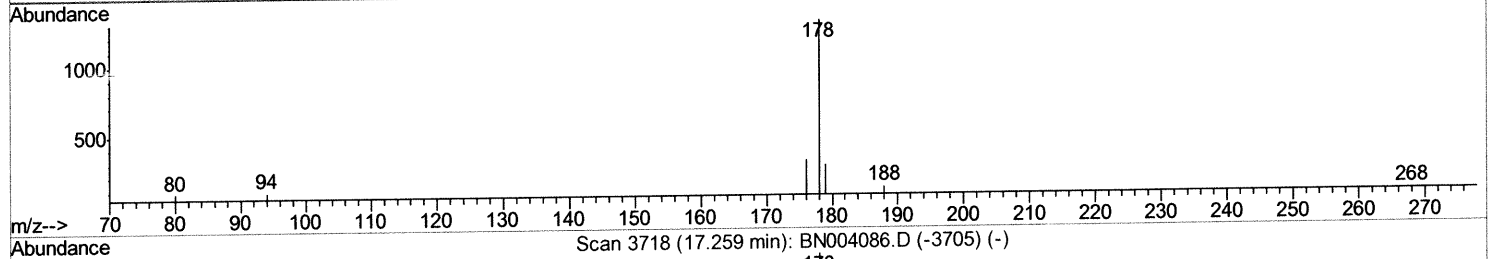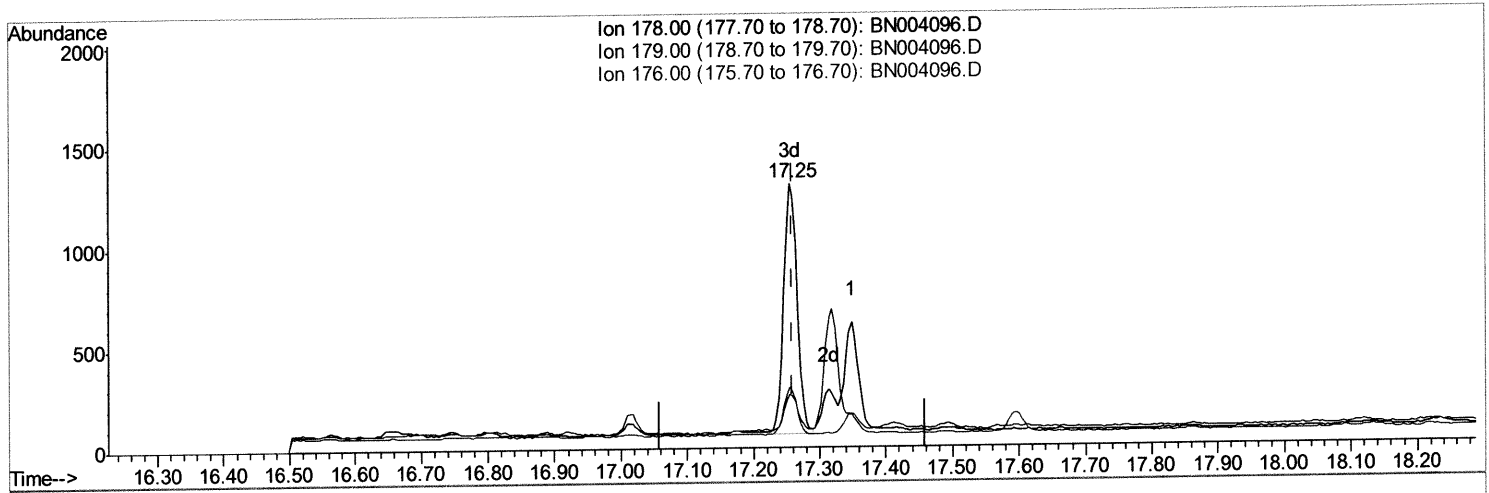

(12) Phenanthrene

17.255min (-0.004) 0.04ng/ul m

response 1761

Ion	Exp%	Act%
178.00	100	100
179.00	15.60	19.98#
176.00	18.70	22.89#
0.00	0.00	0.00

> SJ
12/19/18

Data Path : Z:\SVOASRV\HPCHEM1\BNA_N\DATA\BN121818\
Quantitation Report (Qedit)




Data File : BN004096.D
Acq On : 19 Dec 2018 02:39
Operator : JU/SJ
Sample : J6271-17
Misc :
ALS Vial : 27 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
F9E32

Manual Integrations
APPROVED

Sohil
12/19/2018 4:16:53 PM

Quant Time: Dec 19 04:51:49 2018
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SOM-EPA-SIM-BN111918.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Dec 19 04:08:55 2018
Response via : Initial Calibration

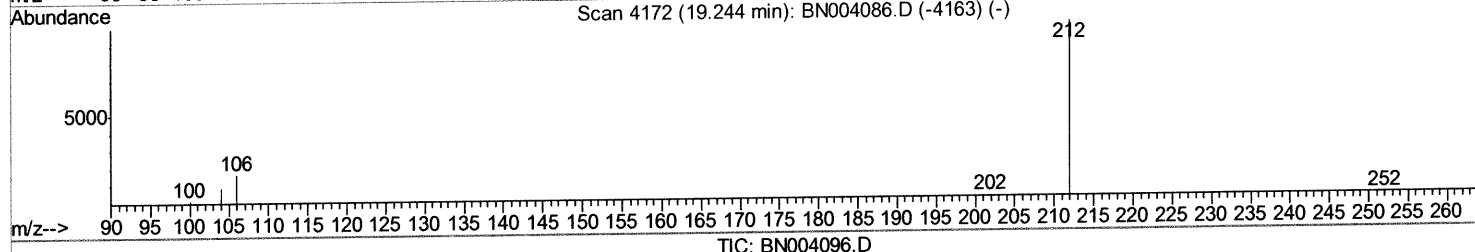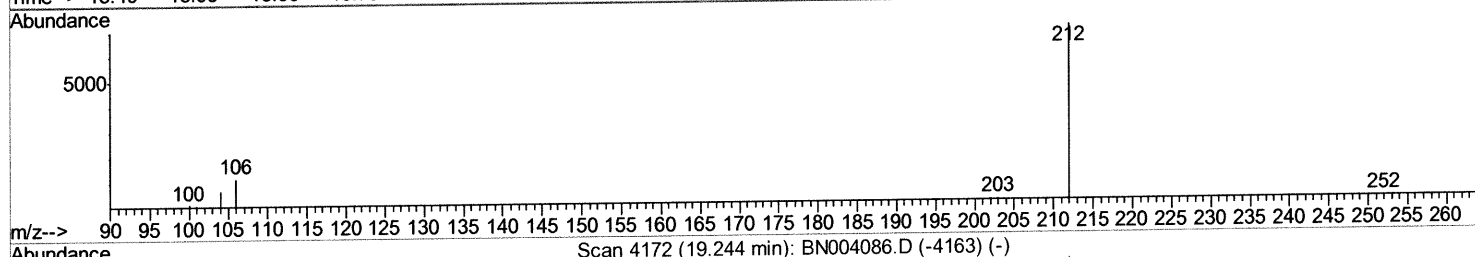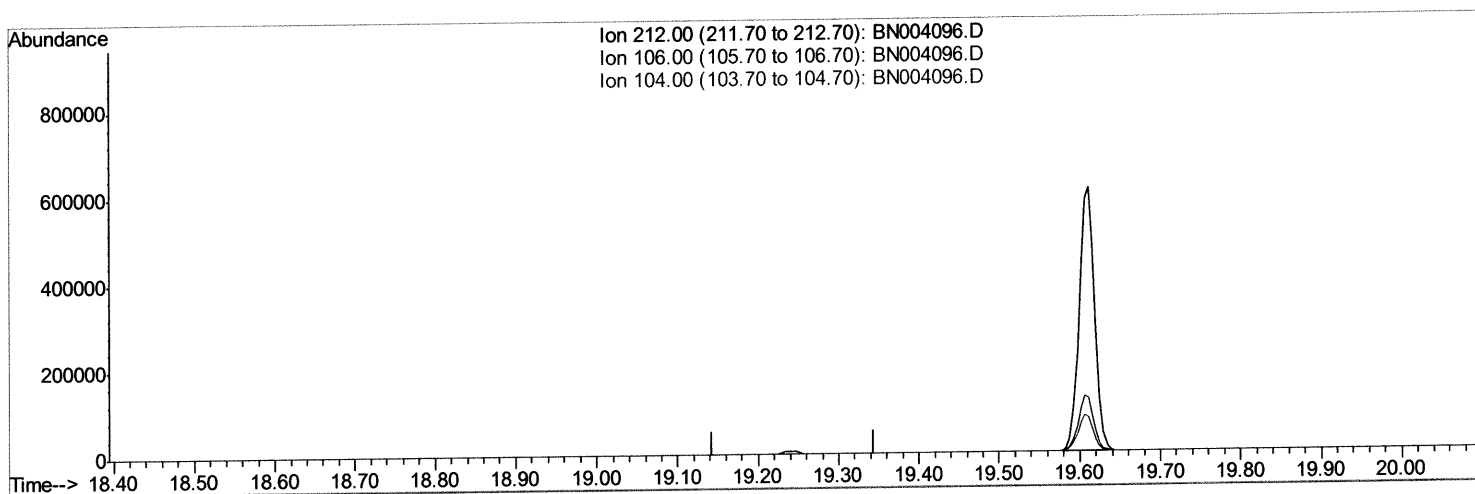

(14) Fluoranthene-d10 (SURR)

19.244min (-19.244) 0.00ng/ul

response 0

Ion	Exp%	Act%
212.00	100	0.00
106.00	14.20	0.00#
104.00	8.00	0.00#
0.00	0.00	0.00

Data Path : Z:\SVOASRV\HPCHEM1\BNA_N\DATA\BN121818\
Quantitation Report (Qedit)




Data File : BN004096.D
Acq On : 19 Dec 2018 02:39
Operator : JU/SJ
Sample : J6271-17
Misc :
ALS Vial : 27 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
F9E32

Manual Integrations
APPROVED

Sohil
12/19/2018 4:16:53 PM

Quant Time: Dec 19 04:51:49 2018
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SOM-EPA-SIM-BN111918.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Dec 19 04:08:55 2018
Response via : Initial Calibration

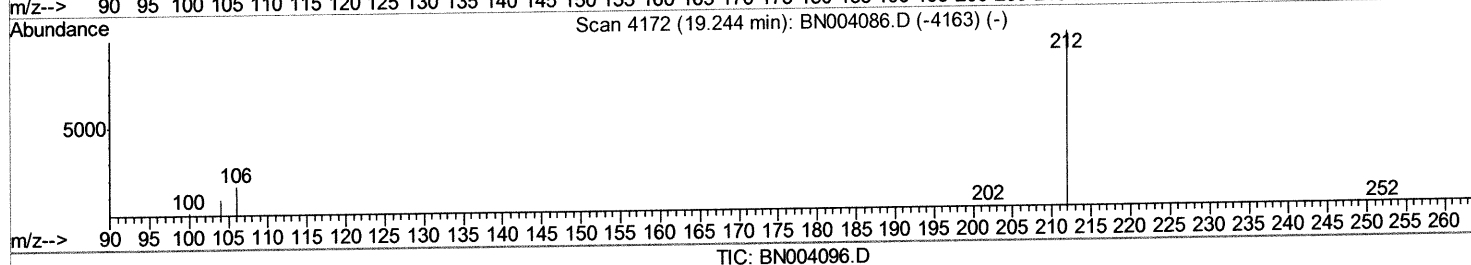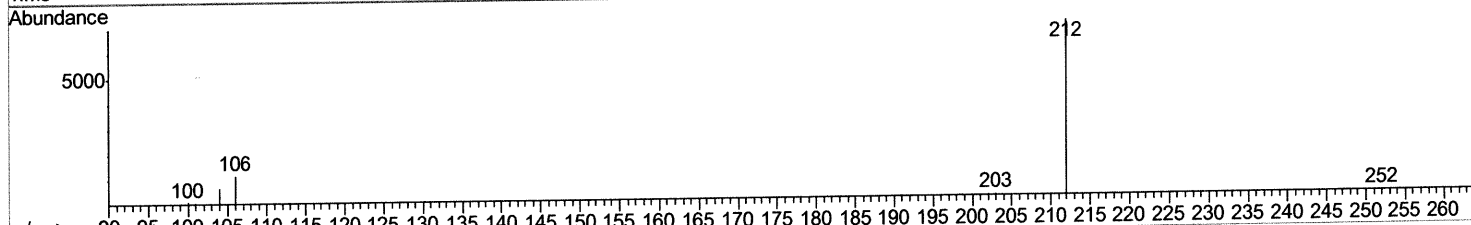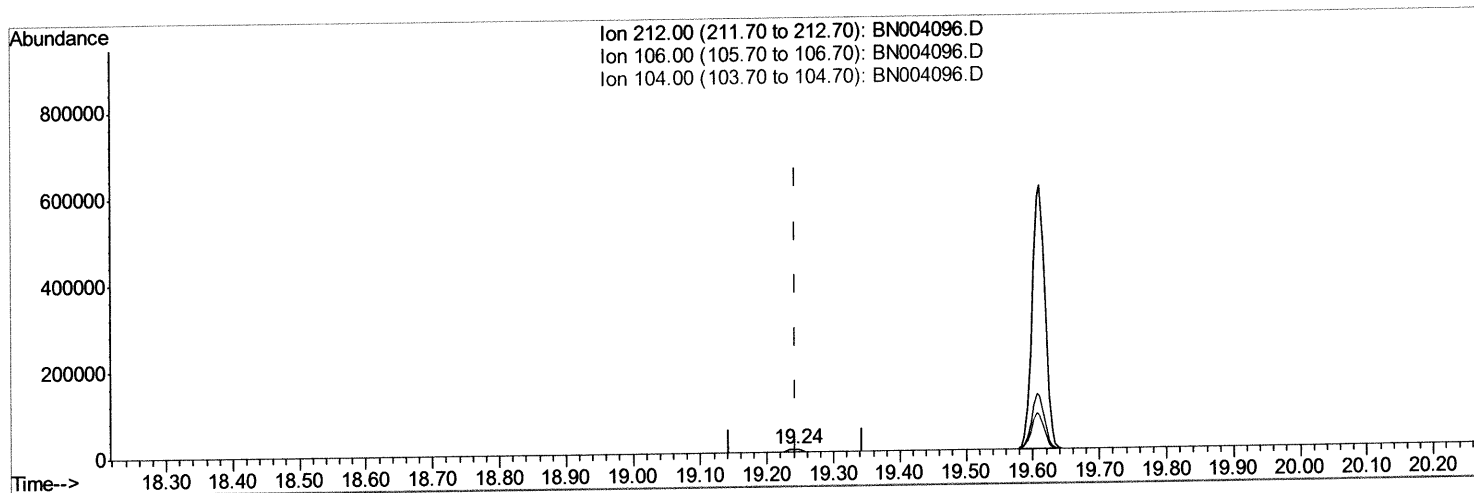

(14) Fluoranthene-d10 (SURR)

19.244min (-0.000) 0.22ng/ul m

response 9381

Ion	Exp%	Act%
212.00	100	100
106.00	14.20	0.00#
104.00	8.00	0.00#
0.00	0.00	0.00

> SJ
12/19/18

Data Path : Z:\SVOASRV\HPCHEM1\BNA_N\DATA\BN121818\
Quantitation Report (Qedit)




Data File : BN004096.D
Acq On : 19 Dec 2018 02:39
Operator : JU/SJ
Sample : J6271-17
Misc :
ALS Vial : 27 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
F9E32

Manual Integrations
APPROVED

Sohil
12/19/2018 4:16:53 PM

Quant Time: Dec 19 04:51:49 2018
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SOM-EPA-SIM-BN111918.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Dec 19 04:08:55 2018
Response via : Initial Calibration

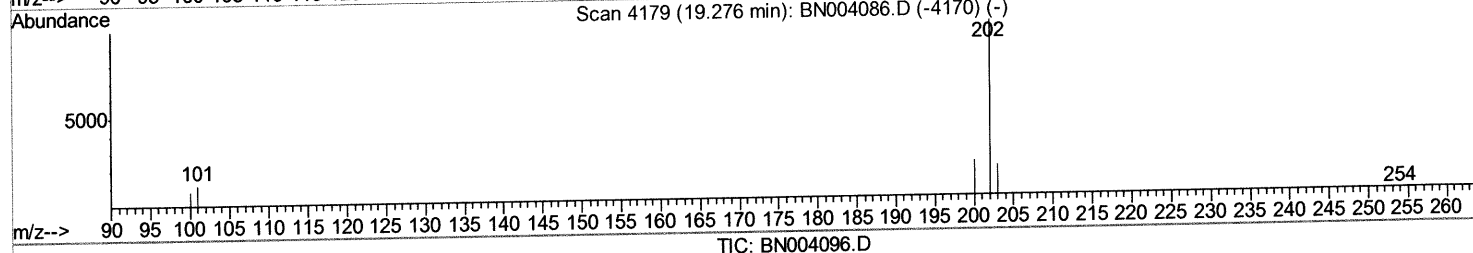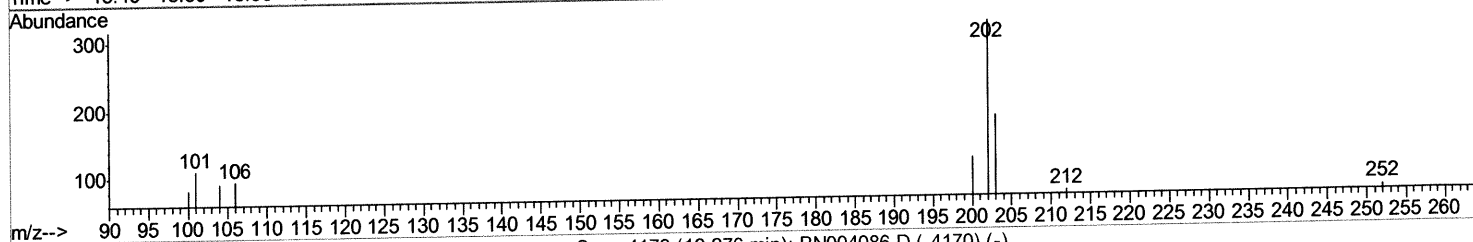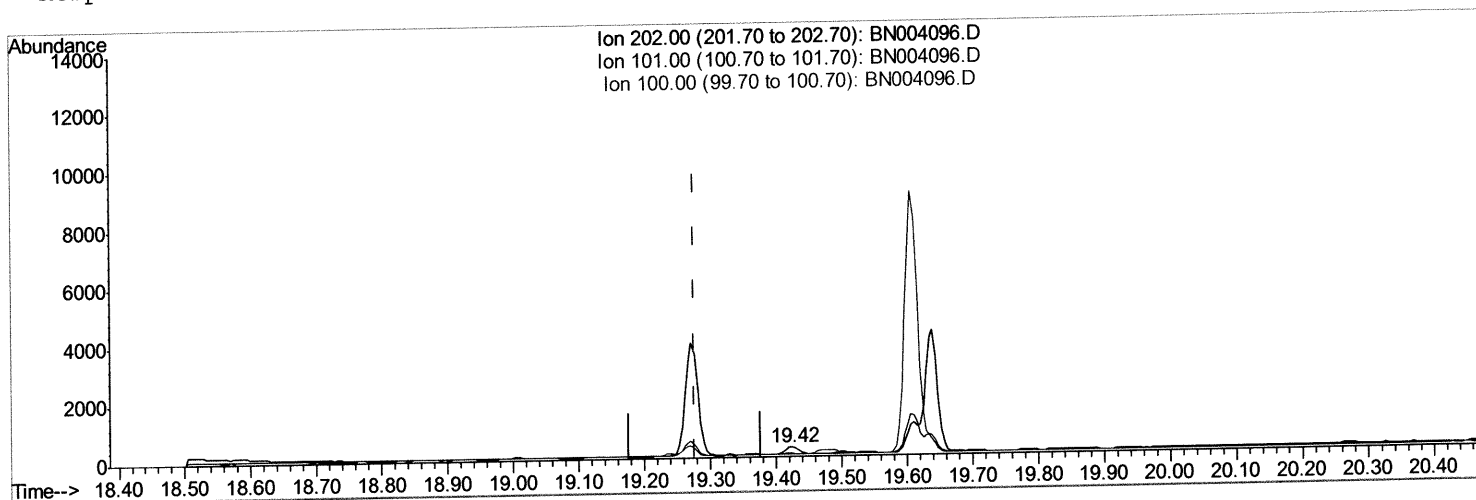

(15) Fluoranthene (C)

19.425min (+0.149) 0.01ng/ul

response 342

Ion	Exp%	Act%
202.00	100	100
101.00	10.70	34.91#
100.00	8.10	26.10
0.00	0.00	0.00

Data Path : Z:\SVOASRV\HPCHEM1\BNA_N\DATA\BN121818\
Quantitation Report (Qedit)




Data File : BN004096.D
Acq On : 19 Dec 2018 02:39
Operator : JU/SJ
Sample : J6271-17
Misc :
ALS Vial : 27 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
F9E32

Manual Integrations
APPROVED

Sohil
12/19/2018 4:16:53 PM

Quant Time: Dec 19 04:51:49 2018
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SOM-EPA-SIM-BN111918.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Dec 19 04:08:55 2018
Response via : Initial Calibration

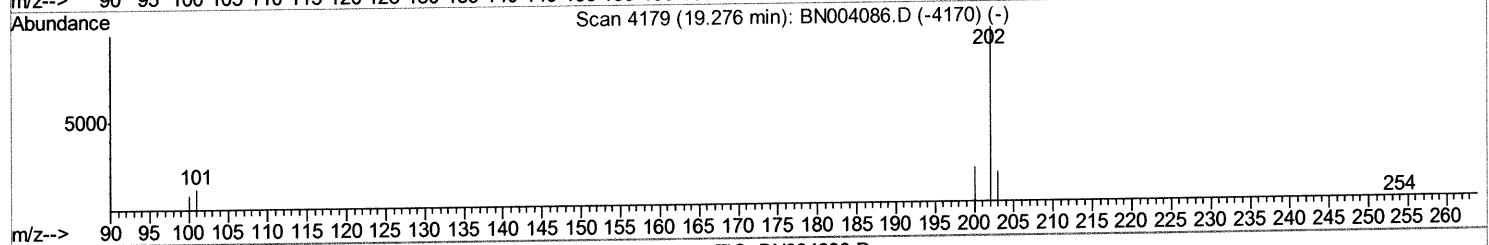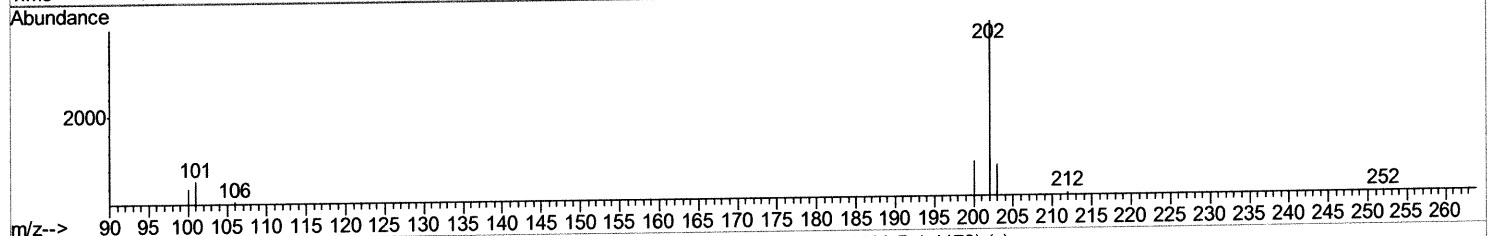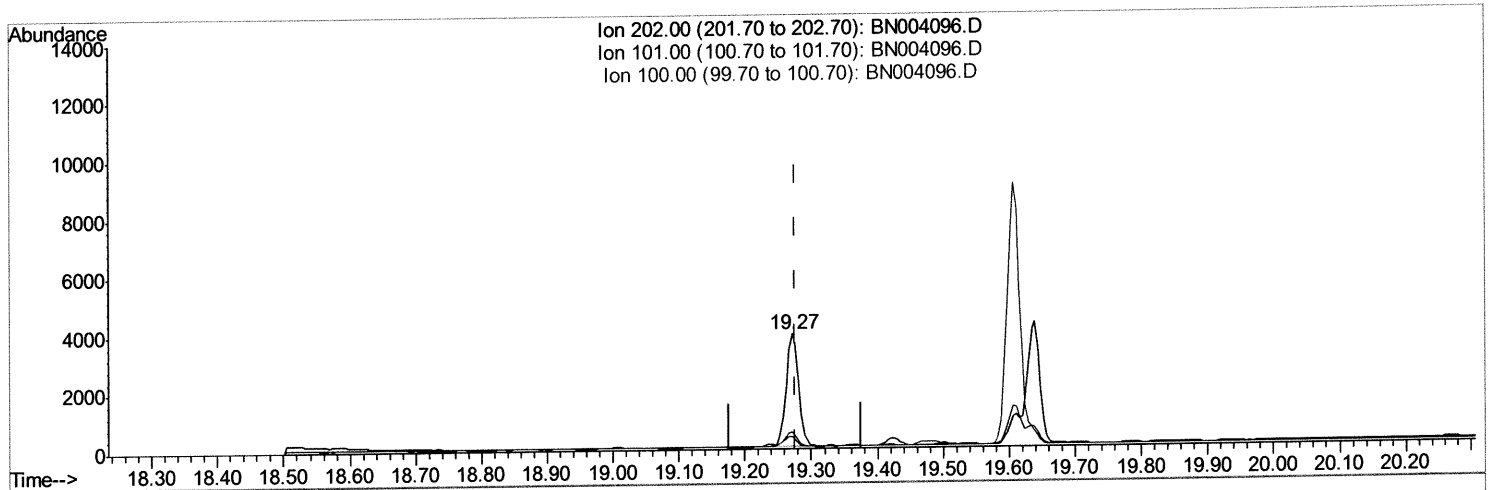

TIC: BN004096.D

(15) Fluoranthene (C)

19.271min (-0.005) 0.09ng/ul m

response 5059

Ion	Exp%	Act%
202.00	100	100
101.00	10.70	14.19
100.00	8.10	10.62
0.00	0.00	0.00

> SJ
12/19/18

Data Path : Z:\SVOASRV\HPCHEM1\BNA_N\DATA\BN121818\
Quantitation Report (Qedit)




Data File : BN004096.D
Acq On : 19 Dec 2018 02:39
Operator : JU/SJ
Sample : J6271-17
Misc :
ALS Vial : 27 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampled :
F9E32

Manual Integrations
APPROVED

Sohil
12/19/2018 4:16:53 PM

Quant Time: Dec 19 04:51:49 2018
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SOM-EPA-SIM-BN111918.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Dec 19 04:08:55 2018
Response via : Initial Calibration

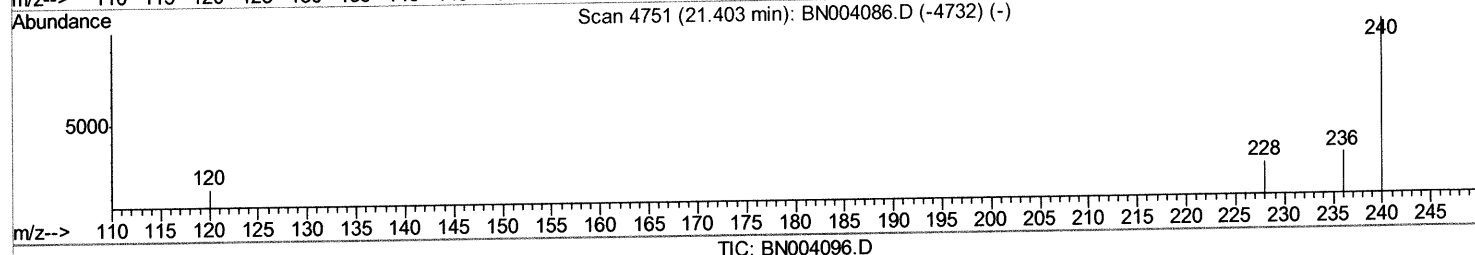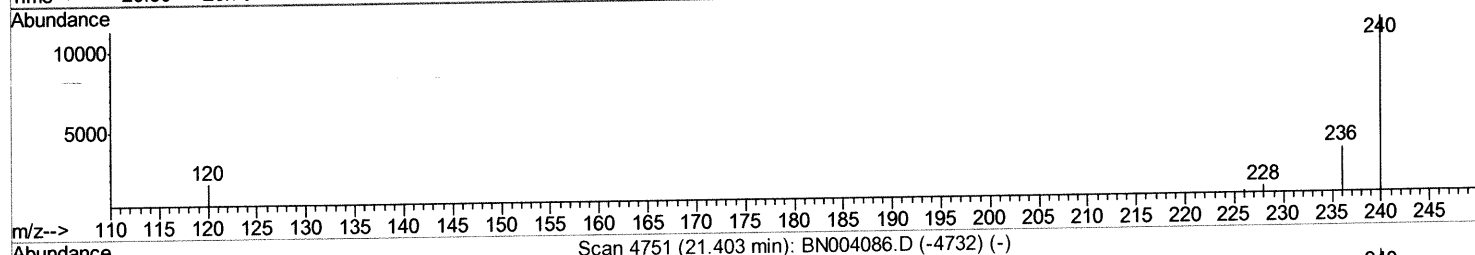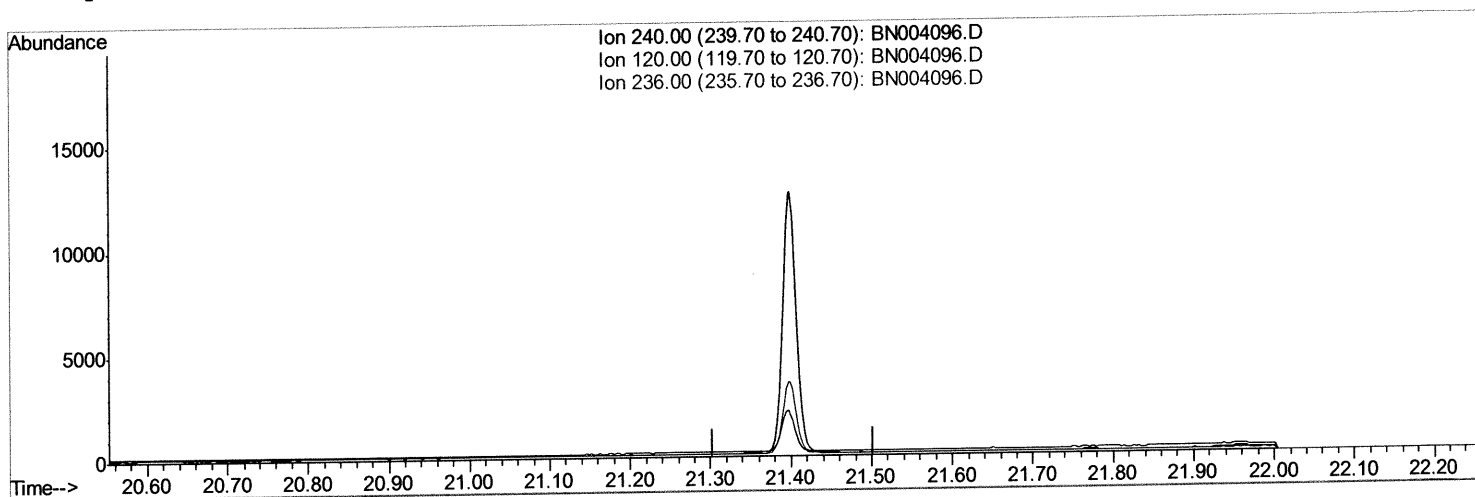

(16) Chrysene-d12 (I)

21.403min (-21.403) 0.00ng/ul

response 0

Ion	Exp%	Act%
240.00	100	0.00
120.00	14.00	0.00#
236.00	27.60	0.00#
0.00	0.00	0.00

Data Path : Z:\SVOASRV\HPCHEM1\BNA_N\DATA\BN121818\
Quantitation Report (Qedit)




Data File : BN004096.D
Acq On : 19 Dec 2018 02:39
Operator : JU/SJ
Sample : J6271-17
Misc :
ALS Vial : 27 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
F9E32

Manual Integrations
APPROVED

Sohil
12/19/2018 4:16:53 PM

Quant Time: Dec 19 04:51:49 2018
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SOM-EPA-SIM-BN111918.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Dec 19 04:08:55 2018
Response via : Initial Calibration

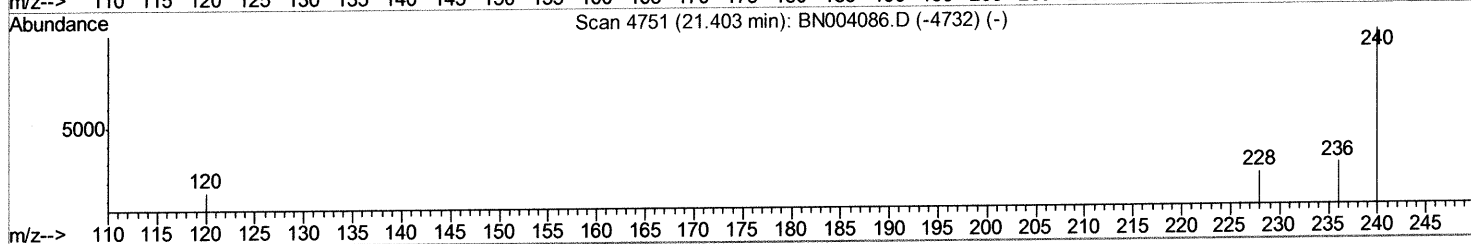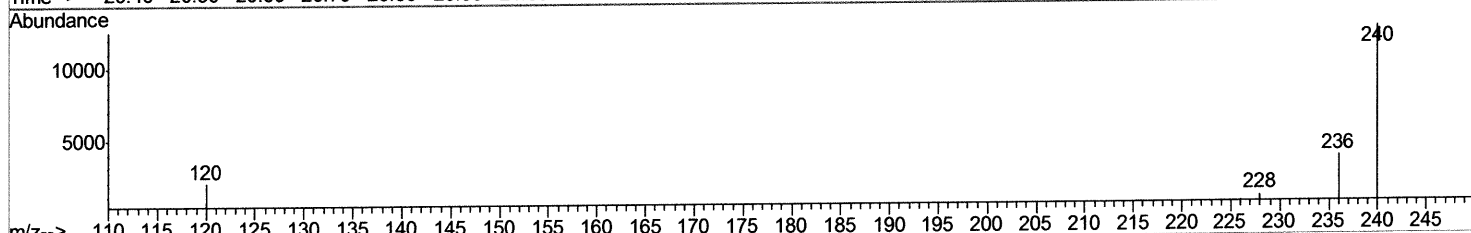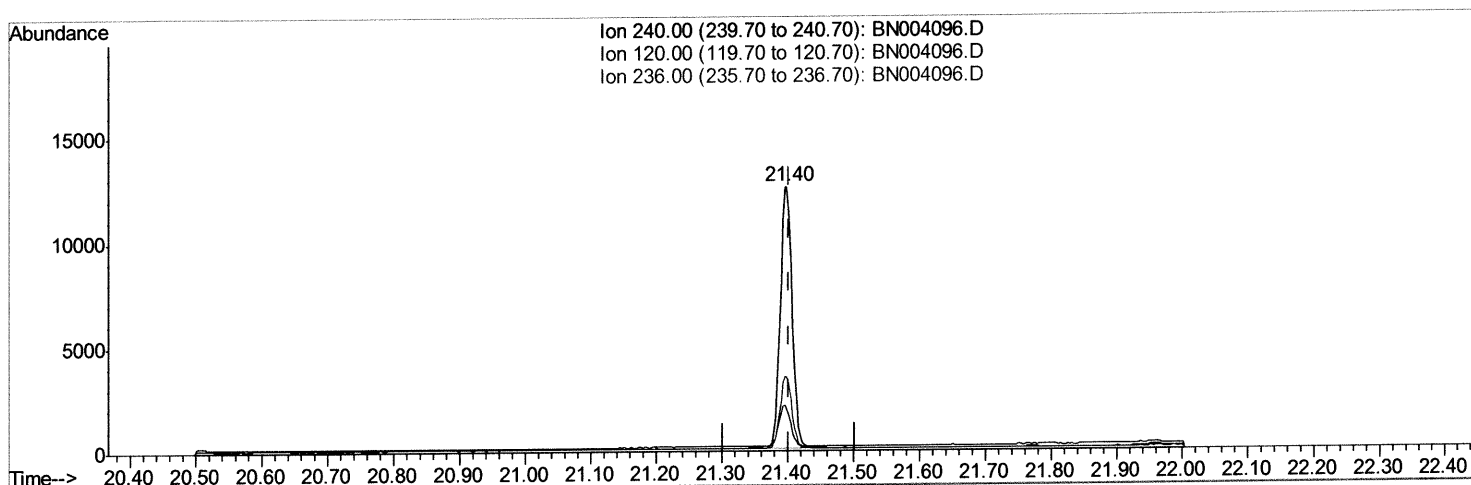

TIC: BN004096.D

(16) Chrysene-d12 (I)

21.400min (-0.003) 0.40ng/ul m

response 15507

Ion	Exp%	Act%
240.00	100	100
120.00	14.00	16.07
236.00	27.60	28.01
0.00	0.00	0.00

> SJ
12/19/18

Data Path : Z:\SVOASRV\HPCHEM1\BNA_N\DATA\BN121818\
Quantitation Report (Qedit)




Data File : BN004096.D
Acq On : 19 Dec 2018 02:39
Operator : JU/SJ
Sample : J6271-17
Misc :
ALS Vial : 27 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
F9E32

Manual Integrations
APPROVED

Sohil
12/19/2018 4:16:53 PM

Quant Time: Dec 19 04:53:02 2018
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SOM-EPA-SIM-BN111918.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Dec 19 04:08:55 2018
Response via : Initial Calibration

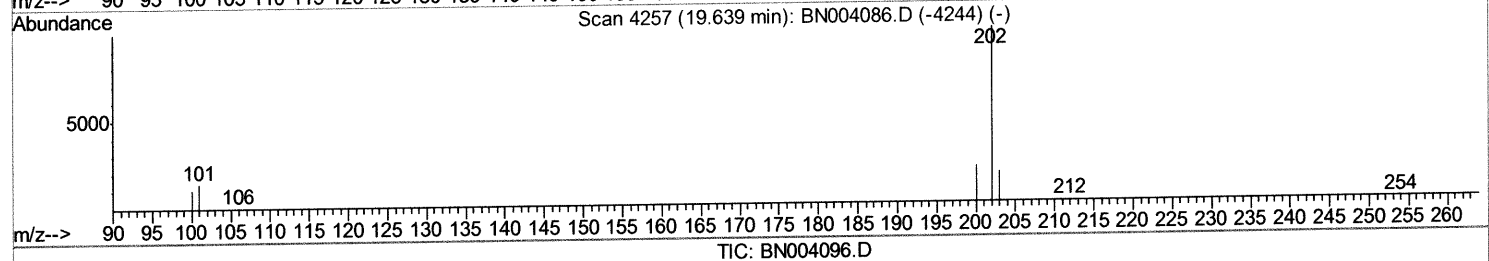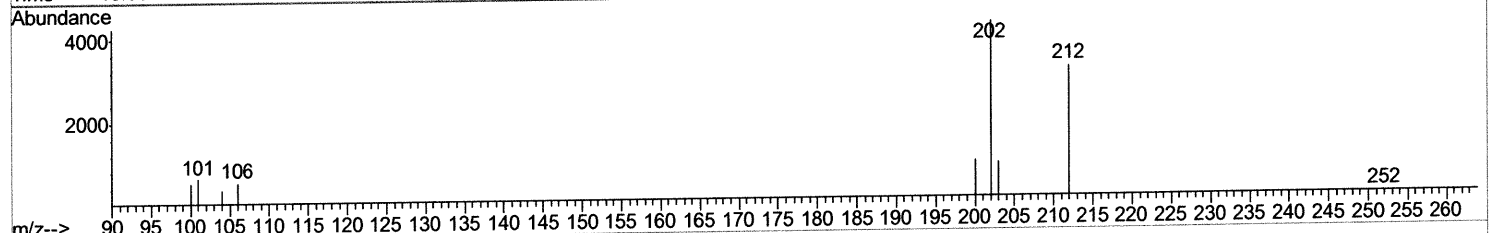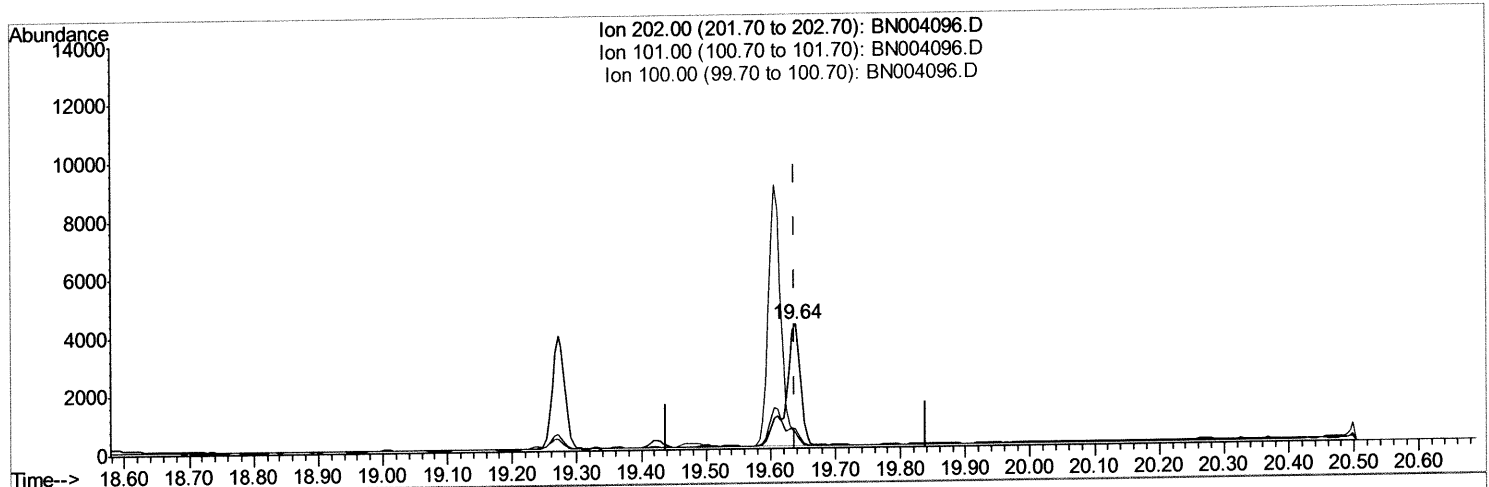

(17) Pyrene

19.639min (-0.000) 0.12ng/ul

response 6614

Ion	Exp%	Act%
202.00	100	100
101.00	12.90	15.59#
100.00	10.60	12.87#
0.00	0.00	0.00

Data Path : Z:\SVOASRV\HPCHEM1\BNA_N\DATA\BN121818\
Quantitation Report (Qedit)




Data File : BN004096.D
Acq On : 19 Dec 2018 02:39
Operator : JU/SJ
Sample : J6271-17
Misc :
ALS Vial : 27 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampled :
F9E32

Manual Integrations
APPROVED

Sohil
12/19/2018 4:16:53 PM

Quant Time: Dec 19 04:53:02 2018
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SOM-EPA-SIM-BN111918.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Dec 19 04:08:55 2018
Response via : Initial Calibration

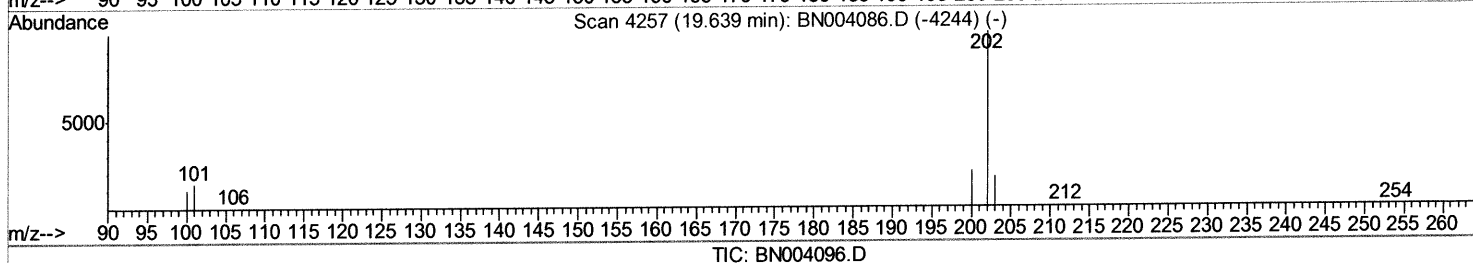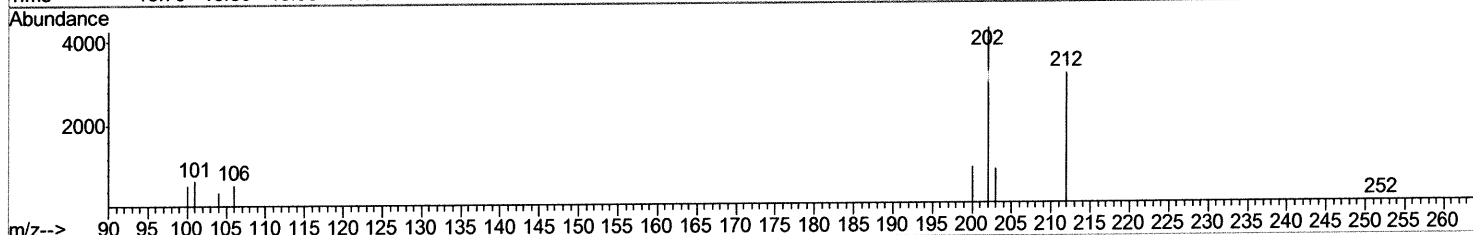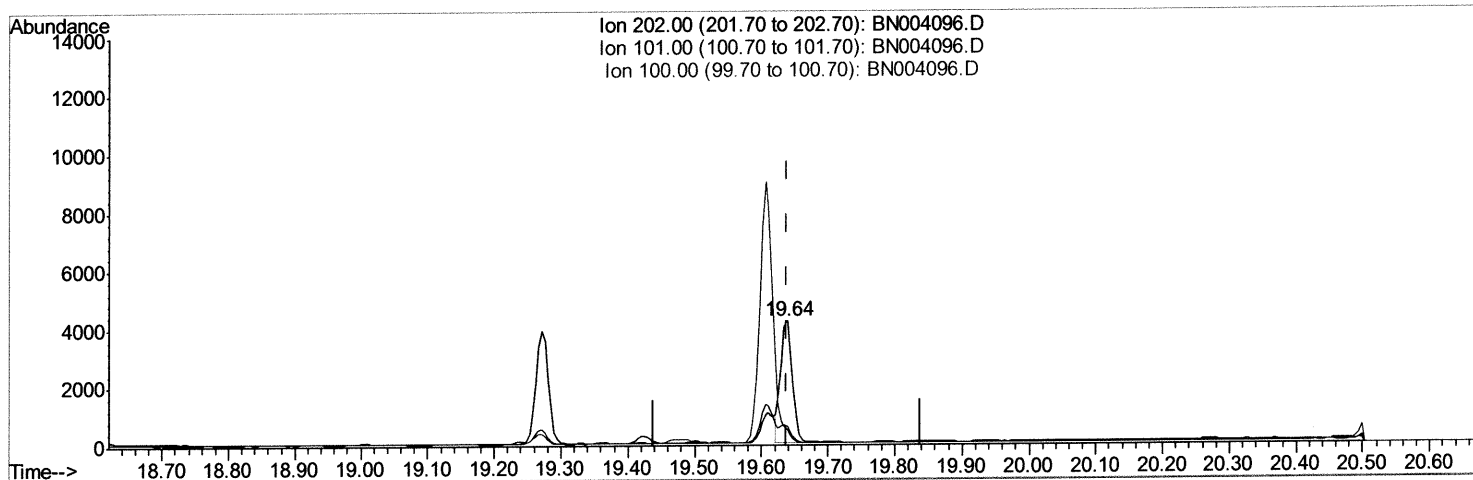

TIC: BN004096.D

(17) Pyrene

19.639min (-0.000) 0.10ng/ul m

response 5286

Ion	Exp%	Act%
202.00	100	100
101.00	12.90	15.59#
100.00	10.60	12.87#
0.00	0.00	0.00

> SJ
12/19/18

Data Path : Z:\SVOASRV\HPCHEM1\BNA_N\DATA\BN121818\
Quantitation Report (Qedit)




Data File : BN004096.D
Acq On : 19 Dec 2018 02:39
Operator : JU/SJ
Sample : J6271-17
Misc :
ALS Vial : 27 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
F9E32

Manual Integrations
APPROVED

Sohil
12/19/2018 4:16:53 PM

Quant Time: Dec 19 04:53:02 2018
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SOM-EPA-SIM-BN111918.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Dec 19 04:08:55 2018
Response via : Initial Calibration

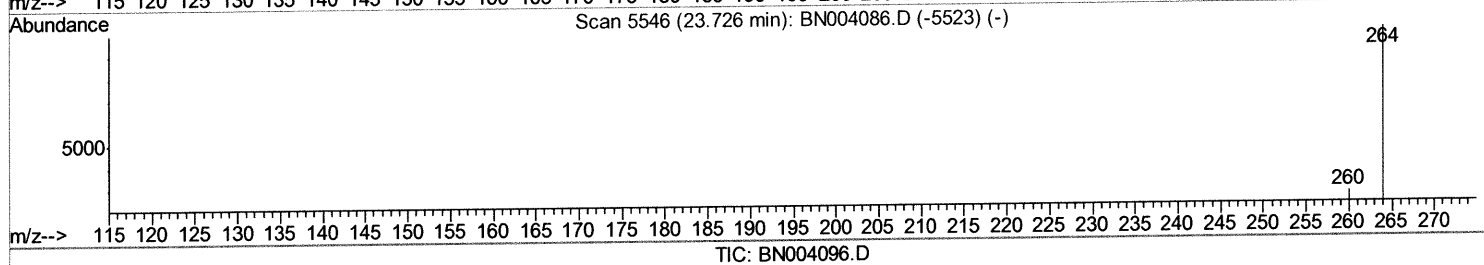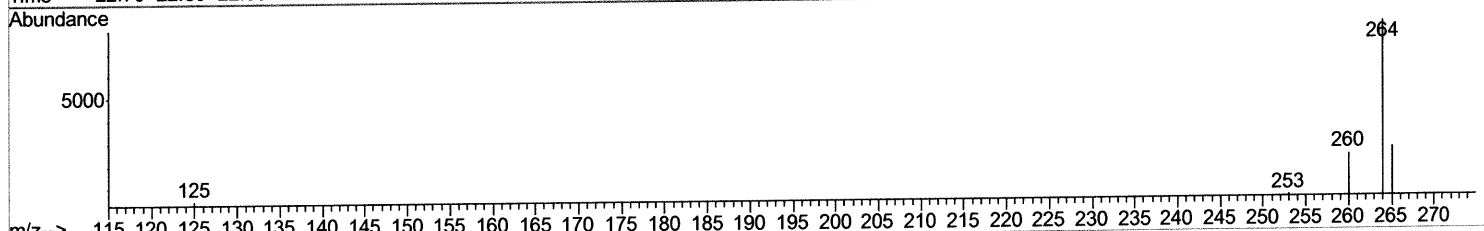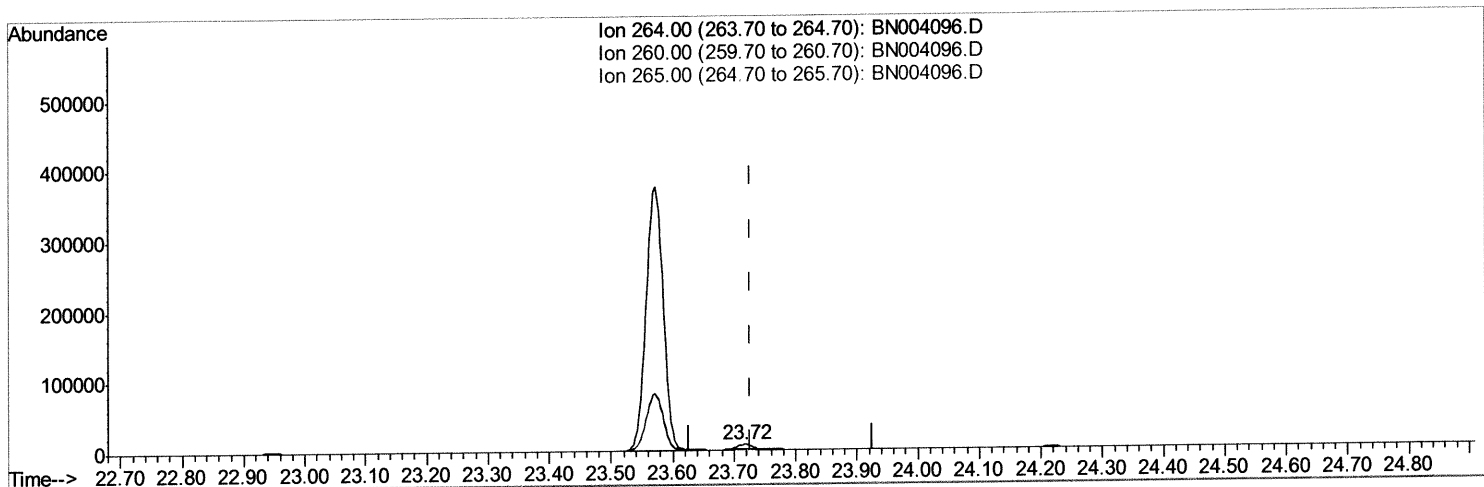

TIC: BN004096.D

(20) Perylene-d12 (I)

23.718min (-0.009) 0.40ng/ul

response 15334

Ion	Exp%	Act%
264.00	100	100
260.00	26.20	26.74
265.00	33.50	30.64
0.00	0.00	0.00

Data Path : Z:\SVOASRV\HPCHEM1\BNA_N\DATA\BN121818\
Quantitation Report (Qedit)




Data File : BN004096.D
Acq On : 19 Dec 2018 02:39
Operator : JU/SJ
Sample : J6271-17
Misc :
ALS Vial : 27 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
F9E32

Manual Integrations
APPROVED

Sohil
12/19/2018 4:16:53 PM

Quant Time: Dec 19 04:53:02 2018
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SOM-EPA-SIM-BN111918.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Dec 19 04:08:55 2018
Response via : Initial Calibration

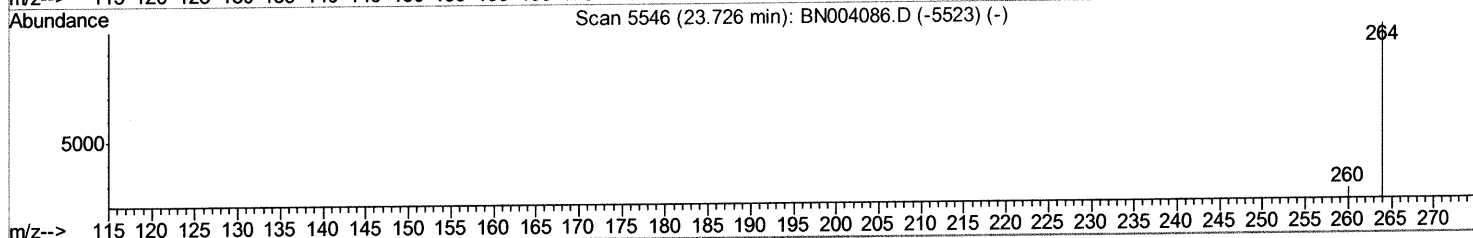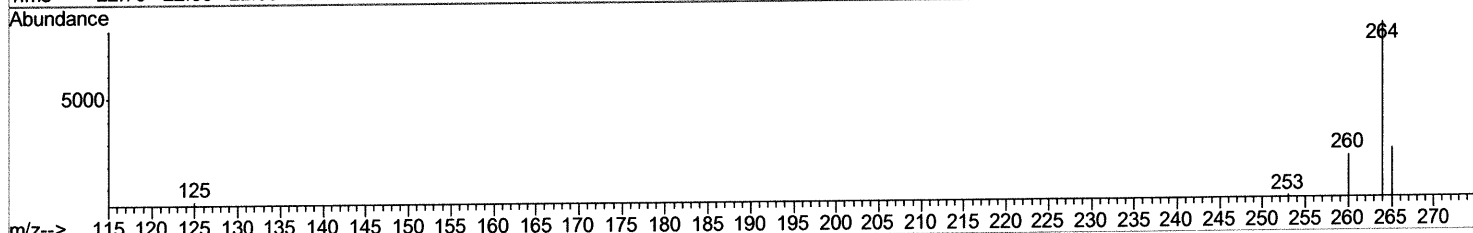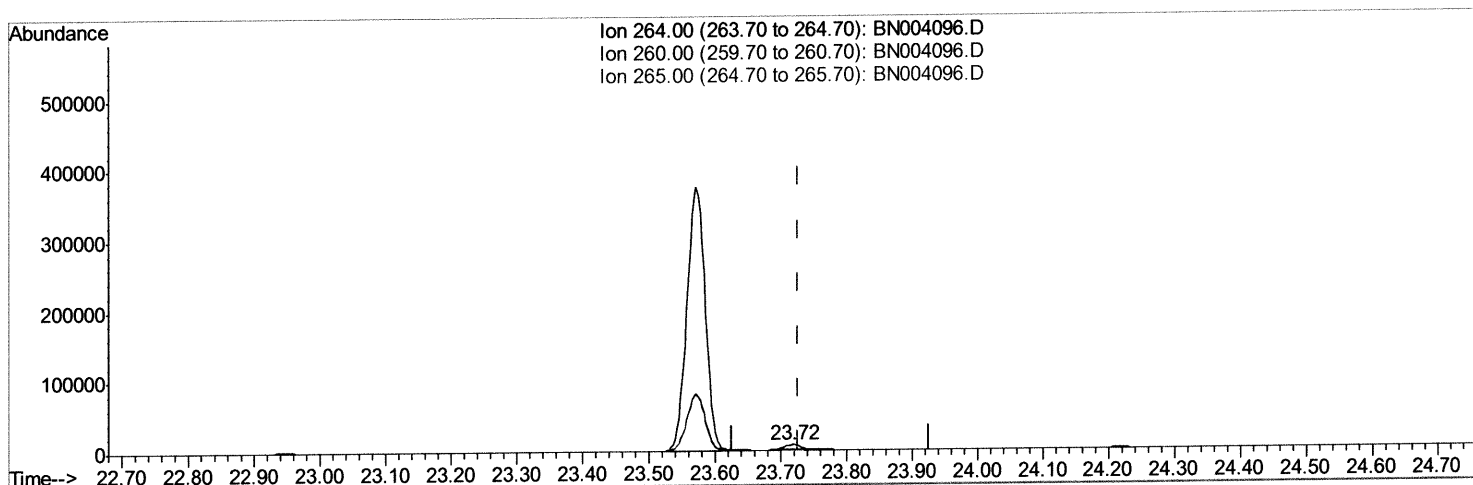

TIC: BN004096.D

(20) Perylene-d12 (I)

23.718min (-0.009) 0.40ng/ul m

response 13714

Ion	Exp%	Act%
264.00	100	100
260.00	26.20	26.74
265.00	33.50	30.64
0.00	0.00	0.00

> SJ
12/19/18

Data Path : Z:\SVOASRV\HPCHEM1\BNA_N\DATA\BN121818\
Quantitation Report (Qedit)




Data File : BN004096.D
Acq On : 19 Dec 2018 02:39
Operator : JU/SJ
Sample : J6271-17
Misc :
ALS Vial : 27 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
F9E32

Manual Integrations
APPROVED

Sohil
12/19/2018 4:16:53 PM

Quant Time: Dec 19 04:53:41 2018
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SOM-EPA-SIM-BN111918.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Dec 19 04:08:55 2018
Response via : Initial Calibration

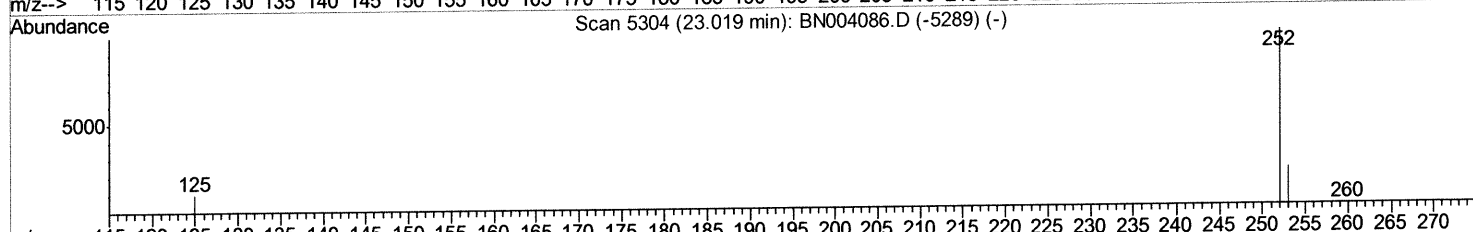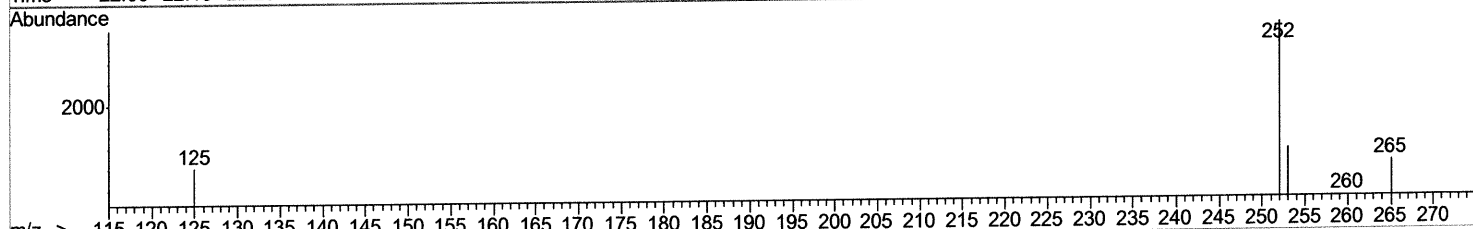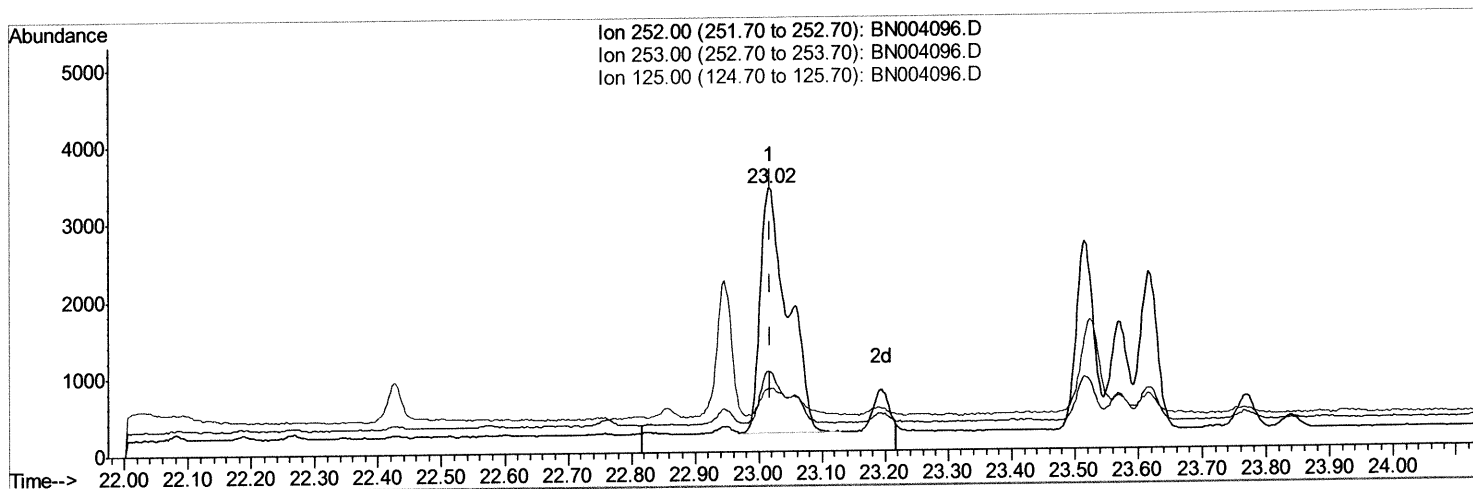

TIC: BN004096.D

(21) Benzo(b)fluoranthene
23.016min (-0.003) 0.17ng/ul
response 9691

Ion	Exp%	Act%
252.00	100	100
253.00	23.00	30.63
125.00	11.20	23.94#
0.00	0.00	0.00

Data Path : Z:\SVOASRV\HPCHEM1\BNA_N\DATA\BN121818\
Quantitation Report (Qedit)




Data File : BN004096.D
Acq On : 19 Dec 2018 02:39
Operator : JU/SJ
Sample : J6271-17
Misc :
ALS Vial : 27 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampled :
F9E32

Manual Integrations
APPROVED

Sohil
12/19/2018 4:16:53 PM

Quant Time: Dec 19 04:53:41 2018
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SOM-EPA-SIM-BN111918.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Dec 19 04:08:55 2018
Response via : Initial Calibration

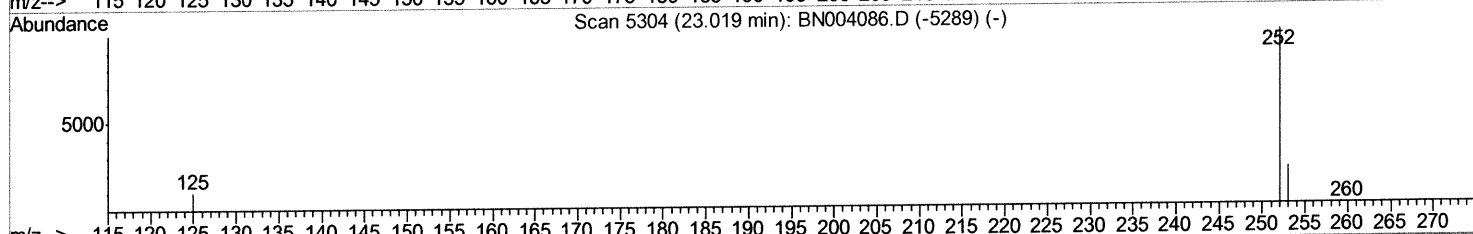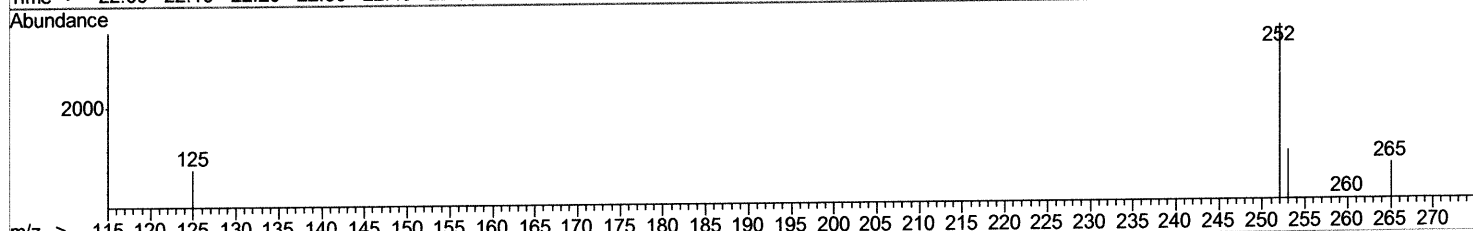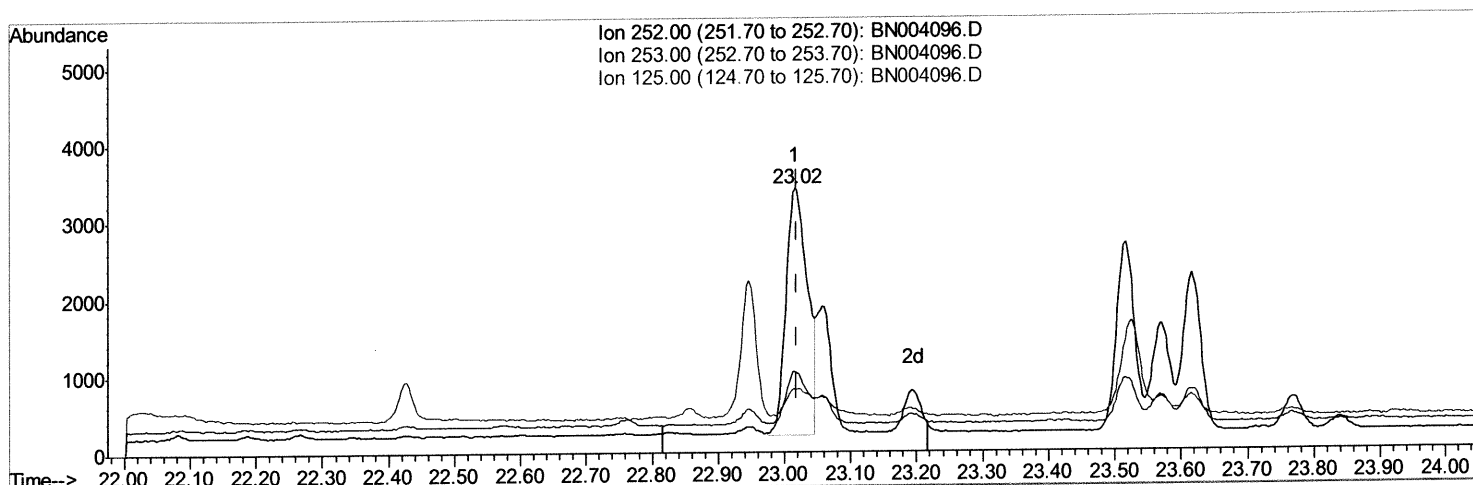

TIC: BN004096.D

(21) Benzo(b)fluoranthene

23.016min (-0.003) 0.13ng/ul m

response 7164

Ion	Exp%	Act%
252.00	100	100
253.00	23.00	30.63
125.00	11.20	23.94#
0.00	0.00	0.00

> 55
12/19/18

Data Path : Z:\SVOASRV\HPCHEM1\BNA_N\DATA\BN121818\
Quantitation Report (Qedit)




Data File : BN004096.D
Acq On : 19 Dec 2018 02:39
Operator : JU/SJ
Sample : J6271-17
Misc :
ALS Vial : 27 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
F9E32

Manual Integrations
APPROVED

Sohil
12/19/2018 4:16:53 PM

Quant Time: Dec 19 04:53:41 2018
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SOM-EPA-SIM-BN111918.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Dec 19 04:08:55 2018
Response via : Initial Calibration

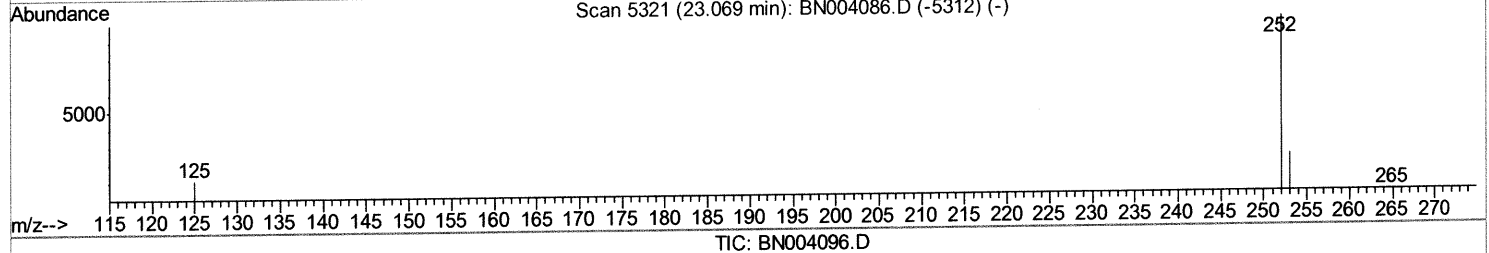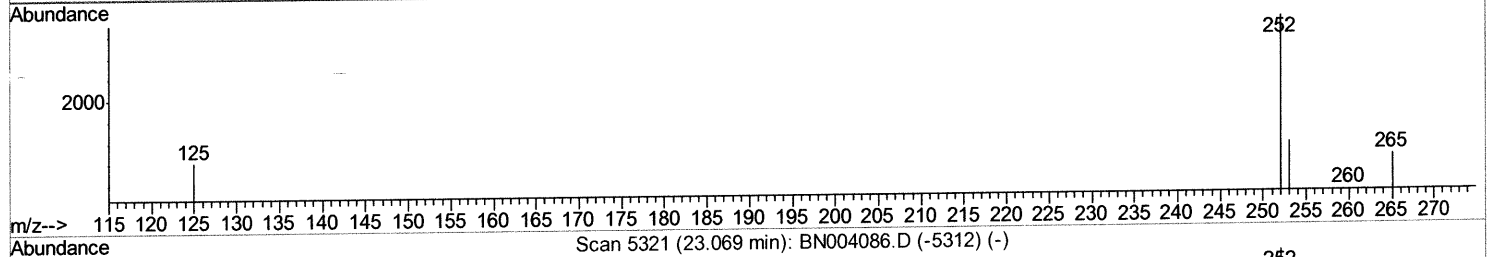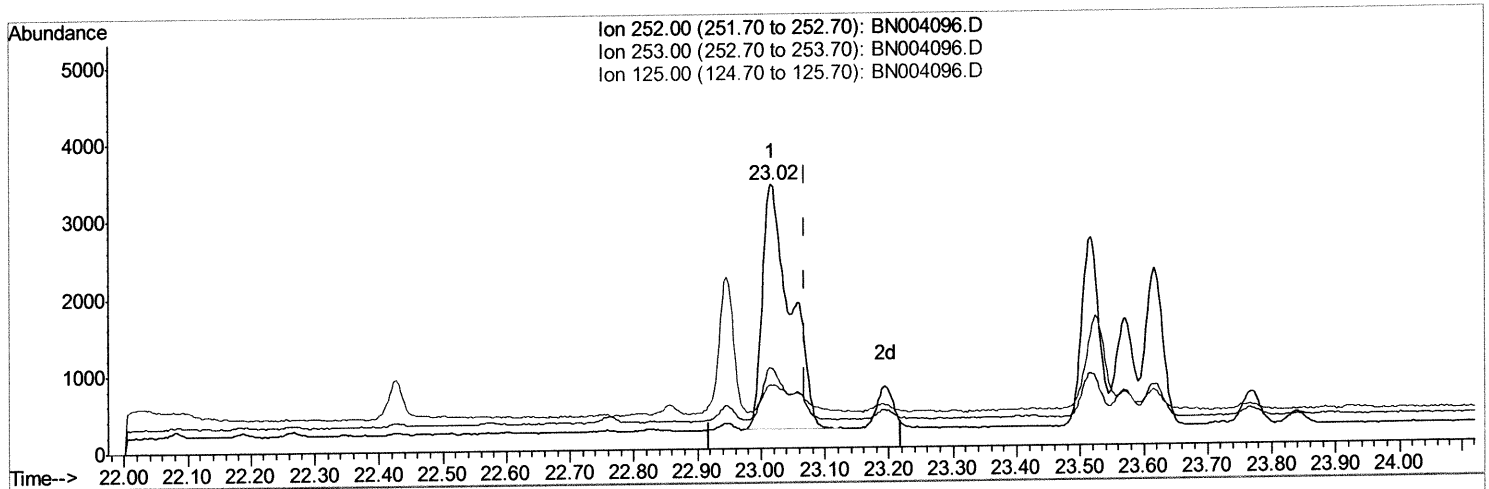

(22) Benzo(k)fluoranthene
23.016min (-0.053) 0.17ng/ul
response 9640
Ion Exp% Act%
252.00 100 100
253.00 23.10 30.63#
125.00 11.30 23.94#
0.00 0.00 0.00

Data Path : Z:\SVOASRV\HPCHEM1\BNA_N\DATA\BN121818\
Quantitation Report (Qedit)




Data File : BN004096.D
Acq On : 19 Dec 2018 02:39
Operator : JU/SJ
Sample : J6271-17
Misc :
ALS Vial : 27 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampled :
F9E32

Manual Integrations
APPROVED

Sohil
12/19/2018 4:16:53 PM

Quant Time: Dec 19 04:53:41 2018
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SOM-EPA-SIM-BN111918.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Dec 19 04:08:55 2018
Response via : Initial Calibration

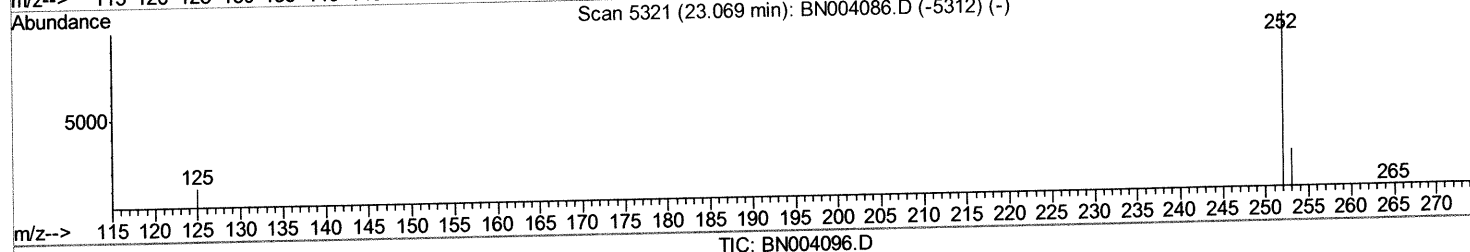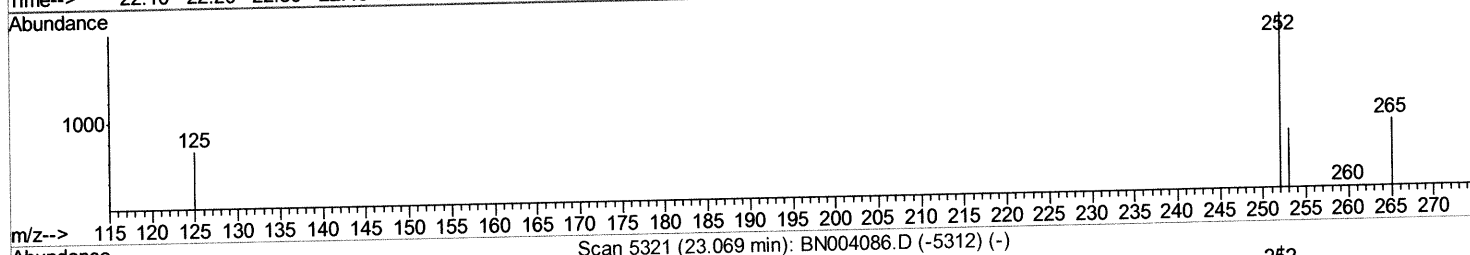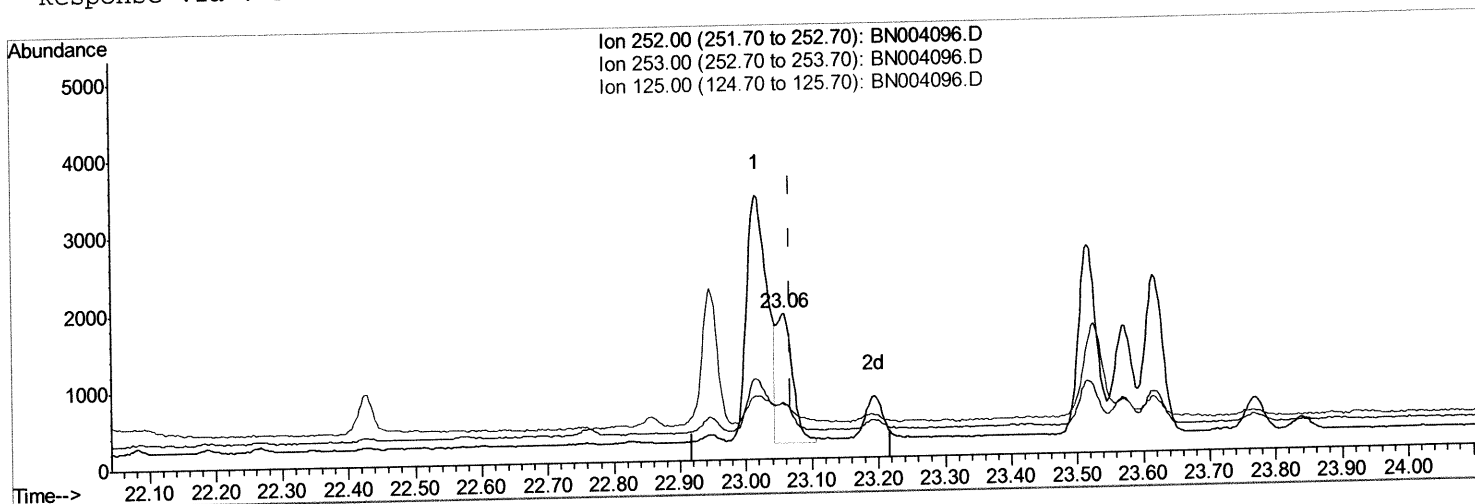

(22) Benzo(k)fluoranthene

23.057min (-0.012) 0.05ng/ul m

response 2942

Ion	Exp%	Act%
252.00	100	100
253.00	23.10	38.36#
125.00	11.30	37.57#
0.00	0.00	0.00

> SJ
12/19/18

Data Path : Z:\SVOASRV\HPCHEM1\BNA_N\DATA\BN121818\
Quantitation Report (QT Reviewed)

Data File : BN004096.D
Acq On : 19 Dec 2018 02:39
Operator : JU/SJ
Sample : J6271-17
Misc :
ALS Vial : 27 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
F9E32

Manual Integrations
APPROVED

Sohil
12/19/2018 4:16:53 PM

Quant Time: Dec 19 04:54:57 2018
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SOM-EPA-SIM-BN111918.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Dec 19 04:08:55 2018
Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	7.83	152	2086	0.40	ng/ul	0.00
2) Naphthalene-d8	10.63	136	10173	0.40	ng/ul	0.00
6) Acenaphthene-d10	14.47	164	6007	0.40	ng/ul	0.00
10) Phenanthrene-d10	17.21	188	14900m	0.40	ng/ul	0.00
16) Chrysene-d12	21.40	240	15507m	0.40	ng/ul	0.00
20) Perylene-d12	23.72	264	13714m	0.40	ng/ul	0.00

System Monitoring Compounds	R.T.	QIon	Response	Conc	Units	Dev(Min)
4) 2-Methylnaphthalene-d10	12.22	152	3139	0.20	ng/ul	0.00
14) Fluoranthene-d10	19.24	212	9381m	0.22	ng/ul	0.00

Target Compounds	R.T.	QIon	Response	Conc	Units	Qvalue
7) Acenaphthylene	14.19	152	877	0.032	ng/ul#	80
12) Phenanthrene	17.25	178	1761m	0.036	ng/ul	
15) Fluoranthene	19.27	202	5059m	0.088	ng/ul	
17) Pyrene	19.64	202	5286m	0.095	ng/ul	
18) Benzo(a)anthracene	21.38	228	3943	0.081	ng/ul#	90
19) Chrysene	21.43	228	5389	0.096	ng/ul#	92
21) Benzo(b)fluoranthene	23.02	252	7164m	0.126	ng/ul	
22) Benzo(k)fluoranthene	23.06	252	2942m	0.053	ng/ul	
23) Benzo(a)pyrene	23.62	252	3800	0.077	ng/ul#	70
24) Indeno(1,2,3-cd)pyrene	26.08	276	3386	0.060	ng/ul#	94
26) Benzo(g,h,i)perylene	26.82	276	2972	0.061	ng/ul#	72

(#) = qualifier out of range (m) = manual integration (+) = signals summed

SJ
12/19/18